

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR030221\
 Data File : PR049509.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2021 07:15
 Operator : AJ\MA
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Ankita
 3/2/2021 11:27:54 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 07:30:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR030221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 02 07:29:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.663	3.847	12710088	15887362	4.819	4.955
2) SA Decachlor...	10.542	8.902	16075931	46526731	5.671	4.990
Target Compounds						
26) L6 AR-1254-1	6.696	5.735	6409094	5893323	58.635	52.927m
27) L6 AR-1254-2	6.913	5.883	9995066	7049817	59.201	57.808m
28) L6 AR-1254-3	7.283	6.287	10087114	12270289	58.378	52.386
29) L6 AR-1254-4	7.568	6.515	8482307	18825550	59.285	51.895m
30) L6 AR-1254-5	7.986	6.933	7730329	21427718	55.327	49.971

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR030221\
Data File : PR049509.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2021 07:15
Operator : AJ\MA
Sample : AR1254ICC050
Misc :
ALS Vial : 66 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
3/2/2021 11:27:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 07:30:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR030221.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 02 07:29:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

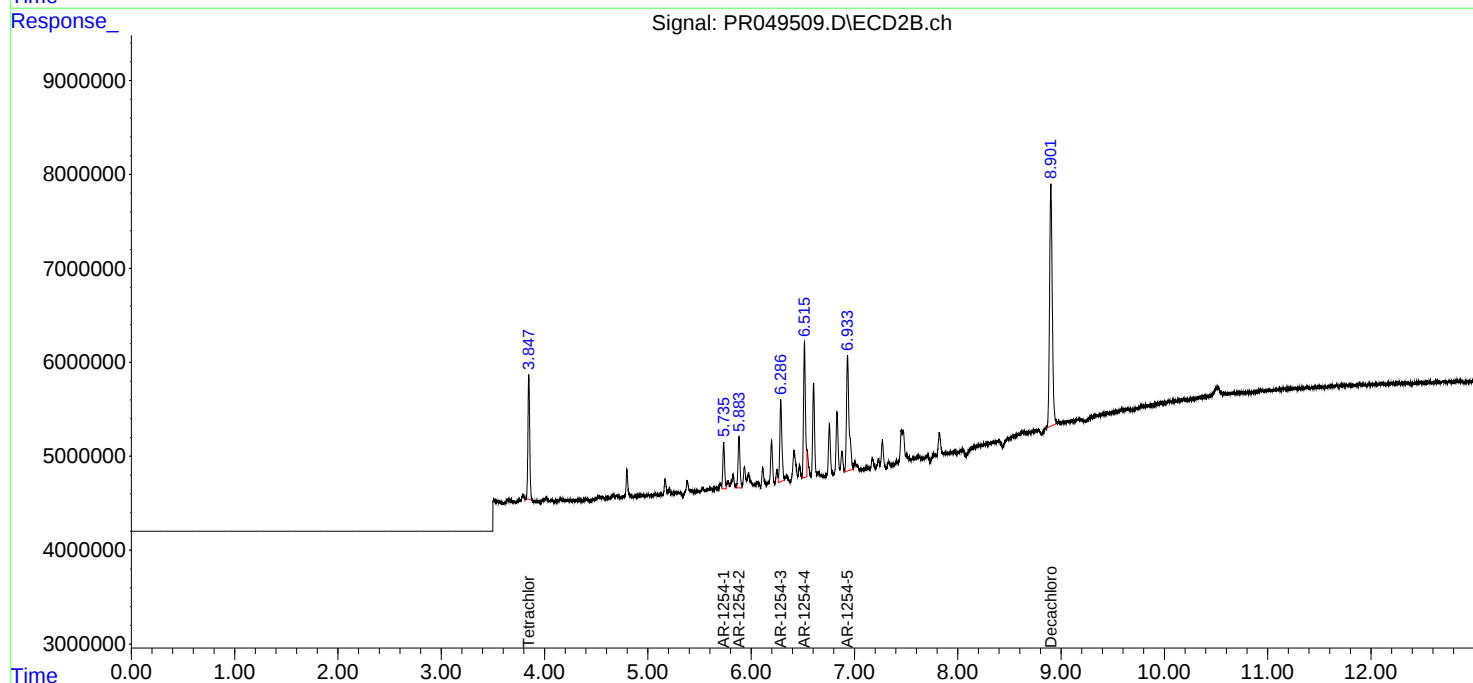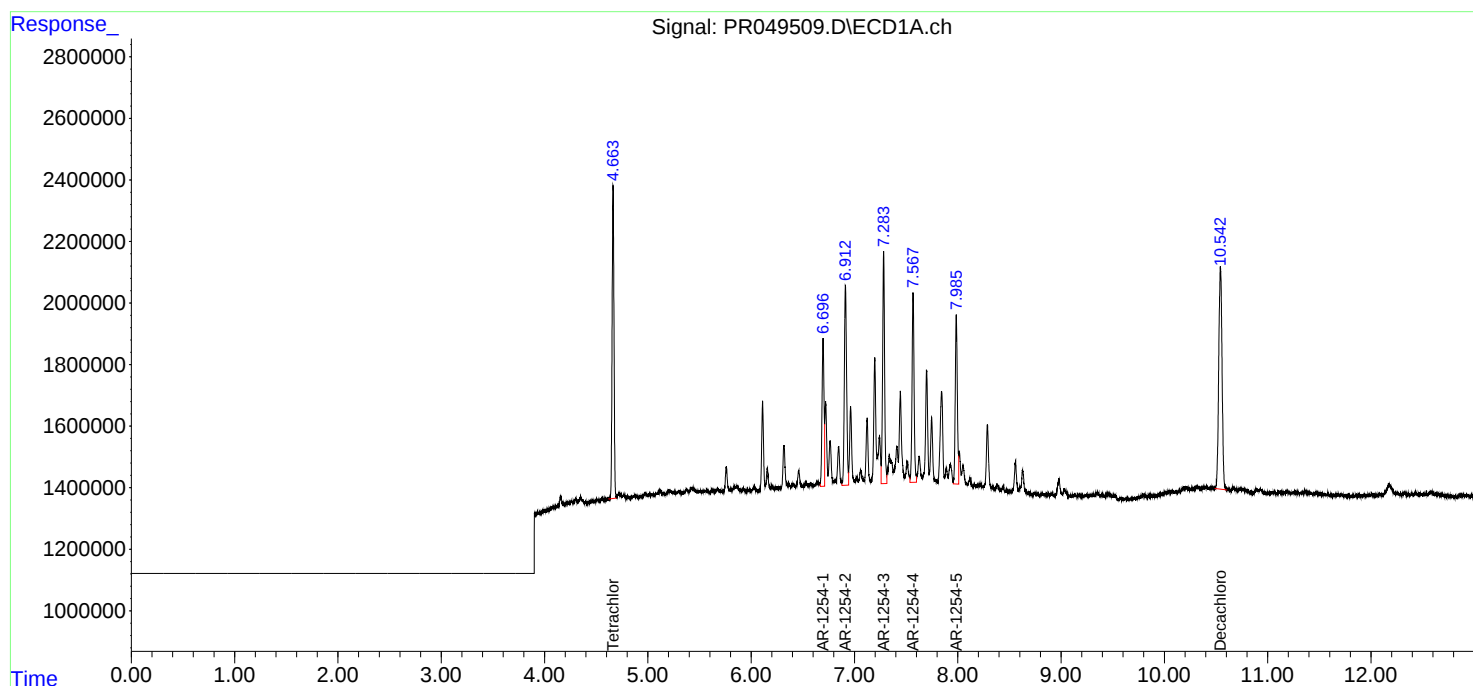

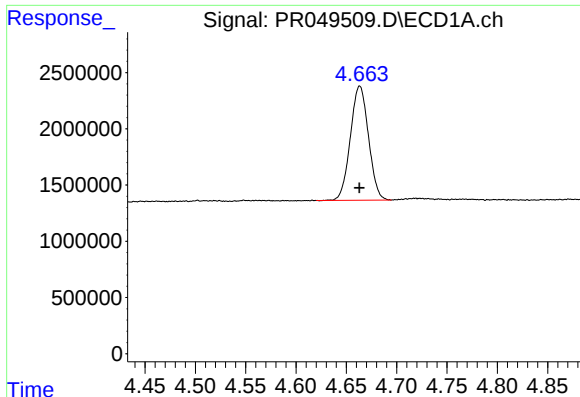


#1 Tetrachloro-m-xylene

R.T.: 4.663 min
Delta R.T.: 0.000 min
Response: 12710088
Conc: 4.82 ng/ml

Instrument :
ECD_R
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
3/2/2021 11:27:54 AM

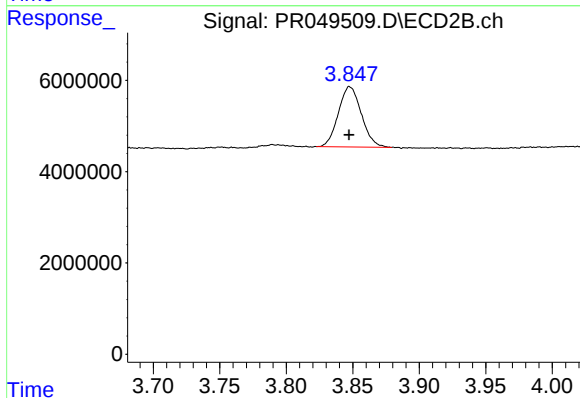


#1 Tetrachloro-m-xylene

R.T.: 3.847 min
Delta R.T.: 0.000 min
Response: 15887362
Conc: 4.95 ng/ml

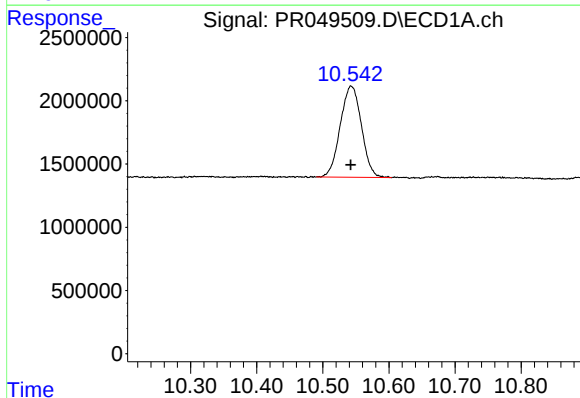


#2 Decachlorobiphenyl

R.T.: 10.542 min
Delta R.T.: 0.000 min
Response: 16075931
Conc: 5.67 ng/ml

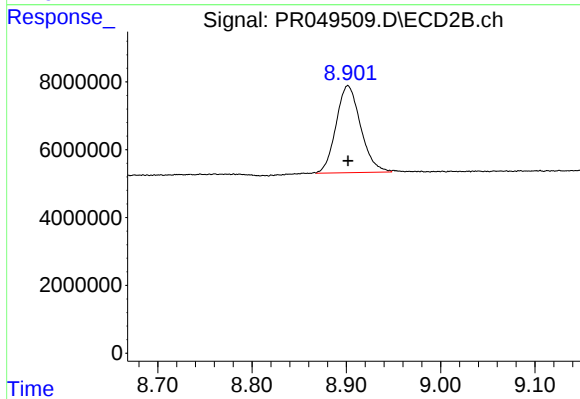

#2 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: 0.000 min
Response: 46526731
Conc: 4.99 ng/ml

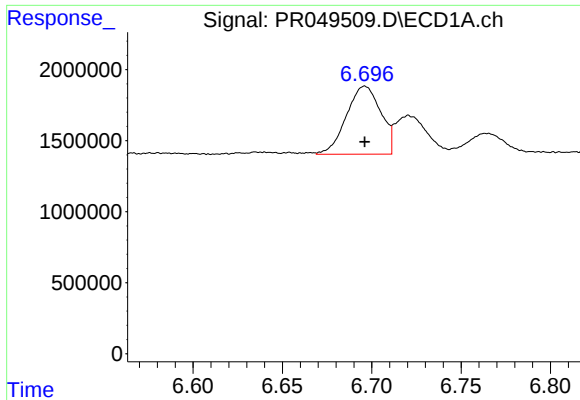


#26 AR-1254-1

R.T.: 6.696 min
Delta R.T.: 0.000 min
Response: 6409094
Conc: 58.63 ng/ml

Instrument :
ECD_R
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
3/2/2021 11:27:54 AM

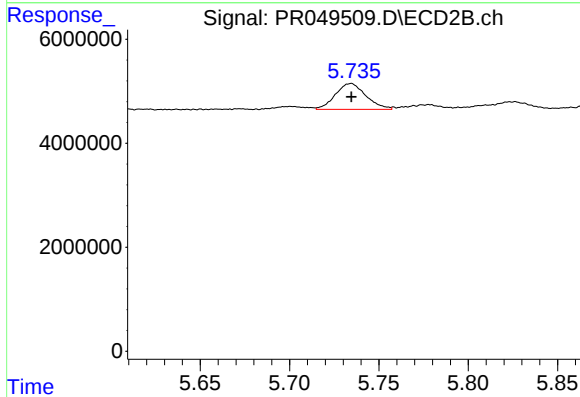


#26 AR-1254-1

R.T.: 5.735 min
Delta R.T.: 0.000 min
Response: 5893323
Conc: 52.93 ng/ml m

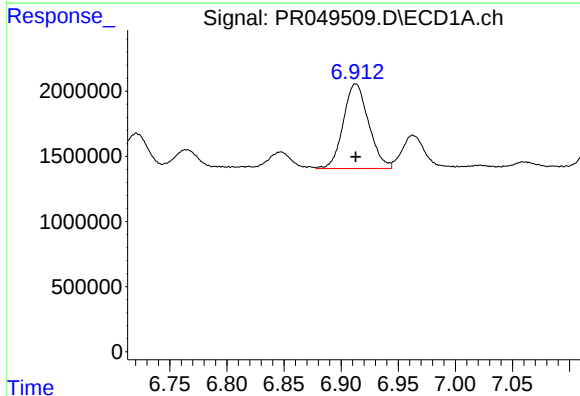


#27 AR-1254-2

R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 9995066
Conc: 59.20 ng/ml

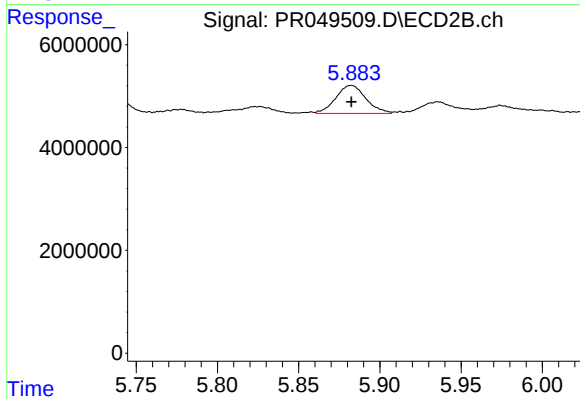

#27 AR-1254-2

R.T.: 5.883 min
Delta R.T.: 0.000 min
Response: 7049817
Conc: 57.81 ng/ml m

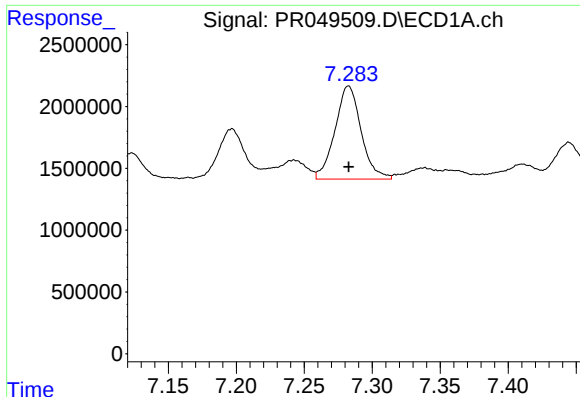


#28 AR-1254-3

R.T.: 7.283 min
Delta R.T.: 0.000 min
Response: 10087114
Conc: 58.38 ng/ml

Instrument :
ECD_R
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
3/2/2021 11:27:54 AM

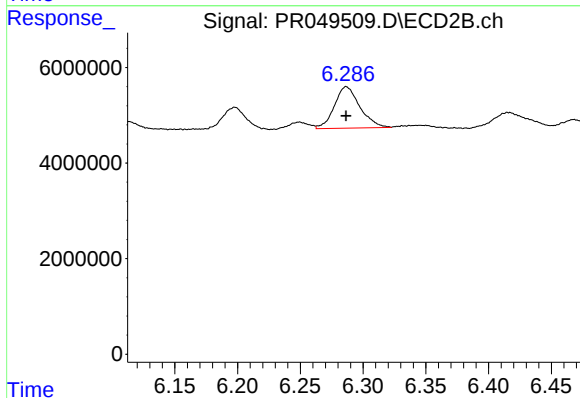


#28 AR-1254-3

R.T.: 6.287 min
Delta R.T.: 0.000 min
Response: 12270289
Conc: 52.39 ng/ml

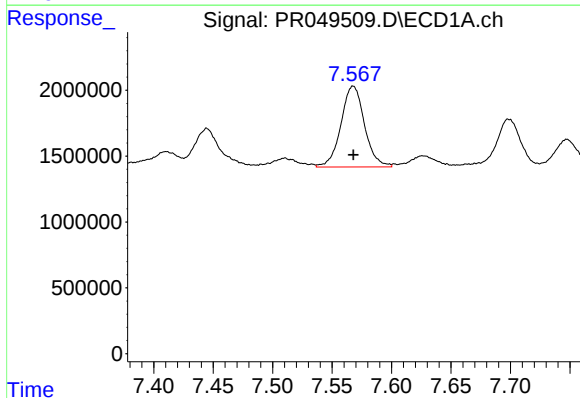


#29 AR-1254-4

R.T.: 7.568 min
Delta R.T.: 0.000 min
Response: 8482307
Conc: 59.28 ng/ml

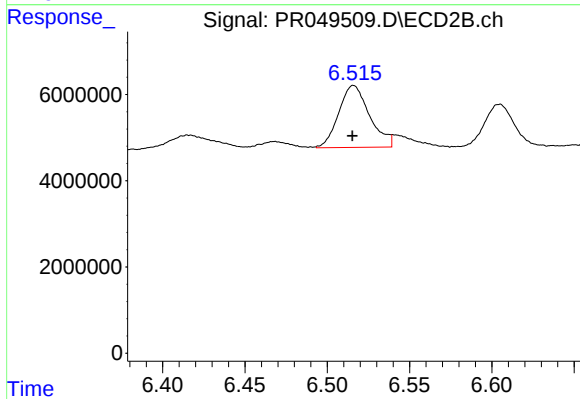

#29 AR-1254-4

R.T.: 6.515 min
Delta R.T.: 0.000 min
Response: 18825550
Conc: 51.90 ng/ml m

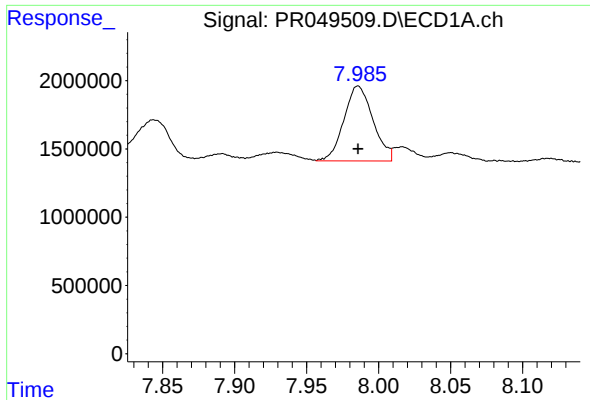


#30 AR-1254-5

R.T.: 7.986 min
Delta R.T.: 0.000 min
Response: 7730329
Conc: 55.33 ng/ml

Instrument :
ECD_R
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Ankita
3/2/2021 11:27:54 AM

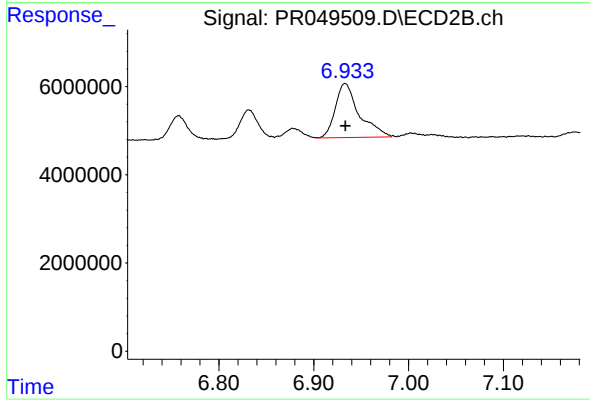

#30 AR-1254-5

R.T.: 6.933 min
Delta R.T.: 0.000 min
Response: 21427718
Conc: 49.97 ng/ml