
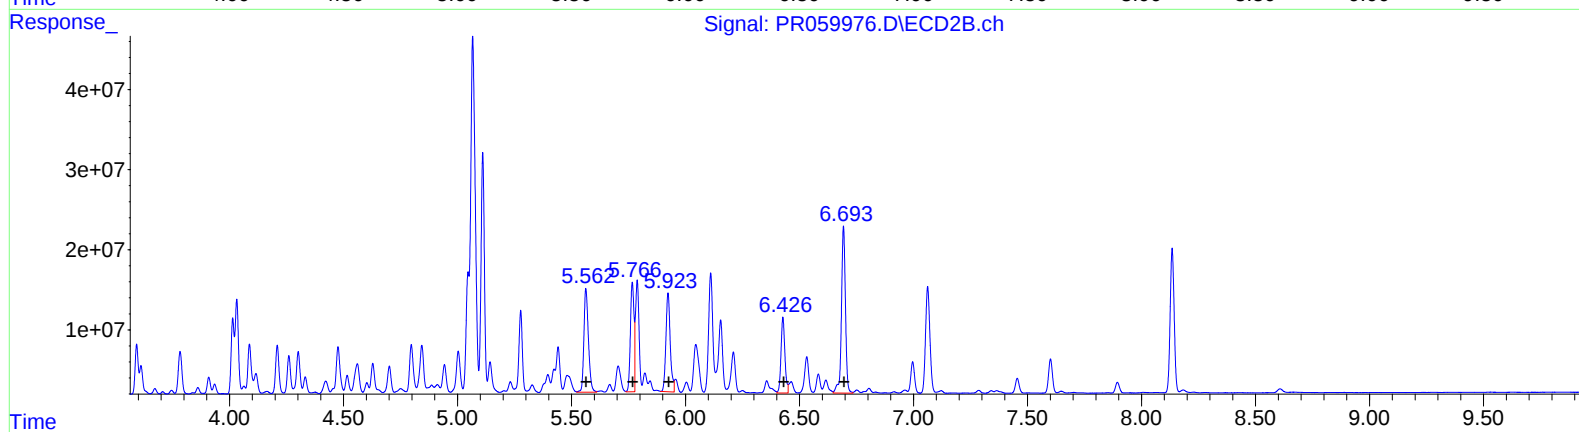


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR030223\
Data File : PR059976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2023 04:47
Operator : YP\AJ
Sample : 01696-14MSD
Misc :
ALS Vial : 49 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 06:18:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR022823CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 28 05:24:37 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

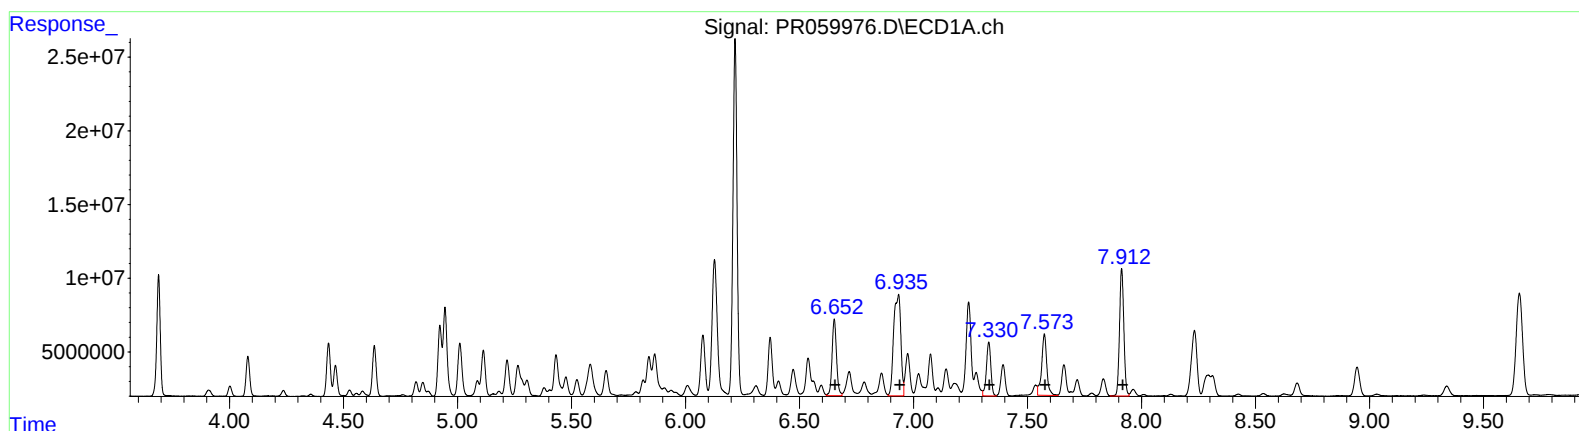

QEdit



(31) AR-1260-1 (L7)
R.T. Response Conc
6.65 70289050 571.36
6.93 149079443 1061.14
7.33 49520721 457.22
7.57 65064179 527.45
7.91 114117427 495.94

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
5.56 177959448 778.15
5.77 149968591 557.52
5.92 162617542 641.97
6.43 111816156 531.62
6.69 254811106 536.10

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR030223\
Data File : PR059976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2023 04:47
Operator : YP\AJ
Sample : 01696-14MSD
Misc :
ALS Vial : 49 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 06:18:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR022823CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 28 05:24:37 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

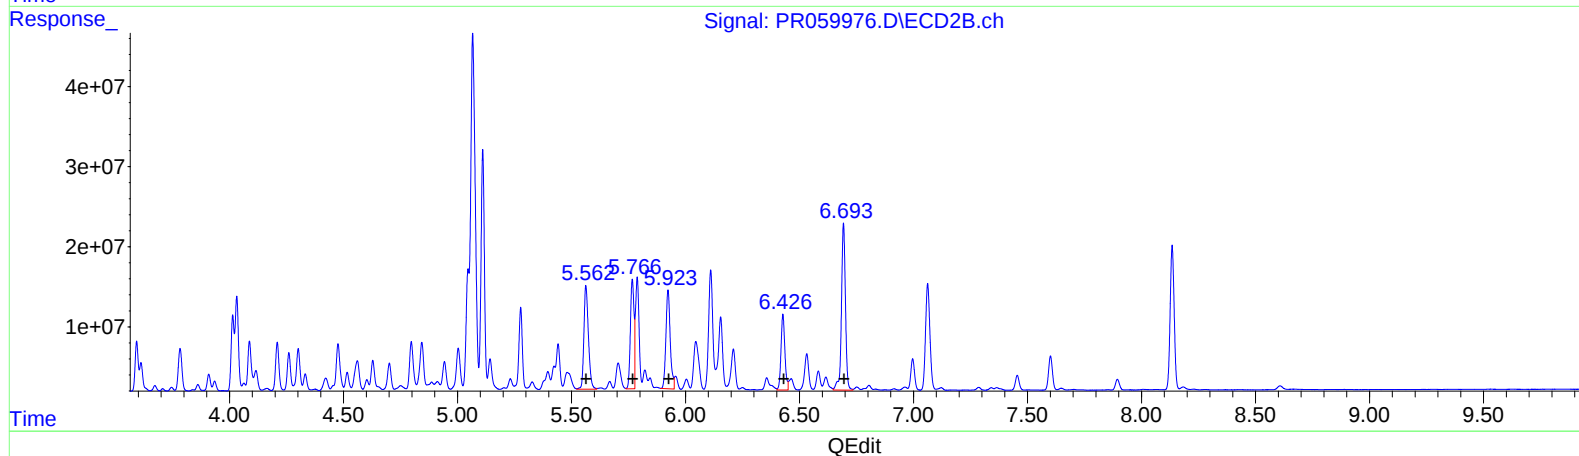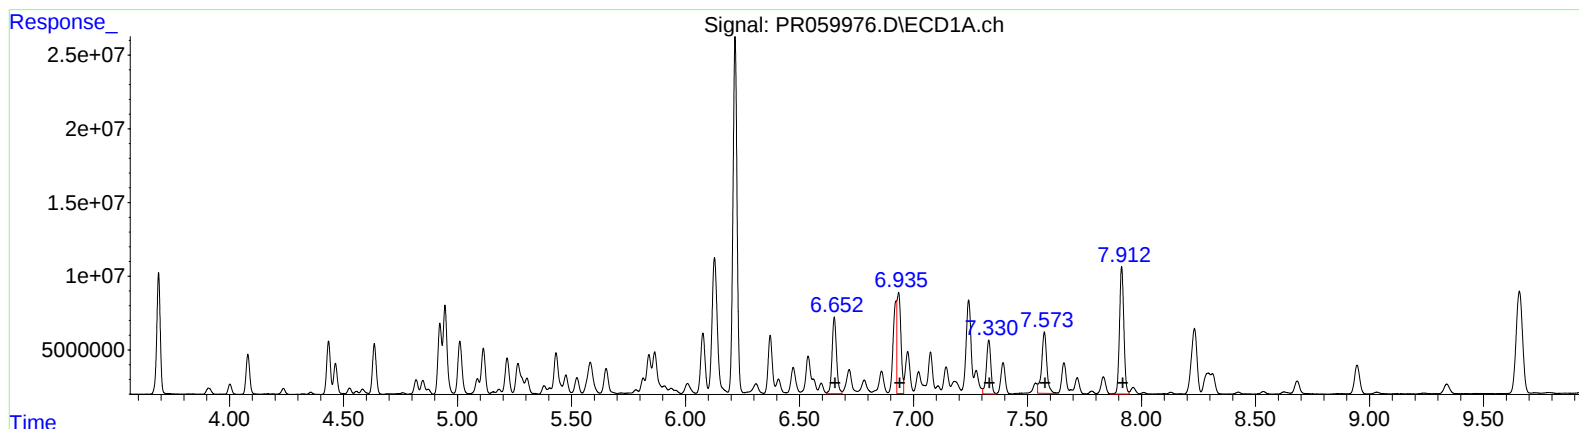

QEdit

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
6.65 70289050 571.36
6.93 81233856 578.22
7.33 49520721 457.22
7.57 65064179 527.45
7.91 114117427 495.94

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
5.56 177959448 778.15
5.77 149968591 557.52
5.92 162617542 641.97
6.43 111816156 531.62
6.69 254811106 536.10