

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR030321\
 Data File : PR049524.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2021 11:05
 Operator : AJ\MA
 Sample : M1521-05RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 OB-722RE

Manual Integrations
 APPROVED

Ankita
 3/4/2021 9:09:52 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 16:18:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR030221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 02 08:11:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.667	3.845	28115401	37428982	10.607m	11.893m
2) SA Decachlor...	10.549	8.902	35022730	91770489	12.330	10.107

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR030321\
Data File : PR049524.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2021 11:05
Operator : AJ\MA
Sample : M1521-05RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
OB-722RE


Manual Integrations
APPROVED

Ankita
3/4/2021 9:09:52 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 16:18:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR030221.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 02 08:11:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

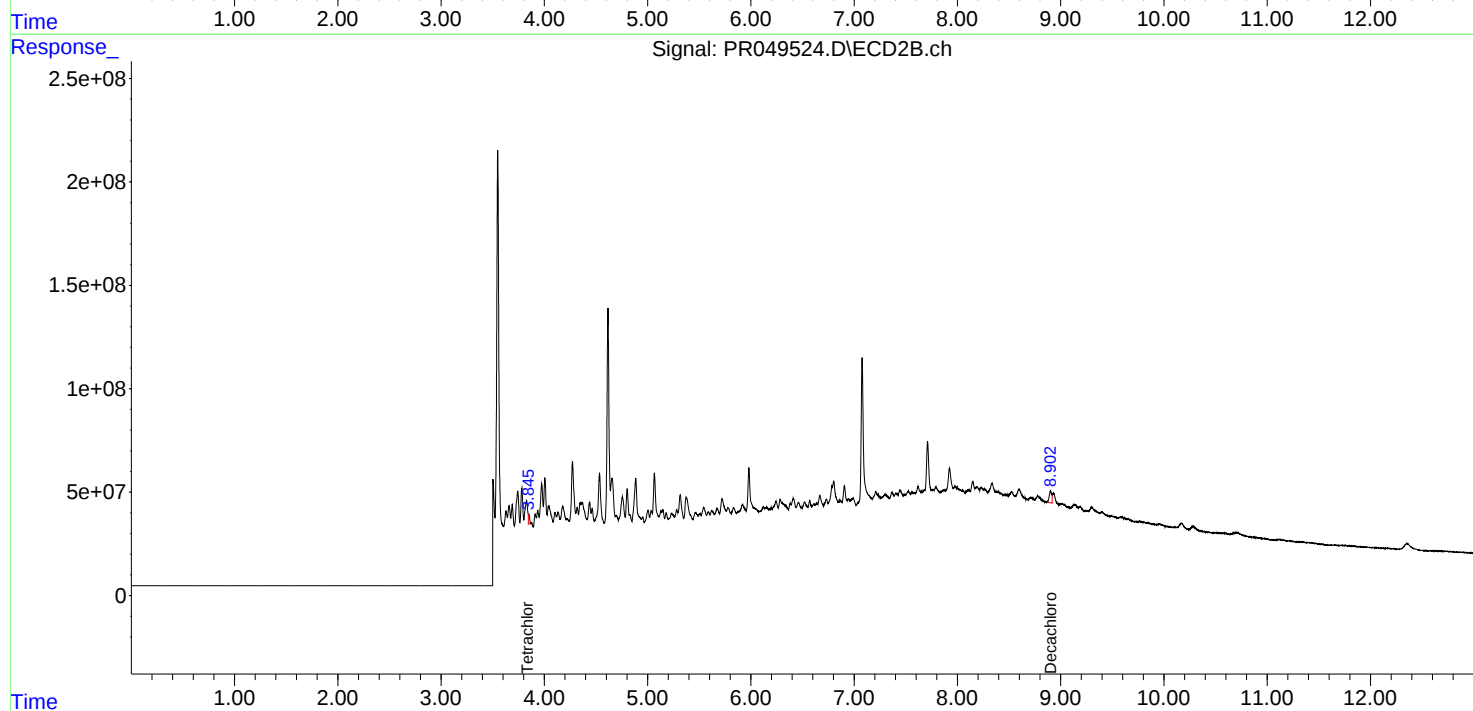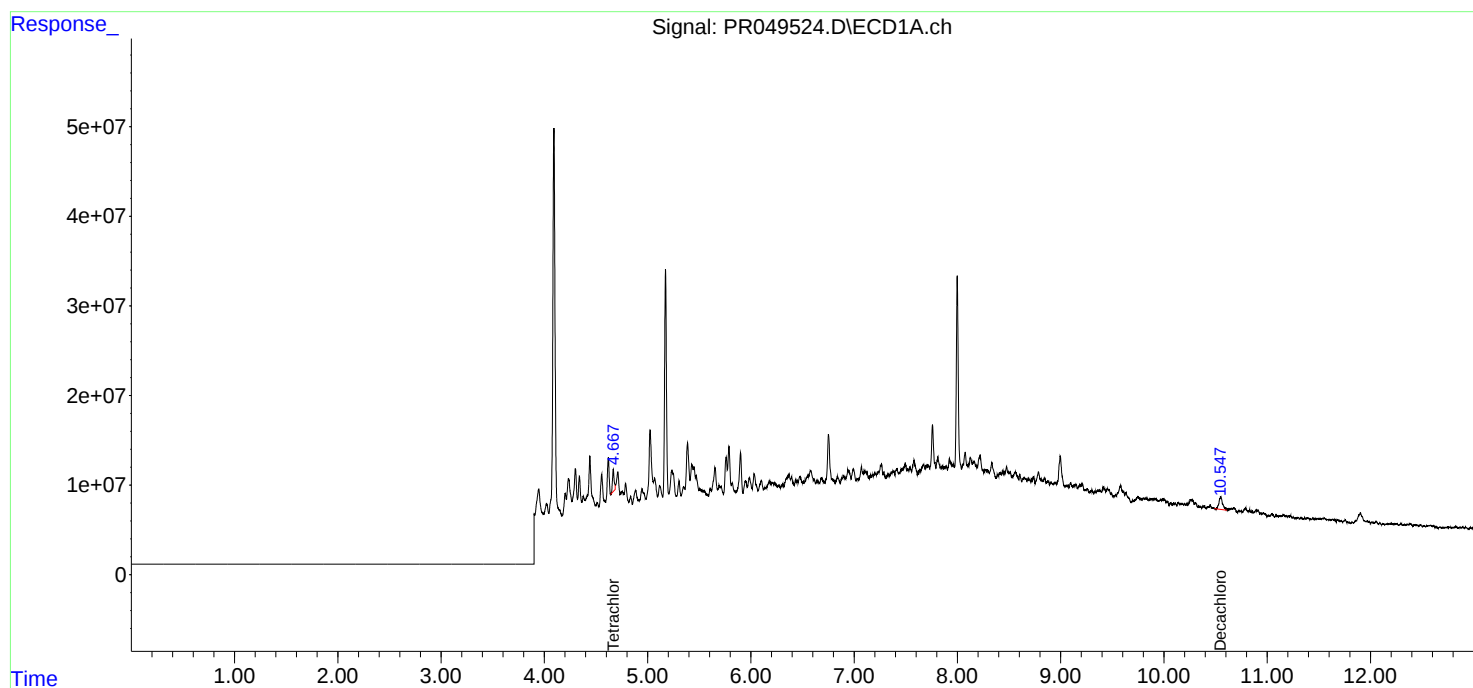

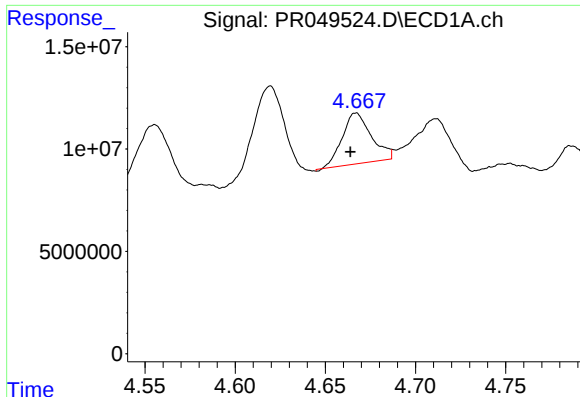


#1 Tetrachloro-m-xylene

R.T.: 4.667 min
Delta R.T.: 0.003 min
Response: 28115401
Conc: 10.61 ng/ml m

Instrument :
ECD_R
ClientSampleId :
OB-722RE


Manual Integrations
APPROVED

Ankita
3/4/2021 9:09:52 AM

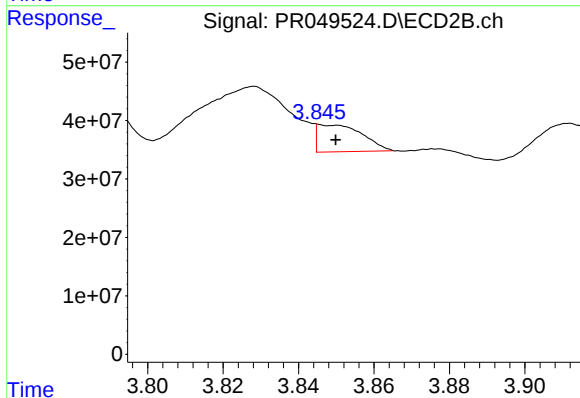


#1 Tetrachloro-m-xylene

R.T.: 3.845 min
Delta R.T.: -0.005 min
Response: 37428982
Conc: 11.89 ng/ml m

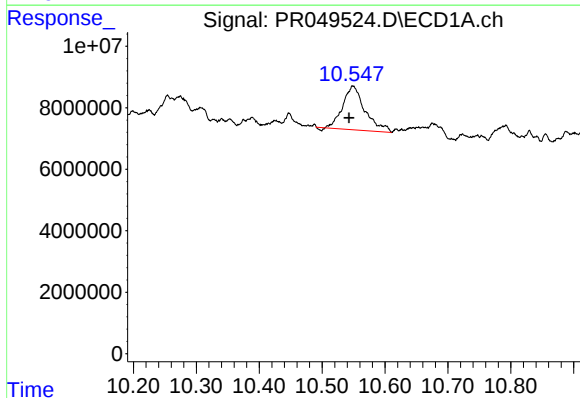

#2 Decachlorobiphenyl

R.T.: 10.549 min
Delta R.T.: 0.006 min
Response: 35022730
Conc: 12.33 ng/ml

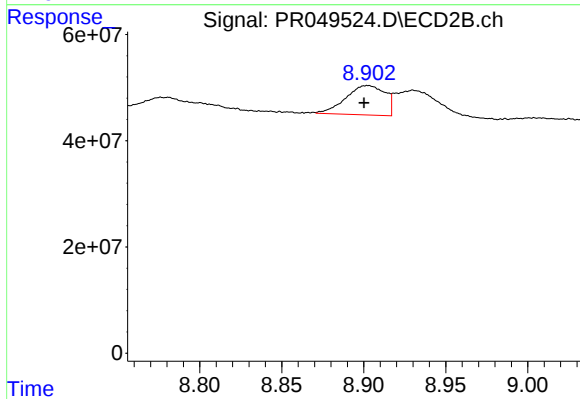

#2 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: 0.002 min
Response: 91770489
Conc: 10.11 ng/ml