

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR030321\
 Data File : PR049525.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2021 11:21
 Operator : AJ\MA
 Sample : M1520-02RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 NCQ-632RE

Manual Integrations
 APPROVED

Ankita
 3/4/2021 9:09:54 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 16:19:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR030221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 02 08:11:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.669	3.844	17502161	44987839	6.603m	14.295m#
2) SA Decachlor...	10.545	8.902	12855636	74821558	4.526	8.241 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR030321\
Data File : PR049525.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2021 11:21
Operator : AJ\MA
Sample : M1520-02RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
NCQ-632RE


Manual Integrations
APPROVED

Ankita
3/4/2021 9:09:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 16:19:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR030221.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 02 08:11:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

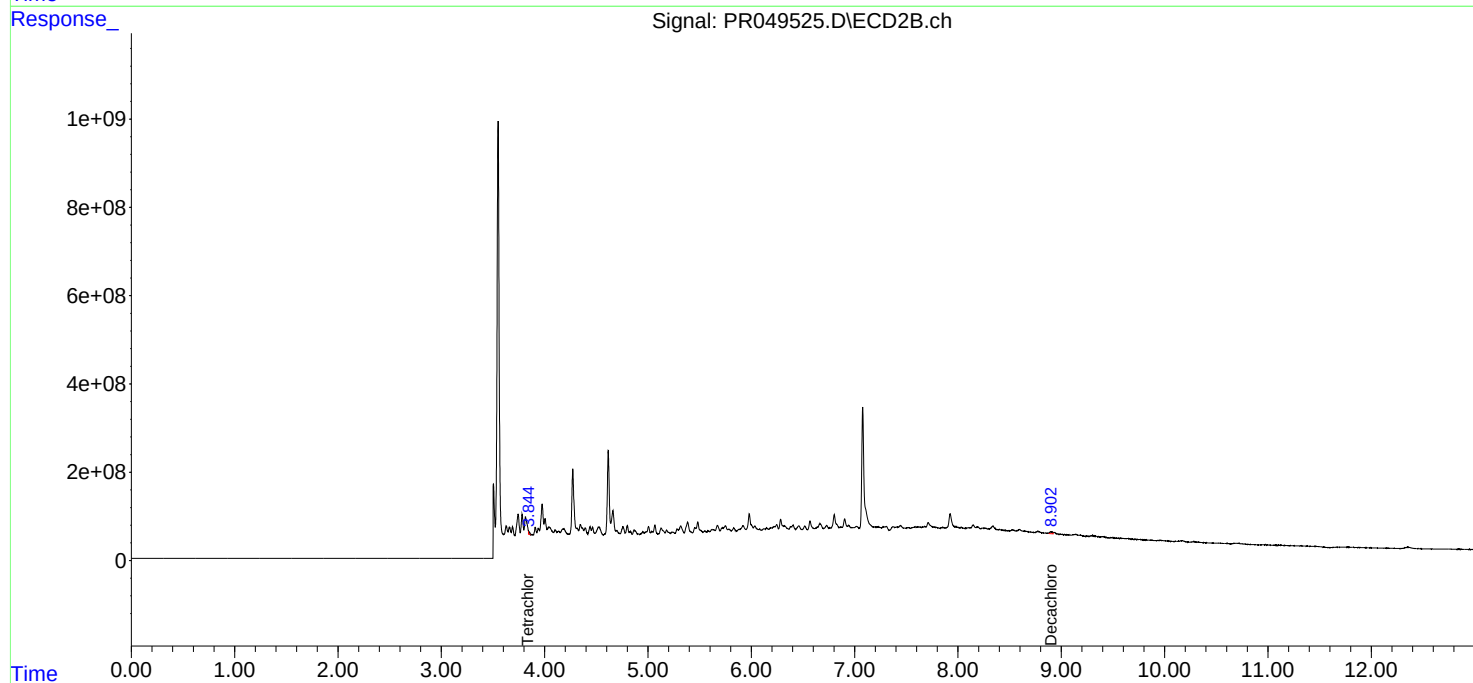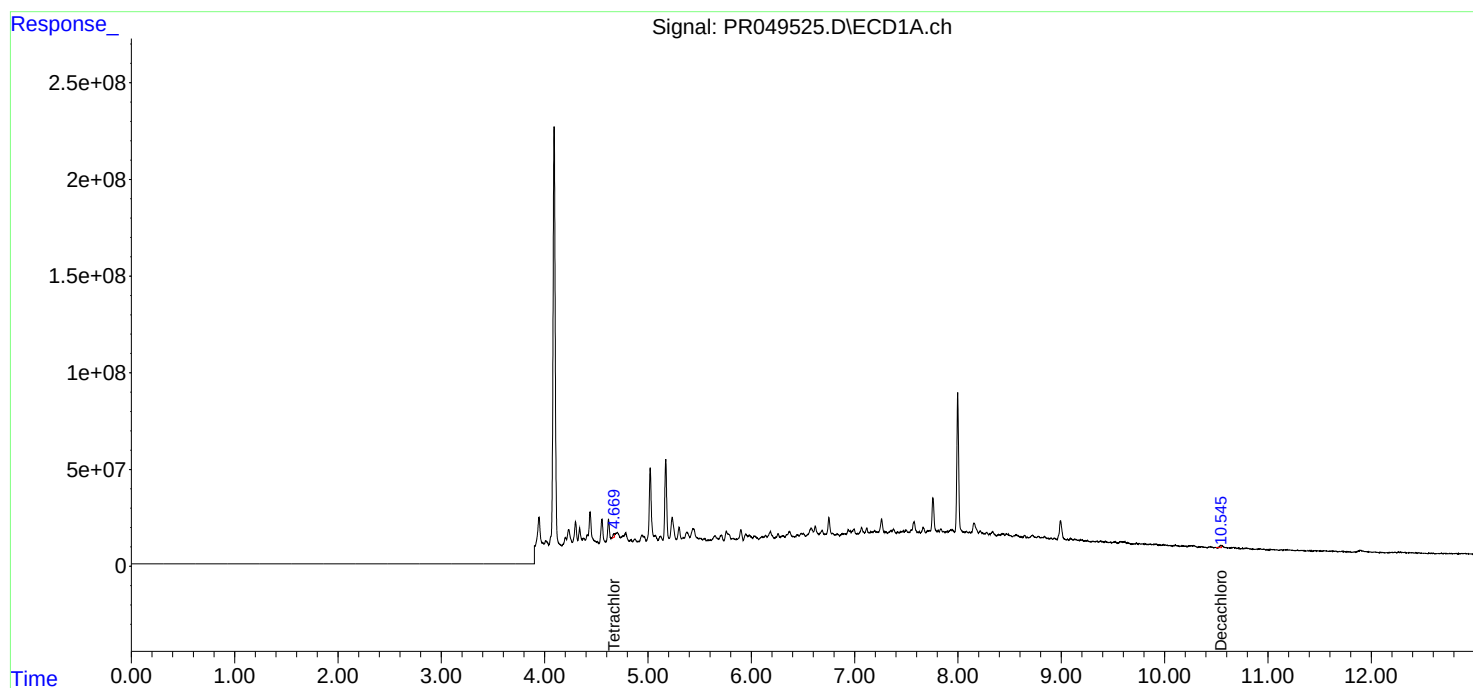

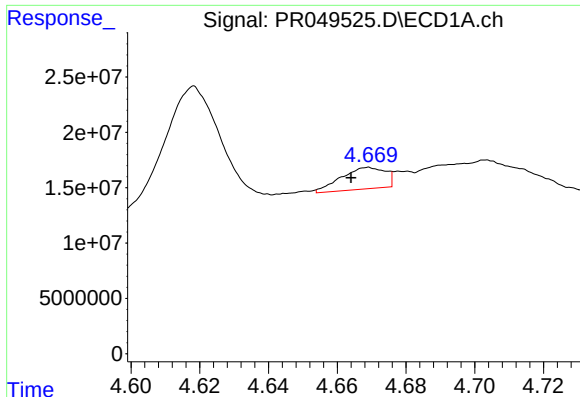


#1 Tetrachloro-m-xylene

R.T.: 4.669 min
Delta R.T.: 0.005 min
Response: 17502161
Conc: 6.60 ng/ml m

Instrument :
ECD_R
ClientSampleId :
NCQ-632RE


Manual Integrations
APPROVED

Ankita
3/4/2021 9:09:54 AM

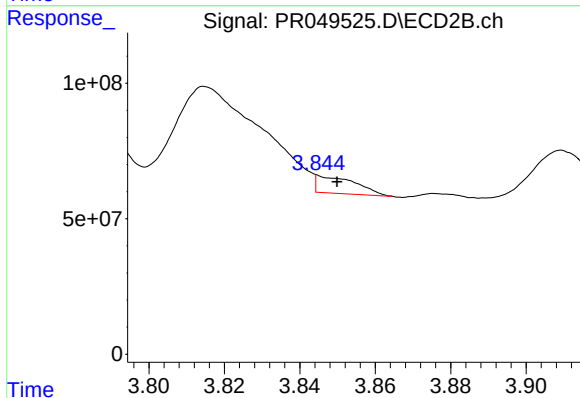


#1 Tetrachloro-m-xylene

R.T.: 3.844 min
Delta R.T.: -0.006 min
Response: 44987839
Conc: 14.29 ng/ml m

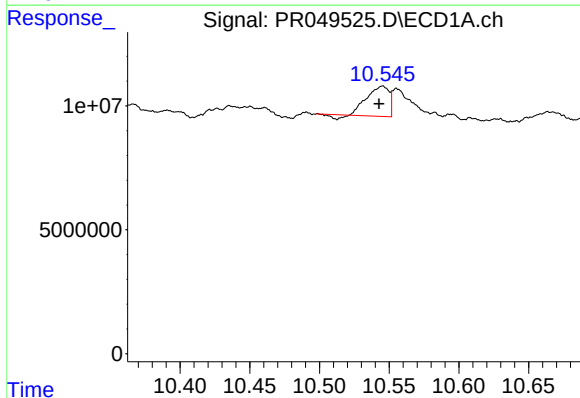

#2 Decachlorobiphenyl

R.T.: 10.545 min
Delta R.T.: 0.003 min
Response: 12855636
Conc: 4.53 ng/ml

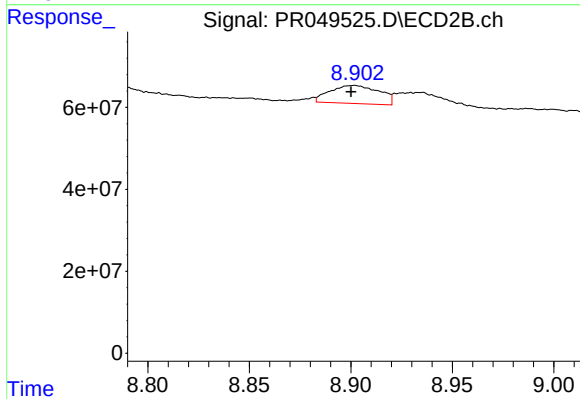

#2 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: 0.002 min
Response: 74821558
Conc: 8.24 ng/ml