

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR030423\
 Data File : PR060014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2023 10:30
 Operator : YP\AJ
 Sample : 01697-02MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1


Instrument :
 ECD_R
 ClientSampleId :
 EXHM9MS

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/06/2023
 Supervised By :Ankita Jodhani 03/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 20:53:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR022823CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 28 05:24:37 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

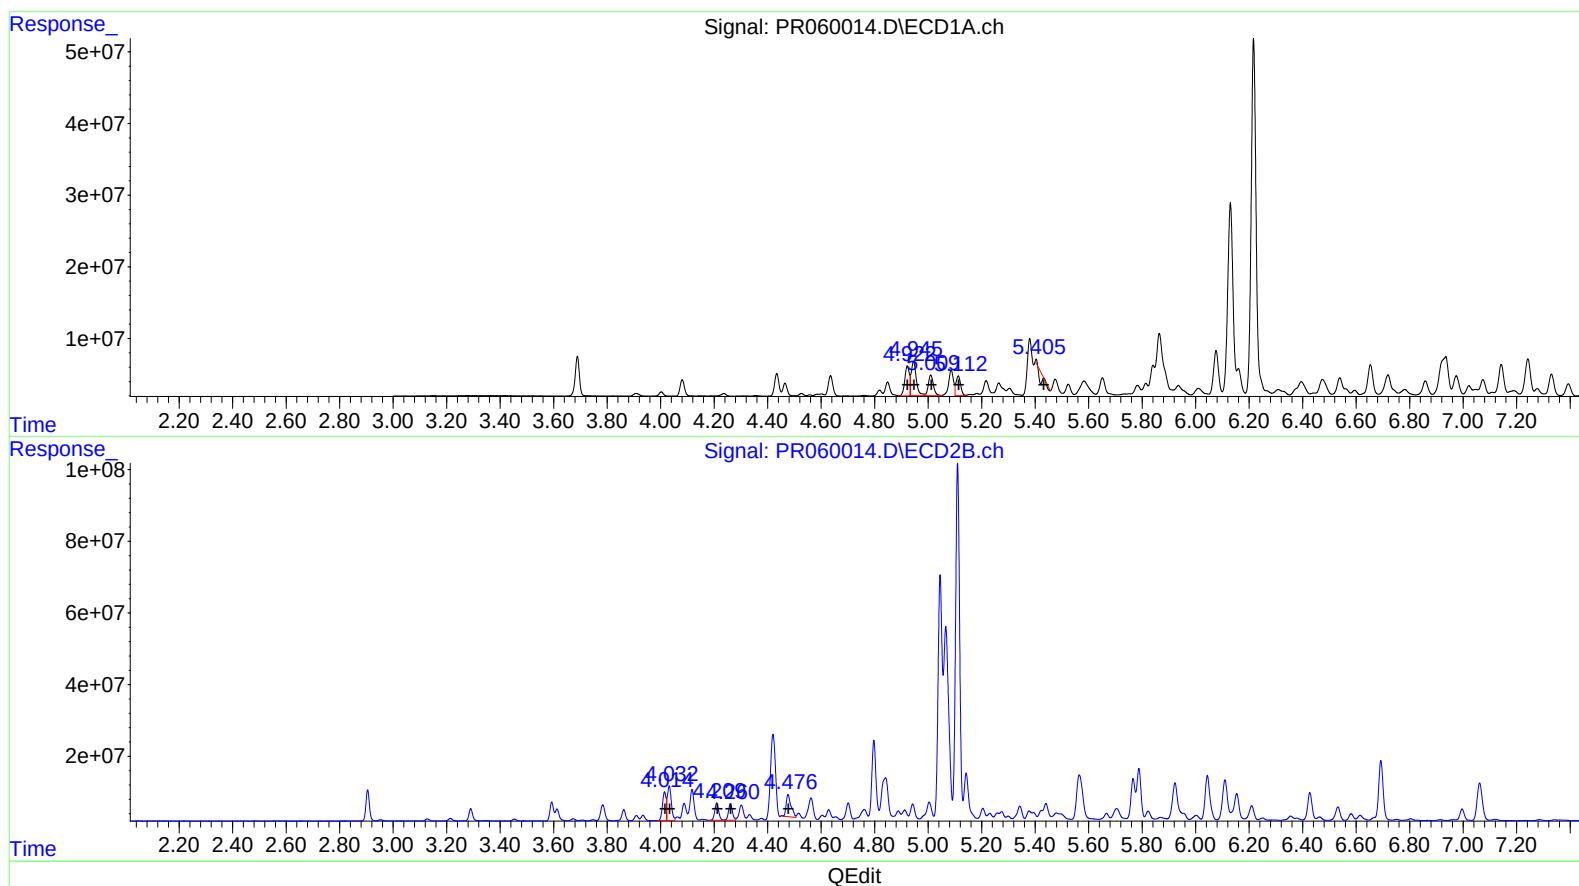

(3) AR-1016-1 (L1)

R.T.	Response	Conc
4.92	49718294	529.20
4.95	64300091	476.66
5.01	38526507	441.62
5.11	32963027	475.38
5.43	-13904800	-206.06

(3) AR-1016-1 #2 (L1)

R.T.	Response	Conc
4.01	74963972	546.11
4.03	101078649	494.64
4.21	49447692	470.57
4.26	47194065	549.59
4.48	78430535	701.01

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR030423\
 Data File : PR060014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2023 10:30
 Operator : YP\AJ
 Sample : 01697-02MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1



Instrument :
 ECD_R
 ClientSampleId :
 EXHM9MS

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/06/2023
 Supervised By :Ankita Jodhani 03/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 20:53:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR022823CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 28 05:24:37 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

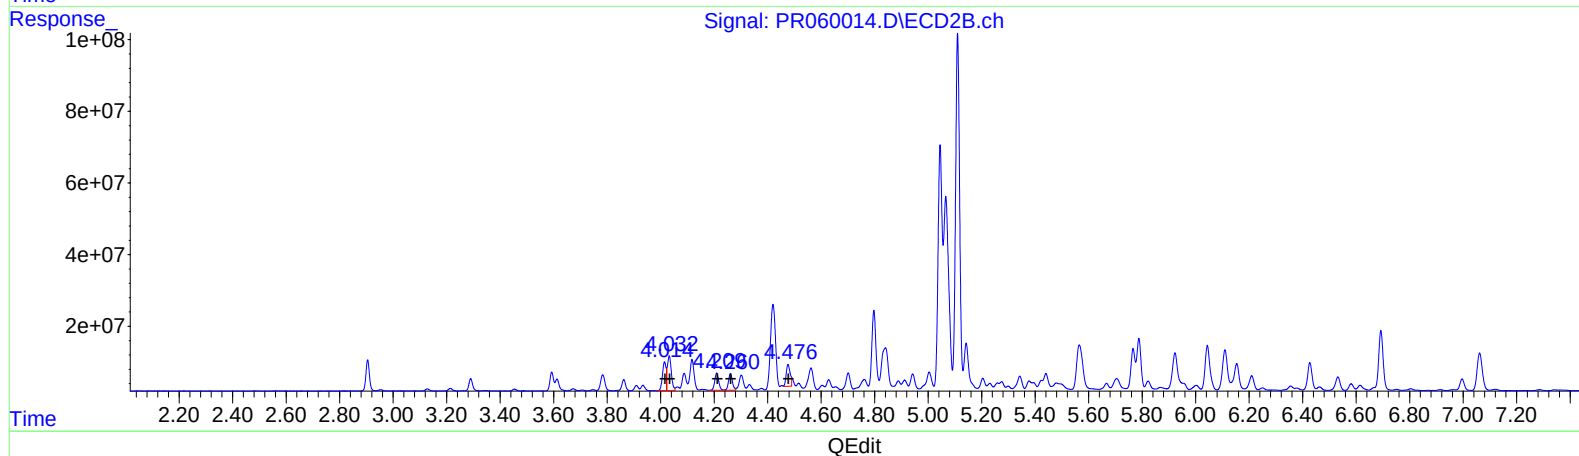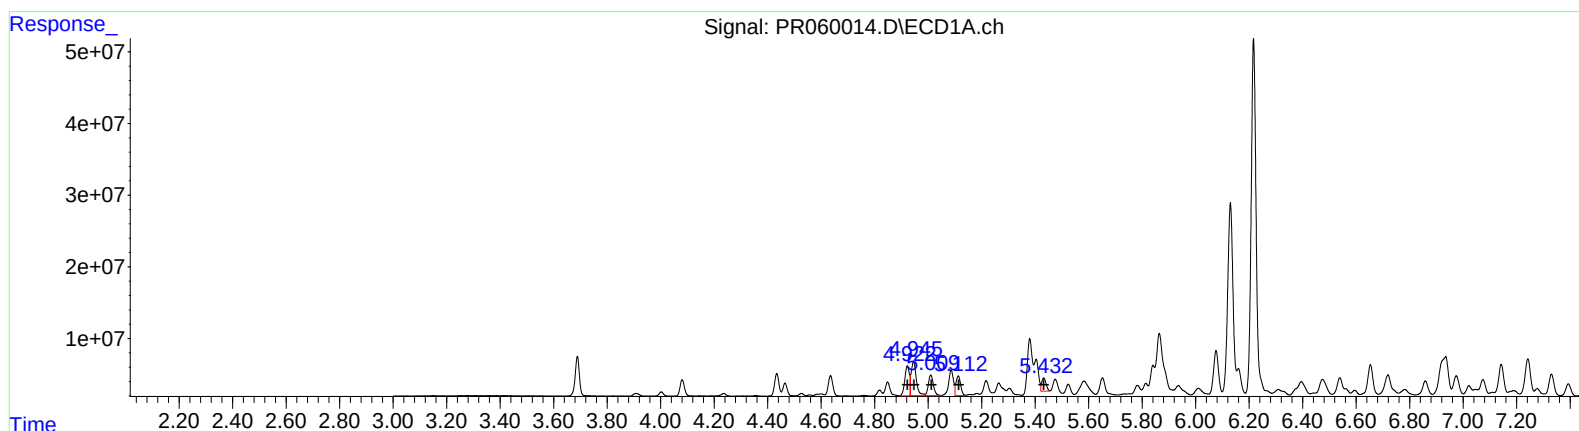

QEdit

(3) AR-1016-1 #2 (L1)		
R.T.	Response	Conc
4.92	49718294	529.20
4.95	64300091	476.66
5.01	38526507	441.62
5.11	32963027	475.38
5.43	20771441	307.81

(3) AR-1016-1 #2 (L1)		
R.T.	Response	Conc
4.01	74963972	546.11
4.03	101078649	494.64
4.21	49447692	470.57
4.26	47194065	549.59
4.48	63175277	564.66

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR030423\
 Data File : PR060014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2023 10:30
 Operator : YP\AJ
 Sample : 01697-02MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1



Instrument :
 ECD_R
 ClientSampleId :
 EXHM9MS

Manual IntegrationsAPPROVED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 20:53:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR022823CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 28 05:24:37 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Reviewed By :Yogesh Patel 03/06/2023
 Supervised By :Ankita Jodhani 03/06/2023

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

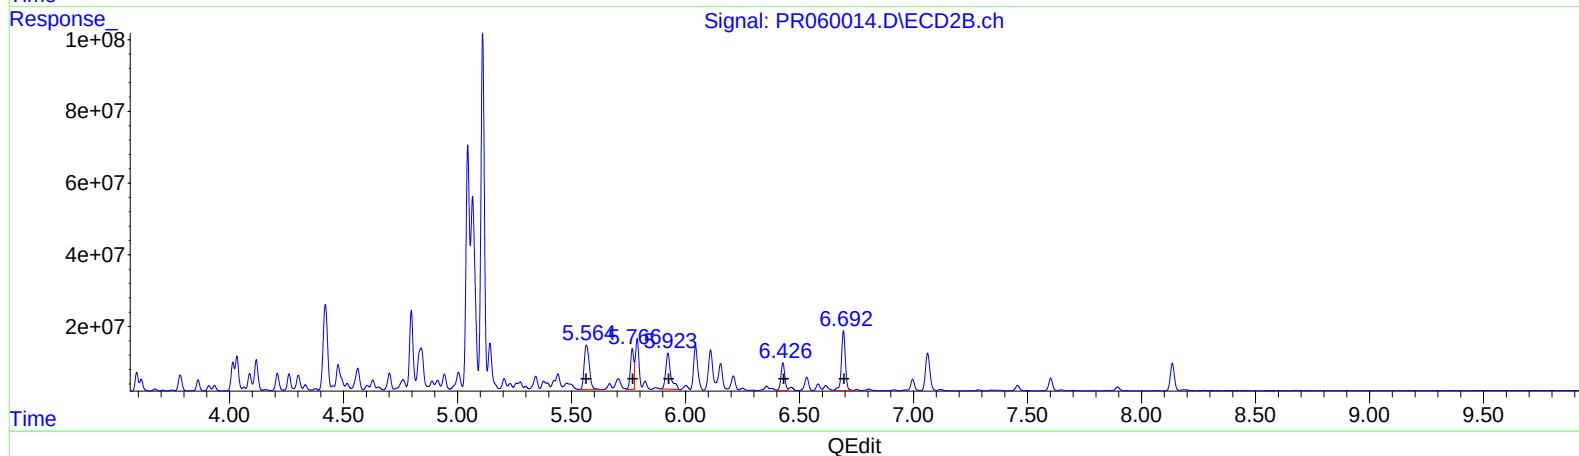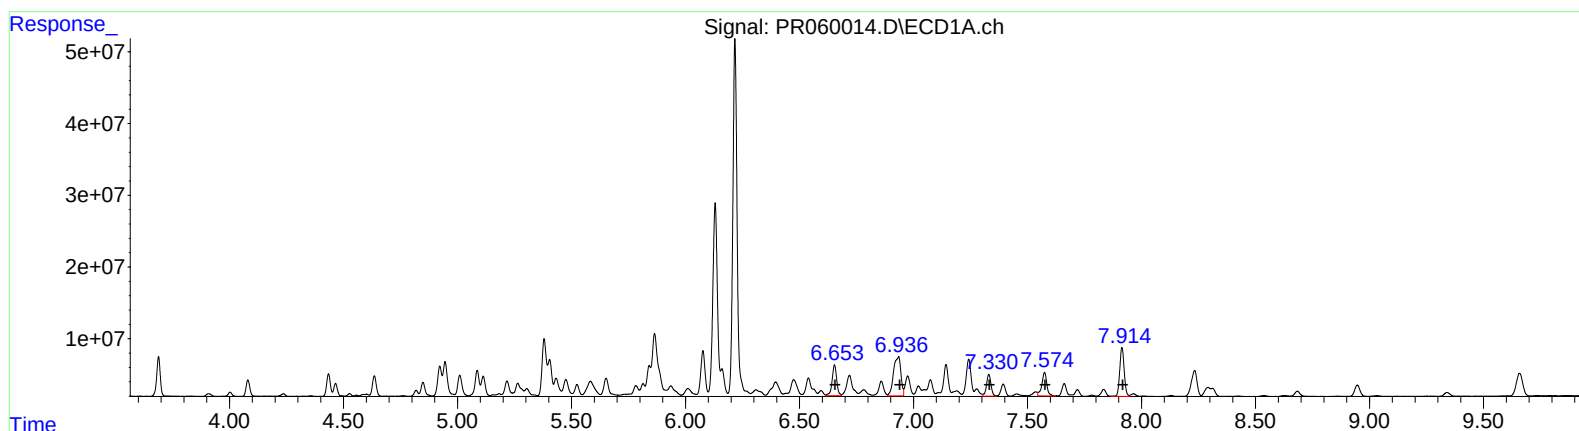

(31) AR-1260-1 (L7)
 R.T. Response Conc
 6.65 59580396 484.31
 6.94 121585154 865.43
 7.33 41785487 385.80
 7.57 50231128 407.20
 7.91 92368051 401.42

(31) AR-1260-1 #2 (L7)
 R.T. Response Conc
 5.57 197253535 862.51
 5.77 117703656 437.58
 5.92 155454432 613.69
 6.43 90217966 428.93
 6.69 202603851 426.26

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR030423\
 Data File : PR060014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2023 10:30
 Operator : YP\AJ
 Sample : 01697-02MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1



Instrument :
 ECD_R
 ClientSampleId :
 EXHM9MS

Manual IntegrationsAPPROVED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 20:53:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR022823CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 28 05:24:37 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Reviewed By :Yogesh Patel 03/06/2023
 Supervised By :Ankita Jodhani 03/06/2023

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

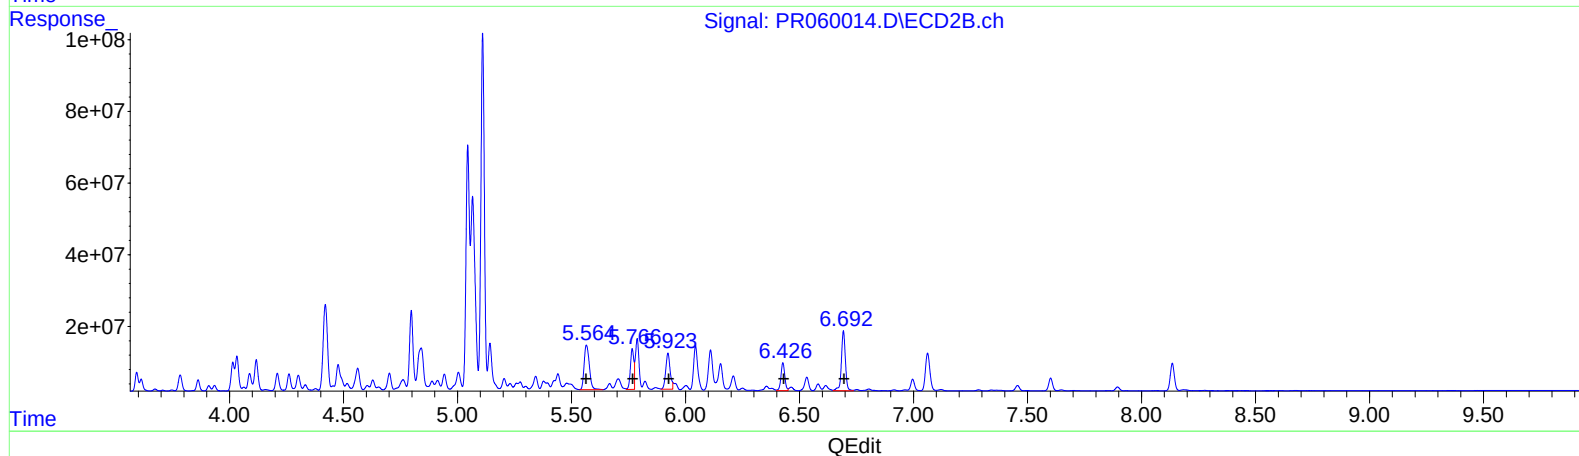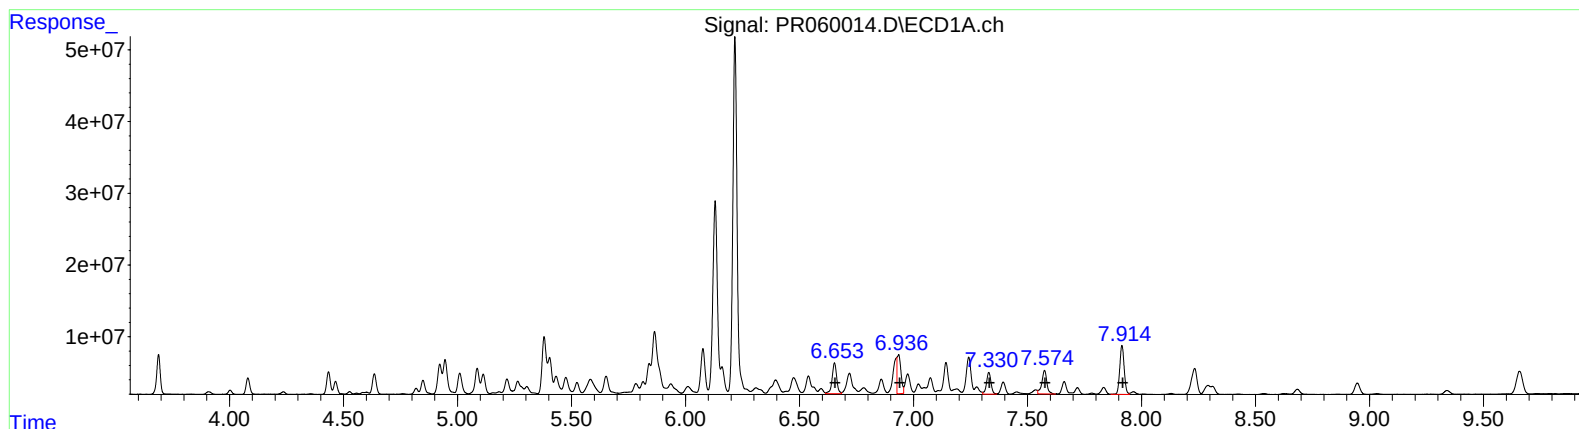

QEdit

(31) AR-1260-1 #2 (L7)	R.T.	Response	Conc
	6.65	59580396	484.31
	6.94	63732793	453.65
	7.33	41785487	385.80
	7.57	50231128	407.20
	7.91	92368051	401.42

(31) AR-1260-1 #2 (L7)	R.T.	Response	Conc
	5.57	197253535	862.51
	5.77	117703656	437.58
	5.92	133540786	527.18
	6.43	90217966	428.93
	6.69	202603851	426.26