

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR030719\
 Data File : PR035980.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2019 17:55
 Operator : SM\SJ
 Sample : K1757-03RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 TP-6CD-SRE

Manual Integrations
 APPROVED

Sohil
 3/8/2019 9:19:25 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 23:48:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR030119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 07 10:54:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.410	3.484	23788043	78489452	14.968	14.945
2) SA Decachlor...	10.070	8.354	14222937	48924168	8.894	7.454m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR030719\
Data File : PR035980.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2019 17:55
Operator : SM\SJ
Sample : K1757-03RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
TP-6CD-SRE


Manual Integrations
APPROVED

Sohil
3/8/2019 9:19:25 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 23:48:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR030119.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 07 10:54:32 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

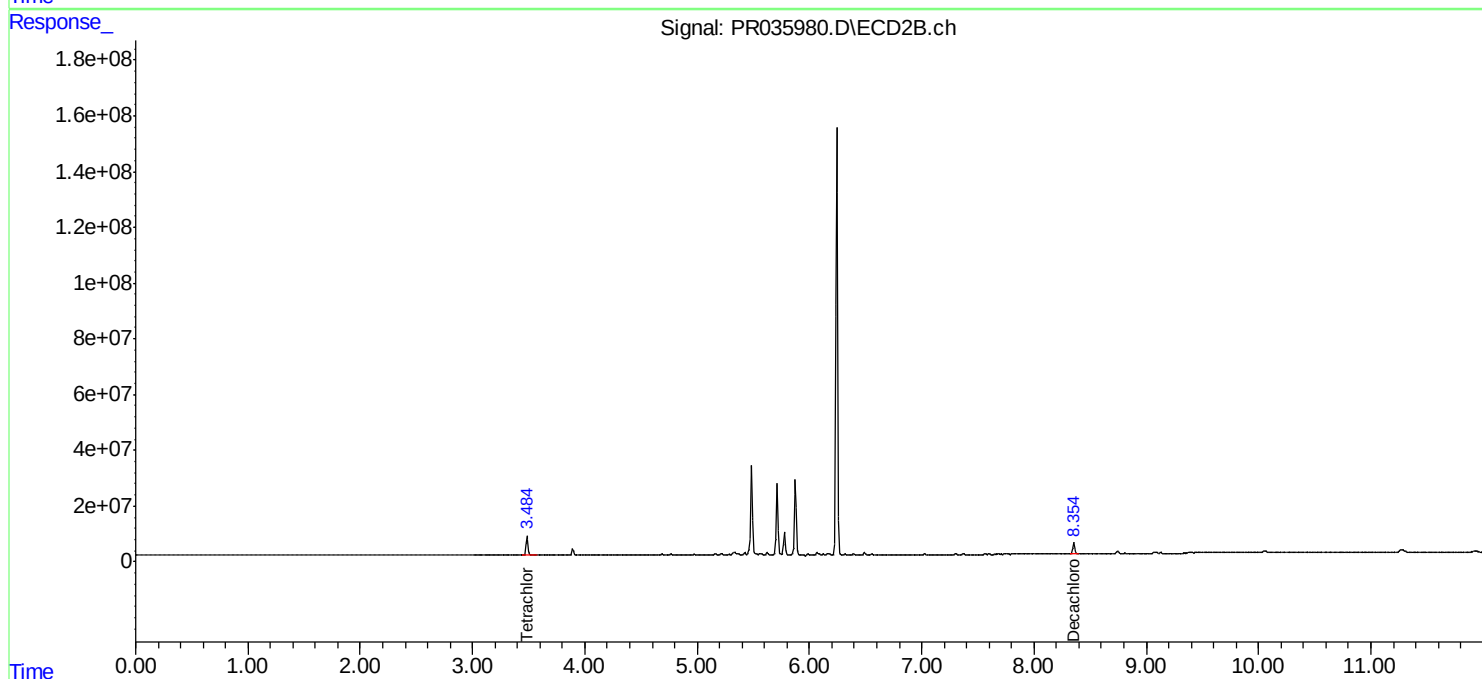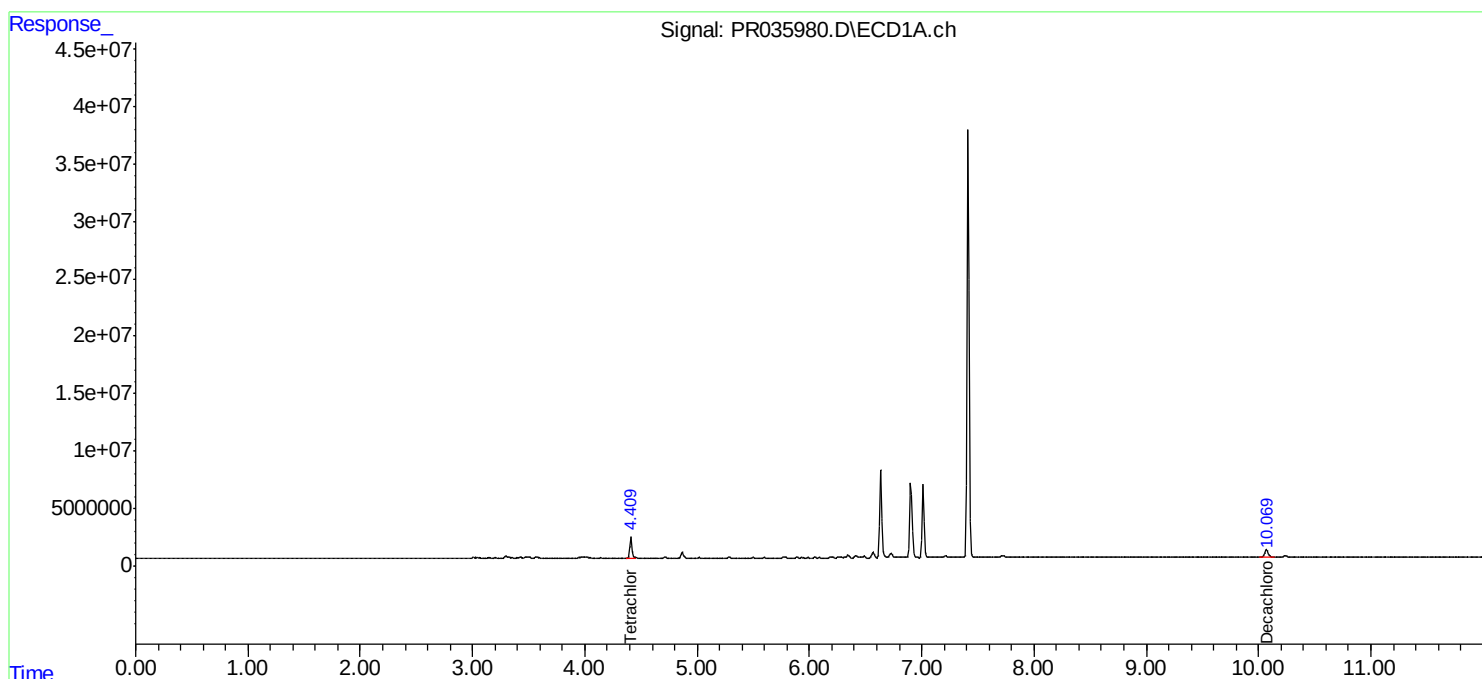

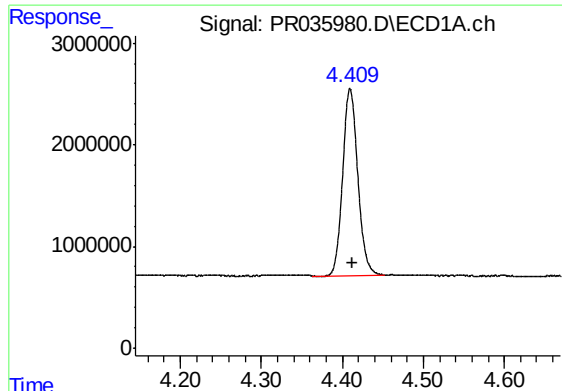


#1 Tetrachloro-m-xylene

R.T.: 4.410 min
Delta R.T.: -0.002 min
Response: 23788043
Conc: 14.97 ng/ml

Instrument :
ECD_R
ClientSampleId :
TP-6CD-SRE


Manual Integrations
APPROVED

Sohil
3/8/2019 9:19:25 AM

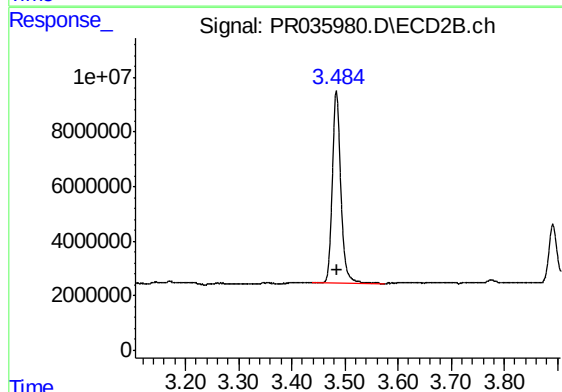


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: -0.002 min
Response: 78489452
Conc: 14.94 ng/ml

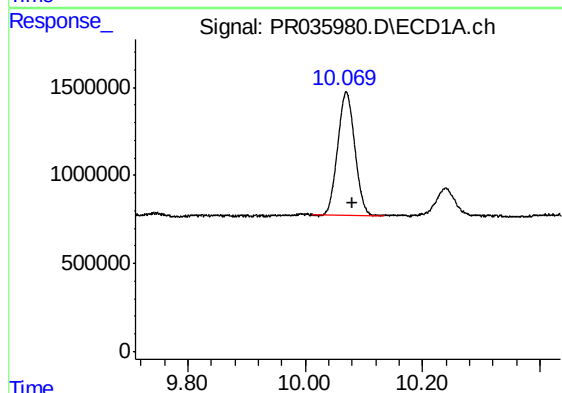

#2 Decachlorobiphenyl

R.T.: 10.070 min
Delta R.T.: -0.010 min
Response: 14222937
Conc: 8.89 ng/ml

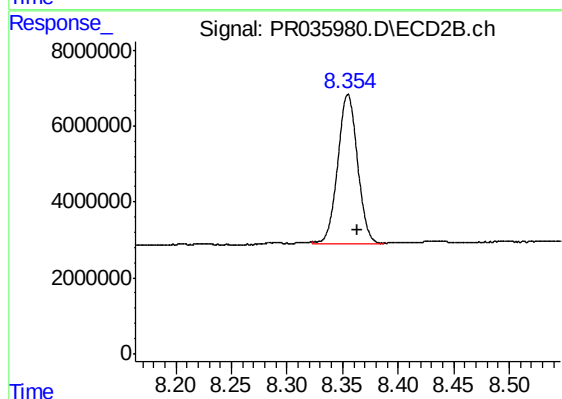

#2 Decachlorobiphenyl

R.T.: 8.354 min
Delta R.T.: -0.009 min
Response: 48924168
Conc: 7.45 ng/ml m