

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR031222\
 Data File : PR054003.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2022 08:49
 Operator : AJ\MA
 Sample : N1645-09
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT1-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 23:21:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR031122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 10 01:38:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.557	2.805	38834624	24360160	20.399	19.365
2) SA Decachlor...	9.361	7.949	37371489	28178832	22.291	21.550
Target Compounds						
11) L3 AR-1232-1	3.951	3.182	1128957	625993	29.591	23.712
12) L3 AR-1232-2	4.492	3.906	621604	899615	29.358	29.249
13) L3 AR-1232-3	4.799	4.078	995660	412707	24.979	25.924
14) L3 AR-1232-4	4.967	4.169	443674	496969	22.783	36.014 #
15) L3 AR-1232-5	5.065	4.339	363851	392138	25.141	24.593



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR031222\
Data File : PR054003.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2022 08:49
Operator : AJ\MA
Sample : N1645-09
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 23:21:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR031122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 10 01:38:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

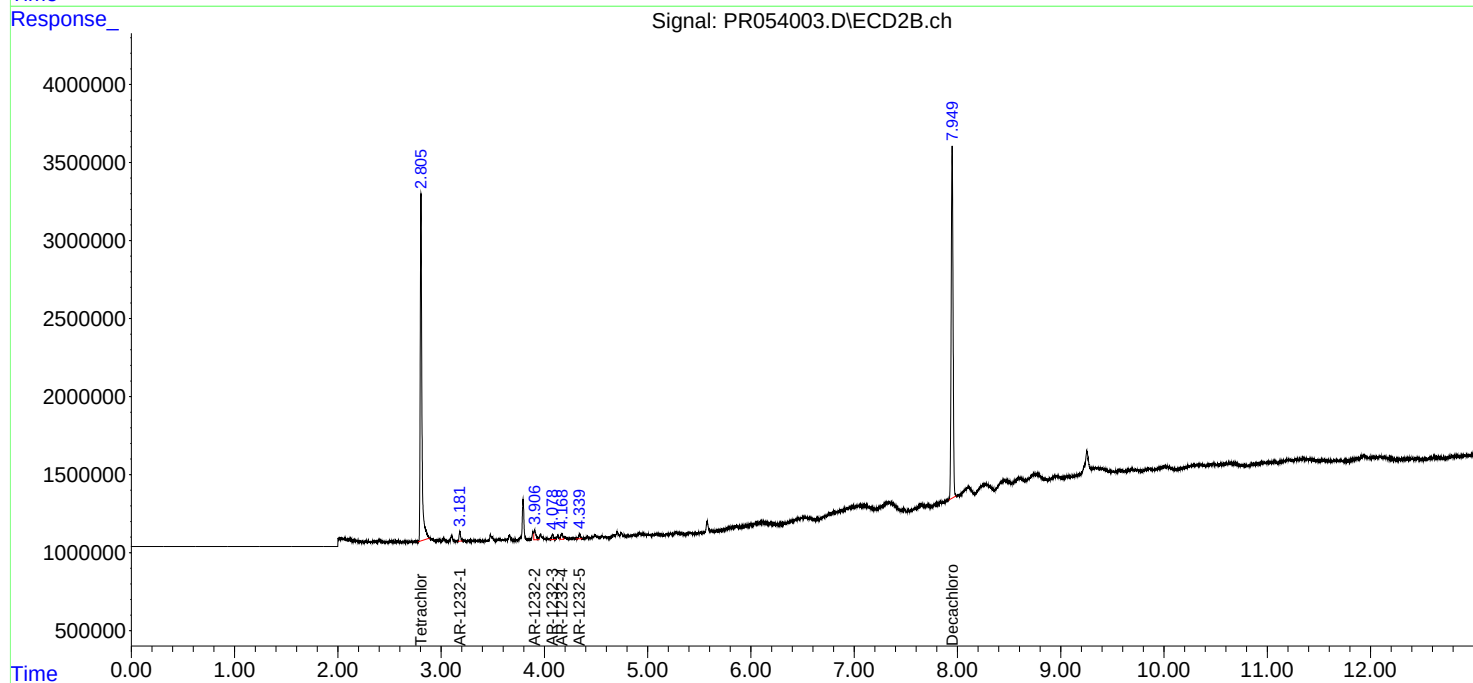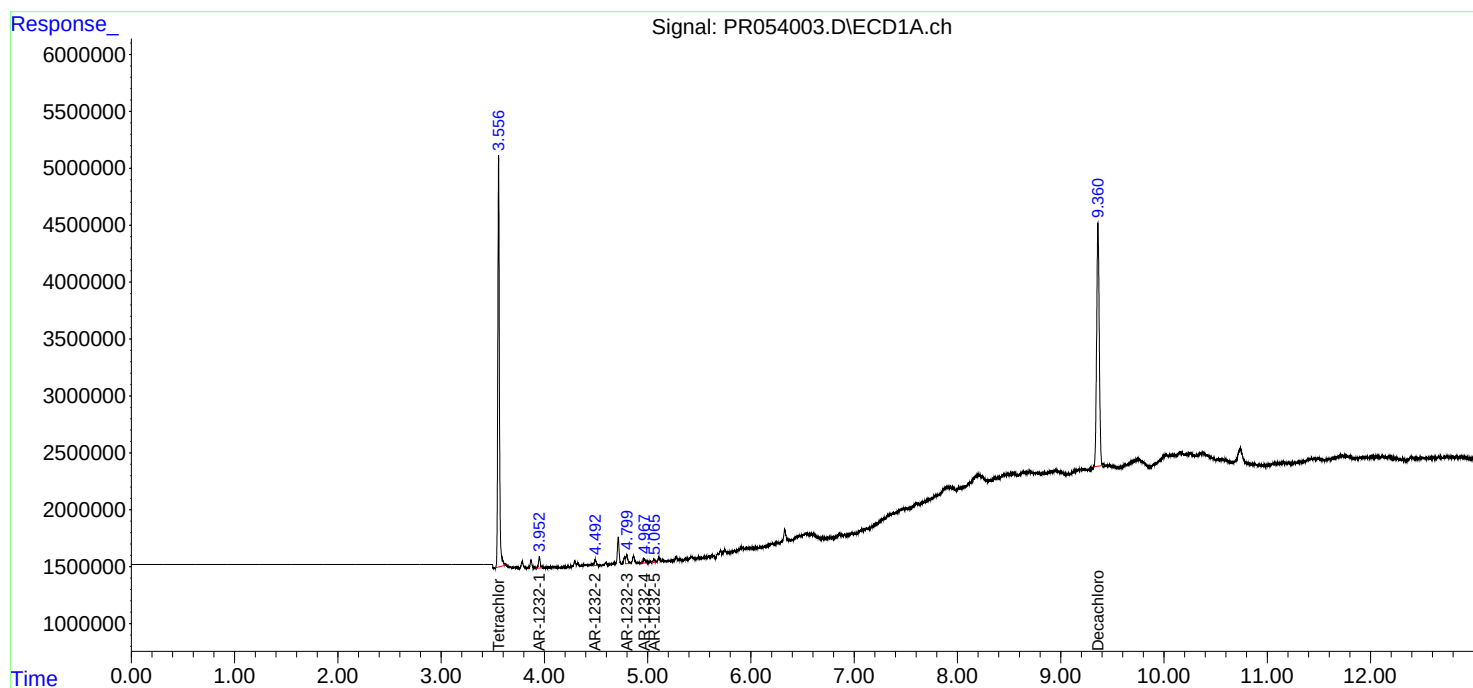


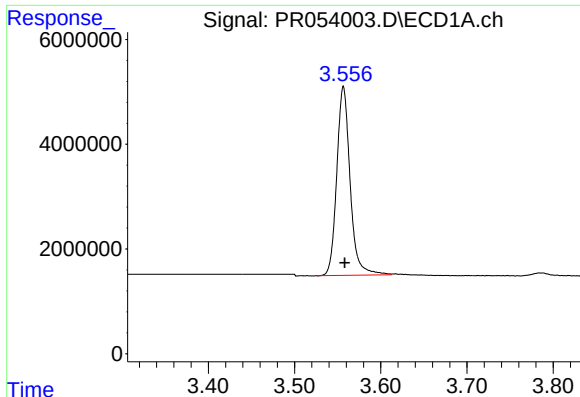

#1 Tetrachloro-m-xylene


R.T.: 3.557 min
Delta R.T.: -0.001 min
Response: 38834624
Conc: 20.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2022

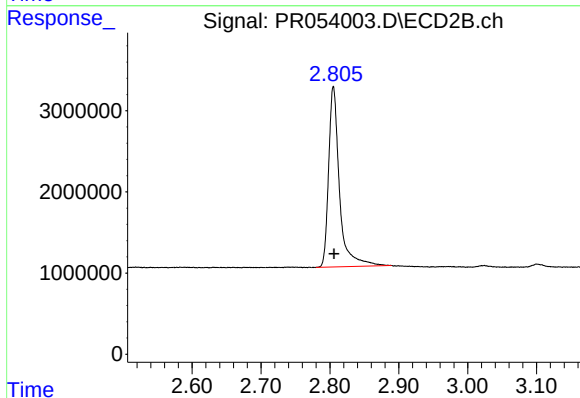


#1 Tetrachloro-m-xylene

R.T.: 2.805 min
Delta R.T.: 0.000 min
Response: 24360160
Conc: 19.37 ng/ml

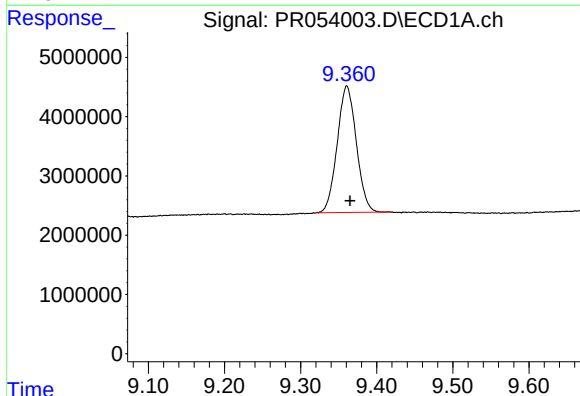


#2 Decachlorobiphenyl

R.T.: 9.361 min
Delta R.T.: -0.004 min
Response: 37371489
Conc: 22.29 ng/ml

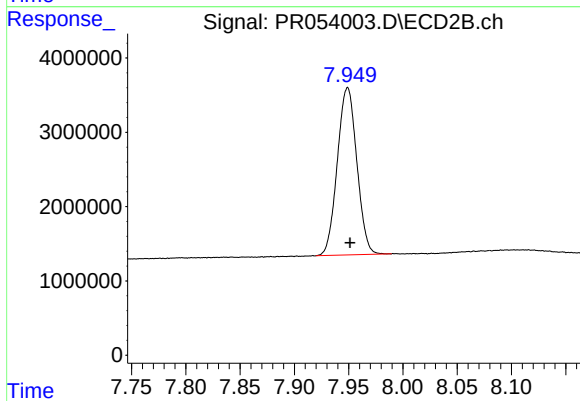

#2 Decachlorobiphenyl


R.T.: 7.949 min
Delta R.T.: -0.002 min
Response: 28178832
Conc: 21.55 ng/ml

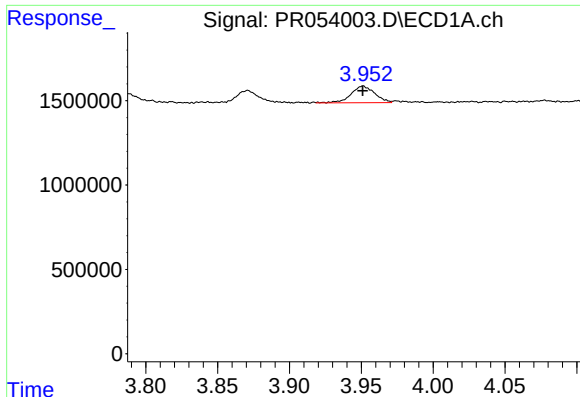

#11 AR-1232-1


R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 1128957
Conc: 29.59 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2022

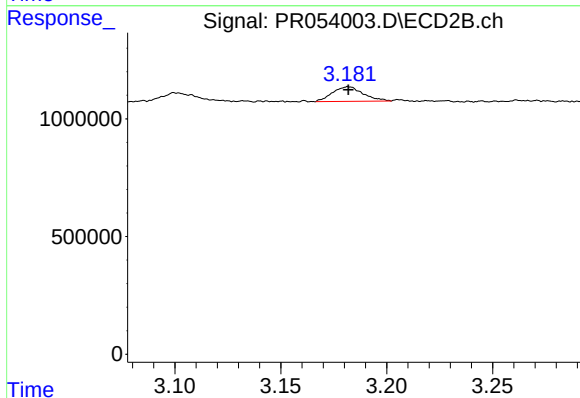


#11 AR-1232-1

R.T.: 3.182 min
Delta R.T.: 0.000 min
Response: 625993
Conc: 23.71 ng/ml

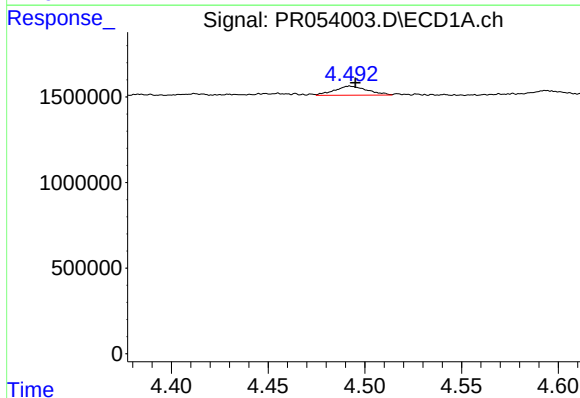


#12 AR-1232-2

R.T.: 4.492 min
Delta R.T.: -0.003 min
Response: 621604
Conc: 29.36 ng/ml

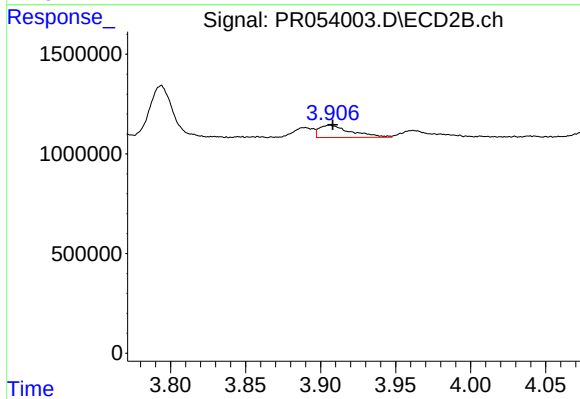

#12 AR-1232-2


R.T.: 3.906 min
Delta R.T.: -0.002 min
Response: 899615
Conc: 29.25 ng/ml

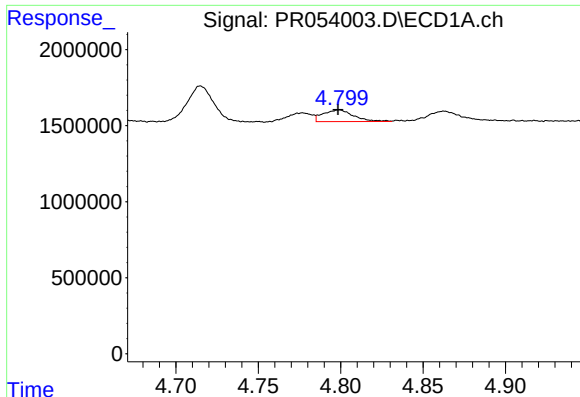

#13 AR-1232-3


R.T.: 4.799 min
Delta R.T.: 0.000 min
Response: 995660
Conc: 24.98 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2022

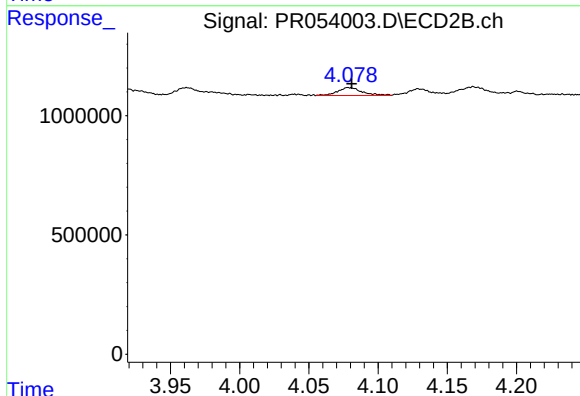


#13 AR-1232-3

R.T.: 4.078 min
Delta R.T.: -0.003 min
Response: 412707
Conc: 25.92 ng/ml

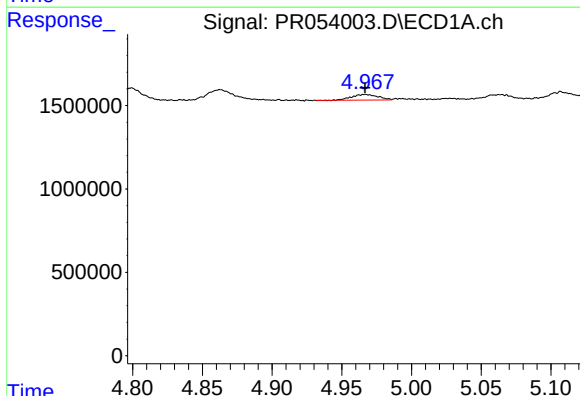


#14 AR-1232-4

R.T.: 4.967 min
Delta R.T.: 0.000 min
Response: 443674
Conc: 22.78 ng/ml

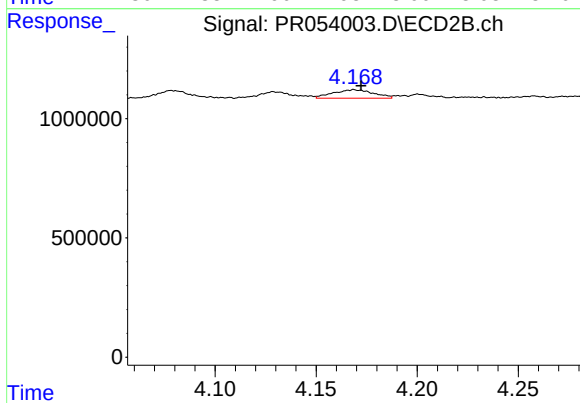

#14 AR-1232-4


R.T.: 4.169 min
Delta R.T.: -0.004 min
Response: 496969
Conc: 36.01 ng/ml

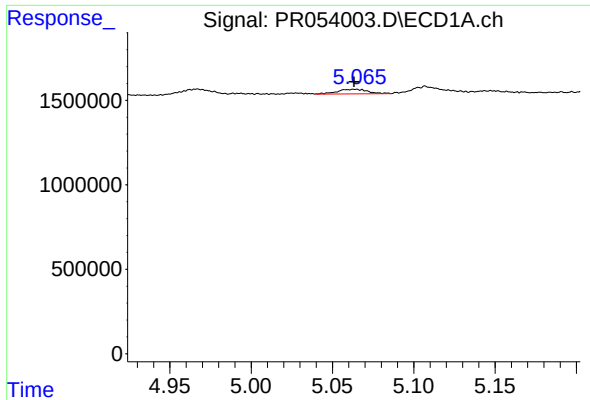

#15 AR-1232-5

R.T.: 5.065 min
Delta R.T.: 0.001 min
Response: 363851
Conc: 25.14 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2022

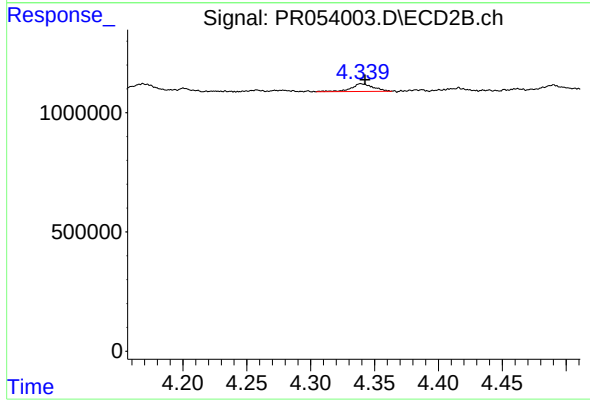

#15 AR-1232-5

R.T.: 4.339 min
Delta R.T.: -0.004 min
Response: 392138
Conc: 24.59 ng/ml