

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR031222\
 Data File : PR054006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2022 09:36
 Operator : AJ\MA
 Sample : N1645-09
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT1-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 23:24:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR031122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 10 01:38:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.557	2.806	39176320	24465803	20.579	19.449
2) SA Decachlor...	9.362	7.948	38088323	28352634	22.719	21.683
Target Compounds						
26) L6 AR-1254-1	5.675	4.702	1956710	1932000	29.663	27.481
27) L6 AR-1254-2	5.907	4.859	3897680	1702214	35.761m	26.231 #
28) L6 AR-1254-3	6.302	5.271	3711503	2462921	32.094m	25.291
29) L6 AR-1254-4	6.612	5.515	2929054	1375079	32.302m	23.767 #
30) L6 AR-1254-5	7.060	5.950	2579001	2105597	28.585	22.971


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR031222\
Data File : PR054006.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2022 09:36
Operator : AJ\MA
Sample : N1645-09
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 23:24:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR031122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 10 01:38:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

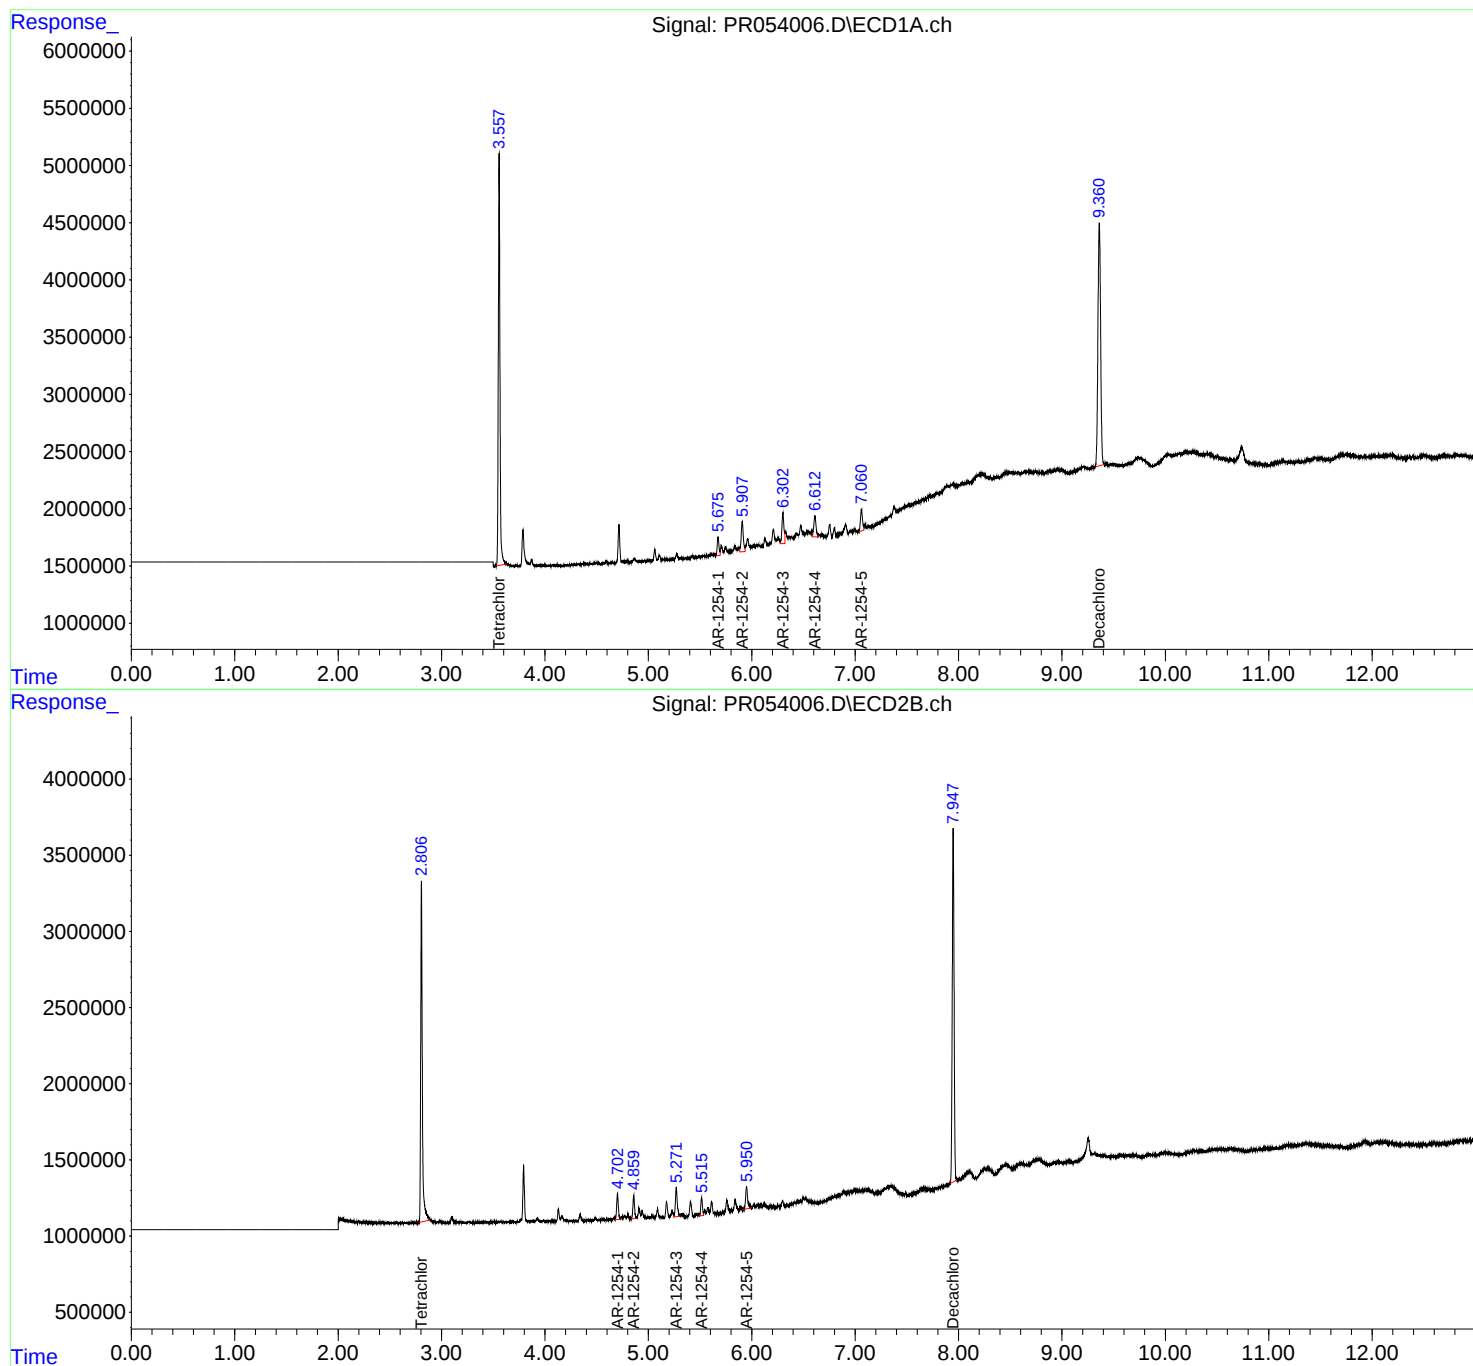


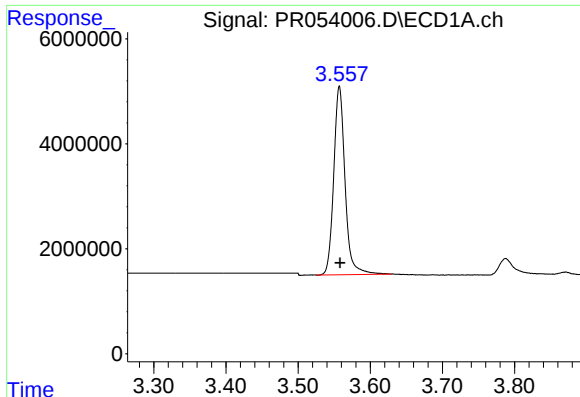

#1 Tetrachloro-m-xylene


R.T.: 3.557 min
Delta R.T.: 0.000 min
Response: 39176320
Conc: 20.58 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2022

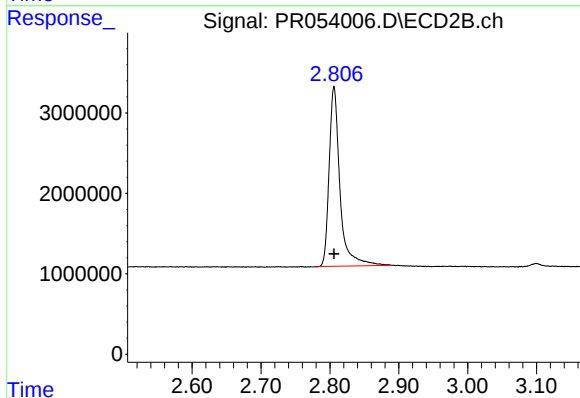


#1 Tetrachloro-m-xylene

R.T.: 2.806 min
Delta R.T.: 0.000 min
Response: 24465803
Conc: 19.45 ng/ml

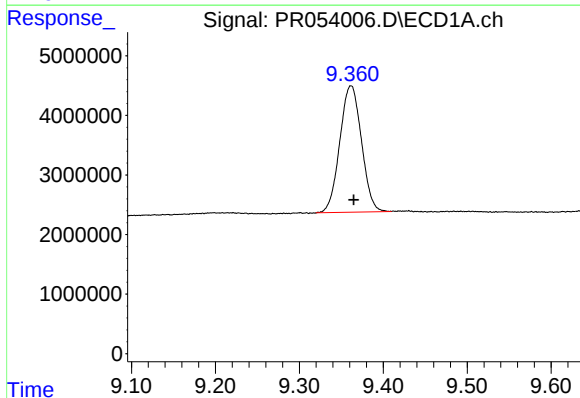


#2 Decachlorobiphenyl

R.T.: 9.362 min
Delta R.T.: -0.003 min
Response: 38088323
Conc: 22.72 ng/ml

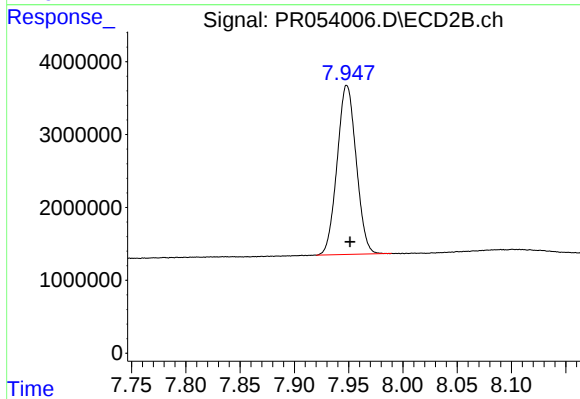

#2 Decachlorobiphenyl


R.T.: 7.948 min
Delta R.T.: -0.003 min
Response: 28352634
Conc: 21.68 ng/ml

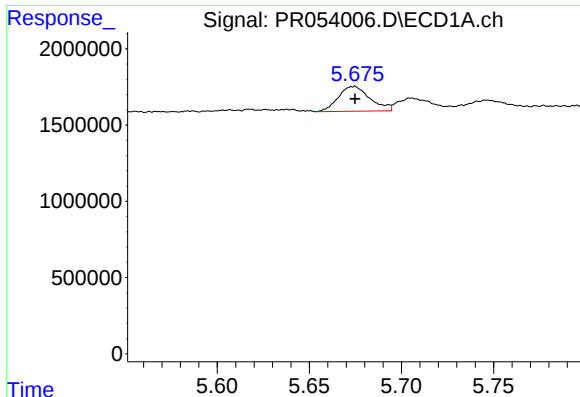

#26 AR-1254-1


R.T.: 5.675 min
Delta R.T.: 0.000 min
Response: 1956710
Conc: 29.66 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2022

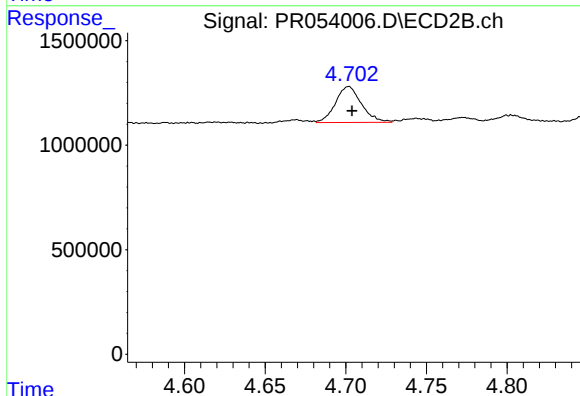


#26 AR-1254-1

R.T.: 4.702 min
Delta R.T.: -0.002 min
Response: 1932000
Conc: 27.48 ng/ml

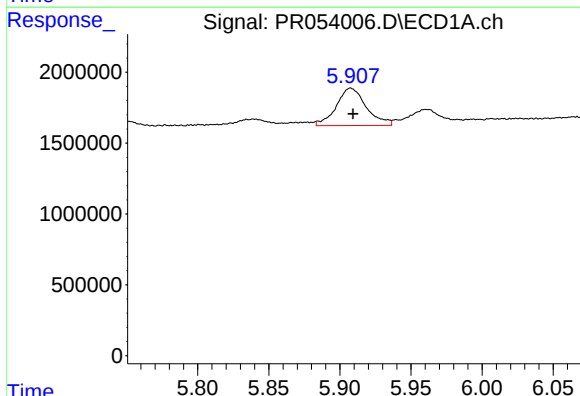


#27 AR-1254-2

R.T.: 5.907 min
Delta R.T.: -0.002 min
Response: 3897680
Conc: 35.76 ng/ml m

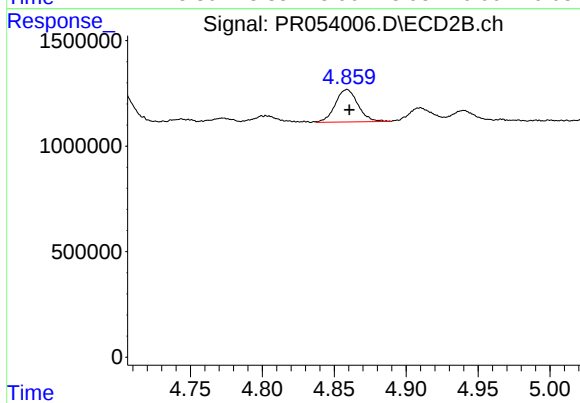

#27 AR-1254-2


R.T.: 4.859 min
Delta R.T.: -0.002 min
Response: 1702214
Conc: 26.23 ng/ml

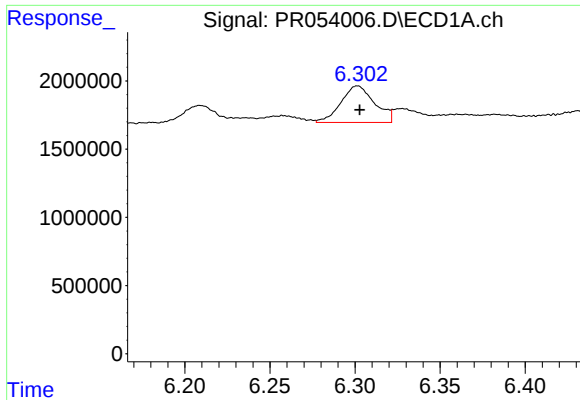

#28 AR-1254-3


R.T.: 6.302 min
Delta R.T.: 0.000 min
Response: 3711503
Conc: 32.09 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2022

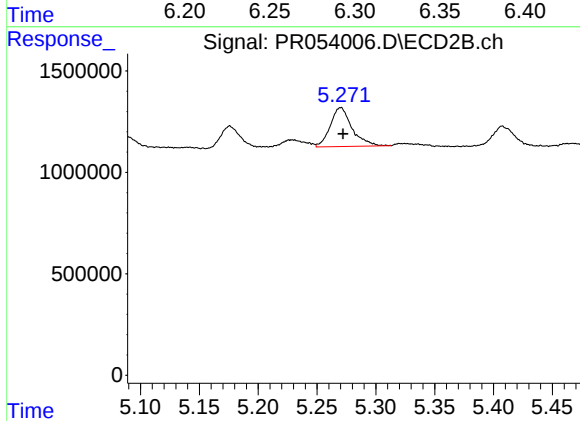


#28 AR-1254-3

R.T.: 5.271 min
Delta R.T.: -0.002 min
Response: 2462921
Conc: 25.29 ng/ml

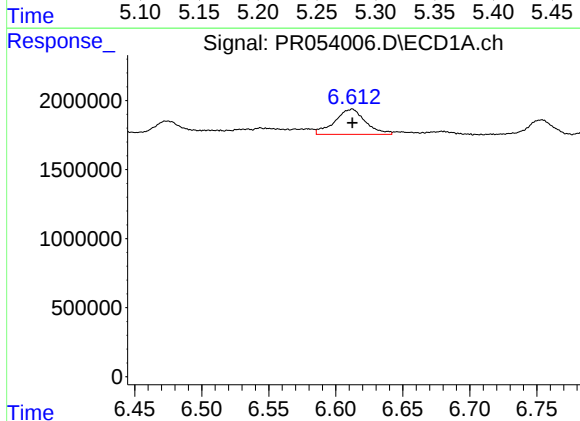


#29 AR-1254-4

R.T.: 6.612 min
Delta R.T.: 0.000 min
Response: 2929054
Conc: 32.30 ng/ml m

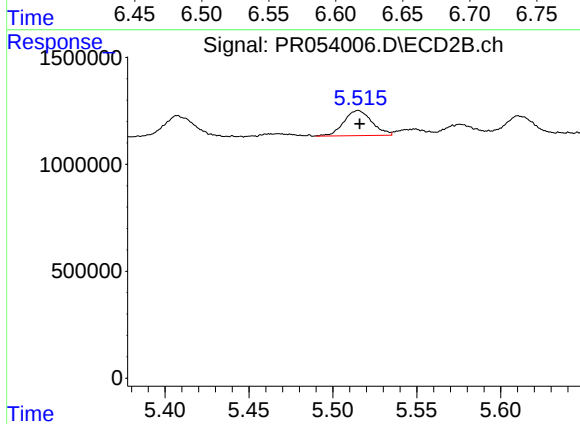

#29 AR-1254-4


R.T.: 5.515 min
Delta R.T.: 0.000 min
Response: 1375079
Conc: 23.77 ng/ml

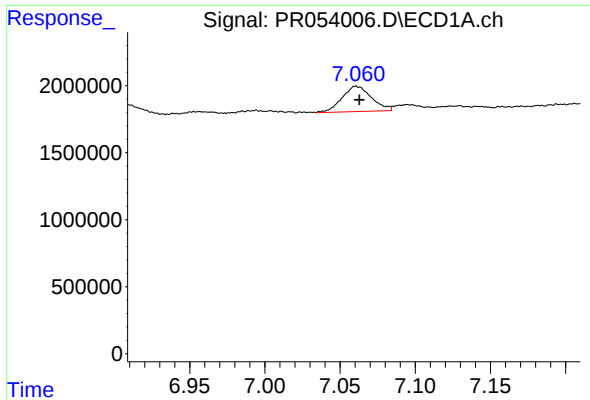

#30 AR-1254-5

R.T.: 7.060 min
Delta R.T.: -0.002 min
Response: 2579001
Conc: 28.59 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2022

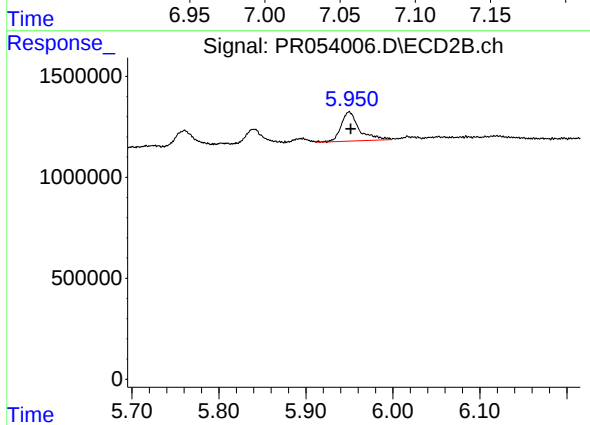

#30 AR-1254-5

R.T.: 5.950 min
Delta R.T.: -0.002 min
Response: 2105597
Conc: 22.97 ng/ml