

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR032119\
 Data File : PR036520.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2019 04:42
 Operator : SM\SJ
 Sample : K2037-01
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MW-00-20190320

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 05:43:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR032019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 20 15:19:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.399	3.473	29038397	86387826	19.186	21.068
2) SA Decachlor...	10.050	8.334	29269790	101.0E6	16.699	18.263

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR032119\
Data File : PR036520.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2019 04:42
Operator : SM\SJ
Sample : K2037-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MW-00-20190320

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 05:43:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR032019.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 20 15:19:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

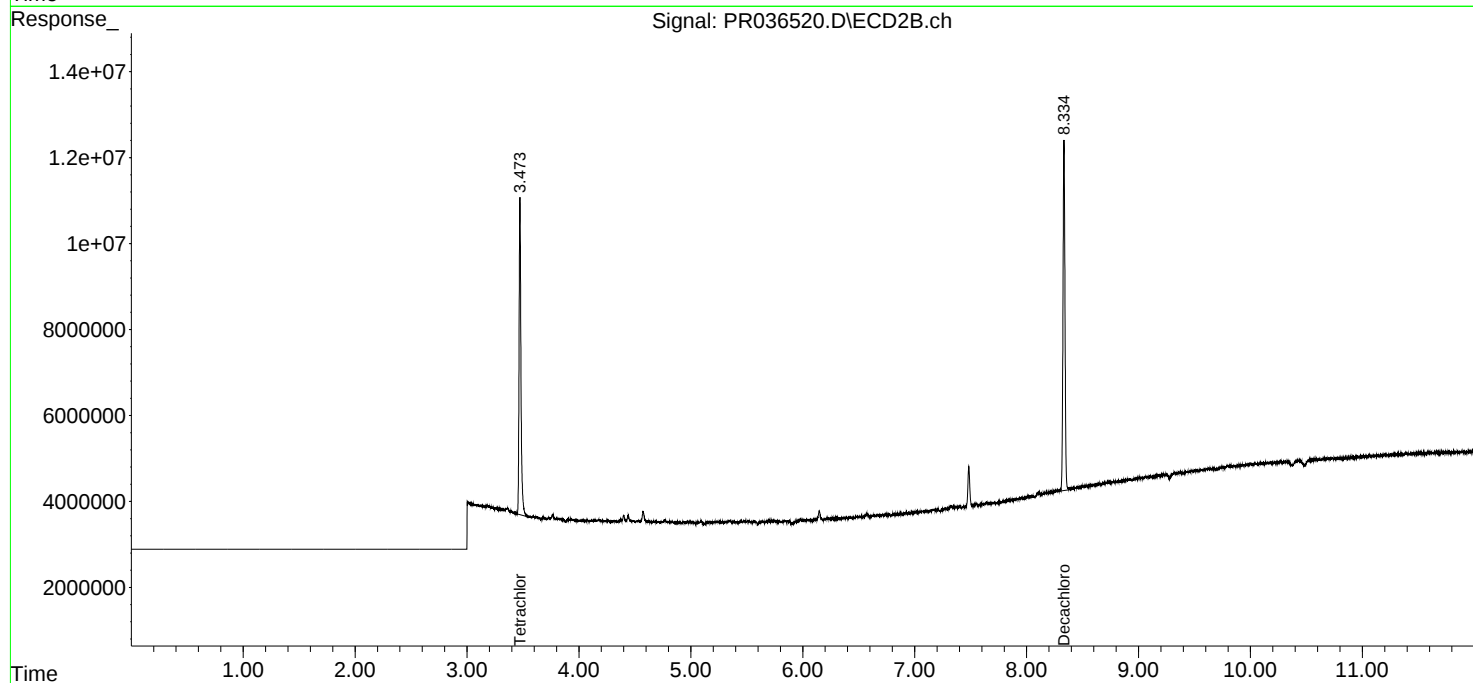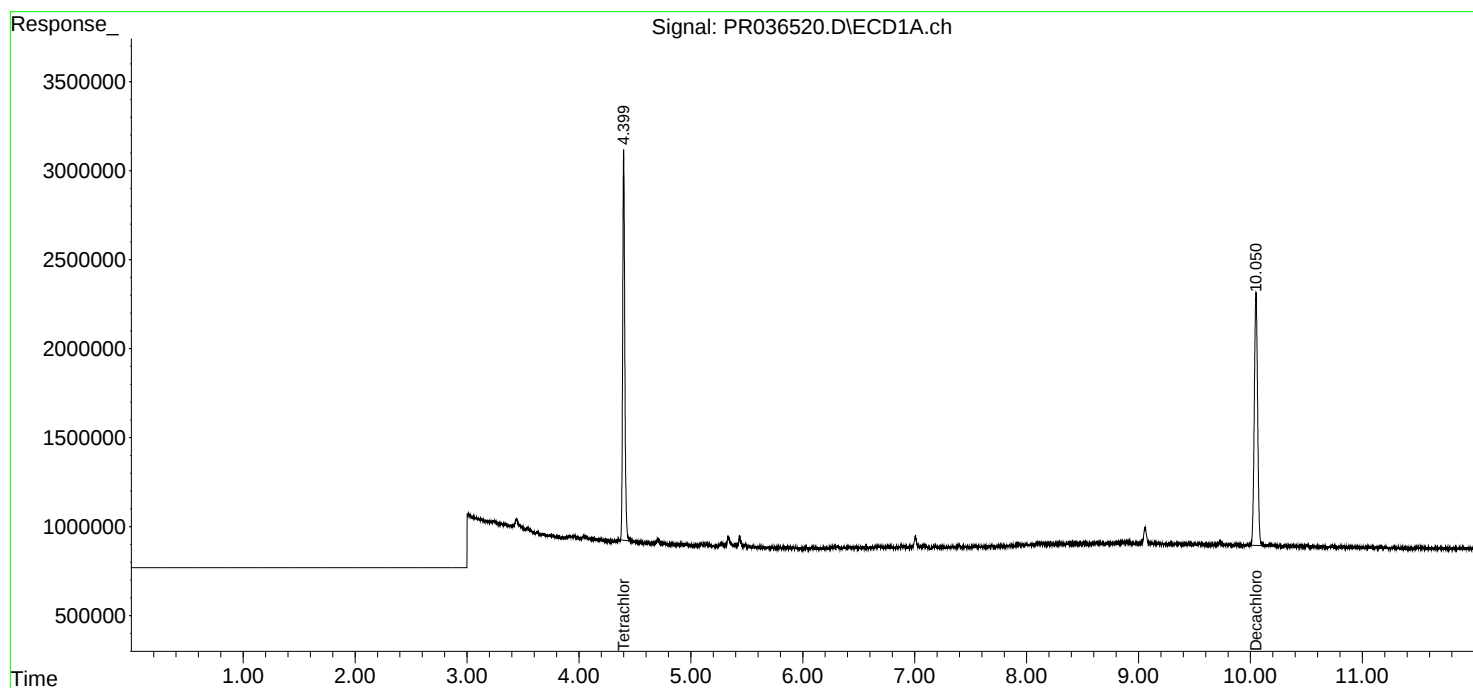


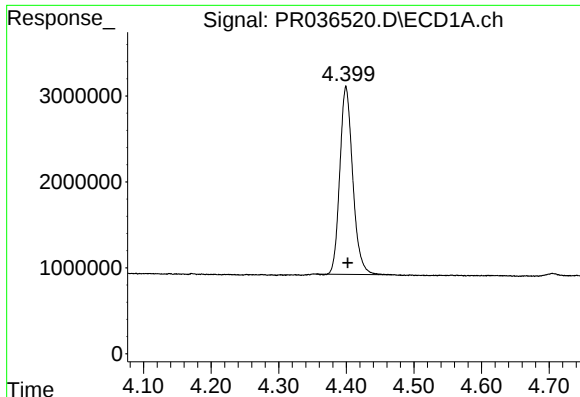

#1 Tetrachloro-m-xylene


R.T.: 4.399 min
Delta R.T.: -0.003 min
Response: 29038397
Conc: 19.19 ng/ml

Instrument :
ECD_R
ClientSampleId :
MW-00-20190320

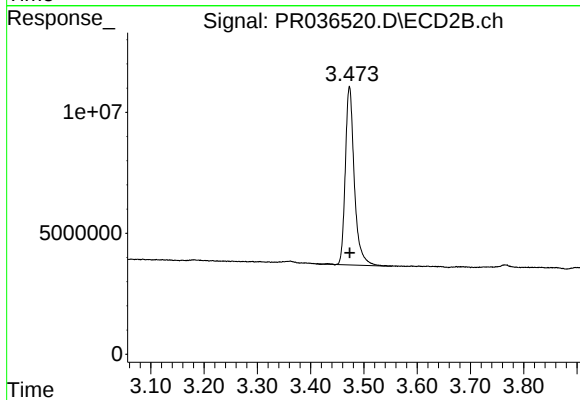


#1 Tetrachloro-m-xylene

R.T.: 3.473 min
Delta R.T.: 0.000 min
Response: 86387826
Conc: 21.07 ng/ml

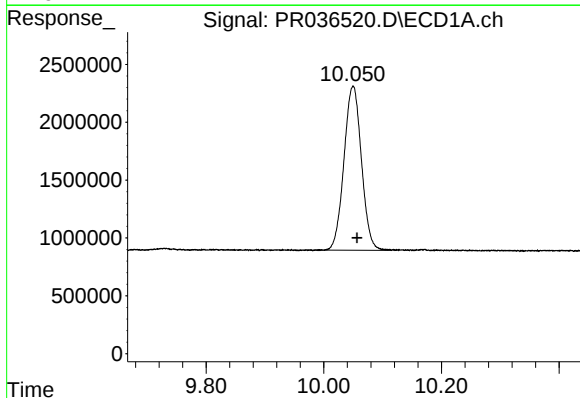

#2 Decachlorobiphenyl

R.T.: 10.050 min
Delta R.T.: -0.007 min
Response: 29269790
Conc: 16.70 ng/ml

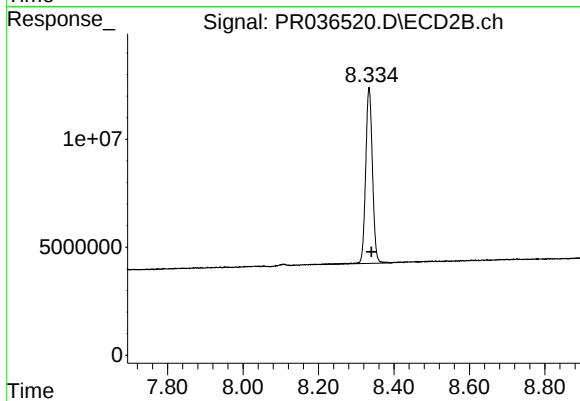

#2 Decachlorobiphenyl

R.T.: 8.334 min
Delta R.T.: -0.006 min
Response: 101037578
Conc: 18.26 ng/ml