

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR032219\
 Data File : PR036532.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2019 08:13
 Operator : SM\SJ
 Sample : K1808-01
 Misc :
 ALS Vial : 141 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 FK-BPM-01-AA0-BB0-AA0A-BB0A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 09:39:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR032019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 20 15:19:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.407	3.472	22715523	67088286	15.008	16.361
2) SA Decachlor...	10.065	8.342	30778634	98423208	17.560	17.790

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR032219\
Data File : PR036532.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2019 08:13
Operator : SM\SJ
Sample : K1808-01
Misc :
ALS Vial : 141 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
FK-BPM-01-AA0-BB0-AA0A-BB0A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 09:39:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR032019.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 20 15:19:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

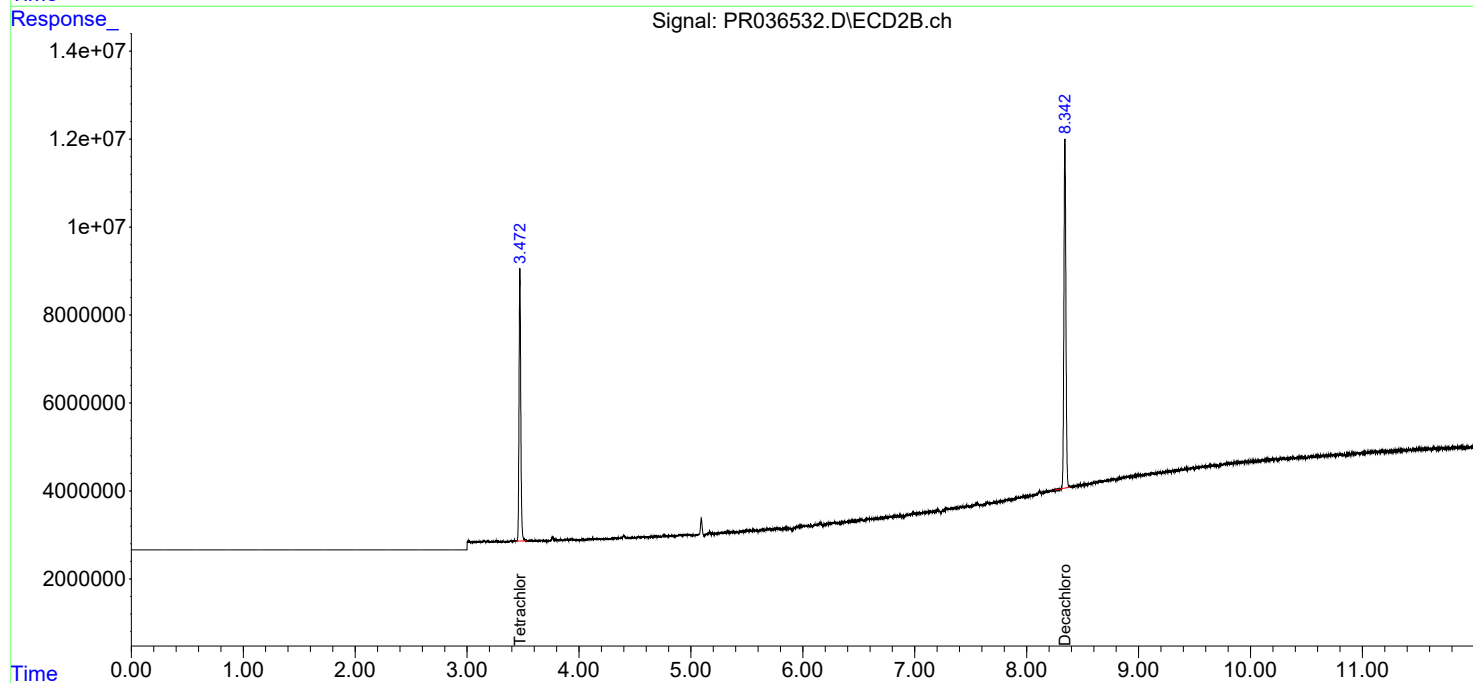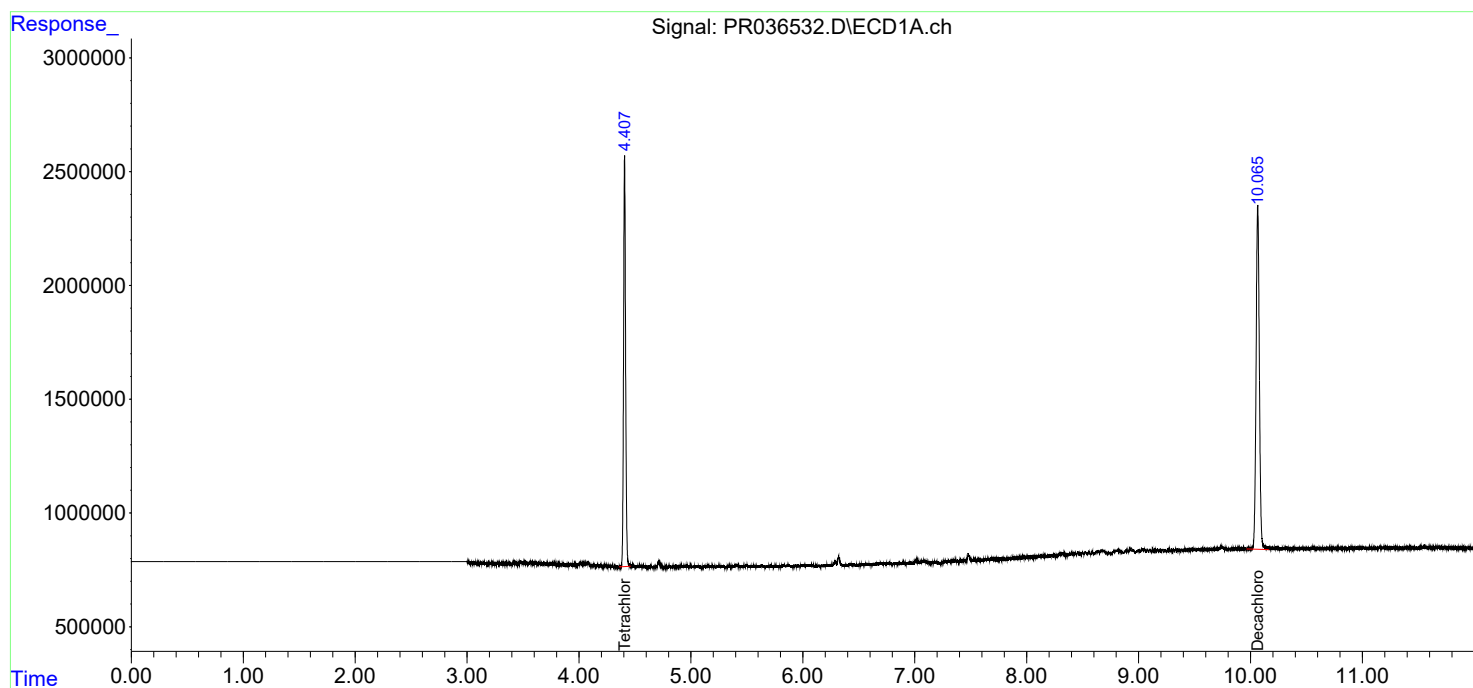


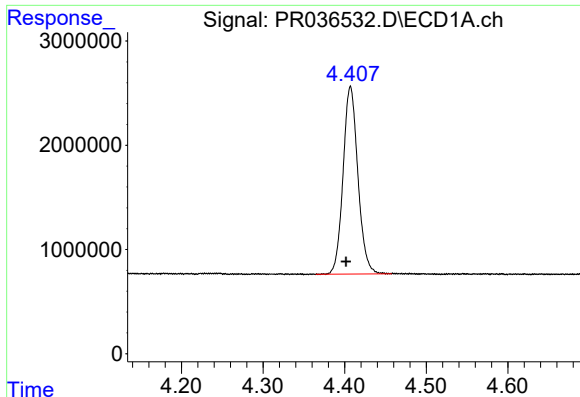

#1 Tetrachloro-m-xylene


R.T.: 4.407 min
Delta R.T.: 0.005 min
Response: 22715523
Conc: 15.01 ng/ml

Instrument :
ECD_R
ClientSampleId :
FK-BPM-01-AA0-BB0-AA0A-BB0A

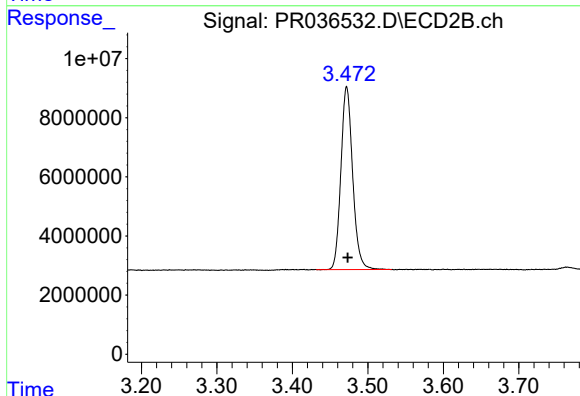


#1 Tetrachloro-m-xylene

R.T.: 3.472 min
Delta R.T.: -0.001 min
Response: 67088286
Conc: 16.36 ng/ml

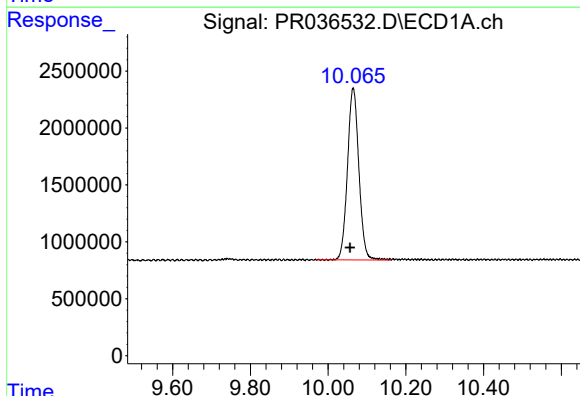

#2 Decachlorobiphenyl

R.T.: 10.065 min
Delta R.T.: 0.008 min
Response: 30778634
Conc: 17.56 ng/ml

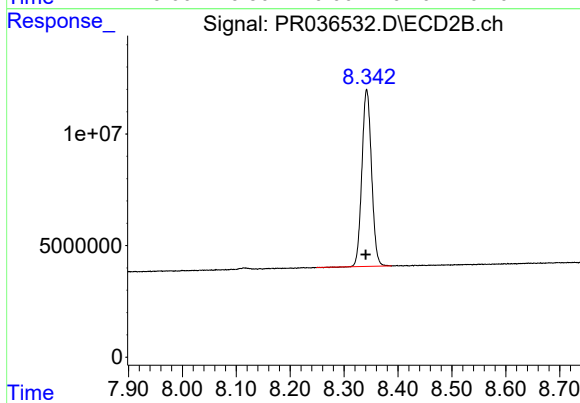

#2 Decachlorobiphenyl

R.T.: 8.342 min
Delta R.T.: 0.002 min
Response: 98423208
Conc: 17.79 ng/ml