

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR032219\
 Data File : PR036535.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2019 08:56
 Operator : SM\SJ
 Sample : K1809-01
 Misc :
 ALS Vial : 144 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 FK-BPM-01-A0-B0-A0A-A0B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 10:14:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR032019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 20 15:19:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.400	3.473	25584253	76027607	16.904	18.541
2) SA Decachlor...	10.048	8.336	33246422	112.0E6	18.968	20.238

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR032219\
Data File : PR036535.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2019 08:56
Operator : SM\SJ
Sample : K1809-01
Misc :
ALS Vial : 144 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
FK-BPM-01-A0-B0-A0A-A0B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 10:14:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR032019.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 20 15:19:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

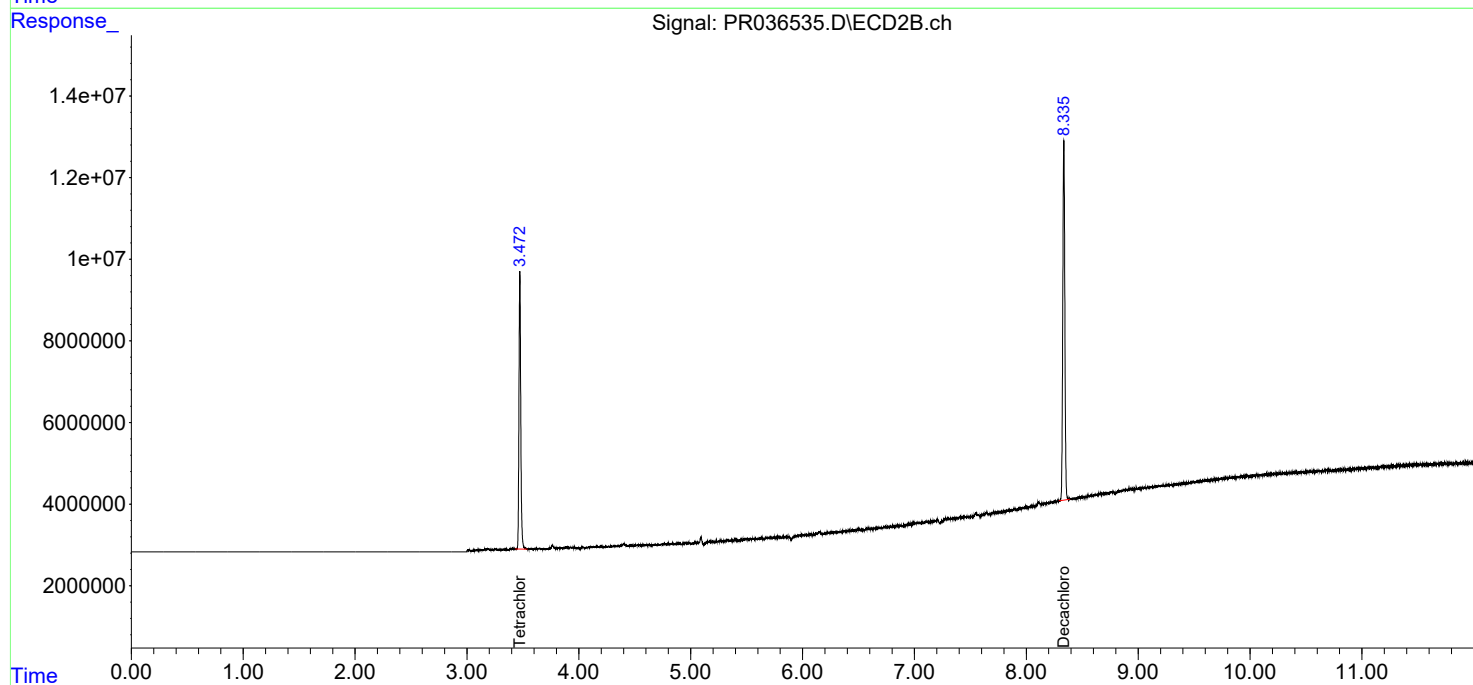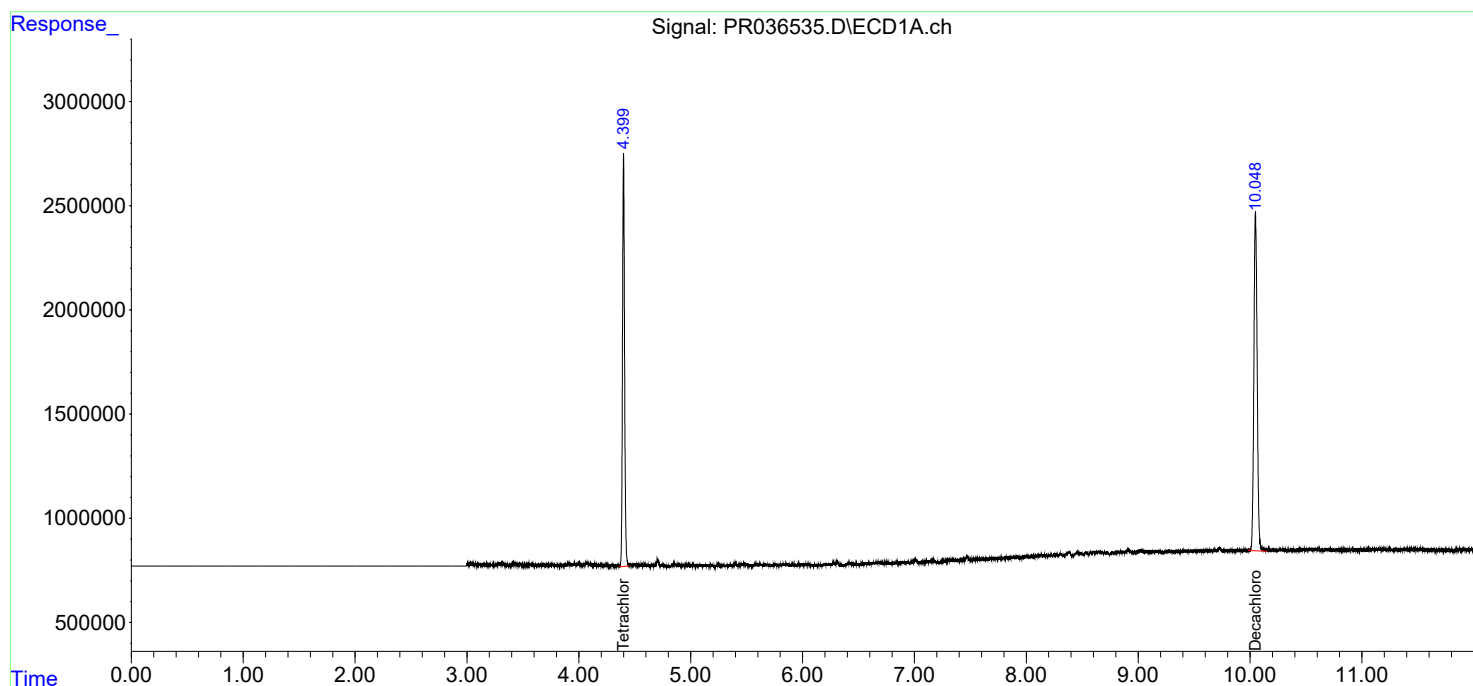


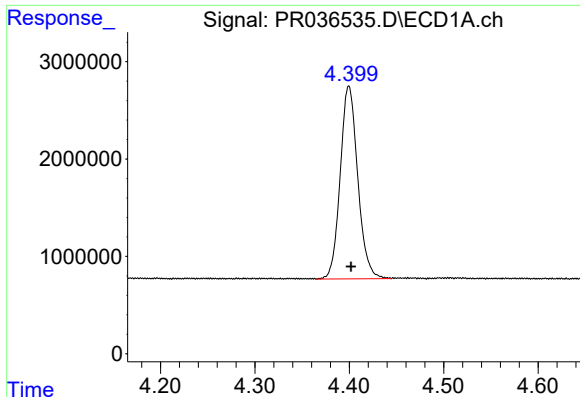

#1 Tetrachloro-m-xylene


R.T.: 4.400 min
Delta R.T.: -0.002 min
Response: 25584253
Conc: 16.90 ng/ml

Instrument :
ECD_R
ClientSampleId :
FK-BPM-01-A0-B0-A0A-A0B

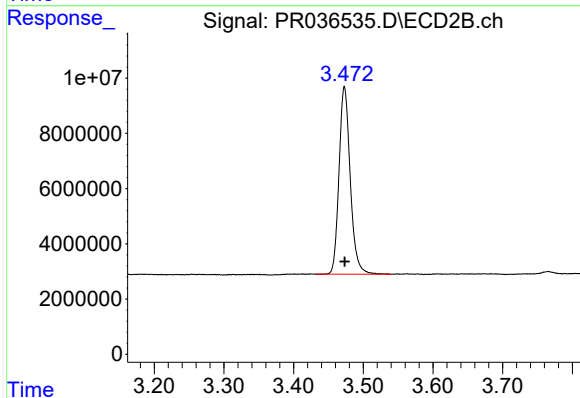


#1 Tetrachloro-m-xylene

R.T.: 3.473 min
Delta R.T.: 0.000 min
Response: 76027607
Conc: 18.54 ng/ml

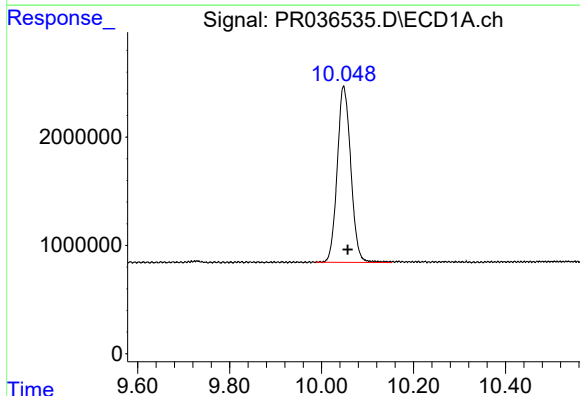

#2 Decachlorobiphenyl

R.T.: 10.048 min
Delta R.T.: -0.009 min
Response: 33246422
Conc: 18.97 ng/ml

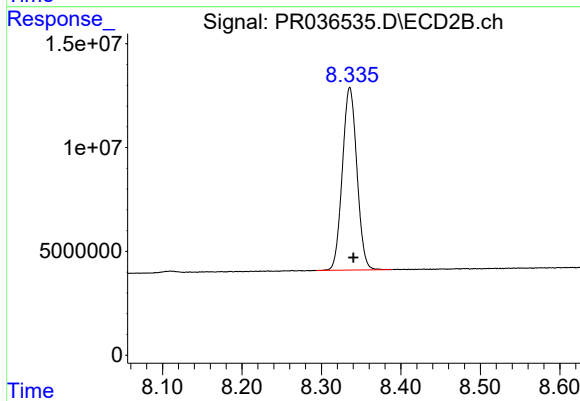

#2 Decachlorobiphenyl

R.T.: 8.336 min
Delta R.T.: -0.004 min
Response: 111961845
Conc: 20.24 ng/ml