

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR032219\
 Data File : PR036566.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2019 17:15
 Operator : SM\SJ
 Sample : K1938-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 22:39:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR032019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 20 15:19:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.400	3.474	32764577	94298092	21.648	22.997
2)	SA Decachlor...	10.049	8.336	28607344	92134987	16.321	16.654
Target Compounds							
20)	L4 AR-1242-5	0.000	5.319	0	4218283	N.D.	31.186 #
25)	L5 AR-1248-5	0.000	5.319	0	4218283	N.D.	13.955 #
26)	L6 AR-1254-1	0.000	5.319	0	4218283	N.D.	13.262 #
27)	L6 AR-1254-2	0.000	5.493	0	9754257	N.D.	34.917 #
28)	L6 AR-1254-3	7.005	0.000	2095946	0	15.869	N.D. #
29)	L6 AR-1254-4	0.000	6.148	0	6592889	N.D.	18.923 #
32)	L7 AR-1260-2	0.000	6.148	0	6592889	N.D.	14.813 #
33)	L7 AR-1260-3	0.000	6.328	0	3704405	N.D.	10.272 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR032219\
Data File : PR036566.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2019 17:15
Operator : SM\SJ
Sample : K1938-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 22:39:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR032019.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 20 15:19:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

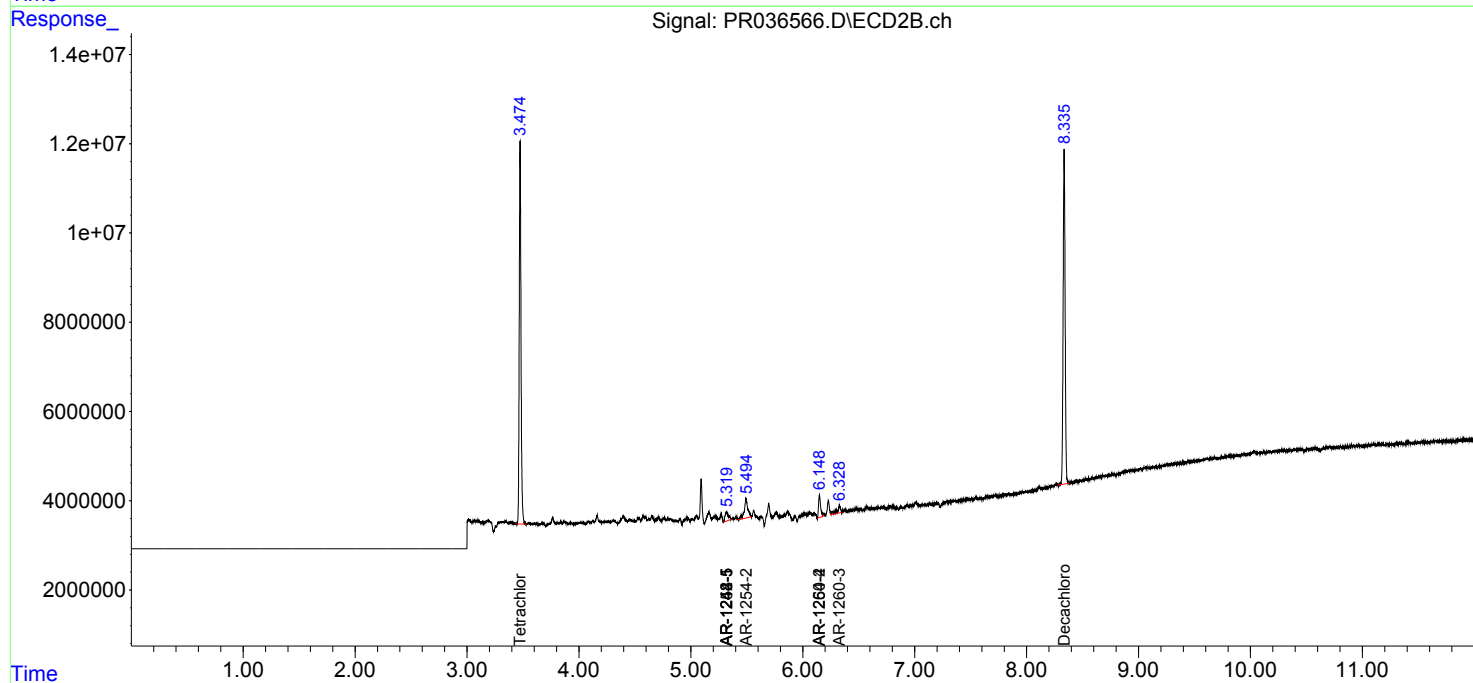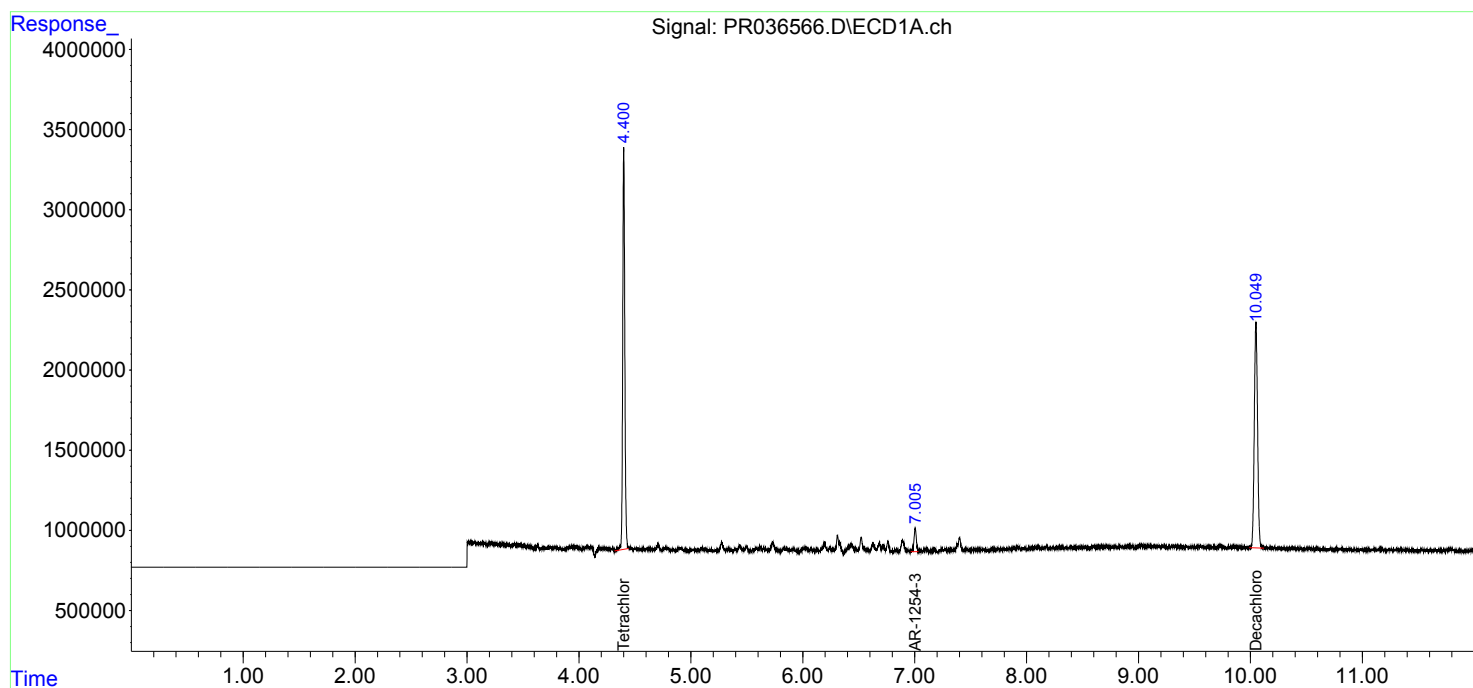


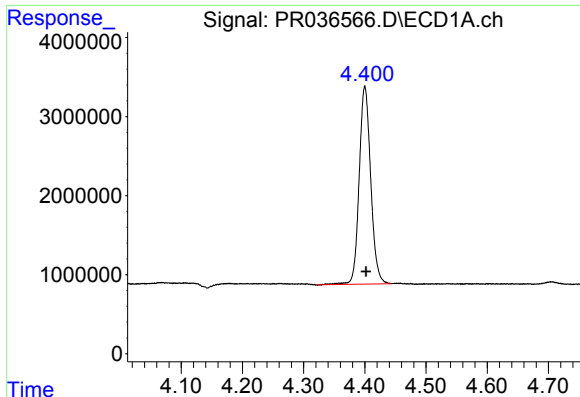

#1 Tetrachloro-m-xylene


R.T.: 4.400 min
Delta R.T.: -0.002 min
Response: 32764577
Conc: 21.65 ng/ml

Instrument :
ECD_R
ClientSampleId :

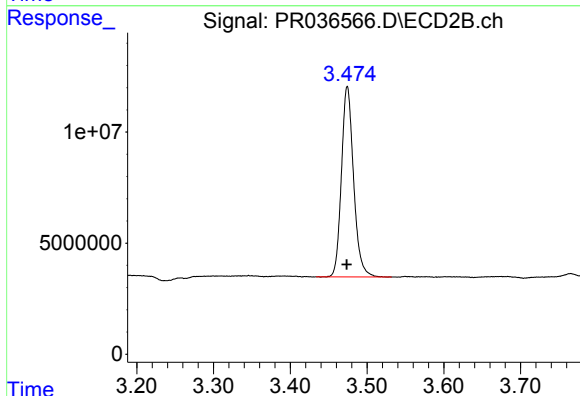


#1 Tetrachloro-m-xylene

R.T.: 3.474 min
Delta R.T.: 0.000 min
Response: 94298092
Conc: 23.00 ng/ml

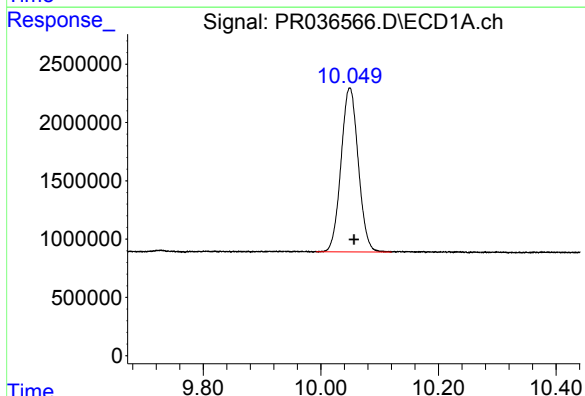


#2 Decachlorobiphenyl

R.T.: 10.049 min
Delta R.T.: -0.007 min
Response: 28607344
Conc: 16.32 ng/ml

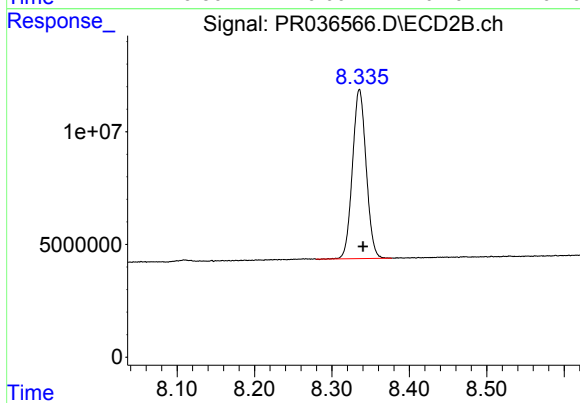

#2 Decachlorobiphenyl


R.T.: 8.336 min
Delta R.T.: -0.005 min
Response: 92134987
Conc: 16.65 ng/ml

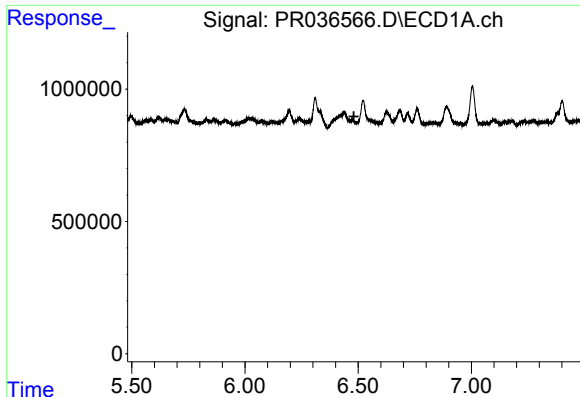

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.481 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :

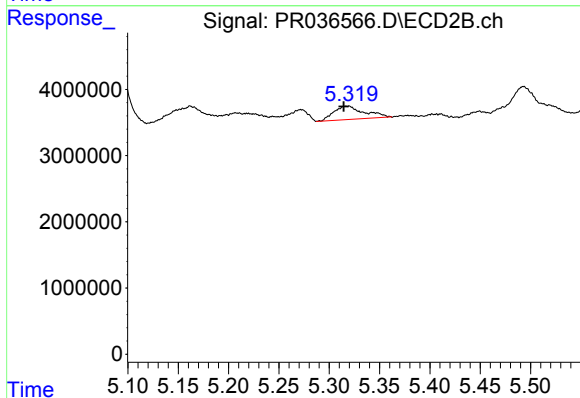


#20 AR-1242-5

R.T.: 5.319 min
Delta R.T.: 0.005 min
Response: 4218283
Conc: 31.19 ng/ml

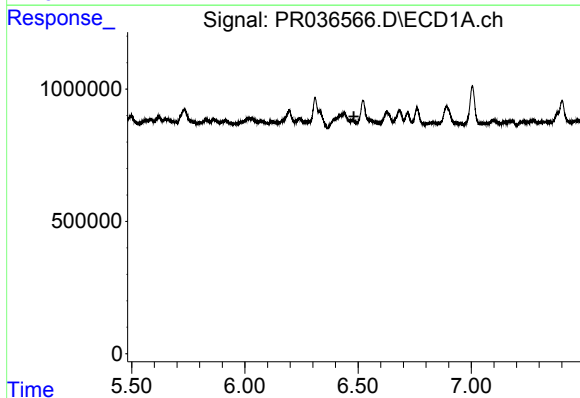


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 6.481 min
Response: 0
Conc: N.D.

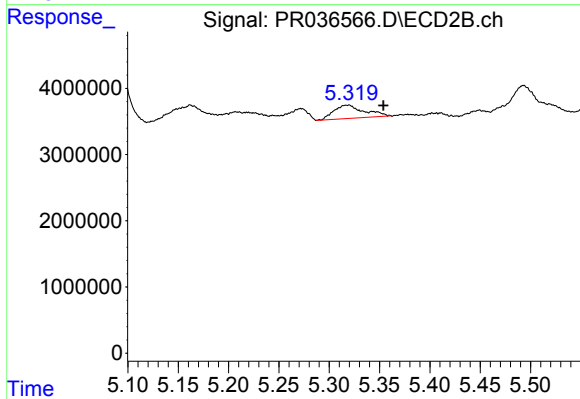

#25 AR-1248-5


R.T.: 5.319 min
Delta R.T.: -0.035 min
Response: 4218283
Conc: 13.96 ng/ml

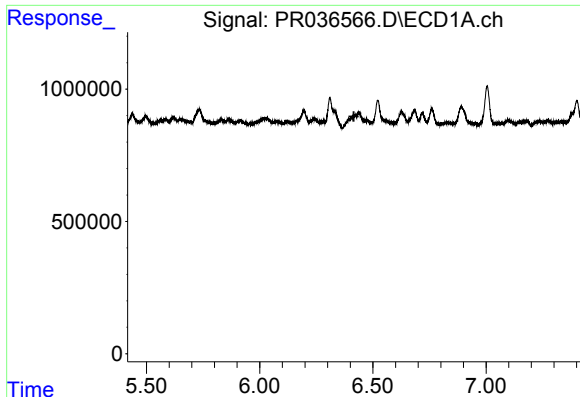

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :

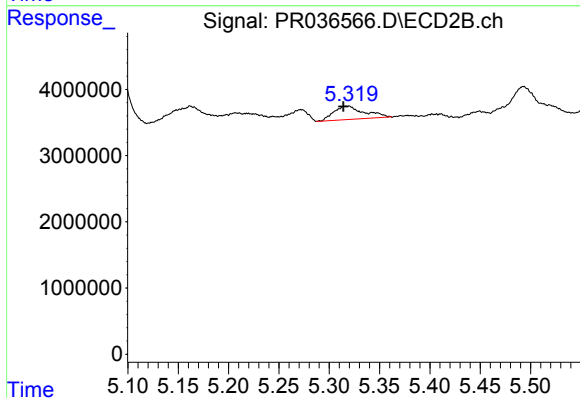


#26 AR-1254-1

R.T.: 5.319 min
Delta R.T.: 0.005 min
Response: 4218283
Conc: 13.26 ng/ml

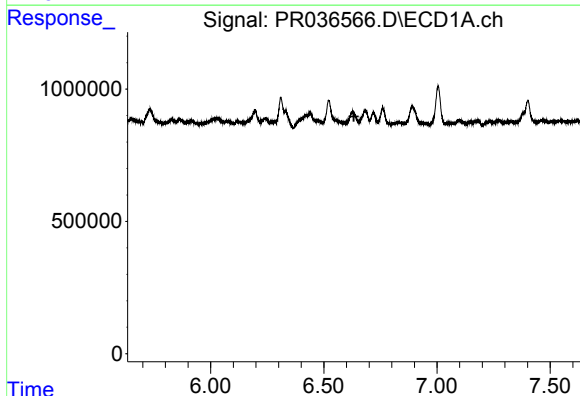


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T.: 6.633 min
Response: 0
Conc: N.D.

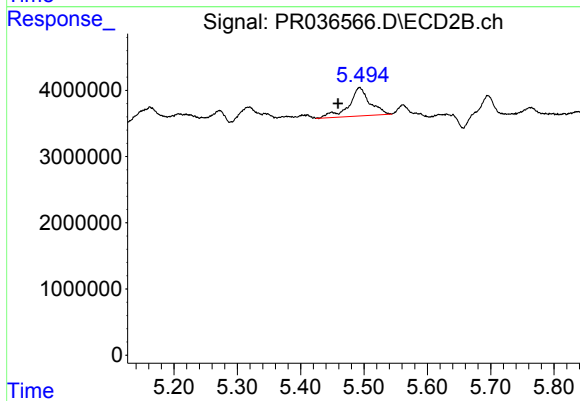

#27 AR-1254-2


R.T.: 5.493 min
Delta R.T.: 0.034 min
Response: 9754257
Conc: 34.92 ng/ml

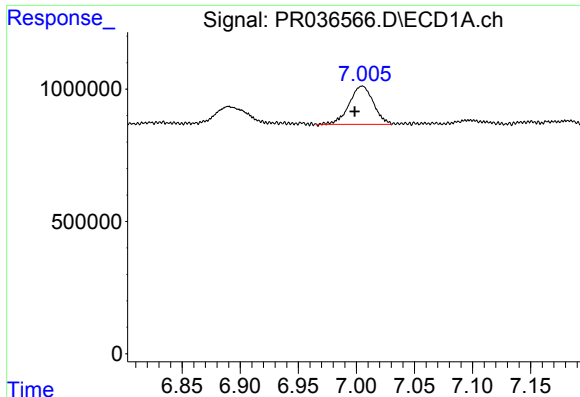

#28 AR-1254-3


R.T.: 7.005 min
Delta R.T.: 0.007 min
Response: 2095946
Conc: 15.87 ng/ml

Instrument :
ECD_R
ClientSampleId :

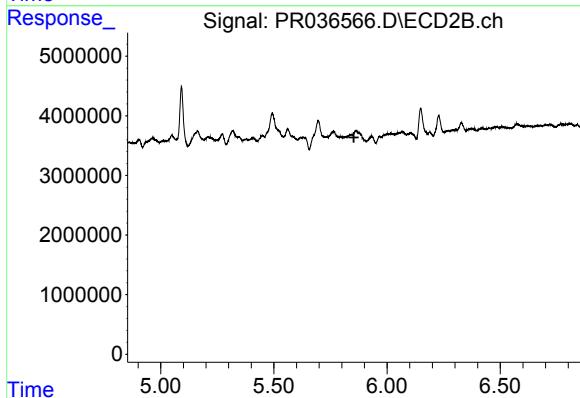


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 5.853 min
Response: 0
Conc: N.D.

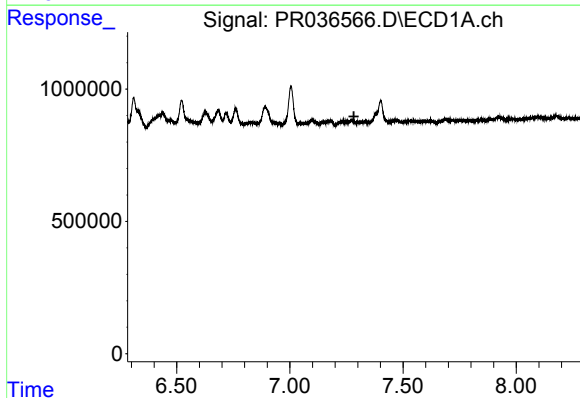


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.283 min
Response: 0
Conc: N.D.

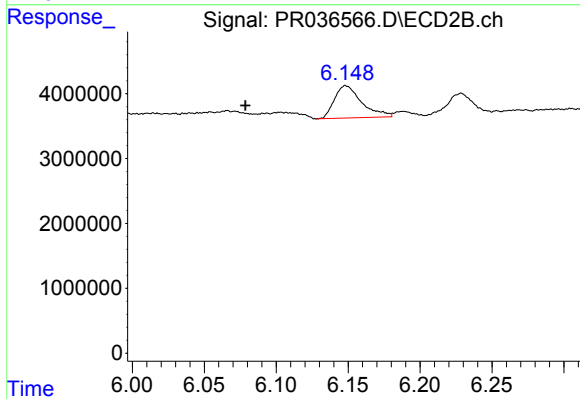

#29 AR-1254-4


R.T.: 6.148 min
Delta R.T.: 0.070 min
Response: 6592889
Conc: 18.92 ng/ml

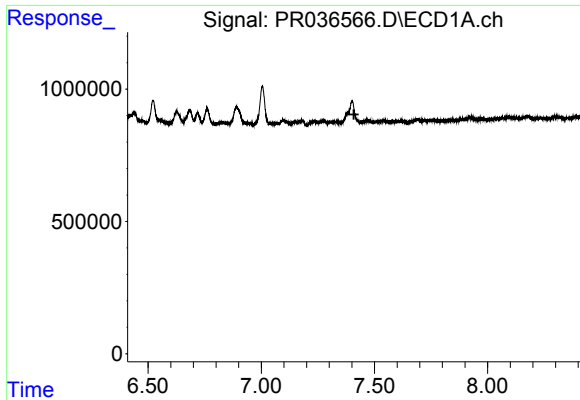

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.409 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :

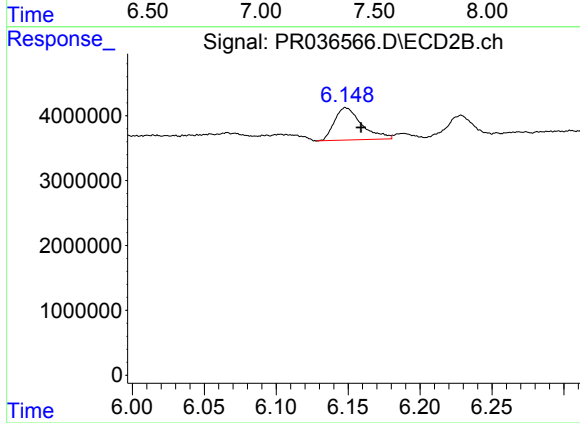


#32 AR-1260-2

R.T.: 6.148 min
Delta R.T.: -0.011 min
Response: 6592889
Conc: 14.81 ng/ml

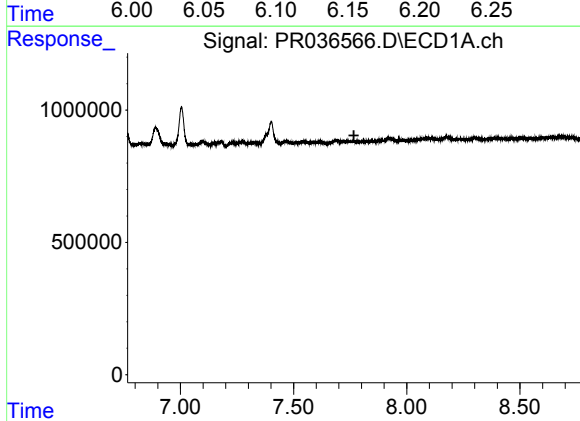

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.766 min
Response: 0
Conc: N.D.

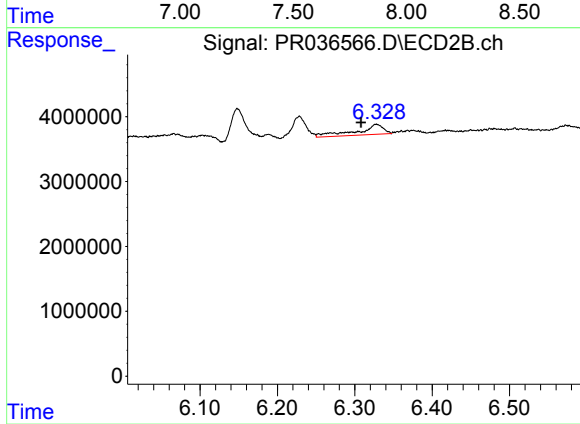

#33 AR-1260-3

R.T.: 6.328 min
Delta R.T.: 0.020 min
Response: 3704405
Conc: 10.27 ng/ml