

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040221\
 Data File : PR049724.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Apr 2021 18:49
 Operator : DD\AJ
 Sample : M1458-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT1-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 01:32:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Apr 03 08:12:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.638	3.822	56184168	112.5E6	14.390	16.962
2)	SA Decachlor...	10.514	8.866	87046546	138.6E6	19.591	18.207
Target Compounds							
3)	L1 AR-1016-1	5.819	4.912	1941748	3419350	12.631	14.240
4)	L1 AR-1016-2	5.843	4.931	2054494	3070002	9.616	8.899
5)	L1 AR-1016-3	5.905	5.108	1236662	2149864	9.631	11.808
6)	L1 AR-1016-4	6.005	5.148	1334939	4746553	12.546	34.141 #
7)	L1 AR-1016-5	6.299	5.363	2898845	5686839	27.057	30.268
8)	L2 AR-1221-1	4.864	0.000	2637631	0	63.810	N.D. #
9)	L2 AR-1221-2	4.950	4.124	836404	1962587	26.808	39.933 #
12)	L3 AR-1232-2	5.550	4.931	992395	3070002	23.415	23.112
13)	L3 AR-1232-3	5.843	5.108	2054494	2149864	24.115	30.921 #
14)	L3 AR-1232-4	6.005	5.191	1334939	4765199	31.322	81.058 #
15)	L3 AR-1232-5	6.091	5.363	2704793	5686839	81.789	86.141
16)	L4 AR-1242-1	5.819	4.912	1941748	3419350	17.318	19.484
17)	L4 AR-1242-2	5.843	4.931	2054494	3070002	13.006	12.228
18)	L4 AR-1242-3	5.905	5.108	1236662	2149864	12.914	16.115
19)	L4 AR-1242-4	6.005	5.191	1334939	4765199	16.660	38.449 #
20)	L4 AR-1242-5	6.742	5.713	3234053	8552216	35.497	50.117 #
21)	L5 AR-1248-1	5.819	4.912	1941748	3419350	22.662	25.338
22)	L5 AR-1248-2	6.091	5.148	2704793	4746553	22.500	26.783
23)	L5 AR-1248-3	6.299	5.191	2898845	4765199	21.404	25.288
24)	L5 AR-1248-4	6.704	5.363	3297892	5686839	20.581	24.445
25)	L5 AR-1248-5	6.742	5.755	3234053	6069474	21.026	24.642
26)	L6 AR-1254-1	6.676	5.713	2615030	8552216	16.438	22.749 #
27)	L6 AR-1254-2	6.901	5.860	3488330	2611778	13.849	8.100 #
28)	L6 AR-1254-3	7.263	6.264	2429615	4207594	8.795	7.381
29)	L6 AR-1254-4	7.569f	6.491	5533971	3171602	26.299	8.871 #
30)	L6 AR-1254-5	7.966	6.909	392648	568418	1.731	1.141 #
31)	L7 AR-1260-1	7.446f	6.410	369872	1692814	1.860	4.720 #
32)	L7 AR-1260-2	7.679	6.578	306961	6214450	1.257	13.998 #
33)	L7 AR-1260-3	0.000	6.735	0	632657	N.D.	1.504 #
35)	L7 AR-1260-5	0.000	7.449	0	440922	N.D.	0.481 #
36)	L8 AR-1262-1	0.000	6.909	0	568418	N.D.	2.215 #
37)	L8 AR-1262-2	0.000	7.449	0	440922	N.D.	0.448 #
38)	L8 AR-1262-3	0.000	7.712f	0	49913	N.D.	0.139 #
39)	L8 AR-1262-4	0.000	7.795	0	863035	N.D.	1.205 #
40)	L8 AR-1262-5	0.000	8.320f	0	1167195	N.D.	3.632 #
41)	L9 AR-1268-1	0.000	7.712f	0	49913	N.D.	0.044 #
42)	L9 AR-1268-2	0.000	7.795	0	863035	N.D.	0.816 #
43)	L9 AR-1268-3	0.000	7.999	0	1613746	N.D.	1.842 #
44)	L9 AR-1268-4	0.000	8.320f	0	1167195	N.D.	3.206 #
45)	L9 AR-1268-5	10.160	8.600	532146	1113897	0.325	0.366

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040221\
Data File : PR049724.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2021 18:49
Operator : DD\AJ
Sample : M1458-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 01:32:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040221.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Apr 03 08:12:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040221\
Data File : PR049724.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Apr 2021 18:49
Operator : DD\AJ
Sample : M1458-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 01:32:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040221.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Apr 03 08:12:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

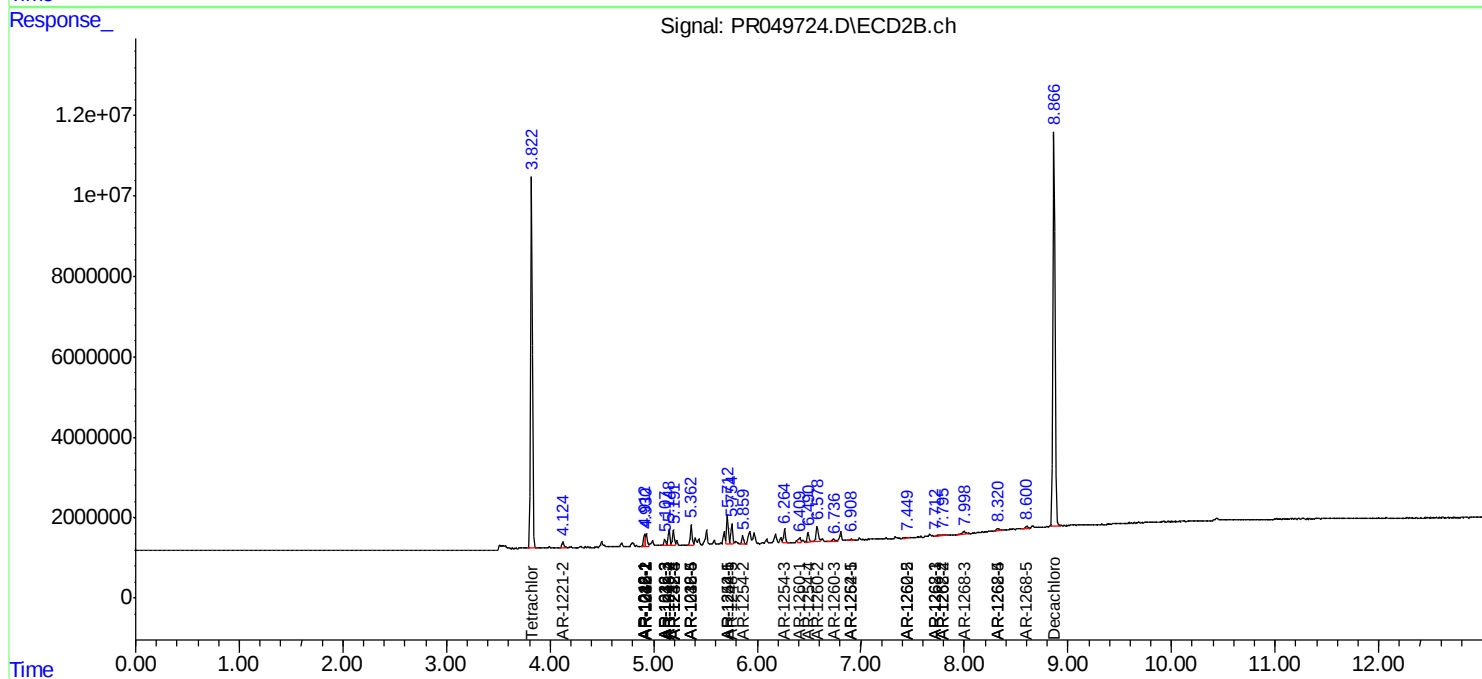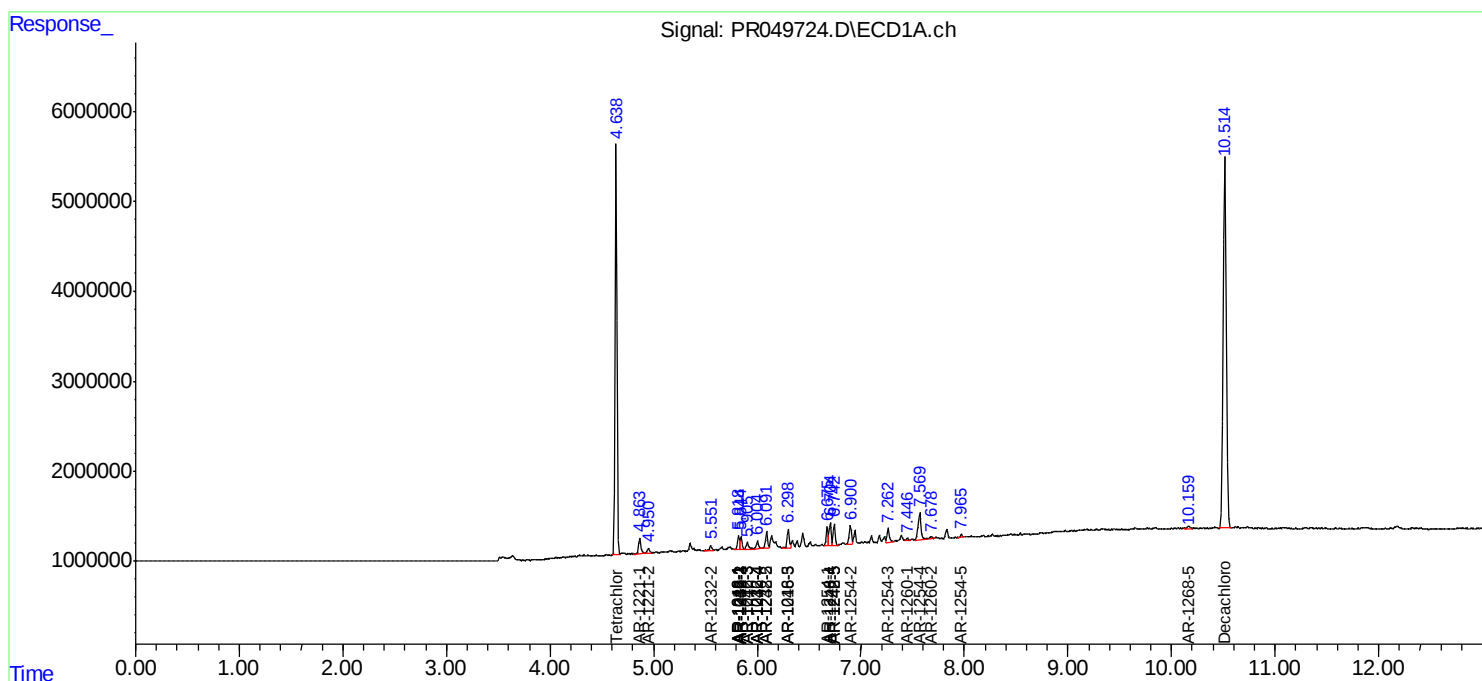


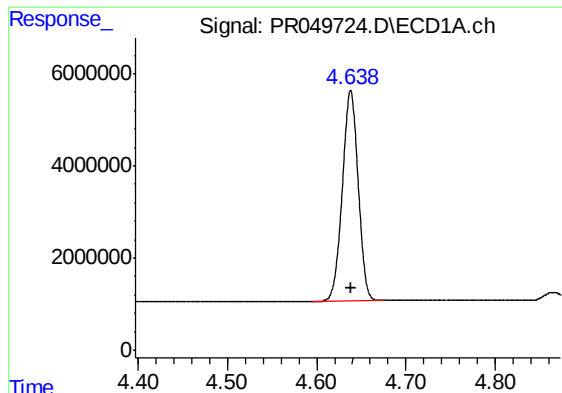

#1 Tetrachloro-m-xylene


R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 56184168
Conc: 14.39 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021

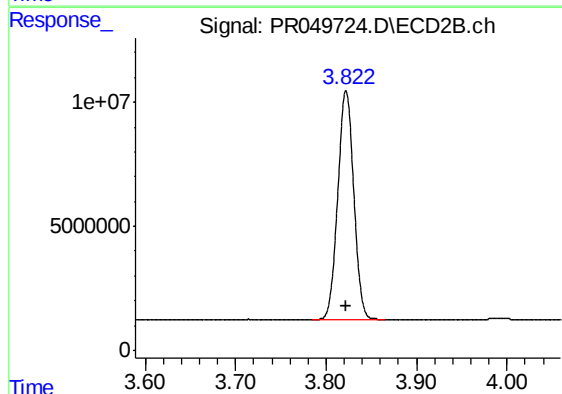


#1 Tetrachloro-m-xylene

R.T.: 3.822 min
Delta R.T.: 0.000 min
Response: 112486115
Conc: 16.96 ng/ml

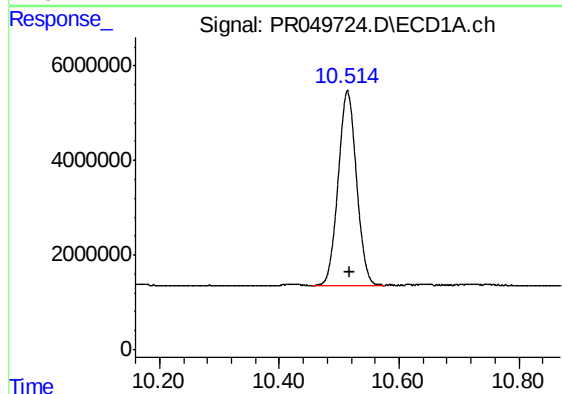


#2 Decachlorobiphenyl

R.T.: 10.514 min
Delta R.T.: -0.003 min
Response: 87046546
Conc: 19.59 ng/ml

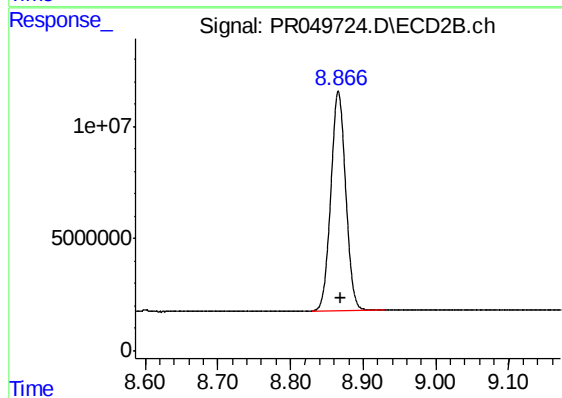

#2 Decachlorobiphenyl


R.T.: 8.866 min
Delta R.T.: -0.003 min
Response: 138615255
Conc: 18.21 ng/ml



#3 AR-1016-1


R.T.: 5.819 min
Delta R.T.: -0.001 min
Response: 1941748
Conc: 12.63 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021




#3 AR-1016-1

R.T.: 4.912 min
Delta R.T.: 0.000 min
Response: 3419350
Conc: 14.24 ng/ml




#4 AR-1016-2

R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 2054494
Conc: 9.62 ng/ml

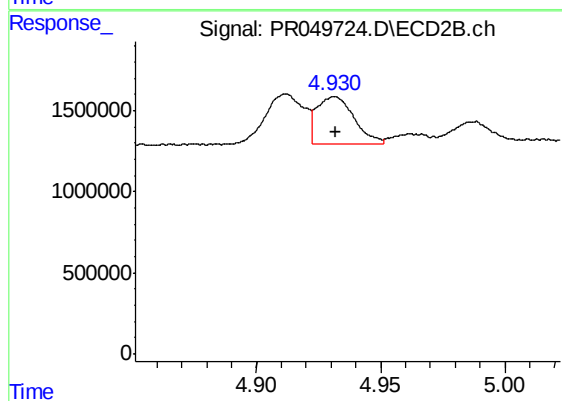

#4 AR-1016-2


R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 3070002
Conc: 8.90 ng/ml

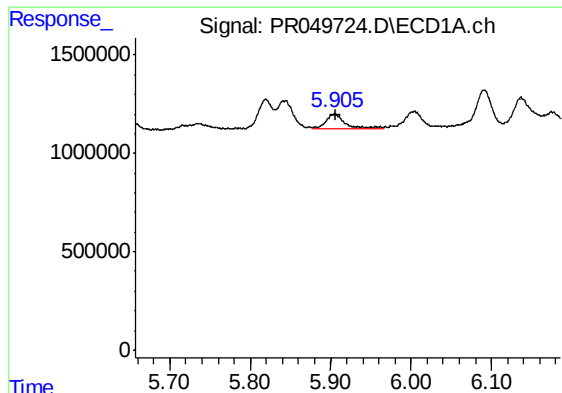

#5 AR-1016-3


R.T.: 5.905 min
Delta R.T.: 0.000 min
Response: 1236662
Conc: 9.63 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021

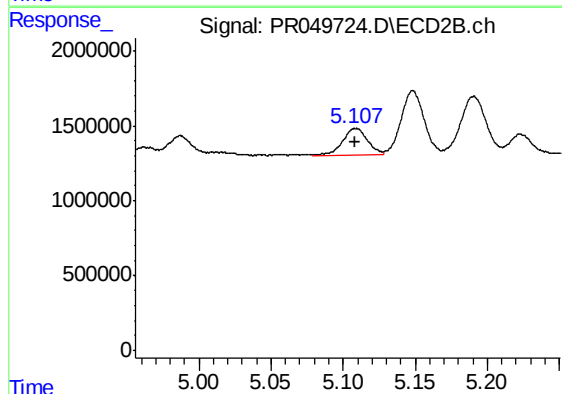


#5 AR-1016-3

R.T.: 5.108 min
Delta R.T.: 0.000 min
Response: 2149864
Conc: 11.81 ng/ml

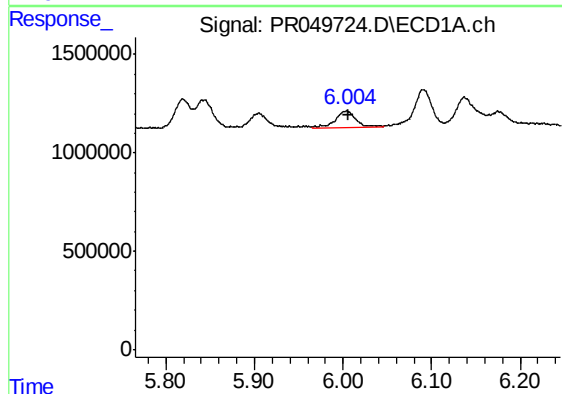


#6 AR-1016-4

R.T.: 6.005 min
Delta R.T.: -0.002 min
Response: 1334939
Conc: 12.55 ng/ml

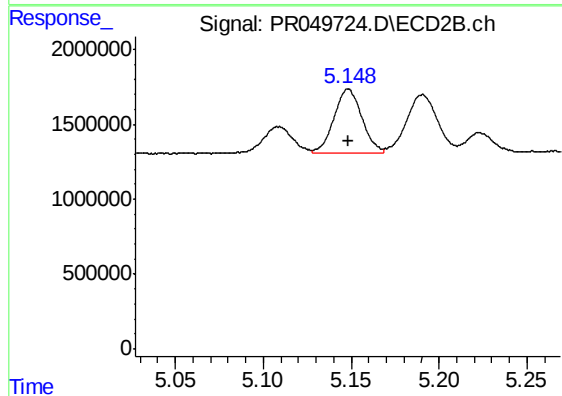

#6 AR-1016-4


R.T.: 5.148 min
Delta R.T.: 0.000 min
Response: 4746553
Conc: 34.14 ng/ml



#7 AR-1016-5


R.T.: 6.299 min
Delta R.T.: 0.000 min
Response: 2898845
Conc: 27.06 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021




#7 AR-1016-5

R.T.: 5.363 min
Delta R.T.: 0.000 min
Response: 5686839
Conc: 30.27 ng/ml




#8 AR-1221-1

R.T.: 4.864 min
Delta R.T.: 0.013 min
Response: 2637631
Conc: 63.81 ng/ml

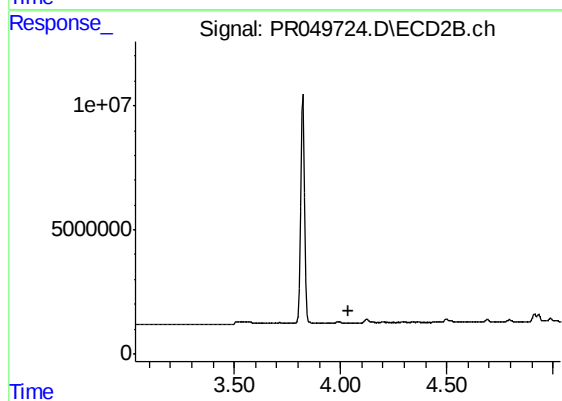

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 4.035 min
Response: 0
Conc: N.D.



#9 AR-1221-2


R.T.: 4.950 min
Delta R.T.: 0.010 min
Response: 836404
Conc: 26.81 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021




#9 AR-1221-2

R.T.: 4.124 min
Delta R.T.: 0.002 min
Response: 1962587
Conc: 39.93 ng/ml




#12 AR-1232-2

R.T.: 5.550 min
Delta R.T.: 0.000 min
Response: 992395
Conc: 23.42 ng/ml

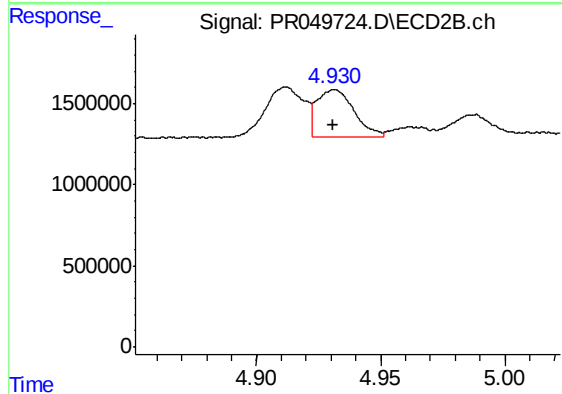

#12 AR-1232-2


R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 3070002
Conc: 23.11 ng/ml



#13 AR-1232-3


R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 2054494
Conc: 24.11 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021




#13 AR-1232-3

R.T.: 5.108 min
Delta R.T.: 0.001 min
Response: 2149864
Conc: 30.92 ng/ml




#14 AR-1232-4

R.T.: 6.005 min
Delta R.T.: -0.001 min
Response: 1334939
Conc: 31.32 ng/ml

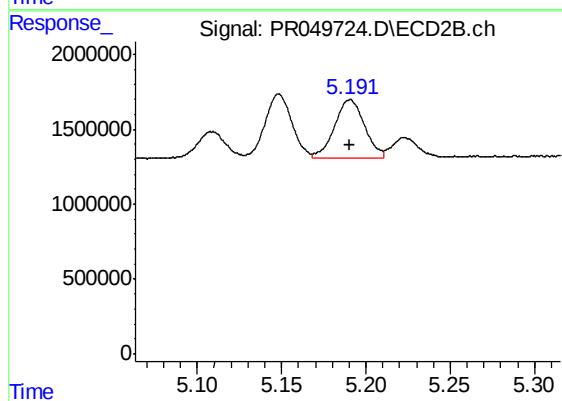

#14 AR-1232-4


R.T.: 5.191 min
Delta R.T.: 0.000 min
Response: 4765199
Conc: 81.06 ng/ml



#15 AR-1232-5


R.T.: 6.091 min
Delta R.T.: 0.000 min
Response: 2704793
Conc: 81.79 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021




#15 AR-1232-5

R.T.: 5.363 min
Delta R.T.: 0.000 min
Response: 5686839
Conc: 86.14 ng/ml




#16 AR-1242-1

R.T.: 5.819 min
Delta R.T.: 0.000 min
Response: 1941748
Conc: 17.32 ng/ml

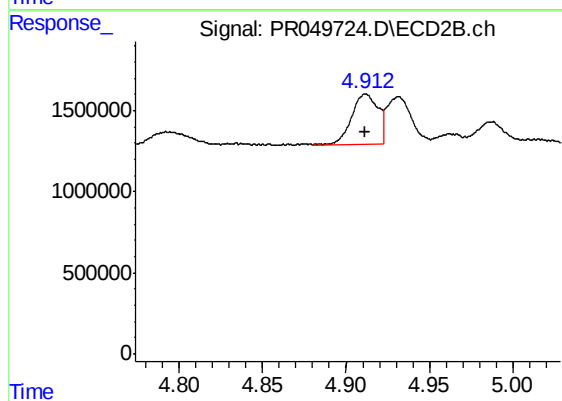

#16 AR-1242-1


R.T.: 4.912 min
Delta R.T.: 0.000 min
Response: 3419350
Conc: 19.48 ng/ml

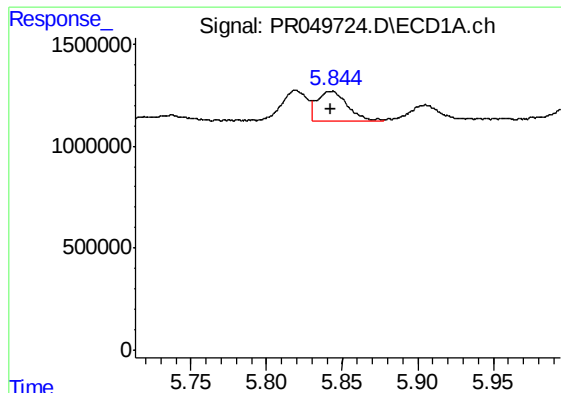

#17 AR-1242-2


R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 2054494
Conc: 13.01 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021

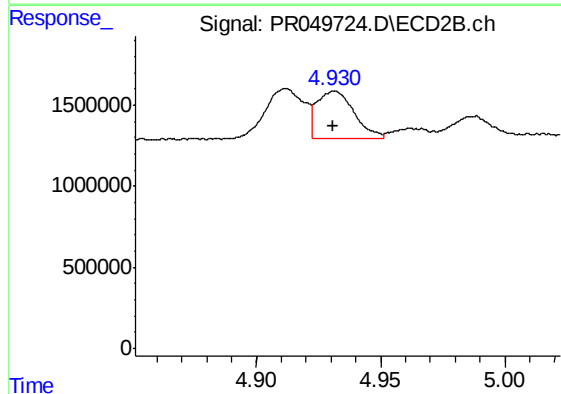


#17 AR-1242-2

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 3070002
Conc: 12.23 ng/ml

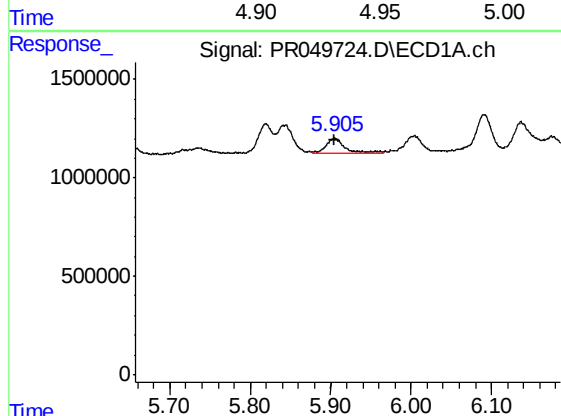


#18 AR-1242-3

R.T.: 5.905 min
Delta R.T.: 0.000 min
Response: 1236662
Conc: 12.91 ng/ml

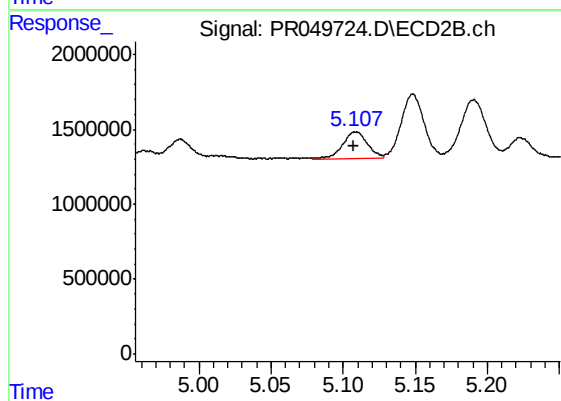

#18 AR-1242-3


R.T.: 5.108 min
Delta R.T.: 0.000 min
Response: 2149864
Conc: 16.11 ng/ml



#19 AR-1242-4


R.T.: 6.005 min
Delta R.T.: 0.000 min
Response: 1334939
Conc: 16.66 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021




#19 AR-1242-4

R.T.: 5.191 min
Delta R.T.: 0.000 min
Response: 4765199
Conc: 38.45 ng/ml




#20 AR-1242-5

R.T.: 6.742 min
Delta R.T.: 0.000 min
Response: 3234053
Conc: 35.50 ng/ml

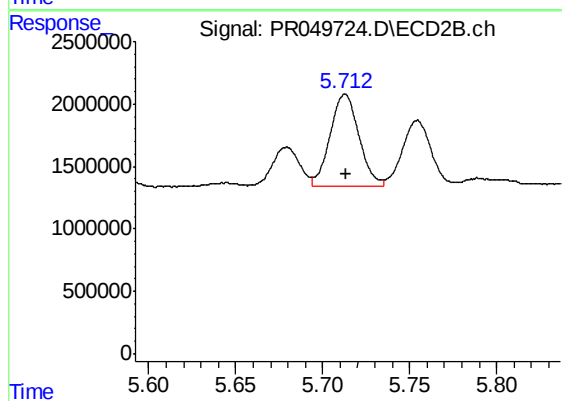

#20 AR-1242-5


R.T.: 5.713 min
Delta R.T.: 0.000 min
Response: 8552216
Conc: 50.12 ng/ml



#21 AR-1248-1


R.T.: 5.819 min
Delta R.T.: 0.000 min
Response: 1941748
Conc: 22.66 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021




#21 AR-1248-1

R.T.: 4.912 min
Delta R.T.: 0.000 min
Response: 3419350
Conc: 25.34 ng/ml




#22 AR-1248-2

R.T.: 6.091 min
Delta R.T.: 0.000 min
Response: 2704793
Conc: 22.50 ng/ml

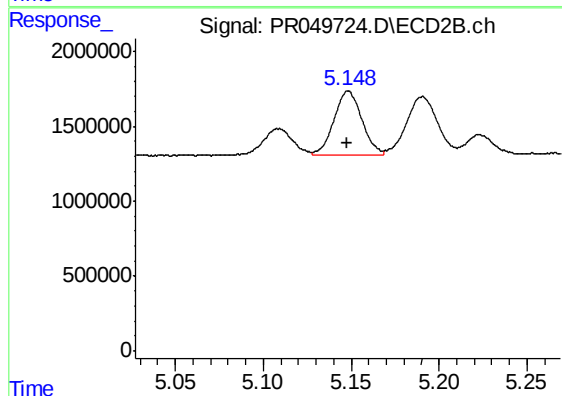

#22 AR-1248-2


R.T.: 5.148 min
Delta R.T.: 0.000 min
Response: 4746553
Conc: 26.78 ng/ml



#23 AR-1248-3


R.T.: 6.299 min
Delta R.T.: 0.000 min
Response: 2898845
Conc: 21.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021




#23 AR-1248-3

R.T.: 5.191 min
Delta R.T.: 0.000 min
Response: 4765199
Conc: 25.29 ng/ml

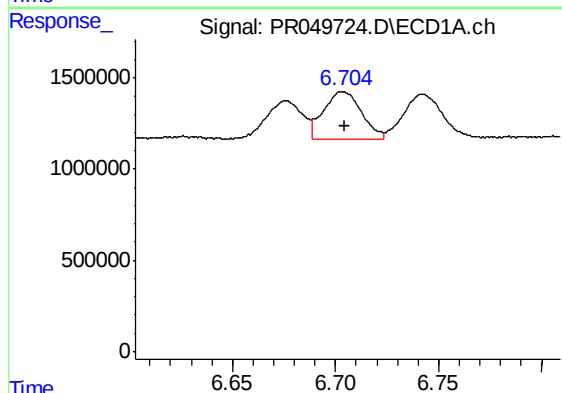


#24 AR-1248-4

R.T.: 6.704 min
Delta R.T.: 0.000 min
Response: 3297892
Conc: 20.58 ng/ml

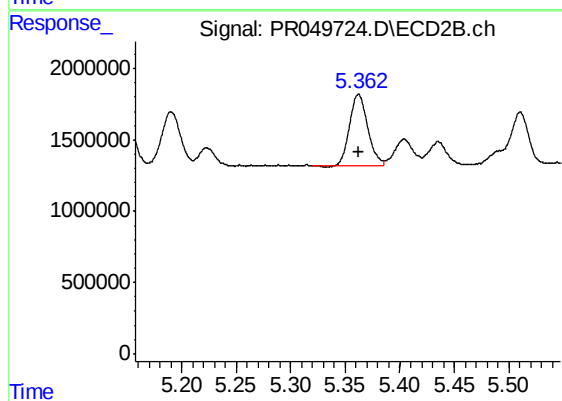

#24 AR-1248-4


R.T.: 5.363 min
Delta R.T.: 0.000 min
Response: 5686839
Conc: 24.44 ng/ml



#25 AR-1248-5


R.T.: 6.742 min
Delta R.T.: 0.000 min
Response: 3234053
Conc: 21.03 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021




#25 AR-1248-5

R.T.: 5.755 min
Delta R.T.: 0.000 min
Response: 6069474
Conc: 24.64 ng/ml

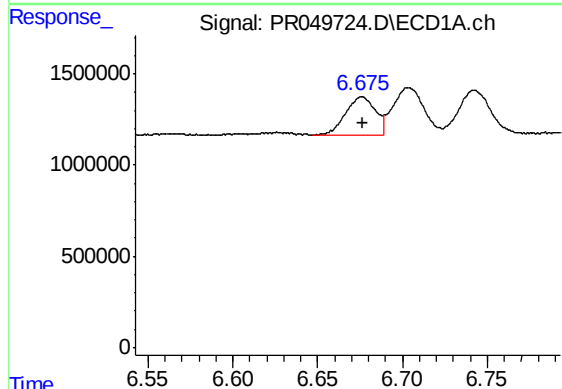


#26 AR-1254-1

R.T.: 6.676 min
Delta R.T.: 0.000 min
Response: 2615030
Conc: 16.44 ng/ml

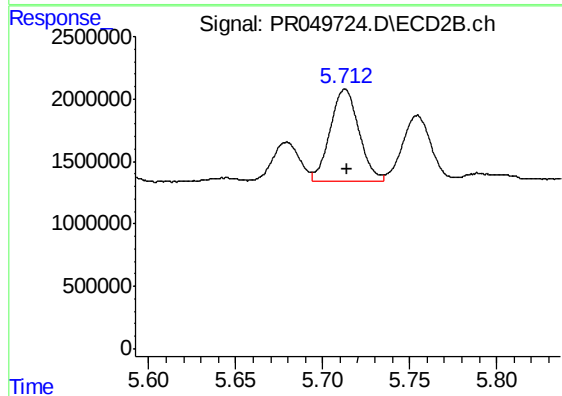

#26 AR-1254-1


R.T.: 5.713 min
Delta R.T.: -0.001 min
Response: 8552216
Conc: 22.75 ng/ml



#27 AR-1254-2


R.T.: 6.901 min
Delta R.T.: 0.007 min
Response: 3488330
Conc: 13.85 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021




#27 AR-1254-2

R.T.: 5.860 min
Delta R.T.: 0.000 min
Response: 2611778
Conc: 8.10 ng/ml




#28 AR-1254-3

R.T.: 7.263 min
Delta R.T.: -0.002 min
Response: 2429615
Conc: 8.79 ng/ml

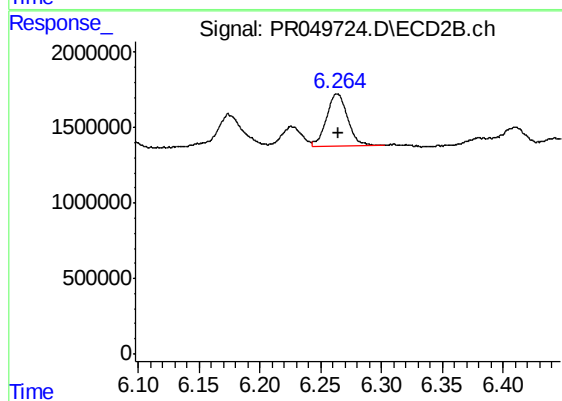

#28 AR-1254-3


R.T.: 6.264 min
Delta R.T.: 0.000 min
Response: 4207594
Conc: 7.38 ng/ml

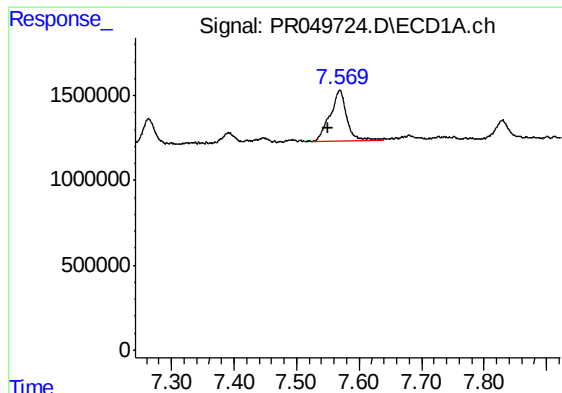

#29 AR-1254-4


R.T.: 7.569 min
Delta R.T.: 0.018 min
Response: 5533971
Conc: 26.30 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021

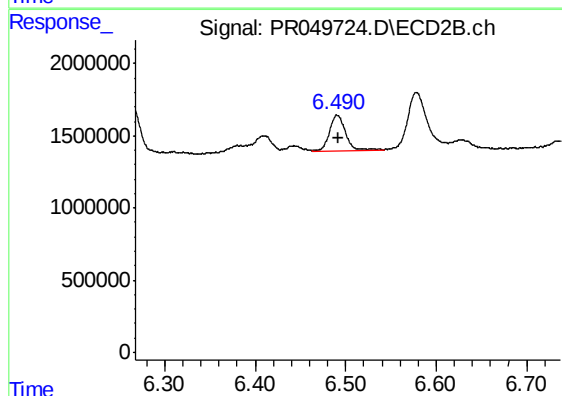


#29 AR-1254-4

R.T.: 6.491 min
Delta R.T.: 0.000 min
Response: 3171602
Conc: 8.87 ng/ml

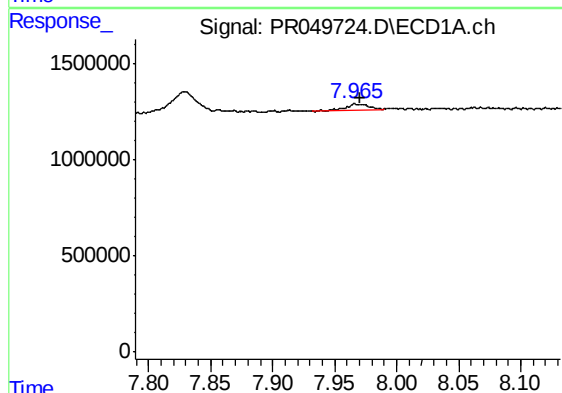


#30 AR-1254-5

R.T.: 7.966 min
Delta R.T.: -0.004 min
Response: 392648
Conc: 1.73 ng/ml

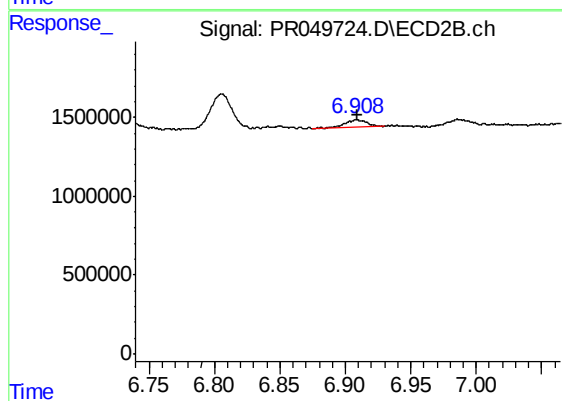

#30 AR-1254-5


R.T.: 6.909 min
Delta R.T.: 0.000 min
Response: 568418
Conc: 1.14 ng/ml

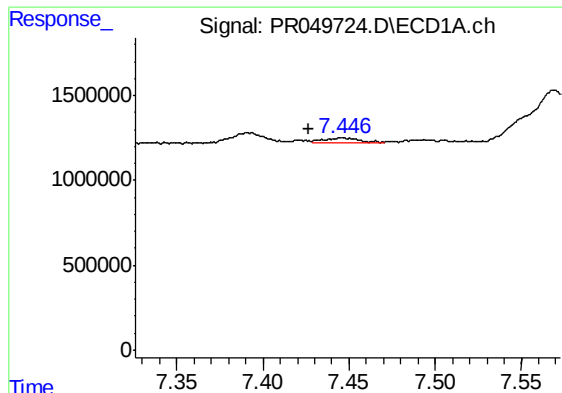

#31 AR-1260-1


R.T.: 7.446 min
Delta R.T.: 0.019 min
Response: 369872
Conc: 1.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021

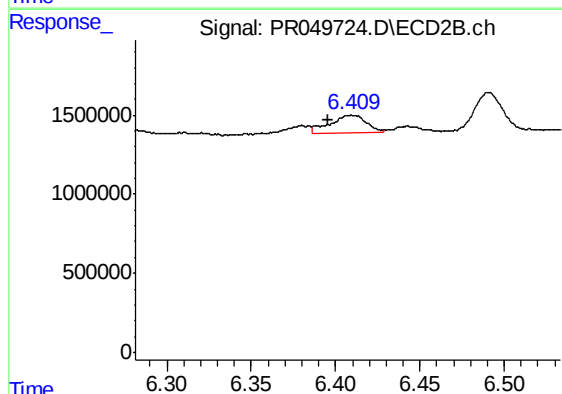


#31 AR-1260-1

R.T.: 6.410 min
Delta R.T.: 0.015 min
Response: 1692814
Conc: 4.72 ng/ml

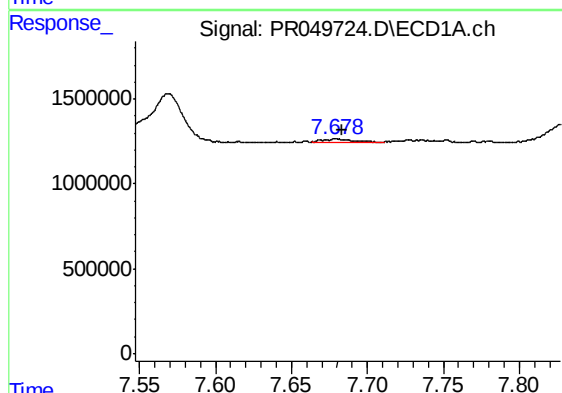


#32 AR-1260-2

R.T.: 7.679 min
Delta R.T.: -0.004 min
Response: 306961
Conc: 1.26 ng/ml

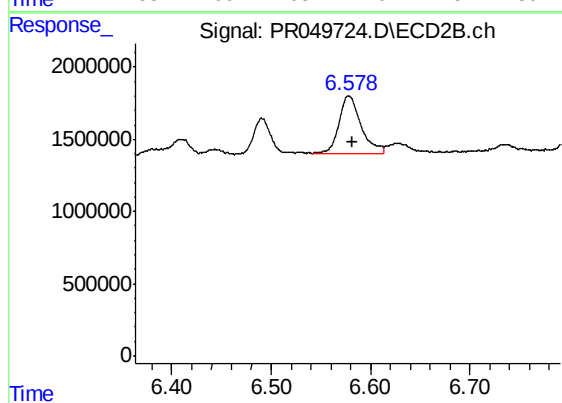

#32 AR-1260-2


R.T.: 6.578 min
Delta R.T.: -0.003 min
Response: 6214450
Conc: 14.00 ng/ml



#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 8.042 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021

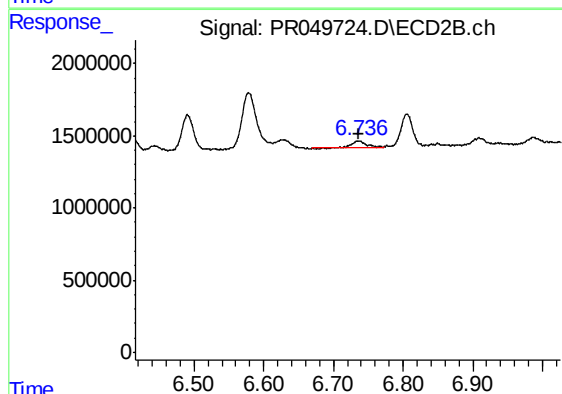


#33 AR-1260-3

R.T.: 6.735 min
Delta R.T.: 0.000 min
Response: 632657
Conc: 1.50 ng/ml

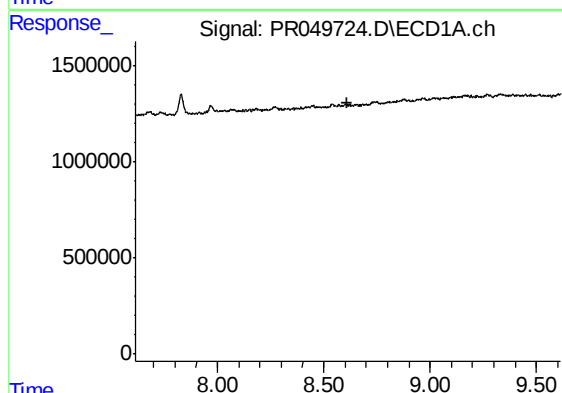


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 8.614 min
Response: 0
Conc: N.D.

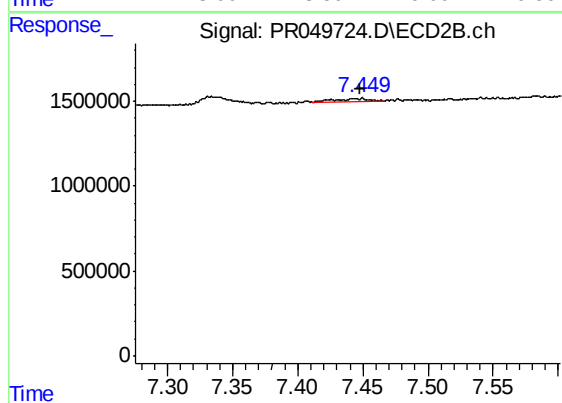

#35 AR-1260-5


R.T.: 7.449 min
Delta R.T.: 0.001 min
Response: 440922
Conc: 0.48 ng/ml



#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 8.041 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021

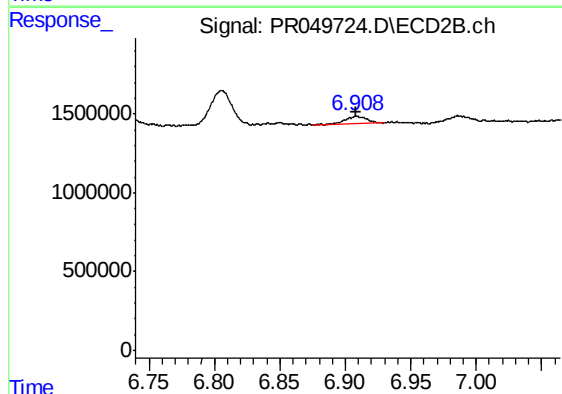


#36 AR-1262-1

R.T.: 6.909 min
Delta R.T.: 0.000 min
Response: 568418
Conc: 2.21 ng/ml




#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.613 min
Response: 0
Conc: N.D.

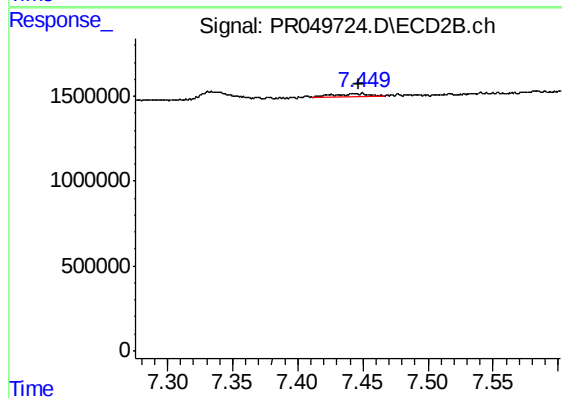

#37 AR-1262-2


R.T.: 7.449 min
Delta R.T.: 0.003 min
Response: 440922
Conc: 0.45 ng/ml



#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.936 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021




#38 AR-1262-3

R.T.: 7.712 min
Delta R.T.: -0.020 min
Response: 49913
Conc: 0.14 ng/ml

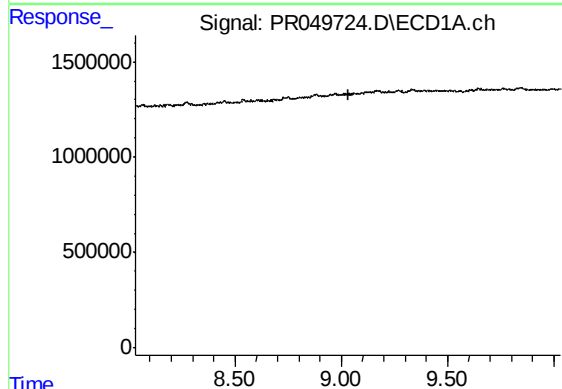


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 9.031 min
Response: 0
Conc: N.D.

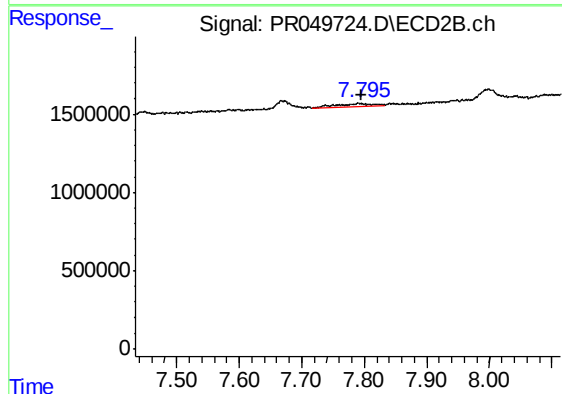

#39 AR-1262-4


R.T.: 7.795 min
Delta R.T.: 0.000 min
Response: 863035
Conc: 1.21 ng/ml



#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 9.728 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021




#40 AR-1262-5

R.T.: 8.320 min
Delta R.T.: 0.024 min
Response: 1167195
Conc: 3.63 ng/ml

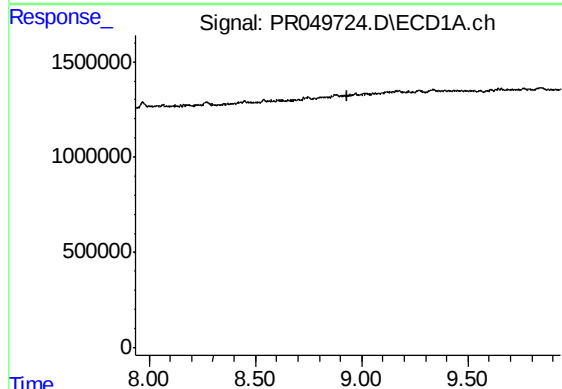


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.935 min
Response: 0
Conc: N.D.

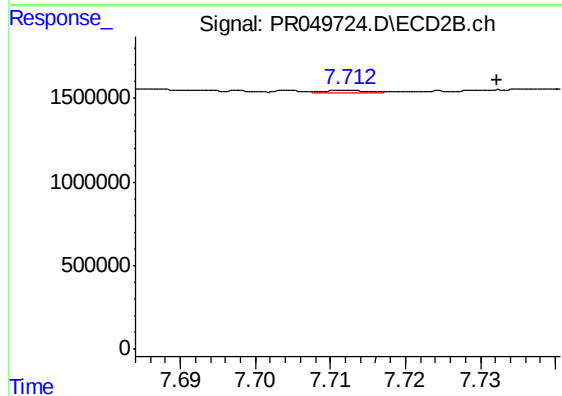

#41 AR-1268-1


R.T.: 7.712 min
Delta R.T.: -0.020 min
Response: 49913
Conc: 0.04 ng/ml



#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 9.036 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021

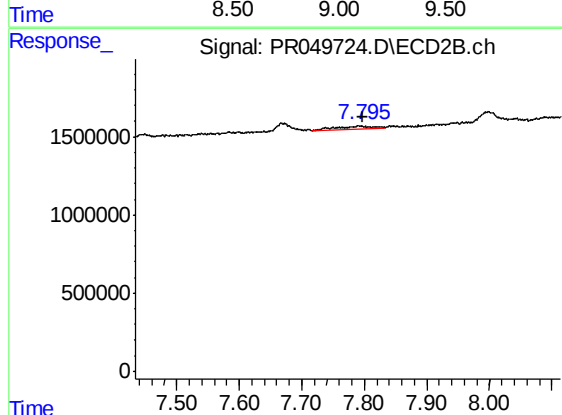


#42 AR-1268-2

R.T.: 7.795 min
Delta R.T.: -0.001 min
Response: 863035
Conc: 0.82 ng/ml

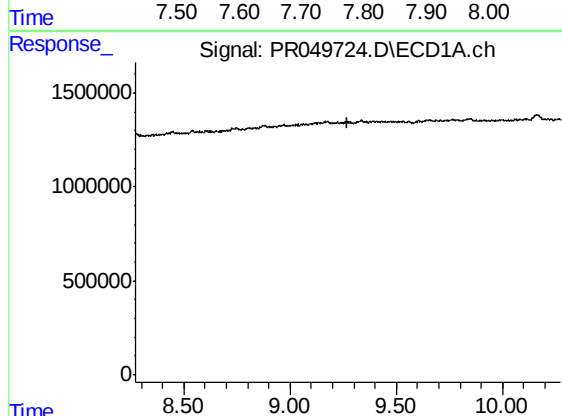


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 9.272 min
Response: 0
Conc: N.D.

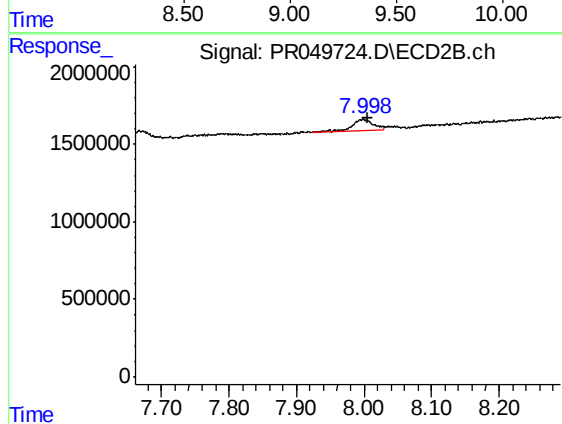

#43 AR-1268-3


R.T.: 7.999 min
Delta R.T.: -0.008 min
Response: 1613746
Conc: 1.84 ng/ml



#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 9.729 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2021

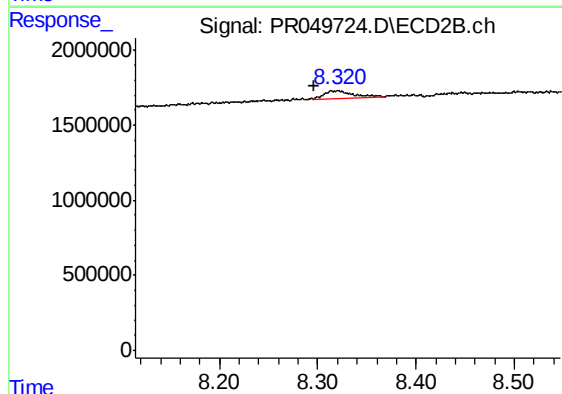


#44 AR-1268-4

R.T.: 8.320 min
Delta R.T.: 0.023 min
Response: 1167195
Conc: 3.21 ng/ml

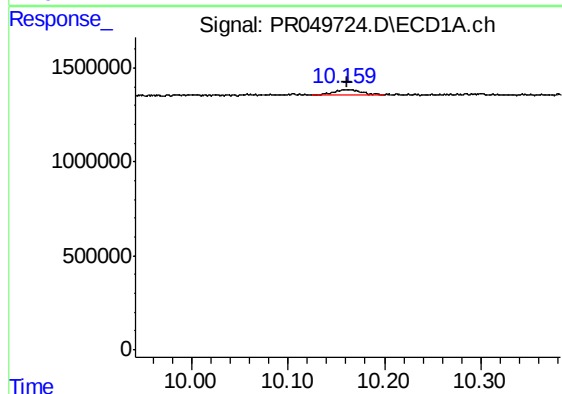

#45 AR-1268-5

R.T.: 10.160 min
Delta R.T.: -0.002 min
Response: 532146
Conc: 0.33 ng/ml

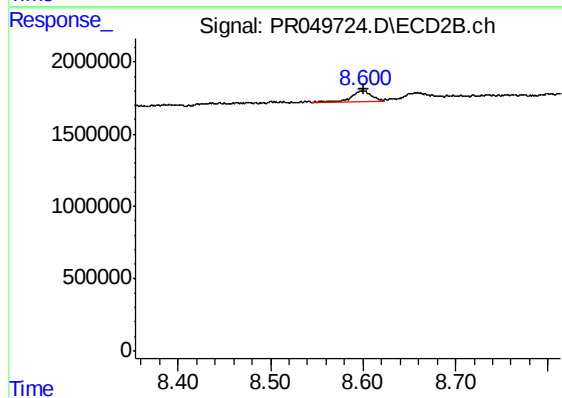

#45 AR-1268-5

R.T.: 8.600 min
Delta R.T.: 0.000 min
Response: 1113897
Conc: 0.37 ng/ml