

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040221\
 Data File : PR049751.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2021 02:03
 Operator : DD\AJ
 Sample : M1458-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 01:53:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Apr 03 08:12:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.636	3.820	88330459	139.3E6	22.623	21.012
2)	SA Decachlor...	10.512	8.863	118.6E6	147.0E6	26.696	19.309 #
Target Compounds							
3)	L1 AR-1016-1	5.818	4.910	7249244	7541940	47.157	31.409 #
4)	L1 AR-1016-2	5.840	4.930	9529468	10090121	44.603	29.249 #
5)	L1 AR-1016-3	5.903	5.106	5956067	5455717	46.387	29.966 #
6)	L1 AR-1016-4	6.003	5.147	4831791	4571685	45.409	32.883 #
7)	L1 AR-1016-5	6.297	5.361	5210857	6046948	48.636	32.184 #
8)	L2 AR-1221-1	4.863	4.032	4141840	497607	100.200	7.808 #
9)	L2 AR-1221-2	4.945	4.121	1968991	3254664	63.108	66.223
10)	L2 AR-1221-3	5.015	4.196	2934841	3672950	30.922	23.338
11)	L3 AR-1232-1	5.015	4.196	2934841	3672950	37.981	29.134
12)	L3 AR-1232-2	5.549	4.930	4503831	10090121	106.267	75.963 #
13)	L3 AR-1232-3	5.840	5.106	9529468	5455717	111.853	78.468 #
14)	L3 AR-1232-4	6.003	5.189	4831791	5346559	113.370	90.947
15)	L3 AR-1232-5	6.090	5.361	4498037	6046948	136.014	91.596 #
16)	L4 AR-1242-1	5.818	4.910	7249244	7541940	64.656	42.975 #
17)	L4 AR-1242-2	5.840	4.930	9529468	10090121	60.329	40.191 #
18)	L4 AR-1242-3	5.903	5.106	5956067	5455717	62.195	40.894 #
19)	L4 AR-1242-4	6.003	5.189	4831791	5346559	60.301	43.140 #
20)	L4 AR-1242-5	6.742	5.713	870800	4406736	9.558	25.824 #
21)	L5 AR-1248-1	5.818	4.910	7249244	7541940	84.606	55.887 #
22)	L5 AR-1248-2	6.090	5.147	4498037	4571685	37.418	25.796 #
23)	L5 AR-1248-3	6.297	5.189	5210857	5346559	38.475	28.373 #
24)	L5 AR-1248-4	6.702	5.361	921514	6046948	5.751	25.992 #
25)	L5 AR-1248-5	6.742	5.754	870800	808305	5.662	3.282 #
26)	L6 AR-1254-1	6.674	5.713	3762091	4406736	23.649	11.722 #
27)	L6 AR-1254-2	6.891	5.859	3849454	4097679	15.283	12.709
28)	L6 AR-1254-3	7.262	6.279	2967339	9574172	10.741	16.795 #
29)	L6 AR-1254-4	7.549	6.489	2823362	1265484	13.417	3.540 #
30)	L6 AR-1254-5	7.967	6.906	12116145	14723292	53.426	29.549 #
31)	L7 AR-1260-1	7.423	6.393	10872615	11238996	54.674	31.336 #
32)	L7 AR-1260-2	7.681	6.579	11047842	13378925	45.254	30.135 #
33)	L7 AR-1260-3	8.039	6.734	8088896	12557183	43.264	29.852 #
34)	L7 AR-1260-4	8.274	7.205	9138701	10766705	41.827	30.210 #
35)	L7 AR-1260-5	8.611	7.444	17666210	25254819	39.165	27.562 #
36)	L8 AR-1262-1	8.039	6.906	8088896	14723292	30.892	57.369 #
37)	L8 AR-1262-2	8.611	7.444	17666210	25254819	35.499	25.646 #
38)	L8 AR-1262-3	8.958f	7.729	11527391	5879119	35.050	16.327 #
39)	L8 AR-1262-4	9.030	7.792	2991482	18919869	12.110	26.426 #
40)	L8 AR-1262-5	9.727	8.293	5748622	7460500	31.902	23.213 #
41)	L9 AR-1268-1	8.958f	7.729	11527391	5879119	19.655	5.241 #
42)	L9 AR-1268-2	9.030	7.792	2991482	18919869	5.556	17.881 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040221\
 Data File : PR049751.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2021 02:03
 Operator : DD\AJ
 Sample : M1458-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 01:53:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Apr 03 08:12:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	9.269	8.001	392216	1284154	0.857	1.465 #
44) L9	AR-1268-4	9.727	8.293	5748622	7460500	28.464	20.490 #
45) L9	AR-1268-5	10.158	8.596	2130588	3731754	1.302	1.226



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040221\
Data File : PR049751.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2021 02:03
Operator : DD\AJ
Sample : M1458-07
Misc : AR1660 LOD 40 PPB
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 01:53:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040221.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Apr 03 08:12:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

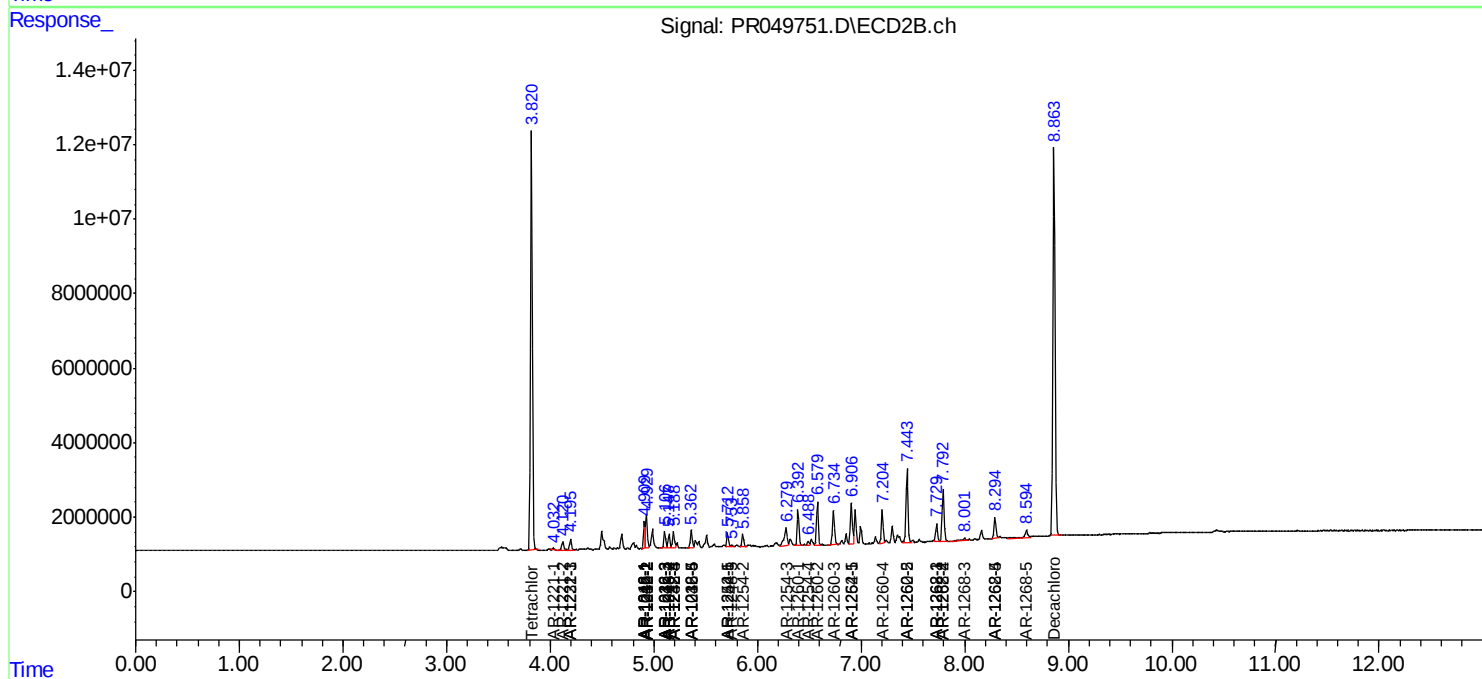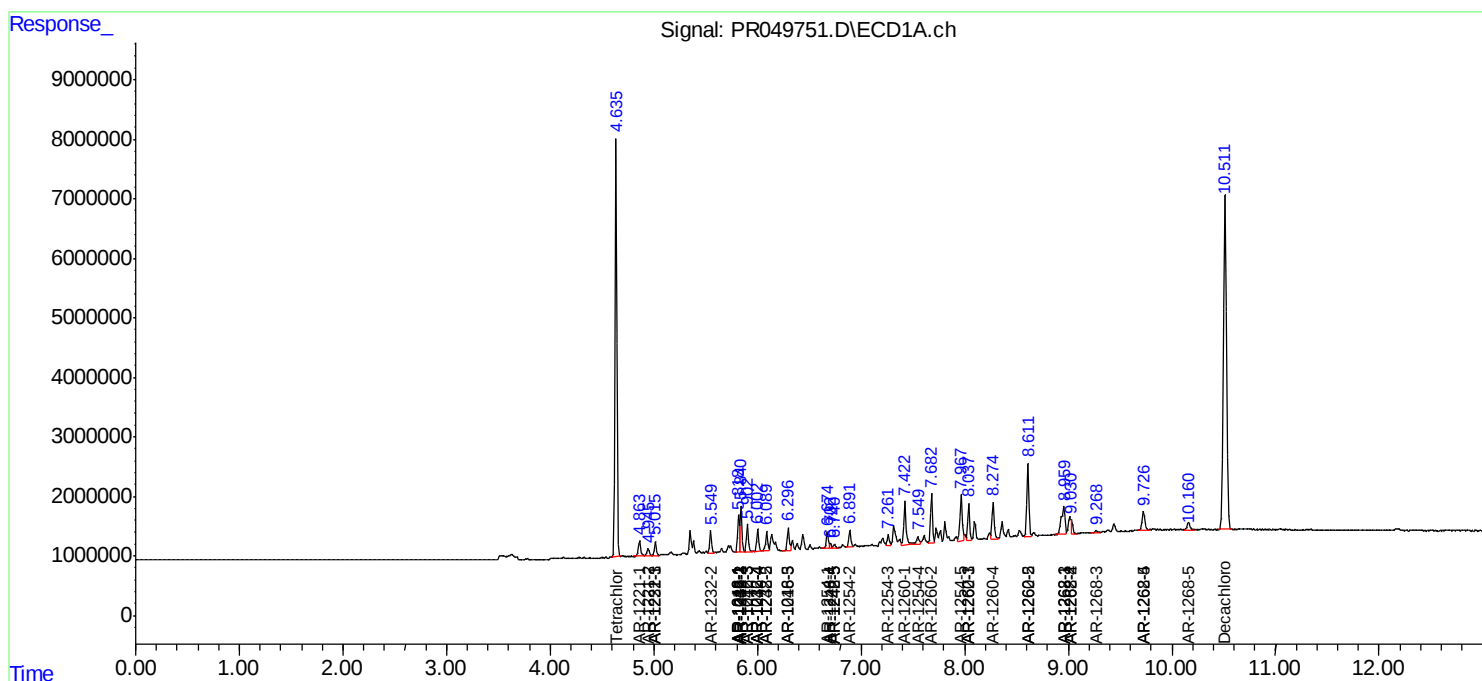


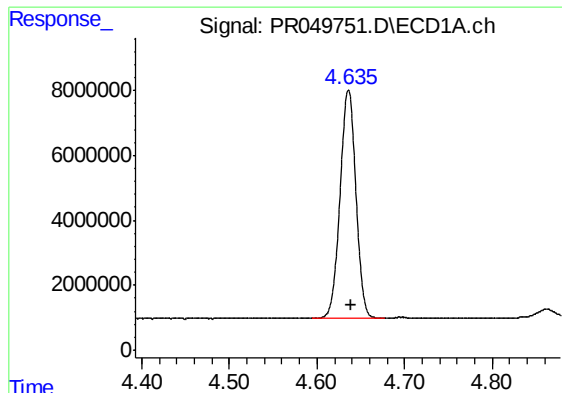

#1 Tetrachloro-m-xylene


R.T.: 4.636 min
Delta R.T.: -0.003 min
Response: 88330459
Conc: 22.62 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

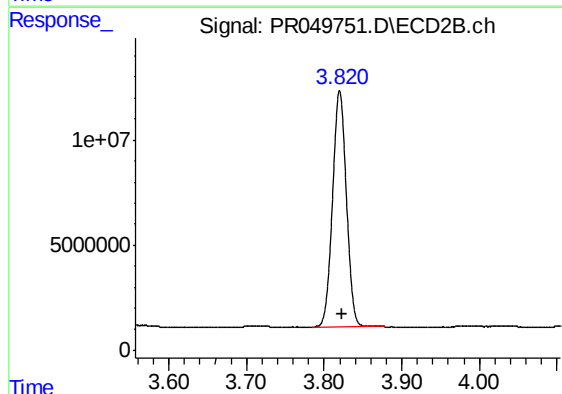


#1 Tetrachloro-m-xylene

R.T.: 3.820 min
Delta R.T.: -0.002 min
Response: 139348300
Conc: 21.01 ng/ml

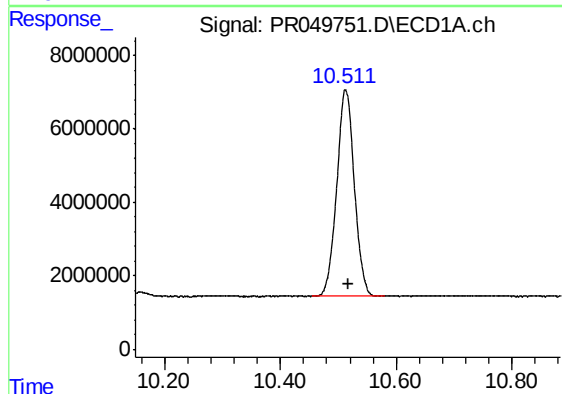


#2 Decachlorobiphenyl

R.T.: 10.512 min
Delta R.T.: -0.004 min
Response: 118614600
Conc: 26.70 ng/ml

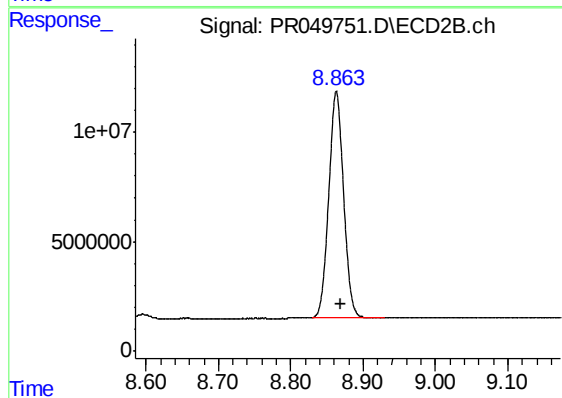

#2 Decachlorobiphenyl


R.T.: 8.863 min
Delta R.T.: -0.006 min
Response: 147003561
Conc: 19.31 ng/ml

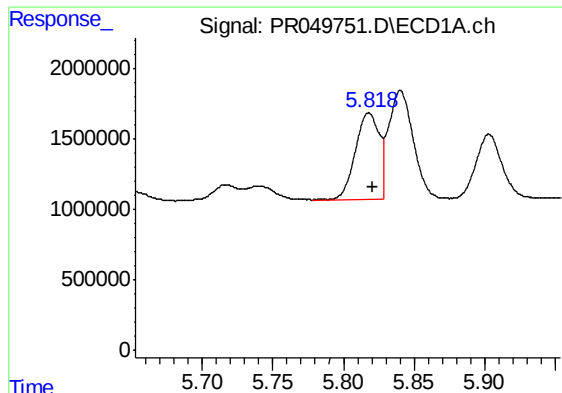

#3 AR-1016-1


R.T.: 5.818 min
Delta R.T.: -0.002 min
Response: 7249244
Conc: 47.16 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

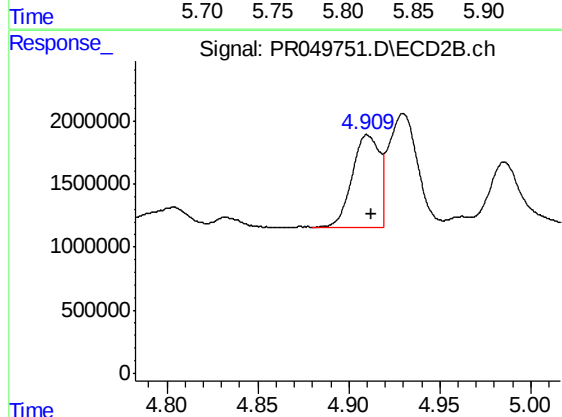


#3 AR-1016-1

R.T.: 4.910 min
Delta R.T.: -0.002 min
Response: 7541940
Conc: 31.41 ng/ml

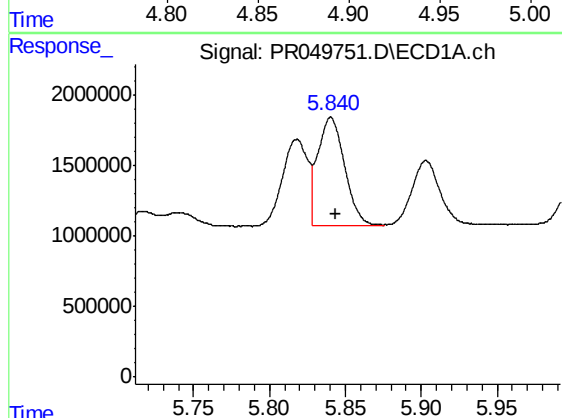


#4 AR-1016-2

R.T.: 5.840 min
Delta R.T.: -0.003 min
Response: 9529468
Conc: 44.60 ng/ml

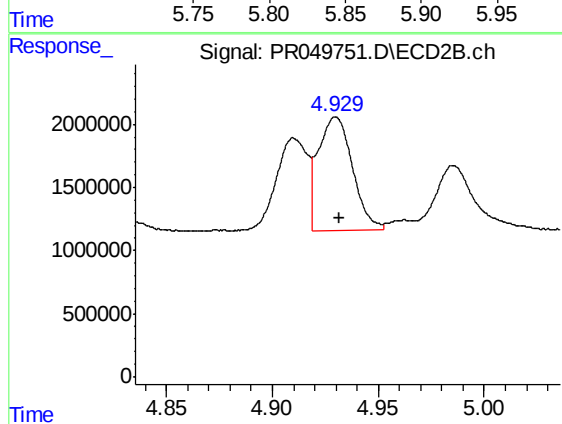

#4 AR-1016-2


R.T.: 4.930 min
Delta R.T.: -0.002 min
Response: 10090121
Conc: 29.25 ng/ml

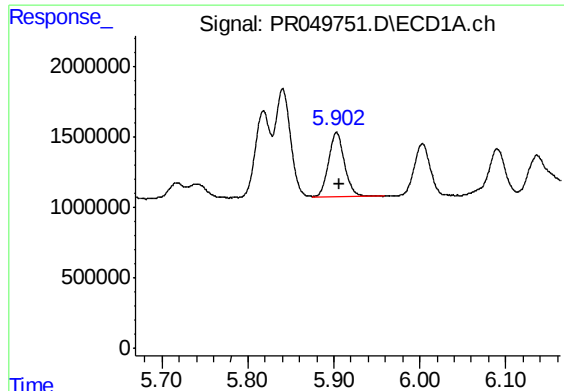

#5 AR-1016-3


R.T.: 5.903 min
Delta R.T.: -0.003 min
Response: 5956067
Conc: 46.39 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

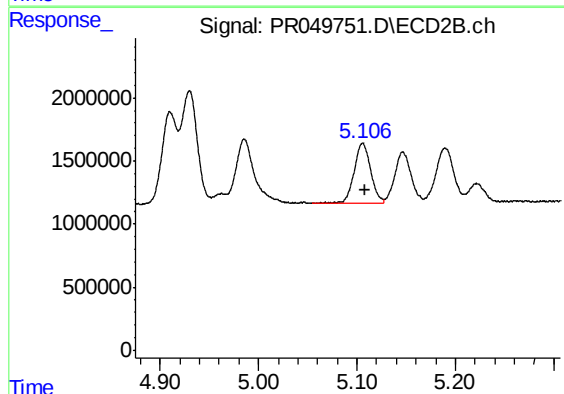


#5 AR-1016-3

R.T.: 5.106 min
Delta R.T.: -0.002 min
Response: 5455717
Conc: 29.97 ng/ml

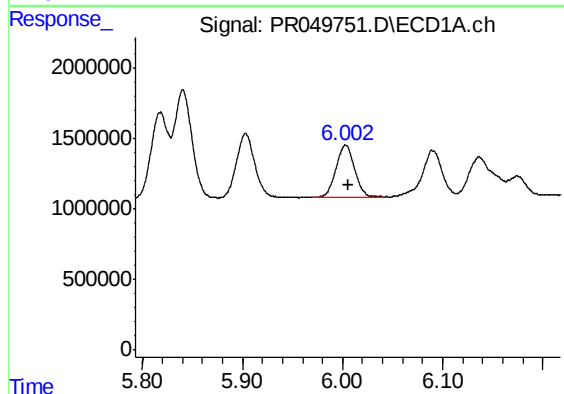


#6 AR-1016-4

R.T.: 6.003 min
Delta R.T.: -0.003 min
Response: 4831791
Conc: 45.41 ng/ml

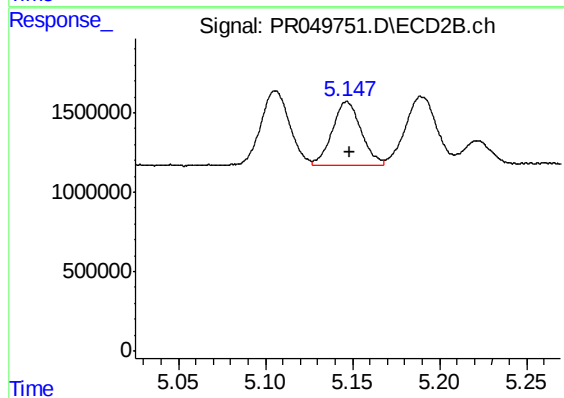

#6 AR-1016-4


R.T.: 5.147 min
Delta R.T.: -0.002 min
Response: 4571685
Conc: 32.88 ng/ml

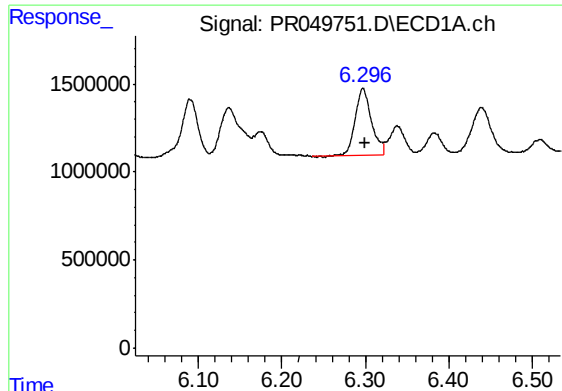

#7 AR-1016-5


R.T.: 6.297 min
Delta R.T.: -0.002 min
Response: 5210857
Conc: 48.64 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

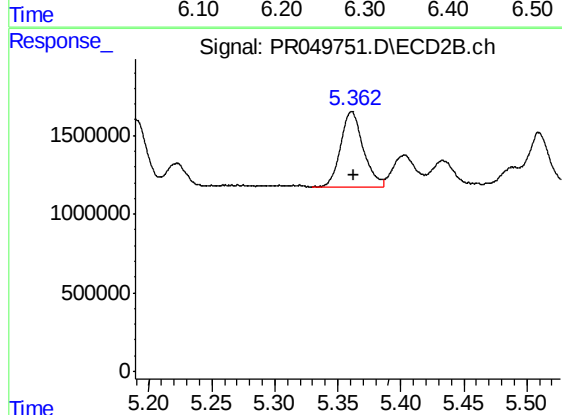


#7 AR-1016-5

R.T.: 5.361 min
Delta R.T.: -0.002 min
Response: 6046948
Conc: 32.18 ng/ml

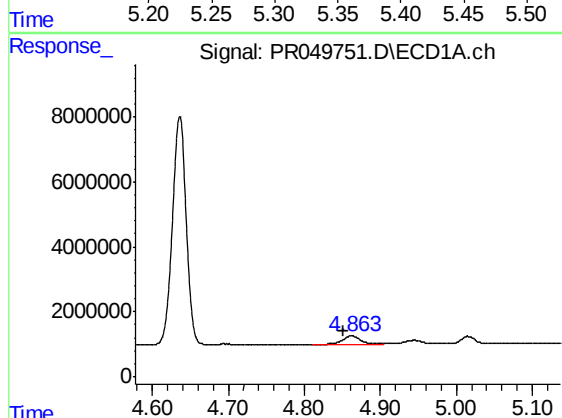


#8 AR-1221-1

R.T.: 4.863 min
Delta R.T.: 0.012 min
Response: 4141840
Conc: 100.20 ng/ml

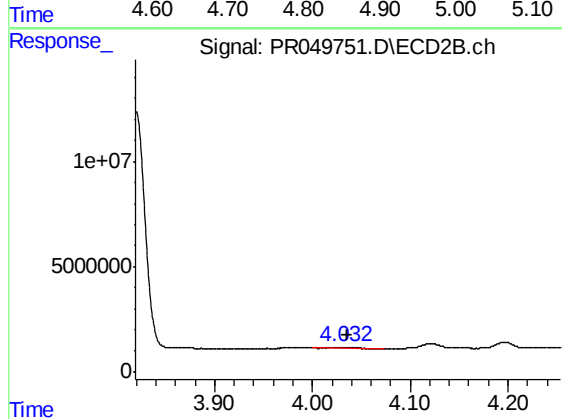

#8 AR-1221-1


R.T.: 4.032 min
Delta R.T.: -0.003 min
Response: 497607
Conc: 7.81 ng/ml

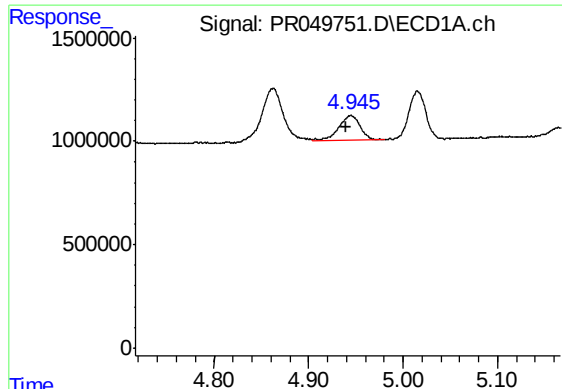

#9 AR-1221-2


R.T.: 4.945 min
Delta R.T.: 0.006 min
Response: 1968991
Conc: 63.11 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

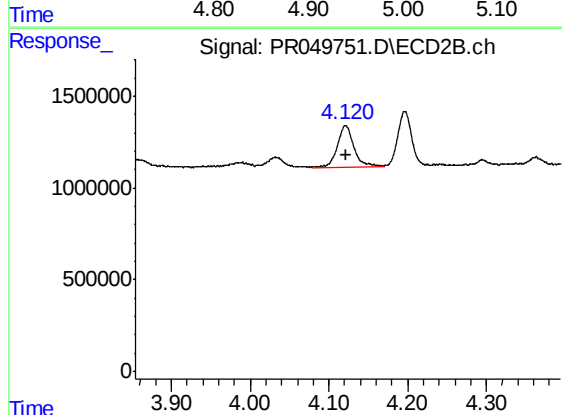


#9 AR-1221-2

R.T.: 4.121 min
Delta R.T.: -0.001 min
Response: 3254664
Conc: 66.22 ng/ml

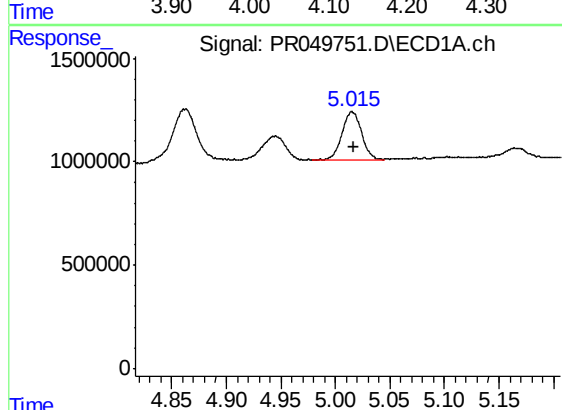


#10 AR-1221-3

R.T.: 5.015 min
Delta R.T.: -0.002 min
Response: 2934841
Conc: 30.92 ng/ml

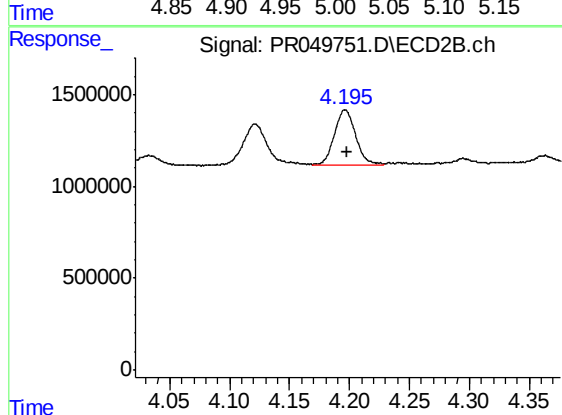

#10 AR-1221-3


R.T.: 4.196 min
Delta R.T.: -0.002 min
Response: 3672950
Conc: 23.34 ng/ml

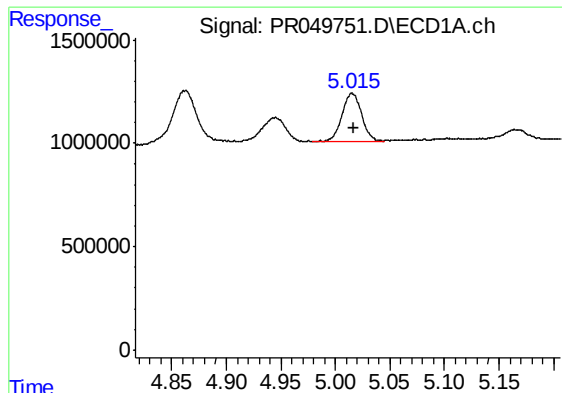

#11 AR-1232-1


R.T.: 5.015 min
Delta R.T.: -0.002 min
Response: 2934841
Conc: 37.98 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

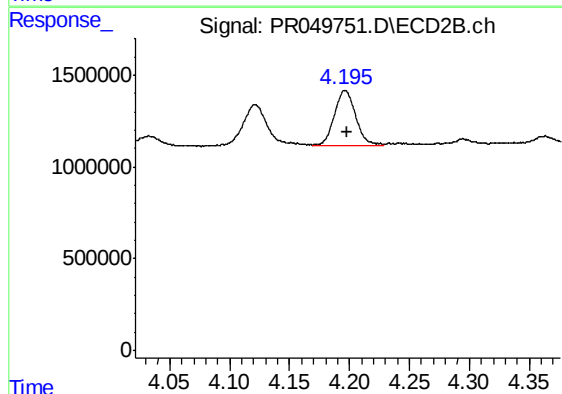


#11 AR-1232-1

R.T.: 4.196 min
Delta R.T.: -0.002 min
Response: 3672950
Conc: 29.13 ng/ml

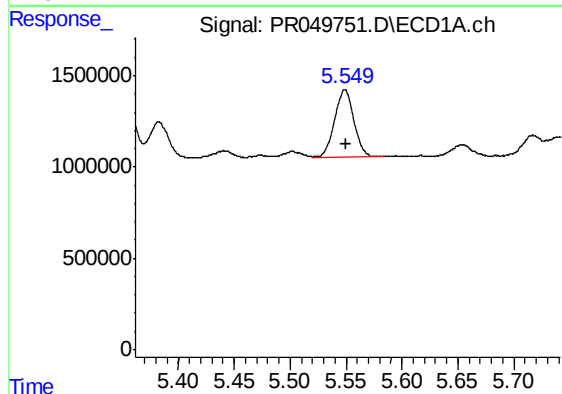


#12 AR-1232-2

R.T.: 5.549 min
Delta R.T.: -0.002 min
Response: 4503831
Conc: 106.27 ng/ml

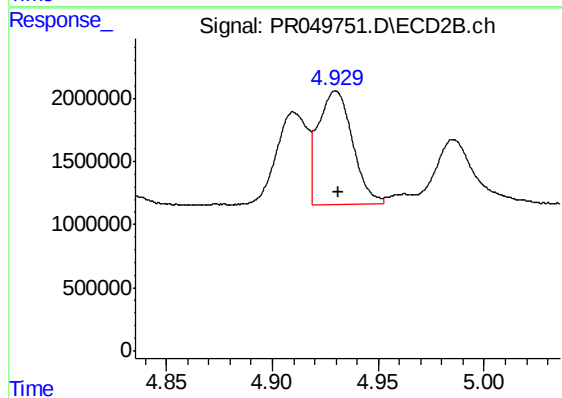

#12 AR-1232-2


R.T.: 4.930 min
Delta R.T.: -0.001 min
Response: 10090121
Conc: 75.96 ng/ml

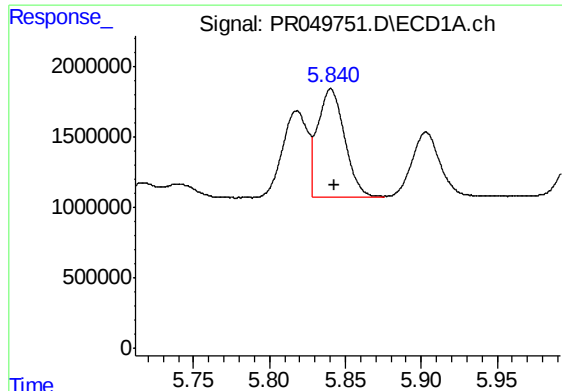

#13 AR-1232-3


R.T.: 5.840 min
Delta R.T.: -0.002 min
Response: 9529468
Conc: 111.85 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

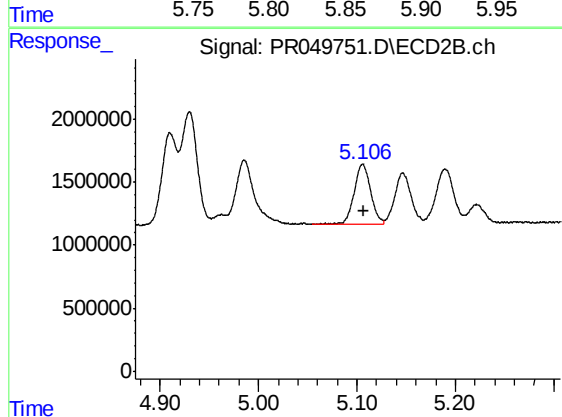


#13 AR-1232-3

R.T.: 5.106 min
Delta R.T.: -0.001 min
Response: 5455717
Conc: 78.47 ng/ml

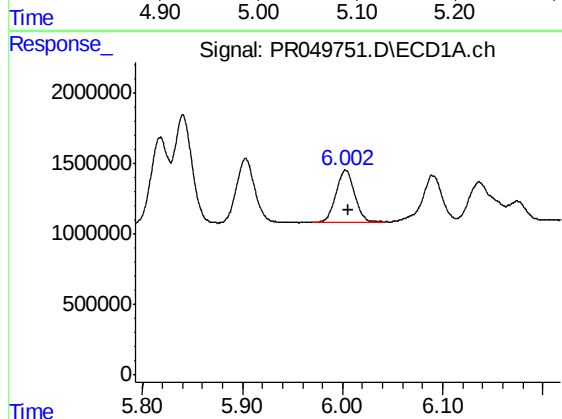


#14 AR-1232-4

R.T.: 6.003 min
Delta R.T.: -0.003 min
Response: 4831791
Conc: 113.37 ng/ml

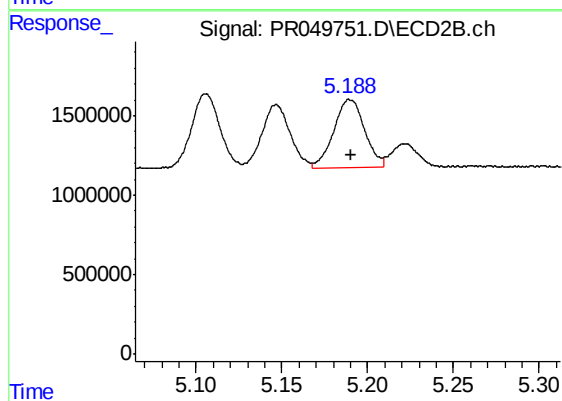

#14 AR-1232-4


R.T.: 5.189 min
Delta R.T.: -0.001 min
Response: 5346559
Conc: 90.95 ng/ml

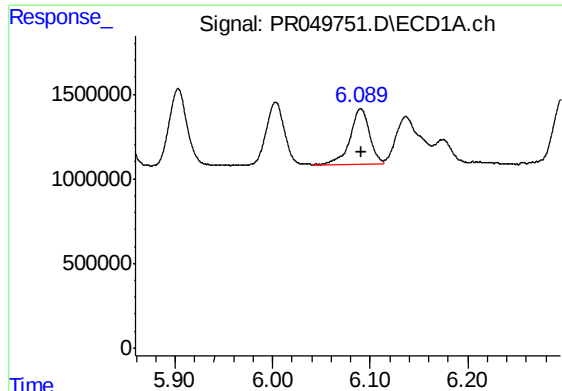

#15 AR-1232-5


R.T.: 6.090 min
Delta R.T.: -0.001 min
Response: 4498037
Conc: 136.01 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

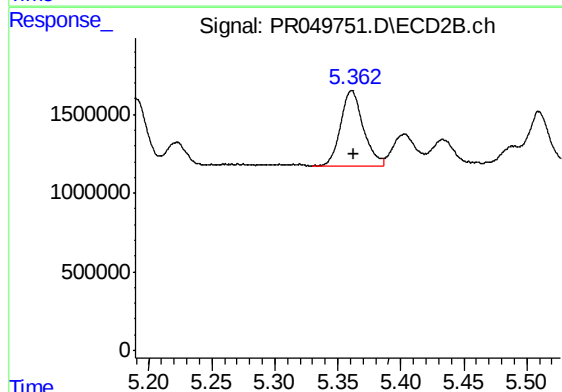


#15 AR-1232-5

R.T.: 5.361 min
Delta R.T.: -0.001 min
Response: 6046948
Conc: 91.60 ng/ml

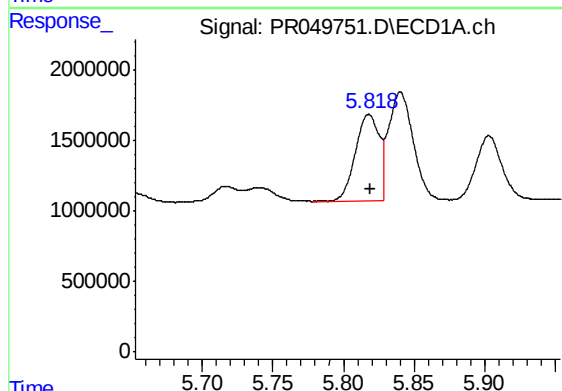


#16 AR-1242-1

R.T.: 5.818 min
Delta R.T.: -0.001 min
Response: 7249244
Conc: 64.66 ng/ml

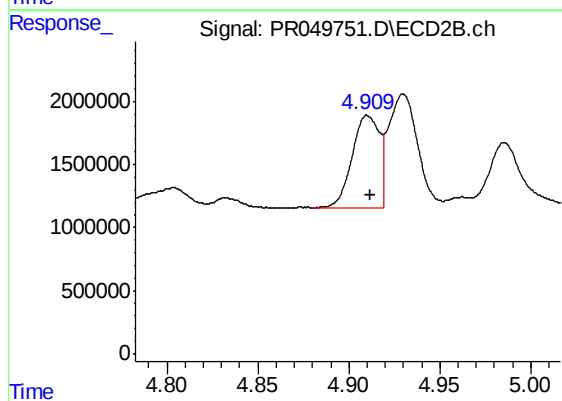

#16 AR-1242-1


R.T.: 4.910 min
Delta R.T.: -0.002 min
Response: 7541940
Conc: 42.97 ng/ml

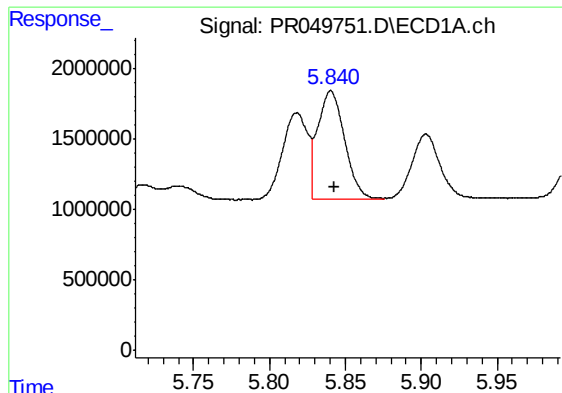

#17 AR-1242-2


R.T.: 5.840 min
Delta R.T.: -0.002 min
Response: 9529468
Conc: 60.33 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

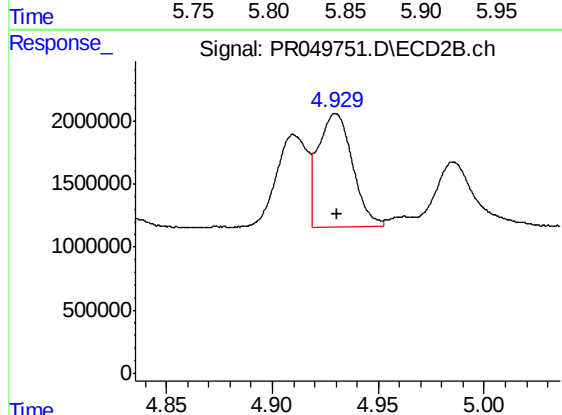


#17 AR-1242-2

R.T.: 4.930 min
Delta R.T.: 0.000 min
Response: 10090121
Conc: 40.19 ng/ml

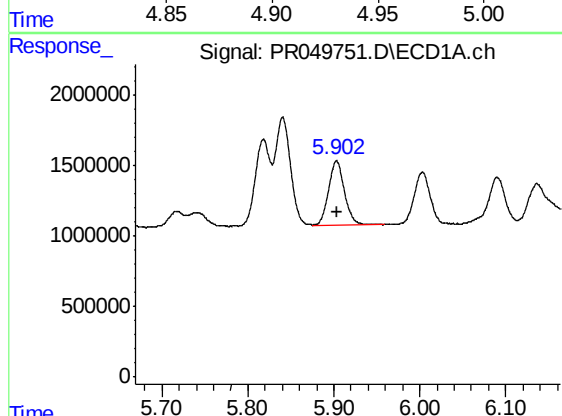


#18 AR-1242-3

R.T.: 5.903 min
Delta R.T.: -0.001 min
Response: 5956067
Conc: 62.19 ng/ml

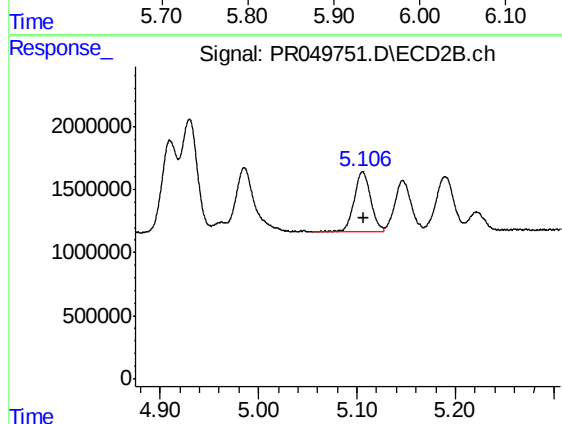

#18 AR-1242-3


R.T.: 5.106 min
Delta R.T.: -0.002 min
Response: 5455717
Conc: 40.89 ng/ml

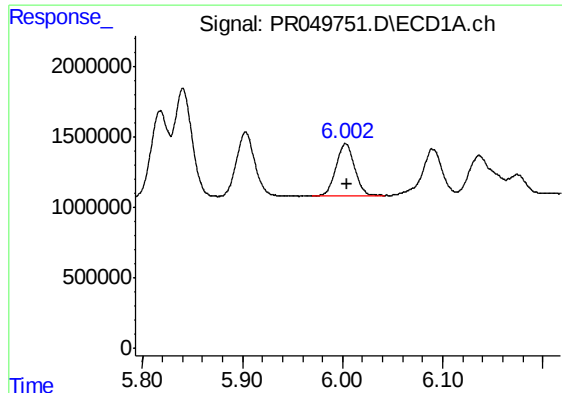

#19 AR-1242-4


R.T.: 6.003 min
Delta R.T.: -0.002 min
Response: 4831791
Conc: 60.30 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

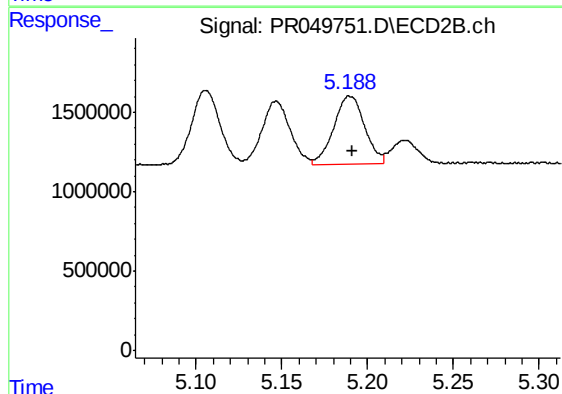


#19 AR-1242-4

R.T.: 5.189 min
Delta R.T.: -0.002 min
Response: 5346559
Conc: 43.14 ng/ml

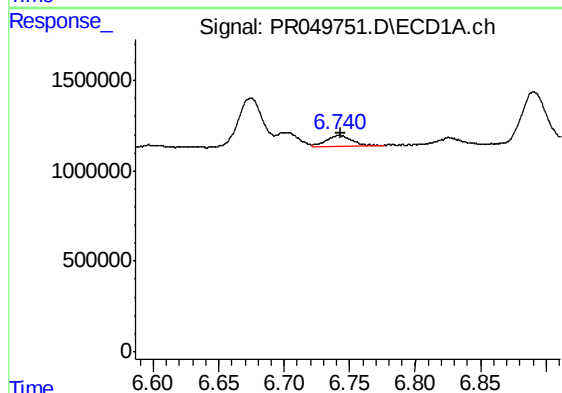


#20 AR-1242-5

R.T.: 6.742 min
Delta R.T.: 0.000 min
Response: 870800
Conc: 9.56 ng/ml

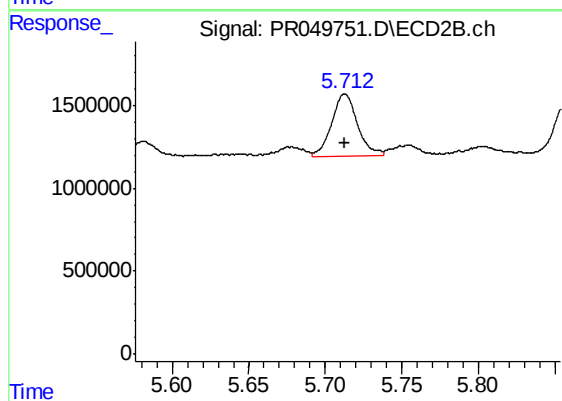

#20 AR-1242-5


R.T.: 5.713 min
Delta R.T.: 0.000 min
Response: 4406736
Conc: 25.82 ng/ml

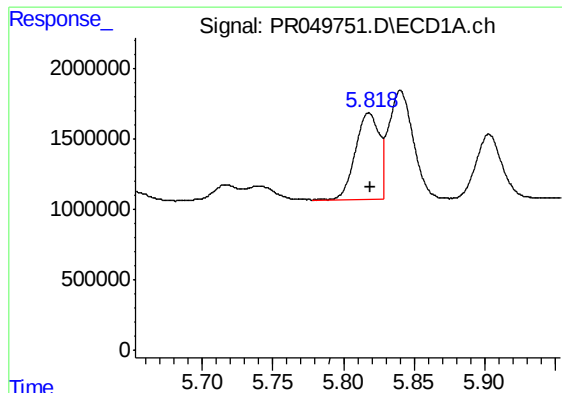

#21 AR-1248-1


R.T.: 5.818 min
Delta R.T.: -0.001 min
Response: 7249244
Conc: 84.61 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

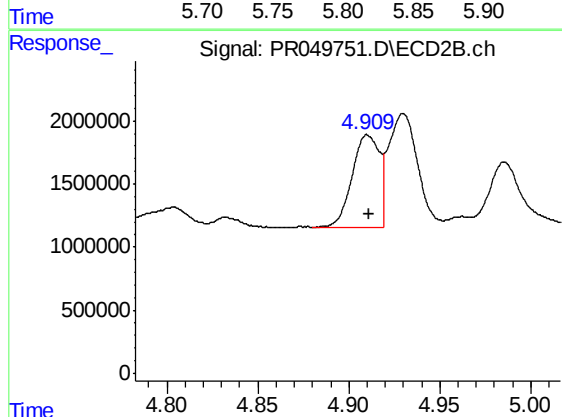


#21 AR-1248-1

R.T.: 4.910 min
Delta R.T.: -0.001 min
Response: 7541940
Conc: 55.89 ng/ml

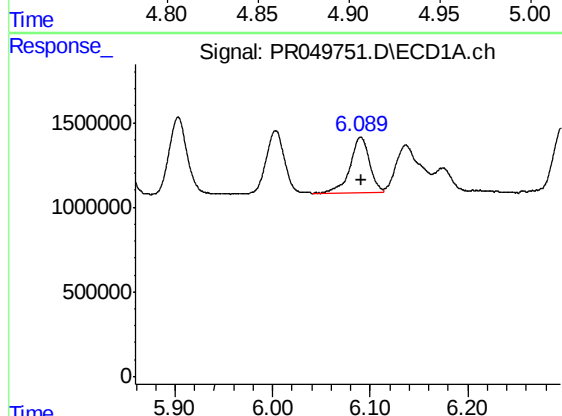


#22 AR-1248-2

R.T.: 6.090 min
Delta R.T.: -0.001 min
Response: 4498037
Conc: 37.42 ng/ml

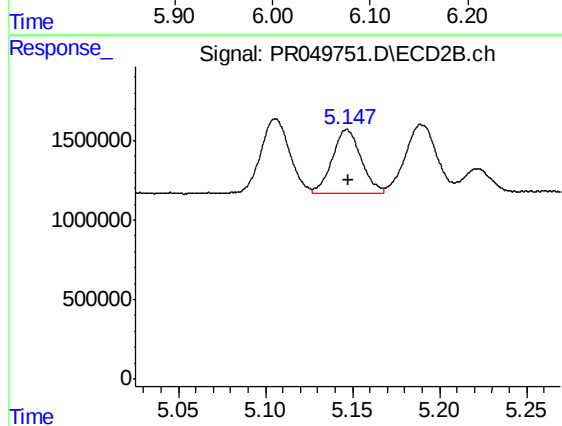

#22 AR-1248-2


R.T.: 5.147 min
Delta R.T.: -0.001 min
Response: 4571685
Conc: 25.80 ng/ml

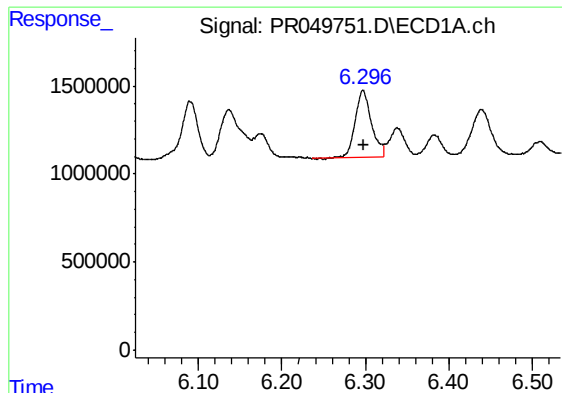

#23 AR-1248-3


R.T.: 6.297 min
Delta R.T.: -0.002 min
Response: 5210857
Conc: 38.48 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

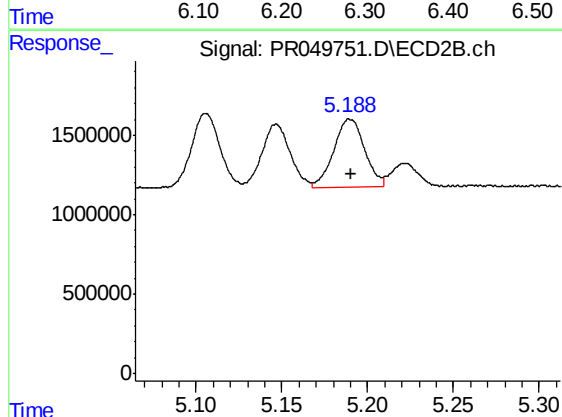


#23 AR-1248-3

R.T.: 5.189 min
Delta R.T.: -0.001 min
Response: 5346559
Conc: 28.37 ng/ml

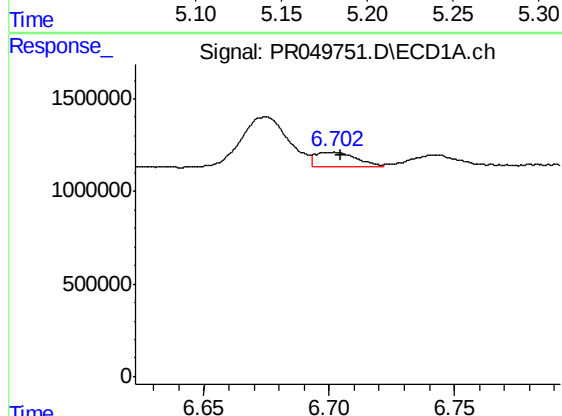


#24 AR-1248-4

R.T.: 6.702 min
Delta R.T.: -0.002 min
Response: 921514
Conc: 5.75 ng/ml

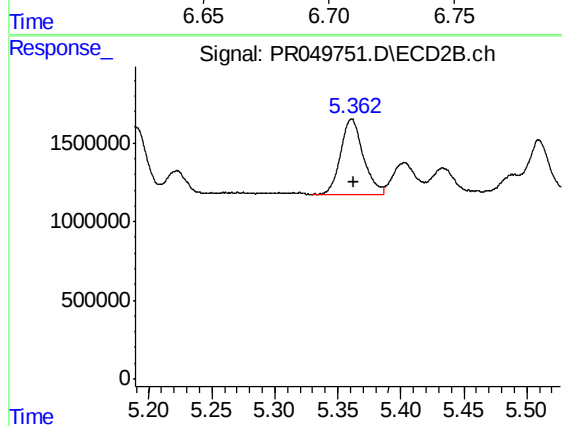

#24 AR-1248-4


R.T.: 5.361 min
Delta R.T.: -0.001 min
Response: 6046948
Conc: 25.99 ng/ml

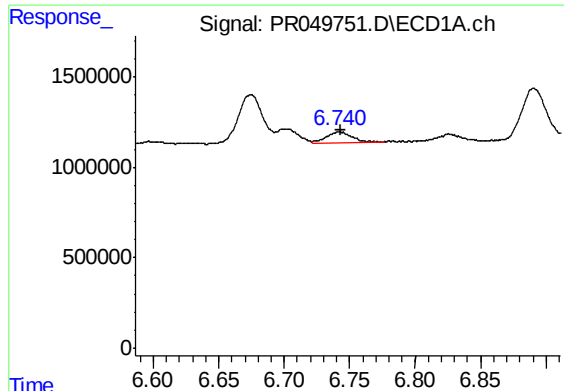

#25 AR-1248-5


R.T.: 6.742 min
Delta R.T.: -0.001 min
Response: 870800
Conc: 5.66 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

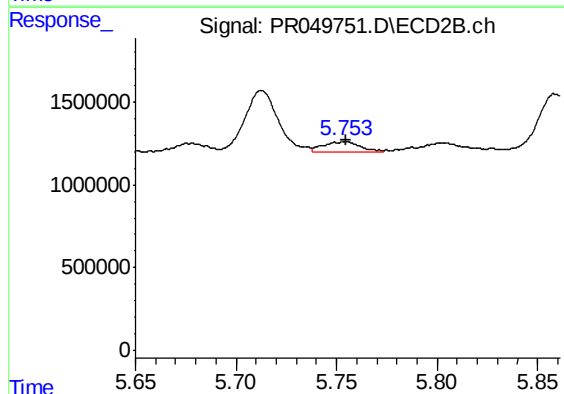


#25 AR-1248-5

R.T.: 5.754 min
Delta R.T.: 0.000 min
Response: 808305
Conc: 3.28 ng/ml

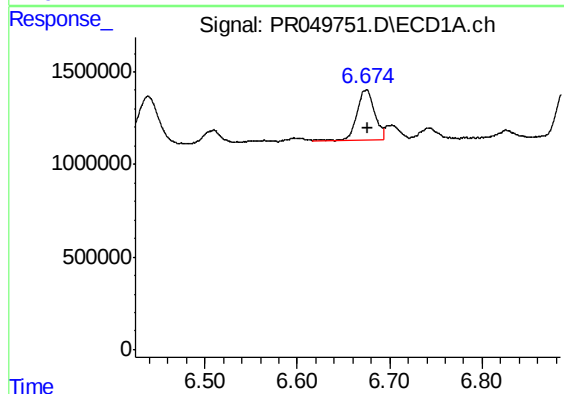


#26 AR-1254-1

R.T.: 6.674 min
Delta R.T.: -0.002 min
Response: 3762091
Conc: 23.65 ng/ml

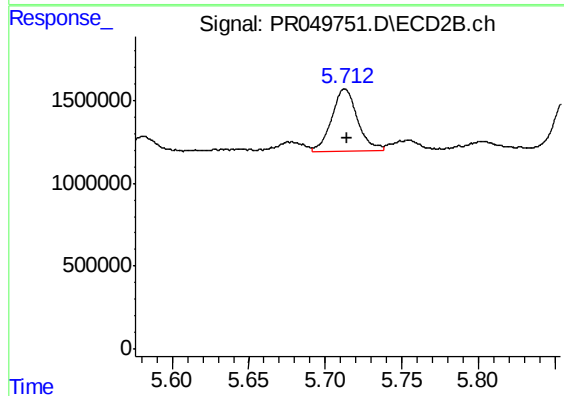

#26 AR-1254-1


R.T.: 5.713 min
Delta R.T.: -0.001 min
Response: 4406736
Conc: 11.72 ng/ml

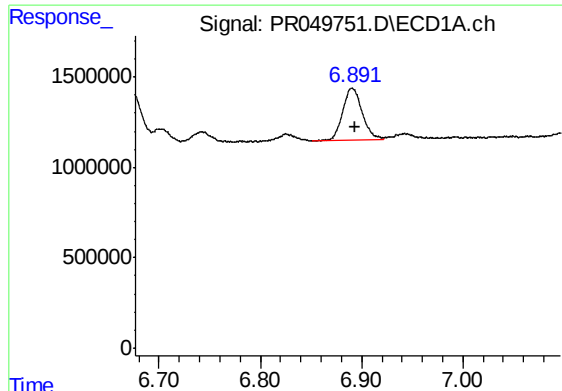

#27 AR-1254-2


R.T.: 6.891 min
Delta R.T.: -0.003 min
Response: 3849454
Conc: 15.28 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

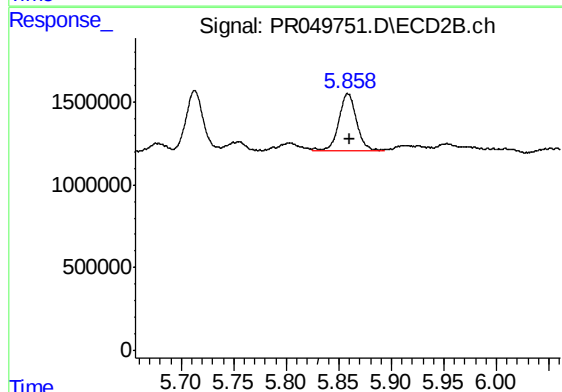


#27 AR-1254-2

R.T.: 5.859 min
Delta R.T.: -0.002 min
Response: 4097679
Conc: 12.71 ng/ml

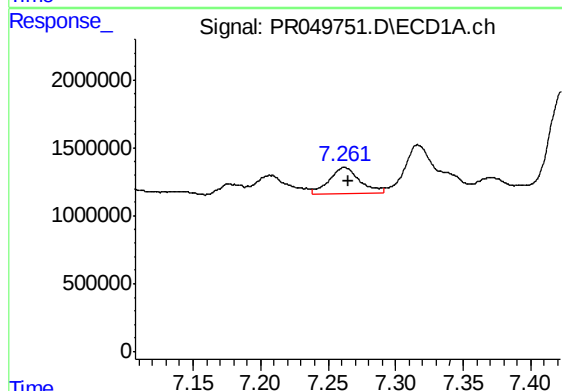


#28 AR-1254-3

R.T.: 7.262 min
Delta R.T.: -0.003 min
Response: 2967339
Conc: 10.74 ng/ml

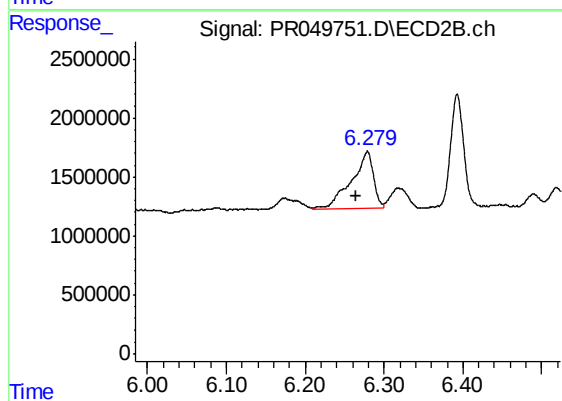

#28 AR-1254-3


R.T.: 6.279 min
Delta R.T.: 0.014 min
Response: 9574172
Conc: 16.80 ng/ml

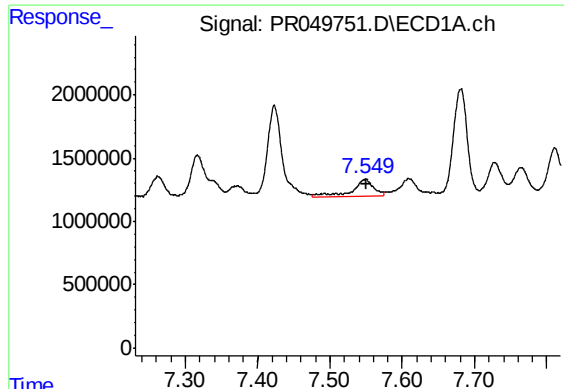

#29 AR-1254-4


R.T.: 7.549 min
Delta R.T.: -0.002 min
Response: 2823362
Conc: 13.42 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

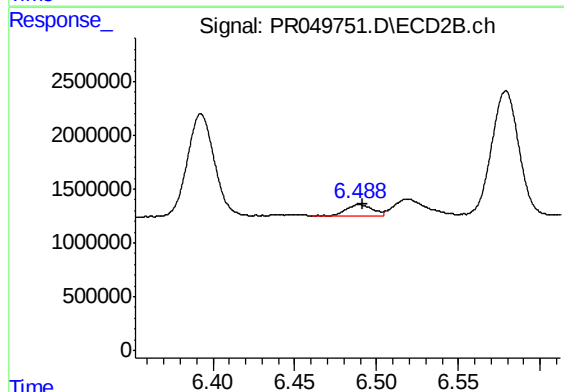


#29 AR-1254-4

R.T.: 6.489 min
Delta R.T.: -0.002 min
Response: 1265484
Conc: 3.54 ng/ml

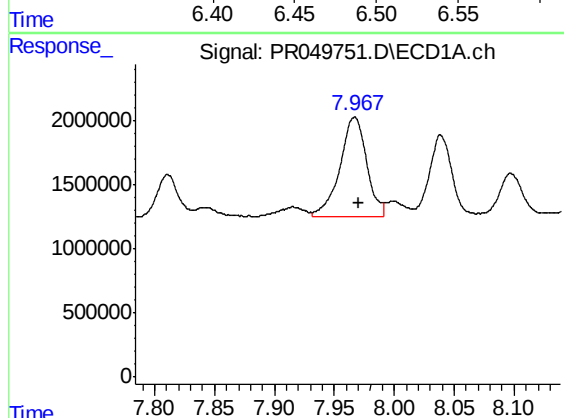


#30 AR-1254-5

R.T.: 7.967 min
Delta R.T.: -0.004 min
Response: 12116145
Conc: 53.43 ng/ml

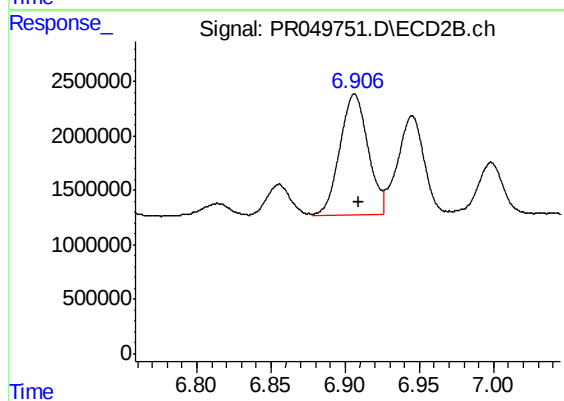

#30 AR-1254-5


R.T.: 6.906 min
Delta R.T.: -0.003 min
Response: 14723292
Conc: 29.55 ng/ml

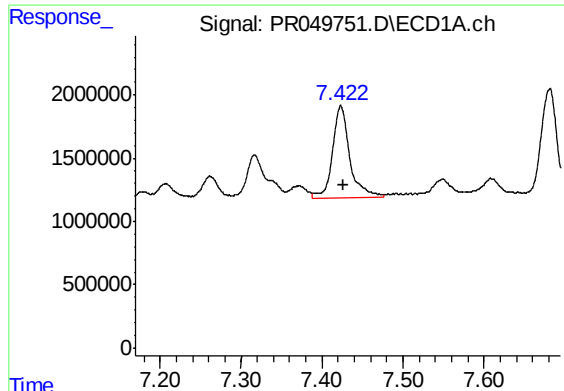

#31 AR-1260-1


R.T.: 7.423 min
Delta R.T.: -0.004 min
Response: 10872615
Conc: 54.67 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

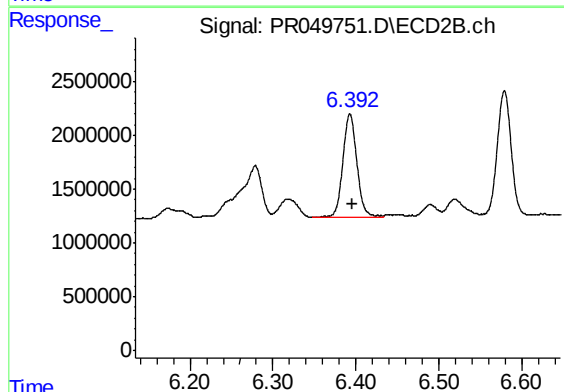


#31 AR-1260-1

R.T.: 6.393 min
Delta R.T.: -0.003 min
Response: 11238996
Conc: 31.34 ng/ml

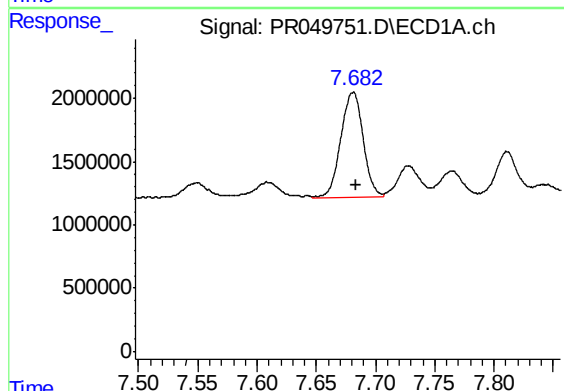


#32 AR-1260-2

R.T.: 7.681 min
Delta R.T.: -0.002 min
Response: 11047842
Conc: 45.25 ng/ml

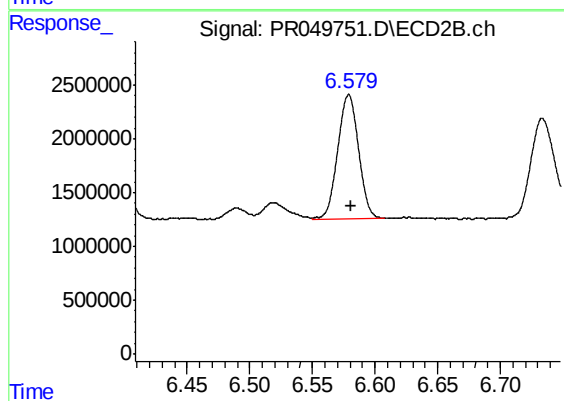

#32 AR-1260-2


R.T.: 6.579 min
Delta R.T.: -0.002 min
Response: 13378925
Conc: 30.14 ng/ml

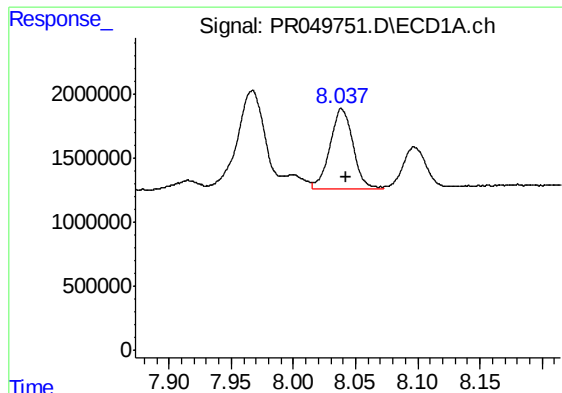

#33 AR-1260-3


R.T.: 8.039 min
Delta R.T.: -0.003 min
Response: 8088896
Conc: 43.26 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

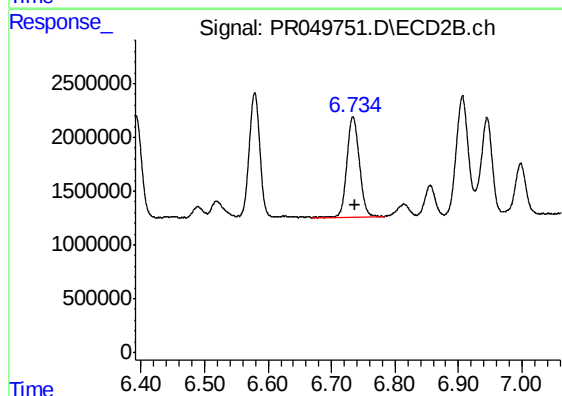


#33 AR-1260-3

R.T.: 6.734 min
Delta R.T.: -0.002 min
Response: 12557183
Conc: 29.85 ng/ml

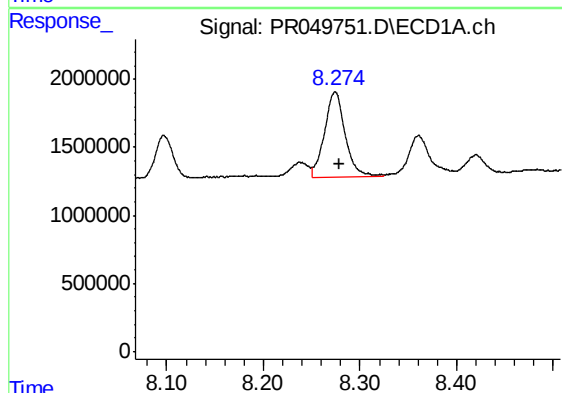


#34 AR-1260-4

R.T.: 8.274 min
Delta R.T.: -0.004 min
Response: 9138701
Conc: 41.83 ng/ml

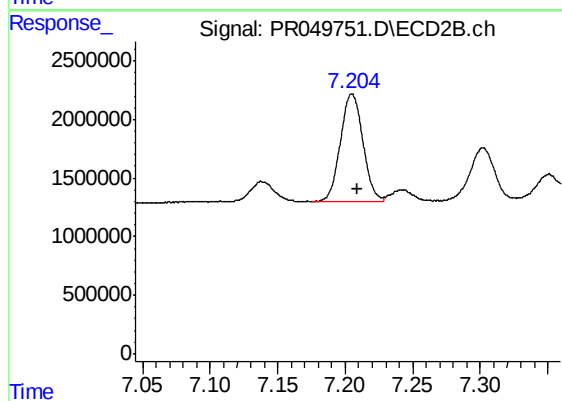

#34 AR-1260-4


R.T.: 7.205 min
Delta R.T.: -0.004 min
Response: 10766705
Conc: 30.21 ng/ml

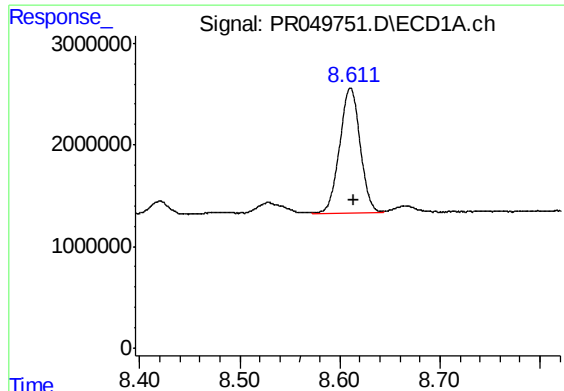

#35 AR-1260-5


R.T.: 8.611 min
Delta R.T.: -0.003 min
Response: 17666210
Conc: 39.16 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

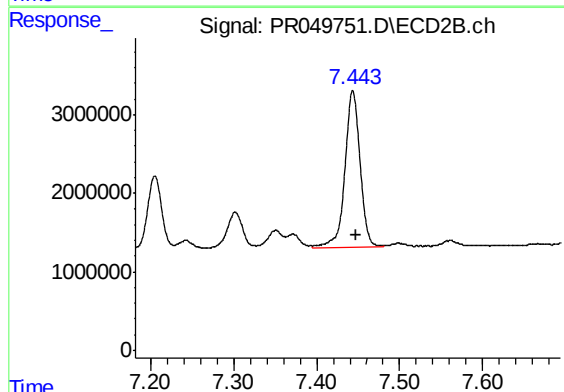


#35 AR-1260-5

R.T.: 7.444 min
Delta R.T.: -0.005 min
Response: 25254819
Conc: 27.56 ng/ml

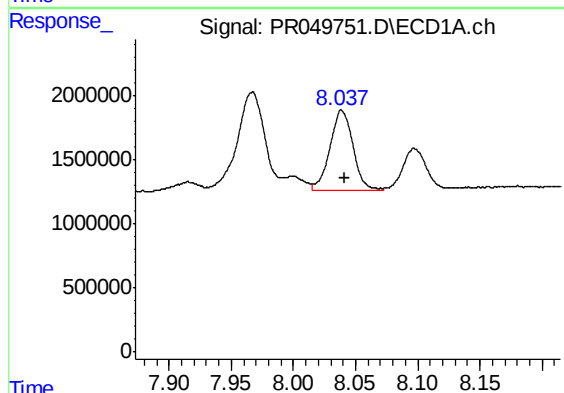


#36 AR-1262-1

R.T.: 8.039 min
Delta R.T.: -0.002 min
Response: 8088896
Conc: 30.89 ng/ml

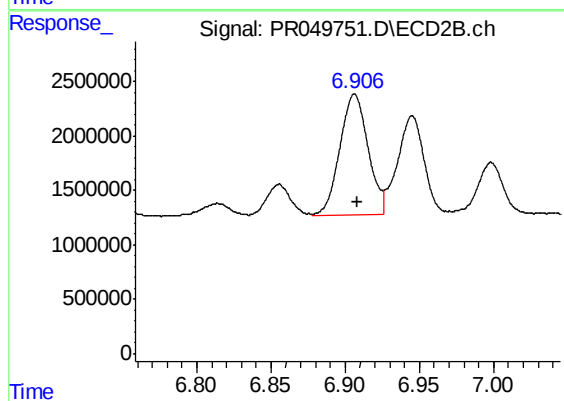

#36 AR-1262-1


R.T.: 6.906 min
Delta R.T.: -0.002 min
Response: 14723292
Conc: 57.37 ng/ml

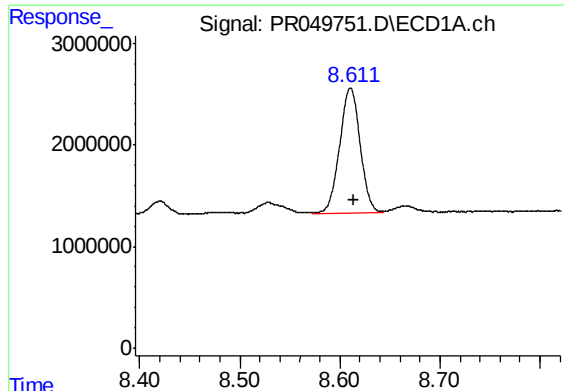

#37 AR-1262-2


R.T.: 8.611 min
Delta R.T.: -0.003 min
Response: 17666210
Conc: 35.50 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

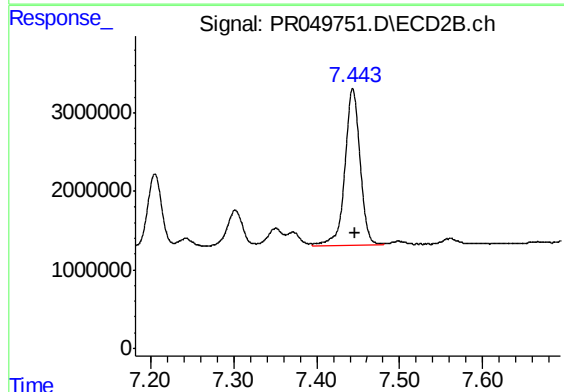


#37 AR-1262-2

R.T.: 7.444 min
Delta R.T.: -0.003 min
Response: 25254819
Conc: 25.65 ng/ml

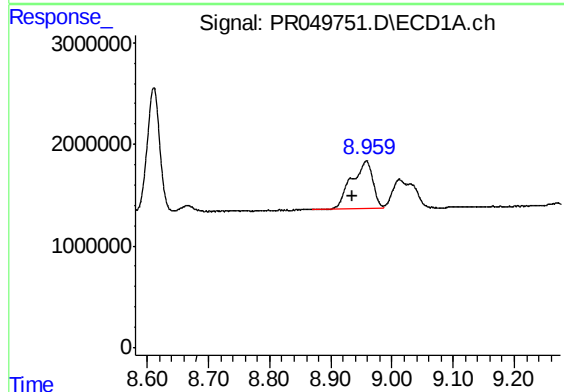


#38 AR-1262-3

R.T.: 8.958 min
Delta R.T.: 0.022 min
Response: 11527391
Conc: 35.05 ng/ml

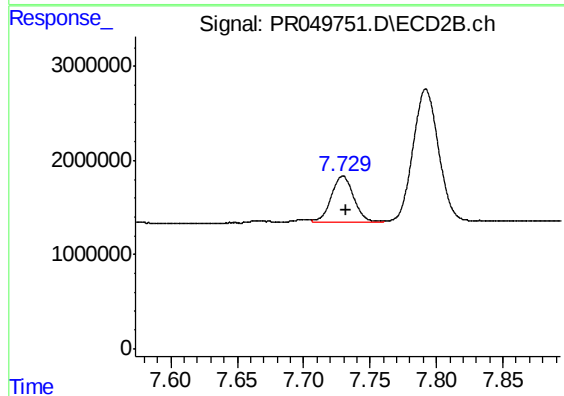

#38 AR-1262-3


R.T.: 7.729 min
Delta R.T.: -0.003 min
Response: 5879119
Conc: 16.33 ng/ml

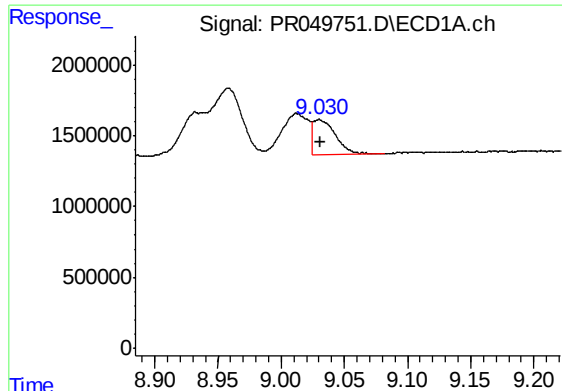

#39 AR-1262-4


R.T.: 9.030 min
Delta R.T.: -0.001 min
Response: 2991482
Conc: 12.11 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

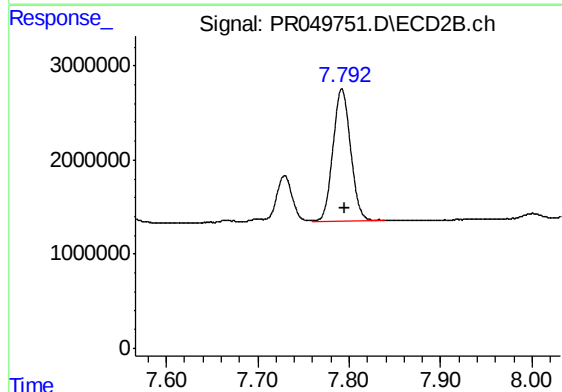


#39 AR-1262-4

R.T.: 7.792 min
Delta R.T.: -0.003 min
Response: 18919869
Conc: 26.43 ng/ml

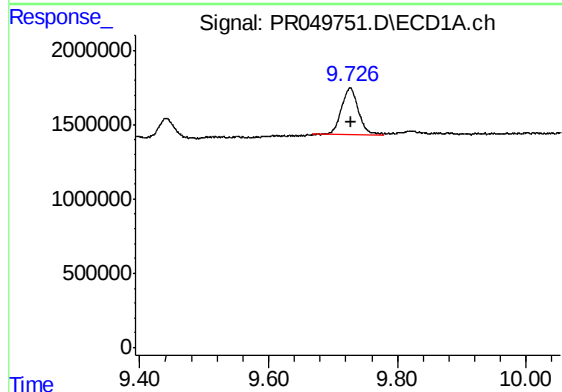


#40 AR-1262-5

R.T.: 9.727 min
Delta R.T.: -0.001 min
Response: 5748622
Conc: 31.90 ng/ml

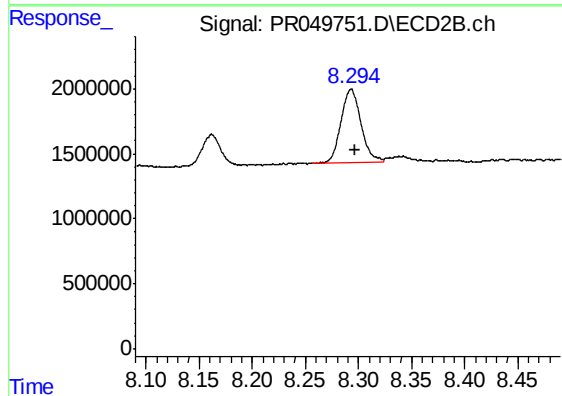

#40 AR-1262-5


R.T.: 8.293 min
Delta R.T.: -0.003 min
Response: 7460500
Conc: 23.21 ng/ml

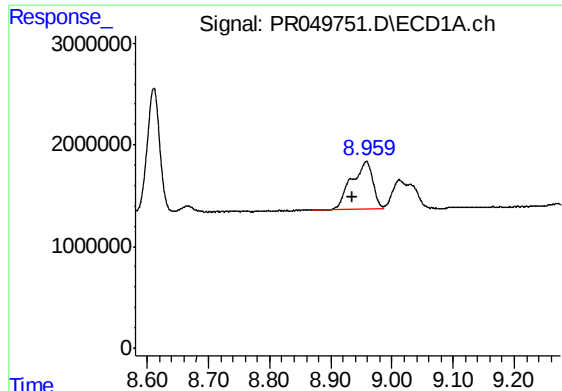

#41 AR-1268-1


R.T.: 8.958 min
Delta R.T.: 0.023 min
Response: 11527391
Conc: 19.65 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

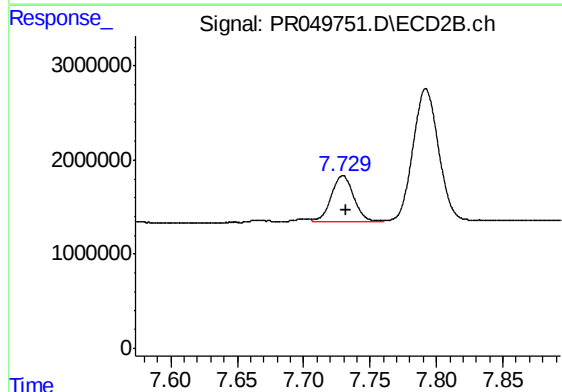


#41 AR-1268-1

R.T.: 7.729 min
Delta R.T.: -0.003 min
Response: 5879119
Conc: 5.24 ng/ml

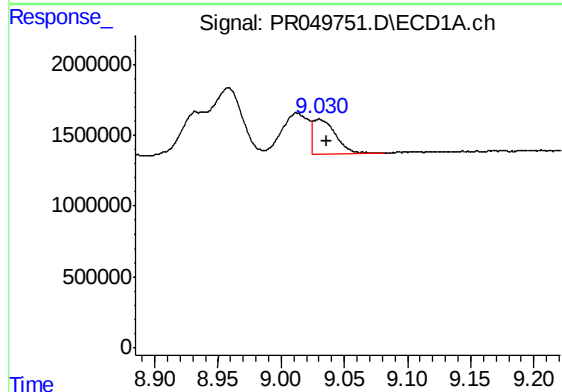


#42 AR-1268-2

R.T.: 9.030 min
Delta R.T.: -0.007 min
Response: 2991482
Conc: 5.56 ng/ml

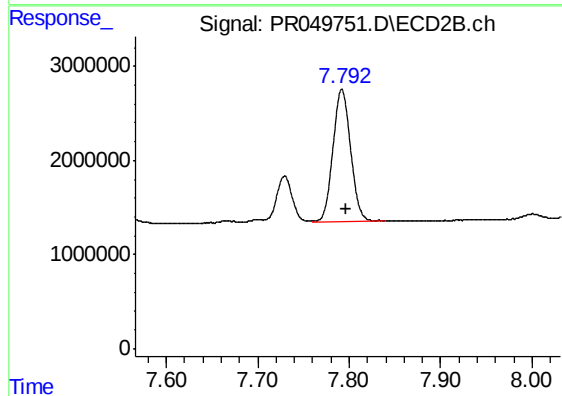

#42 AR-1268-2


R.T.: 7.792 min
Delta R.T.: -0.004 min
Response: 18919869
Conc: 17.88 ng/ml

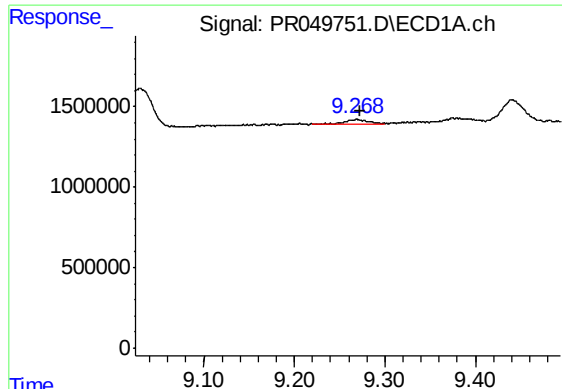

#43 AR-1268-3


R.T.: 9.269 min
Delta R.T.: -0.004 min
Response: 392216
Conc: 0.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

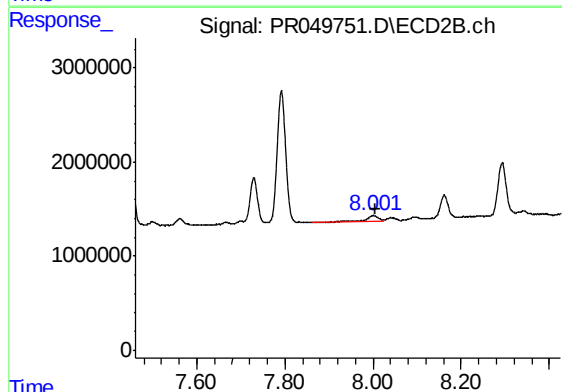


#43 AR-1268-3

R.T.: 8.001 min
Delta R.T.: -0.006 min
Response: 1284154
Conc: 1.47 ng/ml

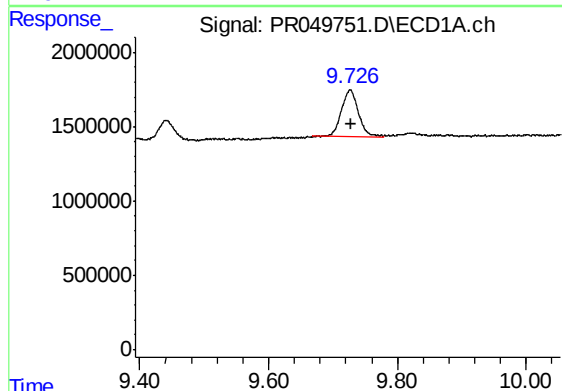


#44 AR-1268-4

R.T.: 9.727 min
Delta R.T.: -0.002 min
Response: 5748622
Conc: 28.46 ng/ml

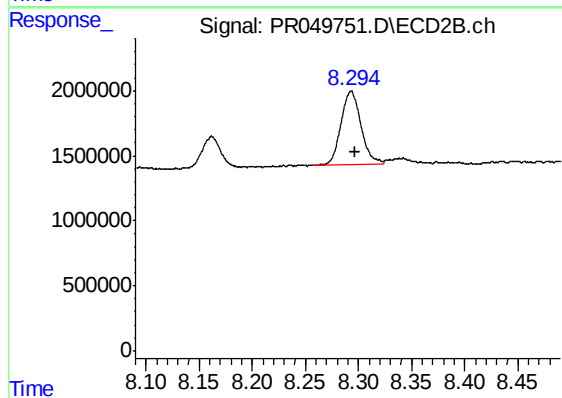

#44 AR-1268-4


R.T.: 8.293 min
Delta R.T.: -0.004 min
Response: 7460500
Conc: 20.49 ng/ml

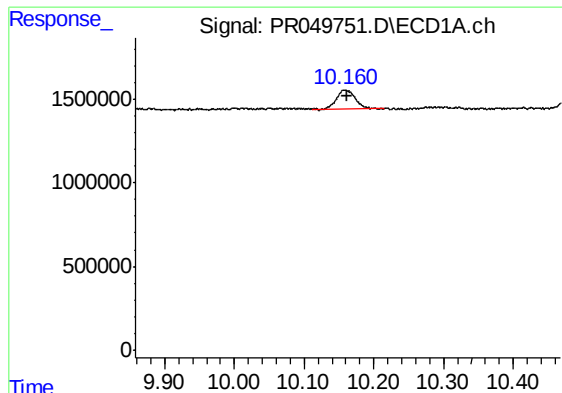

#45 AR-1268-5

R.T.: 10.158 min
Delta R.T.: -0.004 min
Response: 2130588
Conc: 1.30 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

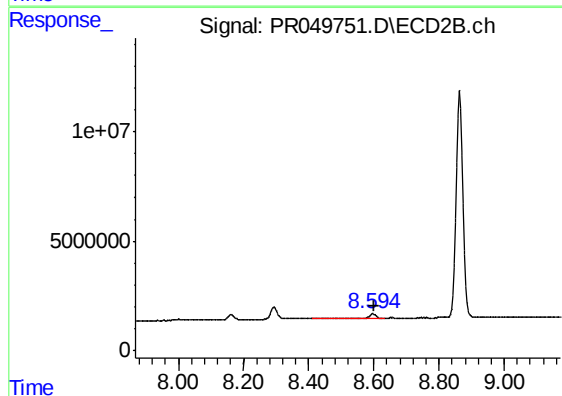

#45 AR-1268-5

R.T.: 8.596 min
Delta R.T.: -0.005 min
Response: 3731754
Conc: 1.23 ng/ml