

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040221\
 Data File : PR049753.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2021 02:34
 Operator : DD\AJ
 Sample : M1458-07
 Misc : AR1232 LOD 40 PPB
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 01:54:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Apr 03 08:12:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.636	3.820	57169495	88638173	14.642	13.366
2)	SA Decachlor...	10.512	8.862	70210265	85937172	15.802	11.288 #
Target Compounds							
3)	L1 AR-1016-1	5.817	4.910	4746647	5031142	30.877	20.953 #
4)	L1 AR-1016-2	5.841	4.929	6494467	7304318	30.398	21.173 #
5)	L1 AR-1016-3	5.903	5.106	4219023	3783368	32.859	20.780 #
6)	L1 AR-1016-4	6.004	5.146	3480804	2695983	32.712	19.392 #
7)	L1 AR-1016-5	6.297	5.361	3328987	3829328	31.071	20.381 #
8)	L2 AR-1221-1	4.857	4.034	3395381	2316740	82.141	36.353 #
9)	L2 AR-1221-2	4.939	4.120	2383836	3291062	76.405	66.964
10)	L2 AR-1221-3	5.015	4.197	5598678	7635701	58.988	48.516
11)	L3 AR-1232-1	5.015	4.197	5598678	7635701	72.455	60.566
12)	L3 AR-1232-2	5.549	4.929	3190413	7304318	75.277	54.990 #
13)	L3 AR-1232-3	5.841	5.106	6494467	3783368	76.230	54.415 #
14)	L3 AR-1232-4	6.004	5.189	3480804	3292269	81.672	56.003 #
15)	L3 AR-1232-5	6.090	5.361	2780178	3829328	84.069	58.005 #
16)	L4 AR-1242-1	5.817	4.910	4746647	5031142	42.335	28.668 #
17)	L4 AR-1242-2	5.841	4.929	6494467	7304318	41.115	29.094 #
18)	L4 AR-1242-3	5.903	5.106	4219023	3783368	44.056	28.359 #
19)	L4 AR-1242-4	6.004	5.189	3480804	3292269	43.441	26.564 #
20)	L4 AR-1242-5	6.741	5.711	3365850	3992275	36.944	23.395 #
21)	L5 AR-1248-1	5.817	4.910	4746647	5031142	55.398	37.282 #
22)	L5 AR-1248-2	6.090	5.146	2780178	2695983	23.127	15.212 #
23)	L5 AR-1248-3	6.297	5.189	3328987	3292269	24.580	17.471 #
24)	L5 AR-1248-4	6.702	5.361	3237840	3829328	20.206	16.460
25)	L5 AR-1248-5	6.741	5.753	3365850	3491179	21.883	14.174 #
26)	L6 AR-1254-1	6.674	5.711	2509088	3992275	15.772	10.620 #
27)	L6 AR-1254-2	6.901	5.859	2804205	875781	11.133	2.716 #
28)	L6 AR-1254-3	7.263	6.263	1543159	1270202	5.586	2.228 #
29)	L6 AR-1254-4	7.548	6.489	695411	886192	3.305	2.479
30)	L6 AR-1254-5	7.971	6.904	270861	354329	1.194	0.711 #
31)	L7 AR-1260-1	7.437	6.410	397637	620245	2.000	1.729
32)	L7 AR-1260-2	7.689	6.575	5444564	492610	22.302	1.110 #
33)	L7 AR-1260-3	0.000	6.712f	0	9886435	N.D.	23.503 #
35)	L7 AR-1260-5	8.615	7.441	314804	761680	0.698	0.831
36)	L8 AR-1262-1	0.000	6.904	0	354329	N.D.	1.381 #
37)	L8 AR-1262-2	8.615	7.441	314804	761680	0.633	0.773
38)	L8 AR-1262-3	0.000	7.703f	0	1575345	N.D.	4.375 #
39)	L8 AR-1262-4	0.000	7.786	0	575702	N.D.	0.804 #
41)	L9 AR-1268-1	0.000	7.703f	0	1575345	N.D.	1.404 #
42)	L9 AR-1268-2	0.000	7.786	0	575702	N.D.	0.544 #
43)	L9 AR-1268-3	0.000	8.003	0	338440	N.D.	0.386 #
45)	L9 AR-1268-5	10.162	8.594	318258	2323769	0.194	0.763 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040221\
Data File : PR049753.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2021 02:34
Operator : DD\AJ
Sample : M1458-07
Misc : AR1232 LOD 40 PPB
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 01:54:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040221.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Apr 03 08:12:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040221\
Data File : PR049753.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2021 02:34
Operator : DD\AJ
Sample : M1458-07
Misc : AR1232 LOD 40 PPB
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 01:54:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040221.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Apr 03 08:12:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

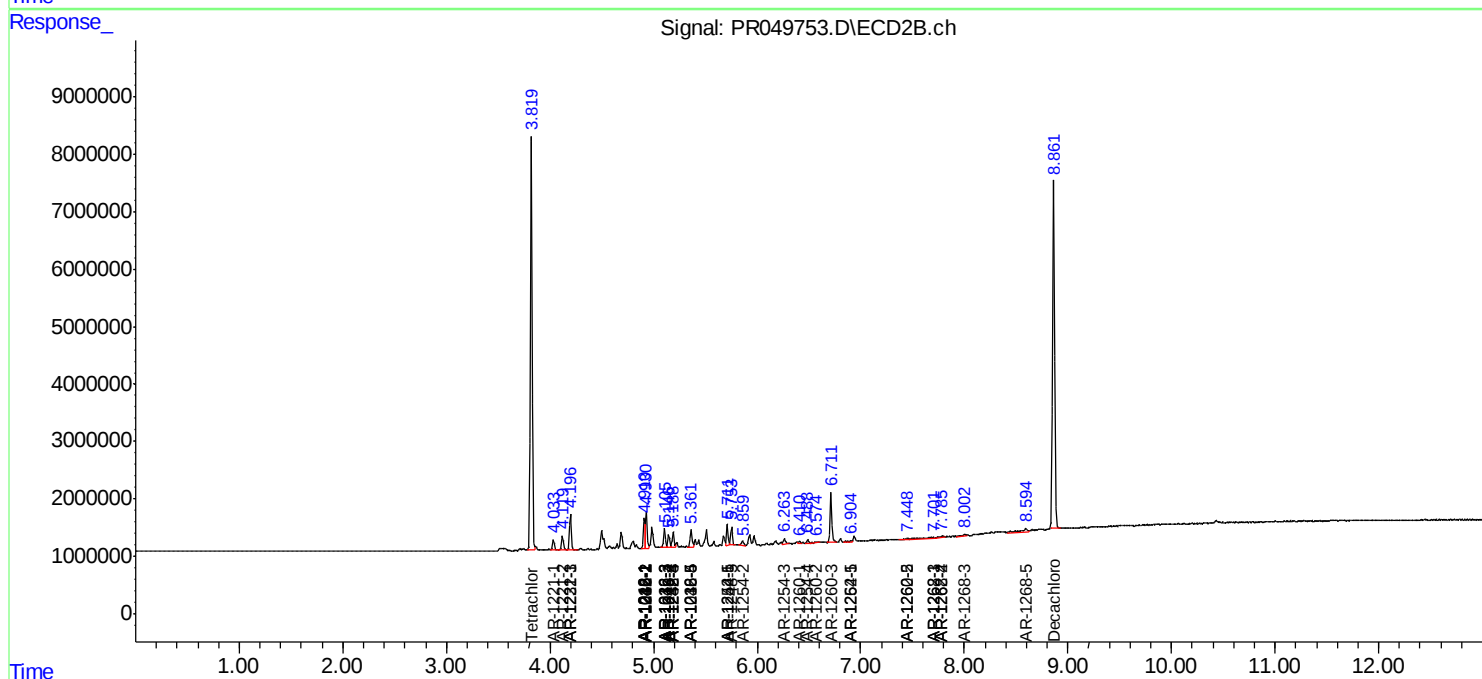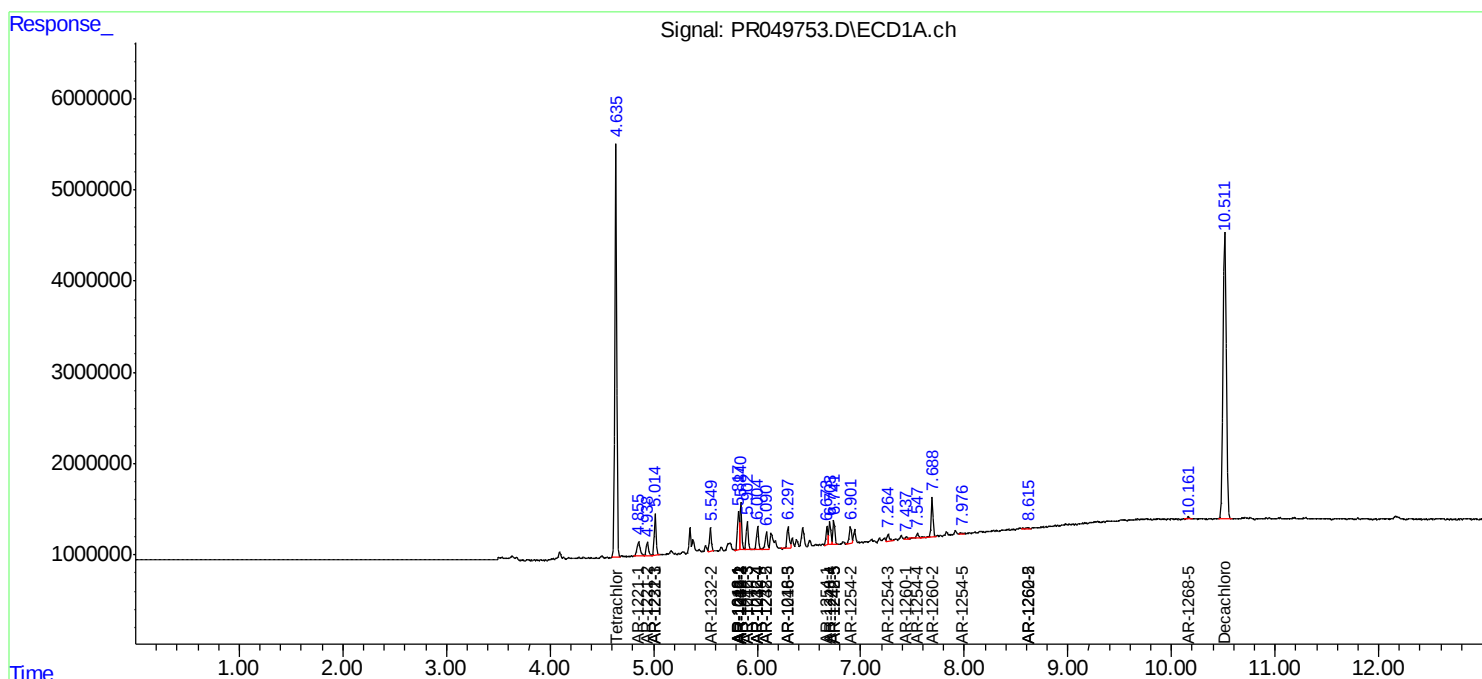




#1 Tetrachloro-m-xylene


R.T.: 4.636 min
Delta R.T.: -0.003 min
Response: 57169495
Conc: 14.64 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




#1 Tetrachloro-m-xylene

R.T.: 3.820 min
Delta R.T.: -0.003 min
Response: 88638173
Conc: 13.37 ng/ml




#2 Decachlorobiphenyl

R.T.: 10.512 min
Delta R.T.: -0.005 min
Response: 70210265
Conc: 15.80 ng/ml

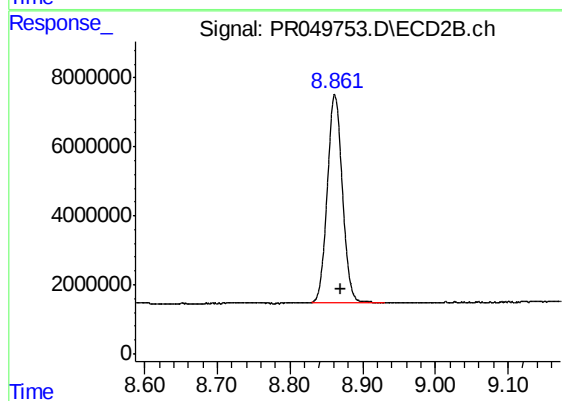

#2 Decachlorobiphenyl


R.T.: 8.862 min
Delta R.T.: -0.007 min
Response: 85937172
Conc: 11.29 ng/ml



#3 AR-1016-1


R.T.: 5.817 min
Delta R.T.: -0.003 min
Response: 4746647
Conc: 30.88 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

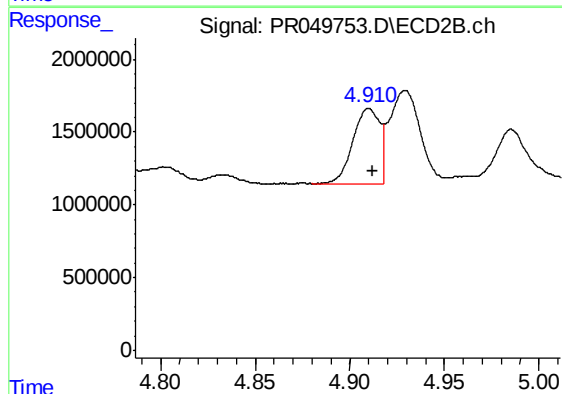


#3 AR-1016-1

R.T.: 4.910 min
Delta R.T.: -0.002 min
Response: 5031142
Conc: 20.95 ng/ml




#4 AR-1016-2

R.T.: 5.841 min
Delta R.T.: -0.003 min
Response: 6494467
Conc: 30.40 ng/ml

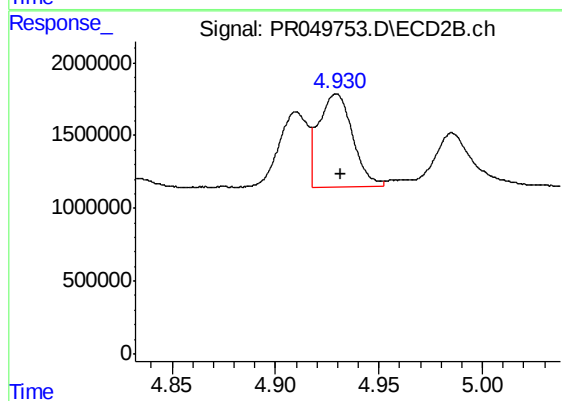

#4 AR-1016-2


R.T.: 4.929 min
Delta R.T.: -0.002 min
Response: 7304318
Conc: 21.17 ng/ml

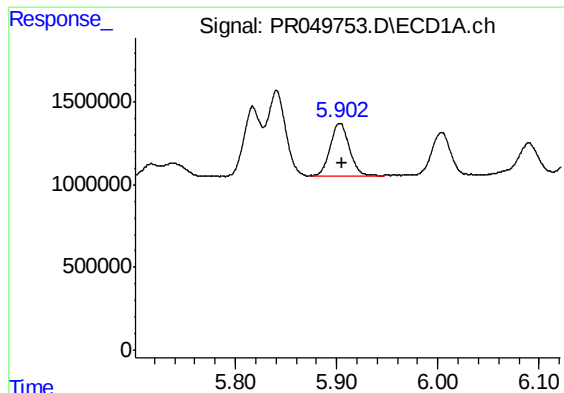

#5 AR-1016-3


R.T.: 5.903 min
Delta R.T.: -0.003 min
Response: 4219023
Conc: 32.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

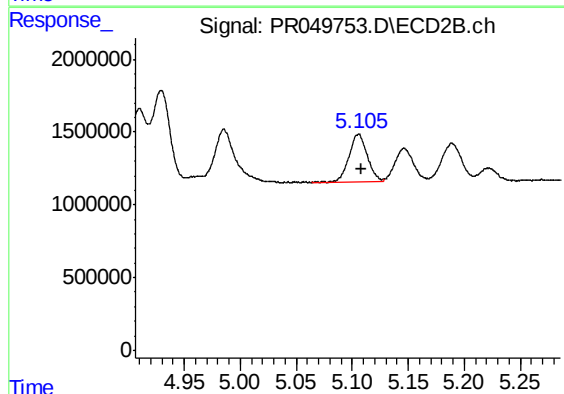


#5 AR-1016-3

R.T.: 5.106 min
Delta R.T.: -0.002 min
Response: 3783368
Conc: 20.78 ng/ml

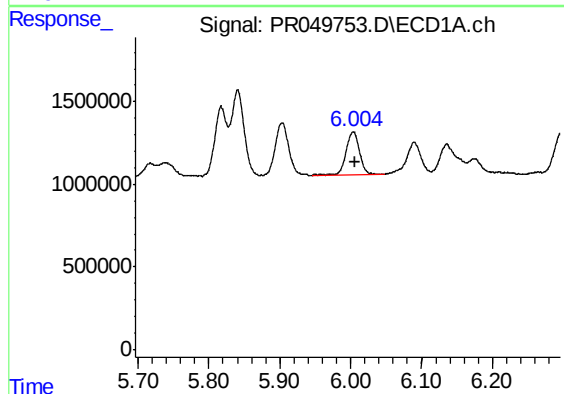


#6 AR-1016-4

R.T.: 6.004 min
Delta R.T.: -0.002 min
Response: 3480804
Conc: 32.71 ng/ml

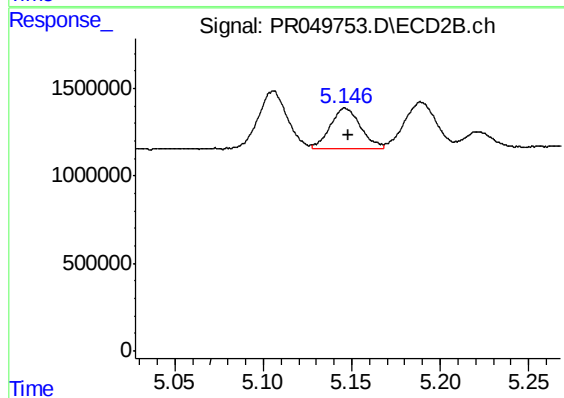

#6 AR-1016-4


R.T.: 5.146 min
Delta R.T.: -0.002 min
Response: 2695983
Conc: 19.39 ng/ml



#7 AR-1016-5


R.T.: 6.297 min
Delta R.T.: -0.002 min
Response: 3328987
Conc: 31.07 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




#7 AR-1016-5

R.T.: 5.361 min
Delta R.T.: -0.002 min
Response: 3829328
Conc: 20.38 ng/ml

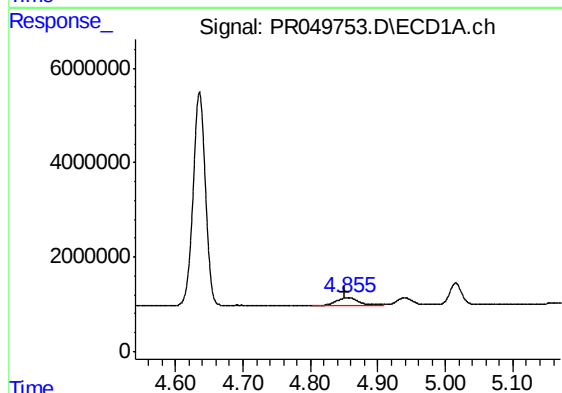


#8 AR-1221-1

R.T.: 4.857 min
Delta R.T.: 0.006 min
Response: 3395381
Conc: 82.14 ng/ml

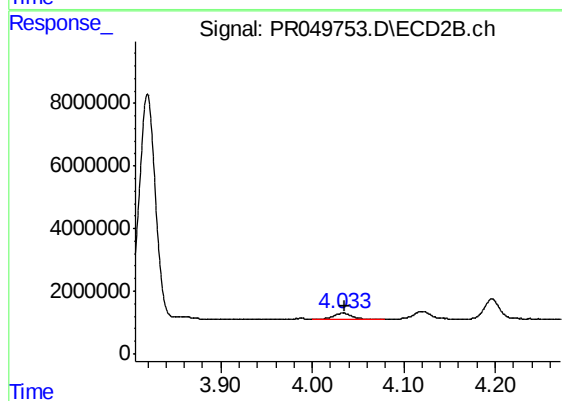

#8 AR-1221-1


R.T.: 4.034 min
Delta R.T.: -0.002 min
Response: 2316740
Conc: 36.35 ng/ml

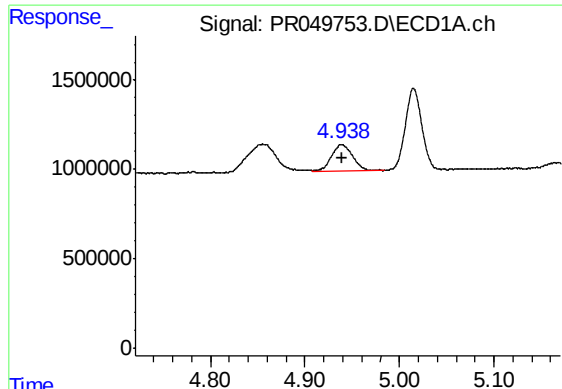

#9 AR-1221-2


R.T.: 4.939 min
Delta R.T.: 0.000 min
Response: 2383836
Conc: 76.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




#9 AR-1221-2

R.T.: 4.120 min
Delta R.T.: -0.002 min
Response: 3291062
Conc: 66.96 ng/ml




#10 AR-1221-3

R.T.: 5.015 min
Delta R.T.: -0.002 min
Response: 5598678
Conc: 58.99 ng/ml

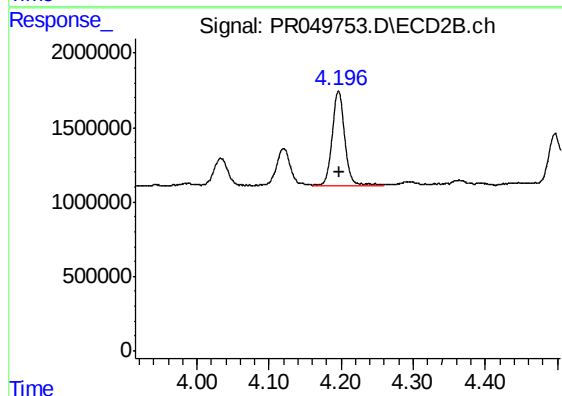

#10 AR-1221-3


R.T.: 4.197 min
Delta R.T.: -0.002 min
Response: 7635701
Conc: 48.52 ng/ml

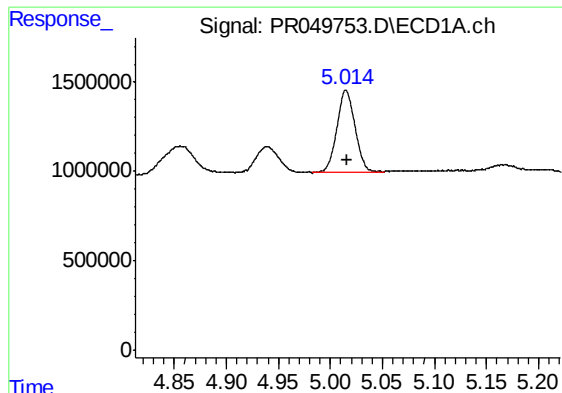

#11 AR-1232-1


R.T.: 5.015 min
Delta R.T.: -0.002 min
Response: 5598678
Conc: 72.45 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




#11 AR-1232-1

R.T.: 4.197 min
Delta R.T.: -0.001 min
Response: 7635701
Conc: 60.57 ng/ml

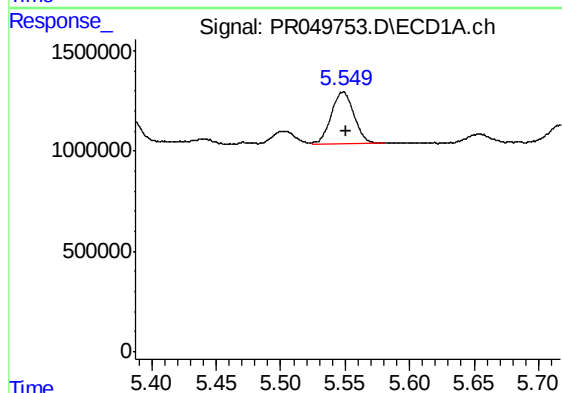


#12 AR-1232-2

R.T.: 5.549 min
Delta R.T.: -0.002 min
Response: 3190413
Conc: 75.28 ng/ml

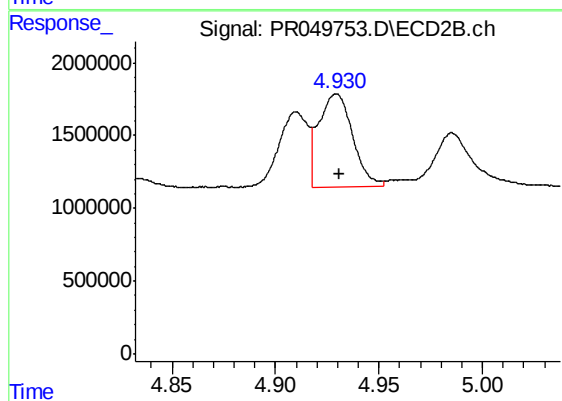

#12 AR-1232-2


R.T.: 4.929 min
Delta R.T.: -0.002 min
Response: 7304318
Conc: 54.99 ng/ml

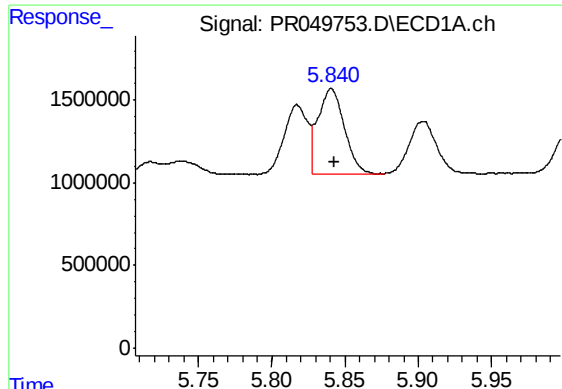

#13 AR-1232-3


R.T.: 5.841 min
Delta R.T.: -0.002 min
Response: 6494467
Conc: 76.23 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

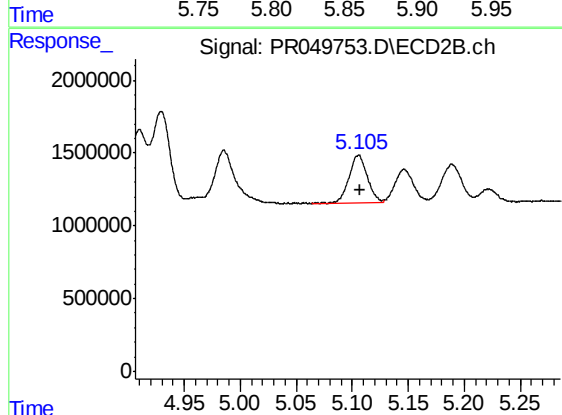


#13 AR-1232-3

R.T.: 5.106 min
Delta R.T.: -0.001 min
Response: 3783368
Conc: 54.41 ng/ml

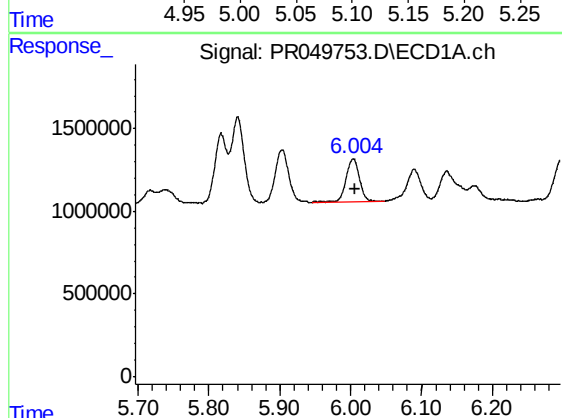


#14 AR-1232-4

R.T.: 6.004 min
Delta R.T.: -0.002 min
Response: 3480804
Conc: 81.67 ng/ml

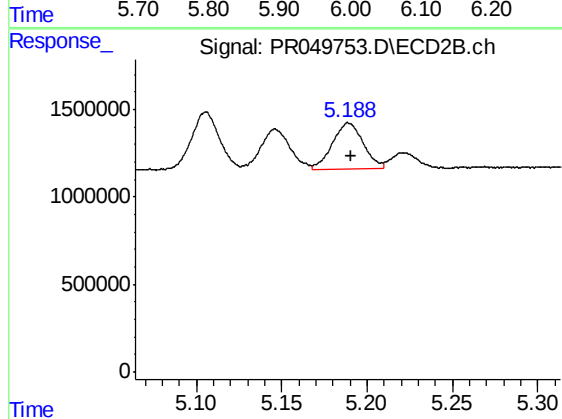

#14 AR-1232-4


R.T.: 5.189 min
Delta R.T.: -0.001 min
Response: 3292269
Conc: 56.00 ng/ml



#15 AR-1232-5


R.T.: 6.090 min
Delta R.T.: -0.002 min
Response: 2780178
Conc: 84.07 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




#15 AR-1232-5

R.T.: 5.361 min
Delta R.T.: -0.002 min
Response: 3829328
Conc: 58.00 ng/ml




#16 AR-1242-1

R.T.: 5.817 min
Delta R.T.: -0.002 min
Response: 4746647
Conc: 42.34 ng/ml

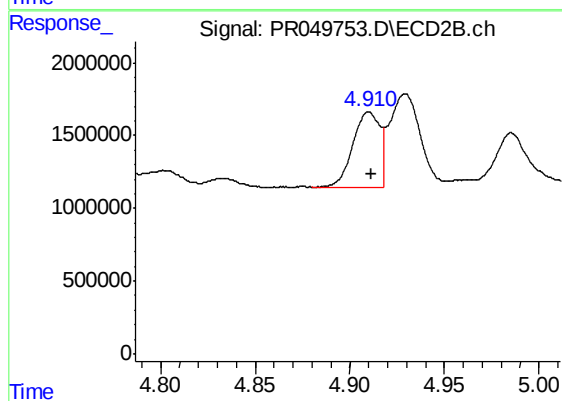

#16 AR-1242-1


R.T.: 4.910 min
Delta R.T.: -0.002 min
Response: 5031142
Conc: 28.67 ng/ml

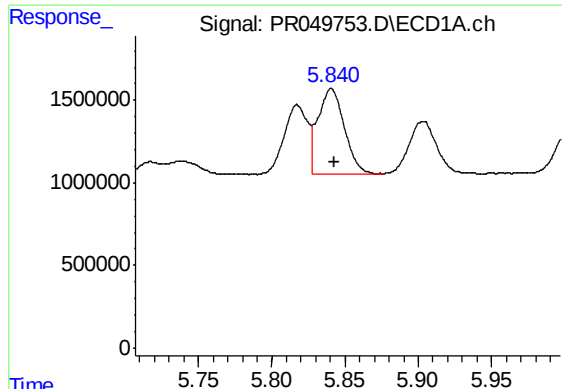

#17 AR-1242-2


R.T.: 5.841 min
Delta R.T.: -0.002 min
Response: 6494467
Conc: 41.11 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

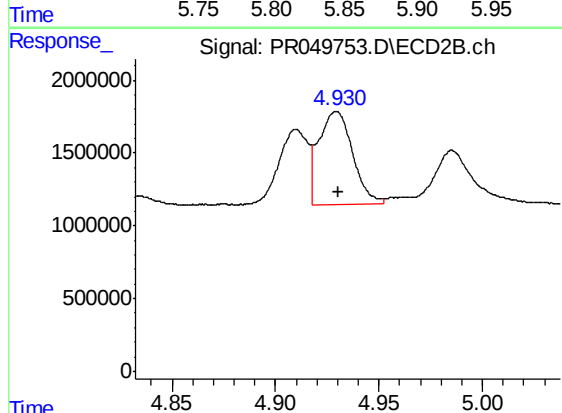


#17 AR-1242-2

R.T.: 4.929 min
Delta R.T.: -0.001 min
Response: 7304318
Conc: 29.09 ng/ml

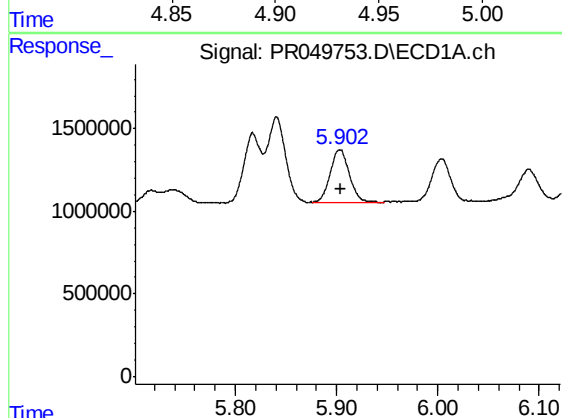


#18 AR-1242-3

R.T.: 5.903 min
Delta R.T.: 0.000 min
Response: 4219023
Conc: 44.06 ng/ml

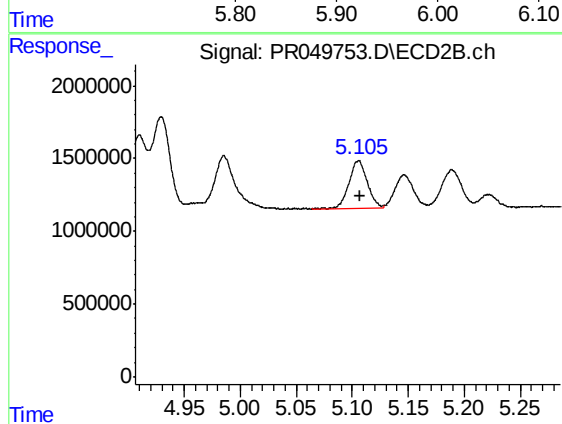

#18 AR-1242-3


R.T.: 5.106 min
Delta R.T.: -0.002 min
Response: 3783368
Conc: 28.36 ng/ml



#19 AR-1242-4


R.T.: 6.004 min
Delta R.T.: -0.001 min
Response: 3480804
Conc: 43.44 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




#19 AR-1242-4

R.T.: 5.189 min
Delta R.T.: -0.002 min
Response: 3292269
Conc: 26.56 ng/ml




#20 AR-1242-5

R.T.: 6.741 min
Delta R.T.: -0.002 min
Response: 3365850
Conc: 36.94 ng/ml

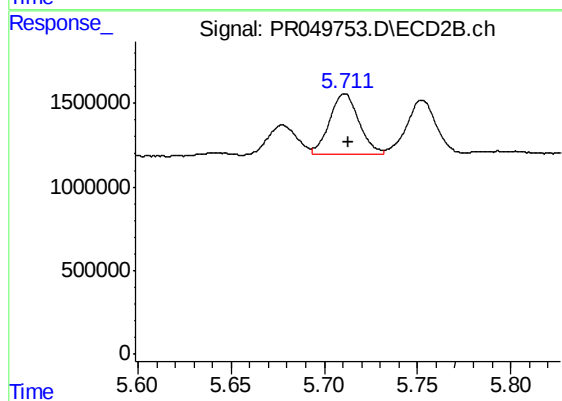

#20 AR-1242-5


R.T.: 5.711 min
Delta R.T.: -0.002 min
Response: 3992275
Conc: 23.40 ng/ml



#21 AR-1248-1


R.T.: 5.817 min
Delta R.T.: -0.002 min
Response: 4746647
Conc: 55.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

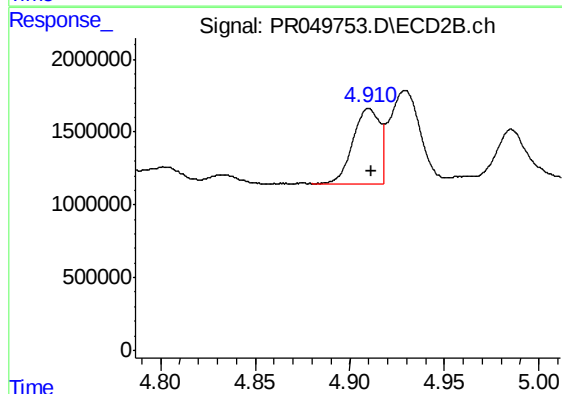


#21 AR-1248-1

R.T.: 4.910 min
Delta R.T.: -0.001 min
Response: 5031142
Conc: 37.28 ng/ml




#22 AR-1248-2

R.T.: 6.090 min
Delta R.T.: -0.002 min
Response: 2780178
Conc: 23.13 ng/ml

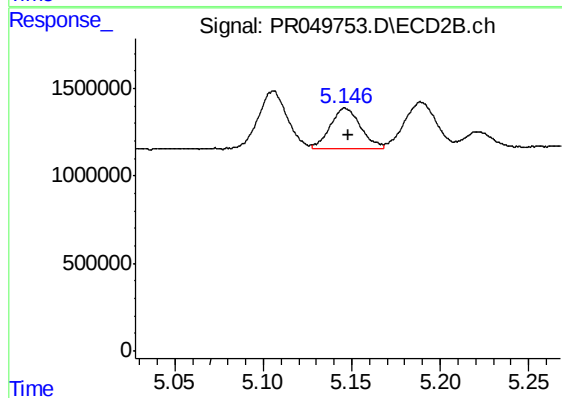

#22 AR-1248-2


R.T.: 5.146 min
Delta R.T.: -0.002 min
Response: 2695983
Conc: 15.21 ng/ml



#23 AR-1248-3


R.T.: 6.297 min
Delta R.T.: -0.002 min
Response: 3328987
Conc: 24.58 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




#23 AR-1248-3

R.T.: 5.189 min
Delta R.T.: -0.001 min
Response: 3292269
Conc: 17.47 ng/ml




#24 AR-1248-4

R.T.: 6.702 min
Delta R.T.: -0.002 min
Response: 3237840
Conc: 20.21 ng/ml

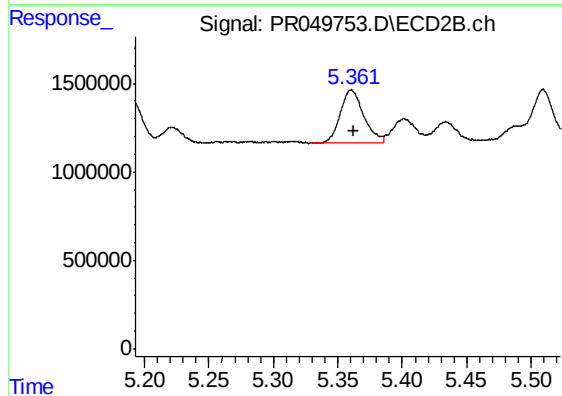

#24 AR-1248-4


R.T.: 5.361 min
Delta R.T.: -0.002 min
Response: 3829328
Conc: 16.46 ng/ml



#25 AR-1248-5


R.T.: 6.741 min
Delta R.T.: -0.002 min
Response: 3365850
Conc: 21.88 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




#25 AR-1248-5

R.T.: 5.753 min
Delta R.T.: -0.002 min
Response: 3491179
Conc: 14.17 ng/ml

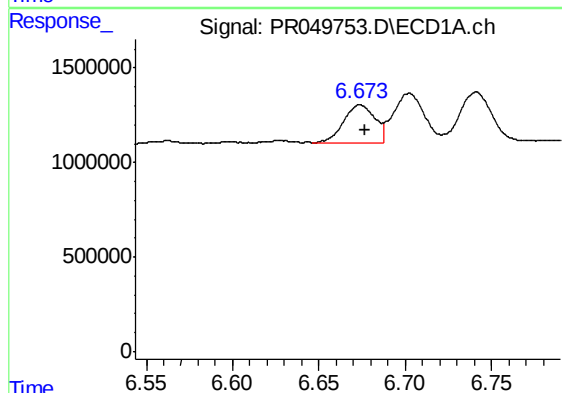


#26 AR-1254-1

R.T.: 6.674 min
Delta R.T.: -0.003 min
Response: 2509088
Conc: 15.77 ng/ml

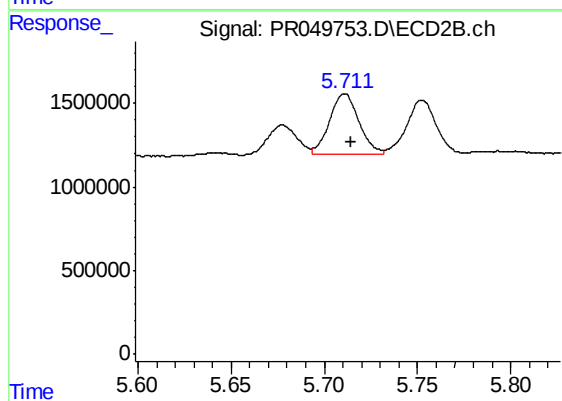

#26 AR-1254-1


R.T.: 5.711 min
Delta R.T.: -0.003 min
Response: 3992275
Conc: 10.62 ng/ml



#27 AR-1254-2


R.T.: 6.901 min
Delta R.T.: 0.007 min
Response: 2804205
Conc: 11.13 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




#27 AR-1254-2

R.T.: 5.859 min
Delta R.T.: -0.002 min
Response: 875781
Conc: 2.72 ng/ml




#28 AR-1254-3

R.T.: 7.263 min
Delta R.T.: -0.001 min
Response: 1543159
Conc: 5.59 ng/ml

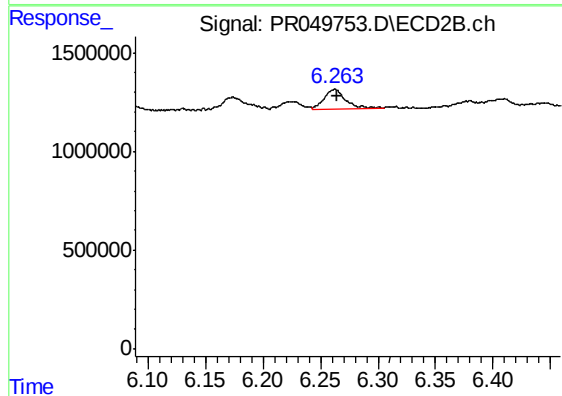

#28 AR-1254-3


R.T.: 6.263 min
Delta R.T.: -0.002 min
Response: 1270202
Conc: 2.23 ng/ml



#29 AR-1254-4


R.T.: 7.548 min
Delta R.T.: -0.004 min
Response: 695411
Conc: 3.30 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




#29 AR-1254-4

R.T.: 6.489 min
Delta R.T.: -0.003 min
Response: 886192
Conc: 2.48 ng/ml




#30 AR-1254-5

R.T.: 7.971 min
Delta R.T.: 0.000 min
Response: 270861
Conc: 1.19 ng/ml

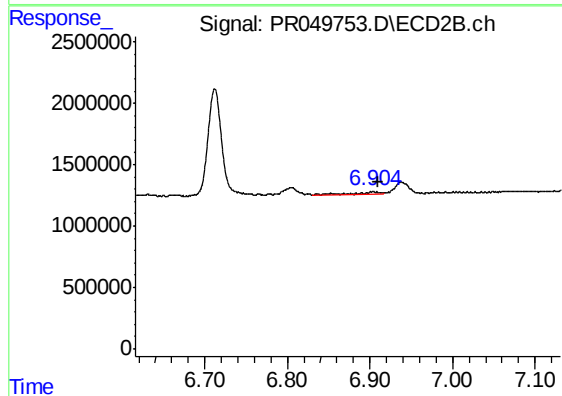

#30 AR-1254-5


R.T.: 6.904 min
Delta R.T.: -0.005 min
Response: 354329
Conc: 0.71 ng/ml

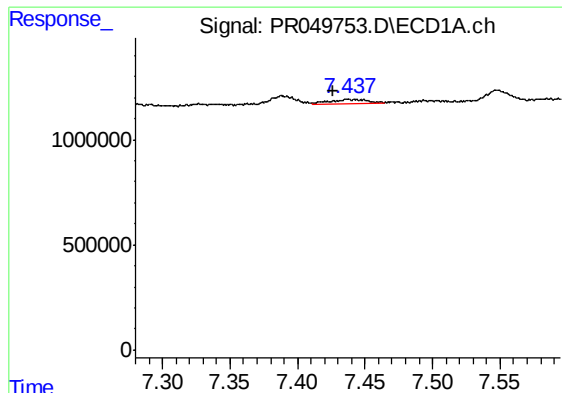

#31 AR-1260-1


R.T.: 7.437 min
Delta R.T.: 0.011 min
Response: 397637
Conc: 2.00 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

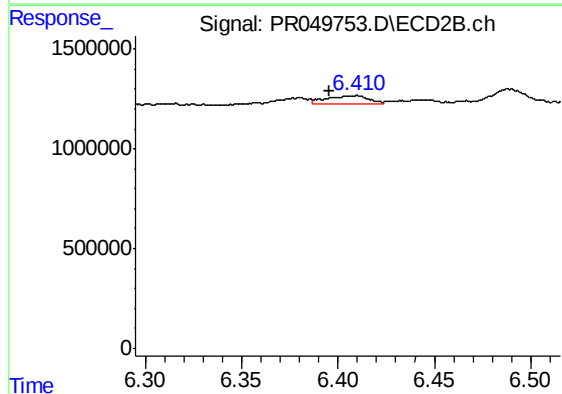


#31 AR-1260-1

R.T.: 6.410 min
Delta R.T.: 0.015 min
Response: 620245
Conc: 1.73 ng/ml

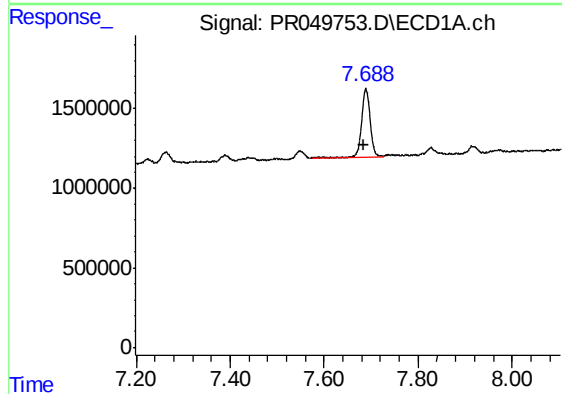


#32 AR-1260-2

R.T.: 7.689 min
Delta R.T.: 0.005 min
Response: 5444564
Conc: 22.30 ng/ml

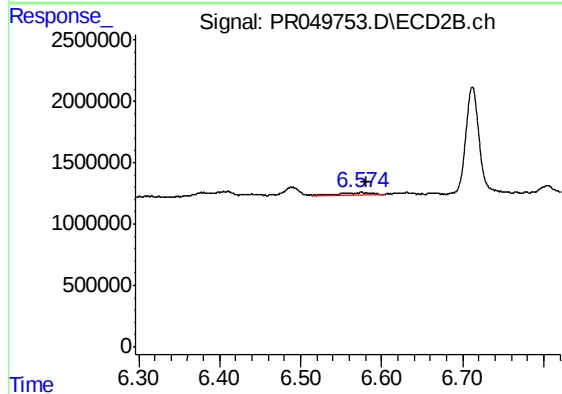

#32 AR-1260-2


R.T.: 6.575 min
Delta R.T.: -0.007 min
Response: 492610
Conc: 1.11 ng/ml



#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.042 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

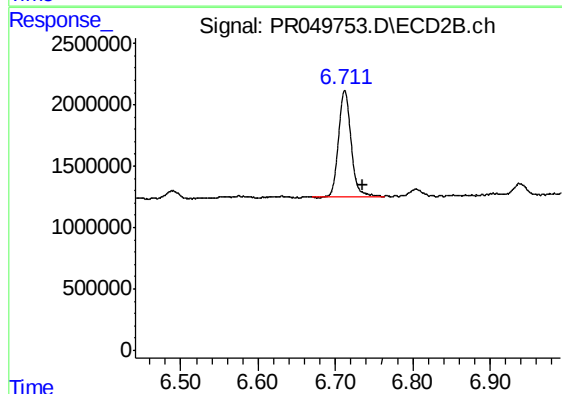


#33 AR-1260-3

R.T.: 6.712 min
Delta R.T.: -0.024 min
Response: 9886435
Conc: 23.50 ng/ml




#35 AR-1260-5

R.T.: 8.615 min
Delta R.T.: 0.001 min
Response: 314804
Conc: 0.70 ng/ml

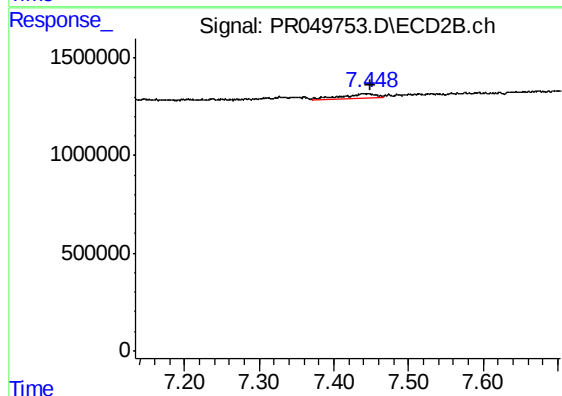

#35 AR-1260-5


R.T.: 7.441 min
Delta R.T.: -0.007 min
Response: 761680
Conc: 0.83 ng/ml



#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 8.041 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

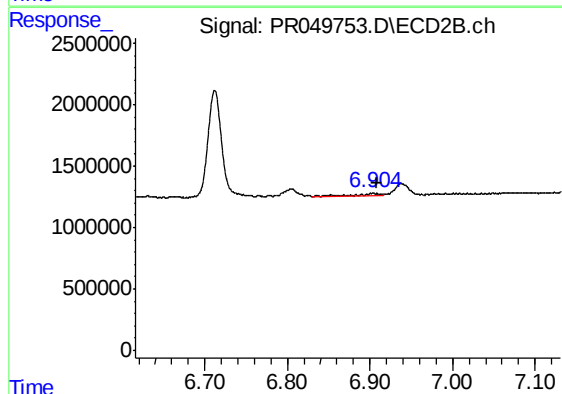


#36 AR-1262-1

R.T.: 6.904 min
Delta R.T.: -0.004 min
Response: 354329
Conc: 1.38 ng/ml




#37 AR-1262-2

R.T.: 8.615 min
Delta R.T.: 0.002 min
Response: 314804
Conc: 0.63 ng/ml

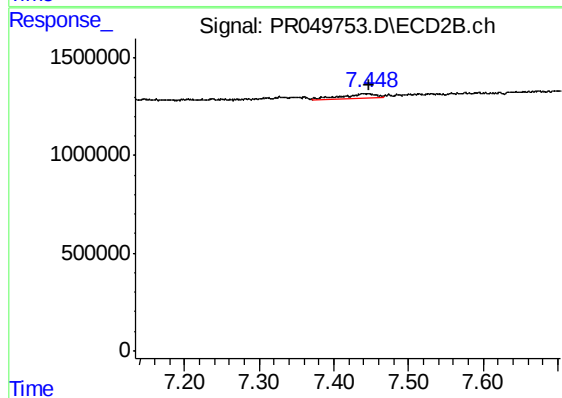

#37 AR-1262-2


R.T.: 7.441 min
Delta R.T.: -0.006 min
Response: 761680
Conc: 0.77 ng/ml



#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 8.936 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




#38 AR-1262-3

R.T.: 7.703 min
Delta R.T.: -0.029 min
Response: 1575345
Conc: 4.37 ng/ml




#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 9.031 min
Response: 0
Conc: N.D.

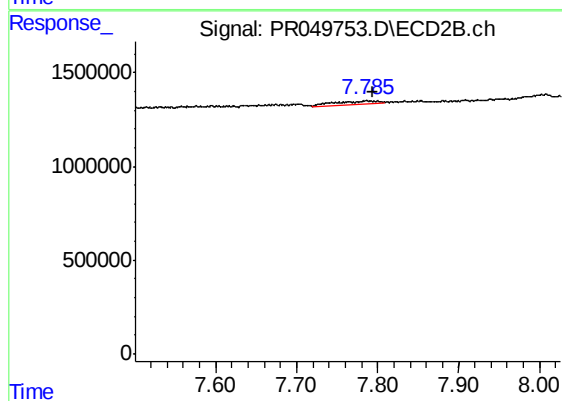

#39 AR-1262-4


R.T.: 7.786 min
Delta R.T.: -0.009 min
Response: 575702
Conc: 0.80 ng/ml



#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.935 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




#41 AR-1268-1

R.T.: 7.703 min
Delta R.T.: -0.029 min
Response: 1575345
Conc: 1.40 ng/ml




#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 9.036 min
Response: 0
Conc: N.D.

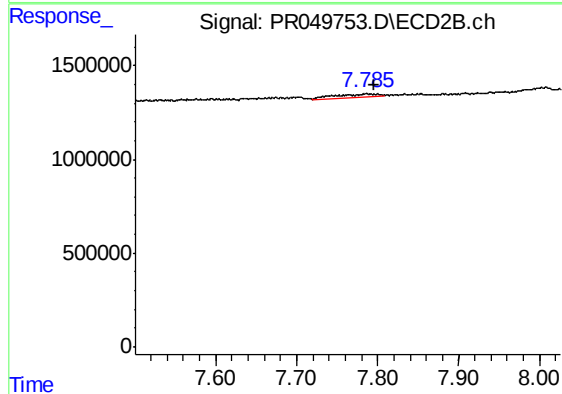

#42 AR-1268-2


R.T.: 7.786 min
Delta R.T.: -0.011 min
Response: 575702
Conc: 0.54 ng/ml



#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.272 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021




#43 AR-1268-3

R.T.: 8.003 min
Delta R.T.: -0.004 min
Response: 338440
Conc: 0.39 ng/ml



#45 AR-1268-5

R.T.: 10.162 min
Delta R.T.: 0.000 min
Response: 318258
Conc: 0.19 ng/ml

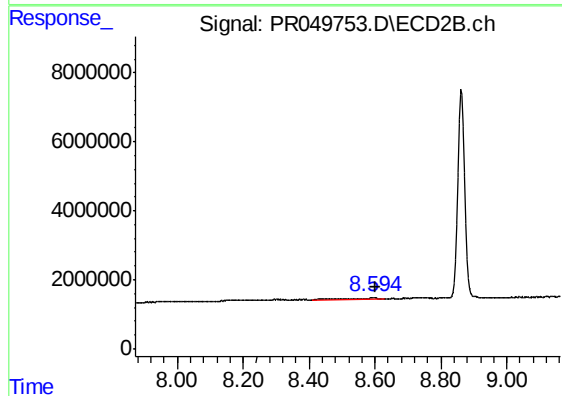

#45 AR-1268-5

R.T.: 8.594 min
Delta R.T.: -0.006 min
Response: 2323769
Conc: 0.76 ng/ml