

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040221\
 Data File : PR049757.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2021 03:36
 Operator : DD\AJ
 Sample : M1458-07
 Misc : AR1262 LOD 40 PPB
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 01:58:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Apr 03 08:12:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.635	3.820	94932954	151.2E6	24.314	22.796
2)	SA Decachlor...	10.514	8.861	115.0E6	144.3E6	25.879	18.949 #
Target Compounds							
3)	L1 AR-1016-1	5.817	4.909	434627	329427	2.827	1.372 #
4)	L1 AR-1016-2	5.841	4.931	482931	441928	2.260	1.281 #
5)	L1 AR-1016-3	5.905	0.000	317643	0	2.474	N.D. #
6)	L1 AR-1016-4	6.006	5.148	386028	483876	3.628	3.480
7)	L1 AR-1016-5	6.299	5.362	294734	230492	2.751	1.227 #
8)	L2 AR-1221-1	4.862	0.000	3331429	0	80.594	N.D. #
9)	L2 AR-1221-2	4.948	4.122	1474027	2422024	47.244	49.281
12)	L3 AR-1232-2	0.000	4.931	0	441928	N.D.	3.327 #
13)	L3 AR-1232-3	5.841	0.000	482931	0	5.668	N.D. #
14)	L3 AR-1232-4	6.006	0.000	386028	0	9.058	N.D. #
15)	L3 AR-1232-5	6.092	5.362	278067	230492	8.408	3.491 #
16)	L4 AR-1242-1	5.817	4.909	434627	329427	3.876	1.877 #
17)	L4 AR-1242-2	5.841	4.931	482931	441928	3.057	1.760 #
18)	L4 AR-1242-3	5.905	0.000	317643	0	3.317	N.D. #
19)	L4 AR-1242-4	6.006	0.000	386028	0	4.818	N.D. #
20)	L4 AR-1242-5	6.743	5.713	326637	2167419	3.585	12.701 #
21)	L5 AR-1248-1	5.817	4.909	434627	329427	5.073	2.441 #
22)	L5 AR-1248-2	6.092	5.148	278067	483876	2.313	2.730
23)	L5 AR-1248-3	6.299	0.000	294734	0	2.176	N.D. #
24)	L5 AR-1248-4	0.000	5.362	0	230492	N.D.	0.991 #
25)	L5 AR-1248-5	6.743	0.000	326637	0	2.124	N.D. #
26)	L6 AR-1254-1	6.674	5.713	2843022	2167419	17.872	5.765 #
27)	L6 AR-1254-2	6.891	5.859	2392879	2385272	9.500	7.398
28)	L6 AR-1254-3	7.262	6.279	1124546	9787499	4.071	17.170 #
29)	L6 AR-1254-4	7.547	6.489	1089420	676161	5.177	1.891 #
30)	L6 AR-1254-5	7.965	6.905	11685381	12629283	51.526	25.346 #
31)	L7 AR-1260-1	7.422	6.392	12394827	14500658	62.329	40.430 #
32)	L7 AR-1260-2	7.680	6.578	13286615	16670665	54.424	37.549 #
33)	L7 AR-1260-3	8.039	6.736	17482805	16810183	93.507	39.963 #
34)	L7 AR-1260-4	8.275	7.204	16444055	21247060	75.264	59.616
35)	L7 AR-1260-5	8.609	7.443	29854125	42199724	66.184	46.054 #
36)	L8 AR-1262-1	8.039	6.905	17482805	12629283	66.767	49.209 #
37)	L8 AR-1262-2	8.609	7.443	29854125	42199724	59.990	42.853 #
38)	L8 AR-1262-3	8.933	7.728	14733696	16891870	44.799	46.911
39)	L8 AR-1262-4	9.030	7.792	7241794	31999441	29.315	44.695 #
40)	L8 AR-1262-5	9.726	8.291	11475829	15077823	63.685	46.913 #
41)	L9 AR-1268-1	8.933	7.728	14733696	16891870	25.122	15.059 #
42)	L9 AR-1268-2	9.030	7.792	7241794	31999441	13.451	30.242 #
43)	L9 AR-1268-3	9.270	8.002	998022	2503081	2.181	2.857 #
44)	L9 AR-1268-4	9.726	8.291	11475829	15077823	56.822	41.411 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040221\
 Data File : PR049757.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2021 03:36
 Operator : DD\AJ
 Sample : M1458-07
 Misc : AR1262 LOD 40 PPB
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 01:58:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Apr 03 08:12:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
45) L9	AR-1268-5	10.159	8.595	4625923	6302747	2.827	2.071 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040221\
Data File : PR049757.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2021 03:36
Operator : DD\AJ
Sample : M1458-07
Misc : AR1262 LOD 40 PPB
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 01:58:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040221.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Apr 03 08:12:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

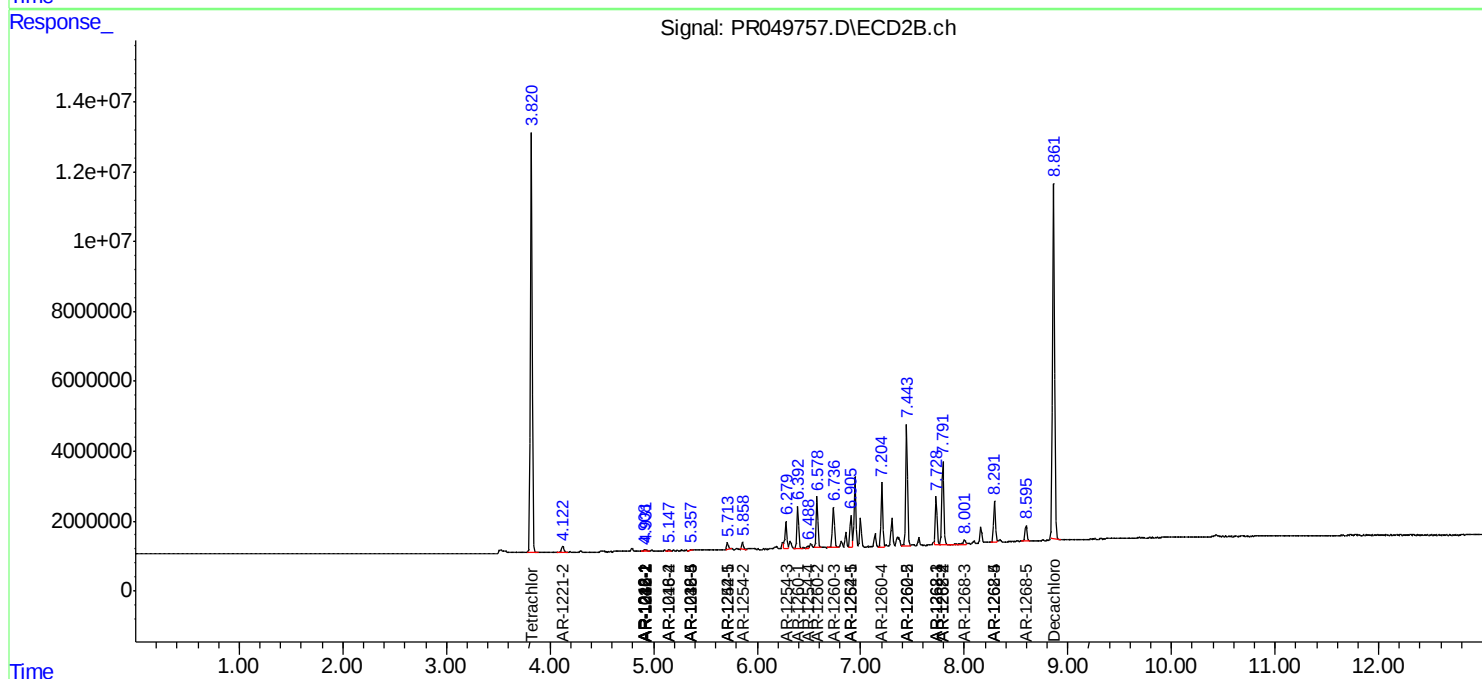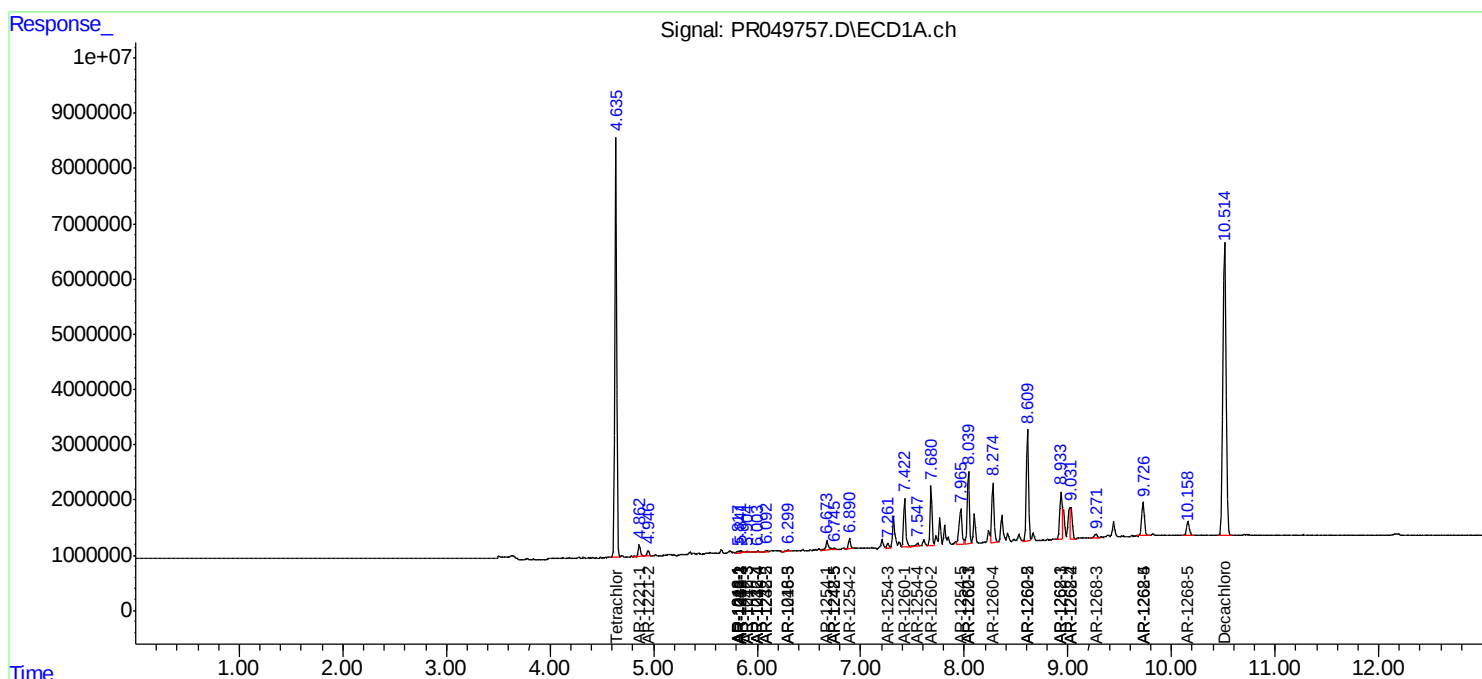


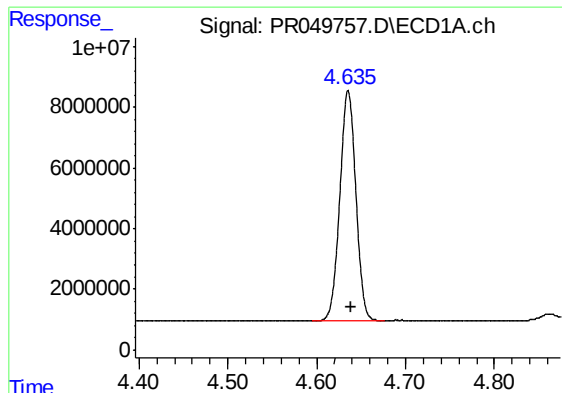

#1 Tetrachloro-m-xylene


R.T.: 4.635 min
Delta R.T.: -0.004 min
Response: 94932954
Conc: 24.31 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

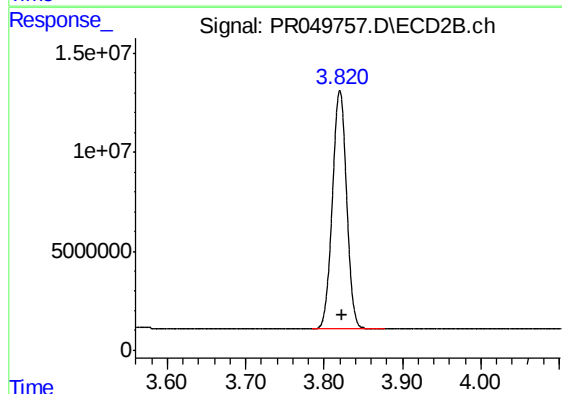


#1 Tetrachloro-m-xylene

R.T.: 3.820 min
Delta R.T.: -0.002 min
Response: 151175345
Conc: 22.80 ng/ml

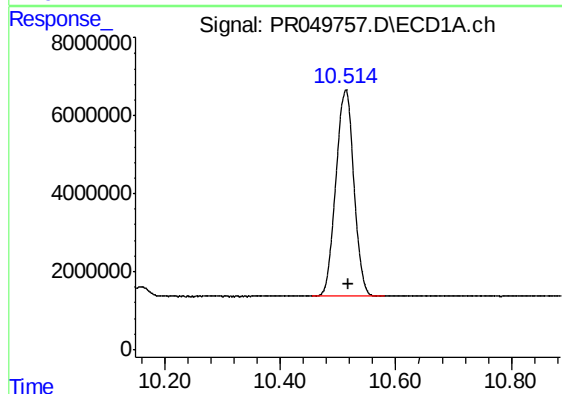


#2 Decachlorobiphenyl

R.T.: 10.514 min
Delta R.T.: -0.003 min
Response: 114984508
Conc: 25.88 ng/ml

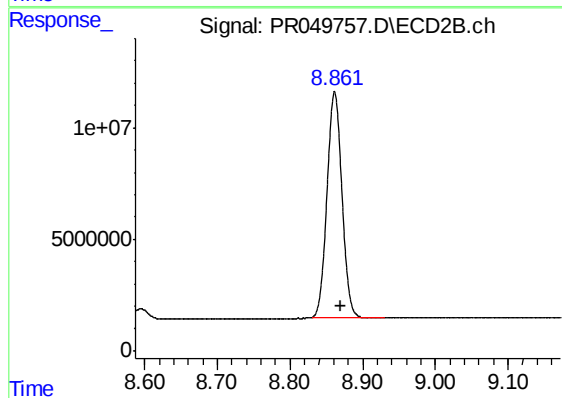

#2 Decachlorobiphenyl


R.T.: 8.861 min
Delta R.T.: -0.008 min
Response: 144264398
Conc: 18.95 ng/ml

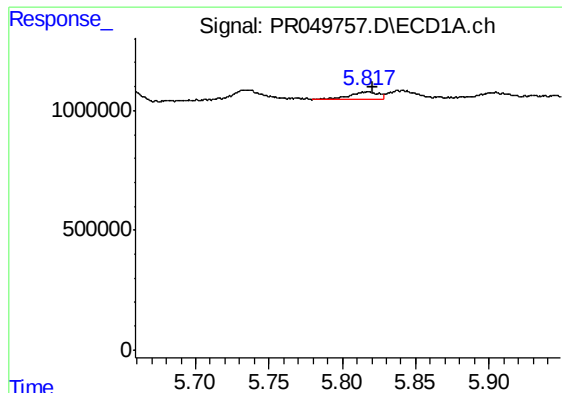

#3 AR-1016-1


R.T.: 5.817 min
Delta R.T.: -0.003 min
Response: 434627
Conc: 2.83 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

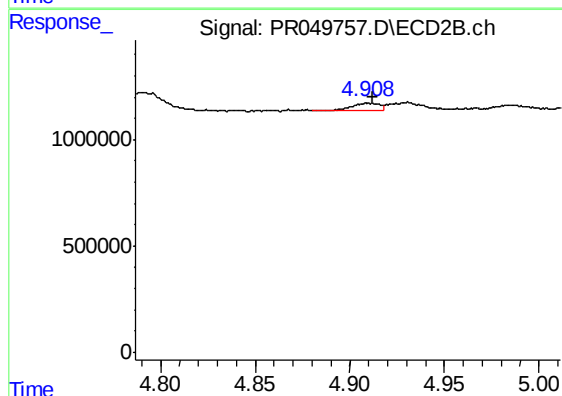


#3 AR-1016-1

R.T.: 4.909 min
Delta R.T.: -0.003 min
Response: 329427
Conc: 1.37 ng/ml

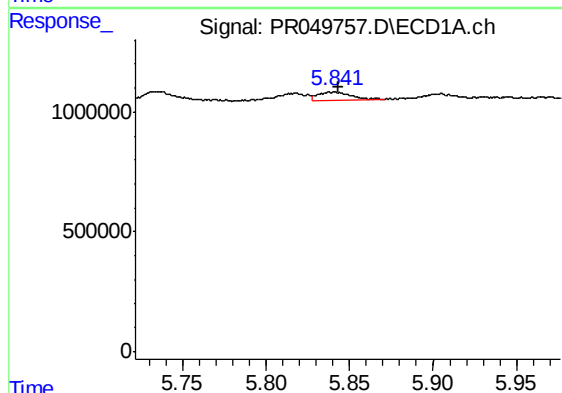


#4 AR-1016-2

R.T.: 5.841 min
Delta R.T.: -0.003 min
Response: 482931
Conc: 2.26 ng/ml

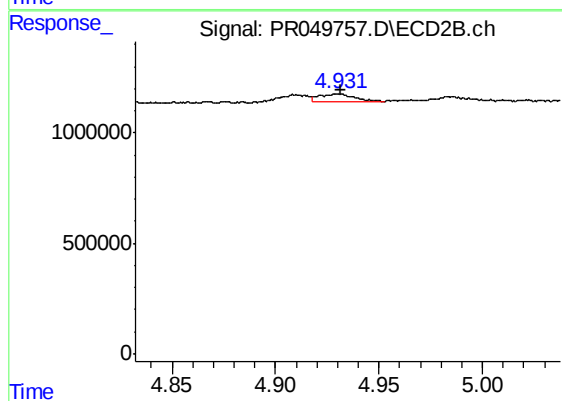

#4 AR-1016-2


R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 441928
Conc: 1.28 ng/ml

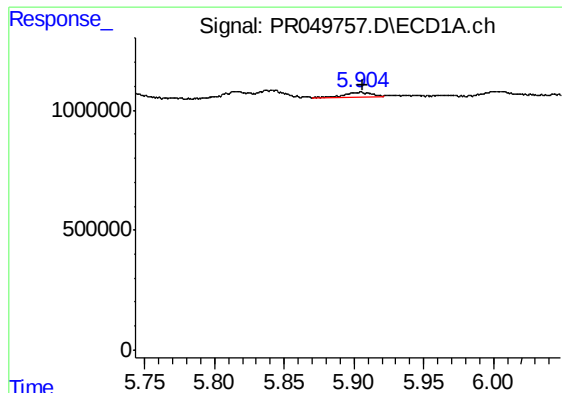

#5 AR-1016-3


R.T.: 5.905 min
Delta R.T.: -0.001 min
Response: 317643
Conc: 2.47 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

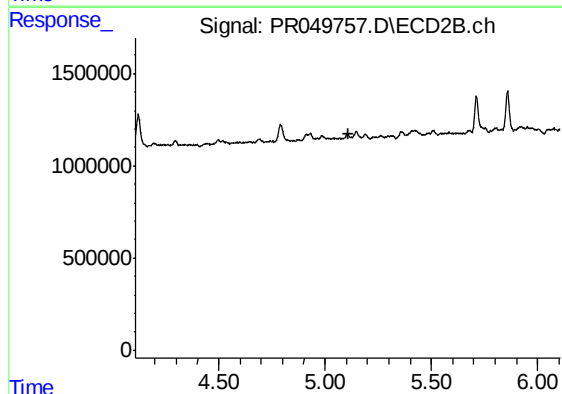


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 5.108 min
Response: 0
Conc: N.D.

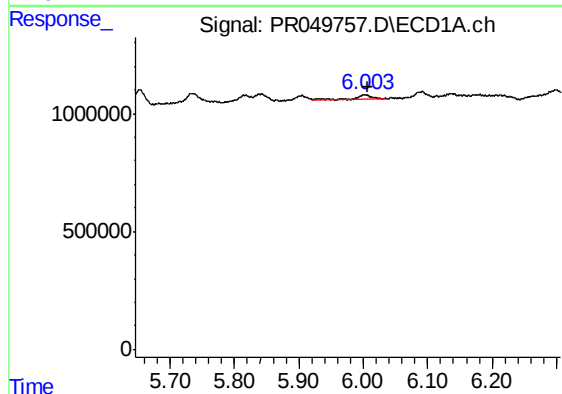


#6 AR-1016-4

R.T.: 6.006 min
Delta R.T.: 0.000 min
Response: 386028
Conc: 3.63 ng/ml

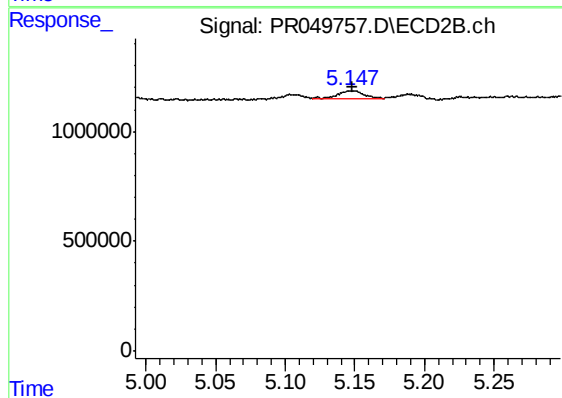

#6 AR-1016-4


R.T.: 5.148 min
Delta R.T.: 0.000 min
Response: 483876
Conc: 3.48 ng/ml

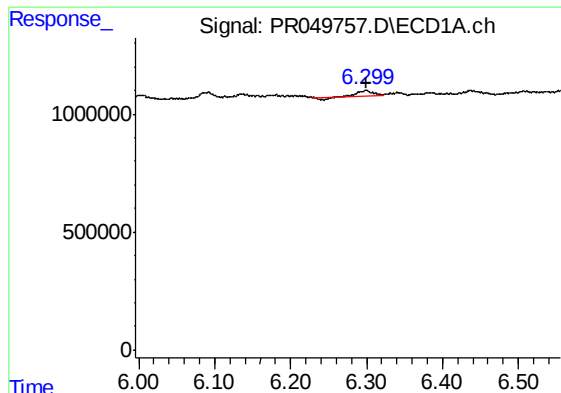

#7 AR-1016-5


R.T.: 6.299 min
Delta R.T.: 0.000 min
Response: 294734
Conc: 2.75 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

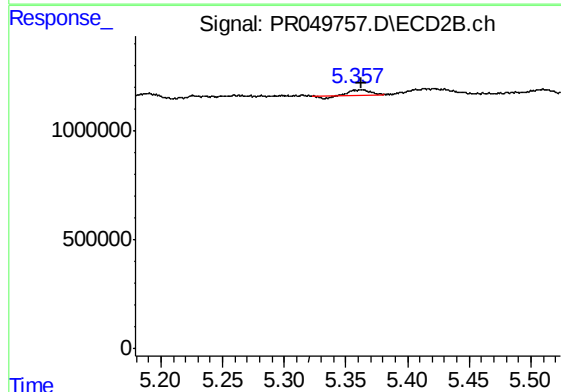


#7 AR-1016-5

R.T.: 5.362 min
Delta R.T.: 0.000 min
Response: 230492
Conc: 1.23 ng/ml

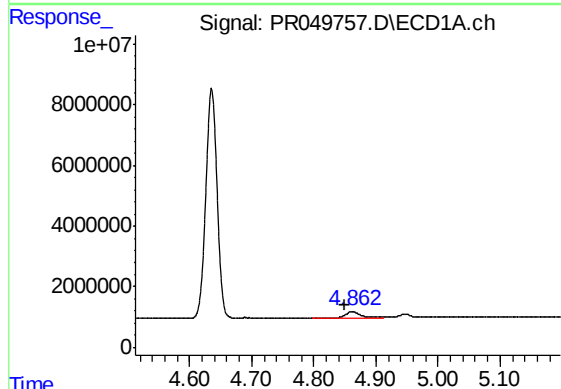


#8 AR-1221-1

R.T.: 4.862 min
Delta R.T.: 0.011 min
Response: 3331429
Conc: 80.59 ng/ml

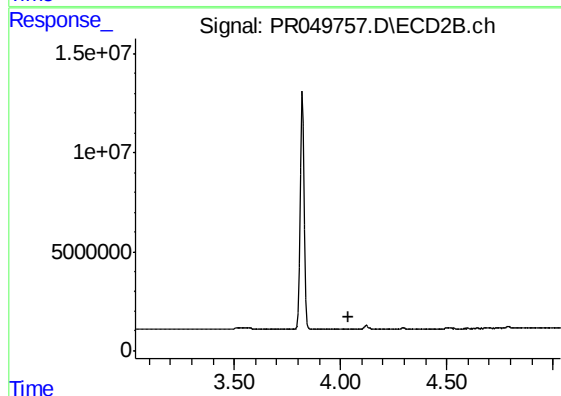

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 4.035 min
Response: 0
Conc: N.D.

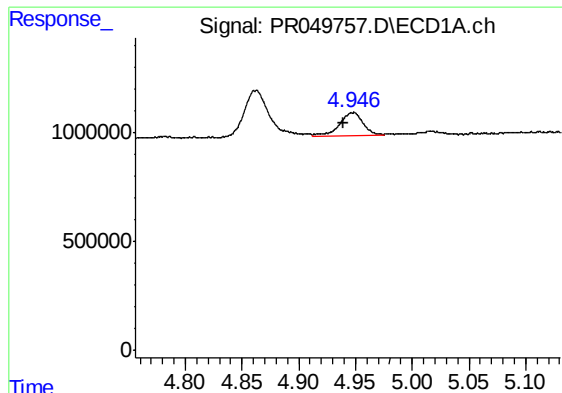

#9 AR-1221-2


R.T.: 4.948 min
Delta R.T.: 0.009 min
Response: 1474027
Conc: 47.24 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

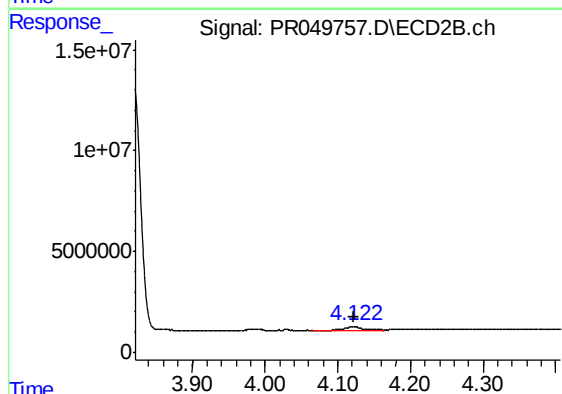


#9 AR-1221-2

R.T.: 4.122 min
Delta R.T.: 0.000 min
Response: 2422024
Conc: 49.28 ng/ml

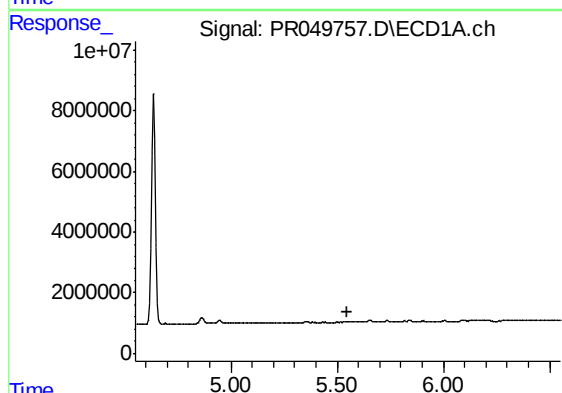


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.551 min
Response: 0
Conc: N.D.

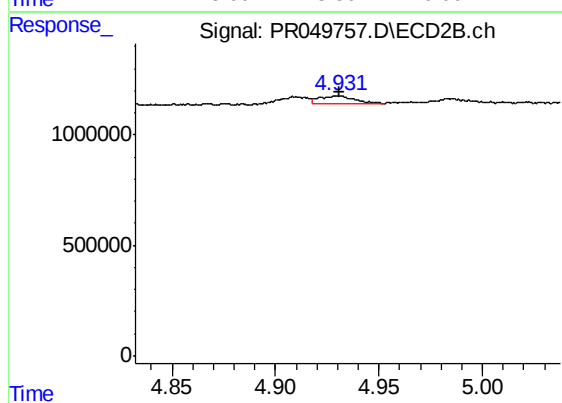

#12 AR-1232-2


R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 441928
Conc: 3.33 ng/ml

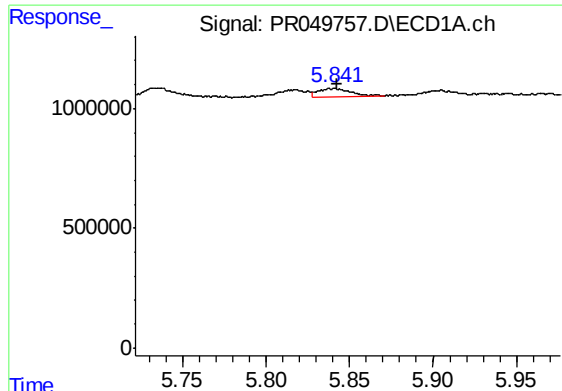

#13 AR-1232-3


R.T.: 5.841 min
Delta R.T.: -0.002 min
Response: 482931
Conc: 5.67 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

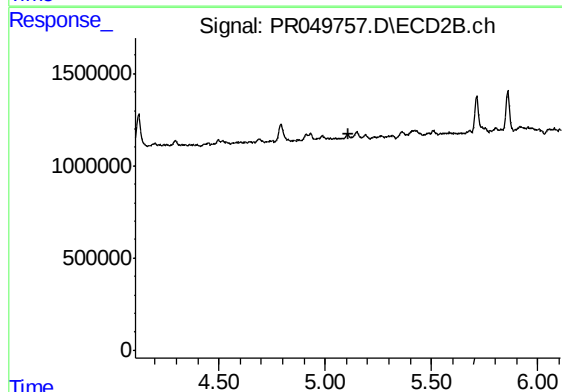


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 5.107 min
Response: 0
Conc: N.D.

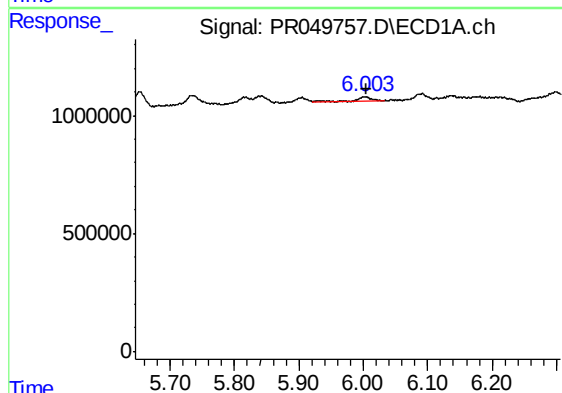


#14 AR-1232-4

R.T.: 6.006 min
Delta R.T.: 0.000 min
Response: 386028
Conc: 9.06 ng/ml

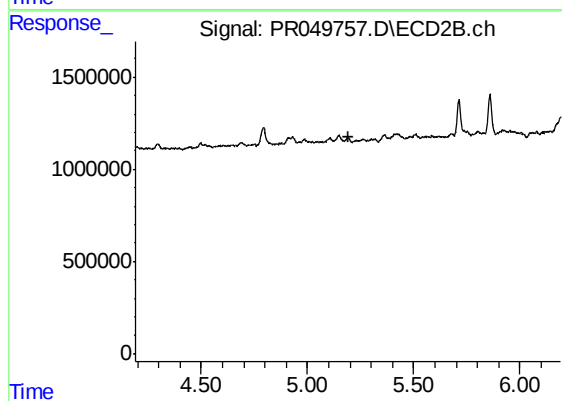

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 5.191 min
Response: 0
Conc: N.D.

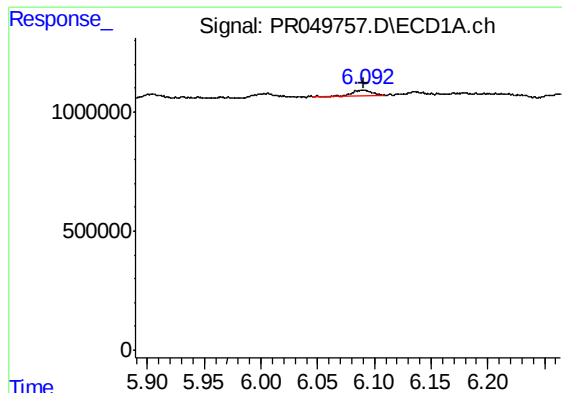

#15 AR-1232-5


R.T.: 6.092 min
Delta R.T.: 0.000 min
Response: 278067
Conc: 8.41 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

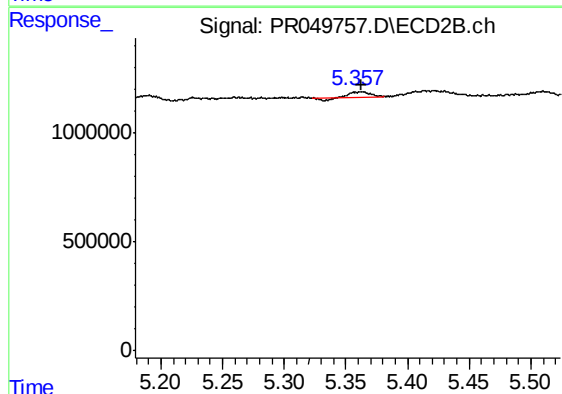


#15 AR-1232-5

R.T.: 5.362 min
Delta R.T.: 0.000 min
Response: 230492
Conc: 3.49 ng/ml

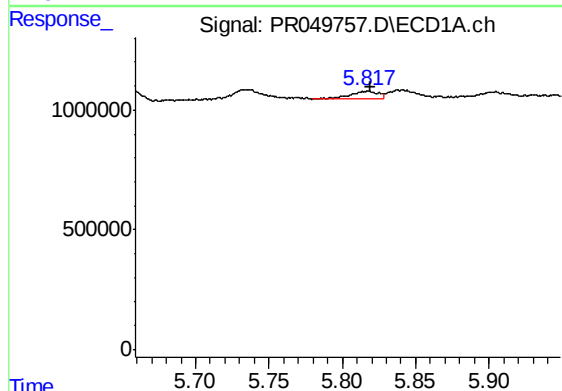


#16 AR-1242-1

R.T.: 5.817 min
Delta R.T.: -0.002 min
Response: 434627
Conc: 3.88 ng/ml

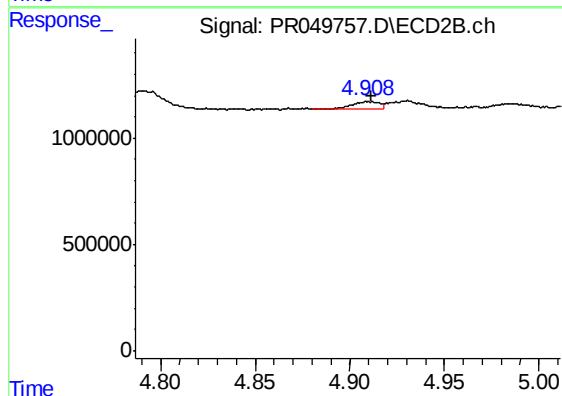

#16 AR-1242-1


R.T.: 4.909 min
Delta R.T.: -0.002 min
Response: 329427
Conc: 1.88 ng/ml

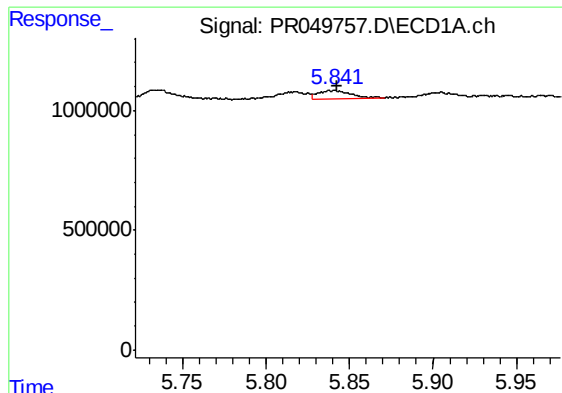

#17 AR-1242-2


R.T.: 5.841 min
Delta R.T.: -0.002 min
Response: 482931
Conc: 3.06 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

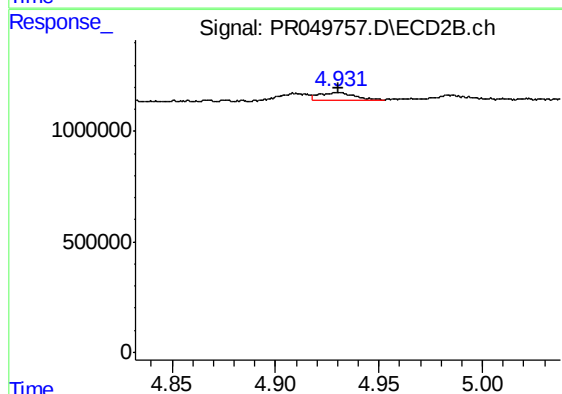


#17 AR-1242-2

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 441928
Conc: 1.76 ng/ml

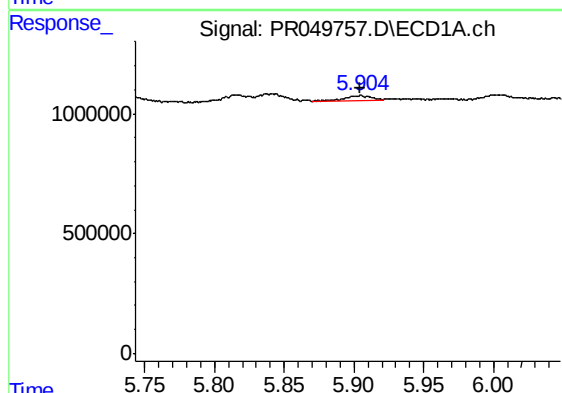


#18 AR-1242-3

R.T.: 5.905 min
Delta R.T.: 0.000 min
Response: 317643
Conc: 3.32 ng/ml

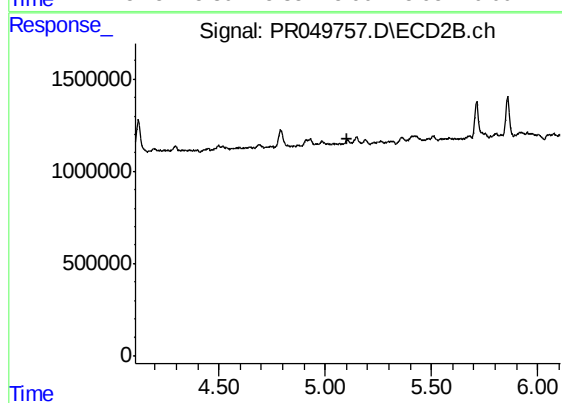

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 5.107 min
Response: 0
Conc: N.D.

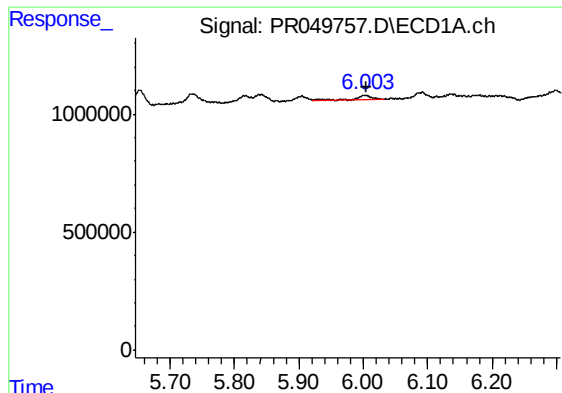

#19 AR-1242-4


R.T.: 6.006 min
Delta R.T.: 0.000 min
Response: 386028
Conc: 4.82 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

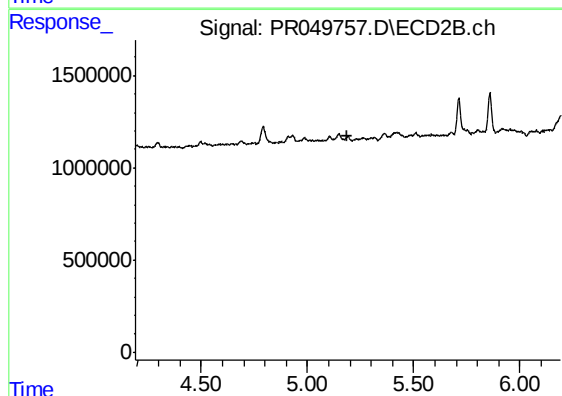


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 5.191 min
Response: 0
Conc: N.D.

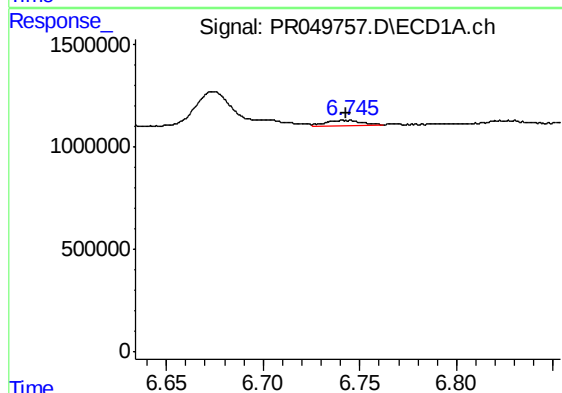


#20 AR-1242-5

R.T.: 6.743 min
Delta R.T.: 0.000 min
Response: 326637
Conc: 3.59 ng/ml

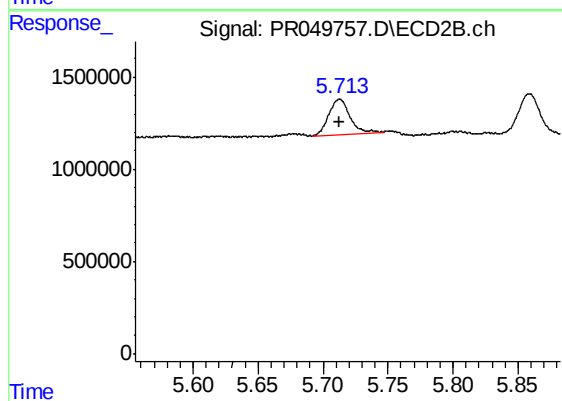

#20 AR-1242-5


R.T.: 5.713 min
Delta R.T.: 0.000 min
Response: 2167419
Conc: 12.70 ng/ml

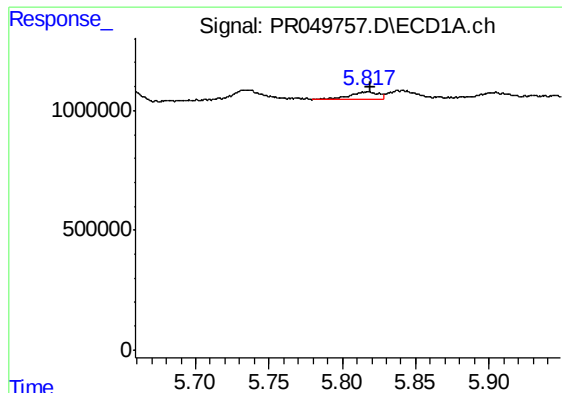

#21 AR-1248-1


R.T.: 5.817 min
Delta R.T.: -0.002 min
Response: 434627
Conc: 5.07 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

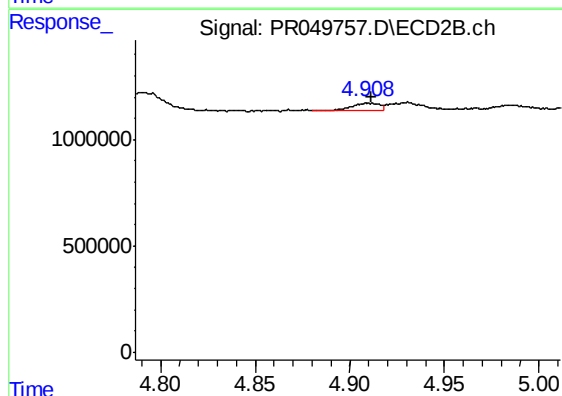


#21 AR-1248-1

R.T.: 4.909 min
Delta R.T.: -0.002 min
Response: 329427
Conc: 2.44 ng/ml

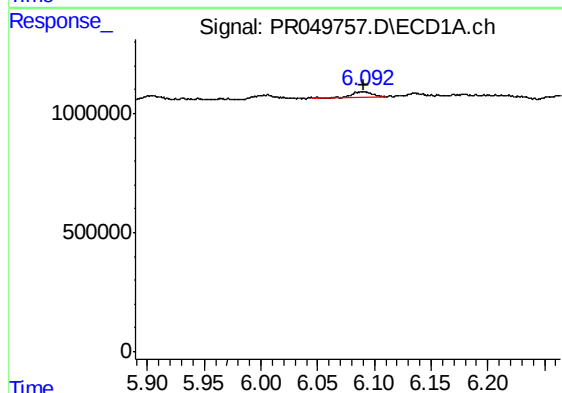


#22 AR-1248-2

R.T.: 6.092 min
Delta R.T.: 0.000 min
Response: 278067
Conc: 2.31 ng/ml

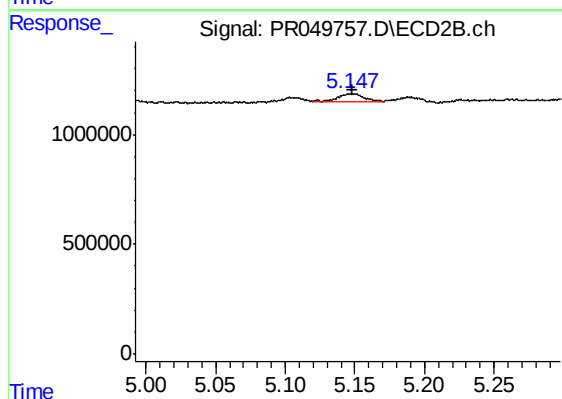

#22 AR-1248-2


R.T.: 5.148 min
Delta R.T.: 0.000 min
Response: 483876
Conc: 2.73 ng/ml

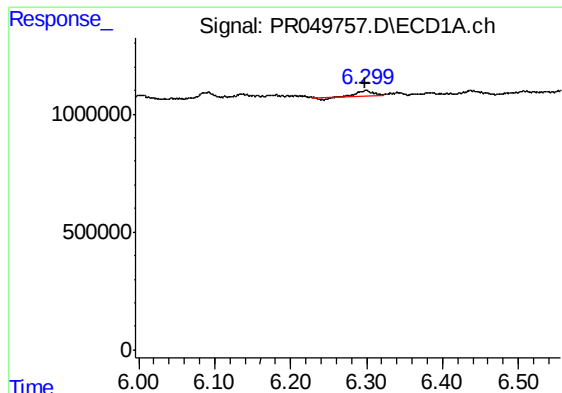

#23 AR-1248-3


R.T.: 6.299 min
Delta R.T.: 0.000 min
Response: 294734
Conc: 2.18 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

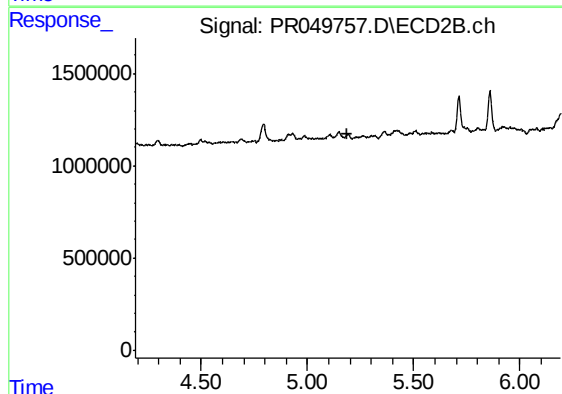


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 5.191 min
Response: 0
Conc: N.D.

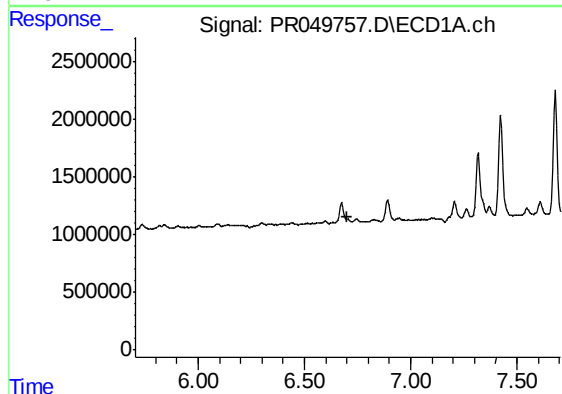


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 6.704 min
Response: 0
Conc: N.D.

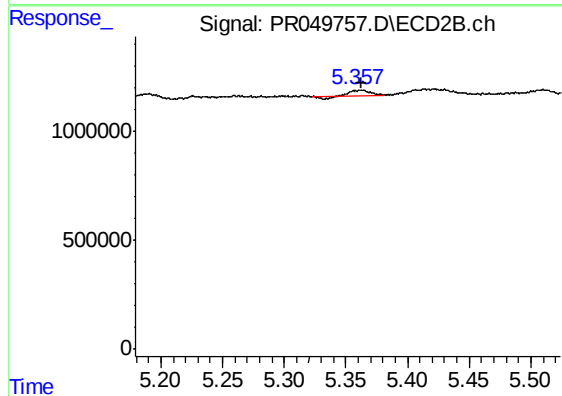

#24 AR-1248-4


R.T.: 5.362 min
Delta R.T.: 0.000 min
Response: 230492
Conc: 0.99 ng/ml

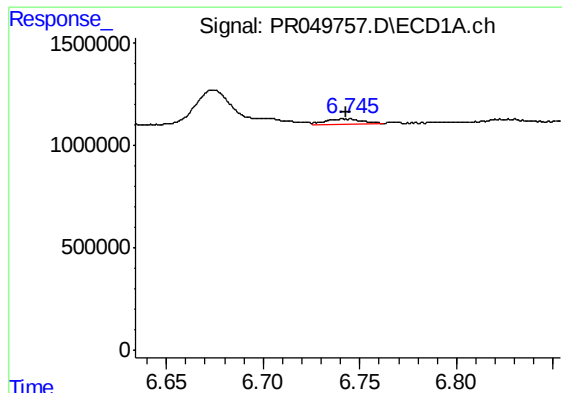

#25 AR-1248-5


R.T.: 6.743 min
Delta R.T.: 0.000 min
Response: 326637
Conc: 2.12 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

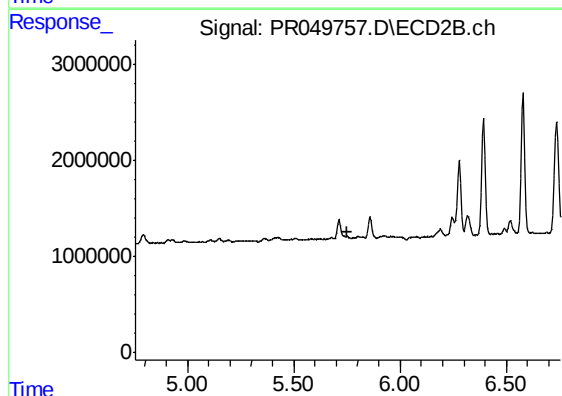


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.755 min
Response: 0
Conc: N.D.

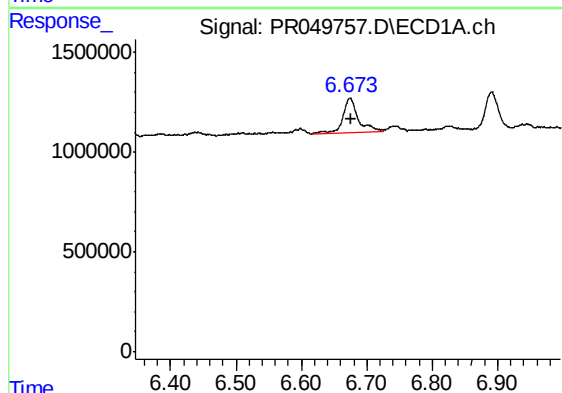


#26 AR-1254-1

R.T.: 6.674 min
Delta R.T.: -0.002 min
Response: 2843022
Conc: 17.87 ng/ml

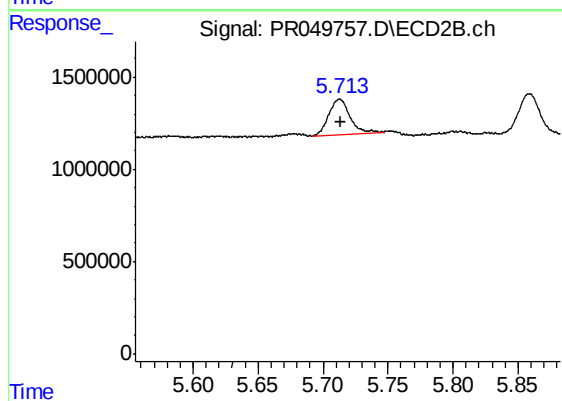

#26 AR-1254-1


R.T.: 5.713 min
Delta R.T.: -0.001 min
Response: 2167419
Conc: 5.77 ng/ml

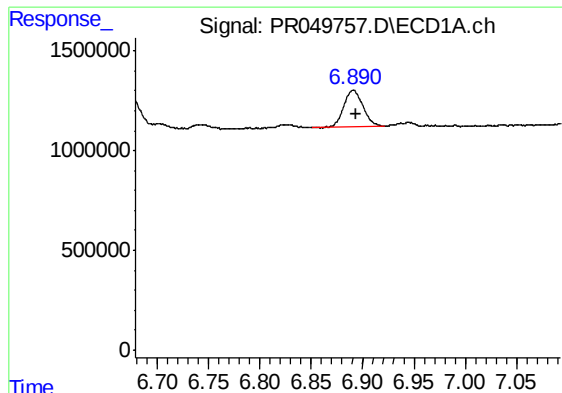

#27 AR-1254-2


R.T.: 6.891 min
Delta R.T.: -0.003 min
Response: 2392879
Conc: 9.50 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

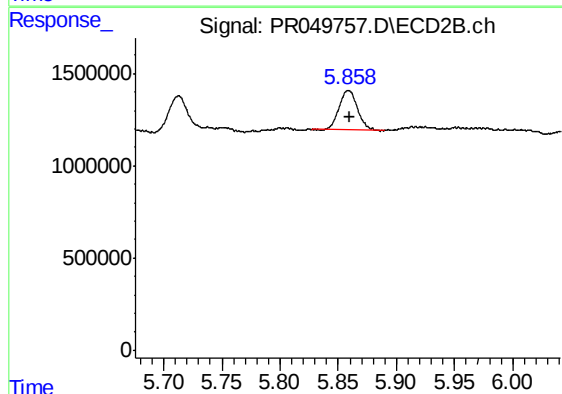


#27 AR-1254-2

R.T.: 5.859 min
Delta R.T.: -0.002 min
Response: 2385272
Conc: 7.40 ng/ml

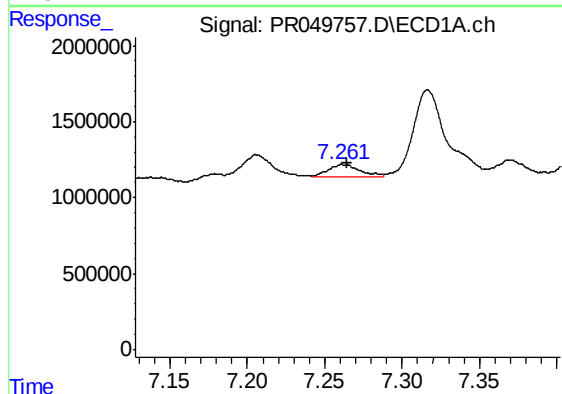


#28 AR-1254-3

R.T.: 7.262 min
Delta R.T.: -0.003 min
Response: 1124546
Conc: 4.07 ng/ml

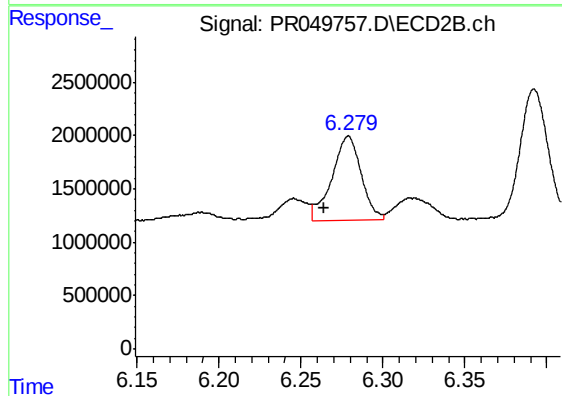

#28 AR-1254-3


R.T.: 6.279 min
Delta R.T.: 0.014 min
Response: 9787499
Conc: 17.17 ng/ml

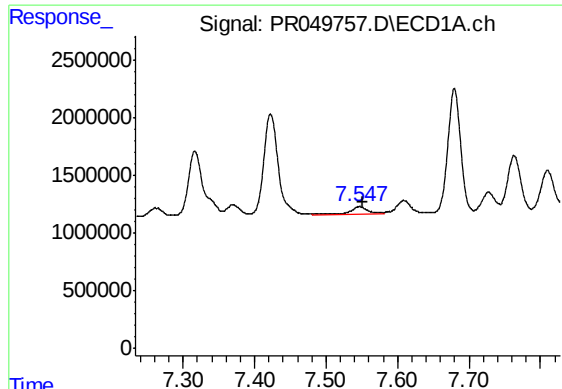

#29 AR-1254-4


R.T.: 7.547 min
Delta R.T.: -0.005 min
Response: 1089420
Conc: 5.18 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

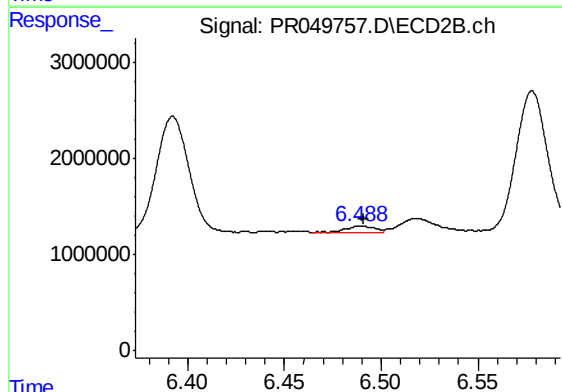


#29 AR-1254-4

R.T.: 6.489 min
Delta R.T.: -0.002 min
Response: 676161
Conc: 1.89 ng/ml

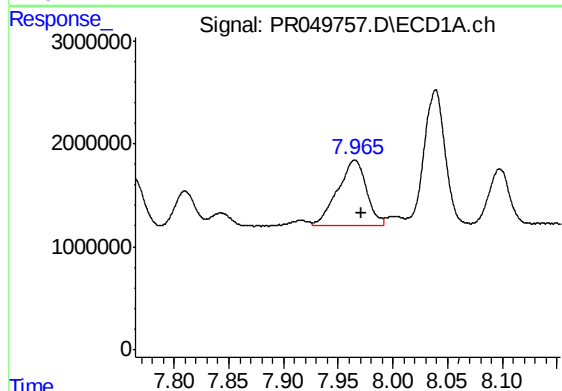


#30 AR-1254-5

R.T.: 7.965 min
Delta R.T.: -0.006 min
Response: 11685381
Conc: 51.53 ng/ml

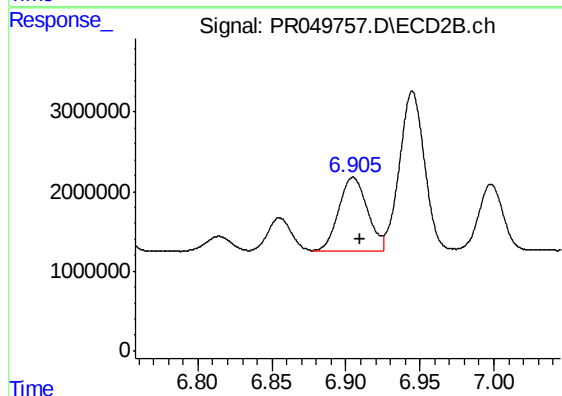

#30 AR-1254-5


R.T.: 6.905 min
Delta R.T.: -0.004 min
Response: 12629283
Conc: 25.35 ng/ml

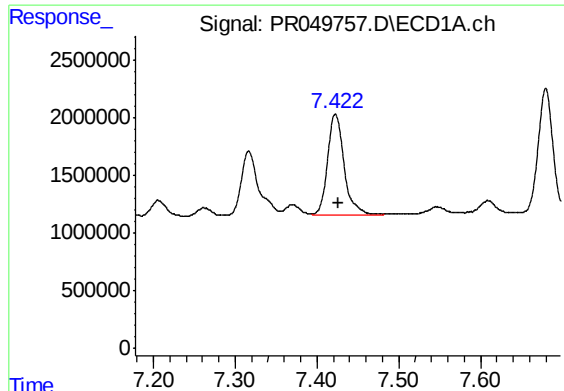

#31 AR-1260-1


R.T.: 7.422 min
Delta R.T.: -0.004 min
Response: 12394827
Conc: 62.33 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

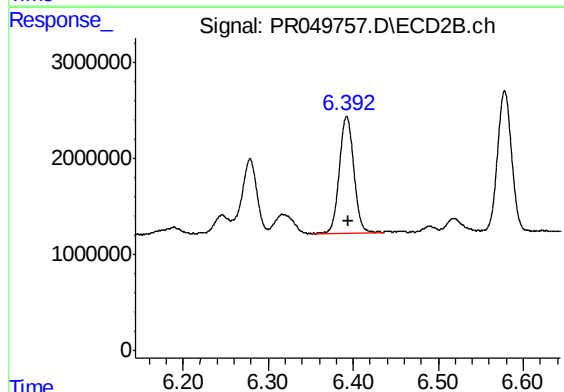


#31 AR-1260-1

R.T.: 6.392 min
Delta R.T.: -0.003 min
Response: 14500658
Conc: 40.43 ng/ml

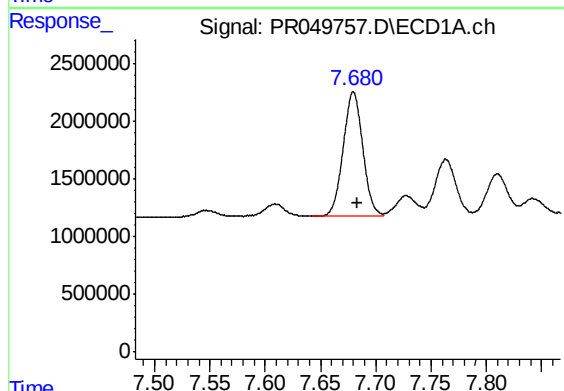


#32 AR-1260-2

R.T.: 7.680 min
Delta R.T.: -0.004 min
Response: 13286615
Conc: 54.42 ng/ml

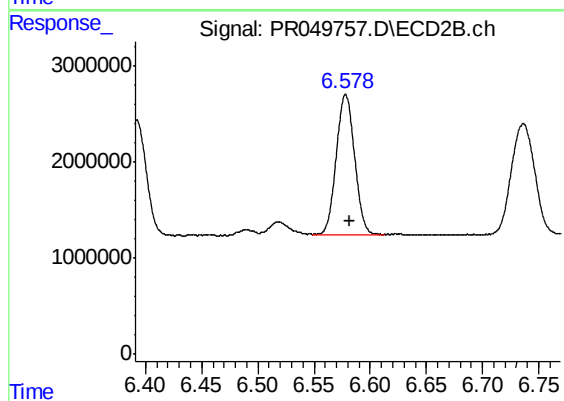

#32 AR-1260-2


R.T.: 6.578 min
Delta R.T.: -0.003 min
Response: 16670665
Conc: 37.55 ng/ml

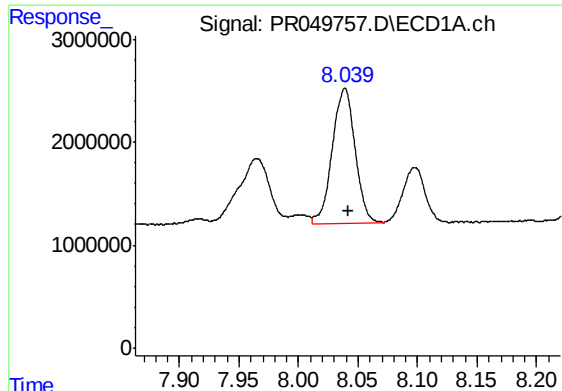

#33 AR-1260-3


R.T.: 8.039 min
Delta R.T.: -0.003 min
Response: 17482805
Conc: 93.51 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

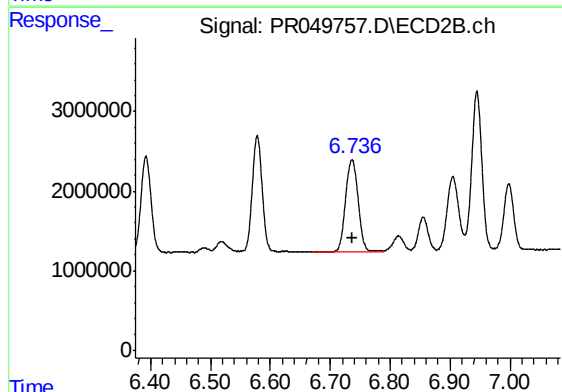


#33 AR-1260-3

R.T.: 6.736 min
Delta R.T.: 0.000 min
Response: 16810183
Conc: 39.96 ng/ml

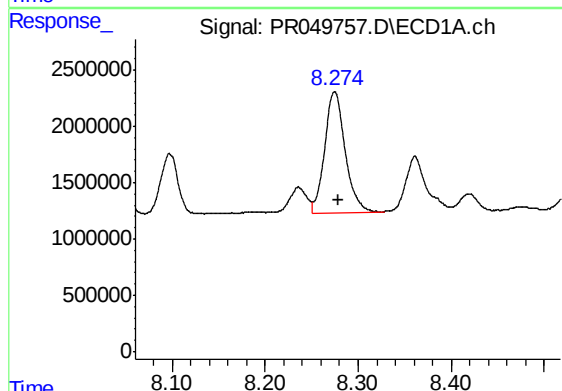


#34 AR-1260-4

R.T.: 8.275 min
Delta R.T.: -0.004 min
Response: 16444055
Conc: 75.26 ng/ml

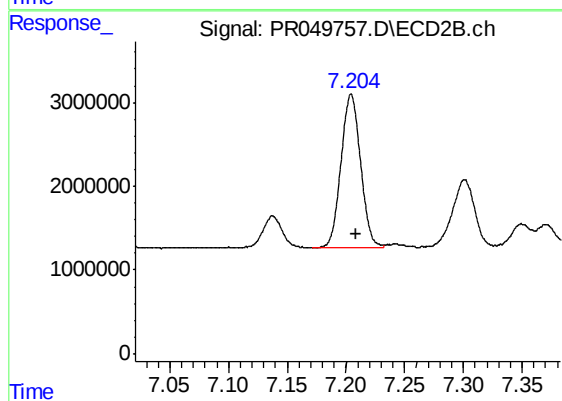

#34 AR-1260-4


R.T.: 7.204 min
Delta R.T.: -0.004 min
Response: 21247060
Conc: 59.62 ng/ml

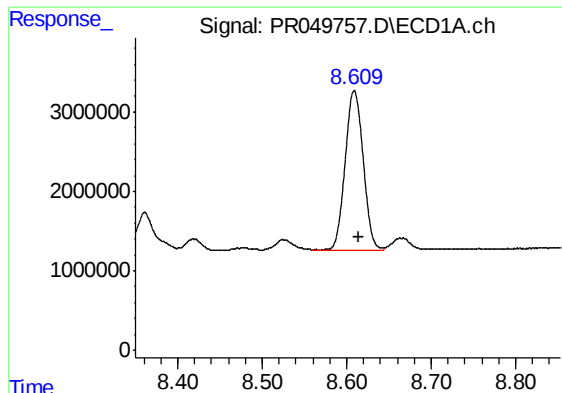

#35 AR-1260-5


R.T.: 8.609 min
Delta R.T.: -0.005 min
Response: 29854125
Conc: 66.18 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

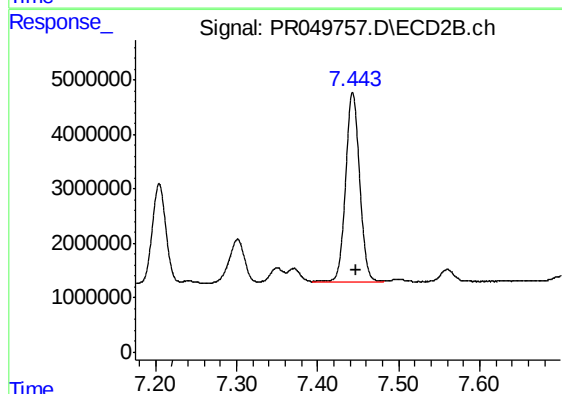


#35 AR-1260-5

R.T.: 7.443 min
Delta R.T.: -0.005 min
Response: 42199724
Conc: 46.05 ng/ml

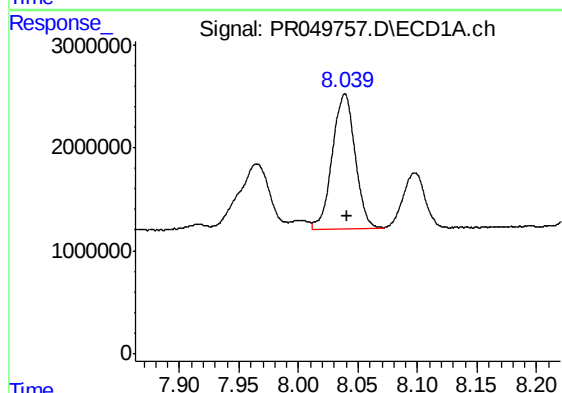


#36 AR-1262-1

R.T.: 8.039 min
Delta R.T.: -0.002 min
Response: 17482805
Conc: 66.77 ng/ml

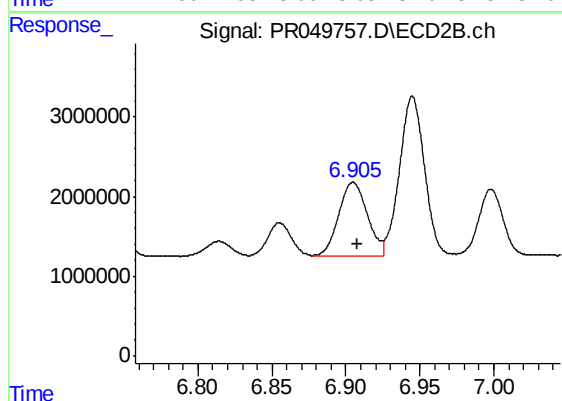

#36 AR-1262-1


R.T.: 6.905 min
Delta R.T.: -0.003 min
Response: 12629283
Conc: 49.21 ng/ml

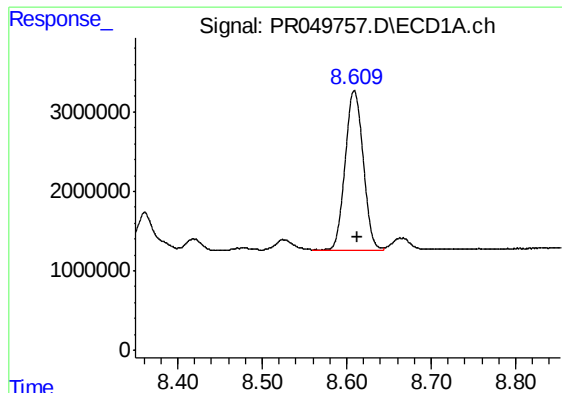

#37 AR-1262-2


R.T.: 8.609 min
Delta R.T.: -0.004 min
Response: 29854125
Conc: 59.99 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

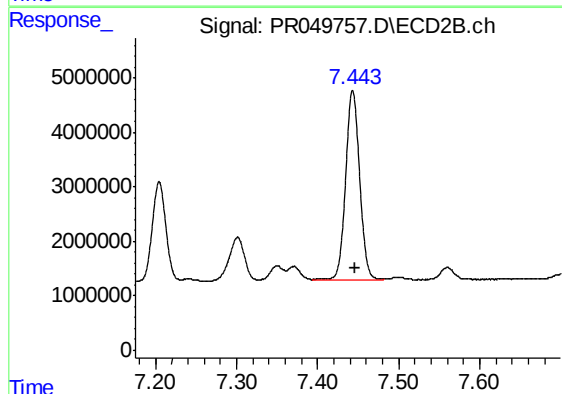


#37 AR-1262-2

R.T.: 7.443 min
Delta R.T.: -0.003 min
Response: 42199724
Conc: 42.85 ng/ml

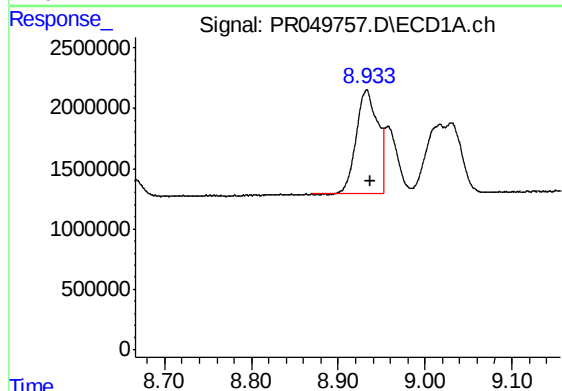


#38 AR-1262-3

R.T.: 8.933 min
Delta R.T.: -0.004 min
Response: 14733696
Conc: 44.80 ng/ml

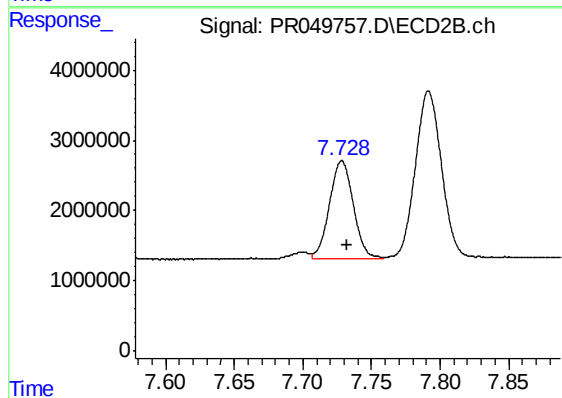

#38 AR-1262-3


R.T.: 7.728 min
Delta R.T.: -0.004 min
Response: 16891870
Conc: 46.91 ng/ml

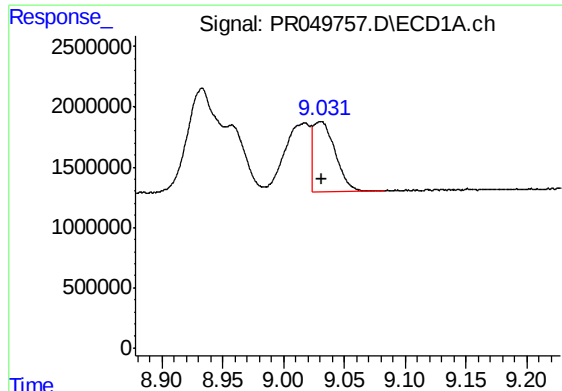

#39 AR-1262-4


R.T.: 9.030 min
Delta R.T.: 0.000 min
Response: 7241794
Conc: 29.32 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

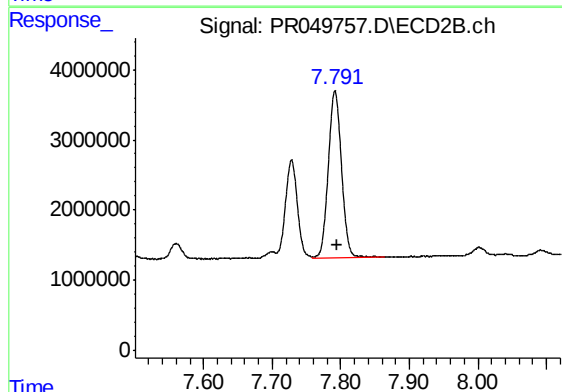


#39 AR-1262-4

R.T.: 7.792 min
Delta R.T.: -0.003 min
Response: 31999441
Conc: 44.70 ng/ml

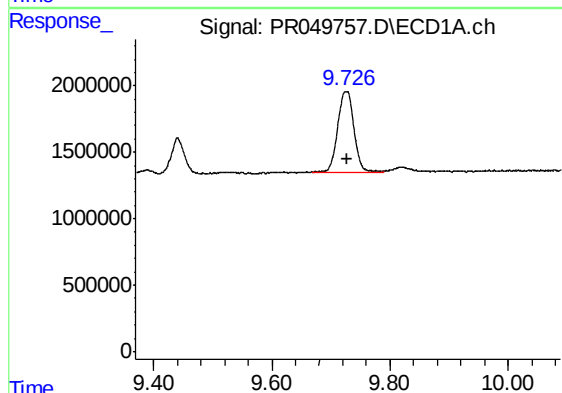


#40 AR-1262-5

R.T.: 9.726 min
Delta R.T.: -0.002 min
Response: 11475829
Conc: 63.69 ng/ml

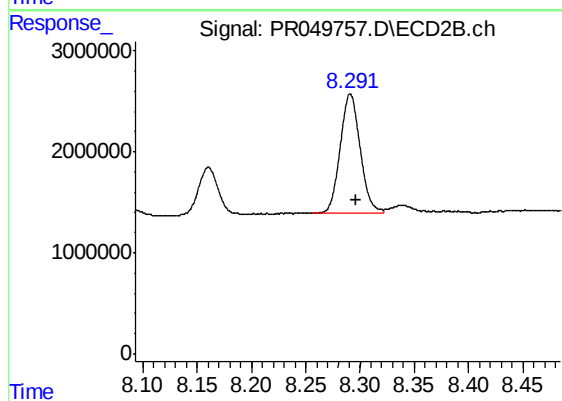

#40 AR-1262-5


R.T.: 8.291 min
Delta R.T.: -0.005 min
Response: 15077823
Conc: 46.91 ng/ml

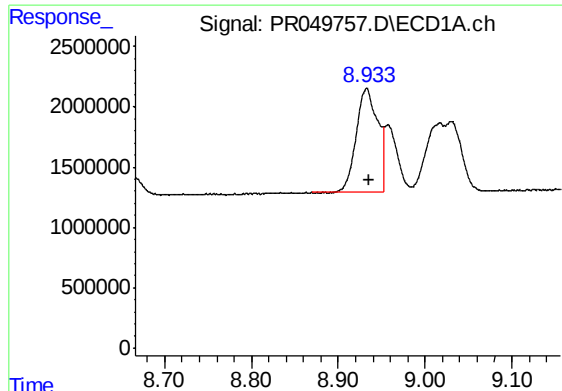

#41 AR-1268-1


R.T.: 8.933 min
Delta R.T.: -0.003 min
Response: 14733696
Conc: 25.12 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

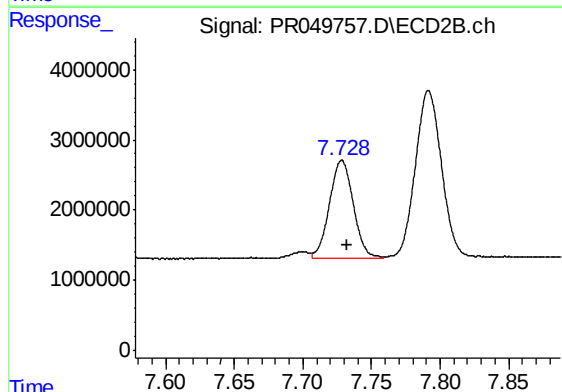


#41 AR-1268-1

R.T.: 7.728 min
Delta R.T.: -0.004 min
Response: 16891870
Conc: 15.06 ng/ml

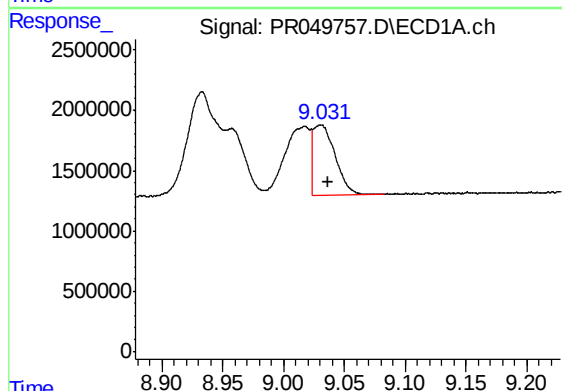


#42 AR-1268-2

R.T.: 9.030 min
Delta R.T.: -0.006 min
Response: 7241794
Conc: 13.45 ng/ml

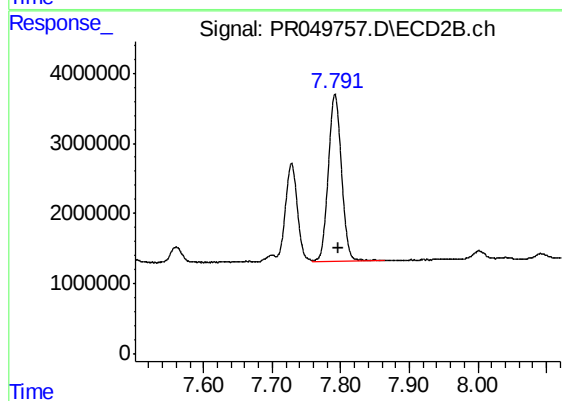

#42 AR-1268-2


R.T.: 7.792 min
Delta R.T.: -0.005 min
Response: 31999441
Conc: 30.24 ng/ml

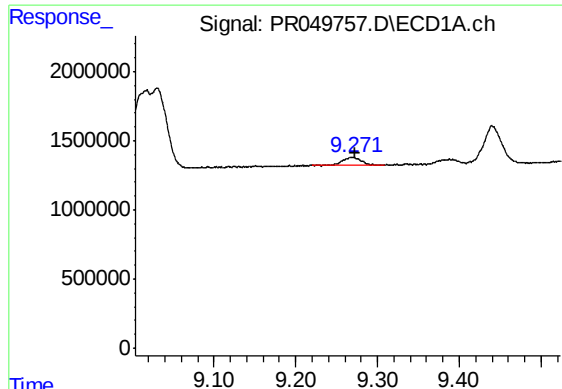

#43 AR-1268-3


R.T.: 9.270 min
Delta R.T.: -0.002 min
Response: 998022
Conc: 2.18 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

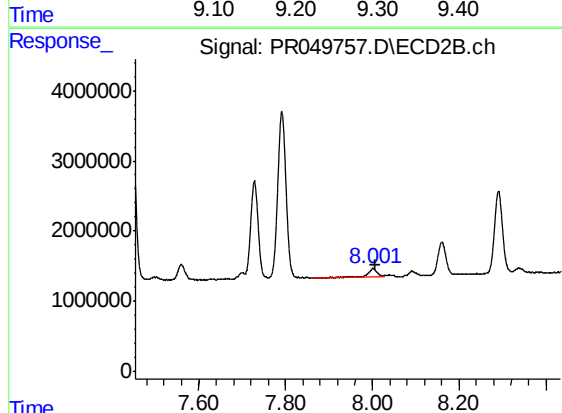


#43 AR-1268-3

R.T.: 8.002 min
Delta R.T.: -0.005 min
Response: 2503081
Conc: 2.86 ng/ml

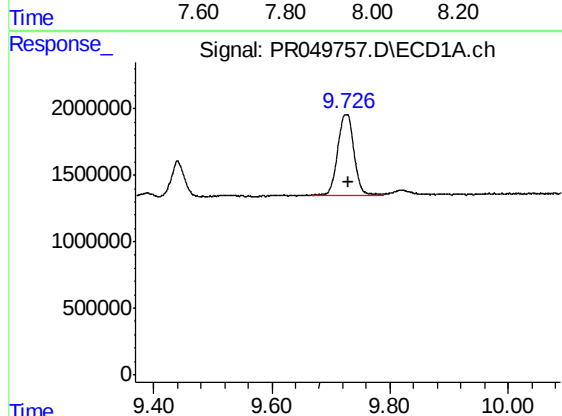


#44 AR-1268-4

R.T.: 9.726 min
Delta R.T.: -0.003 min
Response: 11475829
Conc: 56.82 ng/ml

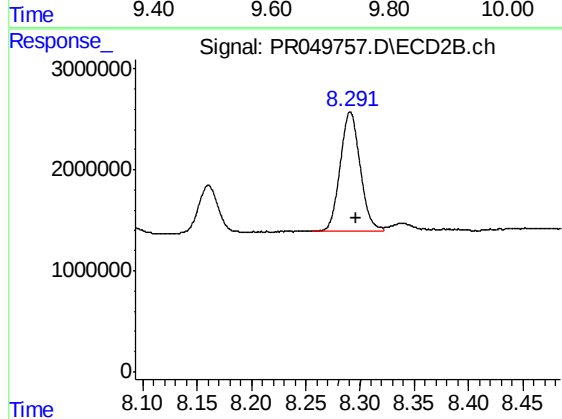

#44 AR-1268-4


R.T.: 8.291 min
Delta R.T.: -0.006 min
Response: 15077823
Conc: 41.41 ng/ml

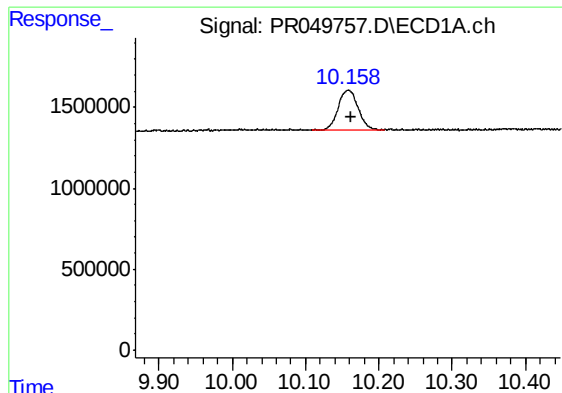

#45 AR-1268-5

R.T.: 10.159 min
Delta R.T.: -0.003 min
Response: 4625923
Conc: 2.83 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

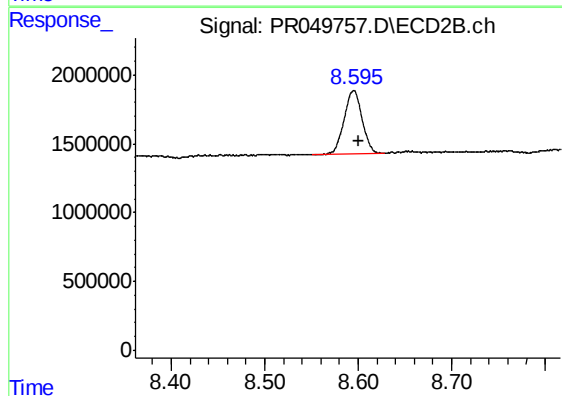

#45 AR-1268-5

R.T.: 8.595 min
Delta R.T.: -0.005 min
Response: 6302747
Conc: 2.07 ng/ml