

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040823\
 Data File : PR060716.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2023 16:20
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 01:47:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 07 15:47:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.687	2.901	54948325	73844240	17.999	17.351
2) SA Decachlor...	9.661	8.128	58033414	81541937	20.458	18.757

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR040823\
Data File : PR060716.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2023 16:20
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 01:47:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040823.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 07 15:47:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

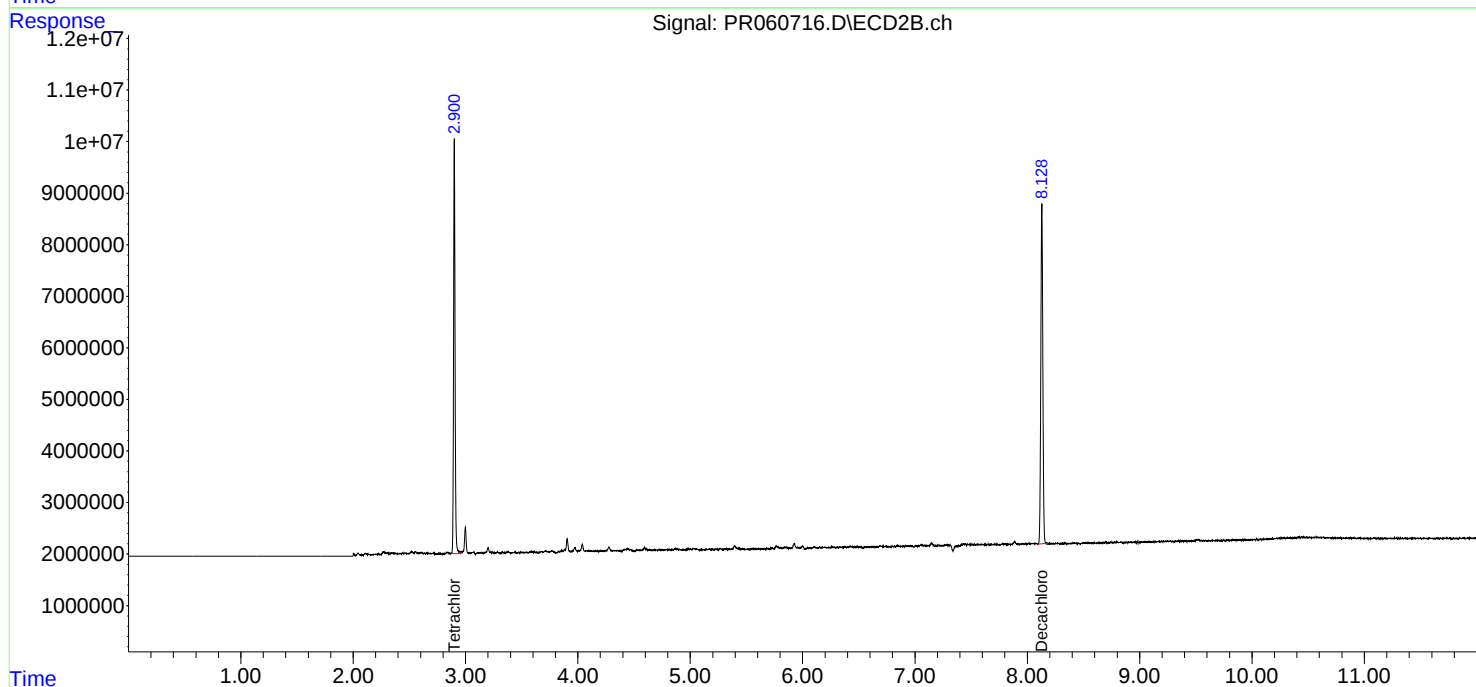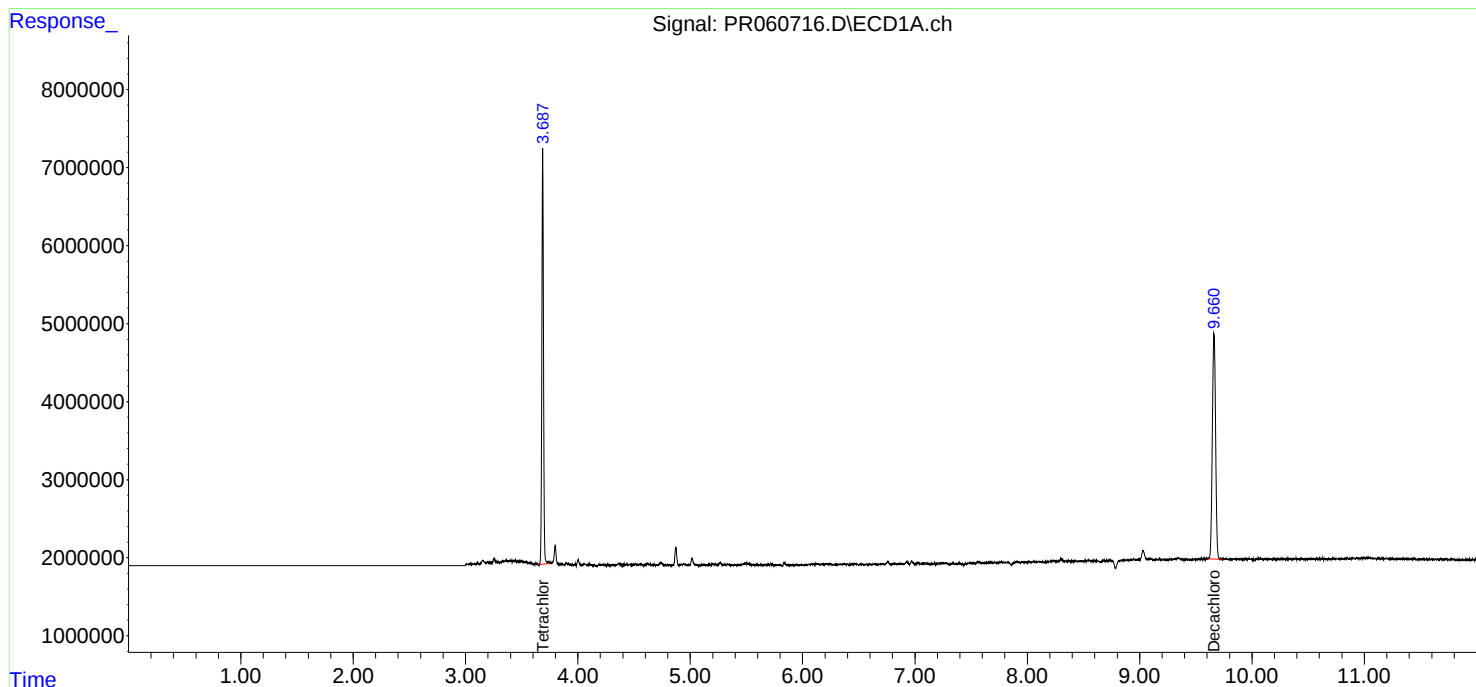


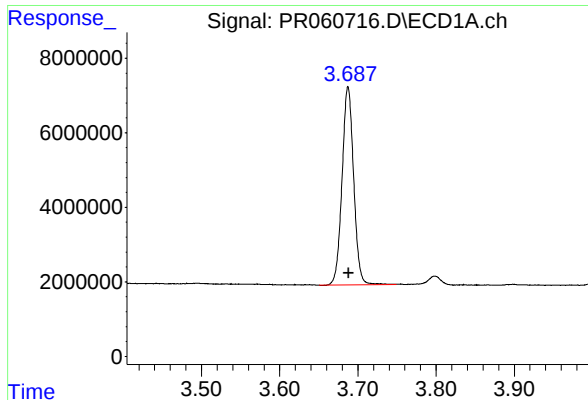

#1 Tetrachloro-m-xylene


R.T.: 3.687 min
Delta R.T.: 0.000 min
Response: 54948325
Conc: 18.00 ng/ml

Instrument :
ECD_R
ClientSampleId :
I.BLK

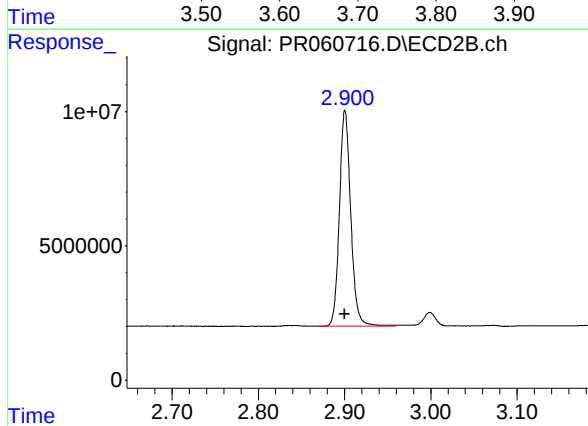


#1 Tetrachloro-m-xylene

R.T.: 2.901 min
Delta R.T.: 0.000 min
Response: 73844240
Conc: 17.35 ng/ml

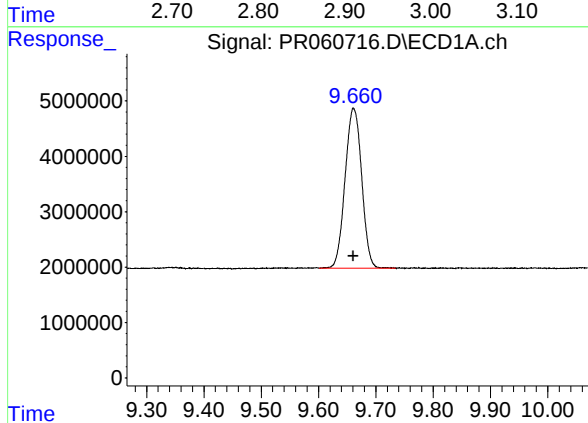

#2 Decachlorobiphenyl

R.T.: 9.661 min
Delta R.T.: 0.000 min
Response: 58033414
Conc: 20.46 ng/ml

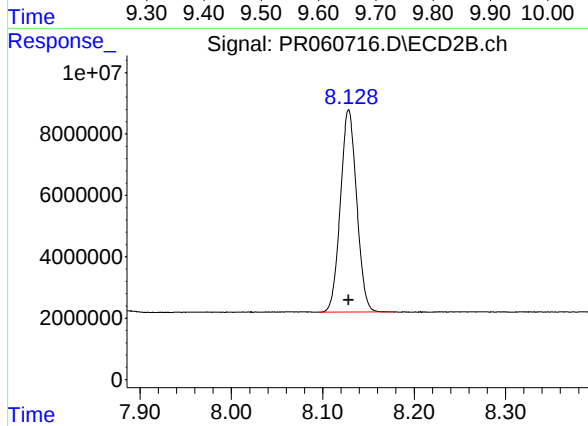

#2 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.000 min
Response: 81541937
Conc: 18.76 ng/ml