

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042021\
 Data File : PR049994.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2021 12:02
 Operator : DD\AJ
 Sample : M2031-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1



Instrument :
 ECD_R
 ClientSampleId :
 BG539

Manual Integrations
 APPROVED

Ankita
 4/22/2021 11:54:42 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 02:49:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040621CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 07 06:22:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

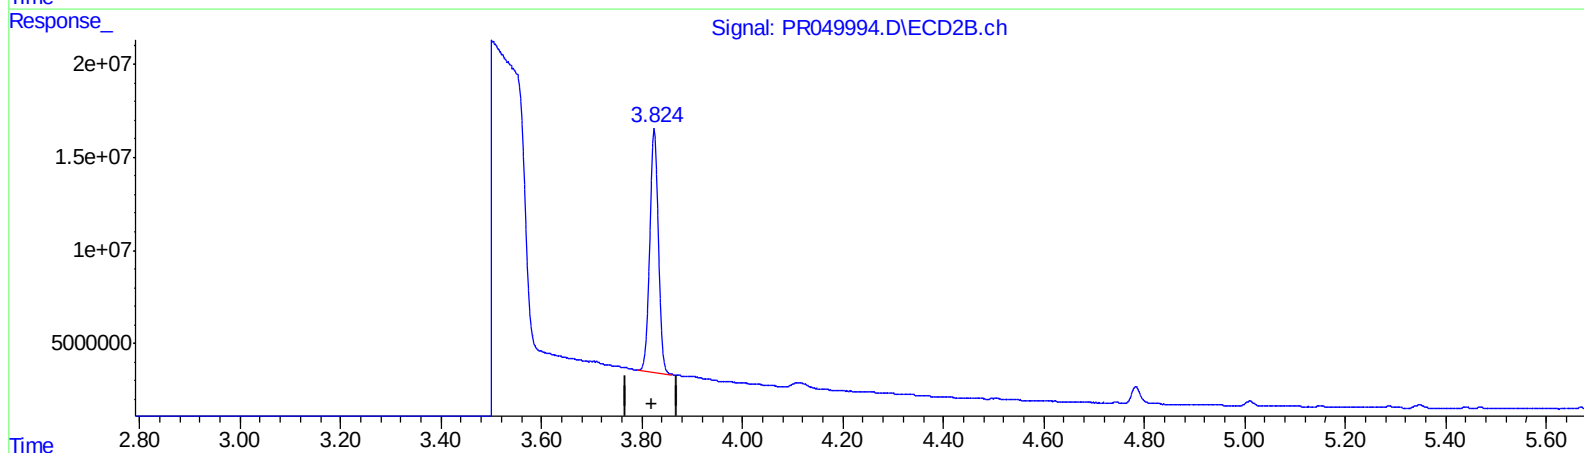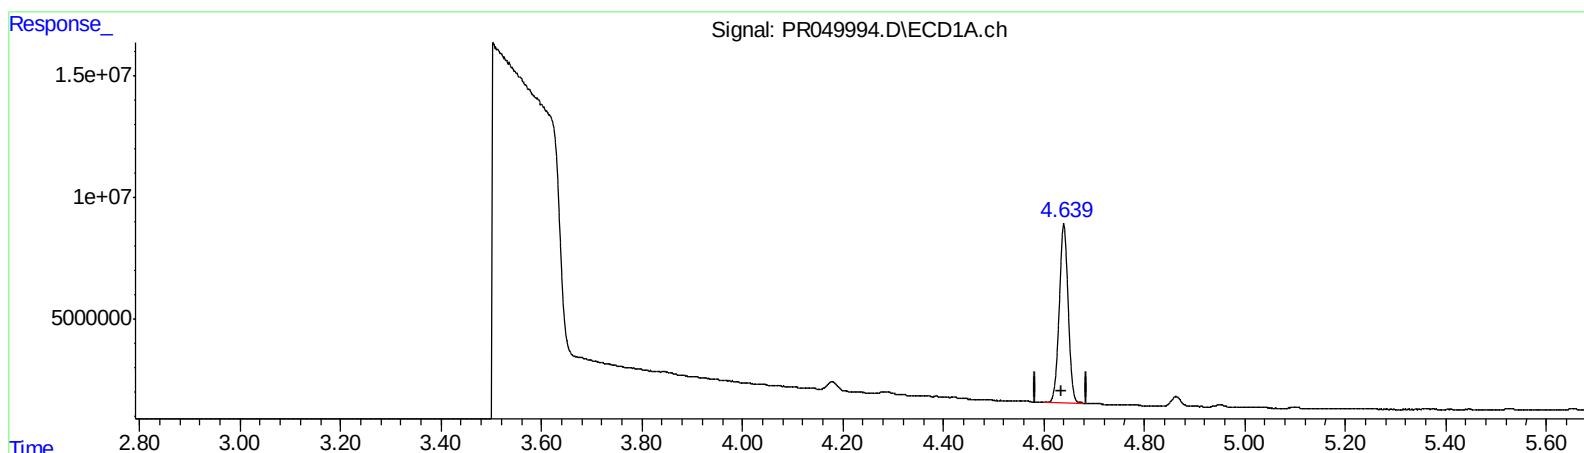

QEdit

(1) Tetrachloro-m-xylene (SA)

4.640min 20.202 ng/ml

response 89875300

(1) Tetrachloro-m-xylene #2 (SA)

3.824min 21.076 ng/ml m

response 155535401

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042021\
Data File : PR049994.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2021 12:02
Operator : DD\AJ
Sample : M2031-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
BG539

Manual Integrations
APPROVED

Ankita
4/22/2021 11:54:42 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 02:49:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR040621CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 07 06:22:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.640	3.824	89875300	155.5E6	20.202	21.076m
2) SA Decachlor...	10.509	8.852	181.4E6	259.0E6	27.488	30.996

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

AJ
04/26/21