

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042121\
 Data File : PL066415.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2021 20:41
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 06:07:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	4.155	61414022	80620046	24.129	20.042
28)	SA Decachlor...	8.168	9.355	43626287	59976444	18.290	18.364
Target Compounds							
2)	A alpha-BHC	3.881	0.000	7925431	0	1.926	N.D. #
4)	MA Heptachlor	4.438f	5.354	1206928	2321543	0.291	0.417 #
8)	B Heptachlo...	0.000	6.070	0	3253969	N.D.	0.704 #
14)	MA Endrin	5.978	0.000	5677824	0	1.628	N.D. #
15)	B Endosulfa...	6.229	7.129	21398859	1739422	6.517	0.499 #
17)	MA 4,4'-DDT	6.336	7.348	2356568	773162	0.739	0.228 #
18)	B Endrin al...	0.000	7.249	0	1784751	N.D.	0.638 #
21)	B Endrin ke...	0.000	7.974	0	1268442	N.D.	0.345 #
27)	Chlordane-5	6.229f	0.000	21398859	0	151.462	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042121\
Data File : PL066415.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2021 20:41
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 06:07:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

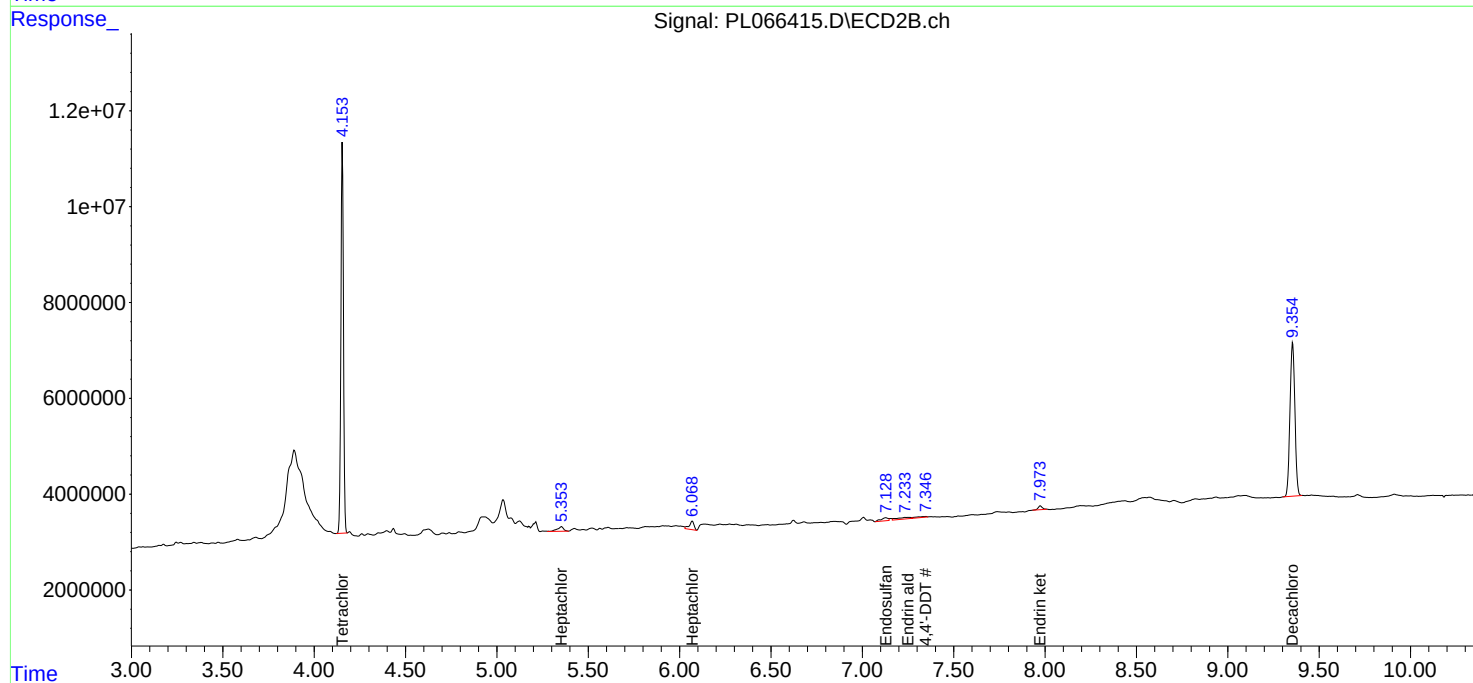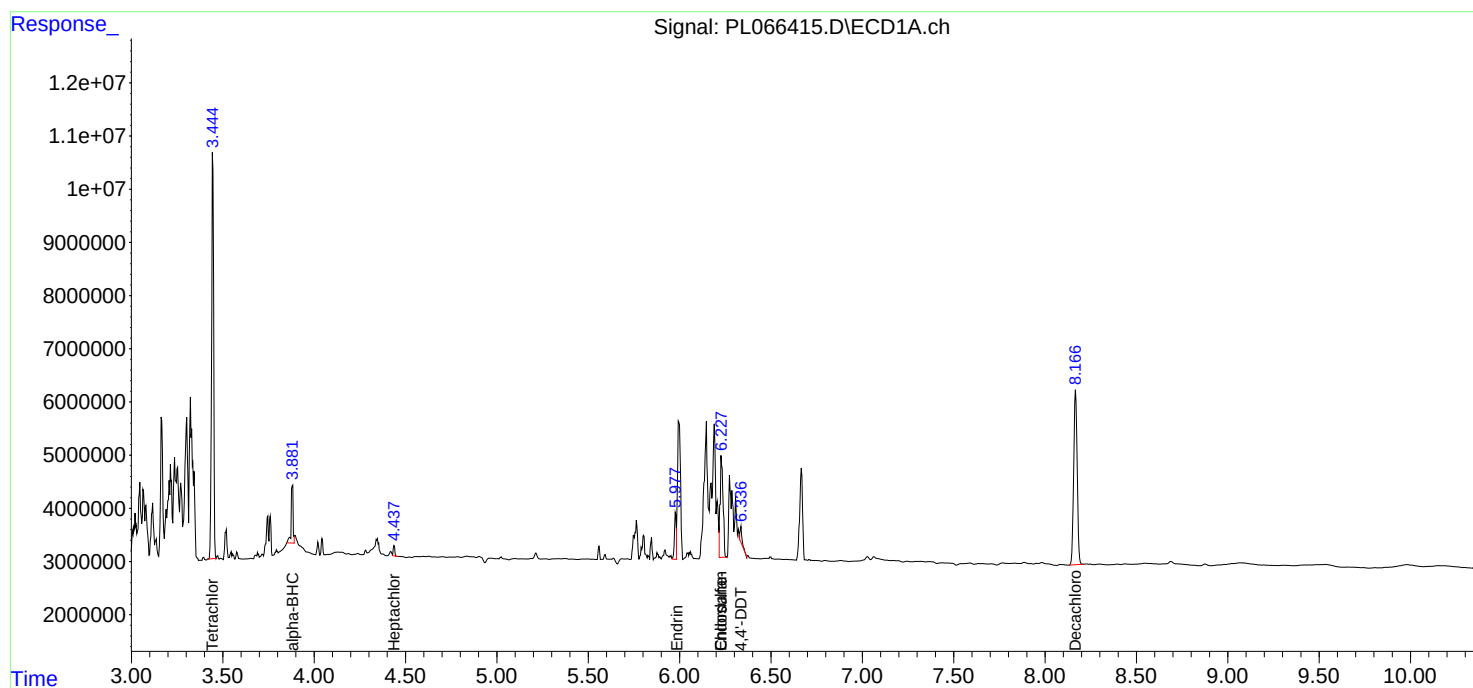


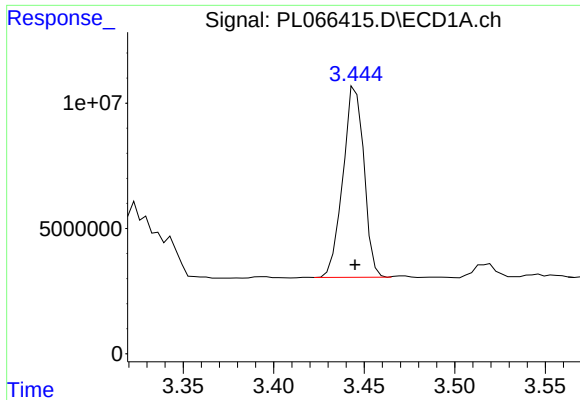

#1 Tetrachloro-m-xylene


R.T.: 3.446 min
Delta R.T.: 0.000 min
Response: 61414022
Conc: 24.13 ng/ml

Instrument :
ECD_R
ClientSampleId :

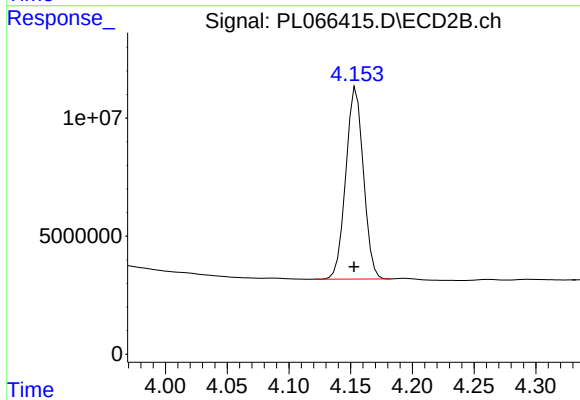


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.002 min
Response: 80620046
Conc: 20.04 ng/ml

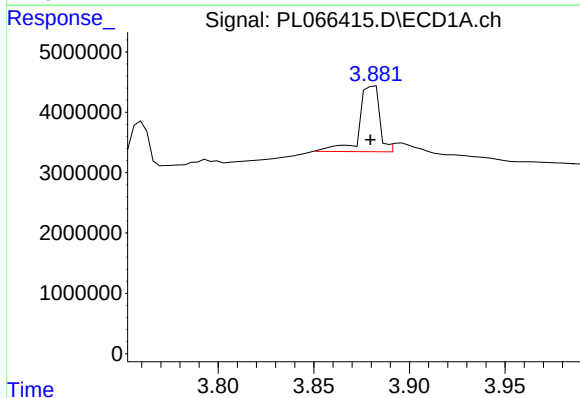


#2 alpha-BHC

R.T.: 3.881 min
Delta R.T.: 0.001 min
Response: 7925431
Conc: 1.93 ng/ml

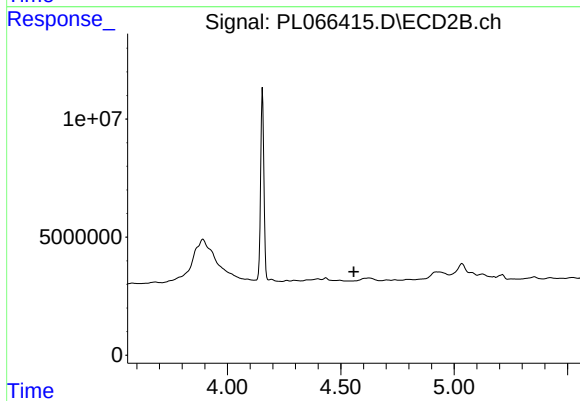

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.558 min
Response: 0
Conc: N.D.

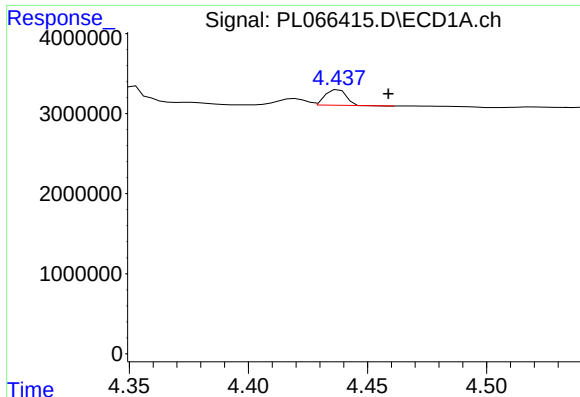

#4 Heptachlor


R.T.: 4.438 min
Delta R.T.: -0.021 min
Response: 1206928
Conc: 0.29 ng/ml

Instrument :
ECD_R
ClientSampleId :

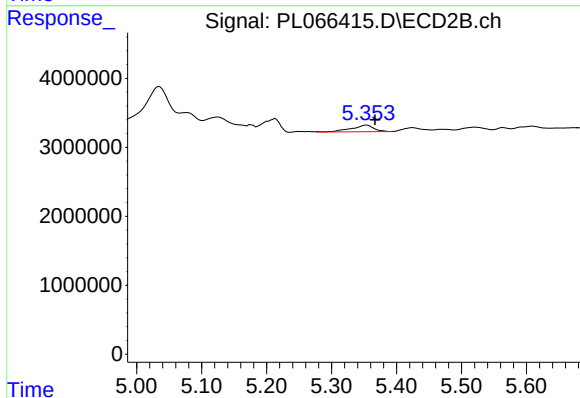


#4 Heptachlor

R.T.: 5.354 min
Delta R.T.: -0.013 min
Response: 2321543
Conc: 0.42 ng/ml

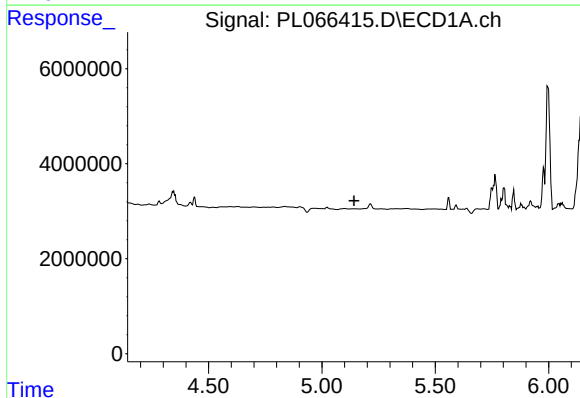


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.143 min
Response: 0
Conc: N.D.

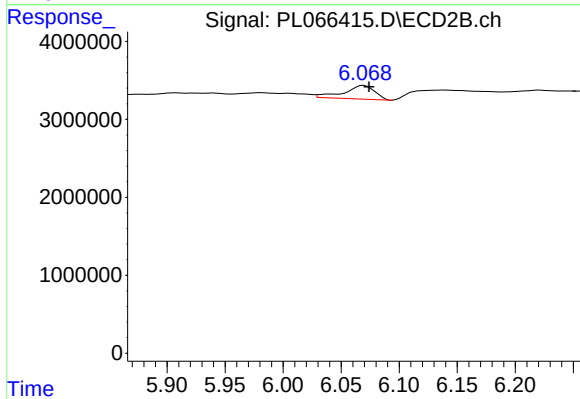

#8 Heptachlor epoxide


R.T.: 6.070 min
Delta R.T.: -0.004 min
Response: 3253969
Conc: 0.70 ng/ml

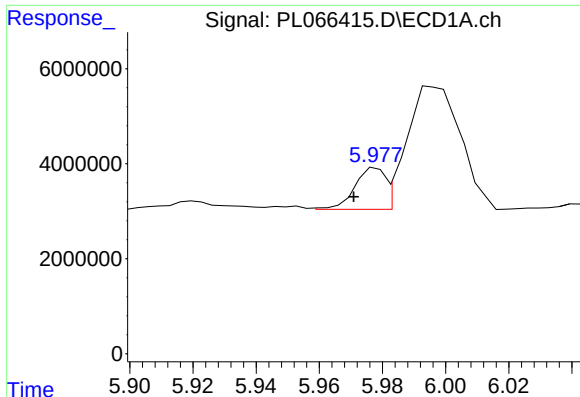

#14 Endrin


R.T.: 5.978 min
Delta R.T.: 0.008 min
Response: 5677824
Conc: 1.63 ng/ml

Instrument :
ECD_R
ClientSampleId :

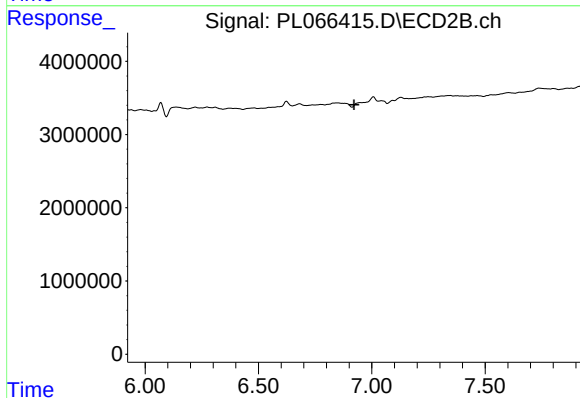


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

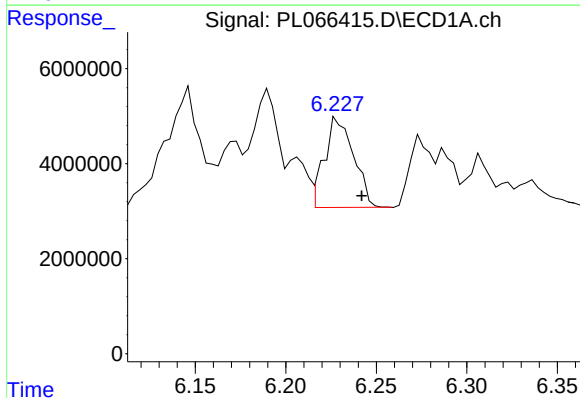


#15 Endosulfan II

R.T.: 6.229 min
Delta R.T.: -0.013 min
Response: 21398859
Conc: 6.52 ng/ml

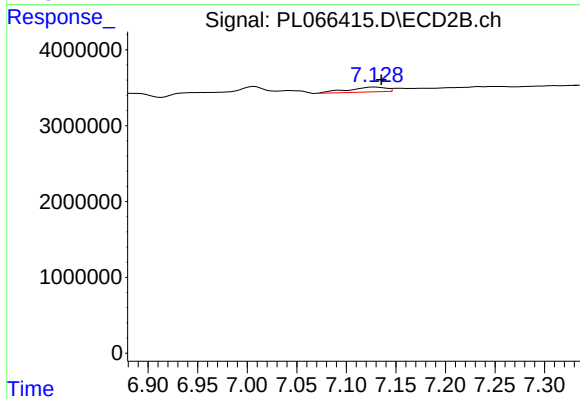

#15 Endosulfan II


R.T.: 7.129 min
Delta R.T.: -0.006 min
Response: 1739422
Conc: 0.50 ng/ml

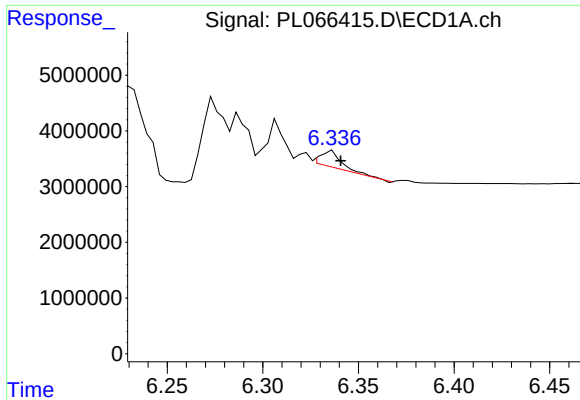

#17 4,4'-DDT


R.T.: 6.336 min
Delta R.T.: -0.005 min
Response: 2356568
Conc: 0.74 ng/ml

Instrument :
ECD_R
ClientSampleId :

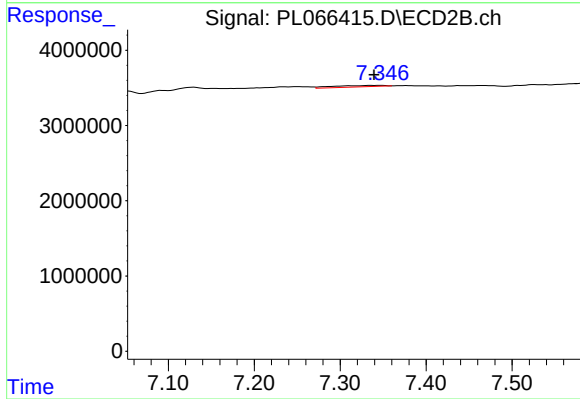


#17 4,4'-DDT

R.T.: 7.348 min
Delta R.T.: 0.009 min
Response: 773162
Conc: 0.23 ng/ml

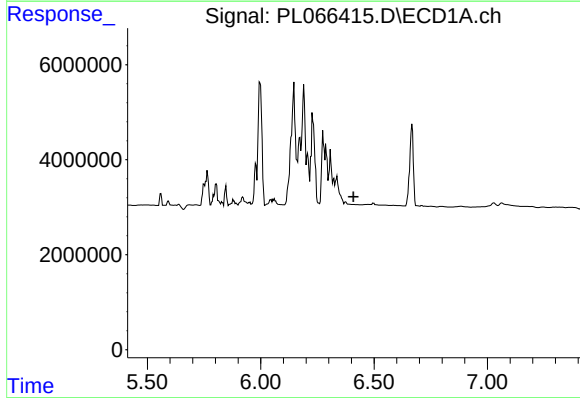


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.409 min
Response: 0
Conc: N.D.

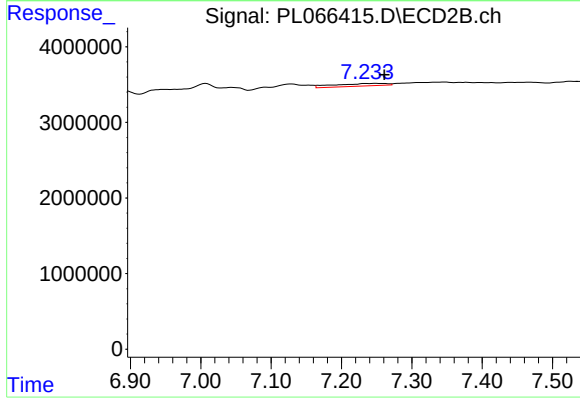

#18 Endrin aldehyde


R.T.: 7.249 min
Delta R.T.: -0.012 min
Response: 1784751
Conc: 0.64 ng/ml

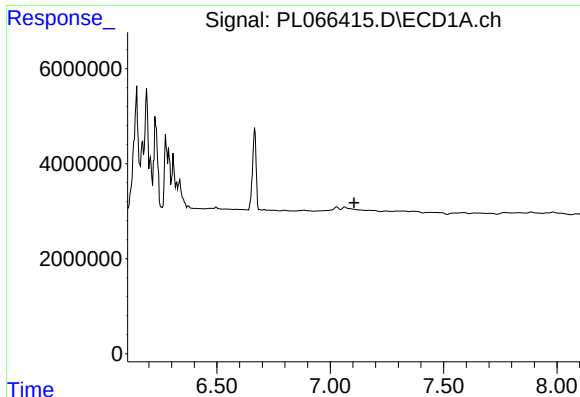

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.105 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :

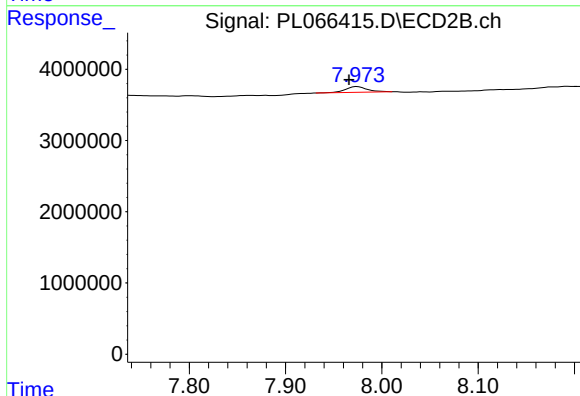


#21 Endrin ketone

R.T.: 7.974 min
Delta R.T.: 0.008 min
Response: 1268442
Conc: 0.34 ng/ml

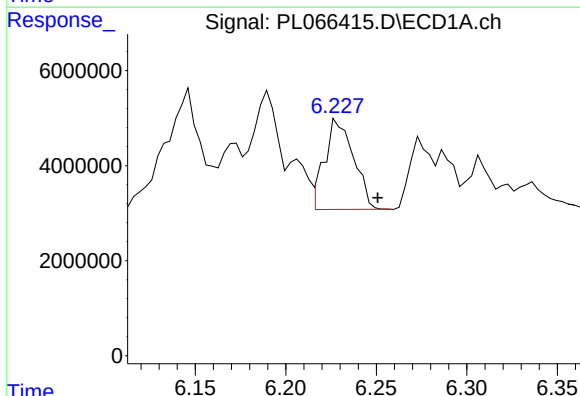


#27 Chlordane-5

R.T.: 6.229 min
Delta R.T.: -0.022 min
Response: 21398859
Conc: 151.46 ng/ml

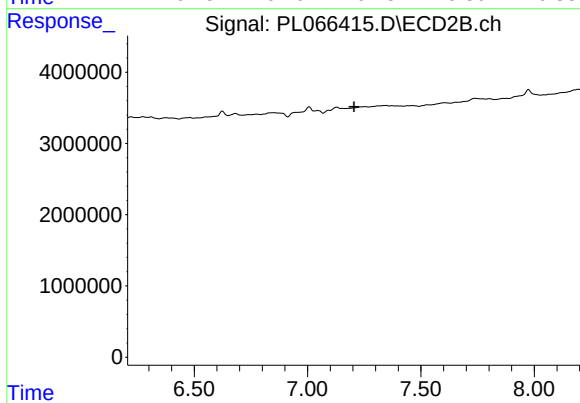

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 7.206 min
Response: 0
Conc: N.D.

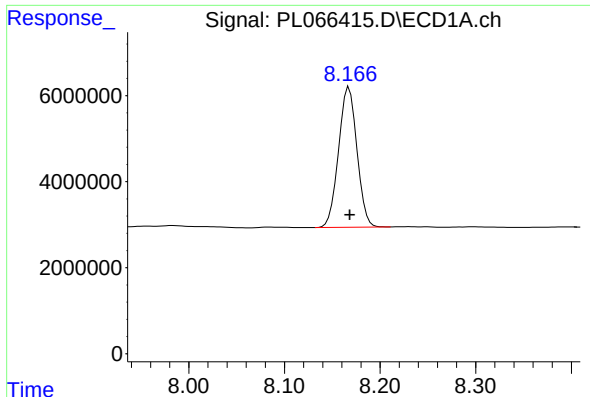

#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.000 min
Response: 43626287
Conc: 18.29 ng/ml

Instrument :
ECD_R
ClientSampleId :

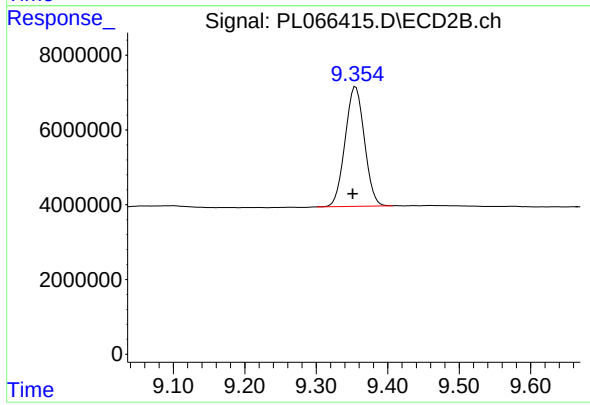

#28 Decachlorobiphenyl

R.T.: 9.355 min
Delta R.T.: 0.004 min
Response: 59976444
Conc: 18.36 ng/ml