

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042121\
 Data File : PS014746.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2021 21:08
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 04:48:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.157	6.883	691.5E6	254.8E6	454.586	547.509
Target Compounds							
7) T	MCPA	7.610f	0.000	9441589	0	1.517	N.D. #
8) T	DICHLORPROP	0.000	7.704	0	7112410	N.D.	14.089
11) T	2,4,5-TP ...	0.000	8.728	0	3908209	N.D.	1.431
12) T	2,4,5-T	0.000	9.204f	0	4803829	N.D.	1.837
13) T	2,4-DB	9.981	9.659	19233155	2189897	12.639	6.313 #
15) T	Picloram	10.932	10.964	74860828	27999779	6.691	7.467
16) T	DCPA	11.422f	10.888	-4638778	1718896	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042121\
Data File : PS014746.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2021 21:08
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 04:48:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

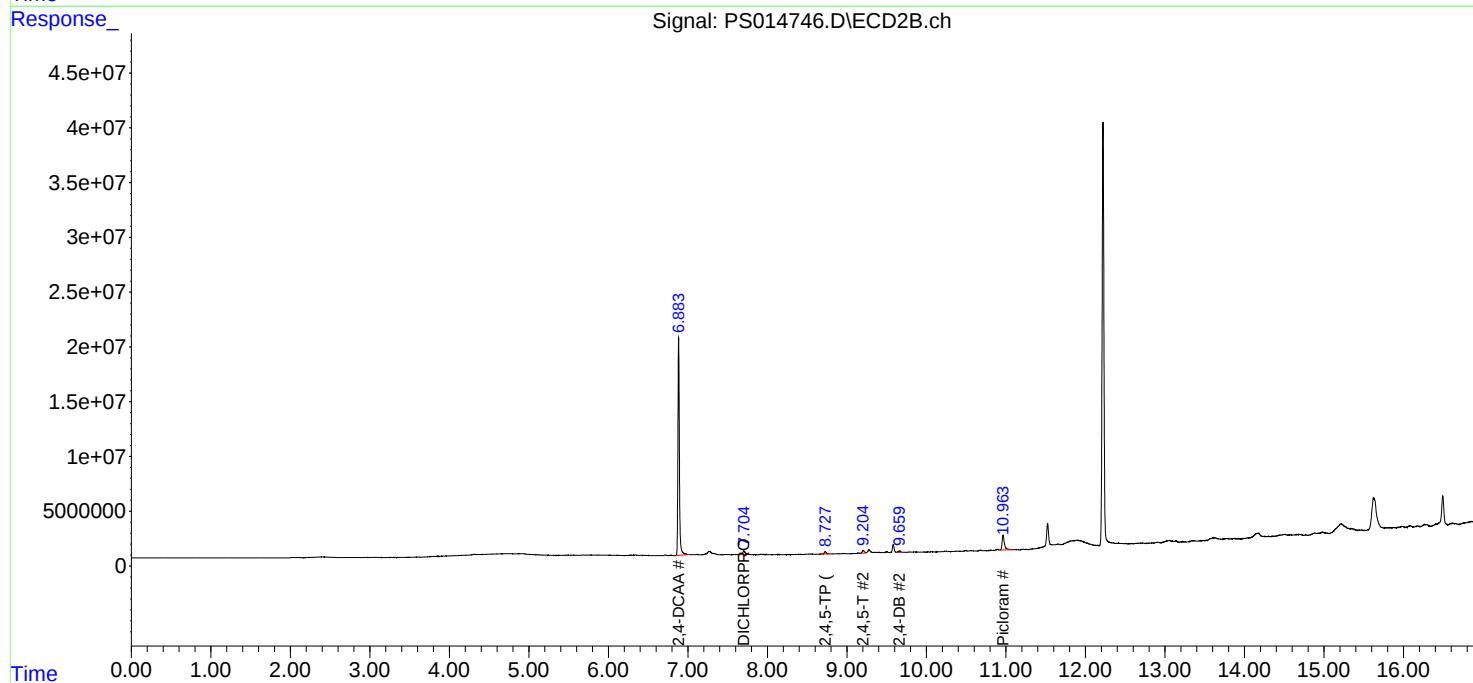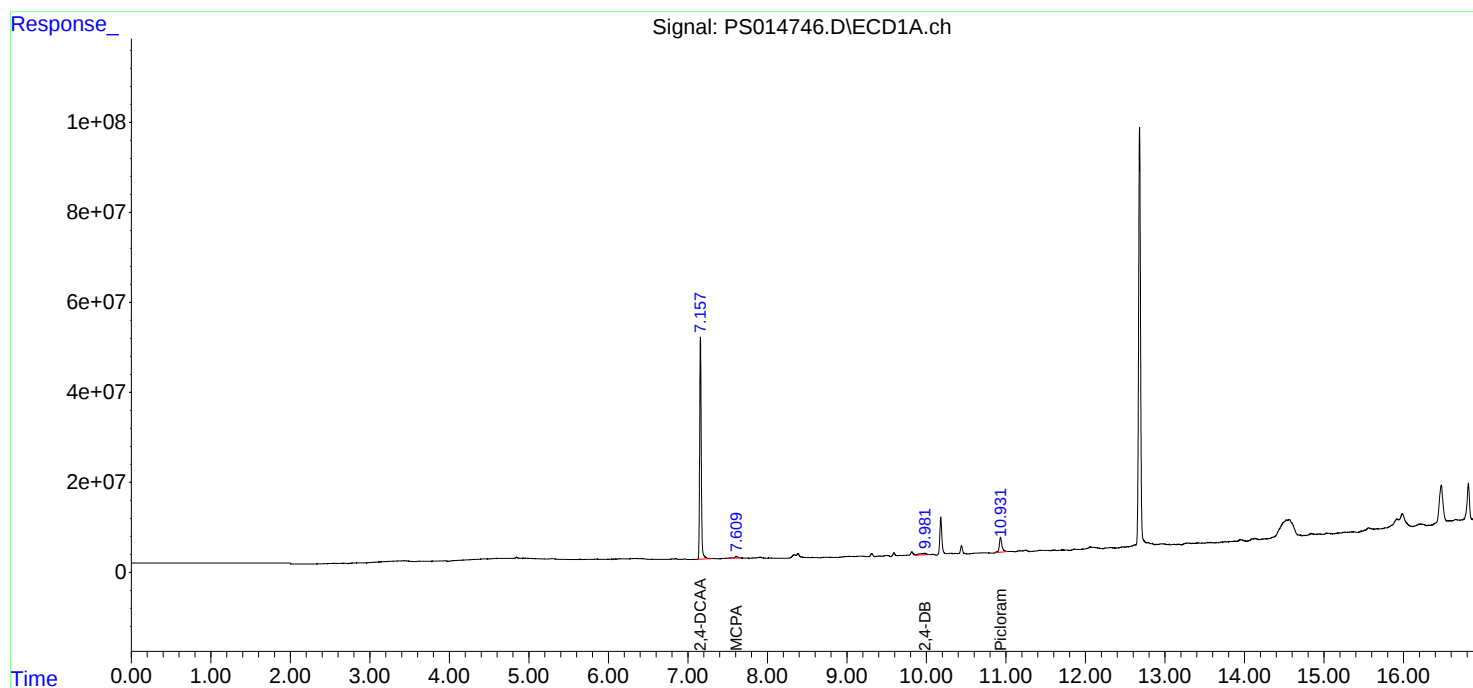


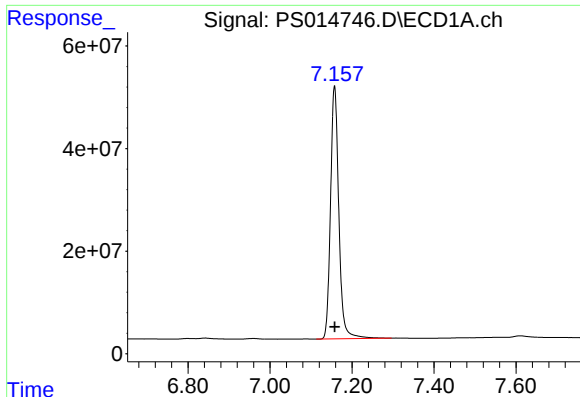

#4 2,4-DCAA


R.T.: 7.157 min
Delta R.T.: 0.000 min
Response: 691514794
Conc: 454.59 ng/ml

Instrument :
ECD_R
ClientSampleId :

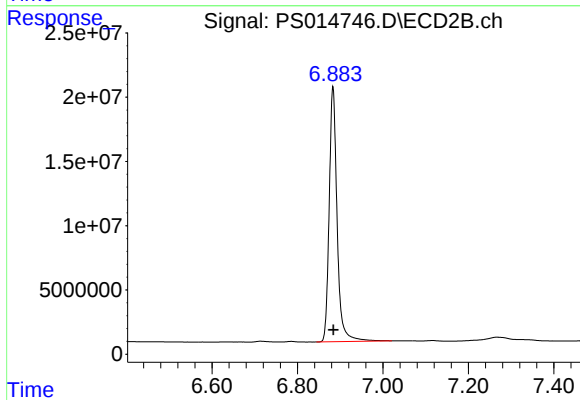


#4 2,4-DCAA

R.T.: 6.883 min
Delta R.T.: 0.000 min
Response: 254840576
Conc: 547.51 ng/ml

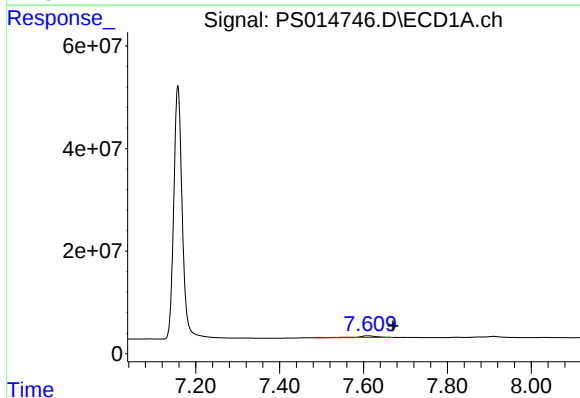


#7 MCPA

R.T.: 7.610 min
Delta R.T.: -0.060 min
Response: 9441589
Conc: 1.52 ug/ml

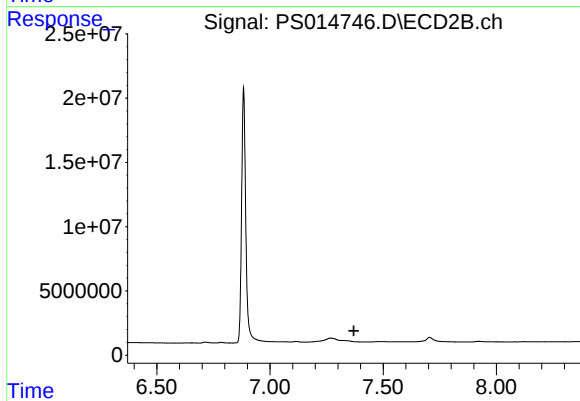

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.370 min
Response: 0
Conc: N.D.

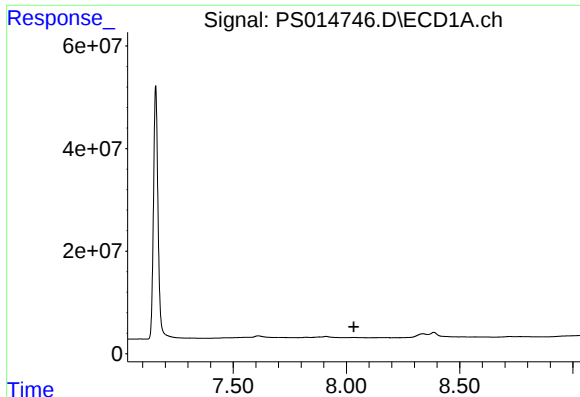

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :

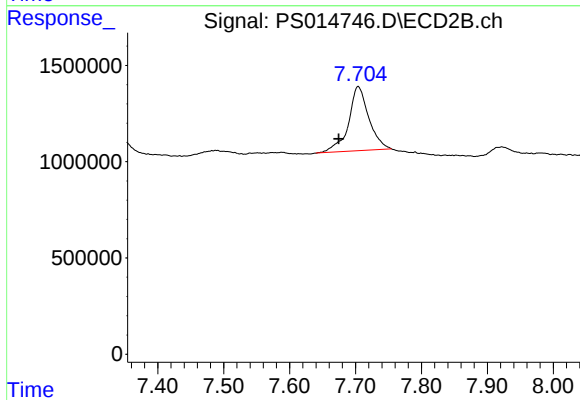


#8 DICHLORPROP

R.T.: 7.704 min
Delta R.T.: 0.029 min
Response: 7112410
Conc: 14.09 ng/ml

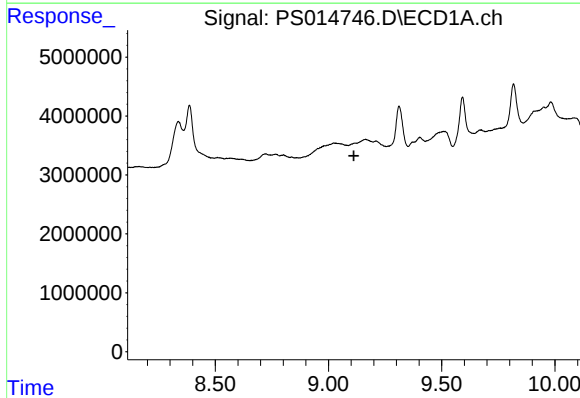


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.112 min
Response: 0
Conc: N.D.

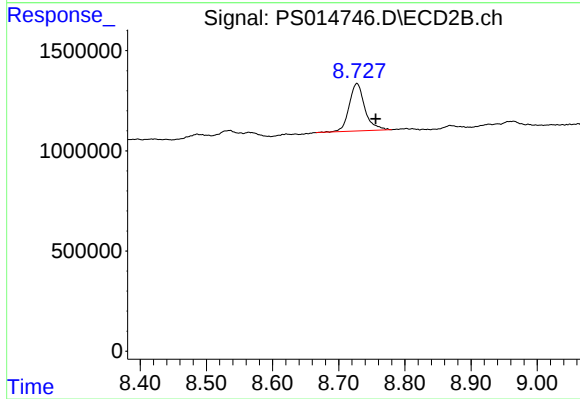

#11 2,4,5-TP (SILVEX)


R.T.: 8.728 min
Delta R.T.: -0.029 min
Response: 3908209
Conc: 1.43 ng/ml

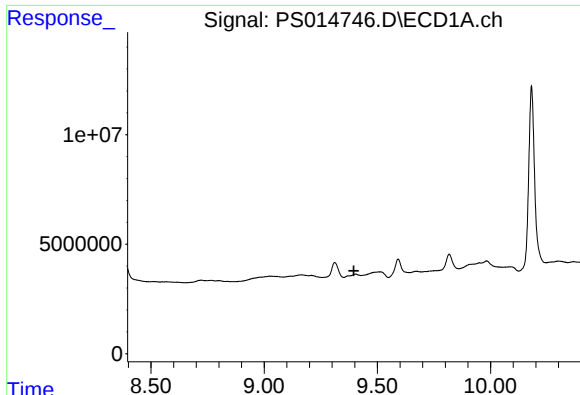

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :

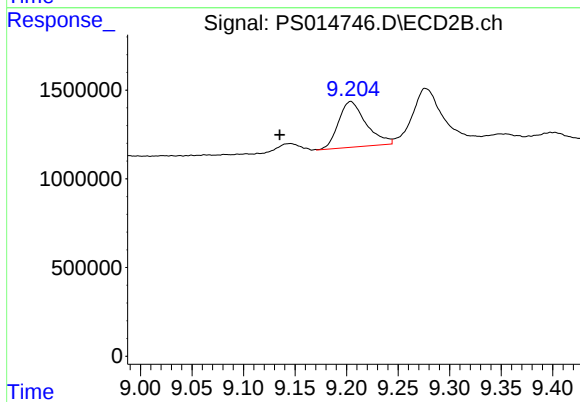


#12 2,4,5-T

R.T.: 9.204 min
Delta R.T.: 0.069 min
Response: 4803829
Conc: 1.84 ng/ml

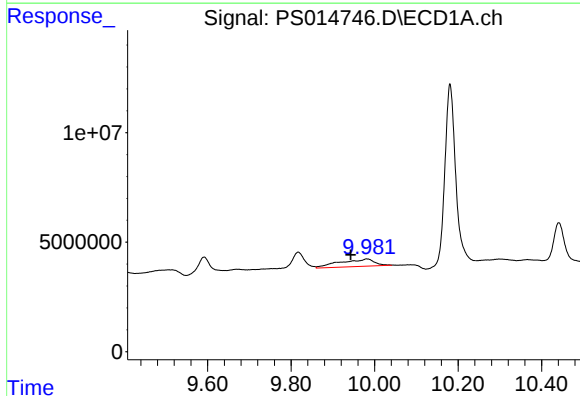


#13 2,4-DB

R.T.: 9.981 min
Delta R.T.: 0.038 min
Response: 19233155
Conc: 12.64 ng/ml

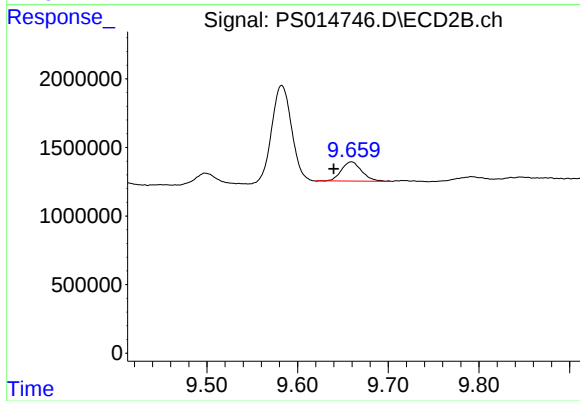

#13 2,4-DB


R.T.: 9.659 min
Delta R.T.: 0.020 min
Response: 2189897
Conc: 6.31 ng/ml

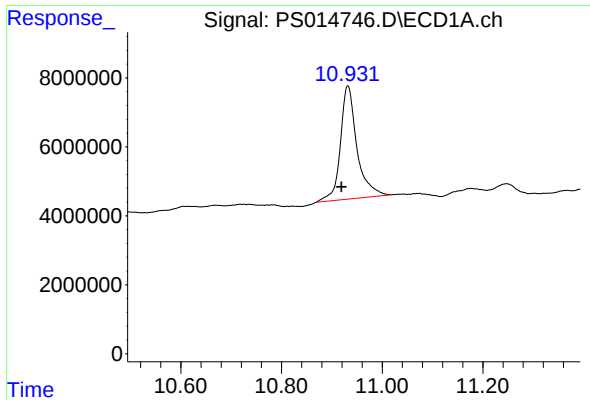

#15 Picloram

R.T.: 10.932 min
Delta R.T.: 0.013 min
Response: 74860828
Conc: 6.69 ng/ml

Instrument :
ECD_R
ClientSampleId :

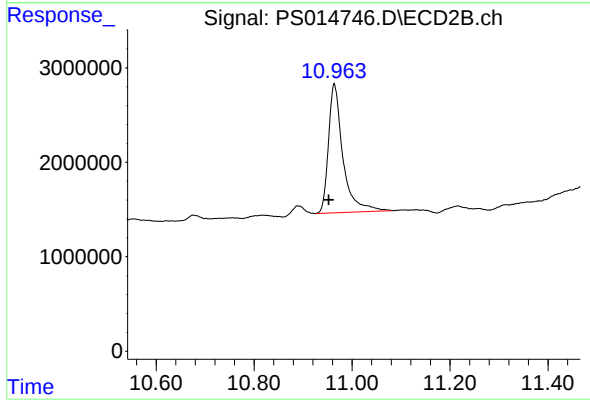

#15 Picloram

R.T.: 10.964 min
Delta R.T.: 0.011 min
Response: 27999779
Conc: 7.47 ng/ml