

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042121\
 Data File : PS014750.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2021 22:40
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 04:50:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
 Quant Title : 8080.M
 QLast Update : Thu Apr 08 14:34:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.157	6.882	694.8E6	254.5E6	456.761	546.848
Target Compounds							
7) T	MCPA	7.608f	0.000	8260531	0	1.327	N.D. #
8) T	DICHLORPROP	0.000	7.704	0	6340205	N.D.	12.559
11) T	2,4,5-TP ...	0.000	8.727	0	3971565	N.D.	1.454
12) T	2,4,5-T	0.000	9.203f	0	4913159	N.D.	1.878
13) T	2,4-DB	9.947	9.658	11511692	2409297	7.565	6.946
15) T	Picloram	10.931	10.964	81092566	26398785	7.248	7.040
16) T	DCPA	0.000	10.889	0	1936497	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042121\
Data File : PS014750.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2021 22:40
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 04:50:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS040821.M
Quant Title : 8080.M
QLast Update : Thu Apr 08 14:34:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

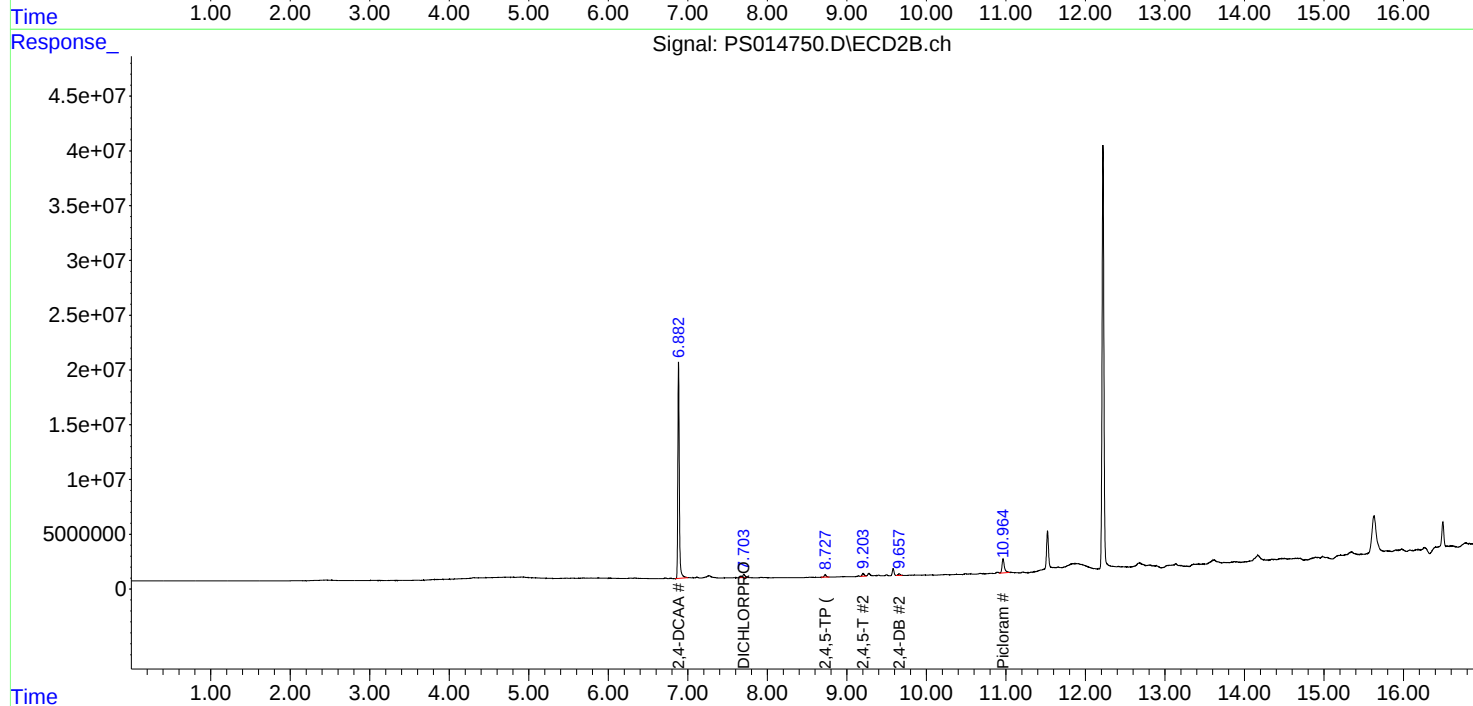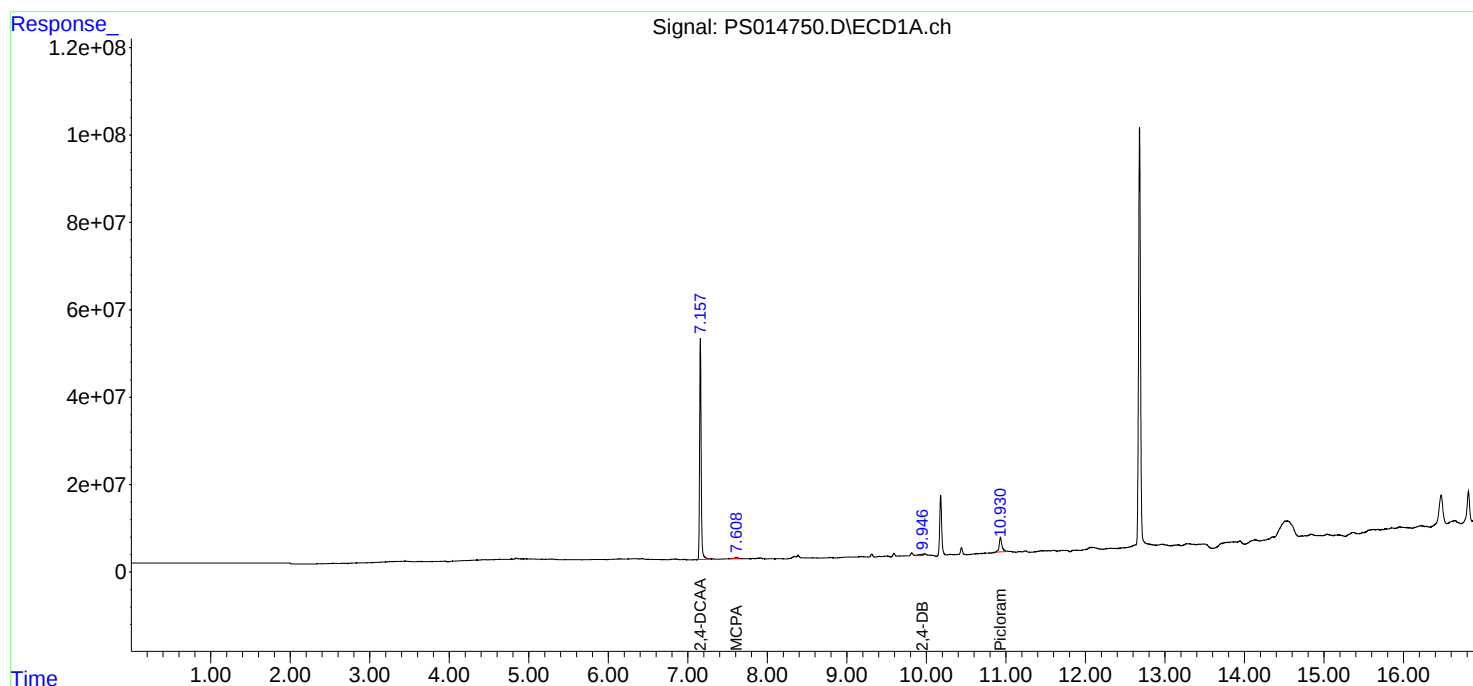


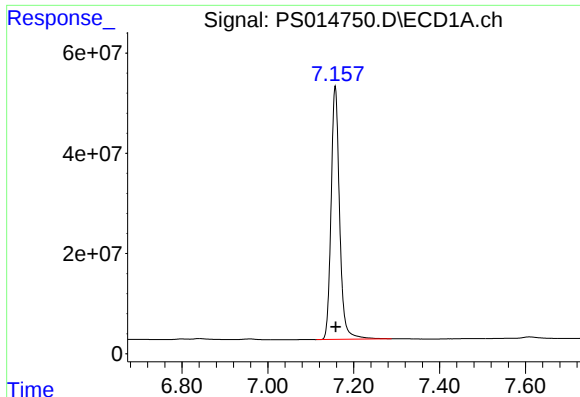

#4 2,4-DCAA


R.T.: 7.157 min
Delta R.T.: 0.000 min
Response: 694822457
Conc: 456.76 ng/ml

Instrument :
ECD_R
ClientSampleId :

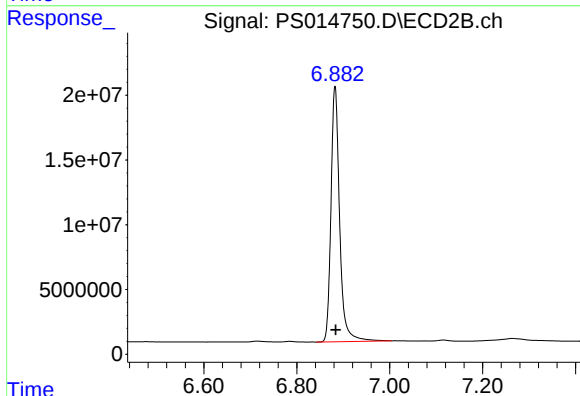


#4 2,4-DCAA

R.T.: 6.882 min
Delta R.T.: -0.001 min
Response: 254533096
Conc: 546.85 ng/ml

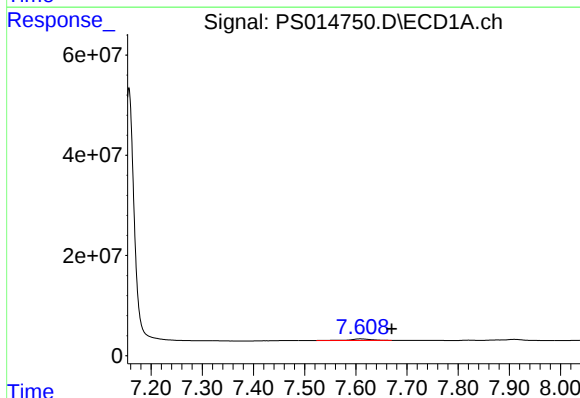


#7 MCPA

R.T.: 7.608 min
Delta R.T.: -0.062 min
Response: 8260531
Conc: 1.33 ug/ml

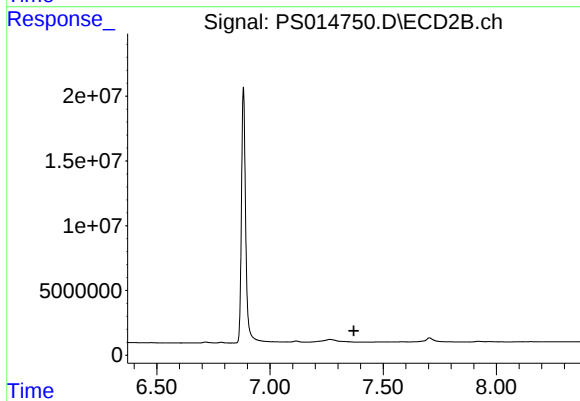

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.370 min
Response: 0
Conc: N.D.

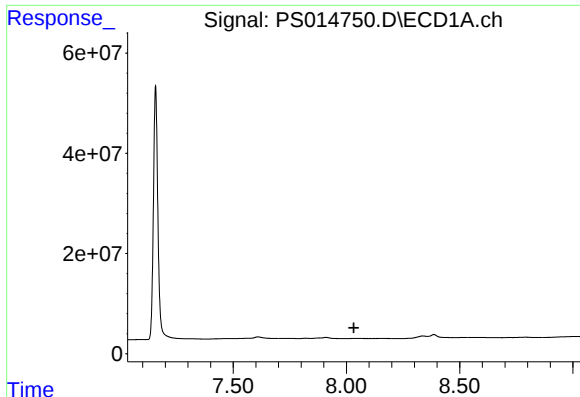

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :

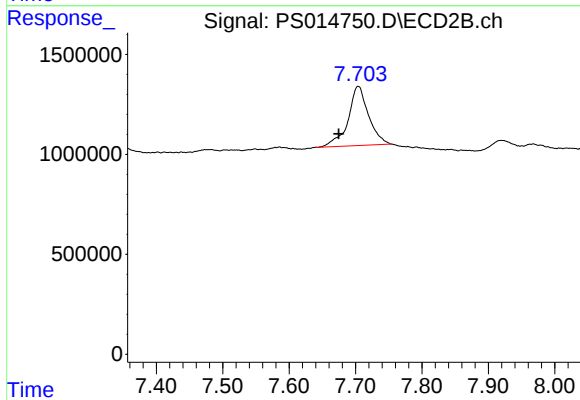


#8 DICHLORPROP

R.T.: 7.704 min
Delta R.T.: 0.029 min
Response: 6340205
Conc: 12.56 ng/ml

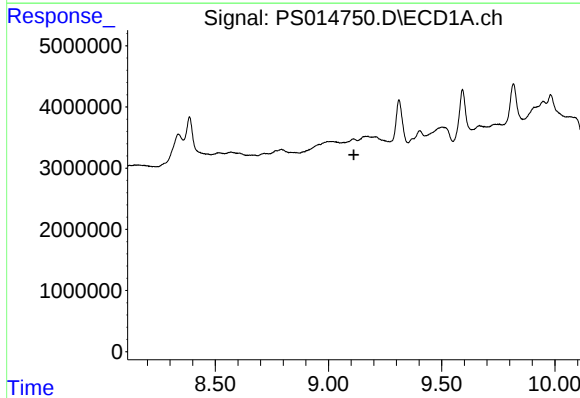


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.112 min
Response: 0
Conc: N.D.

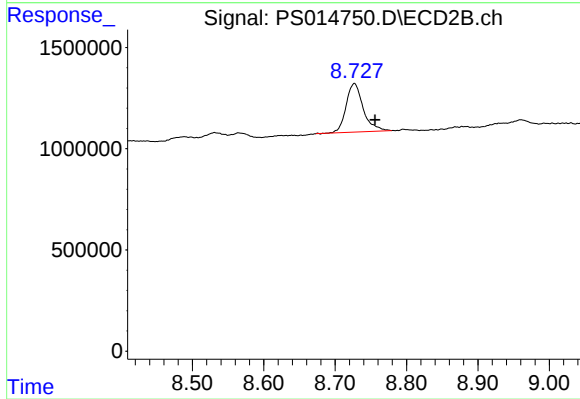

#11 2,4,5-TP (SILVEX)


R.T.: 8.727 min
Delta R.T.: -0.029 min
Response: 3971565
Conc: 1.45 ng/ml

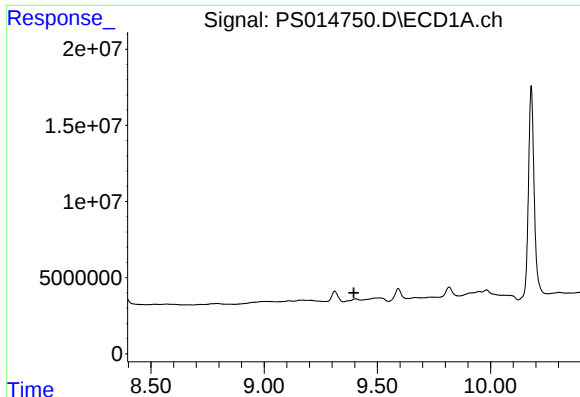

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :

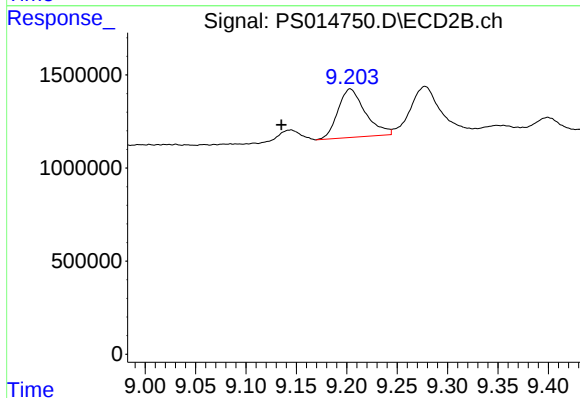


#12 2,4,5-T

R.T.: 9.203 min
Delta R.T.: 0.068 min
Response: 4913159
Conc: 1.88 ng/ml

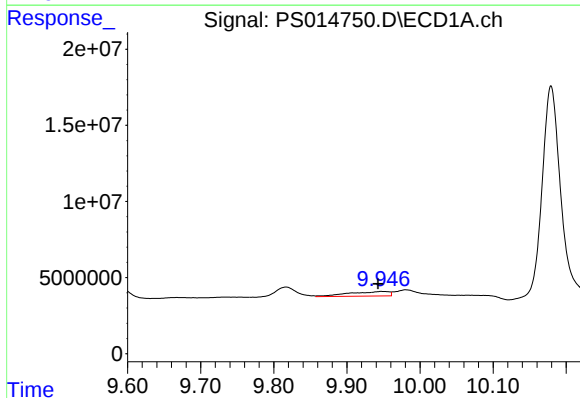


#13 2,4-DB

R.T.: 9.947 min
Delta R.T.: 0.004 min
Response: 11511692
Conc: 7.56 ng/ml

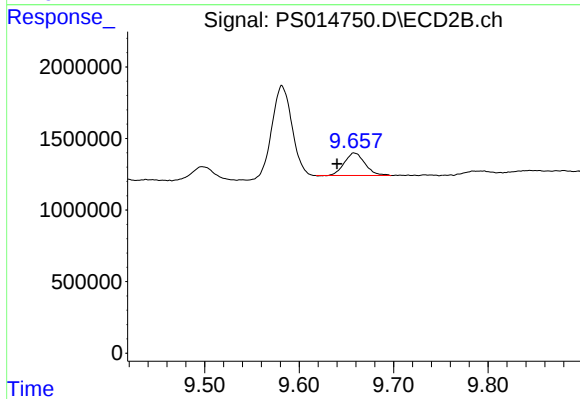

#13 2,4-DB


R.T.: 9.658 min
Delta R.T.: 0.018 min
Response: 2409297
Conc: 6.95 ng/ml

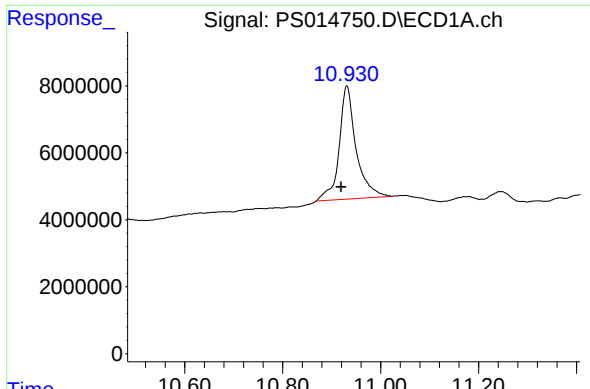

#15 Picloram

R.T.: 10.931 min
Delta R.T.: 0.012 min
Response: 81092566
Conc: 7.25 ng/ml

Instrument :
ECD_R
ClientSampleId :

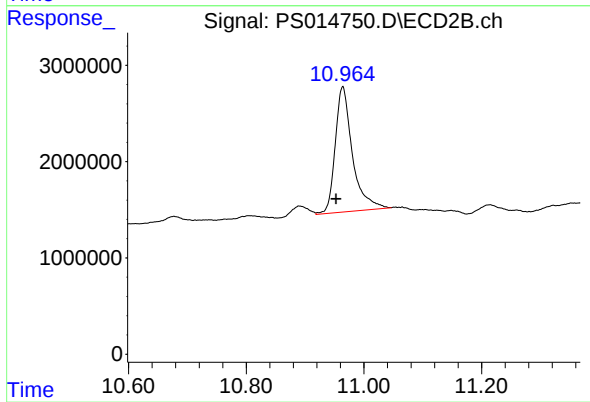

#15 Picloram

R.T.: 10.964 min
Delta R.T.: 0.012 min
Response: 26398785
Conc: 7.04 ng/ml