

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR042423\  
Data File : PR061013.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 25 Apr 2023 03:37  
Operator : AJ\MA  
Sample : 02419-36  
Misc :  
ALS Vial : 65 Sample Multiplier: 1



Instrument :  
ECD\_R  
ClientSampleId :  
EW931

## Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/26/2023  
Supervised By :Ankita Jodhani 04/26/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 25 04:28:00 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR040323CLP.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Tue Apr 04 04:06:01 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

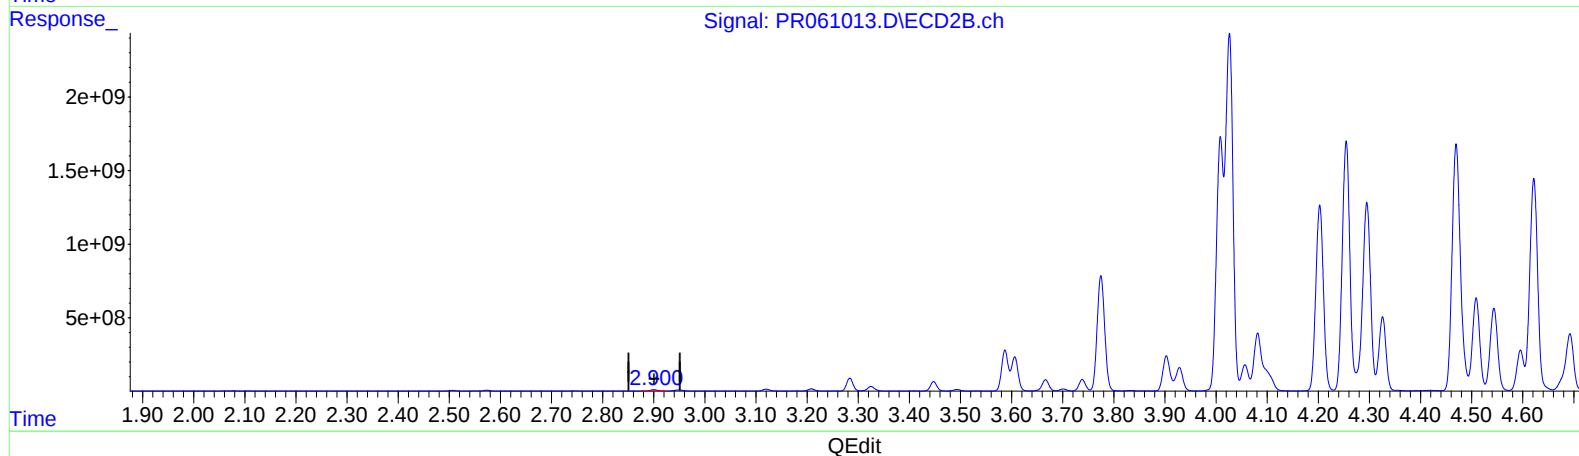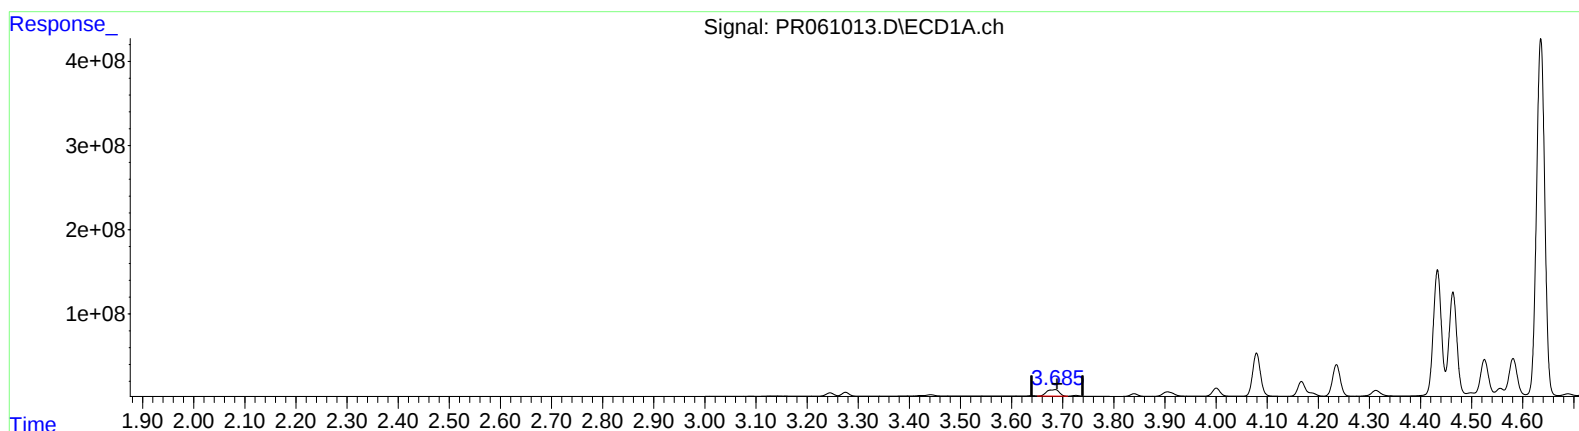

(1) Tetrachloro-m-xylene (SA)

3.685min 37.347 ng/ml

response 127379335

(1) Tetrachloro-m-xylene #2 (SA)

2.900min 19.855 ng/ml

response 92054835

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR042423\  
Data File : PR061013.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 25 Apr 2023 03:37  
Operator : AJ\MA  
Sample : 02419-36  
Misc :  
ALS Vial : 65 Sample Multiplier: 1



Instrument :  
ECD\_R  
ClientSampleId :  
EW931

## Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/26/2023  
Supervised By :Ankita Jodhani 04/26/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 25 04:28:00 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR040323CLP.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Tue Apr 04 04:06:01 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

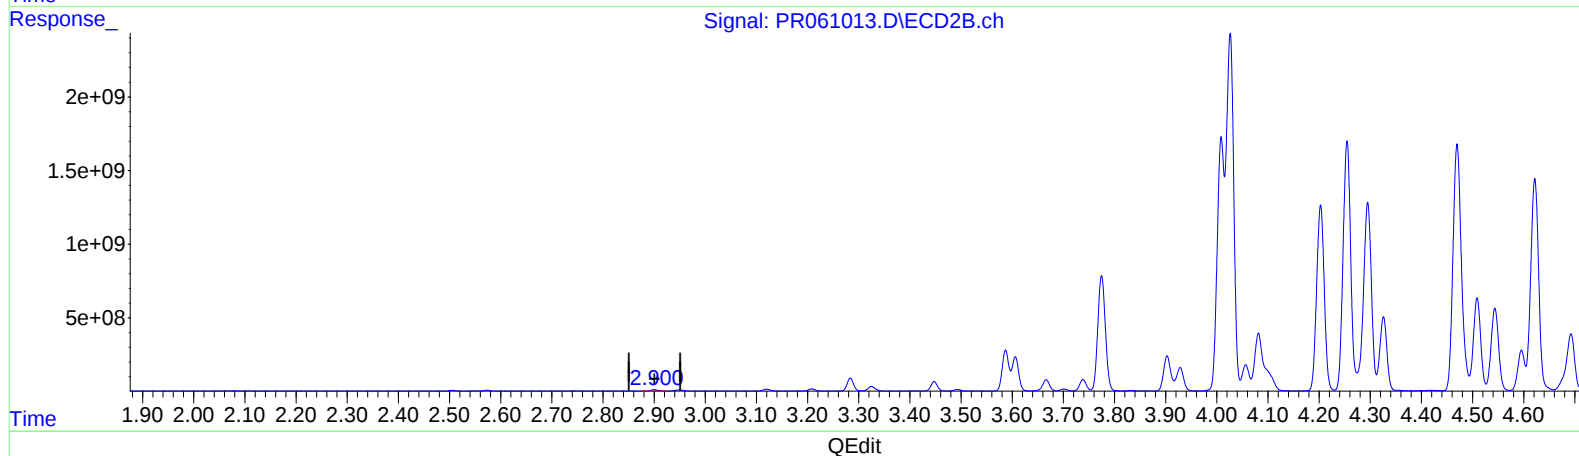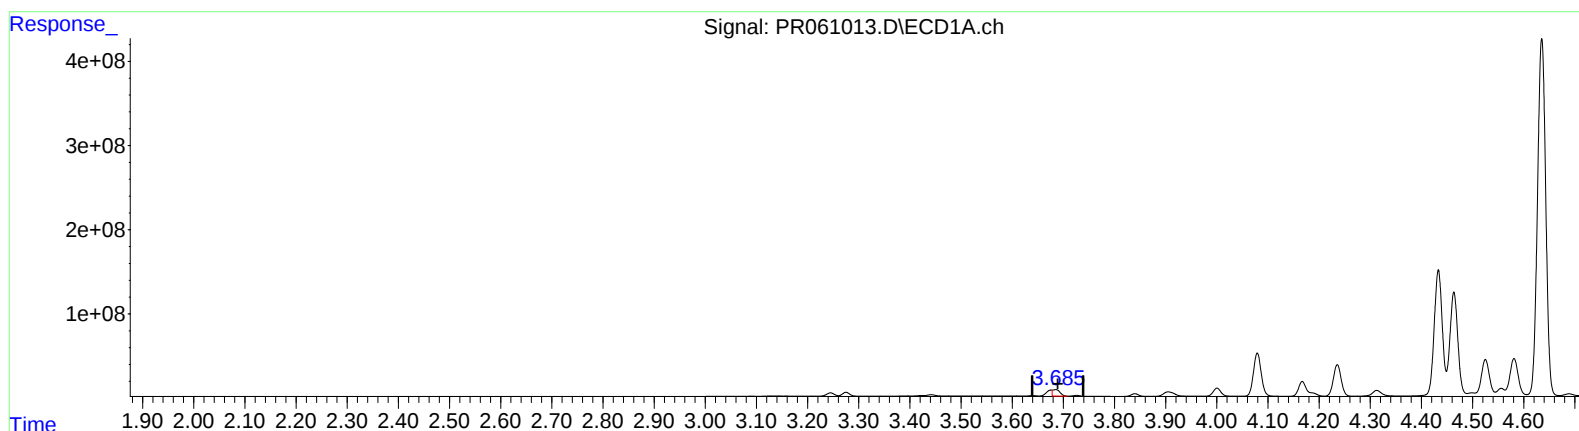

(1) Tetrachloro-m-xylene (SA)

3.685min 22.132 ng/ml m

response 75485844

(1) Tetrachloro-m-xylene #2 (SA)

2.900min 19.855 ng/ml

response 92054835