

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042624\
 Data File : PR066450.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2024 15:08
 Operator : AJ\MA
 Sample : P2260-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 60240

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/29/2024
 Supervised By :mohammad ahmed 05/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 00:56:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 26 07:26:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.657	2.897	23104130	23458152	4.408m	5.248m
2) SA Decachlor...	9.529f	8.141	1070019	5892765	0.457m	1.255 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042624\
Data File : PR066450.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2024 15:08
Operator : AJ\MA
Sample : P2260-04
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
60240


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/29/2024
Supervised By :mohammad ahmed 05/02/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 00:56:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 26 07:26:35 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

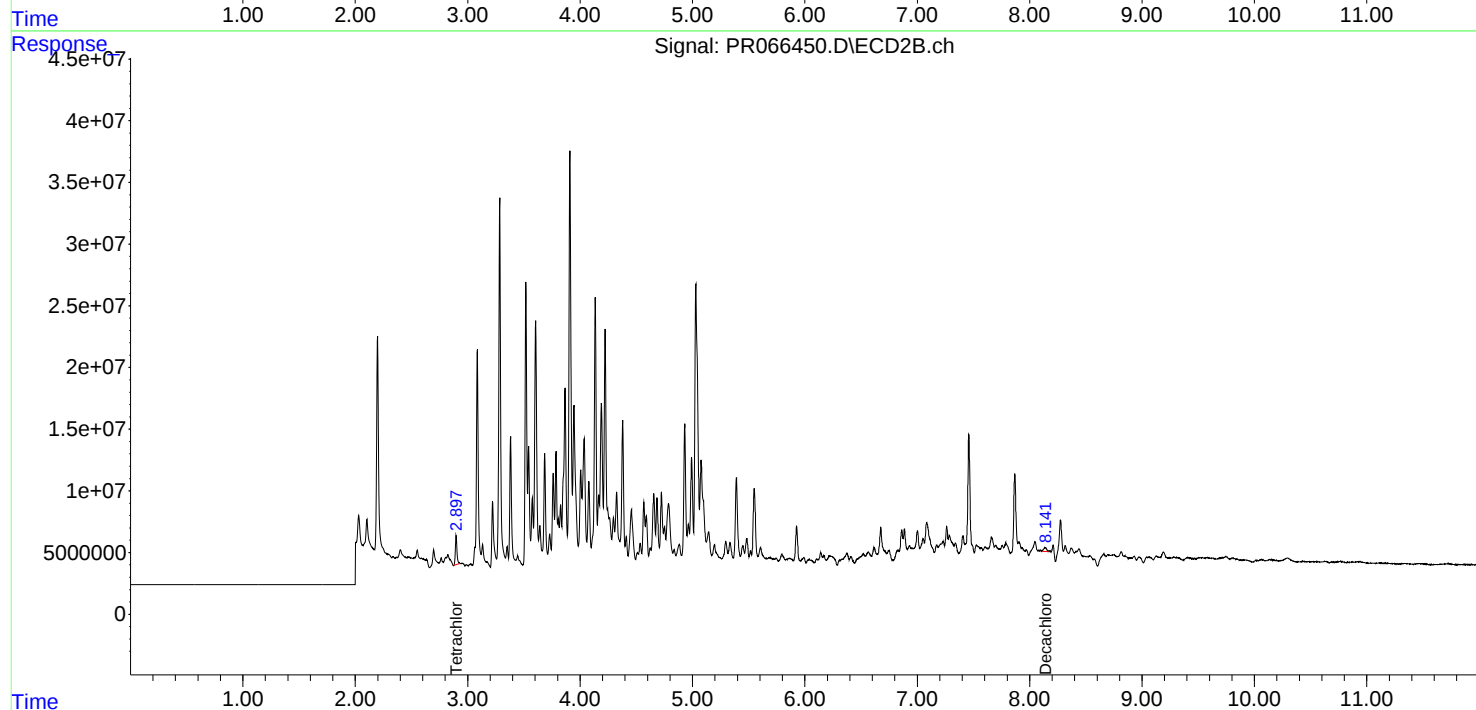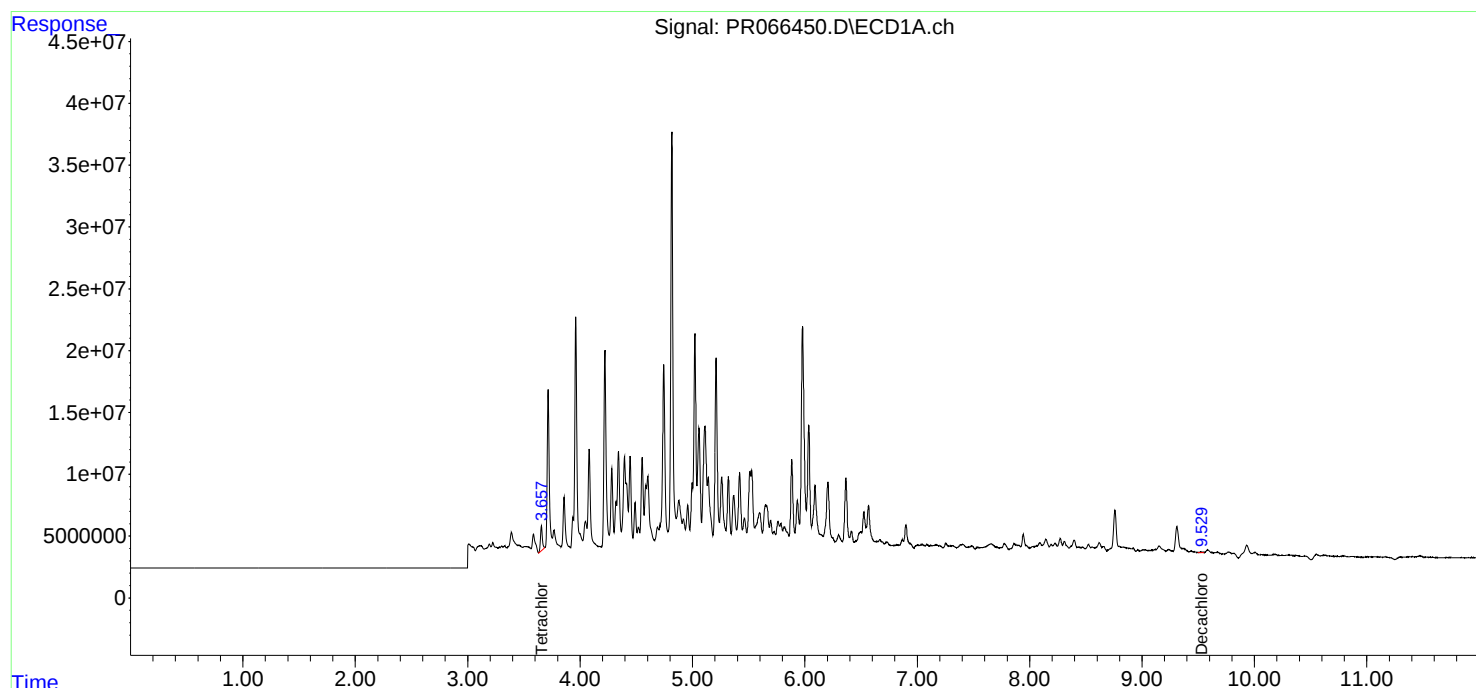

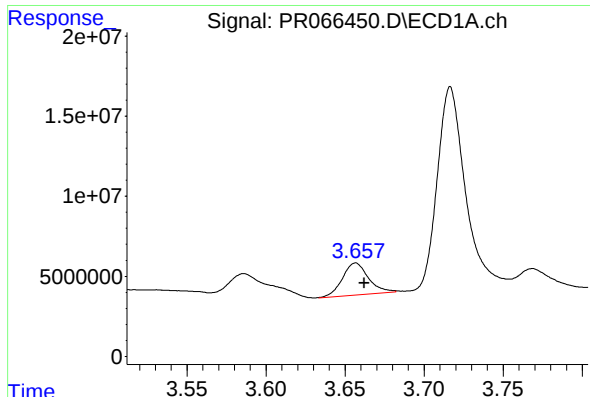


#1 Tetrachloro-m-xylene

R.T.: 3.657 min
Delta R.T.: -0.005 min
Response: 23104130
Conc: 4.41 ng/ml

Instrument :
ECD_R
ClientSampleId :
60240


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/29/2024
Supervised By :mohammad ahmed 05/02/2024

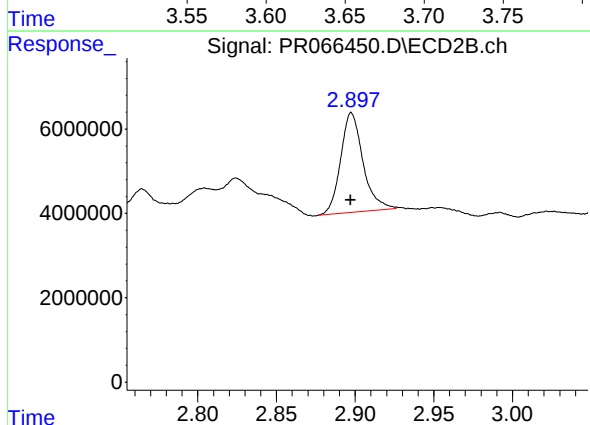


#1 Tetrachloro-m-xylene

R.T.: 2.897 min
Delta R.T.: 0.000 min
Response: 23458152
Conc: 5.25 ng/ml

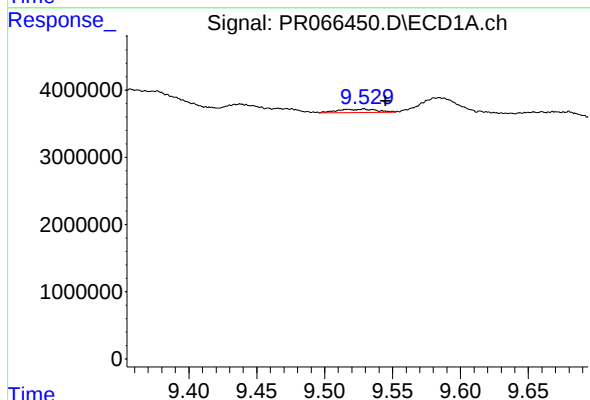

#2 Decachlorobiphenyl

R.T.: 9.529 min
Delta R.T.: -0.016 min
Response: 1070019
Conc: 0.46 ng/ml

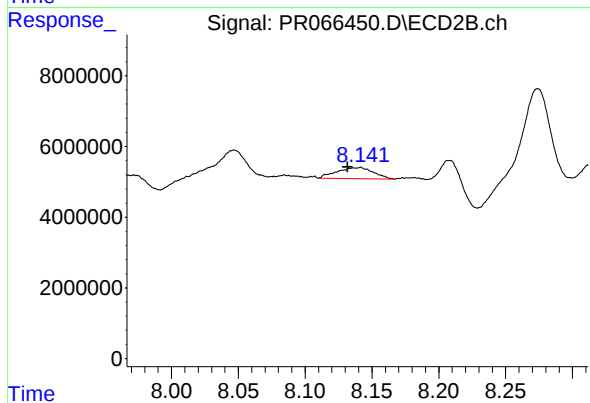

#2 Decachlorobiphenyl

R.T.: 8.141 min
Delta R.T.: 0.010 min
Response: 5892765
Conc: 1.26 ng/ml