

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042924\
 Data File : PR066462.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2024 13:21
 Operator : AJ\MA
 Sample : P2260-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 60240

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/01/2024
 Supervised By :mohammad ahmed 05/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 10:59:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 26 07:26:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.666	2.895	18545783	24161426	3.538m	5.406m#
2) SA Decachlor...	9.556	8.138	738083	2317779	0.315m	0.494m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042924\
Data File : PR066462.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2024 13:21
Operator : AJ\MA
Sample : P2260-04
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
60240


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/01/2024
Supervised By :mohammad ahmed 05/02/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 10:59:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 26 07:26:35 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

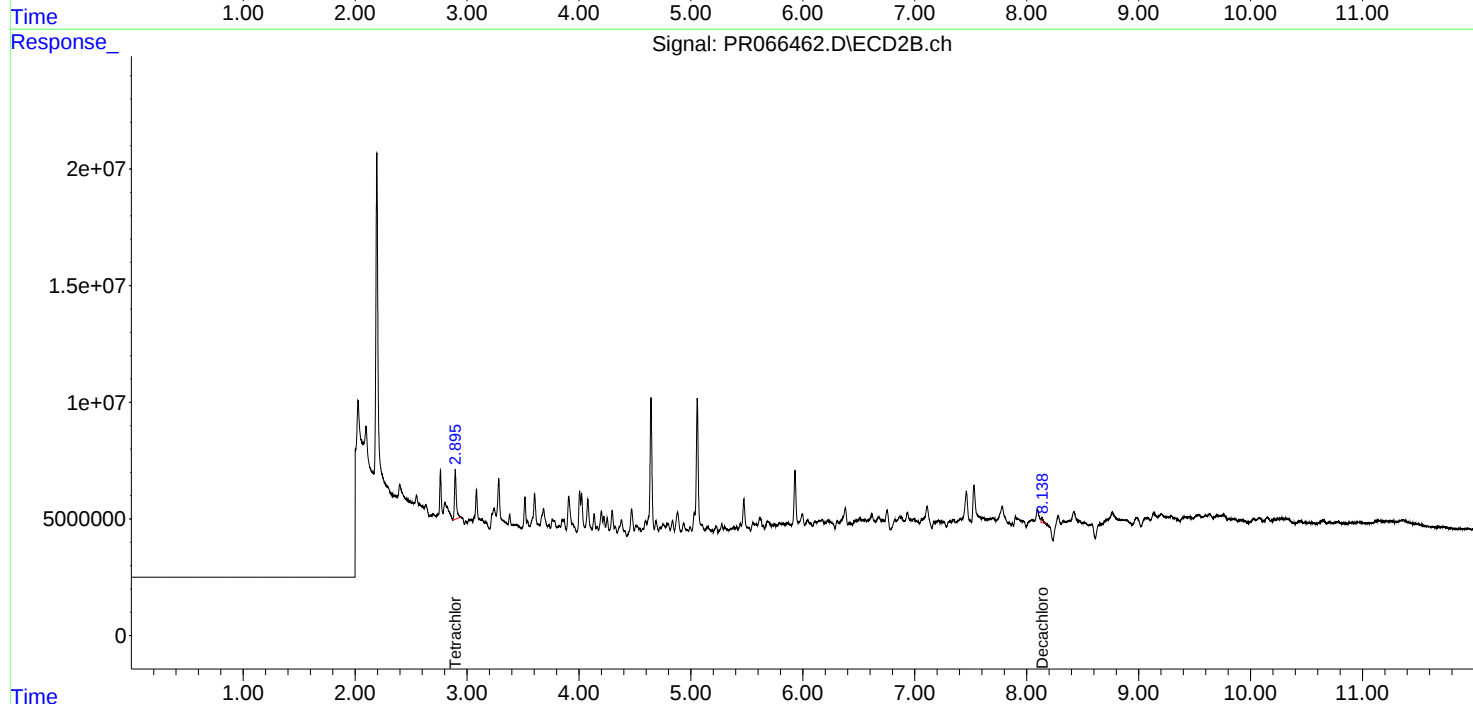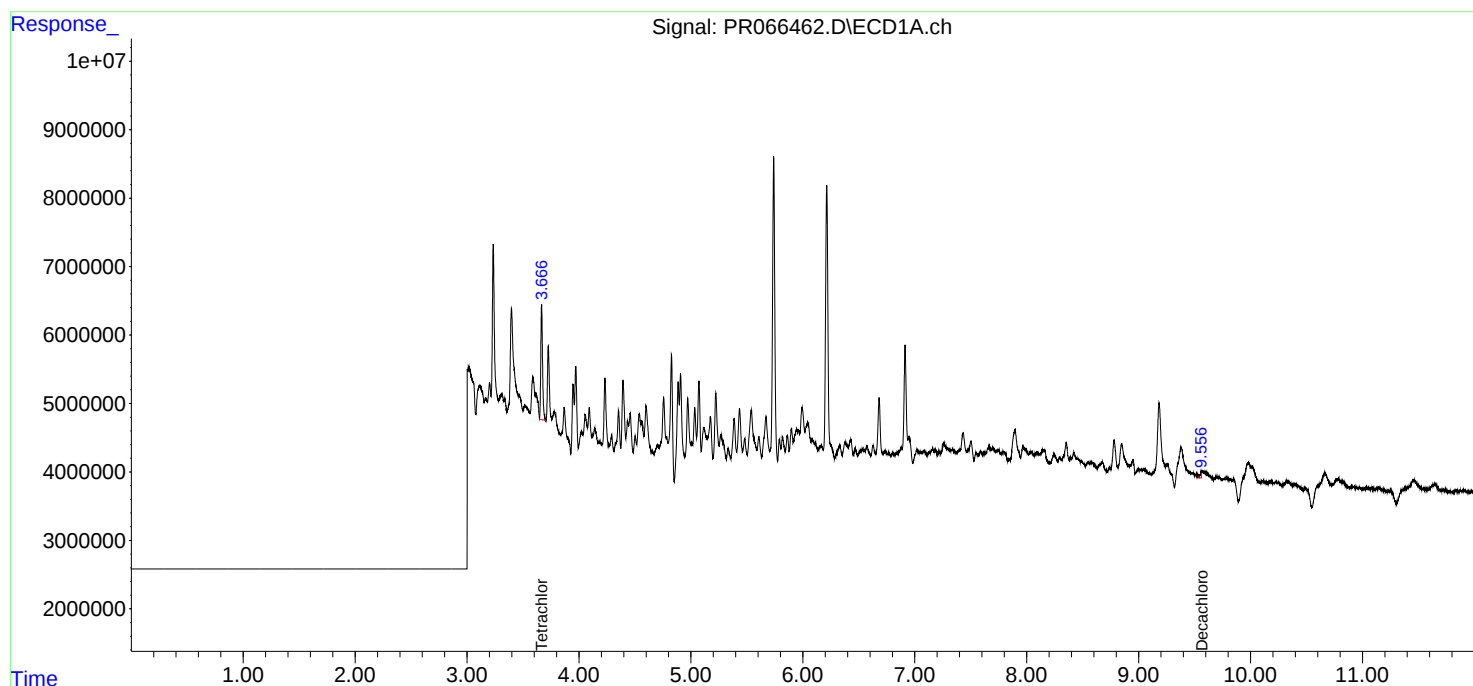

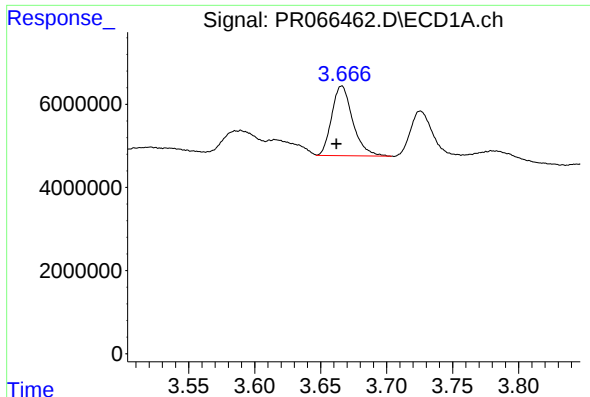


#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: 0.004 min
Response: 18545783
Conc: 3.54 ng/ml

Instrument :
ECD_R
ClientSampleId :
60240


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/01/2024
Supervised By :mohammad ahmed 05/02/2024

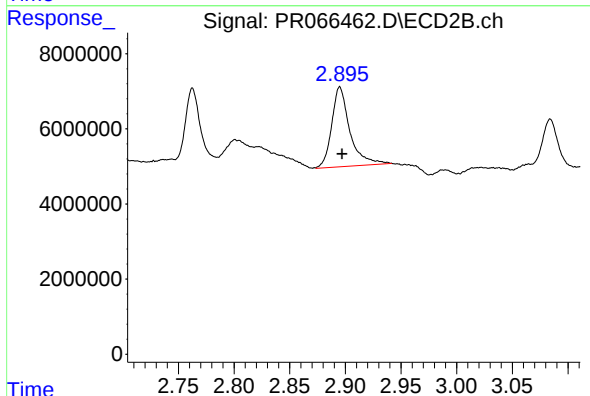


#1 Tetrachloro-m-xylene

R.T.: 2.895 min
Delta R.T.: -0.002 min
Response: 24161426
Conc: 5.41 ng/ml m

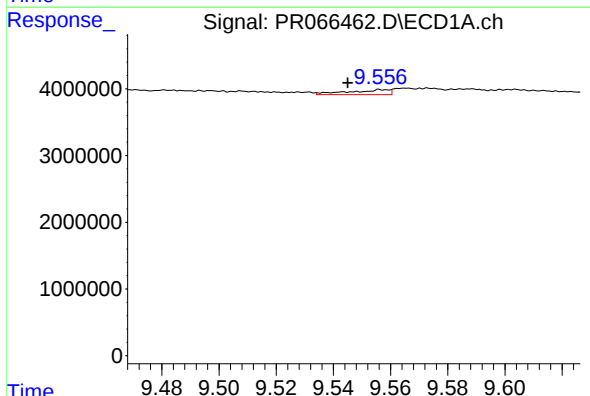

#2 Decachlorobiphenyl

R.T.: 9.556 min
Delta R.T.: 0.011 min
Response: 738083
Conc: 0.32 ng/ml m

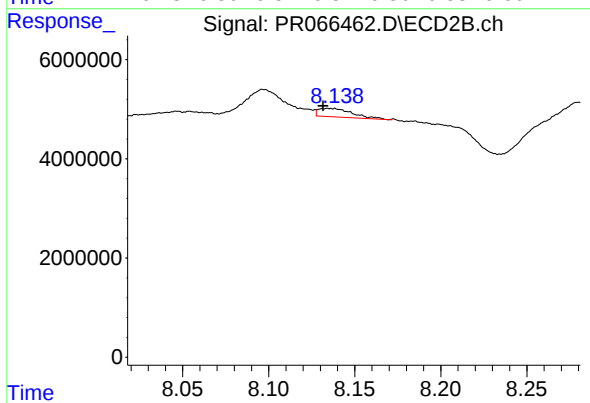

#2 Decachlorobiphenyl

R.T.: 8.138 min
Delta R.T.: 0.007 min
Response: 2317779
Conc: 0.49 ng/ml m