

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042924\
 Data File : PR066463.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Apr 2024 13:53
 Operator : AJ\MA
 Sample : P2260-04RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 60240RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/30/2024
 Supervised By :mohammad ahmed 05/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 30 01:26:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 26 07:26:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	2.895	18477554	22057693	3.525m	4.935m#
2) SA Decachlor...	9.540	8.130	1574266	1748667	0.672	0.373m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR042924\
Data File : PR066463.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Apr 2024 13:53
Operator : AJ\MA
Sample : P2260-04RE
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampleId :
60240RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/30/2024
Supervised By :mohammad ahmed 05/02/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 30 01:26:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 26 07:26:35 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

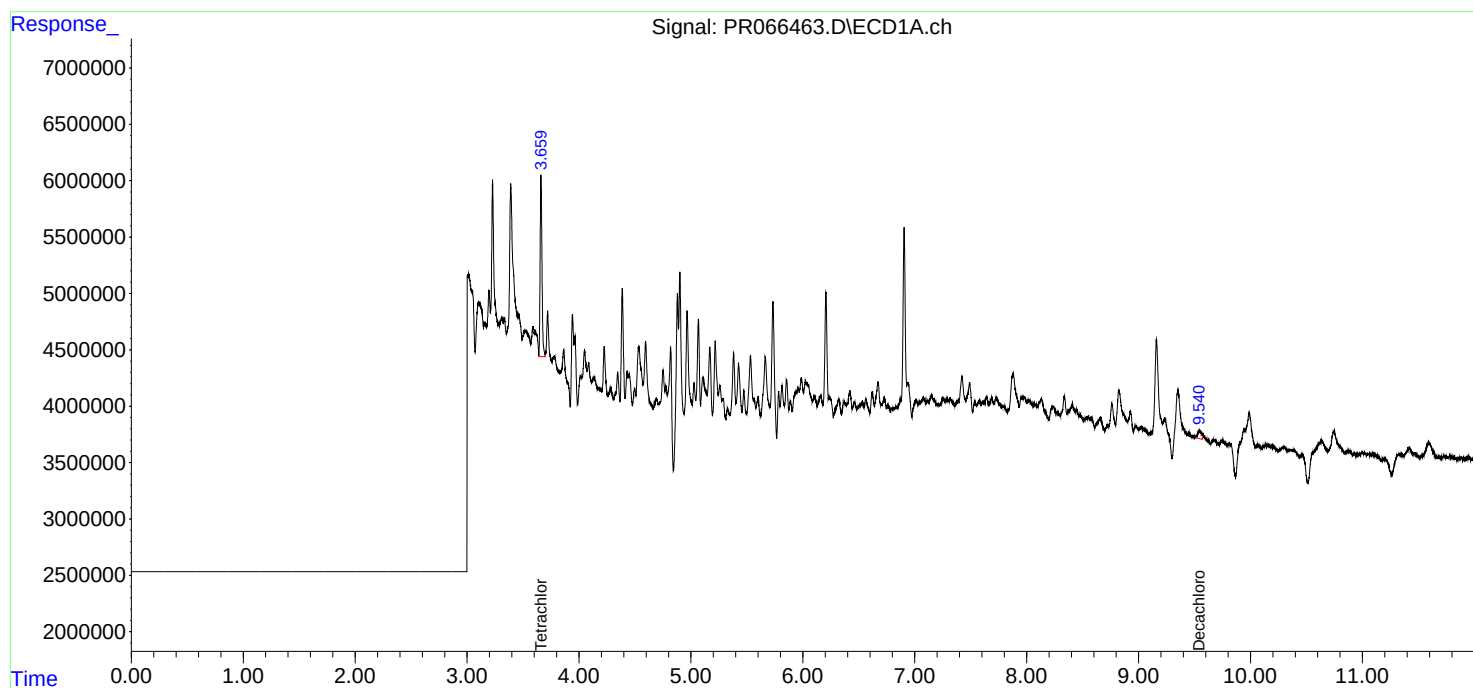

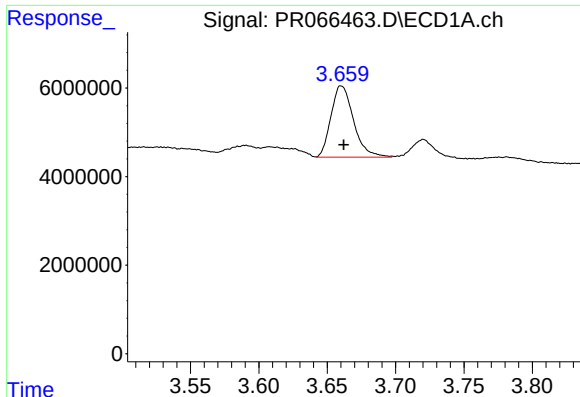


#1 Tetrachloro-m-xylene

R.T.: 3.659 min
Delta R.T.: -0.003 min
Response: 18477554
Conc: 3.53 ng/ml

Instrument :
ECD_R
ClientSampleId :
60240RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/30/2024
Supervised By :mohammad ahmed 05/02/2024

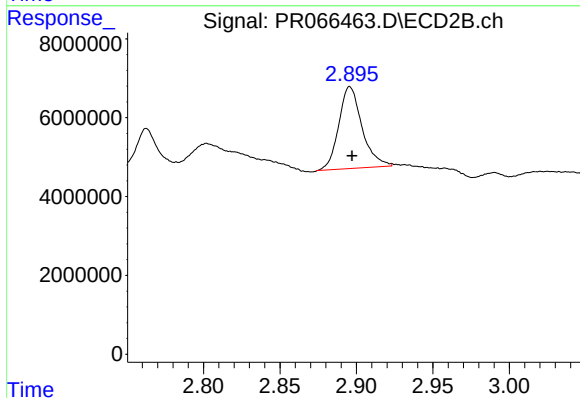


#1 Tetrachloro-m-xylene

R.T.: 2.895 min
Delta R.T.: -0.002 min
Response: 22057693
Conc: 4.93 ng/ml m

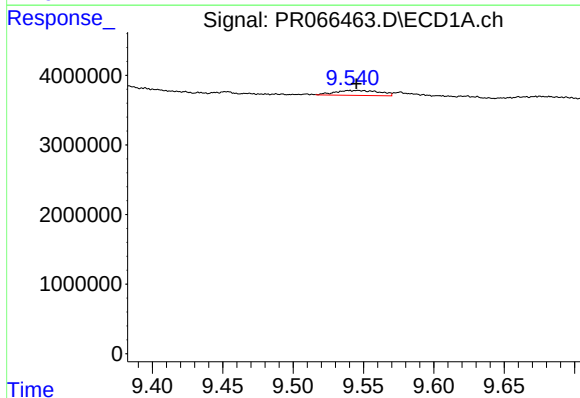

#2 Decachlorobiphenyl

R.T.: 9.540 min
Delta R.T.: -0.005 min
Response: 1574266
Conc: 0.67 ng/ml

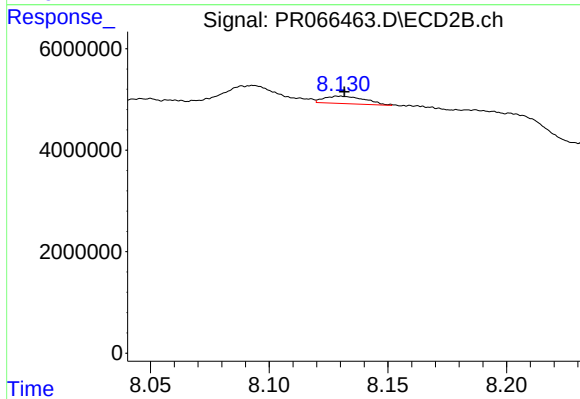

#2 Decachlorobiphenyl

R.T.: 8.130 min
Delta R.T.: -0.002 min
Response: 1748667
Conc: 0.37 ng/ml m