

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR043019\
 Data File : PR037501.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2019 16:20
 Operator : SM\SJ
 Sample : K2241-09
 Misc : AR1262 MDL 25PPB
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 04:13:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.368	3.406	26047258	102.7E6	20.821	21.418
2)	SA Decachlor...	10.000	8.248	34125348	150.9E6	25.802	25.902
Target Compounds							
3)	L1 AR-1016-1	5.459	4.460	526941	1968970	12.229	10.814
4)	L1 AR-1016-2	0.000	4.460	0	1968970	N.D.	6.979 #
5)	L1 AR-1016-3	0.000	4.634	0	457673	N.D.	3.183 #
6)	L1 AR-1016-4	0.000	4.689	0	1201182	N.D.	10.857 #
7)	L1 AR-1016-5	0.000	4.884	0	1103553	N.D.	7.260 #
8)	L2 AR-1221-1	0.000	3.579	0	205321	N.D.	4.032 #
9)	L2 AR-1221-2	4.674	3.696	429249	1325604	47.462	35.696
10)	L2 AR-1221-3	4.674	3.767	429249	270534	14.005	2.209 #
11)	L3 AR-1232-1	4.674	3.767	429249	270534	14.675	2.312 #
12)	L3 AR-1232-2	0.000	4.460	0	1968970	N.D.	14.245 #
13)	L3 AR-1232-3	0.000	4.634	0	457673	N.D.	6.519 #
14)	L3 AR-1232-4	0.000	4.722	0	418524	N.D.	7.014 #
15)	L3 AR-1232-5	0.000	4.884	0	1103553	N.D.	16.171 #
16)	L4 AR-1242-1	5.459	4.460	526941	1968970	15.401	13.437
17)	L4 AR-1242-2	0.000	4.460	0	1968970	N.D.	8.630 #
18)	L4 AR-1242-3	0.000	4.634	0	457673	N.D.	3.958 #
19)	L4 AR-1242-4	0.000	4.722	0	418524	N.D.	3.808 #
20)	L4 AR-1242-5	6.405	5.227	220286	4413517	6.846	26.636 #
21)	L5 AR-1248-1	5.459	4.460	526941	1968970	23.003	19.560
22)	L5 AR-1248-2	0.000	4.689	0	1201182	N.D.	8.802 #
23)	L5 AR-1248-3	0.000	4.722	0	418524	N.D.	2.990 #
24)	L5 AR-1248-4	6.405	4.884	220286	1103553	4.500	6.201 #
25)	L5 AR-1248-5	6.405	5.276	220286	1031027	4.663	5.271
26)	L6 AR-1254-1	6.376	5.227	1152515	4413517	21.096	12.812 #
27)	L6 AR-1254-2	6.589	5.371	712256	5857315	8.311	19.557 #
28)	L6 AR-1254-3	6.974	5.777	1059730	8197296	11.650	17.308 #
29)	L6 AR-1254-4	7.240	5.988	194805	186344	2.907	0.531 #
30)	L6 AR-1254-5	7.654	6.395	3628909	12738243	50.485	28.766 #
31)	L7 AR-1260-1	7.118	5.890	2226514	8745113	33.742	29.921
32)	L7 AR-1260-2	7.371	6.076	3308301	17759572	41.507	38.559
33)	L7 AR-1260-3	7.728	6.225	3721565	11720735	59.473	32.877 #
34)	L7 AR-1260-4	7.955	6.687	3541131	15112506	47.593	49.588
35)	L7 AR-1260-5	8.268	6.930	5690977	31692550	39.351	36.544
36)	L8 AR-1262-1	7.728	6.487	3721565	10218788	35.629	40.774
37)	L8 AR-1262-2	8.268	6.930	5690977	31692550	29.277	25.234
38)	L8 AR-1262-3	8.566	7.205	4112107	20326448	31.268	37.074
39)	L8 AR-1262-4	8.656	7.270	2979805	42655581	30.335	47.519 #
40)	L8 AR-1262-5	9.290	7.761	2011528	10178815	29.135	26.603
41)	L9 AR-1268-1	8.566	7.205	4112107	20326448	22.961	16.512 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR043019\
 Data File : PR037501.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2019 16:20
 Operator : SM\SJ
 Sample : K2241-09
 Misc : AR1262 MDL 25PPB
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 04:13:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.656	7.270	2979805	42655581	18.115	40.282 #
43) L9	AR-1268-3	8.875	7.468	723172	6225863	5.224	7.025 #
44) L9	AR-1268-4	9.290	7.761	2011528	10178815	32.243	28.058
45) L9	AR-1268-5	9.681	8.028	956041	5746883	2.097	2.259



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR043019\
Data File : PR037501.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2019 16:20
Operator : SM\SJ
Sample : K2241-09
Misc : AR1262 MDL 25PPB
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 04:13:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

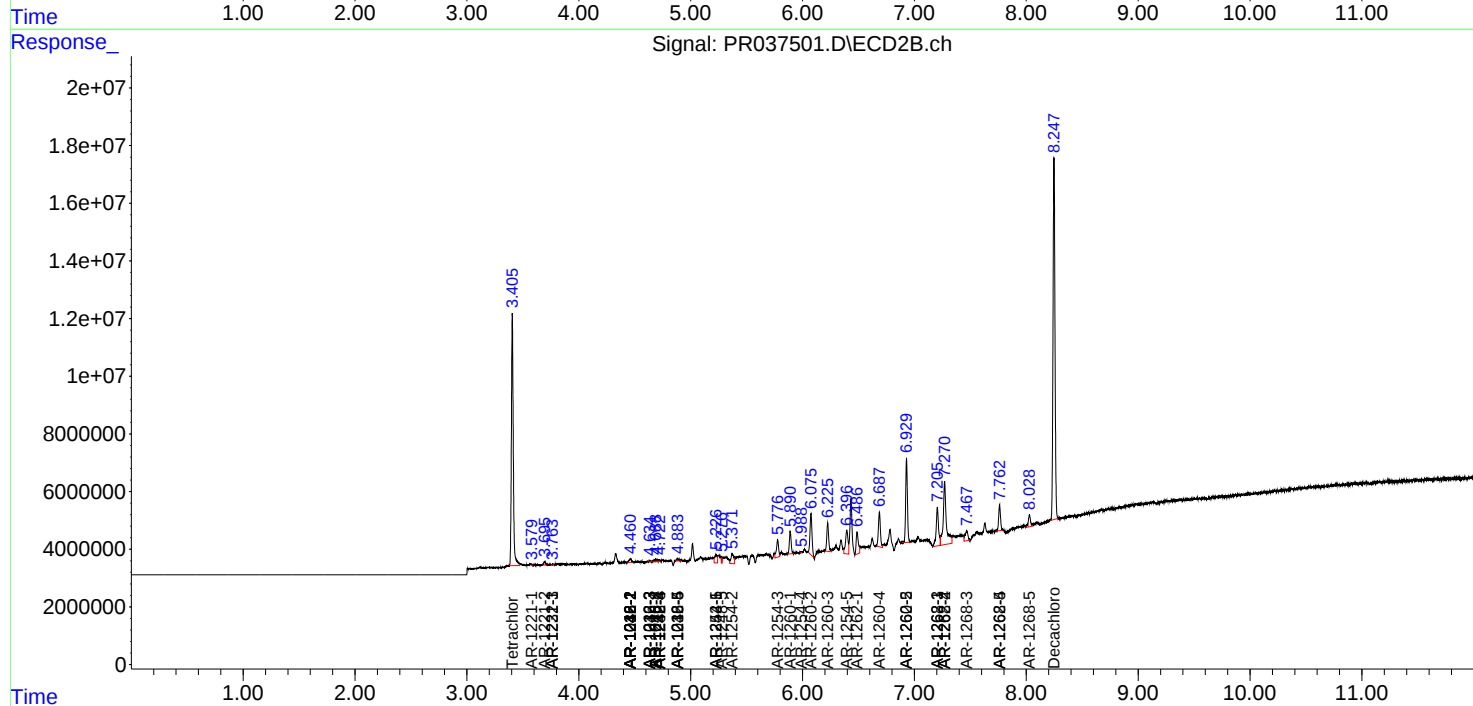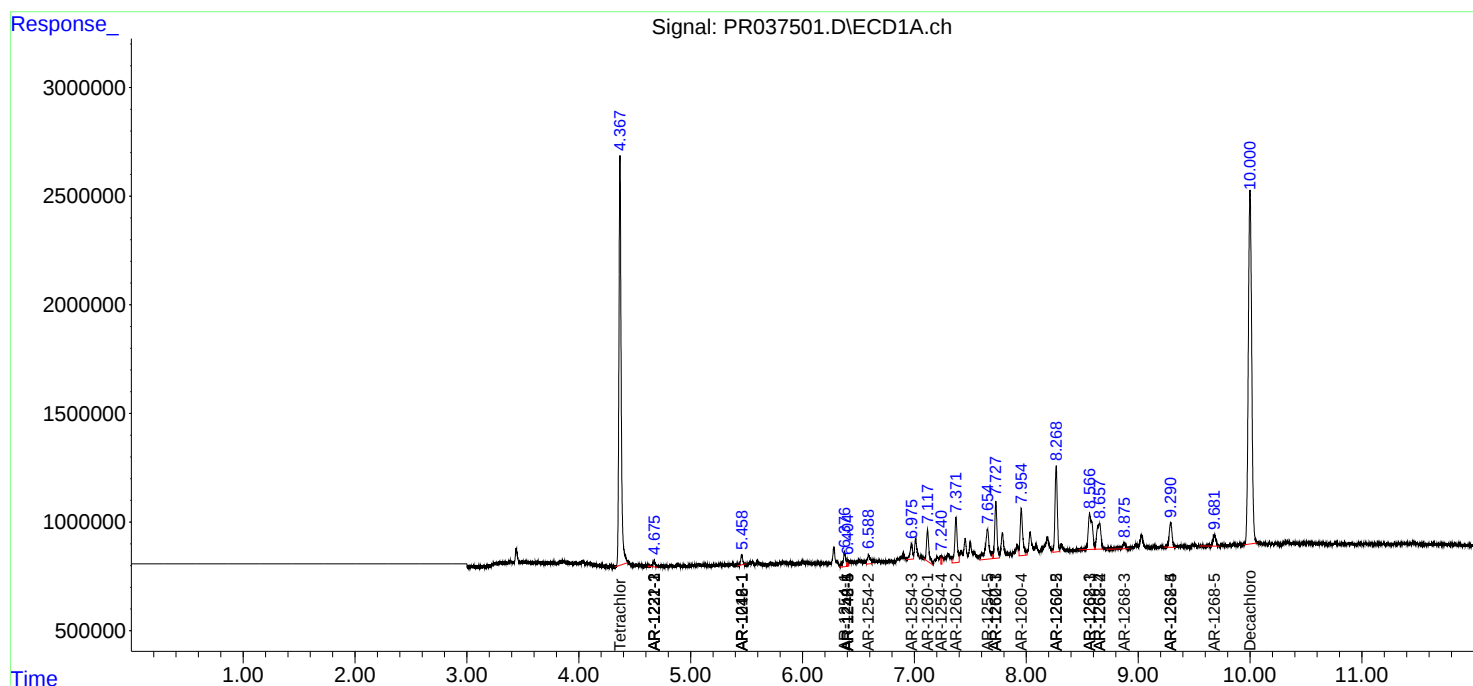


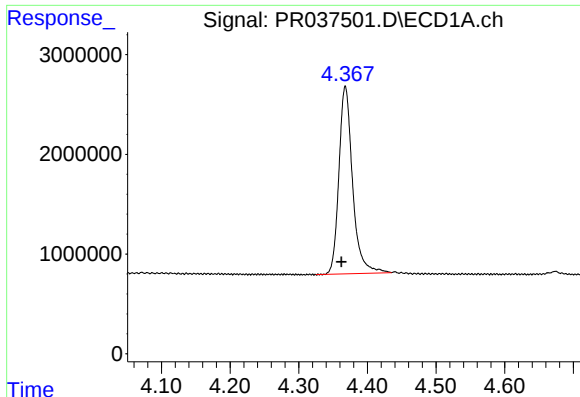

#1 Tetrachloro-m-xylene


R.T.: 4.368 min
Delta R.T.: 0.006 min
Response: 26047258
Conc: 20.82 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

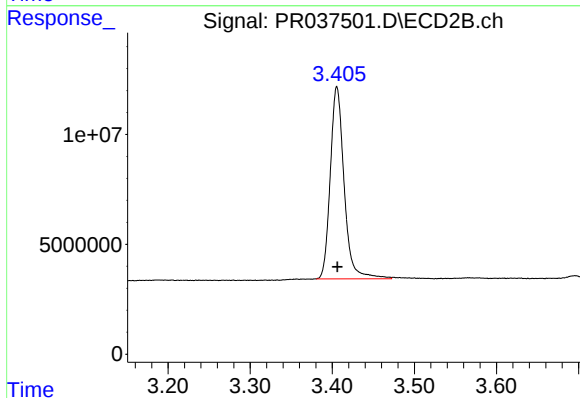


#1 Tetrachloro-m-xylene

R.T.: 3.406 min
Delta R.T.: 0.000 min
Response: 102710615
Conc: 21.42 ng/ml

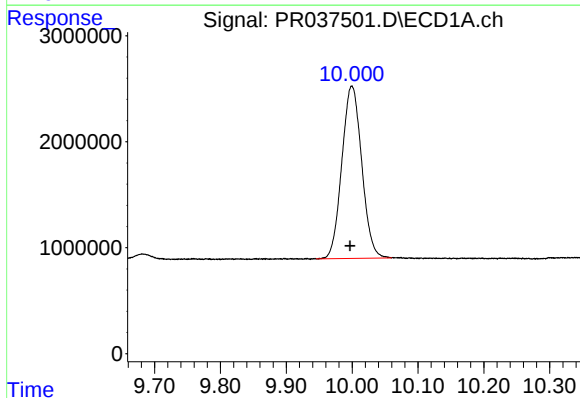


#2 Decachlorobiphenyl

R.T.: 10.000 min
Delta R.T.: 0.003 min
Response: 34125348
Conc: 25.80 ng/ml

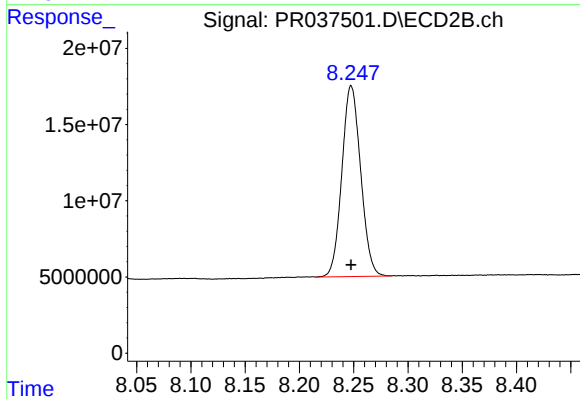

#2 Decachlorobiphenyl


R.T.: 8.248 min
Delta R.T.: 0.000 min
Response: 150859909
Conc: 25.90 ng/ml

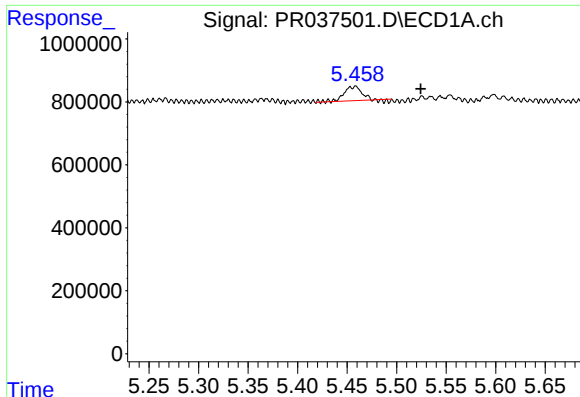

#3 AR-1016-1


R.T.: 5.459 min
Delta R.T.: -0.065 min
Response: 526941
Conc: 12.23 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

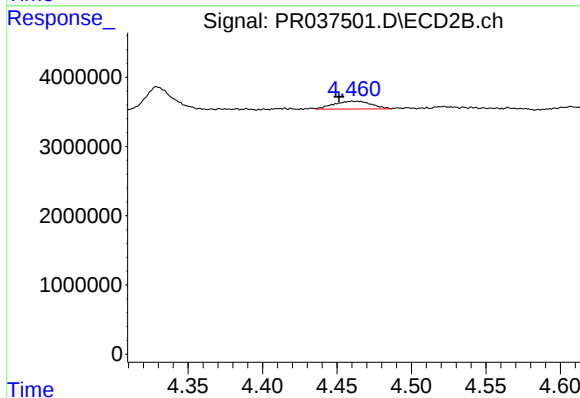


#3 AR-1016-1

R.T.: 4.460 min
Delta R.T.: 0.009 min
Response: 1968970
Conc: 10.81 ng/ml

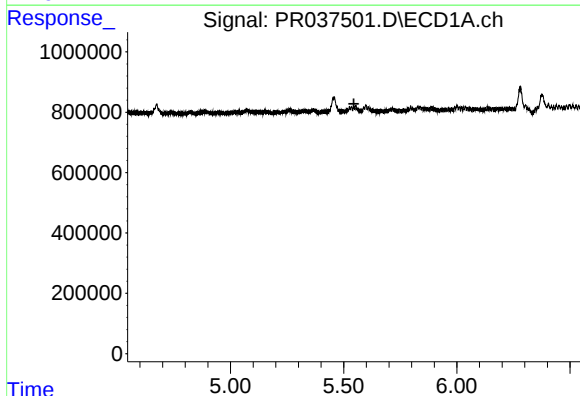


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T. : 5.545 min
Response: 0
Conc: N.D.

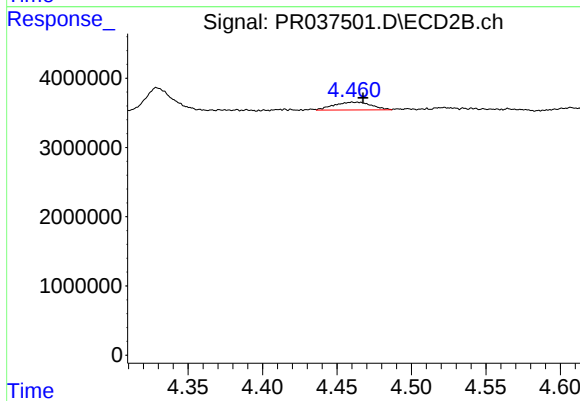

#4 AR-1016-2


R.T.: 4.460 min
Delta R.T.: -0.007 min
Response: 1968970
Conc: 6.98 ng/ml

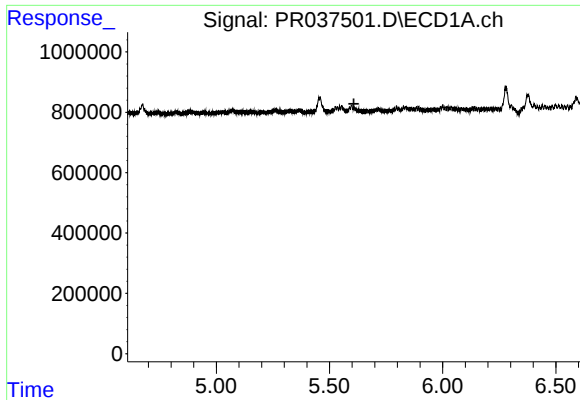

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

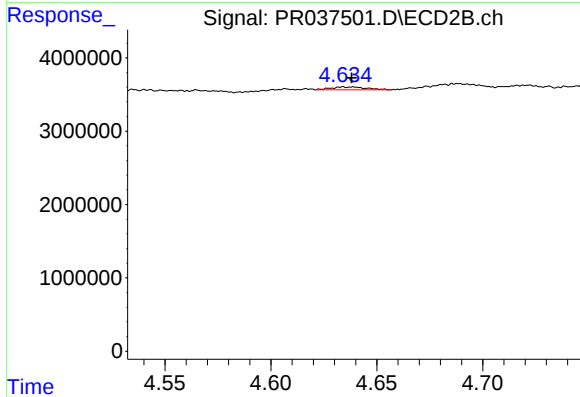


#5 AR-1016-3

R.T.: 4.634 min
Delta R.T.: -0.004 min
Response: 457673
Conc: 3.18 ng/ml

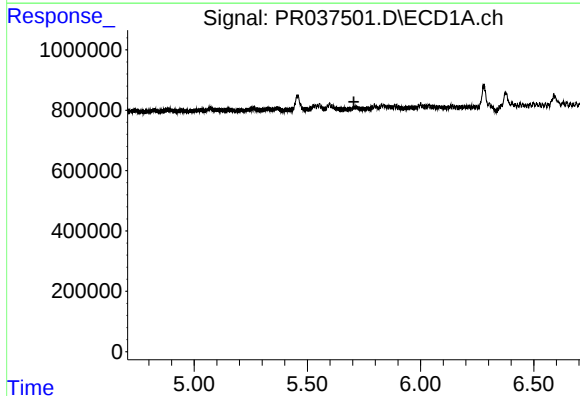


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.705 min
Response: 0
Conc: N.D.

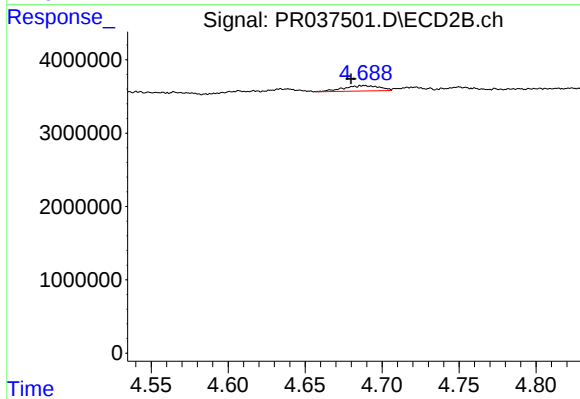

#6 AR-1016-4


R.T.: 4.689 min
Delta R.T.: 0.009 min
Response: 1201182
Conc: 10.86 ng/ml

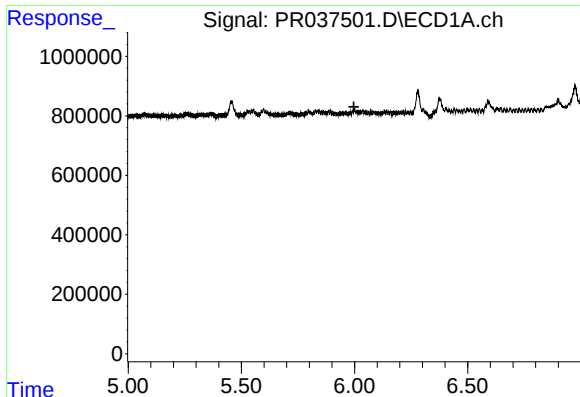

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

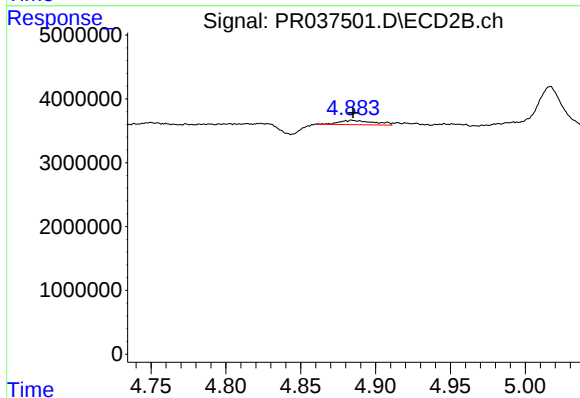


#7 AR-1016-5

R.T.: 4.884 min
Delta R.T.: 0.000 min
Response: 1103553
Conc: 7.26 ng/ml

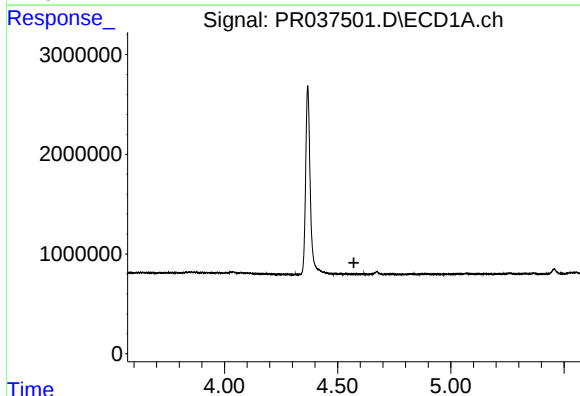


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T.: 4.572 min
Response: 0
Conc: N.D.

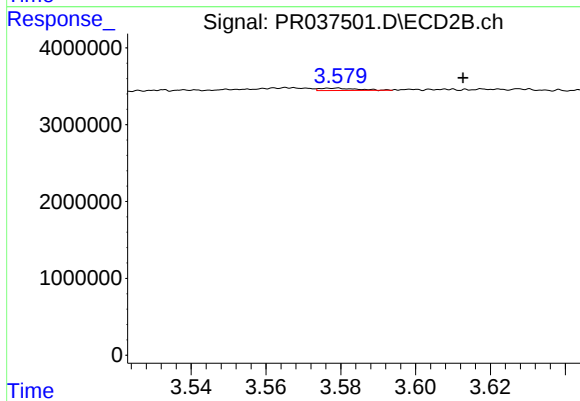

#8 AR-1221-1


R.T.: 3.579 min
Delta R.T.: -0.033 min
Response: 205321
Conc: 4.03 ng/ml

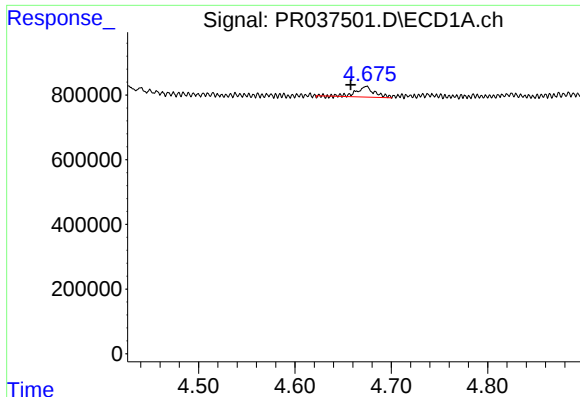

#9 AR-1221-2


R.T.: 4.674 min
Delta R.T.: 0.016 min
Response: 429249
Conc: 47.46 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

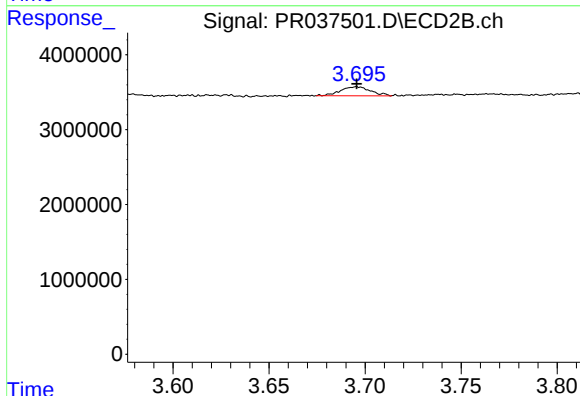


#9 AR-1221-2

R.T.: 3.696 min
Delta R.T.: 0.000 min
Response: 1325604
Conc: 35.70 ng/ml

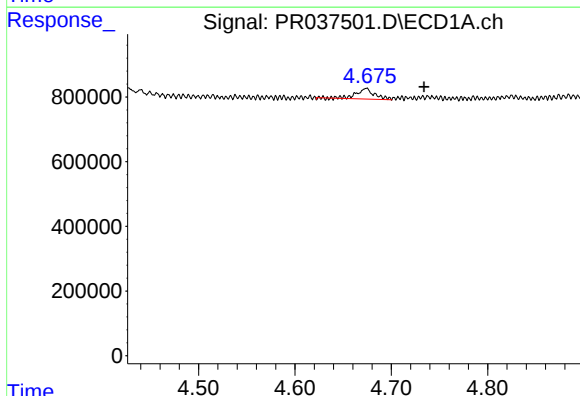


#10 AR-1221-3

R.T.: 4.674 min
Delta R.T.: -0.060 min
Response: 429249
Conc: 14.01 ng/ml

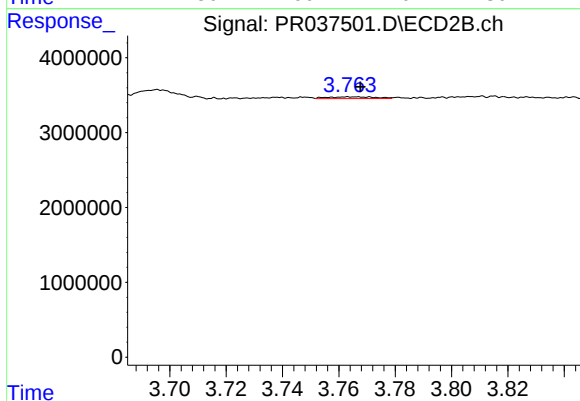

#10 AR-1221-3


R.T.: 3.767 min
Delta R.T.: 0.000 min
Response: 270534
Conc: 2.21 ng/ml

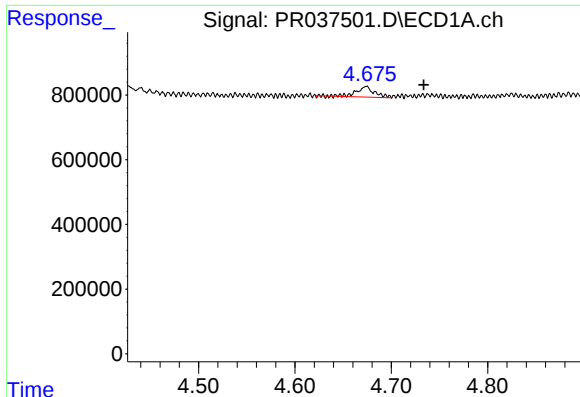

#11 AR-1232-1


R.T.: 4.674 min
Delta R.T.: -0.060 min
Response: 429249
Conc: 14.67 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

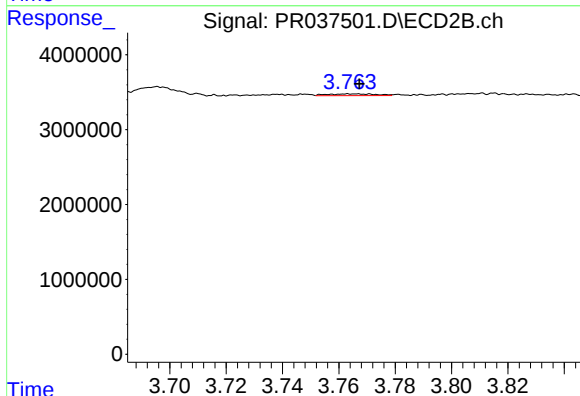


#11 AR-1232-1

R.T.: 3.767 min
Delta R.T.: 0.000 min
Response: 270534
Conc: 2.31 ng/ml

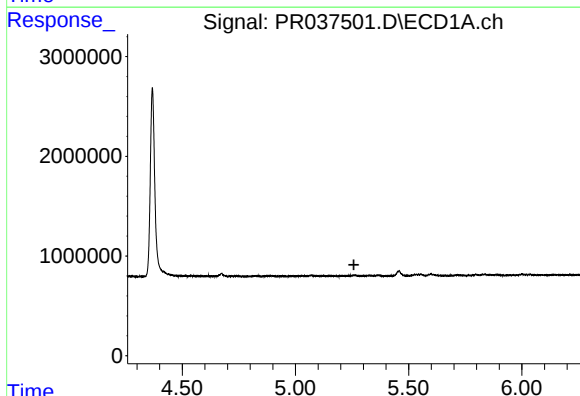


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

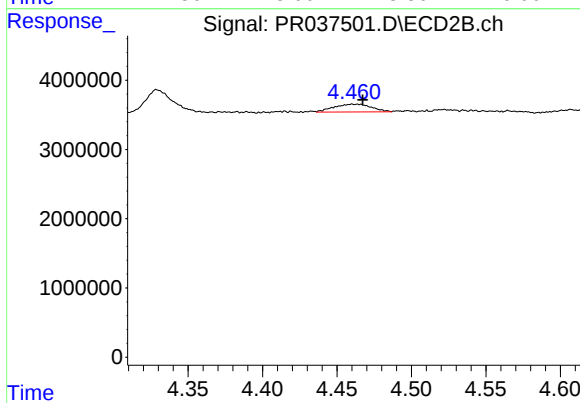

#12 AR-1232-2


R.T.: 4.460 min
Delta R.T.: -0.007 min
Response: 1968970
Conc: 14.24 ng/ml

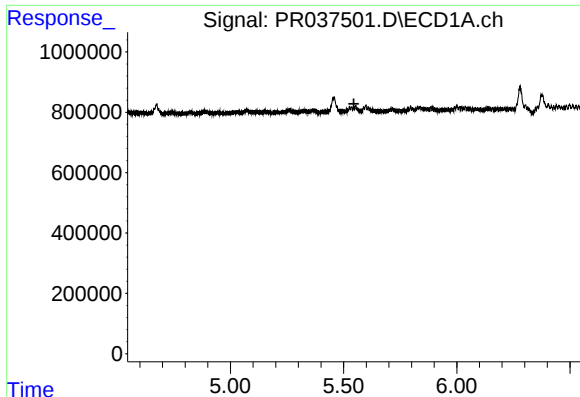

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

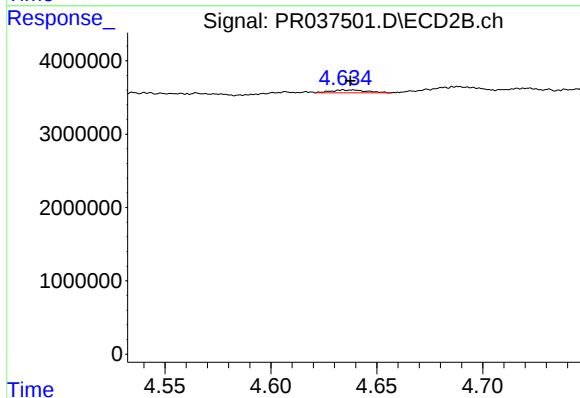


#13 AR-1232-3

R.T.: 4.634 min
Delta R.T.: -0.003 min
Response: 457673
Conc: 6.52 ng/ml

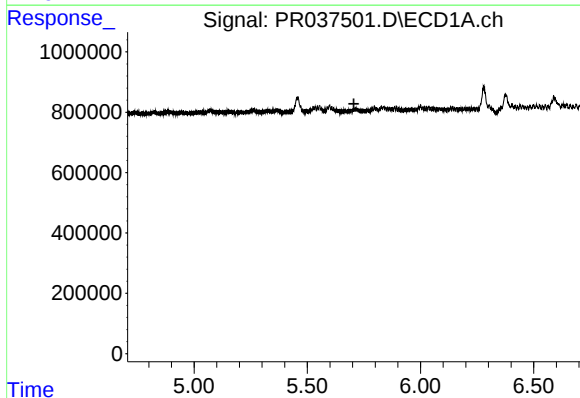


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

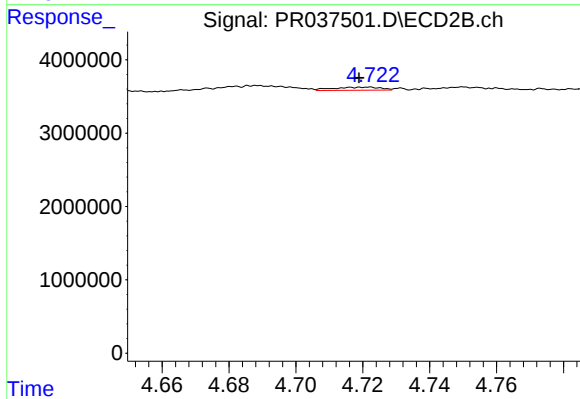

#14 AR-1232-4


R.T.: 4.722 min
Delta R.T.: 0.003 min
Response: 418524
Conc: 7.01 ng/ml

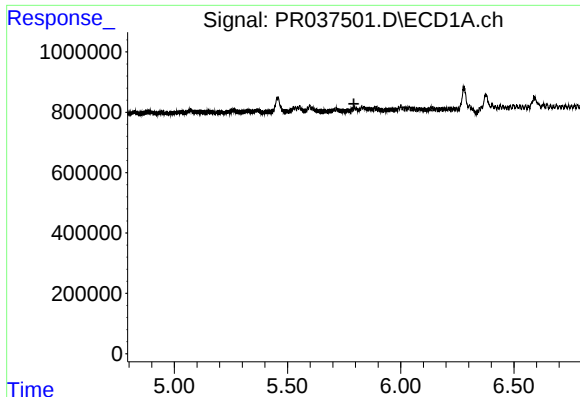

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

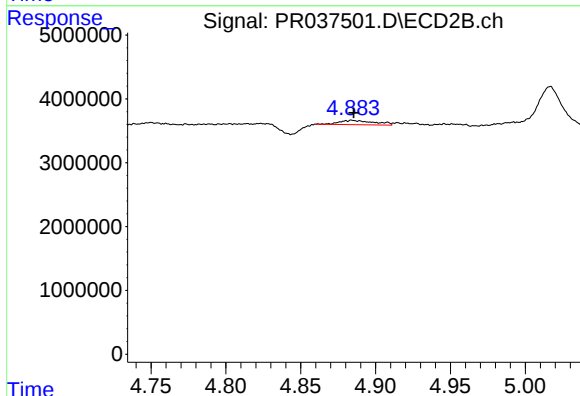


#15 AR-1232-5

R.T.: 4.884 min
Delta R.T.: -0.001 min
Response: 1103553
Conc: 16.17 ng/ml

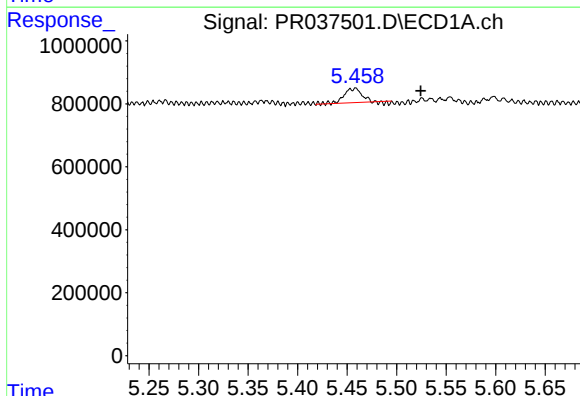


#16 AR-1242-1

R.T.: 5.459 min
Delta R.T.: -0.065 min
Response: 526941
Conc: 15.40 ng/ml

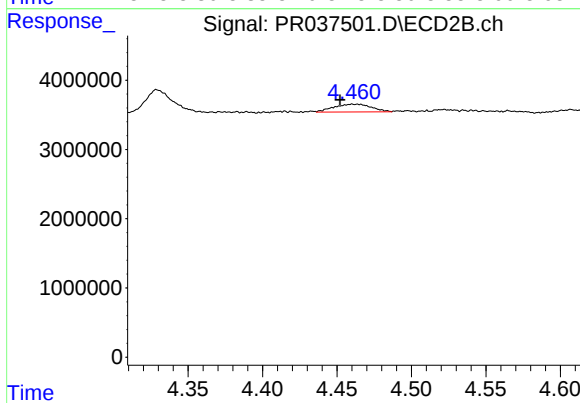

#16 AR-1242-1


R.T.: 4.460 min
Delta R.T.: 0.008 min
Response: 1968970
Conc: 13.44 ng/ml

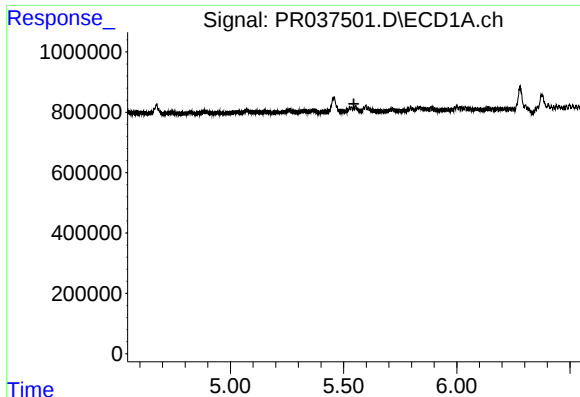

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

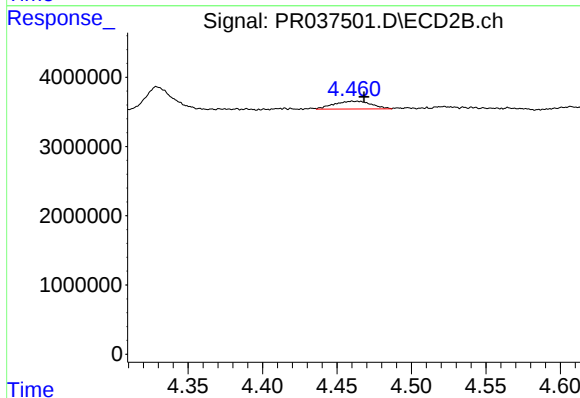


#17 AR-1242-2

R.T.: 4.460 min
Delta R.T.: -0.008 min
Response: 1968970
Conc: 8.63 ng/ml

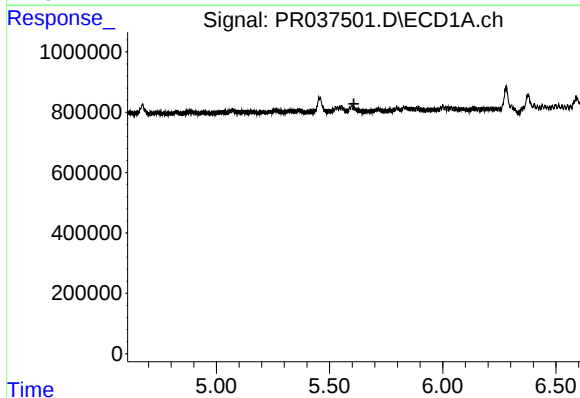


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

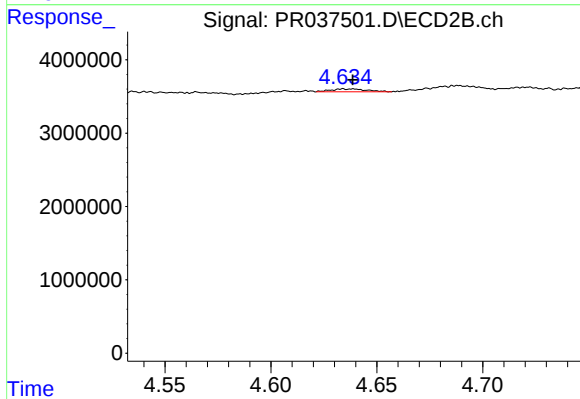

#18 AR-1242-3


R.T.: 4.634 min
Delta R.T.: -0.004 min
Response: 457673
Conc: 3.96 ng/ml

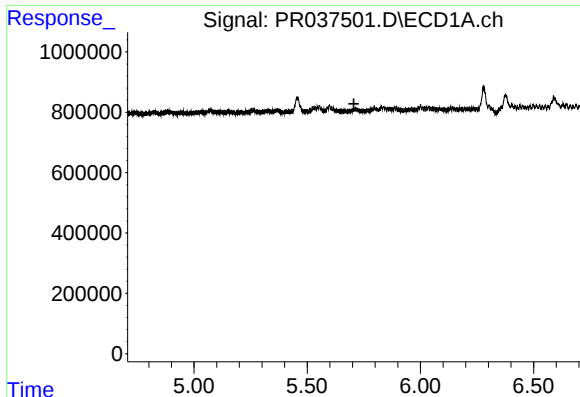

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

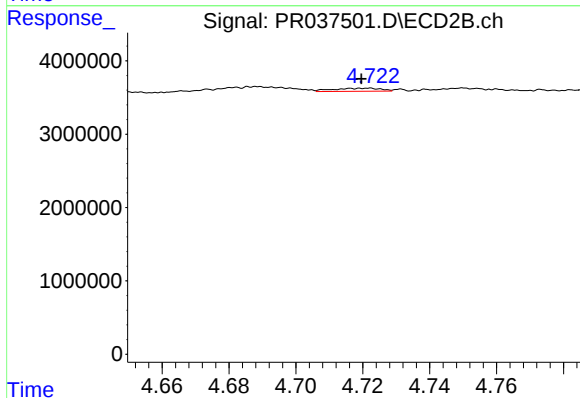


#19 AR-1242-4

R.T.: 4.722 min
Delta R.T.: 0.002 min
Response: 418524
Conc: 3.81 ng/ml

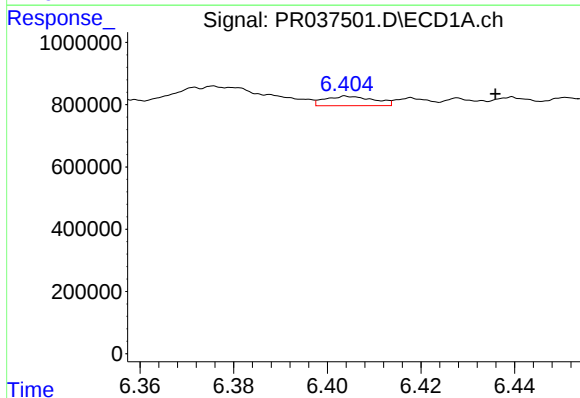


#20 AR-1242-5

R.T.: 6.405 min
Delta R.T.: -0.031 min
Response: 220286
Conc: 6.85 ng/ml

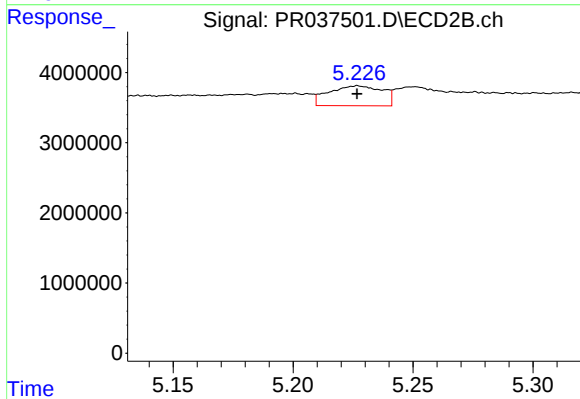

#20 AR-1242-5


R.T.: 5.227 min
Delta R.T.: 0.000 min
Response: 4413517
Conc: 26.64 ng/ml

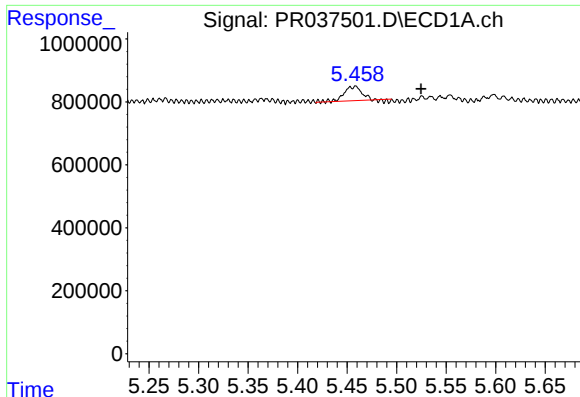

#21 AR-1248-1


R.T.: 5.459 min
Delta R.T.: -0.066 min
Response: 526941
Conc: 23.00 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

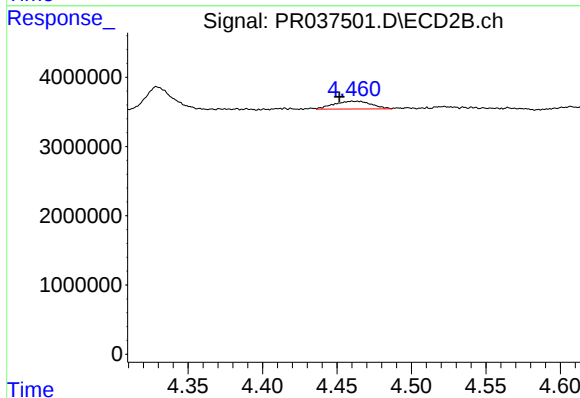


#21 AR-1248-1

R.T.: 4.460 min
Delta R.T.: 0.009 min
Response: 1968970
Conc: 19.56 ng/ml

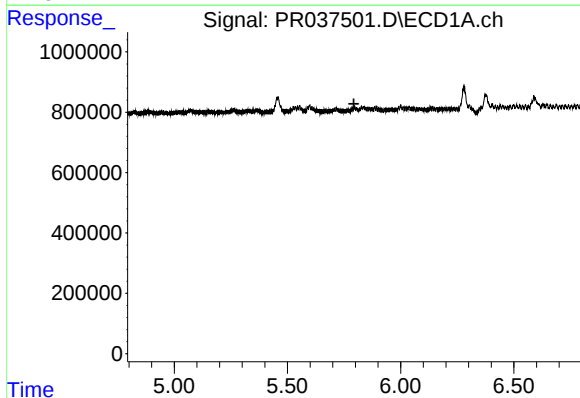


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 5.793 min
Response: 0
Conc: N.D.

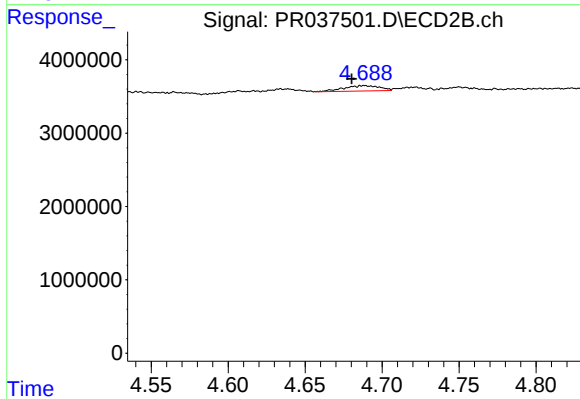

#22 AR-1248-2


R.T.: 4.689 min
Delta R.T.: 0.008 min
Response: 1201182
Conc: 8.80 ng/ml

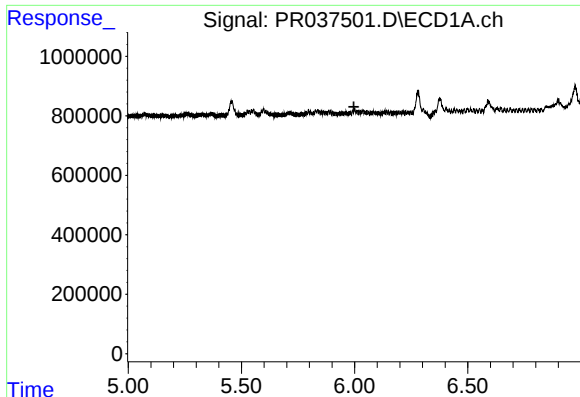

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

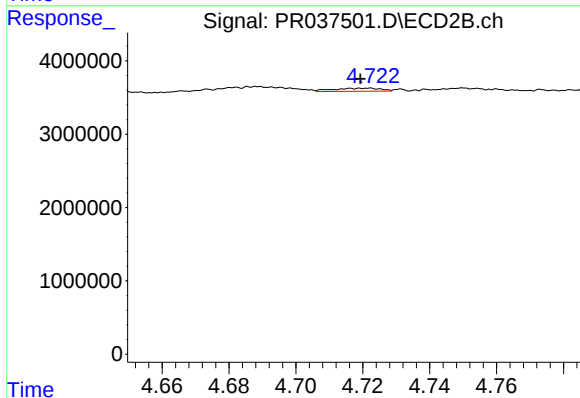


#23 AR-1248-3

R.T.: 4.722 min
Delta R.T.: 0.003 min
Response: 418524
Conc: 2.99 ng/ml

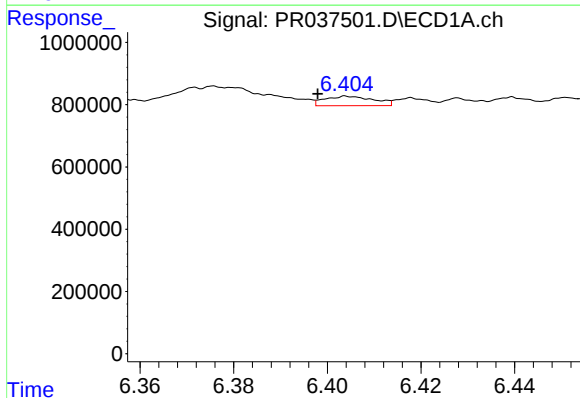


#24 AR-1248-4

R.T.: 6.405 min
Delta R.T.: 0.007 min
Response: 220286
Conc: 4.50 ng/ml

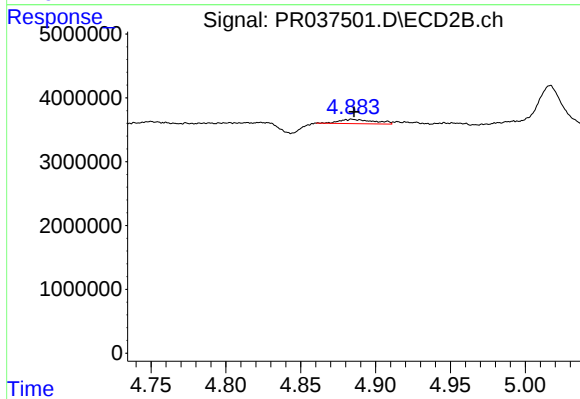

#24 AR-1248-4


R.T.: 4.884 min
Delta R.T.: -0.002 min
Response: 1103553
Conc: 6.20 ng/ml

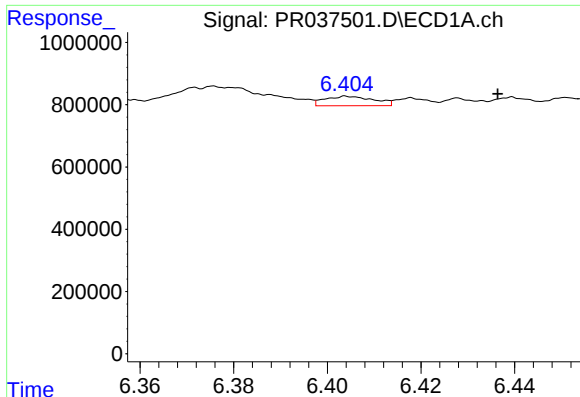

#25 AR-1248-5


R.T.: 6.405 min
Delta R.T.: -0.032 min
Response: 220286
Conc: 4.66 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

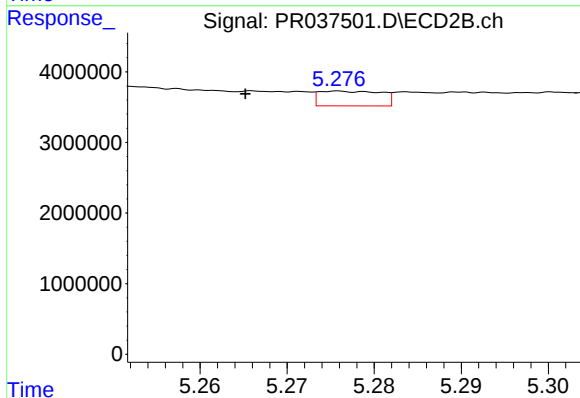


#25 AR-1248-5

R.T.: 5.276 min
Delta R.T.: 0.011 min
Response: 1031027
Conc: 5.27 ng/ml

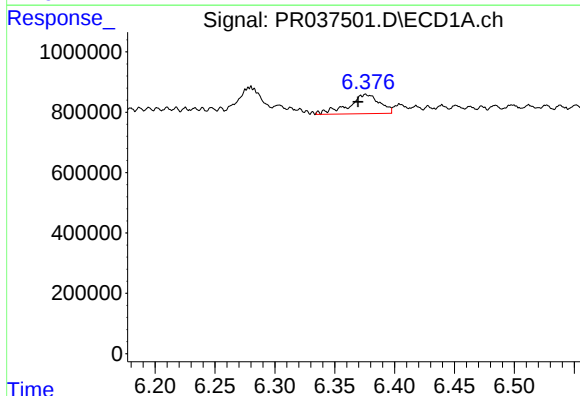


#26 AR-1254-1

R.T.: 6.376 min
Delta R.T.: 0.007 min
Response: 1152515
Conc: 21.10 ng/ml

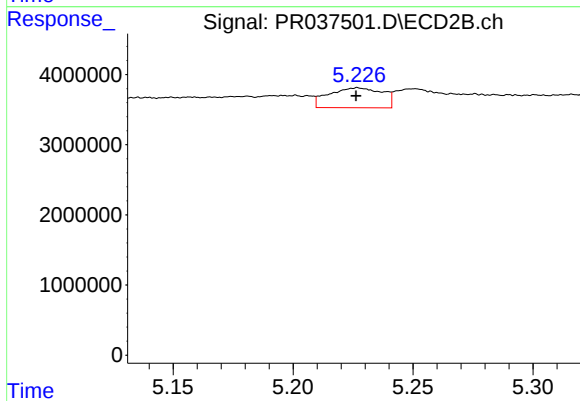

#26 AR-1254-1


R.T.: 5.227 min
Delta R.T.: 0.000 min
Response: 4413517
Conc: 12.81 ng/ml

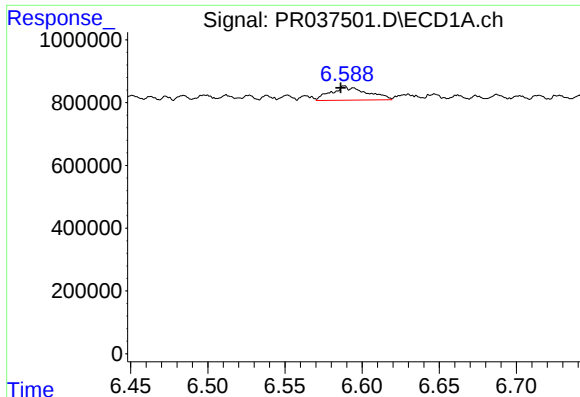

#27 AR-1254-2


R.T.: 6.589 min
Delta R.T.: 0.002 min
Response: 712256
Conc: 8.31 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

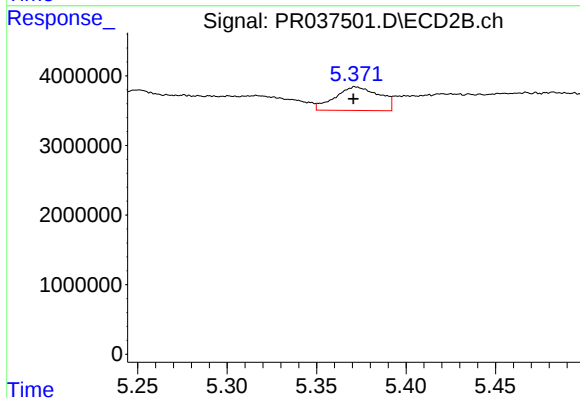


#27 AR-1254-2

R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 5857315
Conc: 19.56 ng/ml

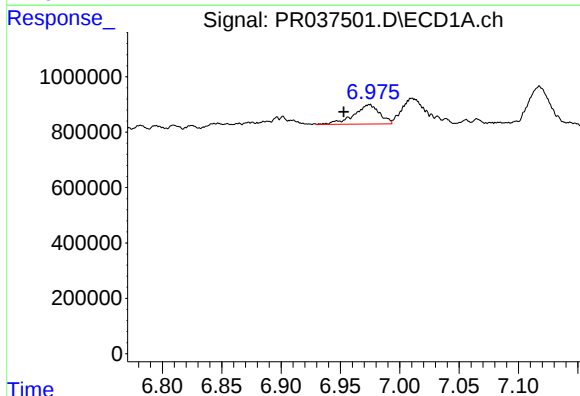


#28 AR-1254-3

R.T.: 6.974 min
Delta R.T.: 0.021 min
Response: 1059730
Conc: 11.65 ng/ml

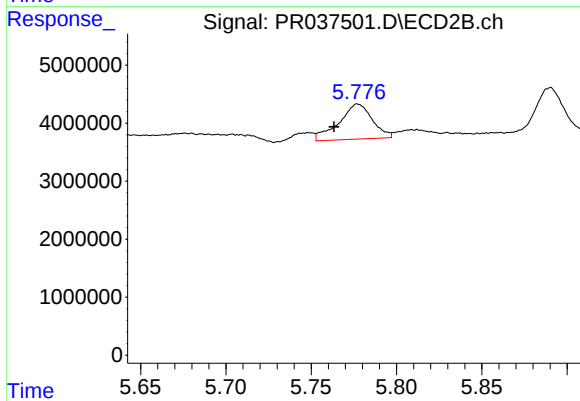

#28 AR-1254-3


R.T.: 5.777 min
Delta R.T.: 0.014 min
Response: 8197296
Conc: 17.31 ng/ml

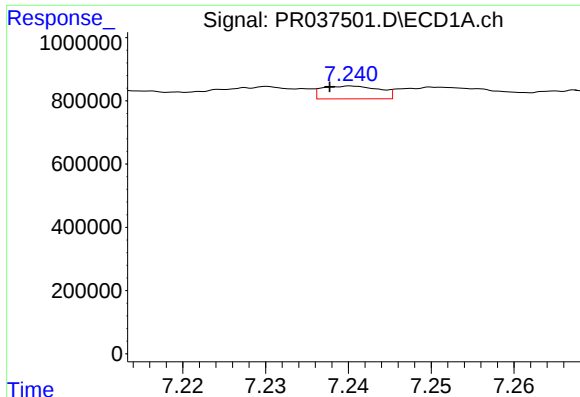

#29 AR-1254-4


R.T.: 7.240 min
Delta R.T.: 0.002 min
Response: 194805
Conc: 2.91 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

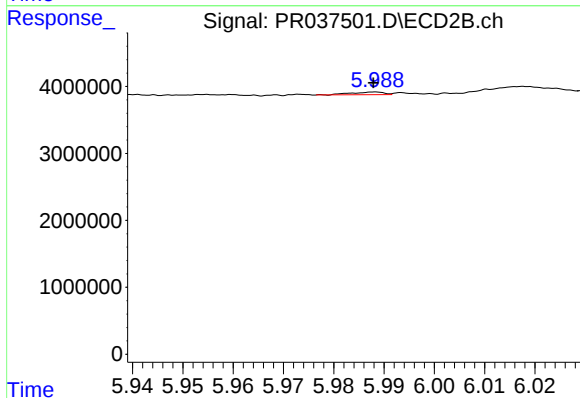


#29 AR-1254-4

R.T.: 5.988 min
Delta R.T.: 0.000 min
Response: 186344
Conc: 0.53 ng/ml

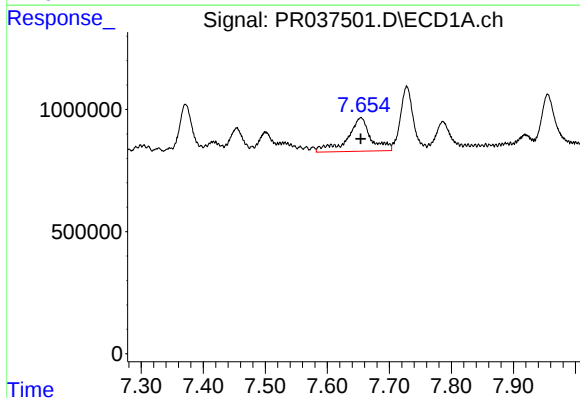


#30 AR-1254-5

R.T.: 7.654 min
Delta R.T.: 0.000 min
Response: 3628909
Conc: 50.49 ng/ml

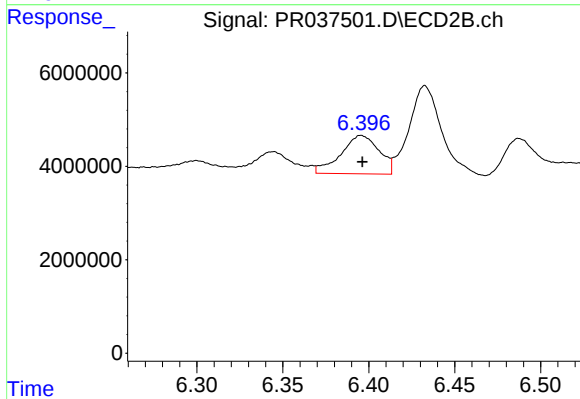

#30 AR-1254-5


R.T.: 6.395 min
Delta R.T.: 0.000 min
Response: 12738243
Conc: 28.77 ng/ml

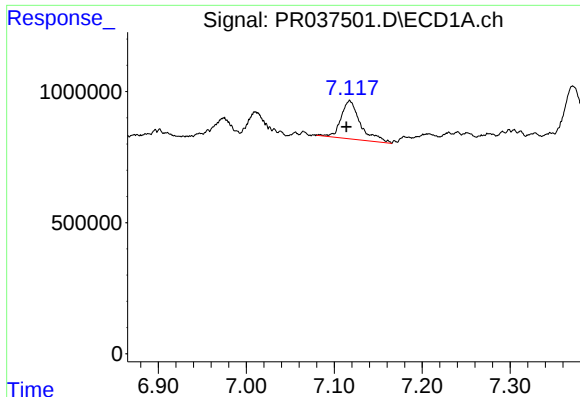

#31 AR-1260-1


R.T.: 7.118 min
Delta R.T.: 0.004 min
Response: 2226514
Conc: 33.74 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

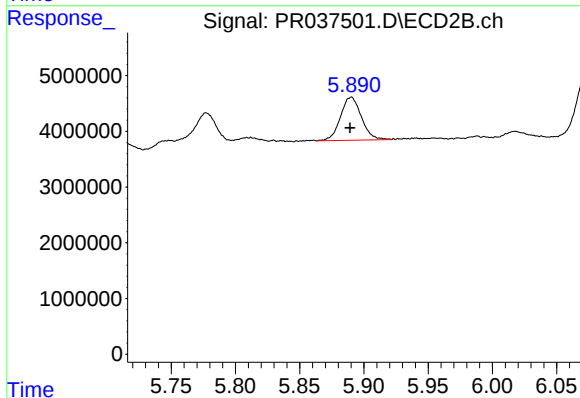


#31 AR-1260-1

R.T.: 5.890 min
Delta R.T.: 0.001 min
Response: 8745113
Conc: 29.92 ng/ml

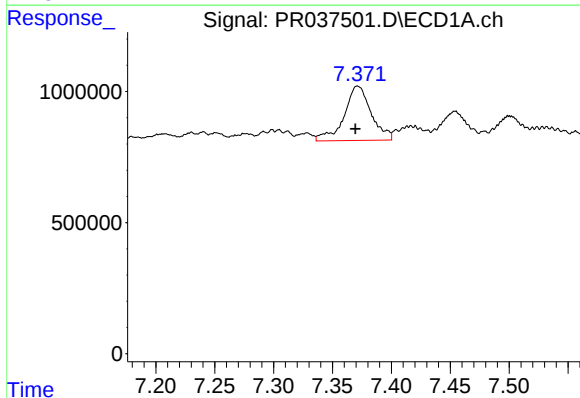


#32 AR-1260-2

R.T.: 7.371 min
Delta R.T.: 0.002 min
Response: 3308301
Conc: 41.51 ng/ml

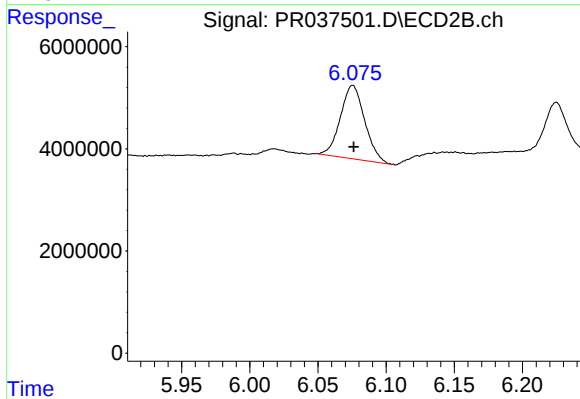

#32 AR-1260-2


R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 17759572
Conc: 38.56 ng/ml

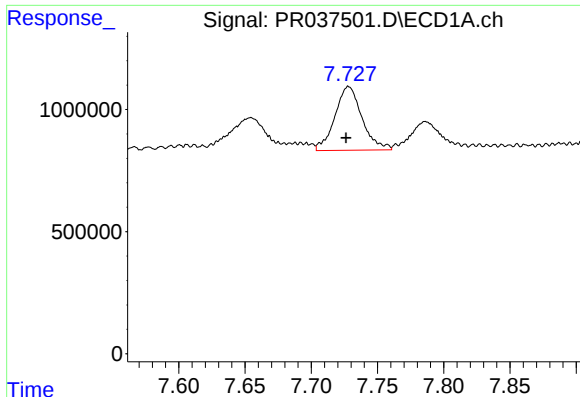

#33 AR-1260-3


R.T.: 7.728 min
Delta R.T.: 0.002 min
Response: 3721565
Conc: 59.47 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

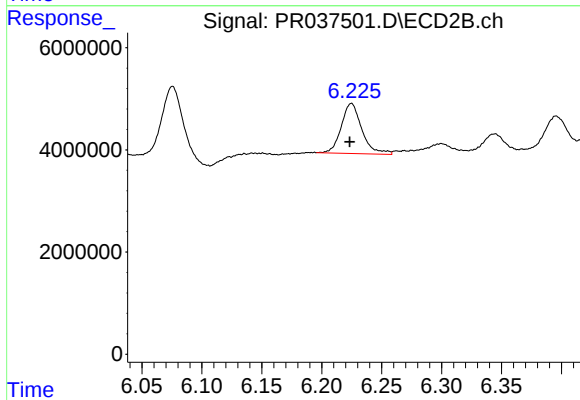


#33 AR-1260-3

R.T.: 6.225 min
Delta R.T.: 0.002 min
Response: 11720735
Conc: 32.88 ng/ml

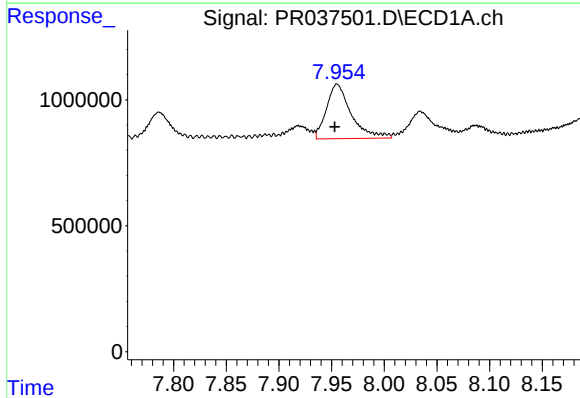


#34 AR-1260-4

R.T.: 7.955 min
Delta R.T.: 0.002 min
Response: 3541131
Conc: 47.59 ng/ml

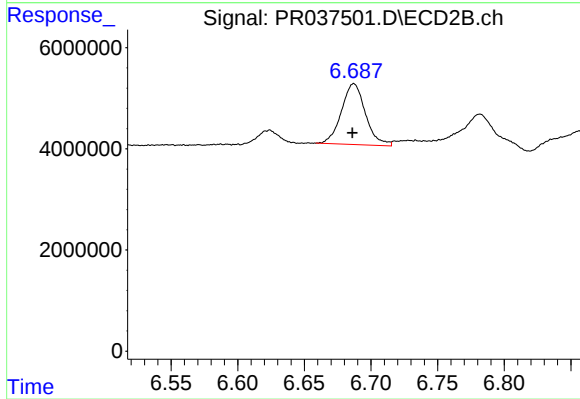

#34 AR-1260-4


R.T.: 6.687 min
Delta R.T.: 0.001 min
Response: 15112506
Conc: 49.59 ng/ml

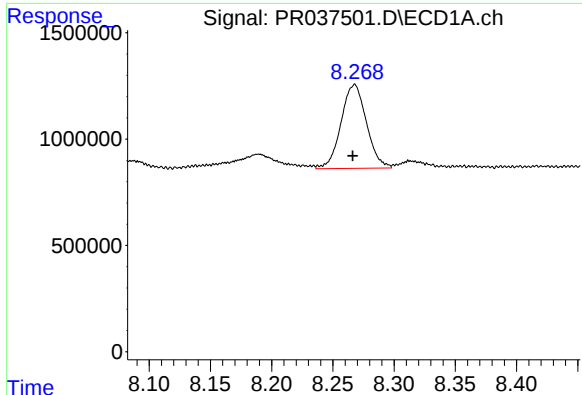

#35 AR-1260-5


R.T.: 8.268 min
Delta R.T.: 0.002 min
Response: 5690977
Conc: 39.35 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

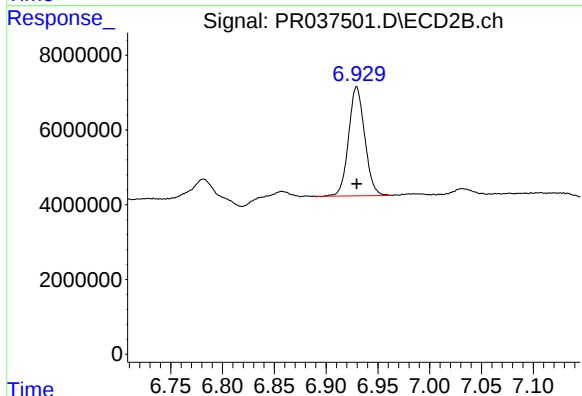


#35 AR-1260-5

R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 31692550
Conc: 36.54 ng/ml

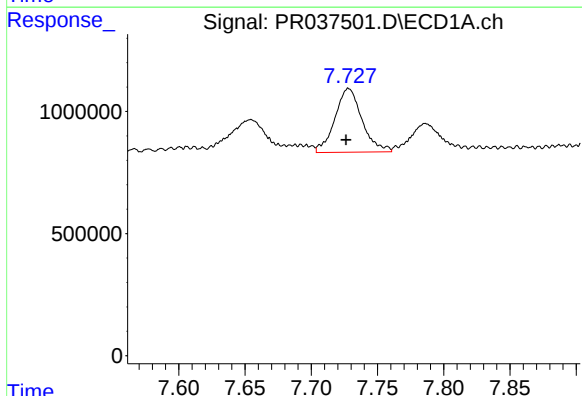


#36 AR-1262-1

R.T.: 7.728 min
Delta R.T.: 0.002 min
Response: 3721565
Conc: 35.63 ng/ml

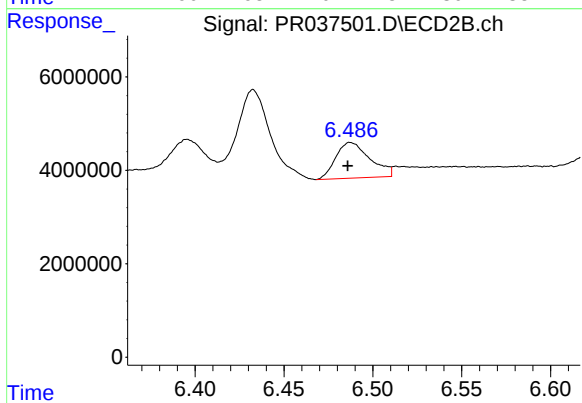

#36 AR-1262-1


R.T.: 6.487 min
Delta R.T.: 0.001 min
Response: 10218788
Conc: 40.77 ng/ml

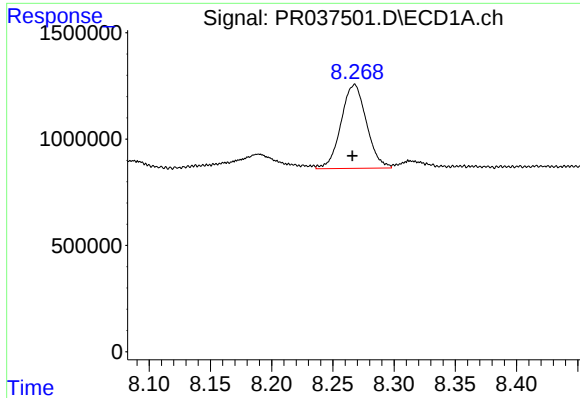

#37 AR-1262-2


R.T.: 8.268 min
Delta R.T.: 0.002 min
Response: 5690977
Conc: 29.28 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

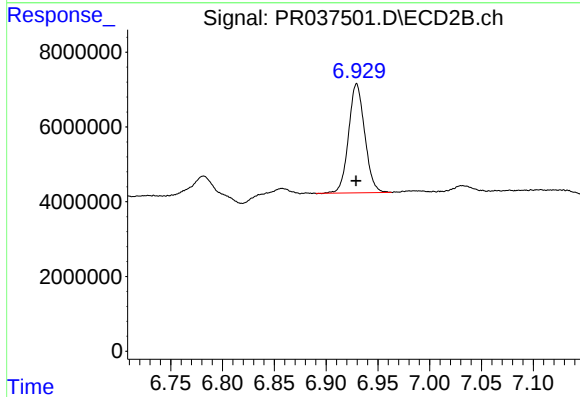


#37 AR-1262-2

R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 31692550
Conc: 25.23 ng/ml

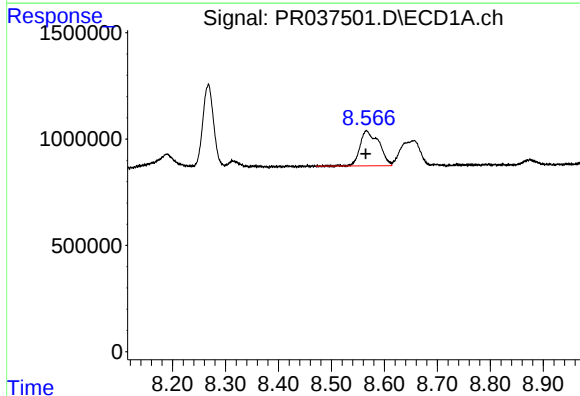


#38 AR-1262-3

R.T.: 8.566 min
Delta R.T.: 0.001 min
Response: 4112107
Conc: 31.27 ng/ml

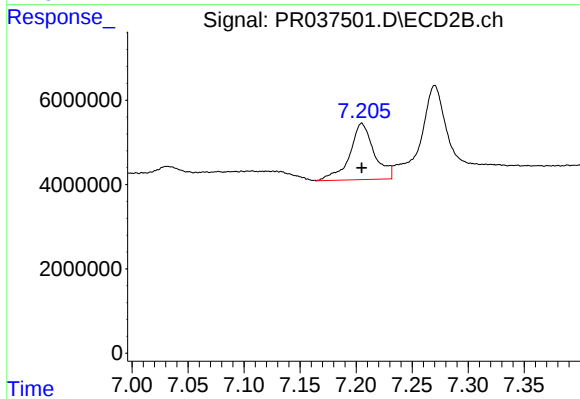

#38 AR-1262-3


R.T.: 7.205 min
Delta R.T.: 0.000 min
Response: 20326448
Conc: 37.07 ng/ml

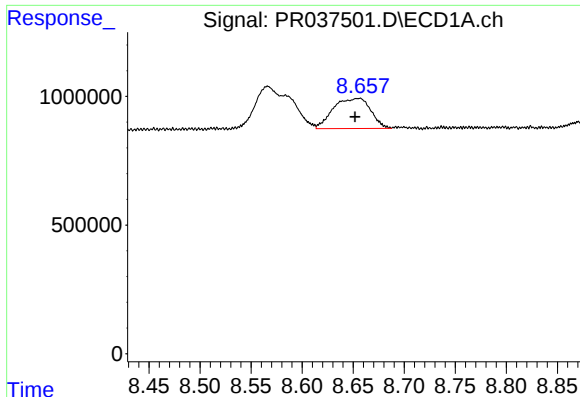

#39 AR-1262-4


R.T.: 8.656 min
Delta R.T.: 0.004 min
Response: 2979805
Conc: 30.34 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

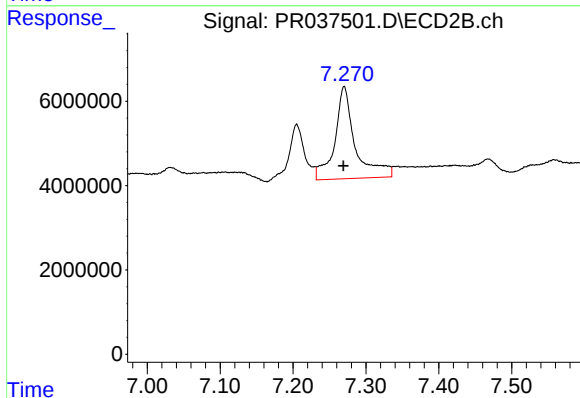


#39 AR-1262-4

R.T.: 7.270 min
Delta R.T.: 0.001 min
Response: 42655581
Conc: 47.52 ng/ml

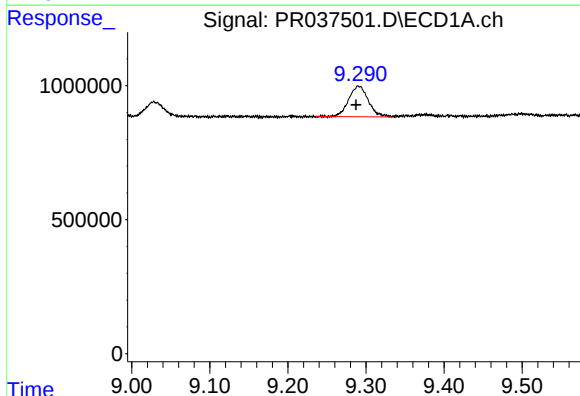


#40 AR-1262-5

R.T.: 9.290 min
Delta R.T.: 0.003 min
Response: 2011528
Conc: 29.14 ng/ml

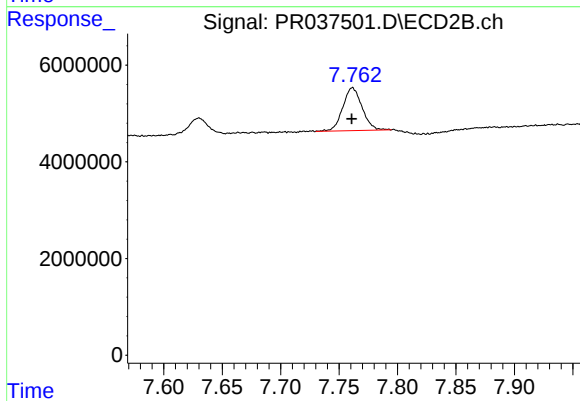

#40 AR-1262-5


R.T.: 7.761 min
Delta R.T.: 0.000 min
Response: 10178815
Conc: 26.60 ng/ml

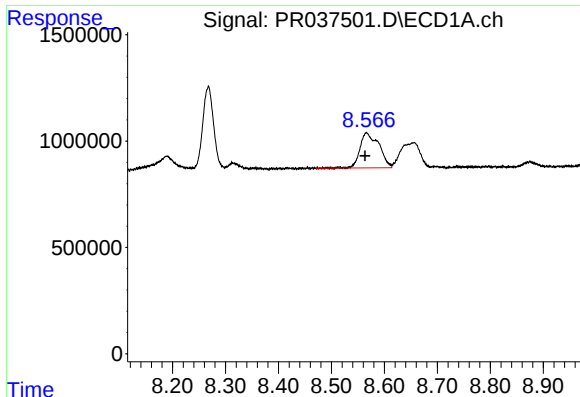

#41 AR-1268-1


R.T.: 8.566 min
Delta R.T.: 0.002 min
Response: 4112107
Conc: 22.96 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

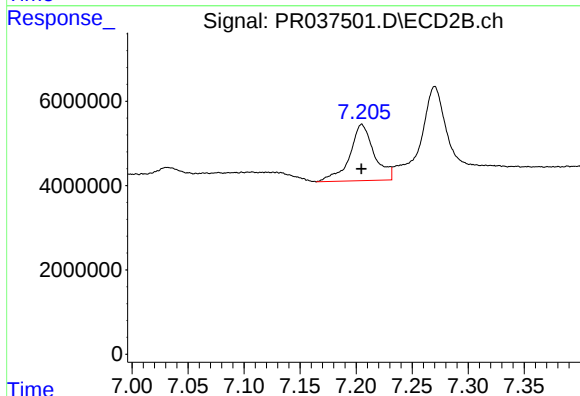


#41 AR-1268-1

R.T.: 7.205 min
Delta R.T.: 0.000 min
Response: 20326448
Conc: 16.51 ng/ml

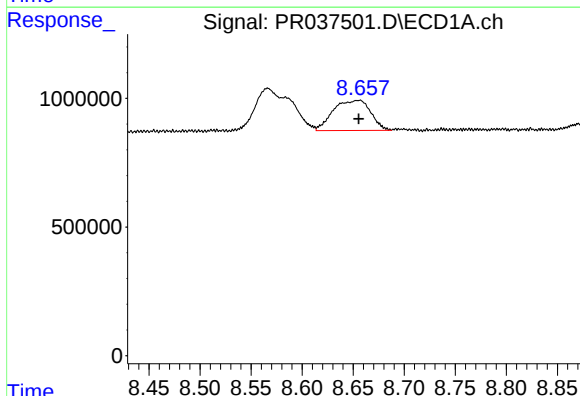


#42 AR-1268-2

R.T.: 8.656 min
Delta R.T.: 0.000 min
Response: 2979805
Conc: 18.11 ng/ml

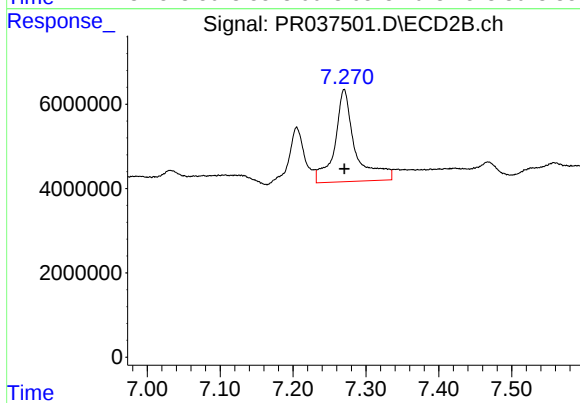

#42 AR-1268-2


R.T.: 7.270 min
Delta R.T.: 0.000 min
Response: 42655581
Conc: 40.28 ng/ml

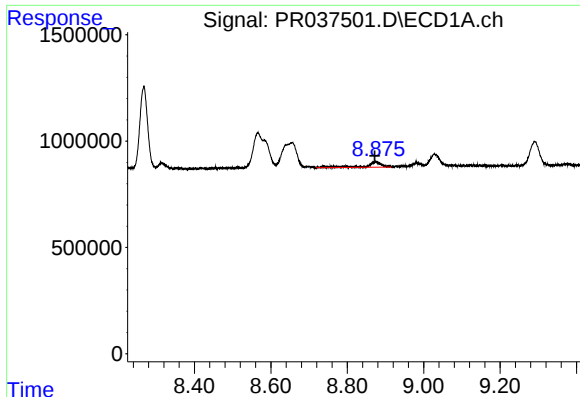

#43 AR-1268-3


R.T.: 8.875 min
Delta R.T.: 0.003 min
Response: 723172
Conc: 5.22 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

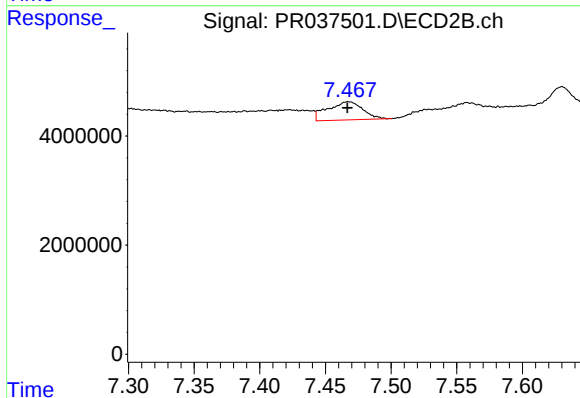


#43 AR-1268-3

R.T.: 7.468 min
Delta R.T.: 0.000 min
Response: 6225863
Conc: 7.03 ng/ml

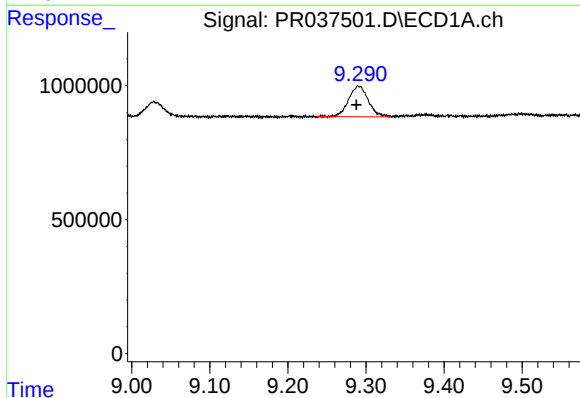


#44 AR-1268-4

R.T.: 9.290 min
Delta R.T.: 0.002 min
Response: 2011528
Conc: 32.24 ng/ml

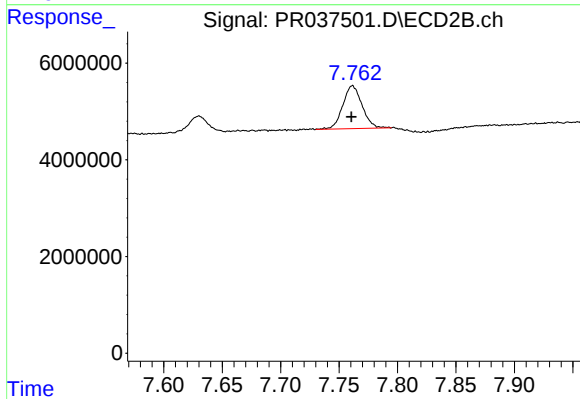

#44 AR-1268-4


R.T.: 7.761 min
Delta R.T.: 0.000 min
Response: 10178815
Conc: 28.06 ng/ml

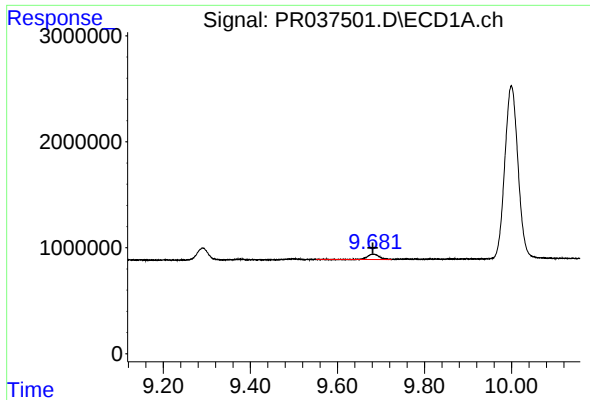

#45 AR-1268-5

R.T.: 9.681 min
Delta R.T.: 0.000 min
Response: 956041
Conc: 2.10 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

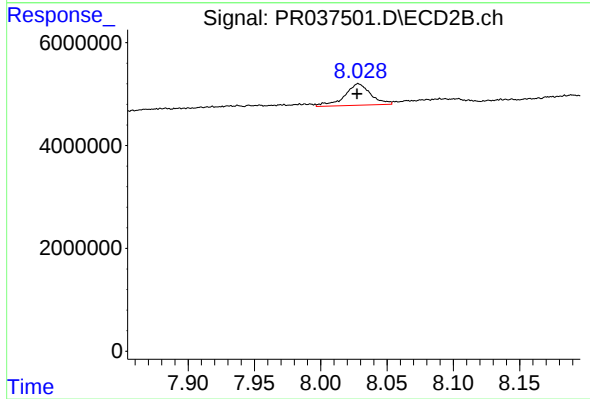

#45 AR-1268-5

R.T.: 8.028 min
Delta R.T.: 0.001 min
Response: 5746883
Conc: 2.26 ng/ml