

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR043019\
 Data File : PR037502.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2019 16:35
 Operator : SM\SJ
 Sample : K2241-09
 Misc : AR1221 MDL 25PPB
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 04:14:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.362	3.407	17335631	68715255	13.857	14.329
2)	SA Decachlor...	9.989	8.245	23988351	108.6E6	18.137	18.649
Target Compounds							
3)	L1 AR-1016-1	0.000	4.464	0	1198769	N.D.	6.584 #
4)	L1 AR-1016-2	0.000	4.469	0	503894	N.D.	1.786 #
5)	L1 AR-1016-3	0.000	4.634	0	318002	N.D.	2.212 #
6)	L1 AR-1016-4	0.000	4.686	0	489622	N.D.	4.426 #
7)	L1 AR-1016-5	0.000	4.882	0	862484	N.D.	5.674 #
8)	L2 AR-1221-1	4.571	3.612	542423	2322146	43.383	45.605
9)	L2 AR-1221-2	4.664	3.695	577765	2461660	63.884	66.288
10)	L2 AR-1221-3	4.734	3.768	1318817	4931349	43.030	40.273
11)	L3 AR-1232-1	4.734	3.768	1318817	4931349	45.086	42.151
12)	L3 AR-1232-2	0.000	4.469	0	503894	N.D.	3.645 #
13)	L3 AR-1232-3	0.000	4.634	0	318002	N.D.	4.530 #
14)	L3 AR-1232-4	0.000	4.699	0	80251	N.D.	1.345 #
15)	L3 AR-1232-5	0.000	4.882	0	862484	N.D.	12.638 #
16)	L4 AR-1242-1	0.000	4.464	0	1198769	N.D.	8.181 #
17)	L4 AR-1242-2	0.000	4.469	0	503894	N.D.	2.209 #
18)	L4 AR-1242-3	0.000	4.634	0	318002	N.D.	2.750 #
19)	L4 AR-1242-4	0.000	4.739	0	65614	N.D.	0.597 #
20)	L4 AR-1242-5	6.371	5.249	930642	11678866	28.921	70.482 #
21)	L5 AR-1248-1	0.000	4.464	0	1198769	N.D.	11.909 #
22)	L5 AR-1248-2	0.000	4.686	0	489622	N.D.	3.588 #
23)	L5 AR-1248-3	0.000	4.739	0	65614	N.D.	0.469 #
24)	L5 AR-1248-4	6.371	4.882	930642	862484	19.010	4.846 #
25)	L5 AR-1248-5	6.371	5.275	930642	1327025	19.701	6.784 #
26)	L6 AR-1254-1	6.371	5.249	930642	11678866	17.035	33.904 #
27)	L6 AR-1254-2	0.000	5.383	0	11099041	N.D.	37.058 #
28)	L6 AR-1254-3	6.969	5.776	1295344	6623328	14.240	13.984
29)	L6 AR-1254-4	0.000	6.038	0	209634	N.D.	0.598 #
30)	L6 AR-1254-5	0.000	6.396	0	12863170	N.D.	29.048 #
31)	L7 AR-1260-1	0.000	5.900	0	253924	N.D.	0.869 #
32)	L7 AR-1260-2	7.370	6.068	54294	5636359	0.681	12.237 #
33)	L7 AR-1260-3	0.000	6.279	0	3602557	N.D.	10.105 #
34)	L7 AR-1260-4	0.000	6.734	0	2585761	N.D.	8.484 #
35)	L7 AR-1260-5	0.000	6.927	0	641821	N.D.	0.740 #
36)	L8 AR-1262-1	0.000	6.496	0	6424038	N.D.	25.633 #
37)	L8 AR-1262-2	0.000	6.927	0	641821	N.D.	0.511 #
38)	L8 AR-1262-3	8.580	7.269	194374	22638976	1.478	41.292 #
39)	L8 AR-1262-4	0.000	7.269	0	22638976	N.D.	25.220 #
40)	L8 AR-1262-5	0.000	7.781	0	643259	N.D.	1.681 #
41)	L9 AR-1268-1	8.580	7.269	194374	22638976	1.085	18.390 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR043019\
 Data File : PR037502.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Apr 2019 16:35
 Operator : SM\SJ
 Sample : K2241-09
 Misc : AR1221 MDL 25PPB
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 01 04:14:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Apr 22 17:27:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.269	0	22638976	N.D.	21.379 #
43) L9	AR-1268-3	0.000	7.466	0	27711190	N.D.	31.268 #
44) L9	AR-1268-4	0.000	7.781	0	643259	N.D.	1.773 #
45) L9	AR-1268-5	0.000	8.026	0	3952013	N.D.	1.553 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR043019\
Data File : PR037502.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Apr 2019 16:35
Operator : SM\SJ
Sample : K2241-09
Misc : AR1221 MDL 25PPB
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 01 04:14:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042219.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Apr 22 17:27:39 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

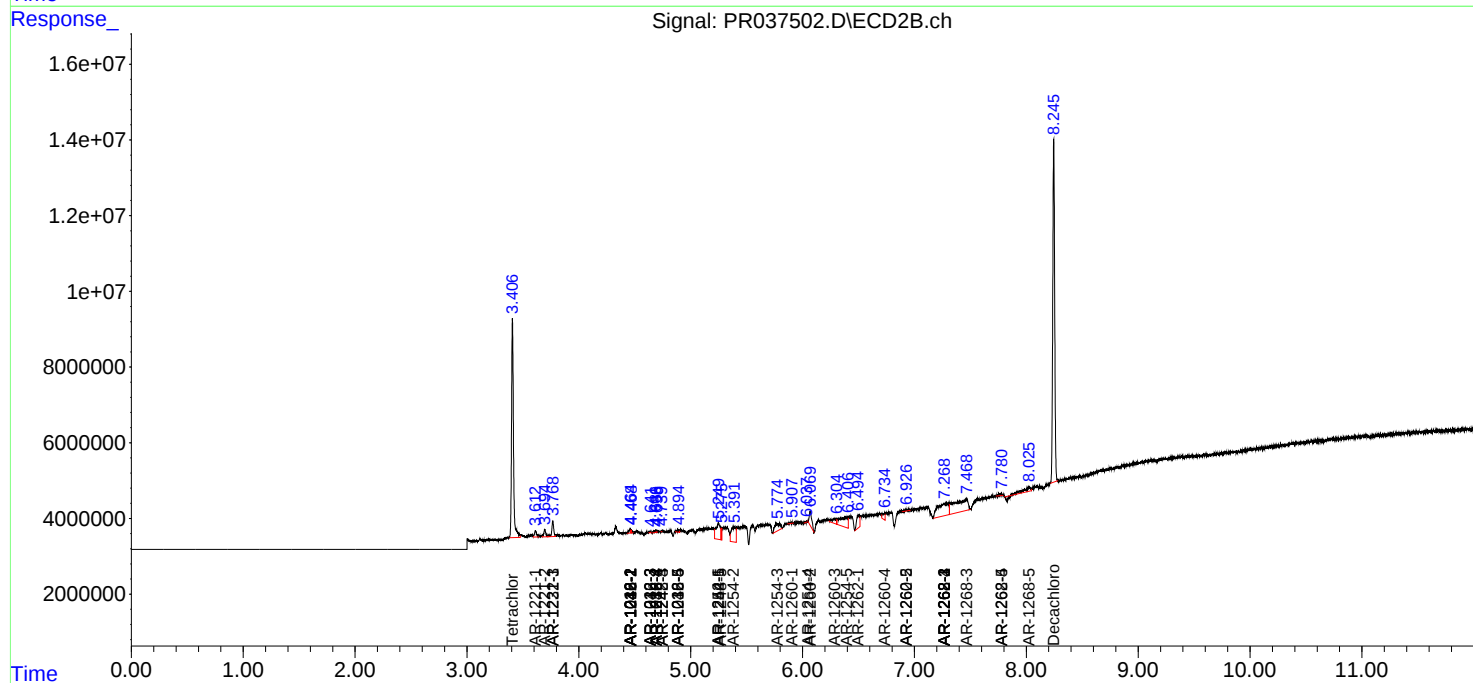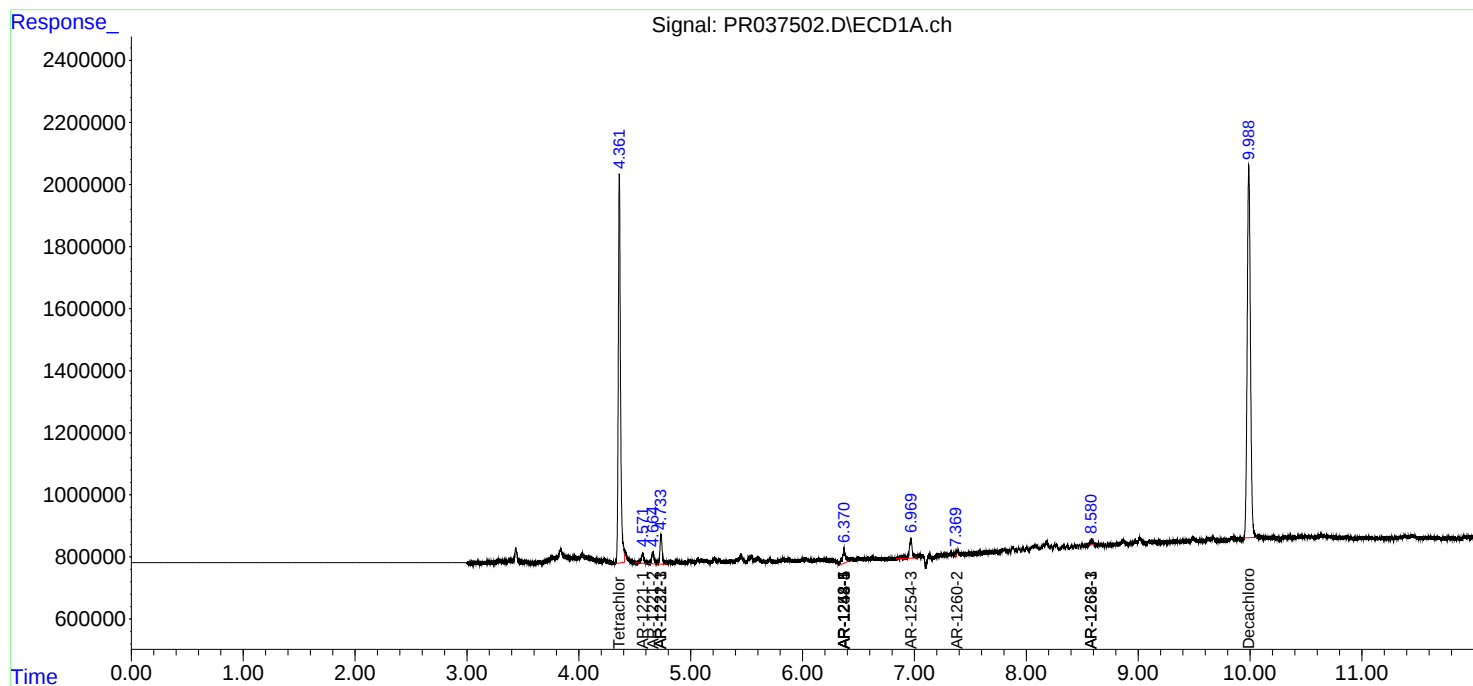


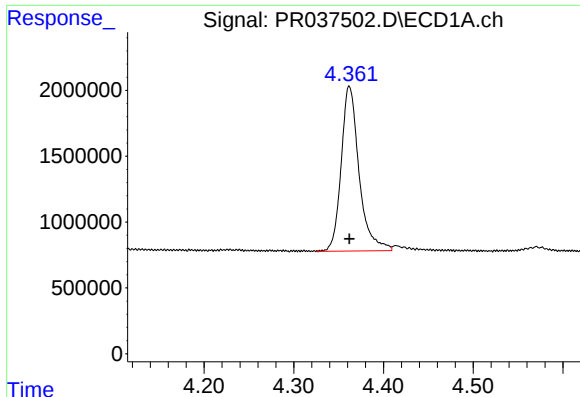

#1 Tetrachloro-m-xylene


R.T.: 4.362 min
Delta R.T.: 0.000 min
Response: 17335631
Conc: 13.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

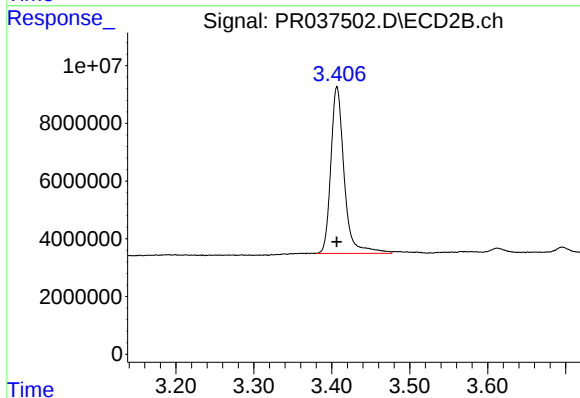


#1 Tetrachloro-m-xylene

R.T.: 3.407 min
Delta R.T.: 0.000 min
Response: 68715255
Conc: 14.33 ng/ml

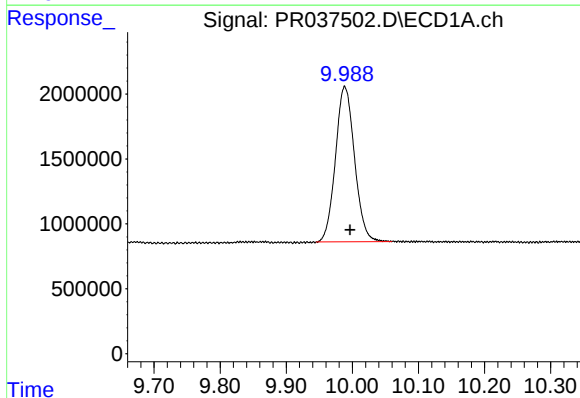


#2 Decachlorobiphenyl

R.T.: 9.989 min
Delta R.T.: -0.008 min
Response: 23988351
Conc: 18.14 ng/ml

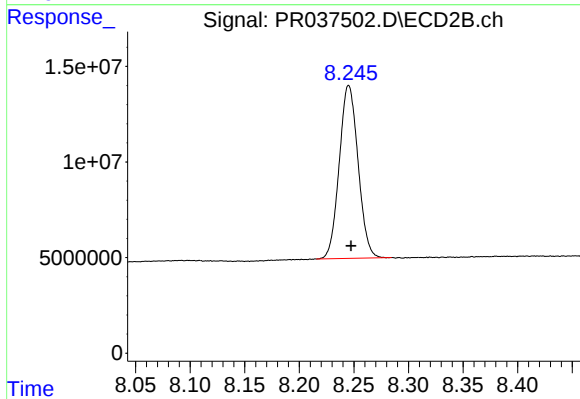

#2 Decachlorobiphenyl


R.T.: 8.245 min
Delta R.T.: -0.002 min
Response: 108614056
Conc: 18.65 ng/ml

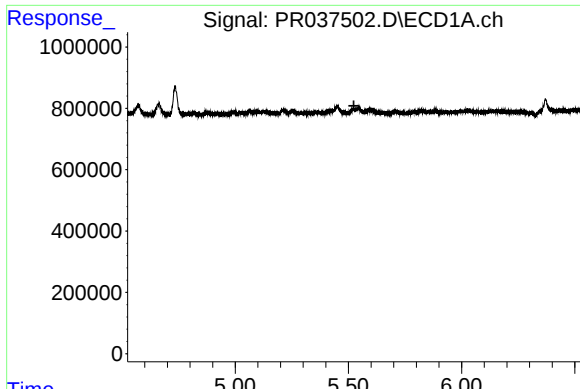

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

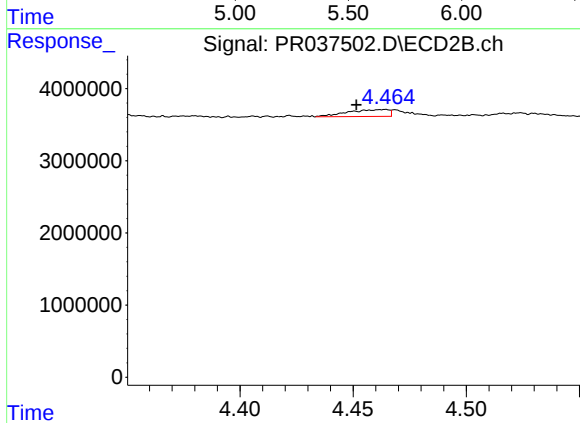


#3 AR-1016-1

R.T.: 4.464 min
Delta R.T.: 0.013 min
Response: 1198769
Conc: 6.58 ng/ml

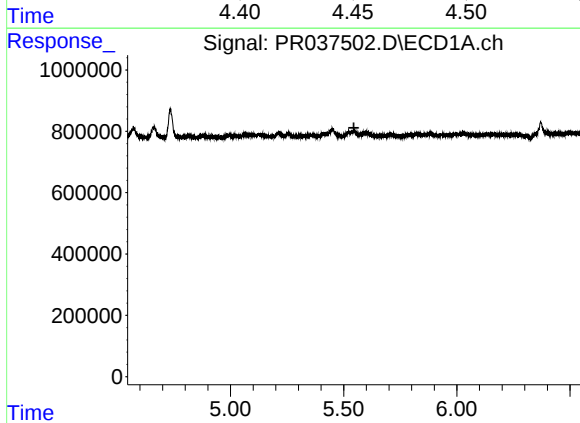


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

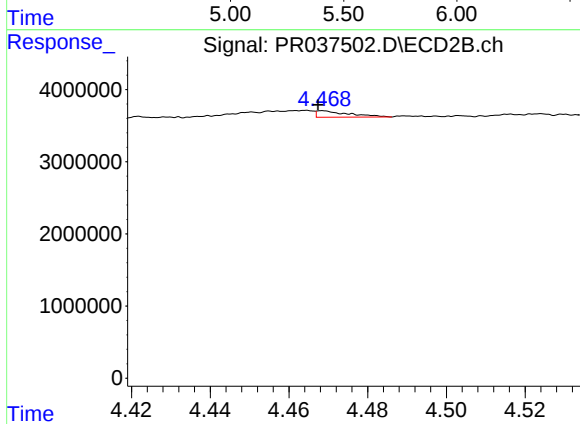

#4 AR-1016-2


R.T.: 4.469 min
Delta R.T.: 0.001 min
Response: 503894
Conc: 1.79 ng/ml

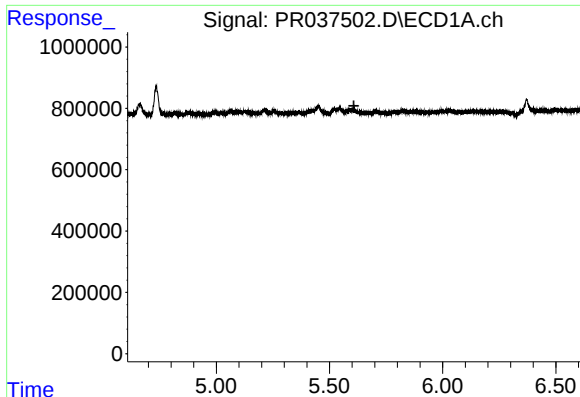

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

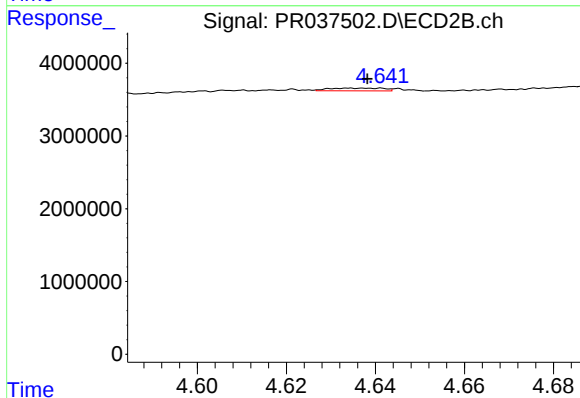


#5 AR-1016-3

R.T.: 4.634 min
Delta R.T.: -0.004 min
Response: 318002
Conc: 2.21 ng/ml

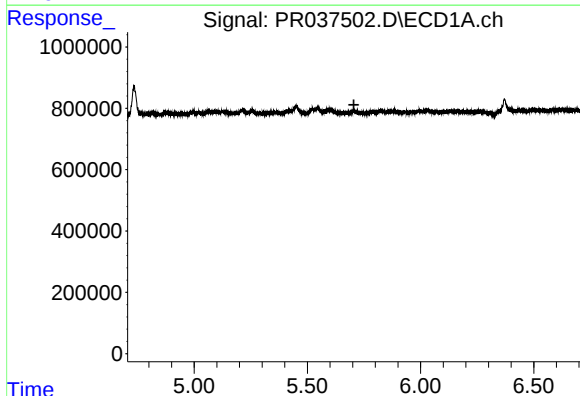


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.705 min
Response: 0
Conc: N.D.

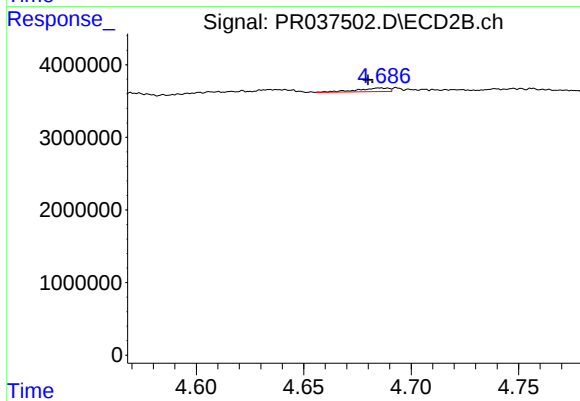

#6 AR-1016-4


R.T.: 4.686 min
Delta R.T.: 0.006 min
Response: 489622
Conc: 4.43 ng/ml

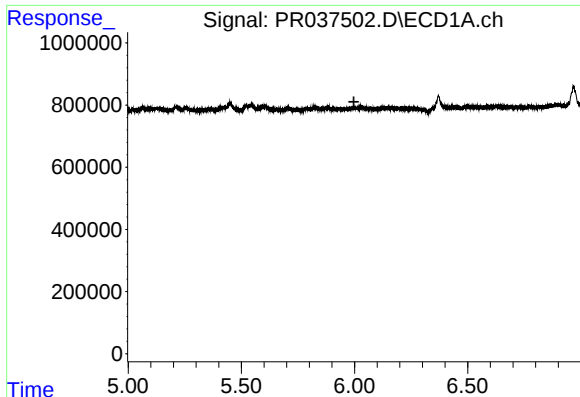

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

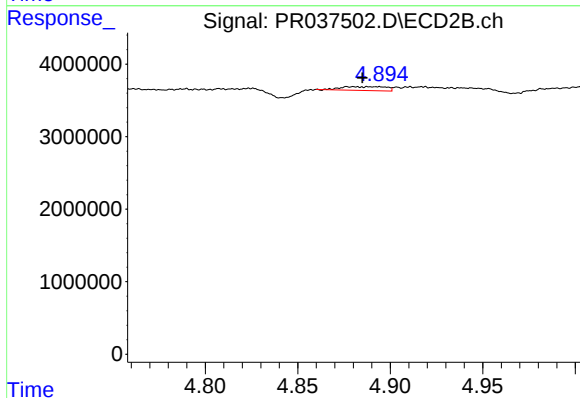


#7 AR-1016-5

R.T.: 4.882 min
Delta R.T.: -0.003 min
Response: 862484
Conc: 5.67 ng/ml

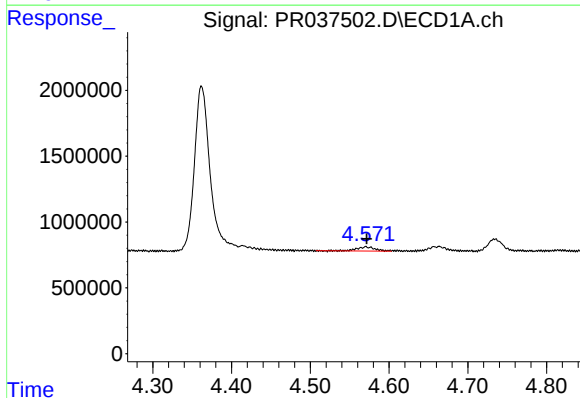


#8 AR-1221-1

R.T.: 4.571 min
Delta R.T.: -0.001 min
Response: 542423
Conc: 43.38 ng/ml

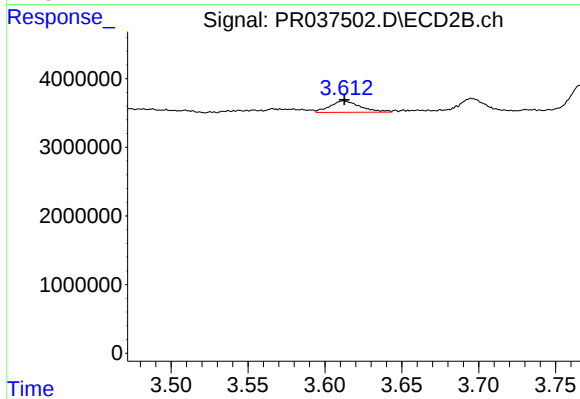

#8 AR-1221-1


R.T.: 3.612 min
Delta R.T.: 0.000 min
Response: 2322146
Conc: 45.61 ng/ml

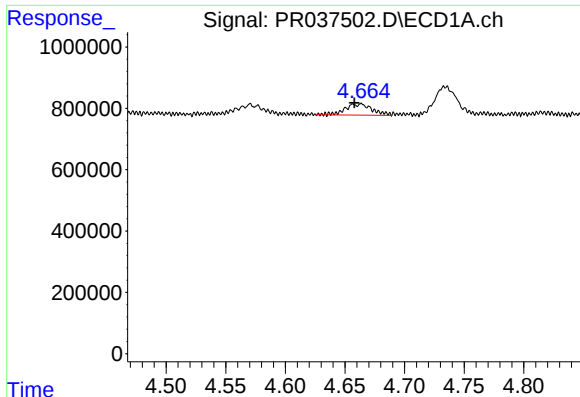

#9 AR-1221-2


R.T.: 4.664 min
Delta R.T.: 0.006 min
Response: 577765
Conc: 63.88 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

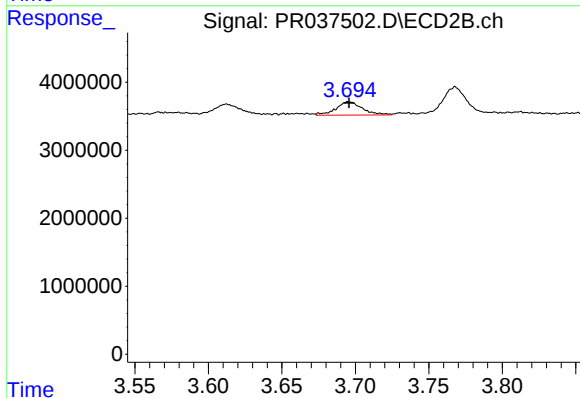


#9 AR-1221-2

R.T.: 3.695 min
Delta R.T.: 0.000 min
Response: 2461660
Conc: 66.29 ng/ml

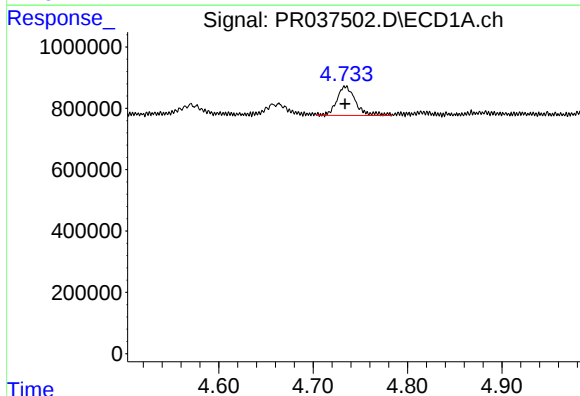


#10 AR-1221-3

R.T.: 4.734 min
Delta R.T.: 0.000 min
Response: 1318817
Conc: 43.03 ng/ml

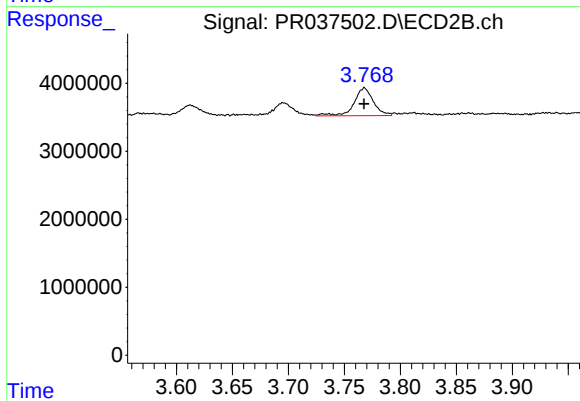

#10 AR-1221-3


R.T.: 3.768 min
Delta R.T.: 0.000 min
Response: 4931349
Conc: 40.27 ng/ml

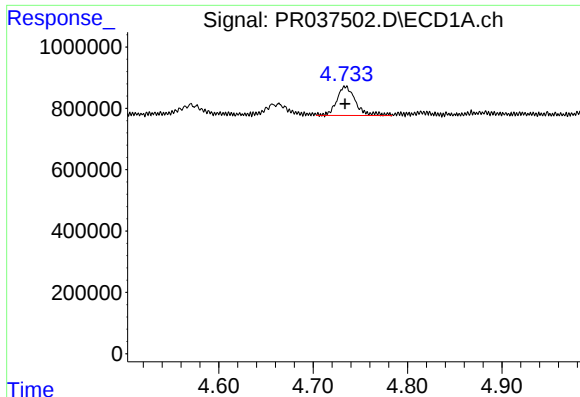

#11 AR-1232-1


R.T.: 4.734 min
Delta R.T.: 0.000 min
Response: 1318817
Conc: 45.09 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

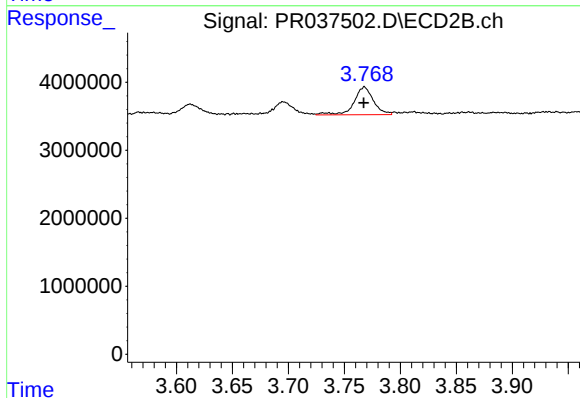


#11 AR-1232-1

R.T.: 3.768 min
Delta R.T.: 0.000 min
Response: 4931349
Conc: 42.15 ng/ml

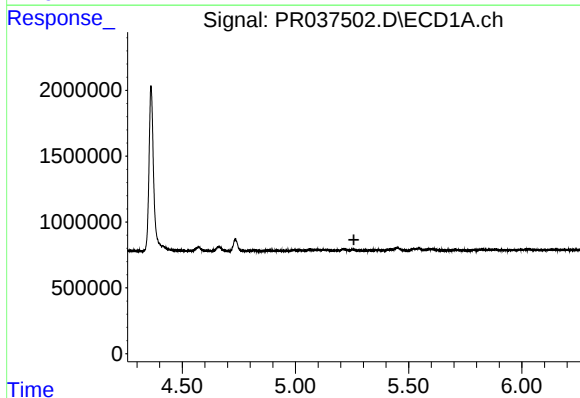


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

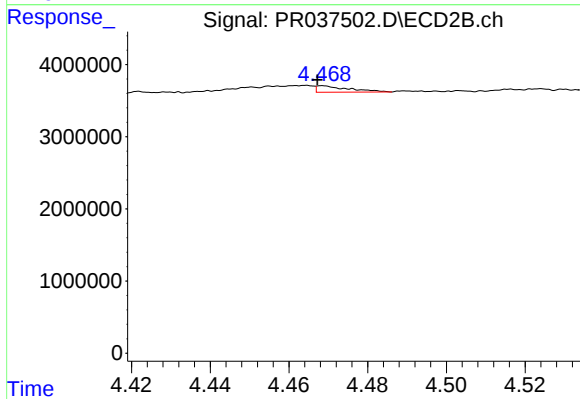

#12 AR-1232-2


R.T.: 4.469 min
Delta R.T.: 0.001 min
Response: 503894
Conc: 3.65 ng/ml

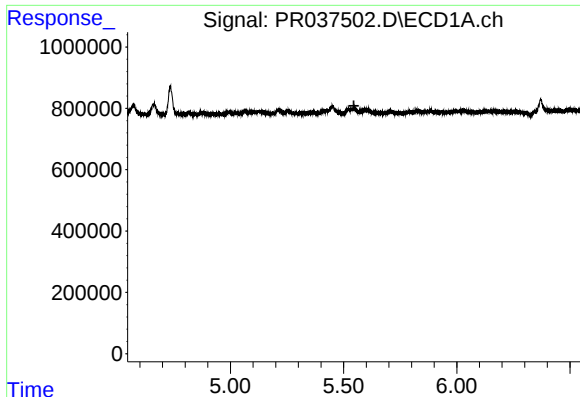

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

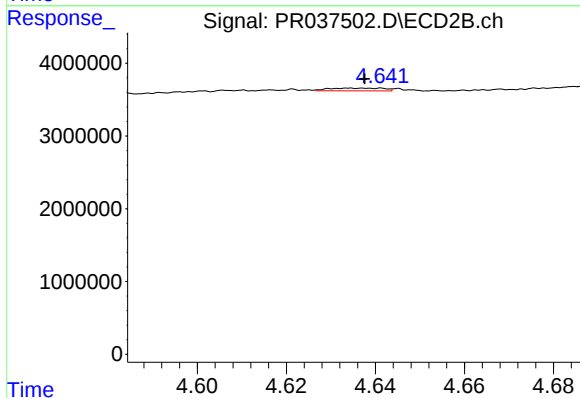


#13 AR-1232-3

R.T.: 4.634 min
Delta R.T.: -0.003 min
Response: 318002
Conc: 4.53 ng/ml

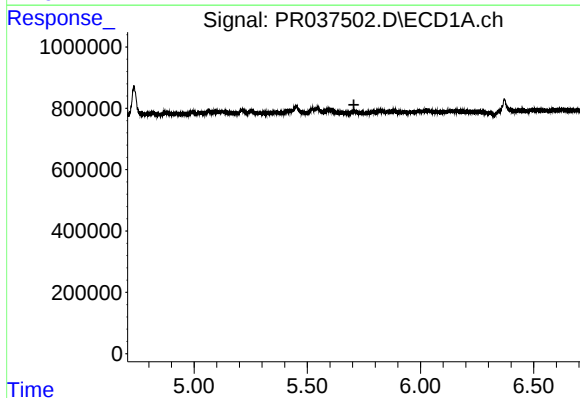


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

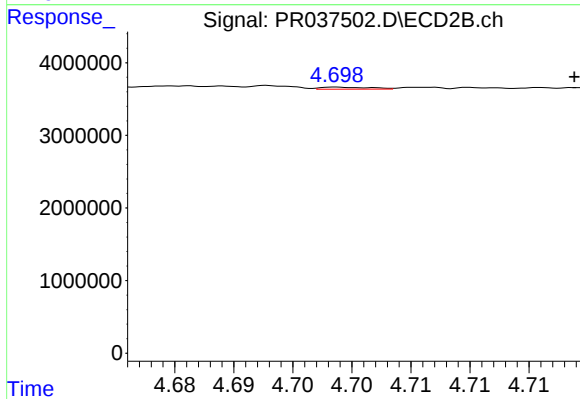

#14 AR-1232-4


R.T.: 4.699 min
Delta R.T.: -0.020 min
Response: 80251
Conc: 1.34 ng/ml

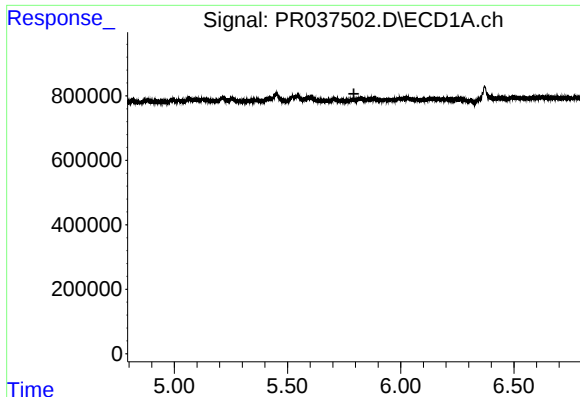

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

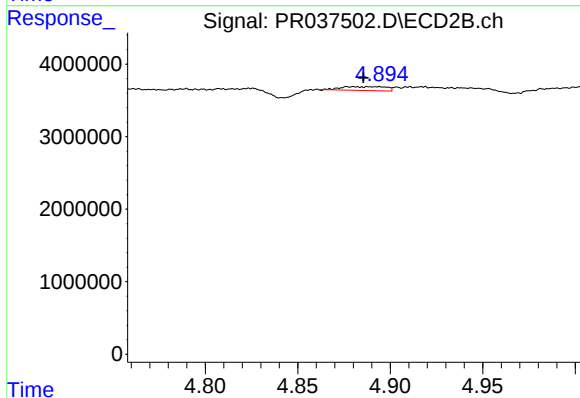


#15 AR-1232-5

R.T.: 4.882 min
Delta R.T.: -0.003 min
Response: 862484
Conc: 12.64 ng/ml

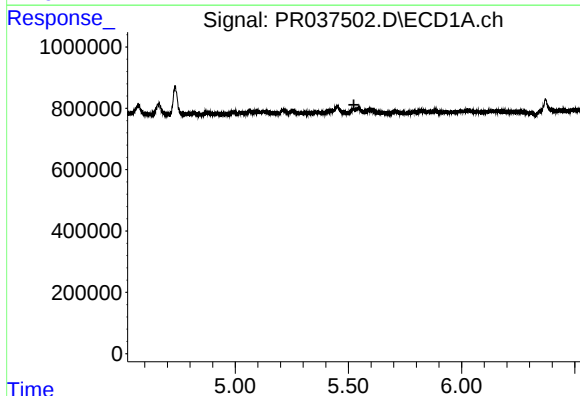


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

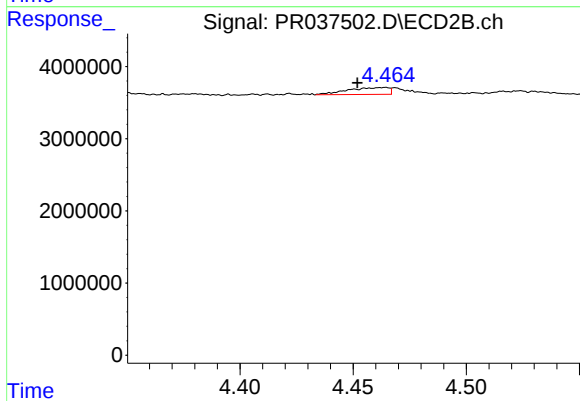

#16 AR-1242-1


R.T.: 4.464 min
Delta R.T.: 0.012 min
Response: 1198769
Conc: 8.18 ng/ml

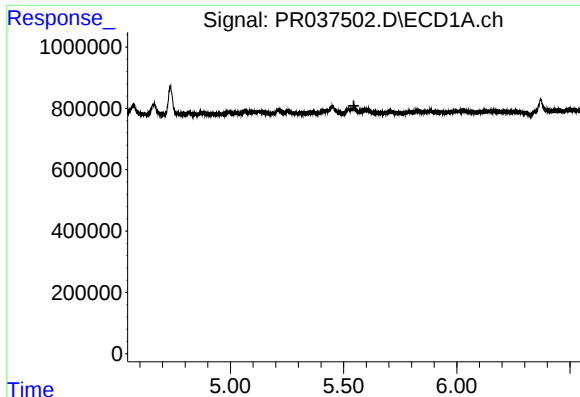

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

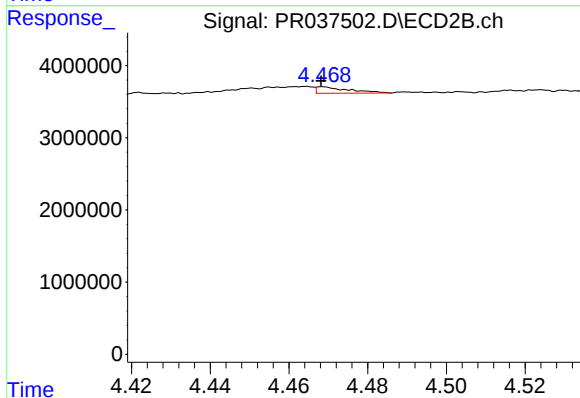


#17 AR-1242-2

R.T.: 4.469 min
Delta R.T.: 0.000 min
Response: 503894
Conc: 2.21 ng/ml

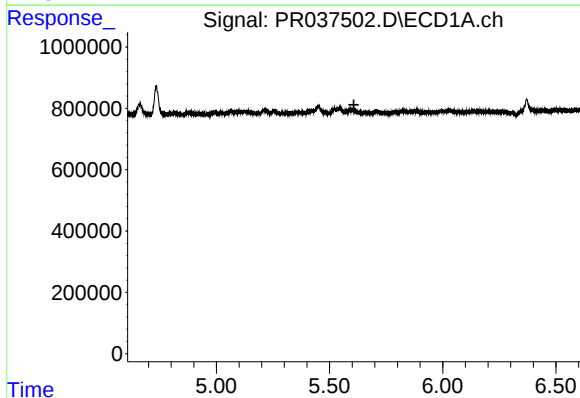


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.608 min
Response: 0
Conc: N.D.

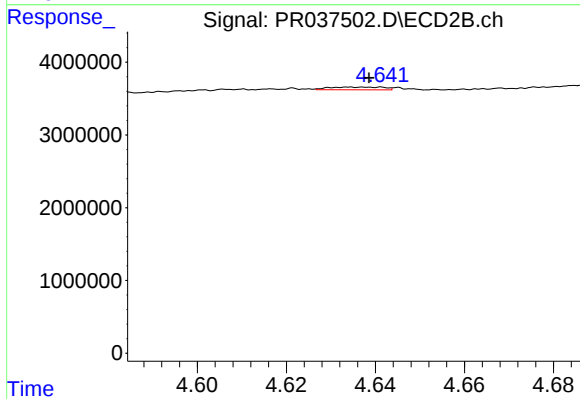

#18 AR-1242-3


R.T.: 4.634 min
Delta R.T.: -0.004 min
Response: 318002
Conc: 2.75 ng/ml

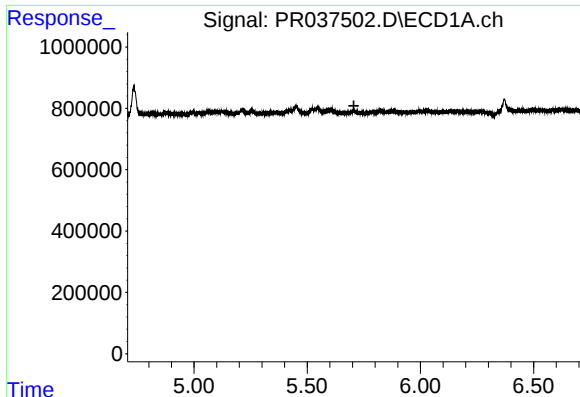

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

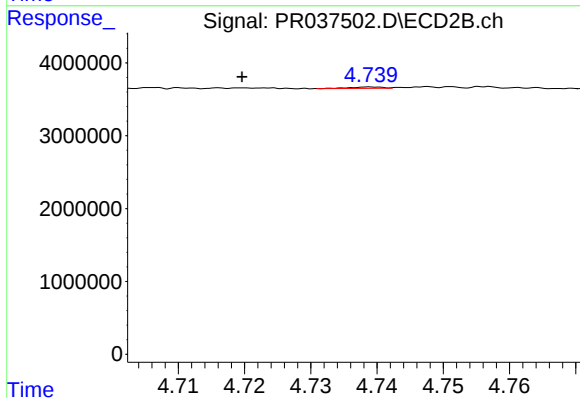


#19 AR-1242-4

R.T.: 4.739 min
Delta R.T.: 0.020 min
Response: 65614
Conc: 0.60 ng/ml

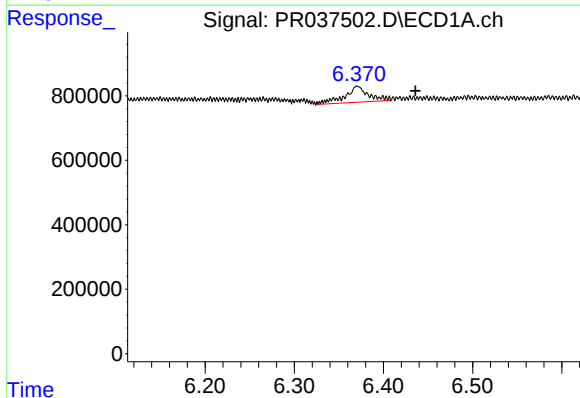


#20 AR-1242-5

R.T.: 6.371 min
Delta R.T.: -0.065 min
Response: 930642
Conc: 28.92 ng/ml

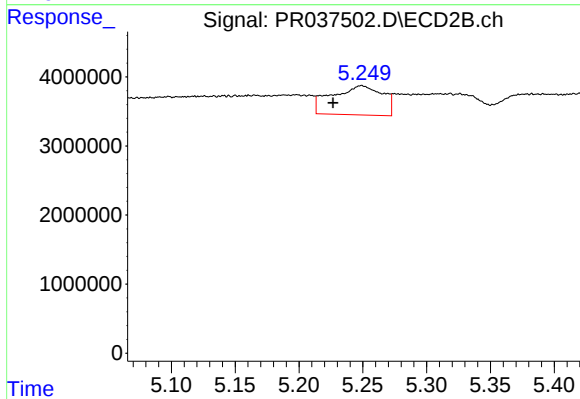

#20 AR-1242-5


R.T.: 5.249 min
Delta R.T.: 0.023 min
Response: 11678866
Conc: 70.48 ng/ml

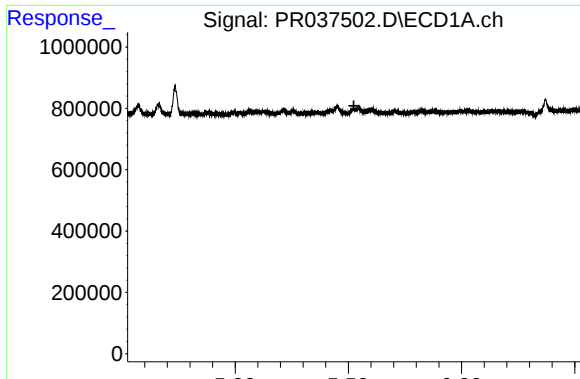

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

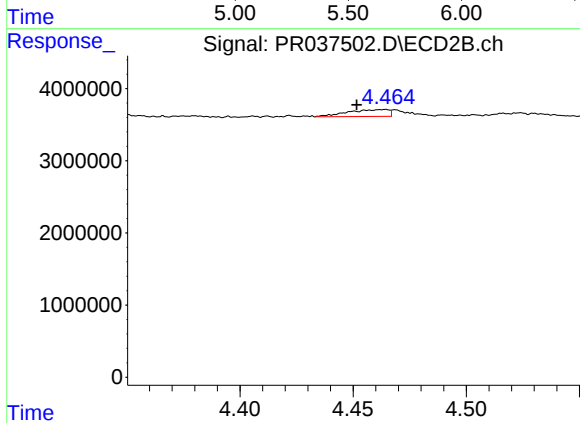


#21 AR-1248-1

R.T.: 4.464 min
Delta R.T.: 0.013 min
Response: 1198769
Conc: 11.91 ng/ml

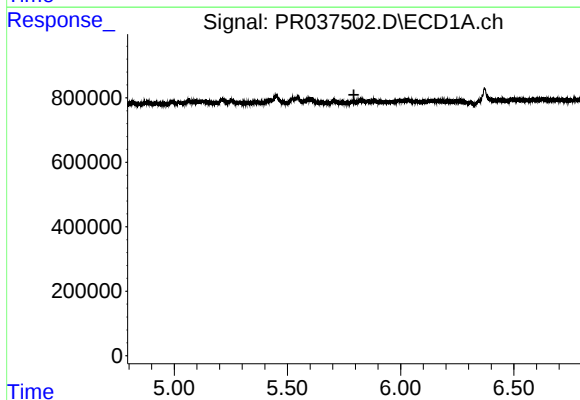


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 5.793 min
Response: 0
Conc: N.D.

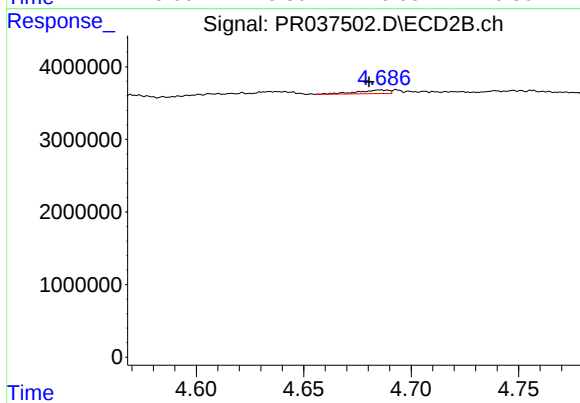

#22 AR-1248-2


R.T.: 4.686 min
Delta R.T.: 0.005 min
Response: 489622
Conc: 3.59 ng/ml

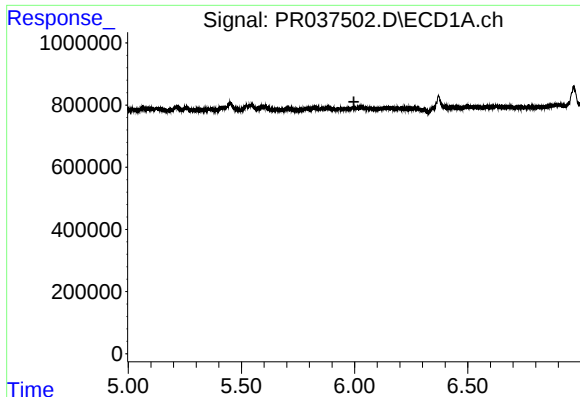

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

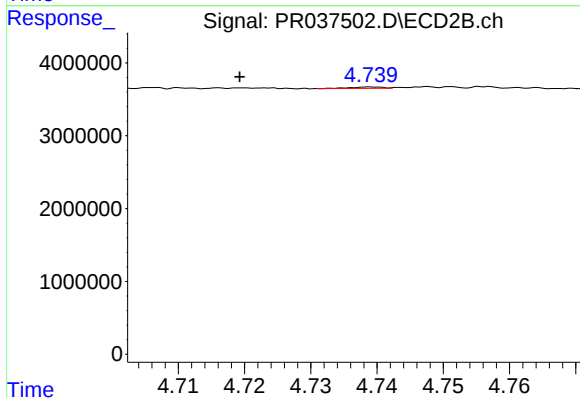


#23 AR-1248-3

R.T.: 4.739 min
Delta R.T.: 0.020 min
Response: 65614
Conc: 0.47 ng/ml

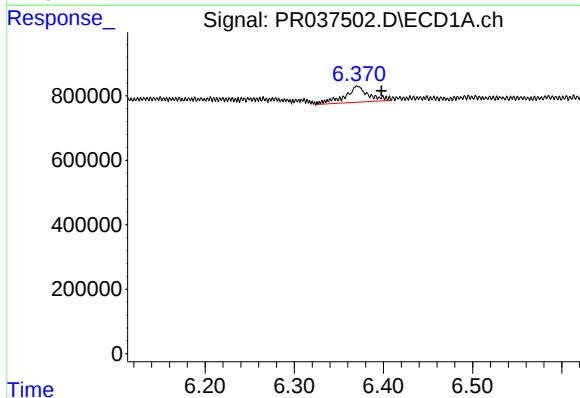


#24 AR-1248-4

R.T.: 6.371 min
Delta R.T.: -0.027 min
Response: 930642
Conc: 19.01 ng/ml

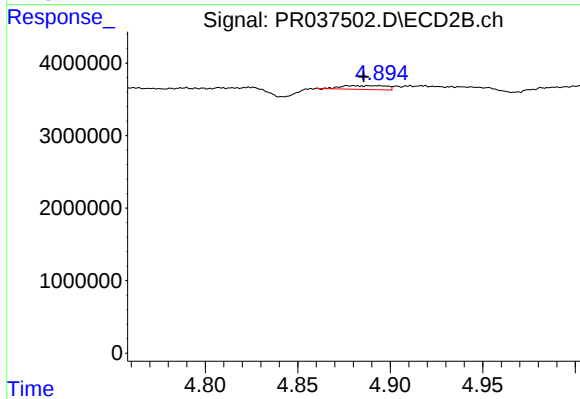

#24 AR-1248-4


R.T.: 4.882 min
Delta R.T.: -0.004 min
Response: 862484
Conc: 4.85 ng/ml

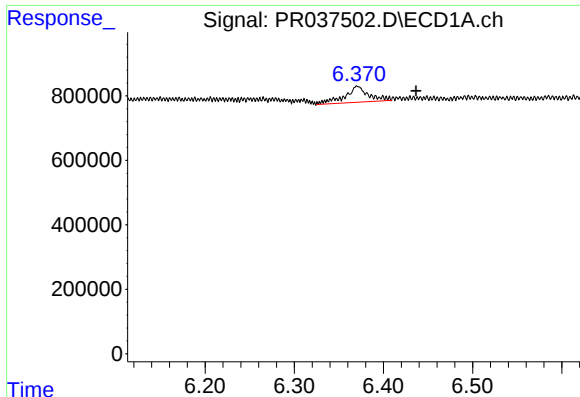

#25 AR-1248-5


R.T.: 6.371 min
Delta R.T.: -0.066 min
Response: 930642
Conc: 19.70 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

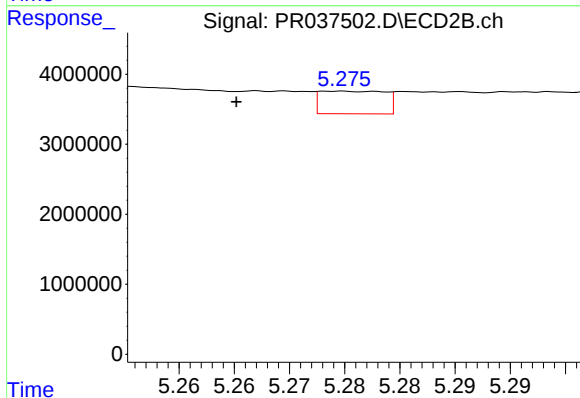


#25 AR-1248-5

R.T.: 5.275 min
Delta R.T.: 0.009 min
Response: 1327025
Conc: 6.78 ng/ml

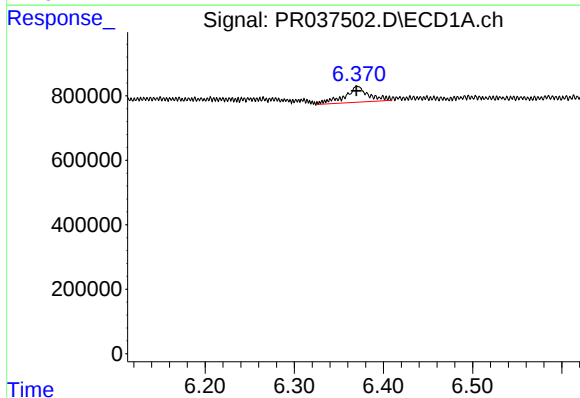


#26 AR-1254-1

R.T.: 6.371 min
Delta R.T.: 0.001 min
Response: 930642
Conc: 17.04 ng/ml

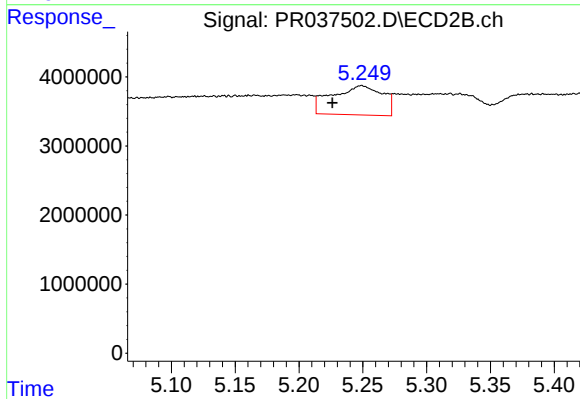

#26 AR-1254-1


R.T.: 5.249 min
Delta R.T.: 0.023 min
Response: 11678866
Conc: 33.90 ng/ml

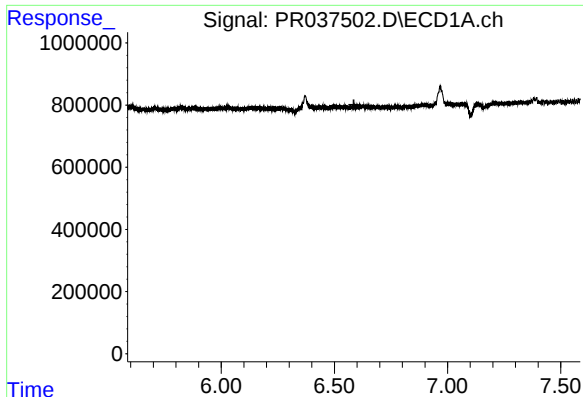

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.586 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

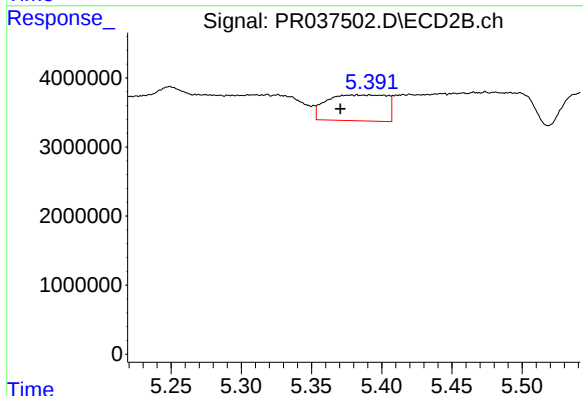


#27 AR-1254-2

R.T.: 5.383 min
Delta R.T.: 0.012 min
Response: 11099041
Conc: 37.06 ng/ml

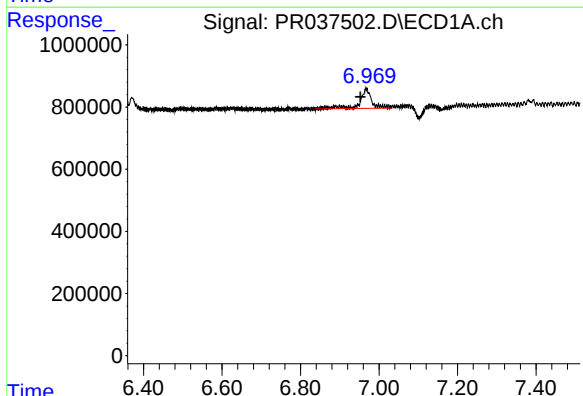


#28 AR-1254-3

R.T.: 6.969 min
Delta R.T.: 0.016 min
Response: 1295344
Conc: 14.24 ng/ml

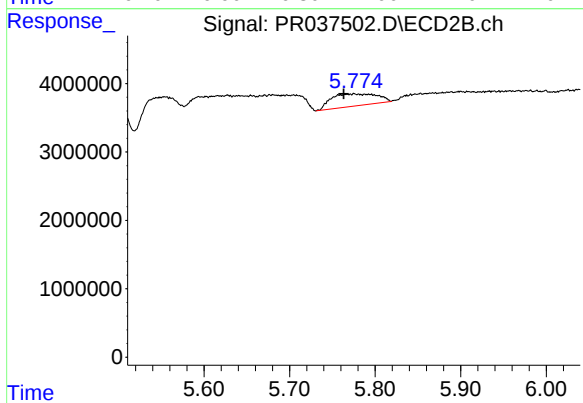

#28 AR-1254-3


R.T.: 5.776 min
Delta R.T.: 0.012 min
Response: 6623328
Conc: 13.98 ng/ml

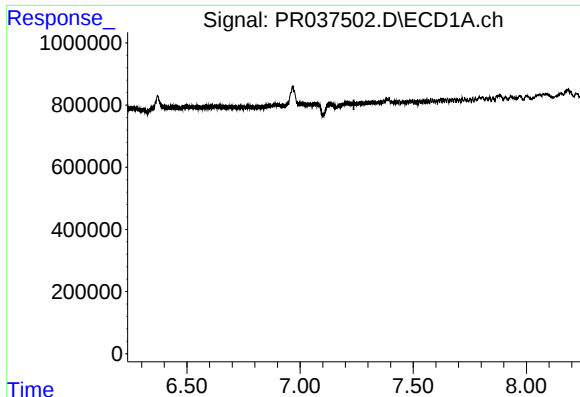

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.238 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

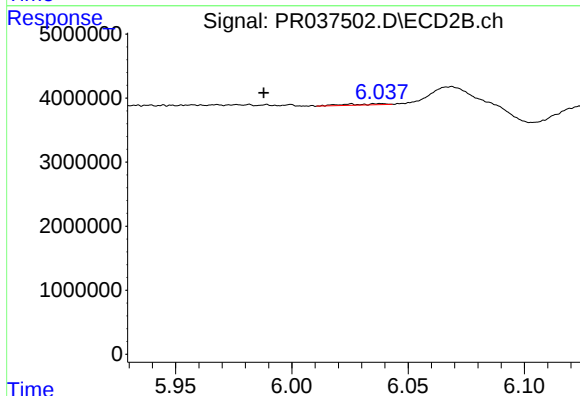


#29 AR-1254-4

R.T.: 6.038 min
Delta R.T.: 0.050 min
Response: 209634
Conc: 0.60 ng/ml

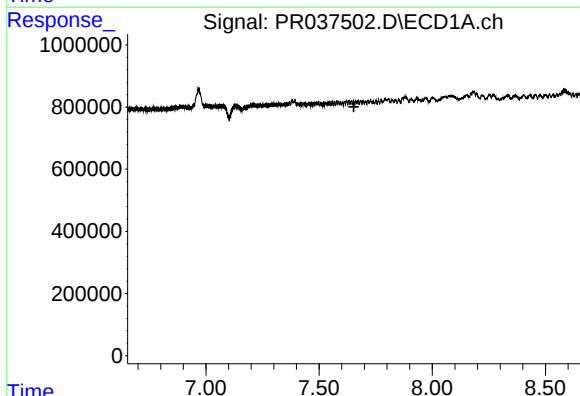


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 7.654 min
Response: 0
Conc: N.D.

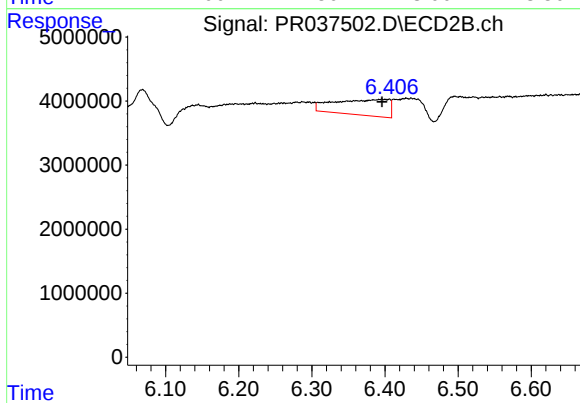

#30 AR-1254-5


R.T.: 6.396 min
Delta R.T.: 0.000 min
Response: 12863170
Conc: 29.05 ng/ml

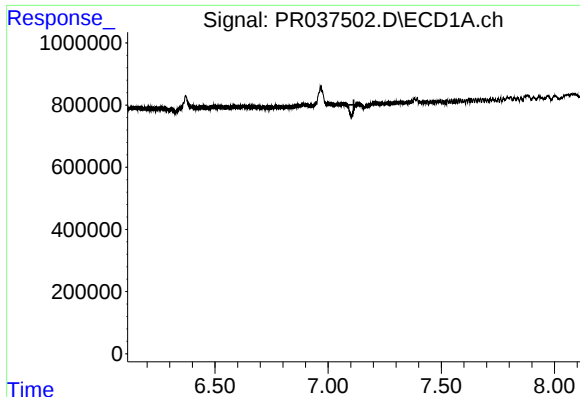

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

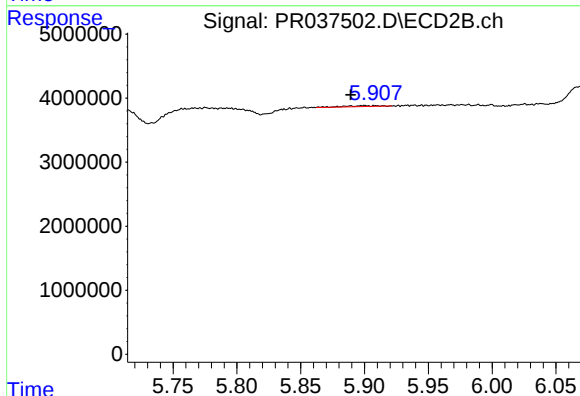


#31 AR-1260-1

R.T.: 5.900 min
Delta R.T.: 0.011 min
Response: 253924
Conc: 0.87 ng/ml

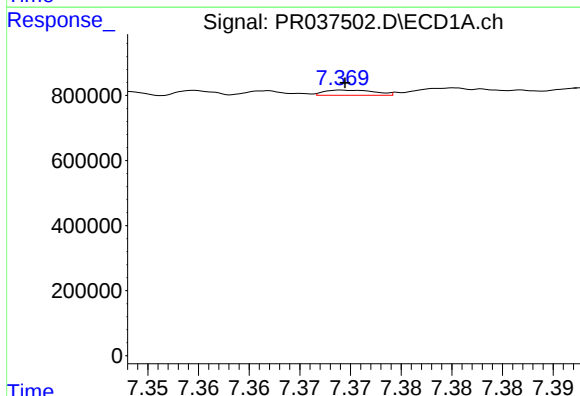


#32 AR-1260-2

R.T.: 7.370 min
Delta R.T.: 0.000 min
Response: 54294
Conc: 0.68 ng/ml

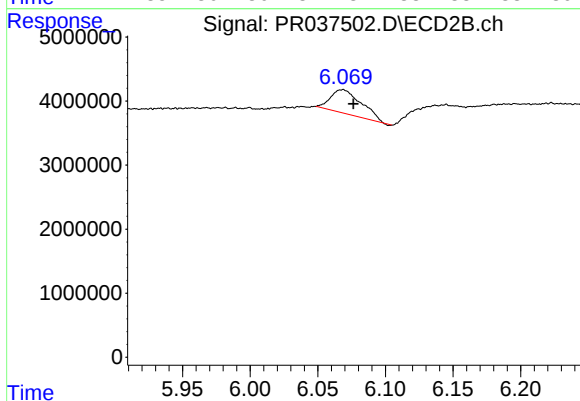

#32 AR-1260-2


R.T.: 6.068 min
Delta R.T.: -0.008 min
Response: 5636359
Conc: 12.24 ng/ml

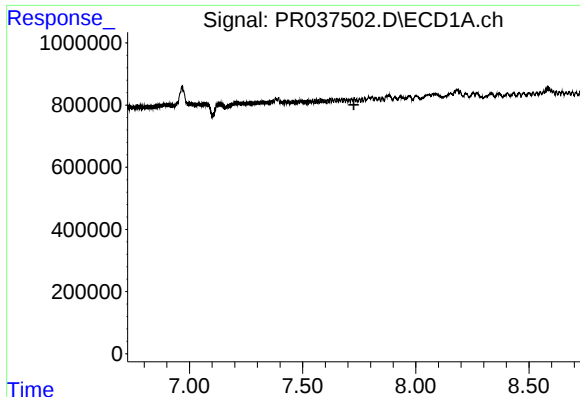

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

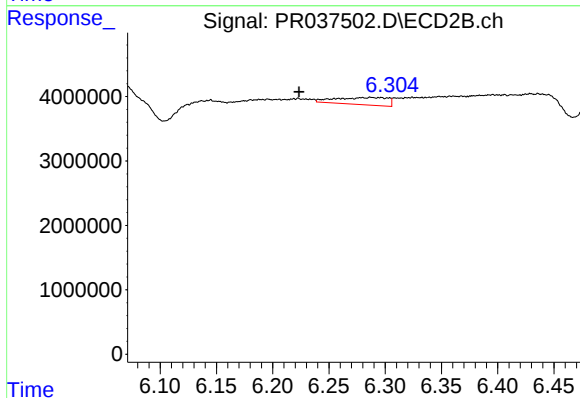


#33 AR-1260-3

R.T.: 6.279 min
Delta R.T.: 0.056 min
Response: 3602557
Conc: 10.11 ng/ml

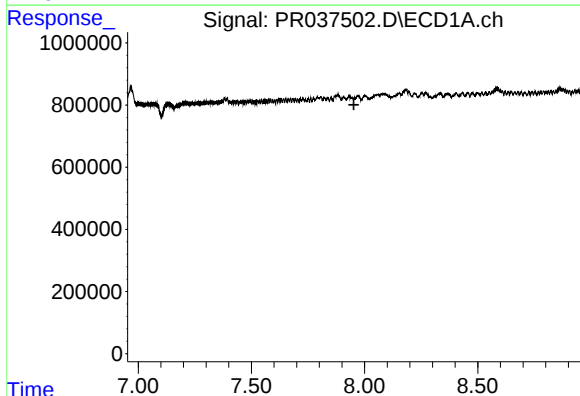


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.953 min
Response: 0
Conc: N.D.

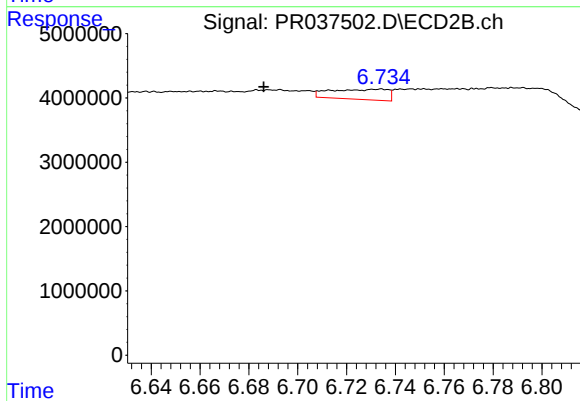

#34 AR-1260-4


R.T.: 6.734 min
Delta R.T.: 0.048 min
Response: 2585761
Conc: 8.48 ng/ml

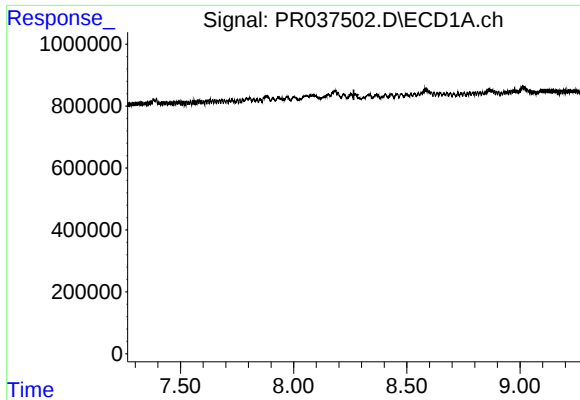

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

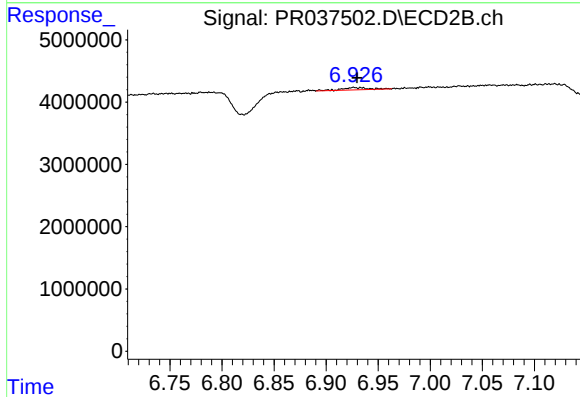


#35 AR-1260-5

R.T.: 6.927 min
Delta R.T.: -0.002 min
Response: 641821
Conc: 0.74 ng/ml

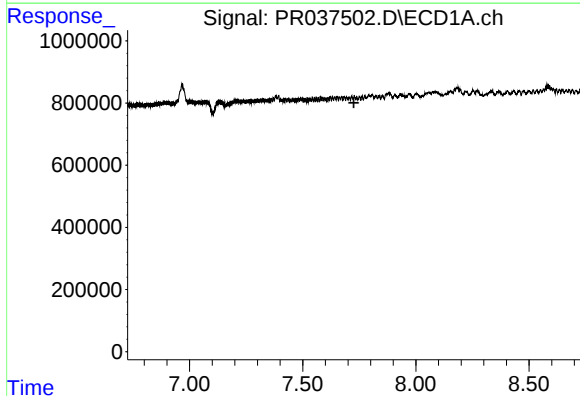


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

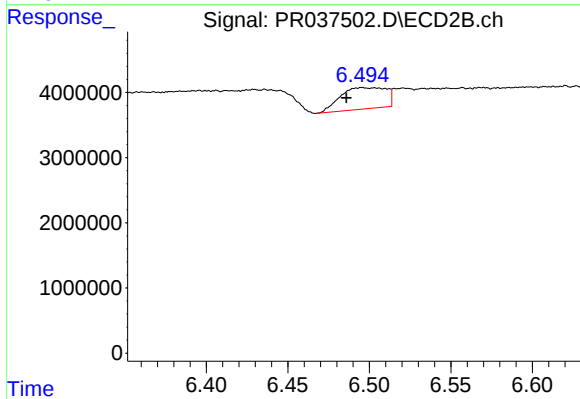

#36 AR-1262-1


R.T.: 6.496 min
Delta R.T.: 0.010 min
Response: 6424038
Conc: 25.63 ng/ml

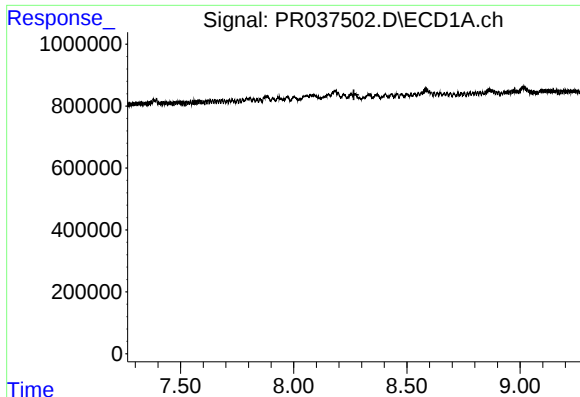

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

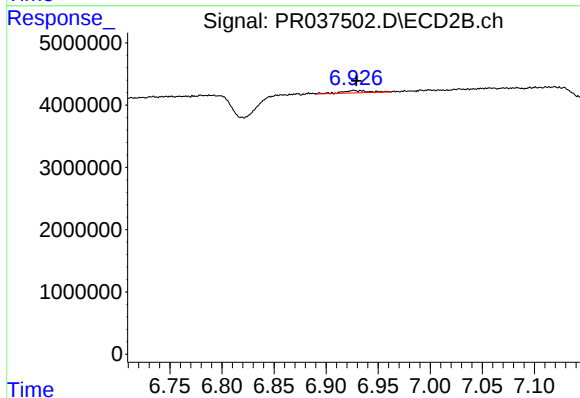


#37 AR-1262-2

R.T.: 6.927 min
Delta R.T.: -0.002 min
Response: 641821
Conc: 0.51 ng/ml

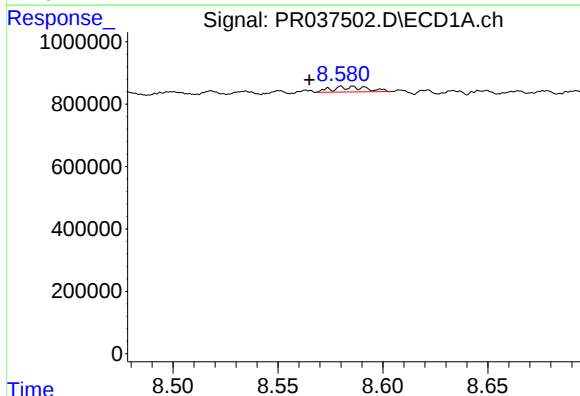


#38 AR-1262-3

R.T.: 8.580 min
Delta R.T.: 0.015 min
Response: 194374
Conc: 1.48 ng/ml

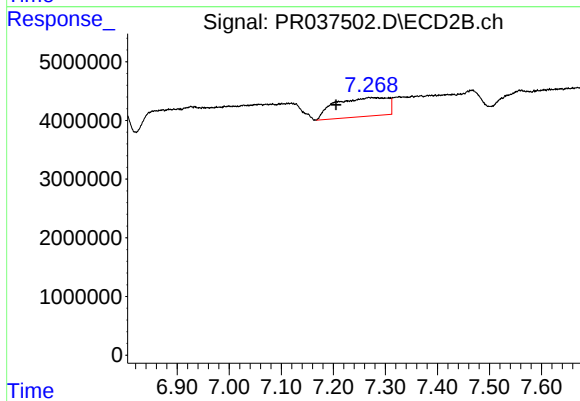

#38 AR-1262-3


R.T.: 7.269 min
Delta R.T.: 0.064 min
Response: 22638976
Conc: 41.29 ng/ml

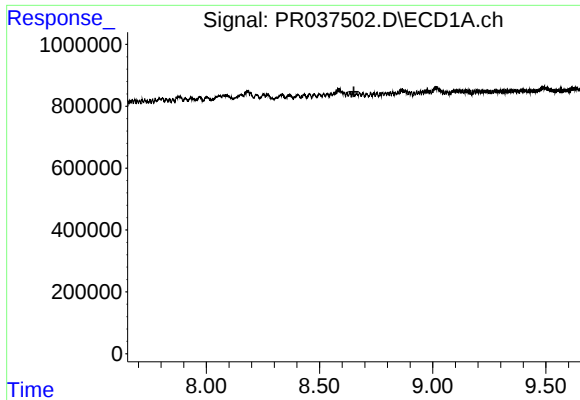

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.652 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

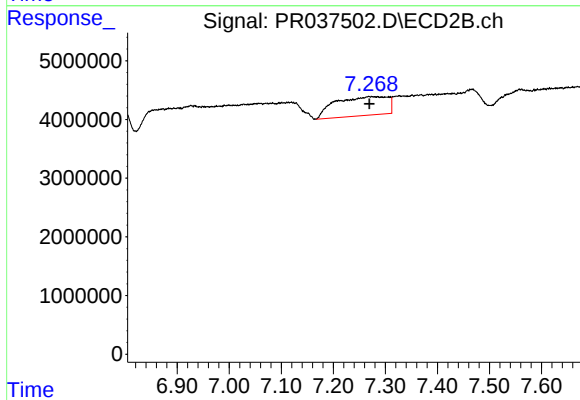


#39 AR-1262-4

R.T.: 7.269 min
Delta R.T.: 0.000 min
Response: 22638976
Conc: 25.22 ng/ml

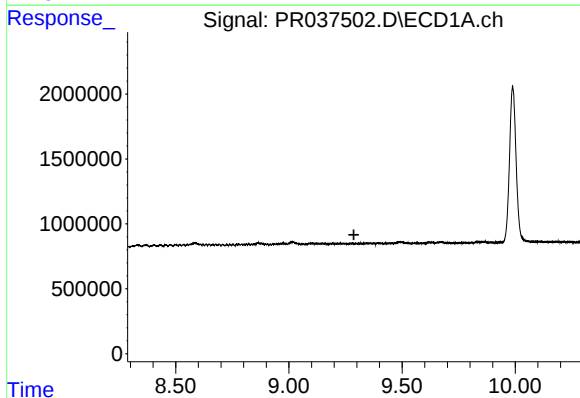


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.287 min
Response: 0
Conc: N.D.

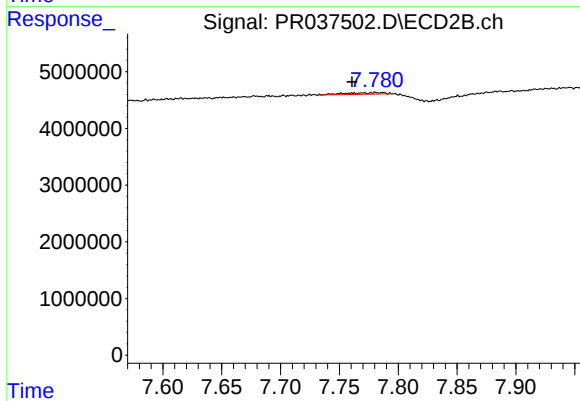

#40 AR-1262-5


R.T.: 7.781 min
Delta R.T.: 0.020 min
Response: 643259
Conc: 1.68 ng/ml

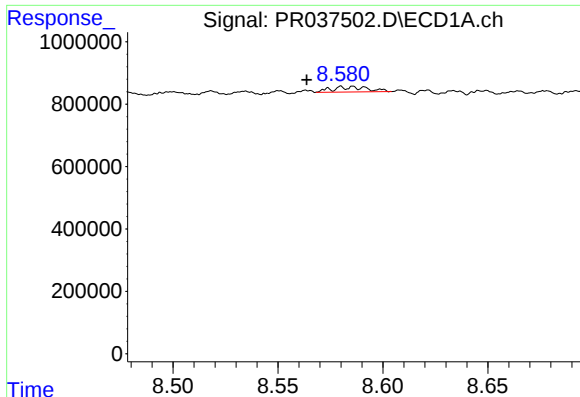

#41 AR-1268-1


R.T.: 8.580 min
Delta R.T.: 0.017 min
Response: 194374
Conc: 1.09 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

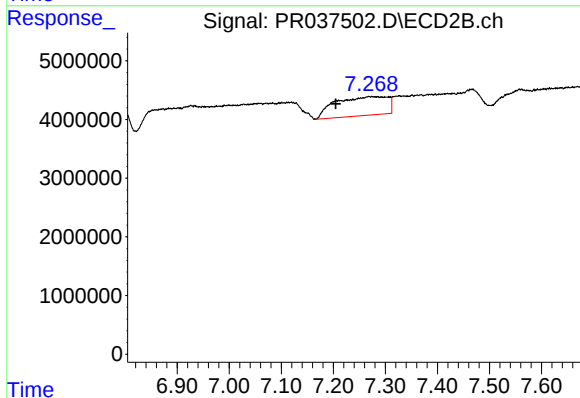


#41 AR-1268-1

R.T.: 7.269 min
Delta R.T.: 0.065 min
Response: 22638976
Conc: 18.39 ng/ml

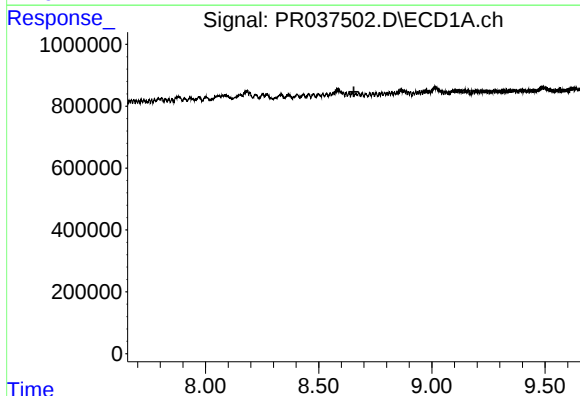


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.655 min
Response: 0
Conc: N.D.

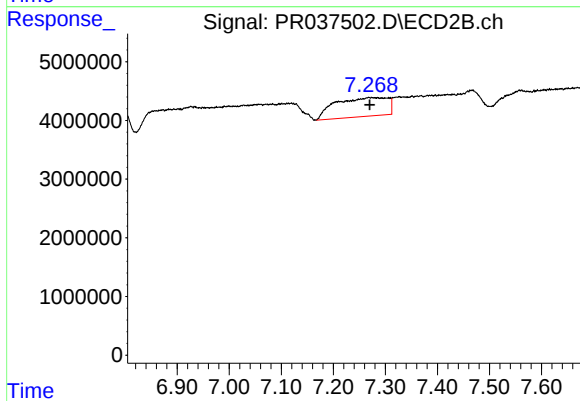

#42 AR-1268-2


R.T.: 7.269 min
Delta R.T.: 0.000 min
Response: 22638976
Conc: 21.38 ng/ml

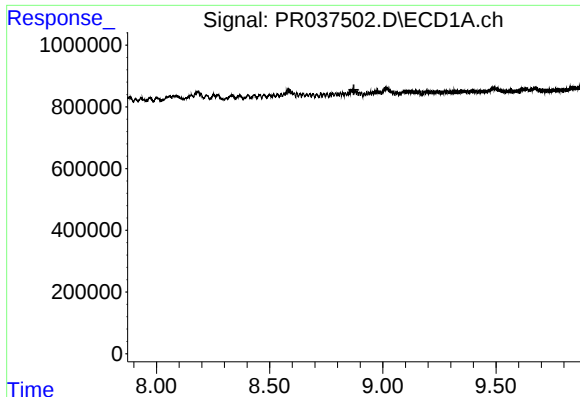

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

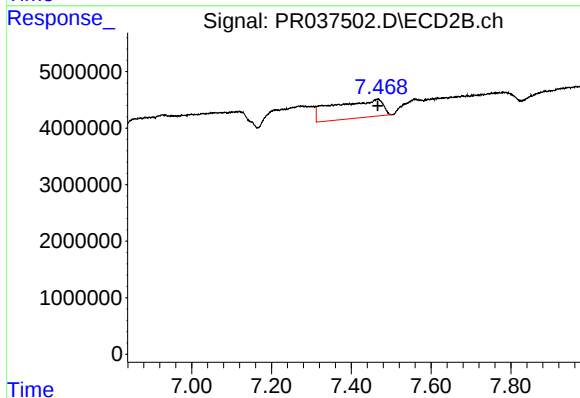


#43 AR-1268-3

R.T.: 7.466 min
Delta R.T.: 0.000 min
Response: 27711190
Conc: 31.27 ng/ml

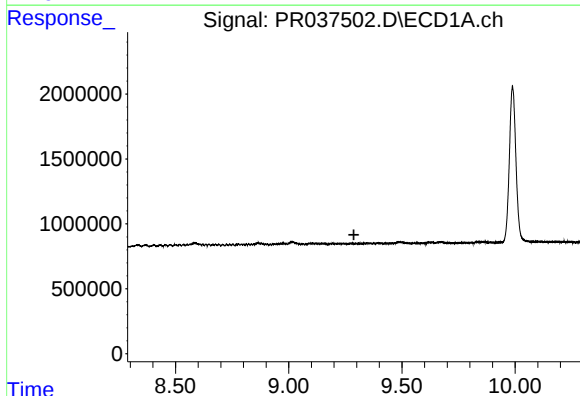


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.288 min
Response: 0
Conc: N.D.

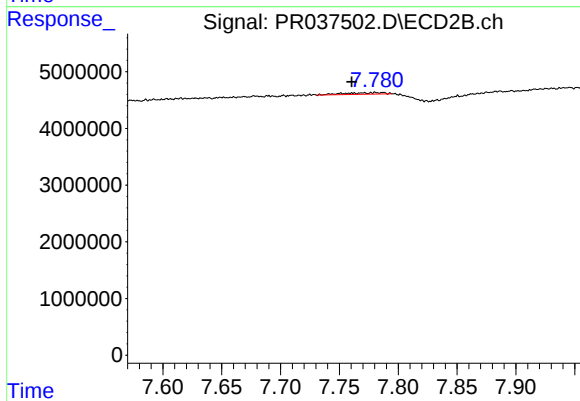

#44 AR-1268-4


R.T.: 7.781 min
Delta R.T.: 0.021 min
Response: 643259
Conc: 1.77 ng/ml

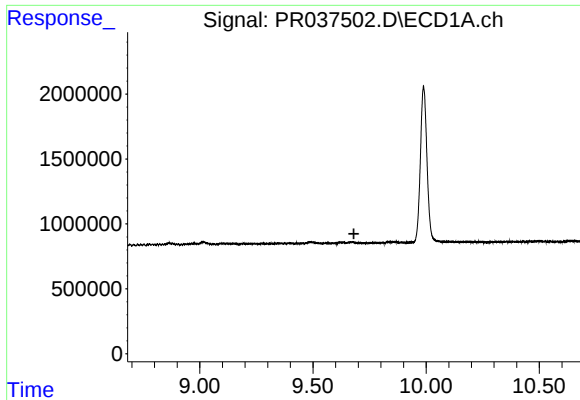

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.681 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

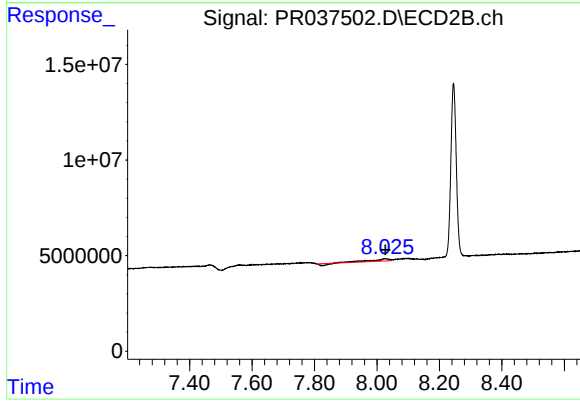

#45 AR-1268-5

R.T.: 8.026 min
Delta R.T.: -0.001 min
Response: 3952013
Conc: 1.55 ng/ml