

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR050224\
 Data File : PR066529.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 May 2024 08:37
 Operator : AJ\MA
 Sample : P2339-07
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 T3484

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/03/2024
 Supervised By :Ankita Jodhani 05/06/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 03 09:01:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 26 07:26:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.657	2.901	56601143	57887313	10.799	12.951m
2) SA Decachlor...	9.534	8.124	27552623	41335972	11.765	8.807 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR050224\
Data File : PR066529.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 May 2024 08:37
Operator : AJ\MA
Sample : P2339-07
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
T3484


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/03/2024
Supervised By :Ankita Jodhani 05/06/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 03 09:01:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 26 07:26:35 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

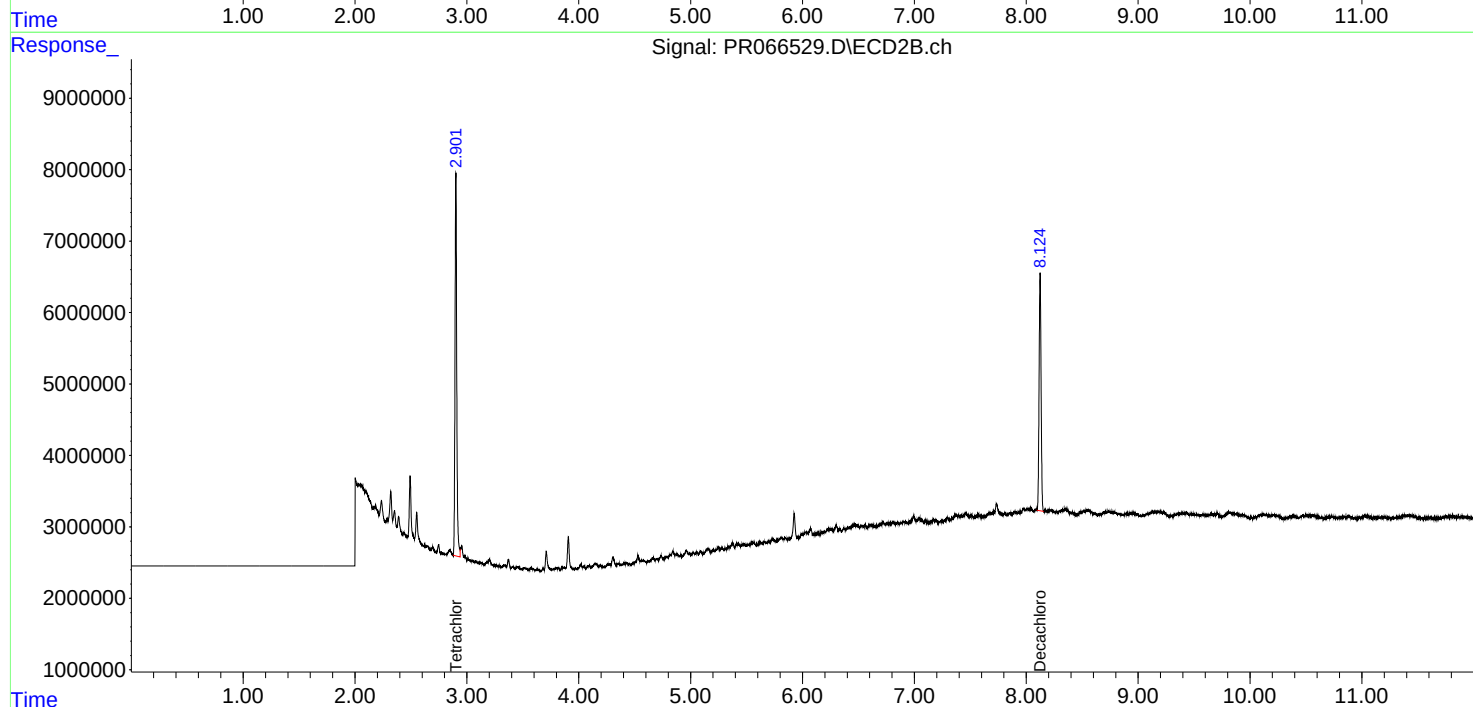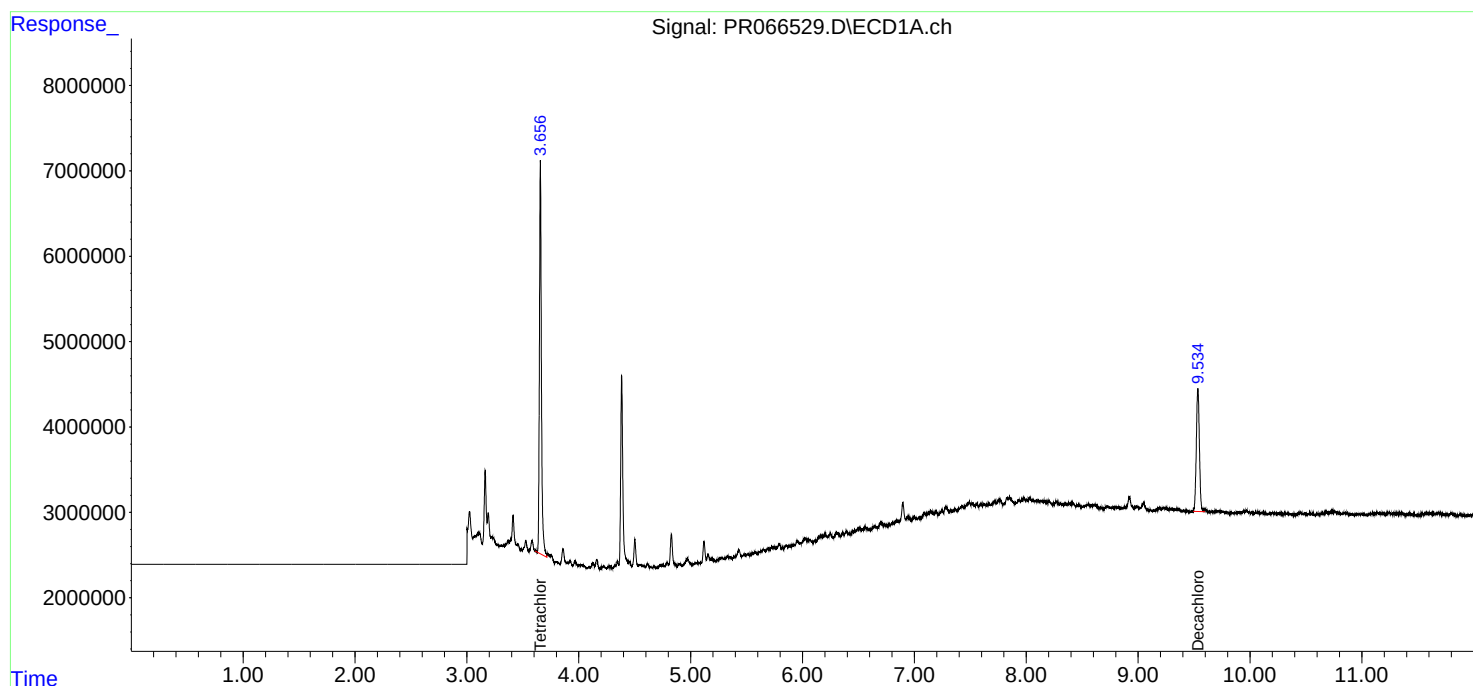

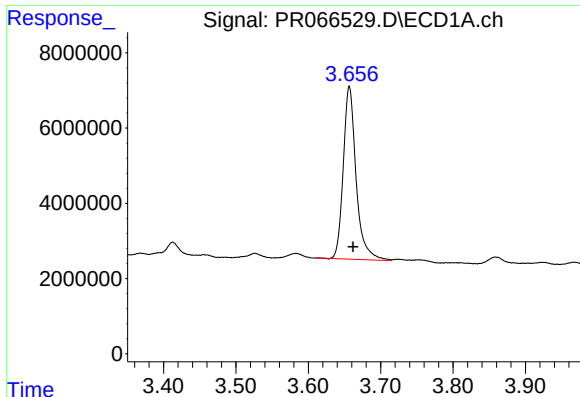


#1 Tetrachloro-m-xylene

R.T.: 3.657 min
Delta R.T.: -0.005 min
Response: 56601143
Conc: 10.80 ng/ml

Instrument :
ECD_R
ClientSampleId :
T3484


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/03/2024
Supervised By :Ankita Jodhani 05/06/2024

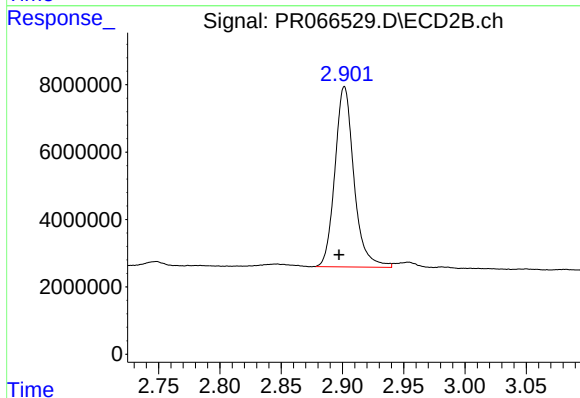


#1 Tetrachloro-m-xylene

R.T.: 2.901 min
Delta R.T.: 0.004 min
Response: 57887313
Conc: 12.95 ng/ml m

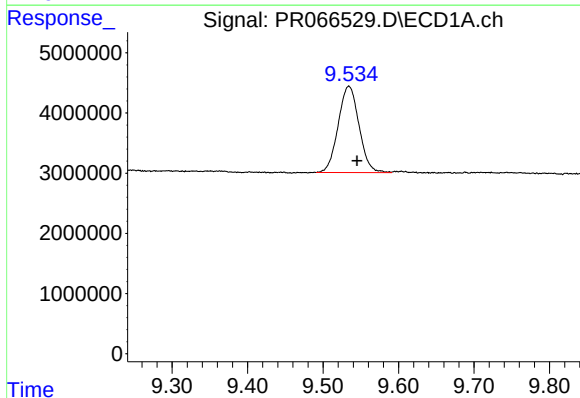

#2 Decachlorobiphenyl

R.T.: 9.534 min
Delta R.T.: -0.011 min
Response: 27552623
Conc: 11.77 ng/ml

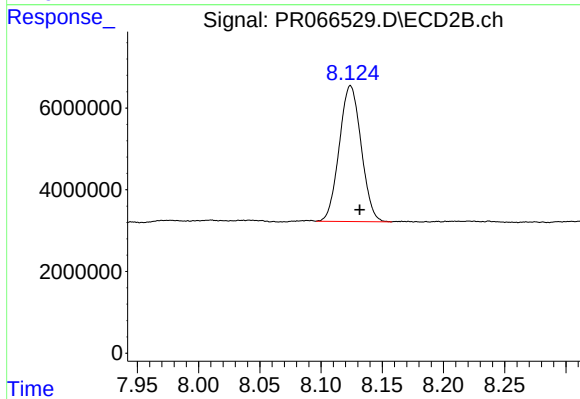

#2 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.008 min
Response: 41335972
Conc: 8.81 ng/ml