

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR050924\
 Data File : PR066652.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2024 05:32
 Operator : AJ\MA
 Sample : P2403-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT2-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 06:56:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 26 07:26:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.653	2.896	119.4E6	100.0E6	22.774	22.378
2) SA Decachlor...	9.533	8.121	50302591	96981643	21.480	20.662
Target Compounds						
3) L1 AR-1016-1	4.894	4.005	810220	444979	5.668	2.946 #
4) L1 AR-1016-2	4.894	4.036	810220	1445362	3.705	6.736 #
5) L1 AR-1016-3	4.967	4.194	2090195	137932	14.393	1.176 #
6) L1 AR-1016-4	5.068	4.275f	173338	1085450	1.509	11.251 #
7) L1 AR-1016-5	0.000	4.467	0	281278	N.D.	2.275 #
8) L2 AR-1221-1	3.875	3.119	2119400	1439979	35.100	26.579
9) L2 AR-1221-2	3.964	3.197	2514608	2301470	56.906	55.432
10) L2 AR-1221-3	4.040	3.281	3220368	3329671	24.794	27.559
11) L3 AR-1232-1	4.040	3.281	3220368	3329671	30.242	33.173
12) L3 AR-1232-2	4.588	4.036	560462	1445362	9.133	14.523 #
13) L3 AR-1232-3	4.894	4.194	810220	137932	7.927	2.575 #
14) L3 AR-1232-4	5.068	4.275f	173338	1085450	3.219	22.380 #
15) L3 AR-1232-5	5.169	4.467	374617	281278	9.311	5.272 #
16) L4 AR-1242-1	4.868	4.005	816403	444979	6.859	3.555 #
17) L4 AR-1242-2	4.894	4.036	810220	1445362	4.508	8.155 #
18) L4 AR-1242-3	4.967	4.194	2090195	137932	17.546	1.435 #
19) L4 AR-1242-4	5.068	4.275f	173338	1085450	1.831	11.370 #
20) L4 AR-1242-5	5.850	0.000	563590	0	6.268	N.D. #
21) L5 AR-1248-1	4.868	4.005	816403	444979	9.433	4.786 #
22) L5 AR-1248-2	5.169	4.275f	374617	1085450	2.814	8.022 #
23) L5 AR-1248-3	0.000	4.275f	0	1085450	N.D.	7.884 #
24) L5 AR-1248-4	0.000	4.467	0	281278	N.D.	1.702 #
25) L5 AR-1248-5	5.850	4.873	563590	633663	3.935	3.927
26) L6 AR-1254-1	5.778	0.000	561133	0	3.377	N.D. #
27) L6 AR-1254-2	6.020	4.985	493288	229737	2.014	1.049 #
28) L6 AR-1254-3	6.396	5.395f	842974	1391153	3.410	4.047
29) L6 AR-1254-4	6.744f	5.669	296205	80005	1.866	0.375 #
30) L6 AR-1254-5	7.154f	6.102	1420300	369736	7.969	1.149 #
31) L7 AR-1260-1	6.577	5.538f	457904	158514	2.203	0.625 #
32) L7 AR-1260-2	6.898f	0.000	903604	0	4.073	N.D. #
33) L7 AR-1260-3	7.255	5.919	989976	516717	5.903	1.775 #
34) L7 AR-1260-4	7.506	6.437	116511	409497	0.654	1.640 #
35) L7 AR-1260-5	7.846	6.676	189693	158097	0.650	0.282 #
36) L8 AR-1262-1	7.255	6.191f	989976	99792	4.340	0.691 #
37) L8 AR-1262-2	7.846	6.437	189693	409497	0.597	1.331 #
38) L8 AR-1262-3	8.155	6.980	411824	222028	1.945	0.916 #
39) L8 AR-1262-4	8.220f	0.000	500692	0	4.584	N.D. #
40) L8 AR-1262-5	0.000	7.591	0	499574	N.D.	2.314 #
41) L9 AR-1268-1	8.155	6.980	411824	222028	1.056	0.307 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR050924\
 Data File : PR066652.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2024 05:32
 Operator : AJ\MA
 Sample : P2403-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT2-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 06:56:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 26 07:26:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.220f	0.000	500692	0	1.457	N.D. #
43) L9	AR-1268-3	0.000	7.275	0	513302	N.D.	0.905 #
44) L9	AR-1268-4	0.000	7.591	0	499574	N.D.	2.047 #
45) L9	AR-1268-5	9.279f	7.881	272472	688833	0.334	0.425 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR050924\
Data File : PR066652.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2024 05:32
Operator : AJ\MA
Sample : P2403-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 67 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 06:56:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 26 07:26:35 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

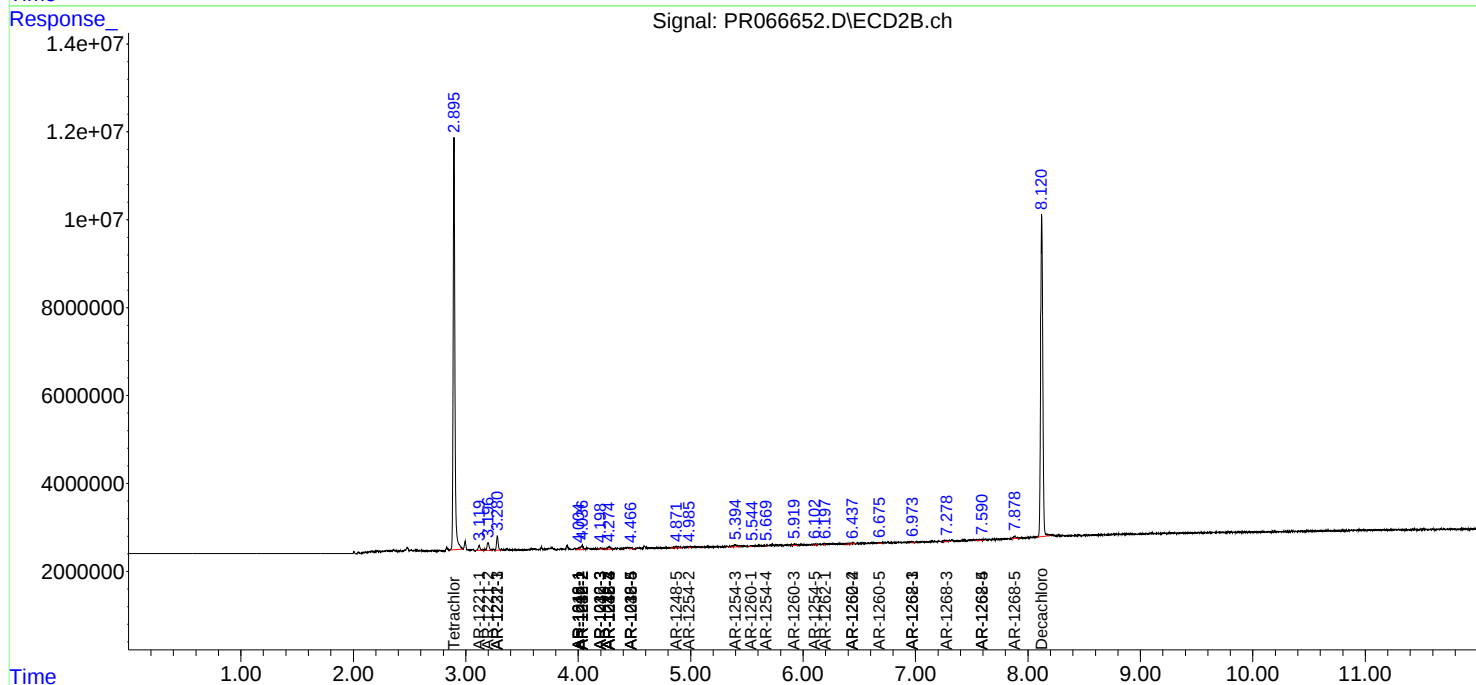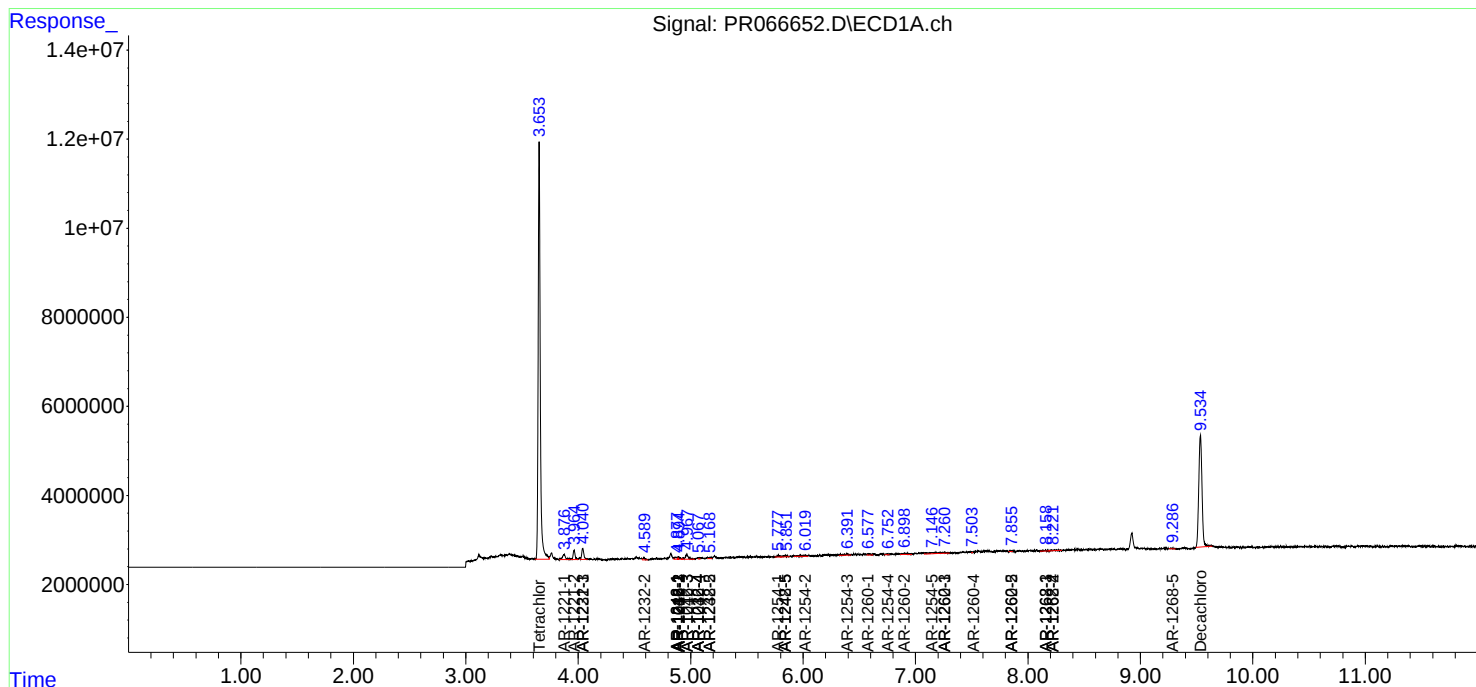


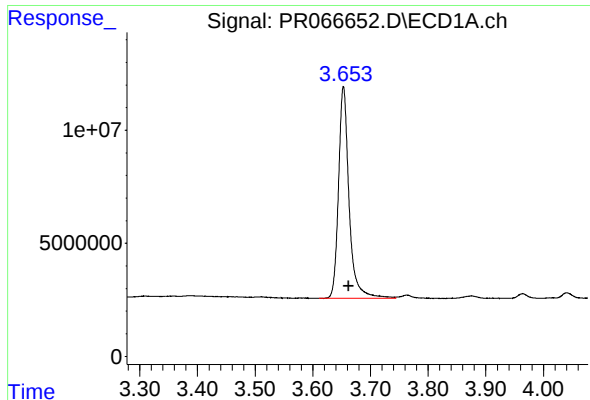

#1 Tetrachloro-m-xylene


R.T.: 3.653 min
Delta R.T.: -0.009 min
Response: 119371731
Conc: 22.77 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

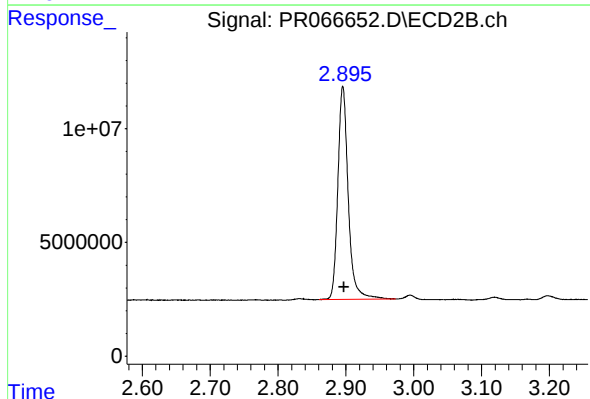


#1 Tetrachloro-m-xylene

R.T.: 2.896 min
Delta R.T.: -0.001 min
Response: 100022357
Conc: 22.38 ng/ml

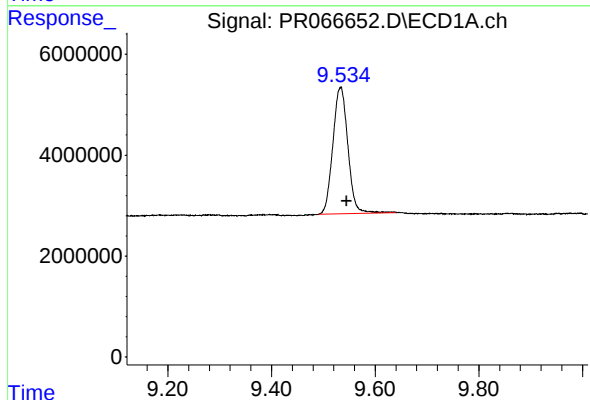


#2 Decachlorobiphenyl

R.T.: 9.533 min
Delta R.T.: -0.012 min
Response: 50302591
Conc: 21.48 ng/ml

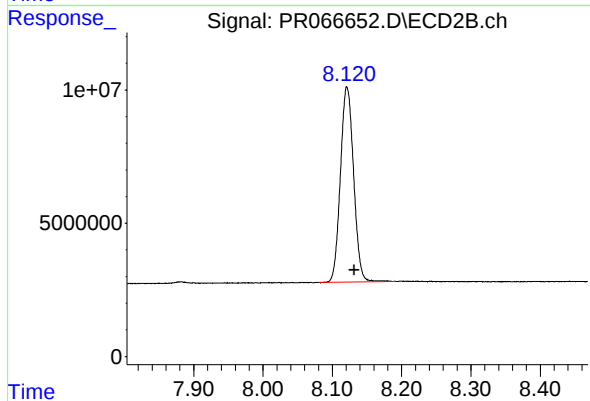

#2 Decachlorobiphenyl


R.T.: 8.121 min
Delta R.T.: -0.010 min
Response: 96981643
Conc: 20.66 ng/ml

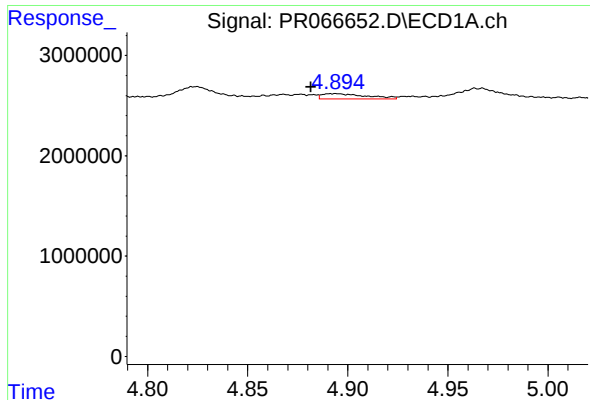

#3 AR-1016-1


R.T.: 4.894 min
Delta R.T.: 0.012 min
Response: 810220
Conc: 5.67 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

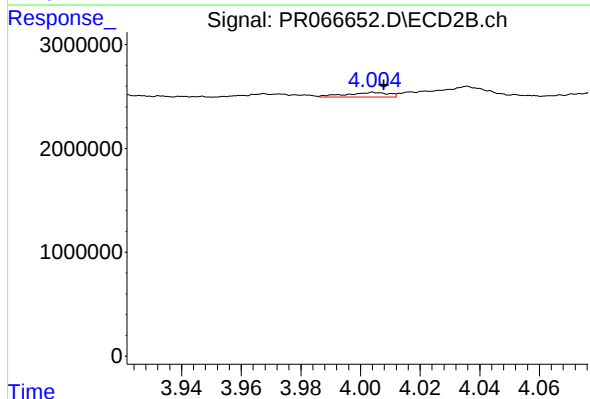


#3 AR-1016-1

R.T.: 4.005 min
Delta R.T.: -0.003 min
Response: 444979
Conc: 2.95 ng/ml

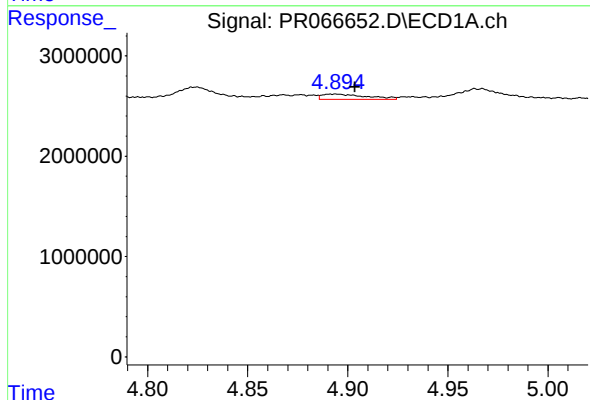


#4 AR-1016-2

R.T.: 4.894 min
Delta R.T.: -0.010 min
Response: 810220
Conc: 3.70 ng/ml

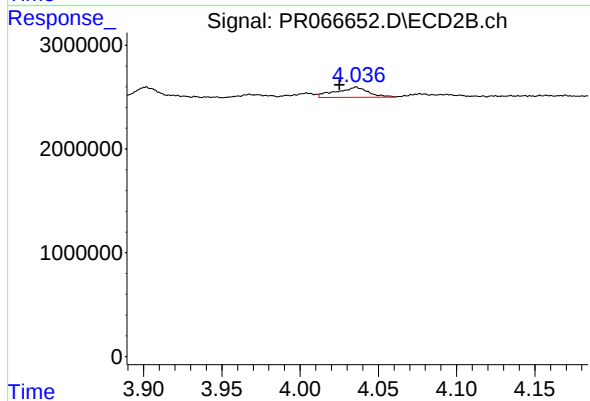

#4 AR-1016-2


R.T.: 4.036 min
Delta R.T.: 0.011 min
Response: 1445362
Conc: 6.74 ng/ml

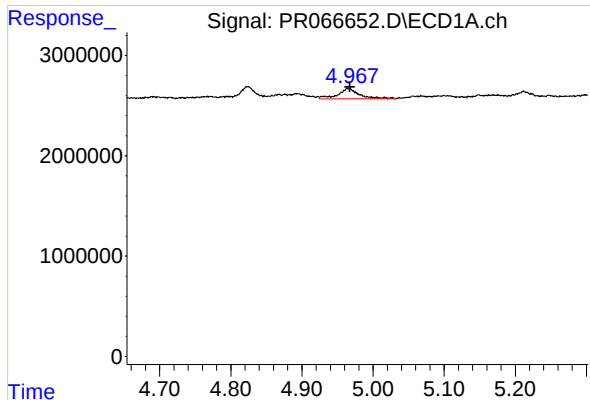

#5 AR-1016-3


R.T.: 4.967 min
Delta R.T.: -0.001 min
Response: 2090195
Conc: 14.39 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

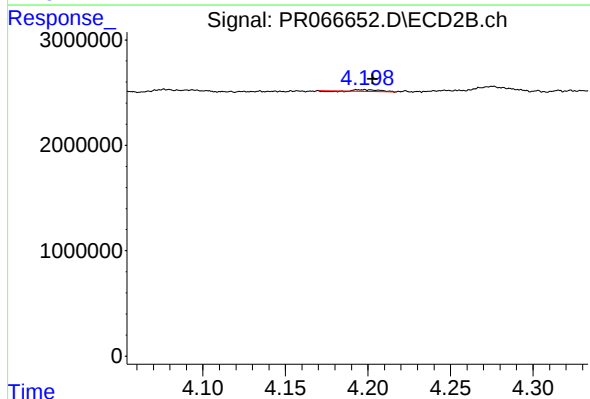


#5 AR-1016-3

R.T.: 4.194 min
Delta R.T.: -0.008 min
Response: 137932
Conc: 1.18 ng/ml

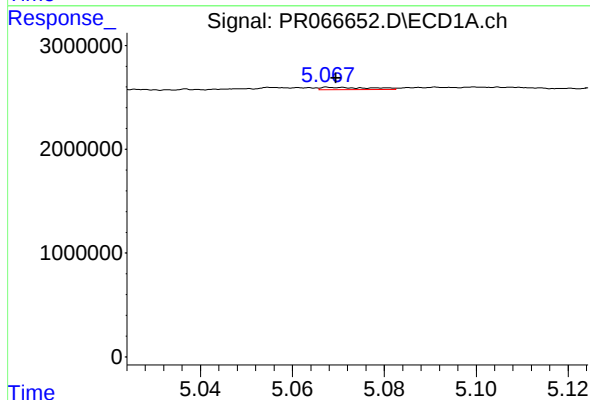


#6 AR-1016-4

R.T.: 5.068 min
Delta R.T.: -0.001 min
Response: 173338
Conc: 1.51 ng/ml

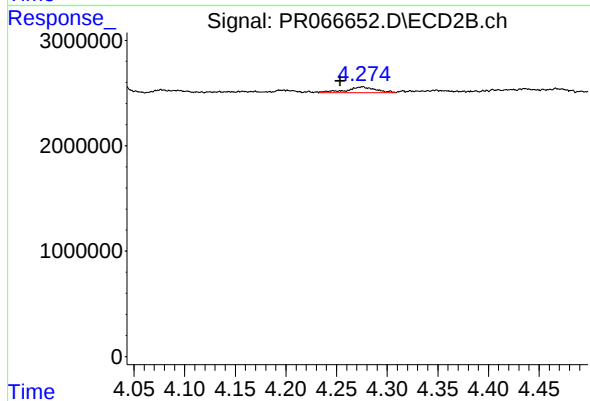

#6 AR-1016-4


R.T.: 4.275 min
Delta R.T.: 0.022 min
Response: 1085450
Conc: 11.25 ng/ml

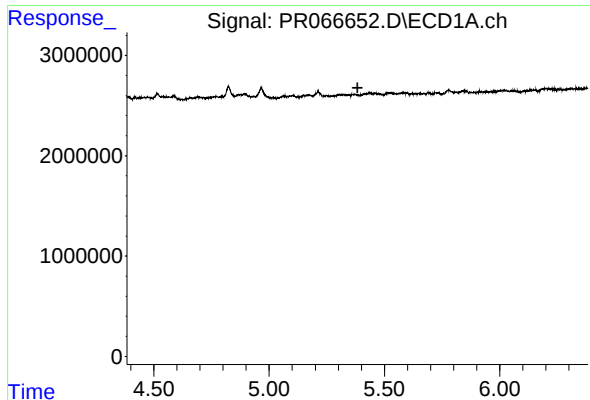

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.383 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

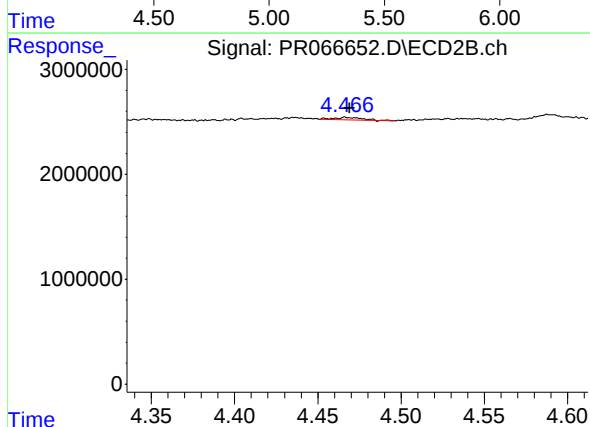


#7 AR-1016-5

R.T.: 4.467 min
Delta R.T.: -0.002 min
Response: 281278
Conc: 2.28 ng/ml

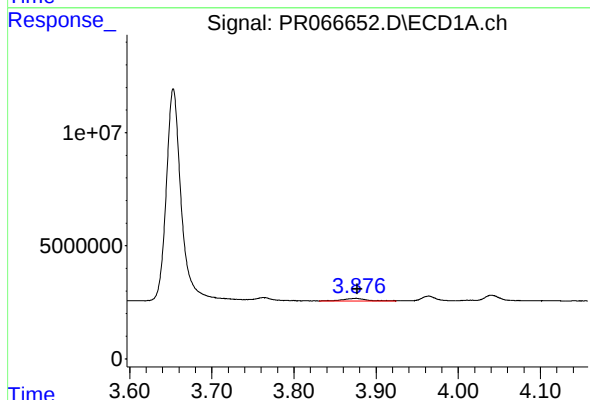


#8 AR-1221-1

R.T.: 3.875 min
Delta R.T.: -0.001 min
Response: 2119400
Conc: 35.10 ng/ml

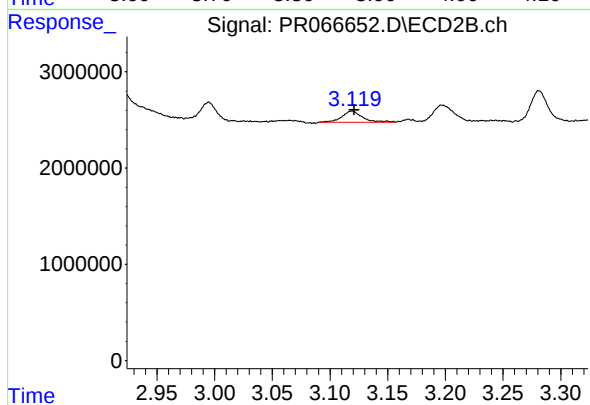

#8 AR-1221-1


R.T.: 3.119 min
Delta R.T.: -0.002 min
Response: 1439979
Conc: 26.58 ng/ml

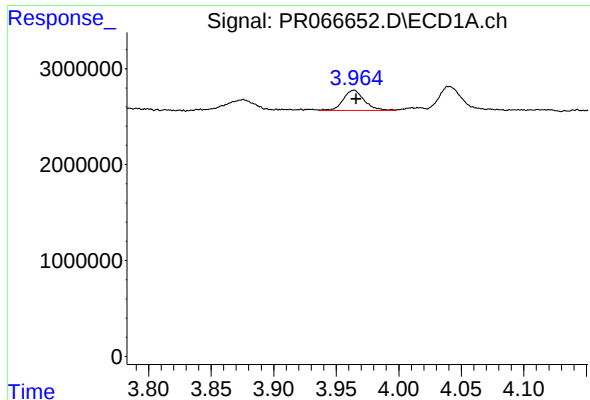

#9 AR-1221-2


R.T.: 3.964 min
Delta R.T.: -0.002 min
Response: 2514608
Conc: 56.91 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

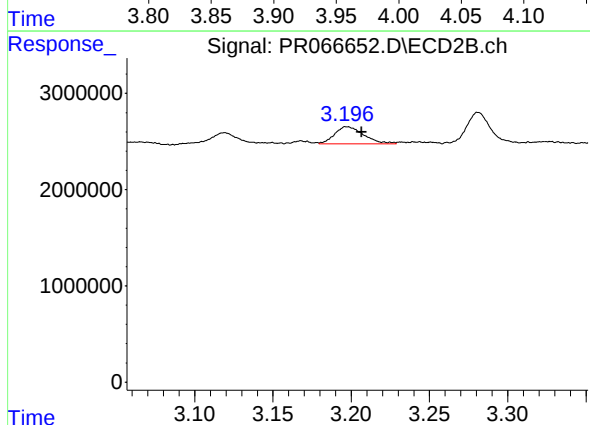


#9 AR-1221-2

R.T.: 3.197 min
Delta R.T.: -0.009 min
Response: 2301470
Conc: 55.43 ng/ml

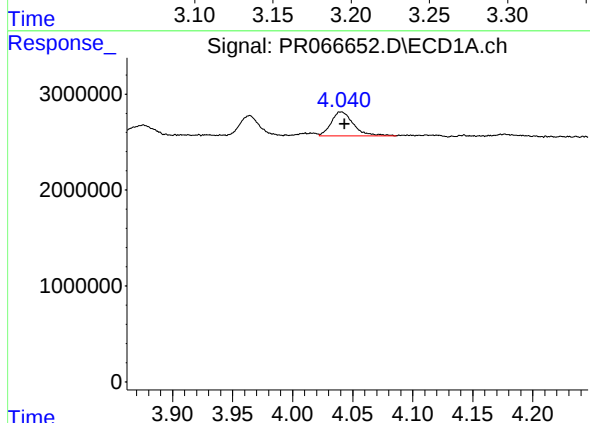


#10 AR-1221-3

R.T.: 4.040 min
Delta R.T.: -0.003 min
Response: 3220368
Conc: 24.79 ng/ml

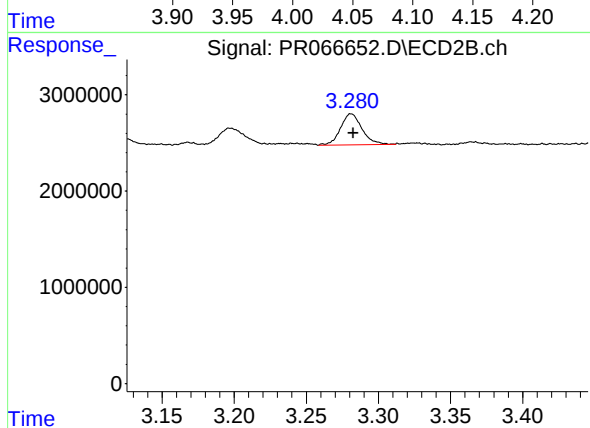

#10 AR-1221-3


R.T.: 3.281 min
Delta R.T.: -0.001 min
Response: 3329671
Conc: 27.56 ng/ml

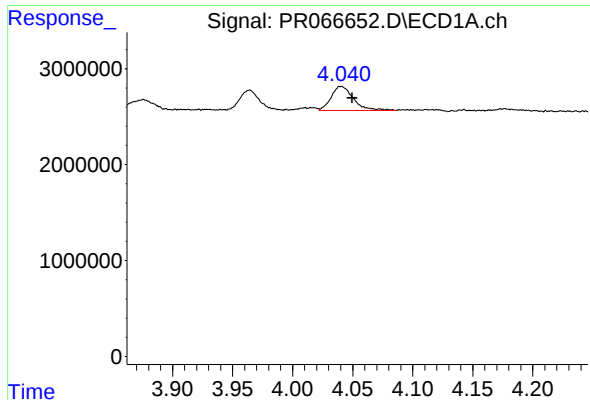

#11 AR-1232-1


R.T.: 4.040 min
Delta R.T.: -0.009 min
Response: 3220368
Conc: 30.24 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

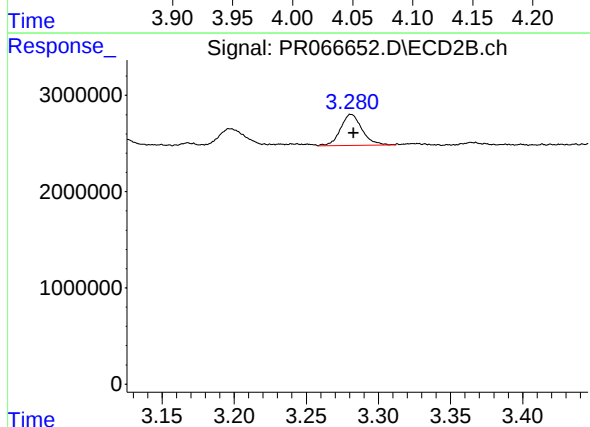


#11 AR-1232-1

R.T.: 3.281 min
Delta R.T.: -0.002 min
Response: 3329671
Conc: 33.17 ng/ml

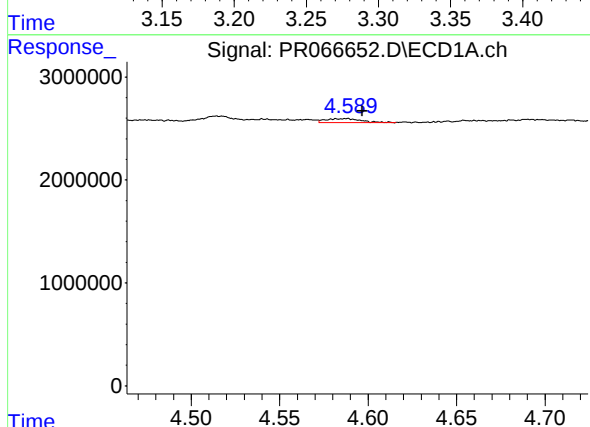


#12 AR-1232-2

R.T.: 4.588 min
Delta R.T.: -0.009 min
Response: 560462
Conc: 9.13 ng/ml

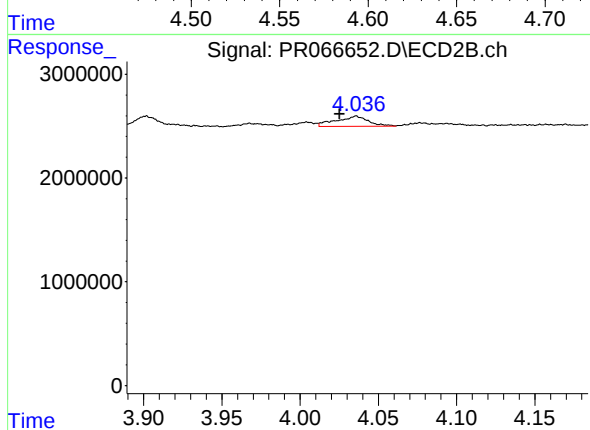

#12 AR-1232-2


R.T.: 4.036 min
Delta R.T.: 0.011 min
Response: 1445362
Conc: 14.52 ng/ml

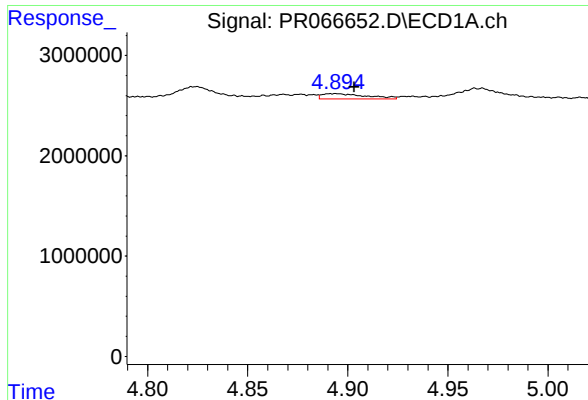

#13 AR-1232-3


R.T.: 4.894 min
Delta R.T.: -0.010 min
Response: 810220
Conc: 7.93 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

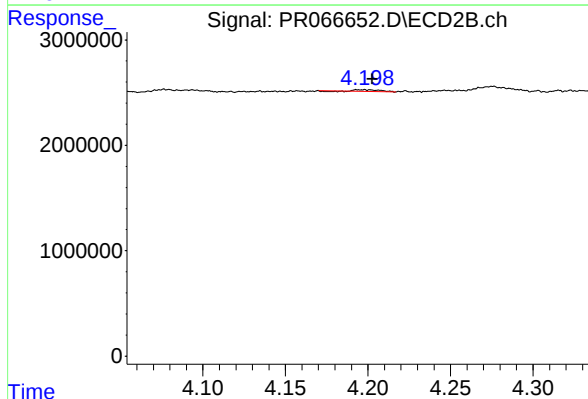


#13 AR-1232-3

R.T.: 4.194 min
Delta R.T.: -0.008 min
Response: 137932
Conc: 2.57 ng/ml

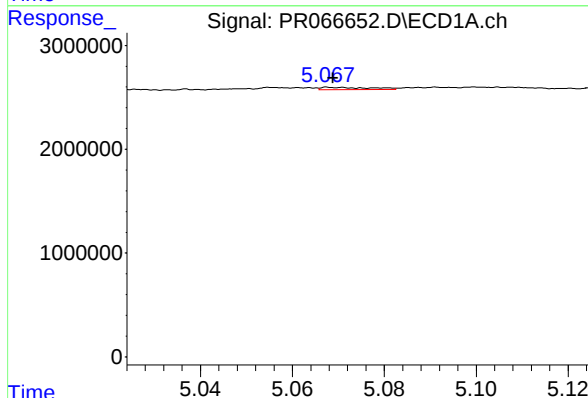


#14 AR-1232-4

R.T.: 5.068 min
Delta R.T.: 0.000 min
Response: 173338
Conc: 3.22 ng/ml

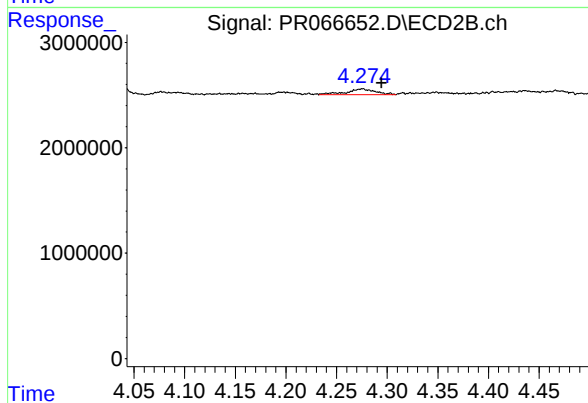

#14 AR-1232-4


R.T.: 4.275 min
Delta R.T.: -0.019 min
Response: 1085450
Conc: 22.38 ng/ml

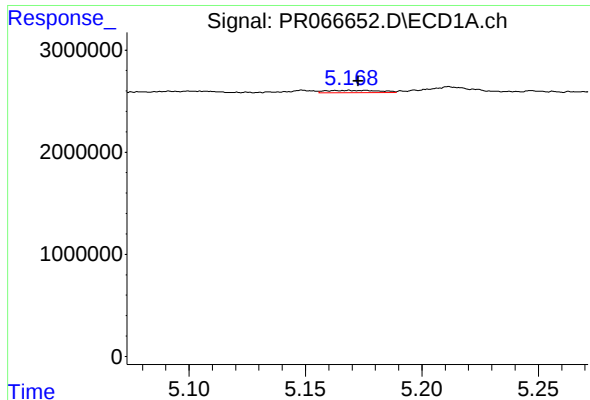

#15 AR-1232-5


R.T.: 5.169 min
Delta R.T.: -0.004 min
Response: 374617
Conc: 9.31 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

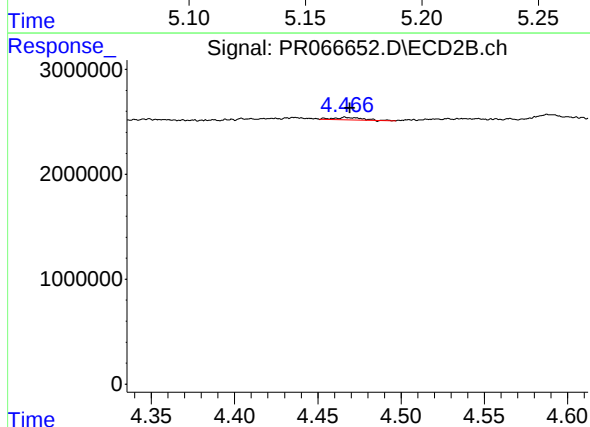


#15 AR-1232-5

R.T.: 4.467 min
Delta R.T.: -0.003 min
Response: 281278
Conc: 5.27 ng/ml

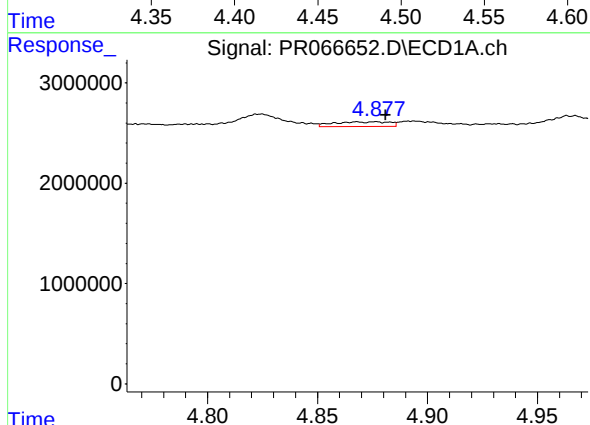


#16 AR-1242-1

R.T.: 4.868 min
Delta R.T.: -0.013 min
Response: 816403
Conc: 6.86 ng/ml

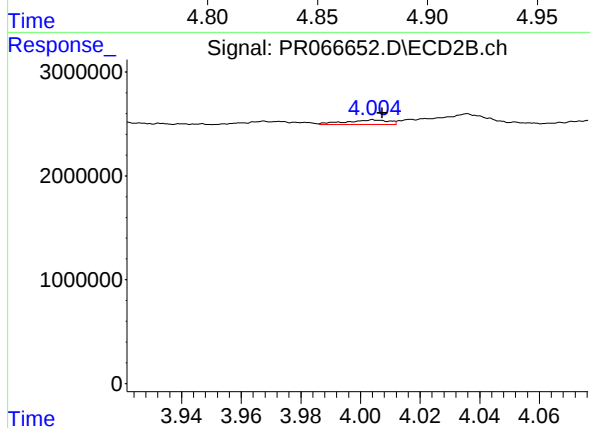

#16 AR-1242-1


R.T.: 4.005 min
Delta R.T.: -0.003 min
Response: 444979
Conc: 3.55 ng/ml

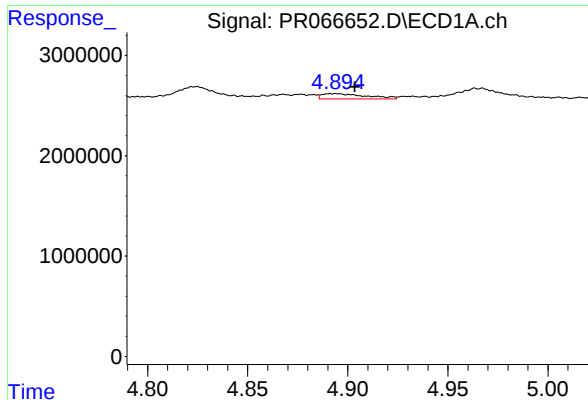

#17 AR-1242-2


R.T.: 4.894 min
Delta R.T.: -0.010 min
Response: 810220
Conc: 4.51 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

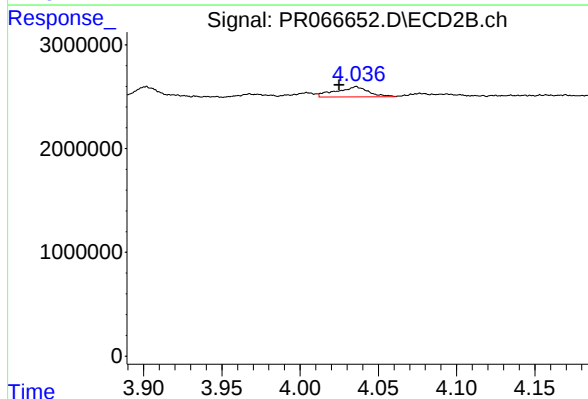


#17 AR-1242-2

R.T.: 4.036 min
Delta R.T.: 0.011 min
Response: 1445362
Conc: 8.15 ng/ml

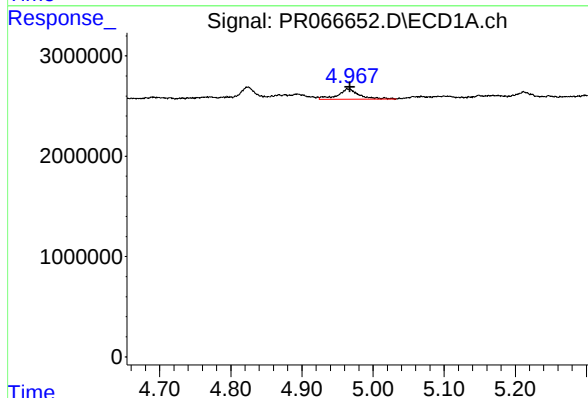


#18 AR-1242-3

R.T.: 4.967 min
Delta R.T.: -0.001 min
Response: 2090195
Conc: 17.55 ng/ml

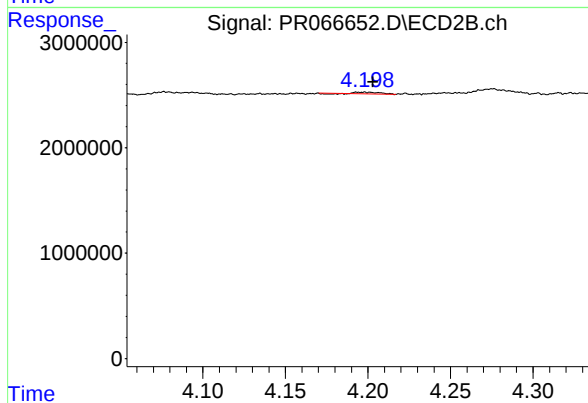

#18 AR-1242-3


R.T.: 4.194 min
Delta R.T.: -0.009 min
Response: 137932
Conc: 1.44 ng/ml

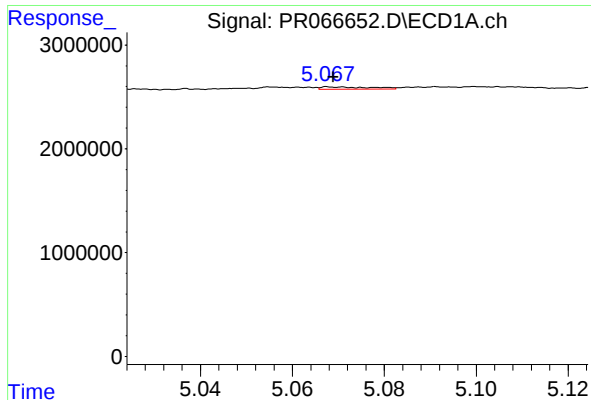

#19 AR-1242-4


R.T.: 5.068 min
Delta R.T.: 0.000 min
Response: 173338
Conc: 1.83 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

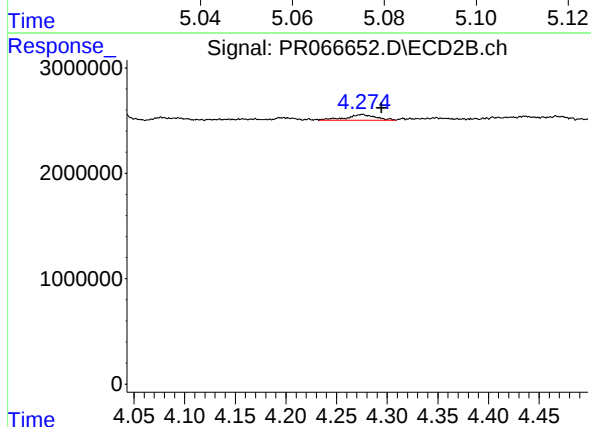


#19 AR-1242-4

R.T.: 4.275 min
Delta R.T.: -0.019 min
Response: 1085450
Conc: 11.37 ng/ml

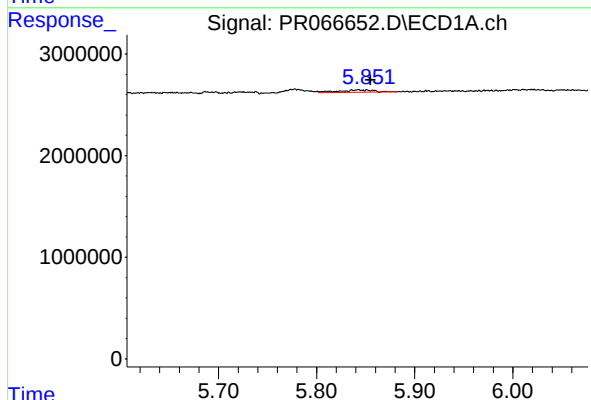


#20 AR-1242-5

R.T.: 5.850 min
Delta R.T.: -0.005 min
Response: 563590
Conc: 6.27 ng/ml

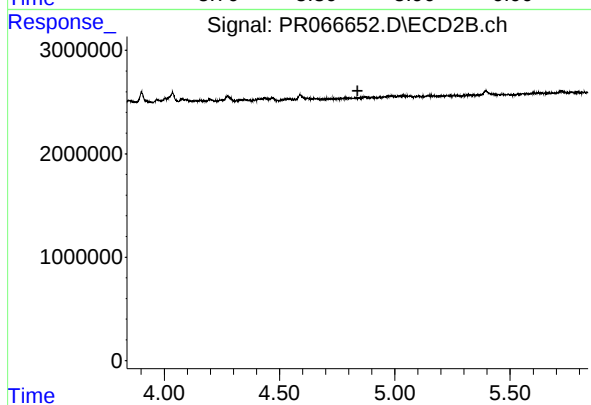

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 4.838 min
Response: 0
Conc: N.D.

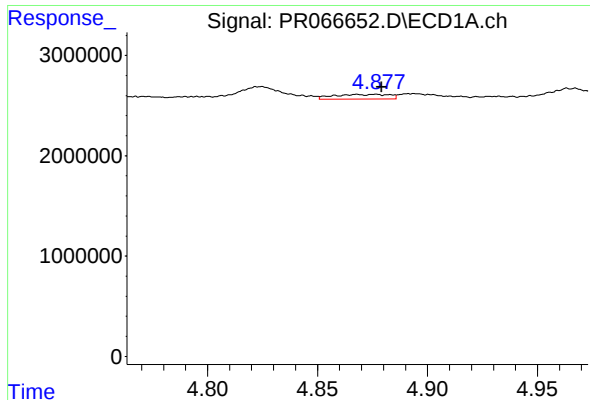

#21 AR-1248-1


R.T.: 4.868 min
Delta R.T.: -0.011 min
Response: 816403
Conc: 9.43 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

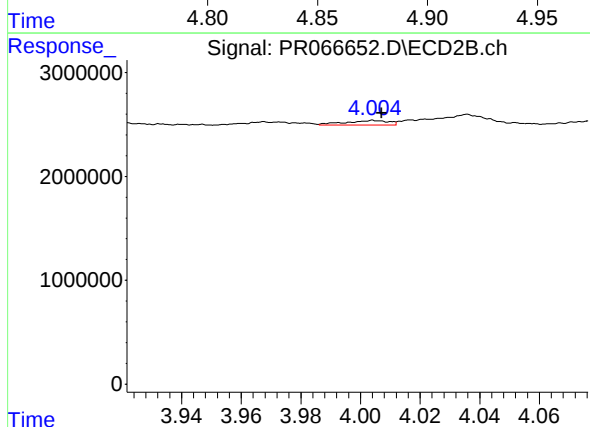


#21 AR-1248-1

R.T.: 4.005 min
Delta R.T.: -0.003 min
Response: 444979
Conc: 4.79 ng/ml

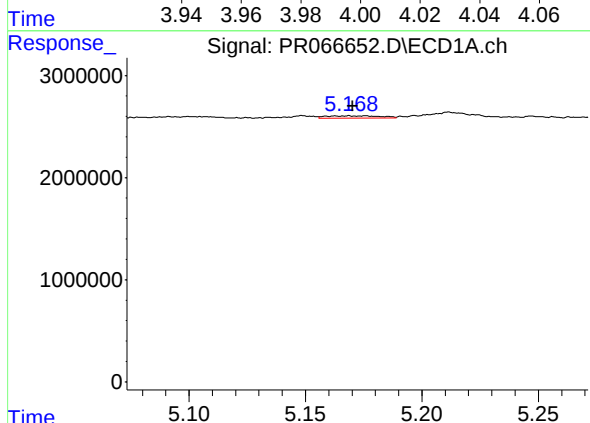


#22 AR-1248-2

R.T.: 5.169 min
Delta R.T.: -0.001 min
Response: 374617
Conc: 2.81 ng/ml

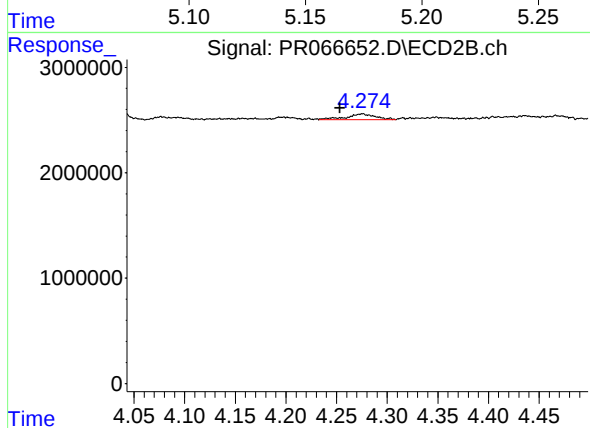

#22 AR-1248-2


R.T.: 4.275 min
Delta R.T.: 0.022 min
Response: 1085450
Conc: 8.02 ng/ml

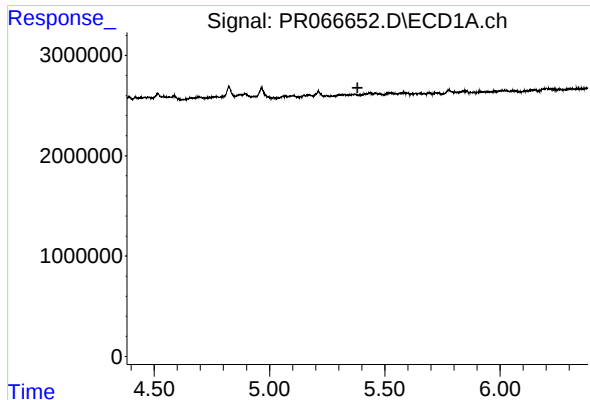

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

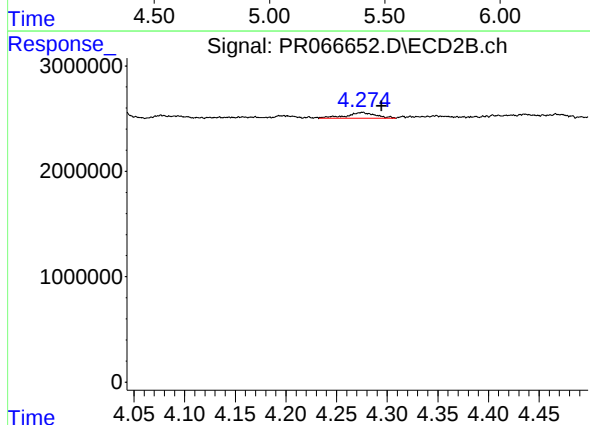


#23 AR-1248-3

R.T.: 4.275 min
Delta R.T.: -0.019 min
Response: 1085450
Conc: 7.88 ng/ml

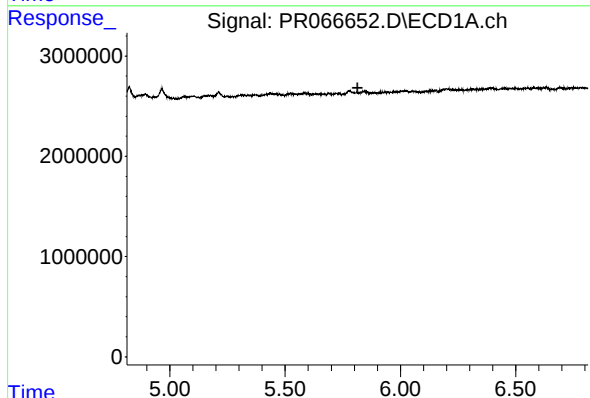


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 5.814 min
Response: 0
Conc: N.D.

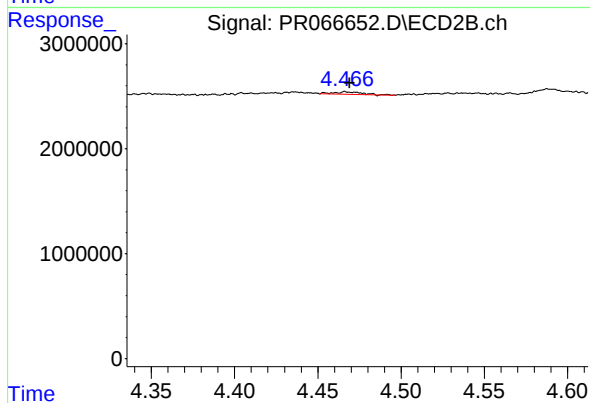

#24 AR-1248-4


R.T.: 4.467 min
Delta R.T.: -0.002 min
Response: 281278
Conc: 1.70 ng/ml

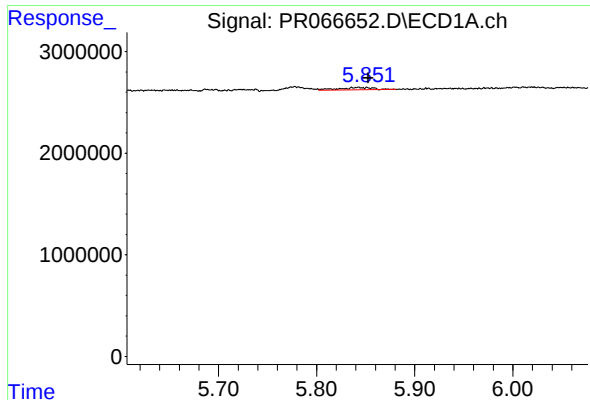

#25 AR-1248-5


R.T.: 5.850 min
Delta R.T.: -0.003 min
Response: 563590
Conc: 3.94 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

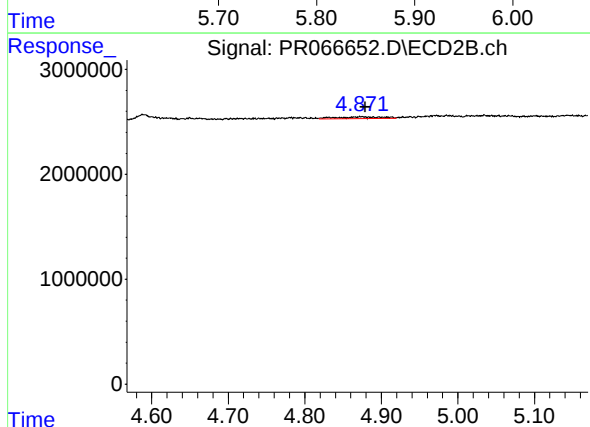


#25 AR-1248-5

R.T.: 4.873 min
Delta R.T.: -0.006 min
Response: 633663
Conc: 3.93 ng/ml

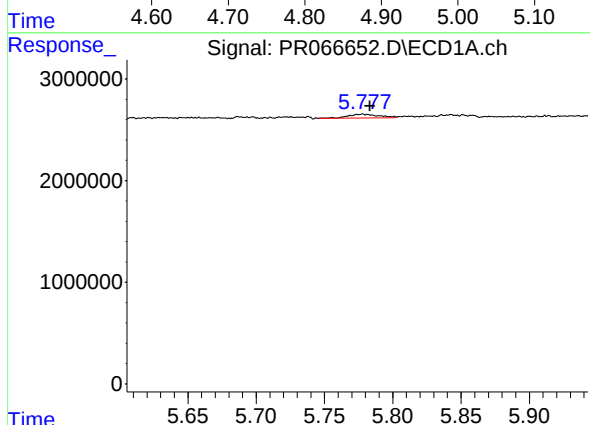


#26 AR-1254-1

R.T.: 5.778 min
Delta R.T.: -0.005 min
Response: 561133
Conc: 3.38 ng/ml

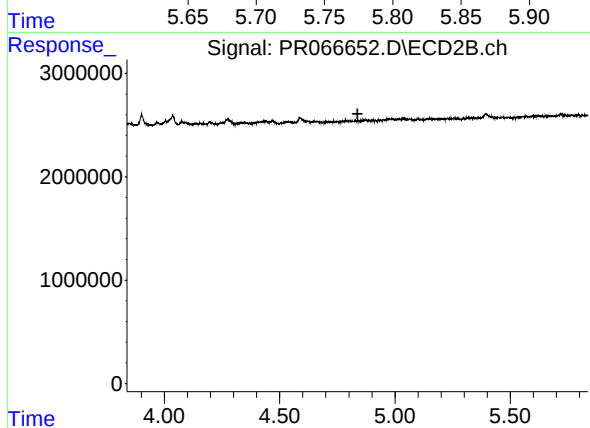

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 4.838 min
Response: 0
Conc: N.D.

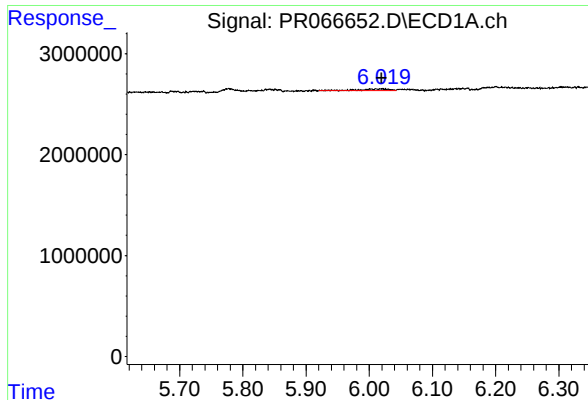

#27 AR-1254-2


R.T.: 6.020 min
Delta R.T.: 0.000 min
Response: 493288
Conc: 2.01 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

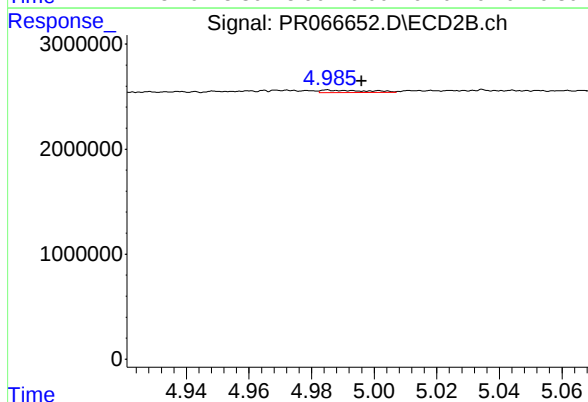


#27 AR-1254-2

R.T.: 4.985 min
Delta R.T.: -0.011 min
Response: 229737
Conc: 1.05 ng/ml

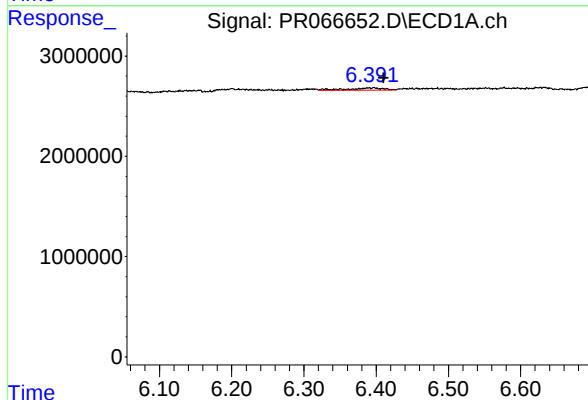


#28 AR-1254-3

R.T.: 6.396 min
Delta R.T.: -0.015 min
Response: 842974
Conc: 3.41 ng/ml

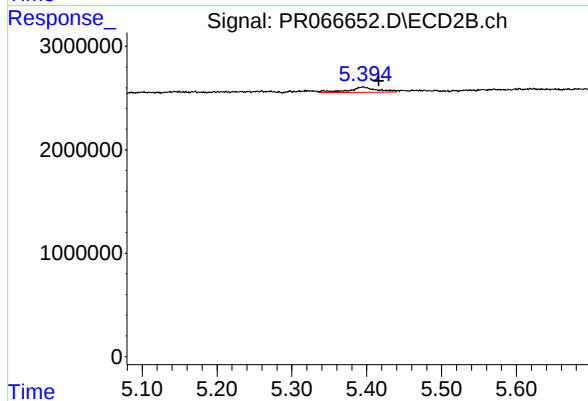

#28 AR-1254-3


R.T.: 5.395 min
Delta R.T.: -0.021 min
Response: 1391153
Conc: 4.05 ng/ml

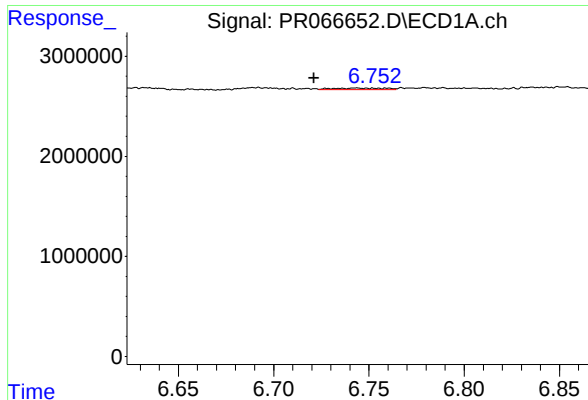

#29 AR-1254-4


R.T.: 6.744 min
Delta R.T.: 0.023 min
Response: 296205
Conc: 1.87 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

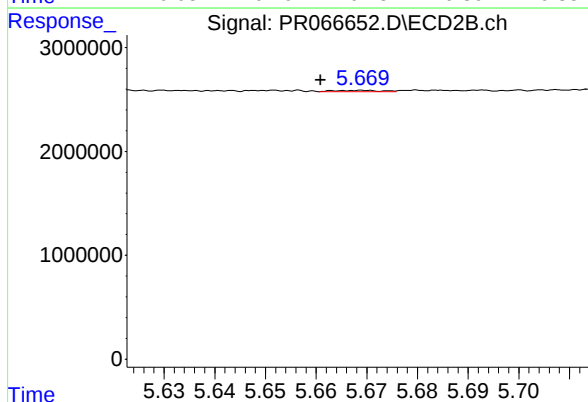


#29 AR-1254-4

R.T.: 5.669 min
Delta R.T.: 0.008 min
Response: 80005
Conc: 0.37 ng/ml

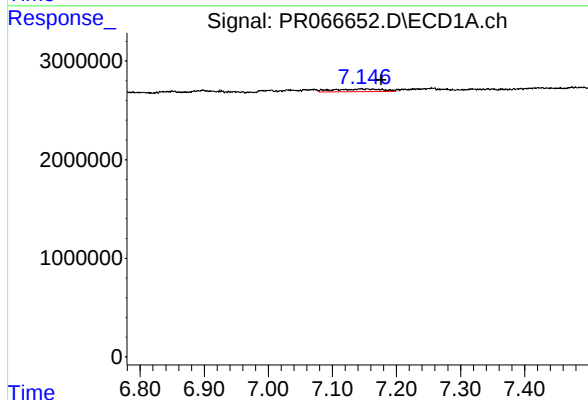


#30 AR-1254-5

R.T.: 7.154 min
Delta R.T.: -0.022 min
Response: 1420300
Conc: 7.97 ng/ml

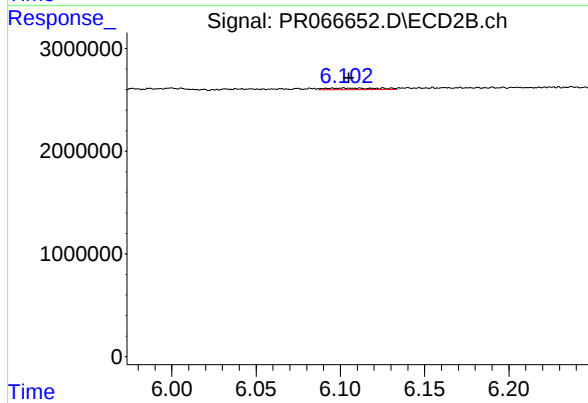

#30 AR-1254-5


R.T.: 6.102 min
Delta R.T.: -0.003 min
Response: 369736
Conc: 1.15 ng/ml

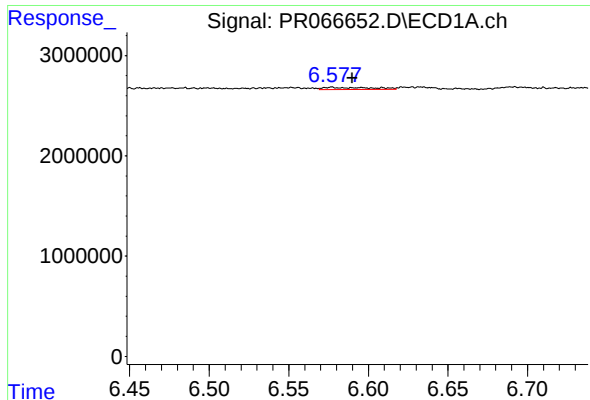

#31 AR-1260-1


R.T.: 6.577 min
Delta R.T.: -0.013 min
Response: 457904
Conc: 2.20 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

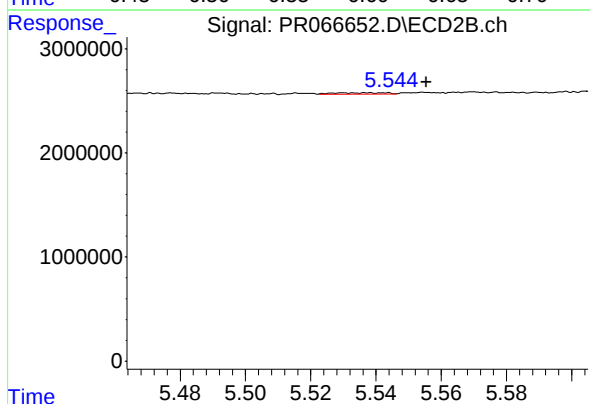


#31 AR-1260-1

R.T.: 5.538 min
Delta R.T.: -0.018 min
Response: 158514
Conc: 0.63 ng/ml

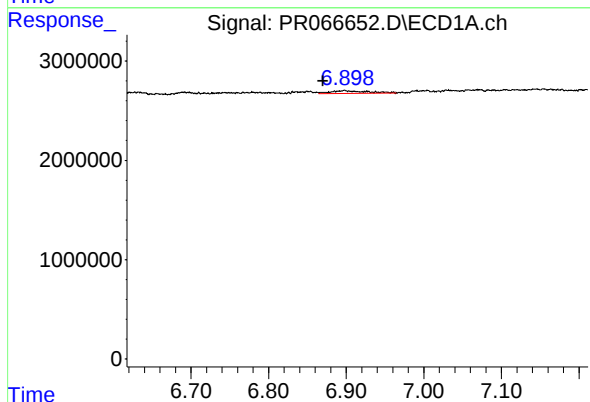


#32 AR-1260-2

R.T.: 6.898 min
Delta R.T.: 0.028 min
Response: 903604
Conc: 4.07 ng/ml

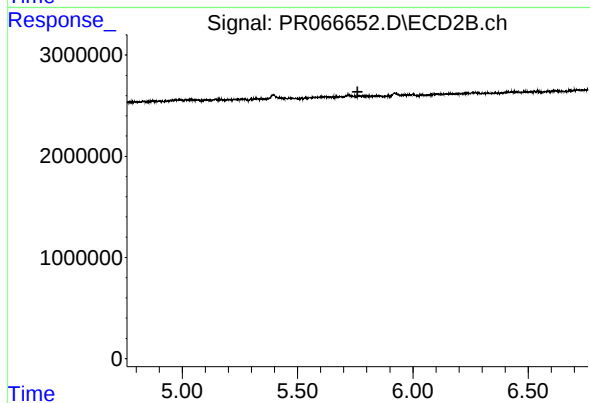

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 5.760 min
Response: 0
Conc: N.D.

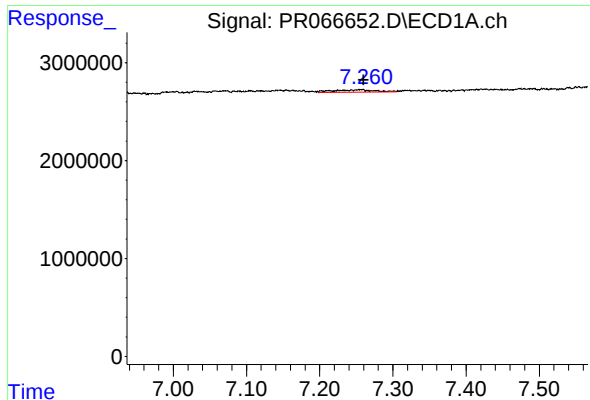

#33 AR-1260-3


R.T.: 7.255 min
Delta R.T.: -0.005 min
Response: 989976
Conc: 5.90 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

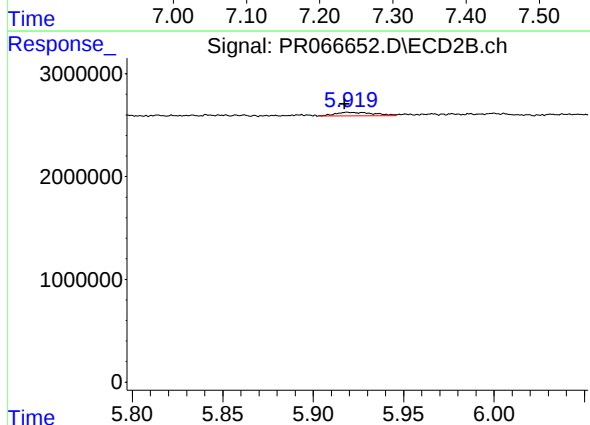


#33 AR-1260-3

R.T.: 5.919 min
Delta R.T.: 0.002 min
Response: 516717
Conc: 1.77 ng/ml

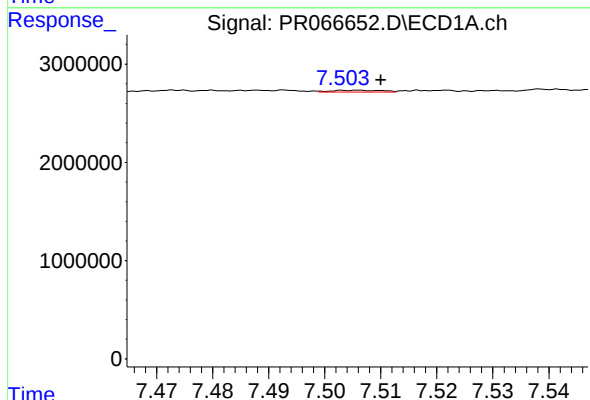


#34 AR-1260-4

R.T.: 7.506 min
Delta R.T.: -0.004 min
Response: 116511
Conc: 0.65 ng/ml

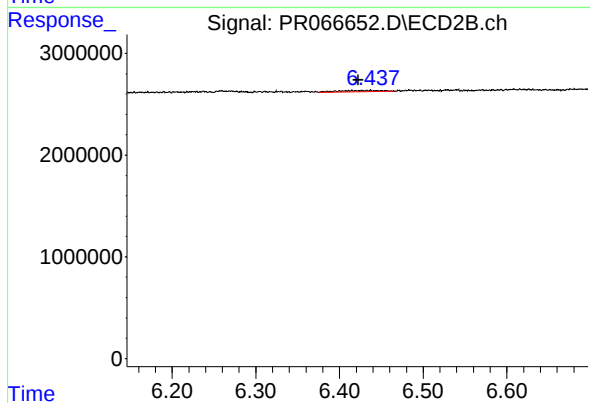

#34 AR-1260-4


R.T.: 6.437 min
Delta R.T.: 0.015 min
Response: 409497
Conc: 1.64 ng/ml

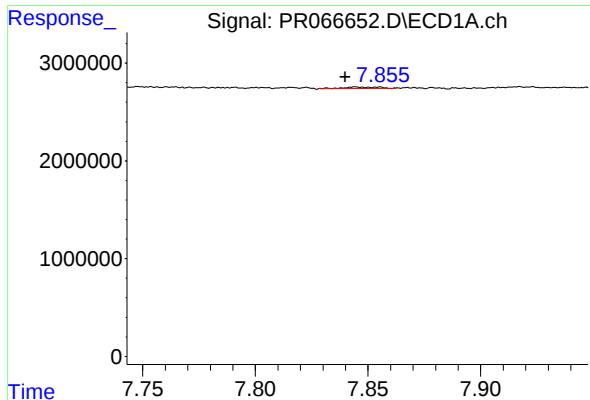

#35 AR-1260-5


R.T.: 7.846 min
Delta R.T.: 0.006 min
Response: 189693
Conc: 0.65 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

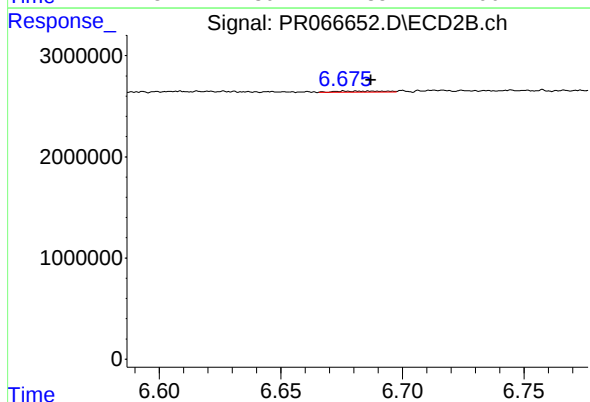


#35 AR-1260-5

R.T.: 6.676 min
Delta R.T.: -0.011 min
Response: 158097
Conc: 0.28 ng/ml

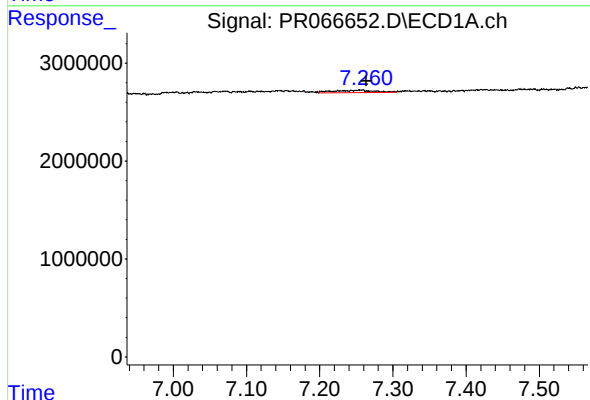


#36 AR-1262-1

R.T.: 7.255 min
Delta R.T.: -0.008 min
Response: 989976
Conc: 4.34 ng/ml

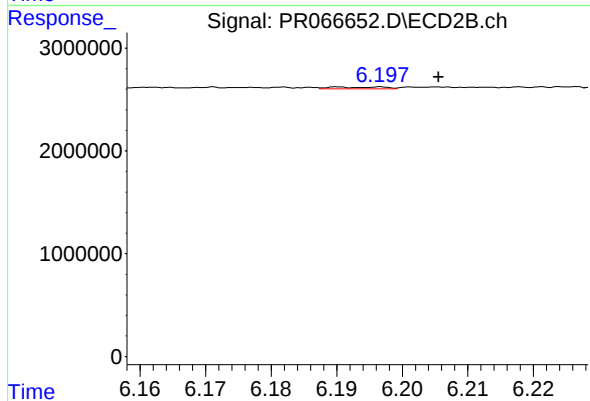

#36 AR-1262-1


R.T.: 6.191 min
Delta R.T.: -0.015 min
Response: 99792
Conc: 0.69 ng/ml

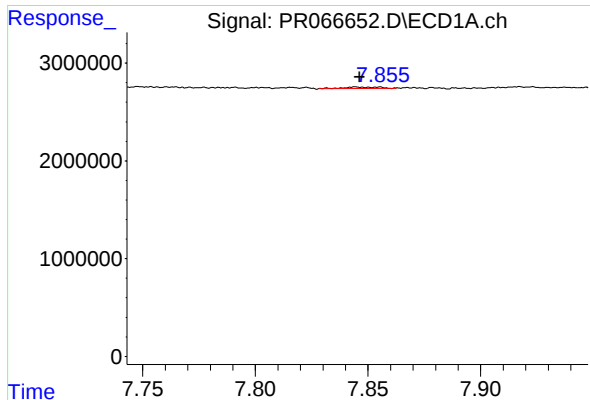

#37 AR-1262-2


R.T.: 7.846 min
Delta R.T.: 0.000 min
Response: 189693
Conc: 0.60 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

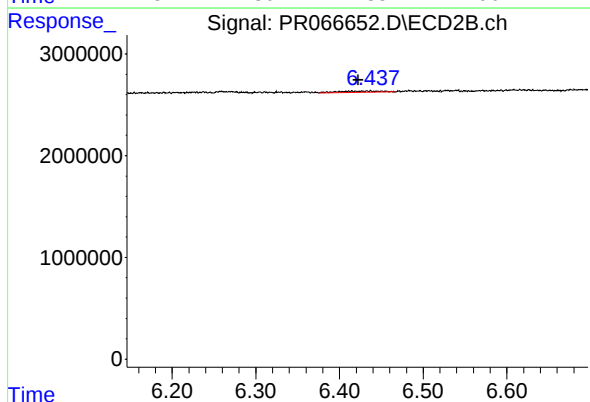


#37 AR-1262-2

R.T.: 6.437 min
Delta R.T.: 0.015 min
Response: 409497
Conc: 1.33 ng/ml

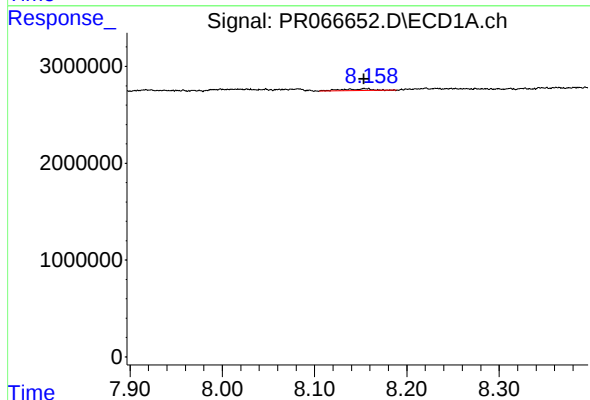


#38 AR-1262-3

R.T.: 8.155 min
Delta R.T.: 0.002 min
Response: 411824
Conc: 1.95 ng/ml

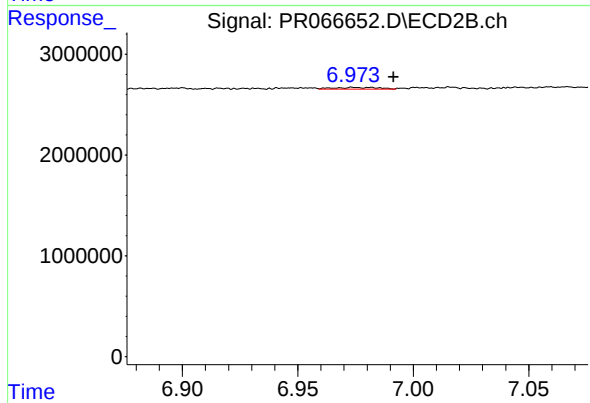

#38 AR-1262-3


R.T.: 6.980 min
Delta R.T.: -0.011 min
Response: 222028
Conc: 0.92 ng/ml

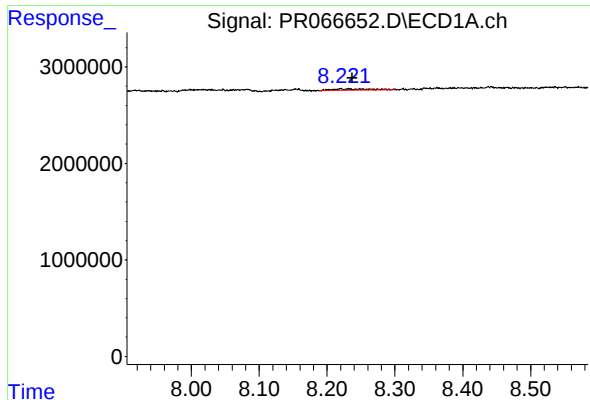

#39 AR-1262-4


R.T.: 8.220 min
Delta R.T.: -0.017 min
Response: 500692
Conc: 4.58 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

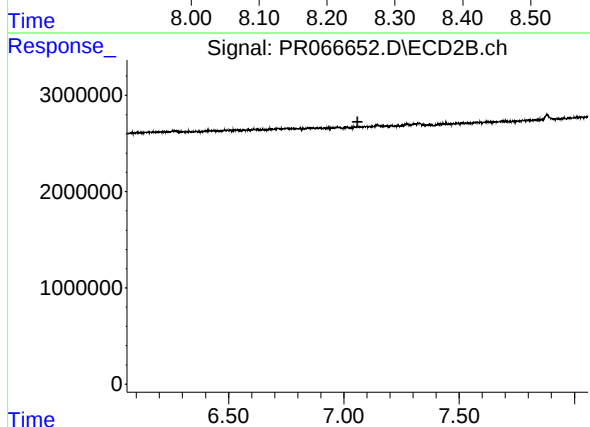


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.059 min
Response: 0
Conc: N.D.

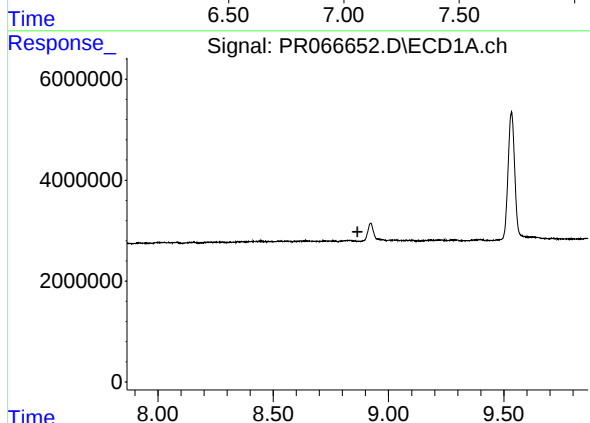


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 8.865 min
Response: 0
Conc: N.D.

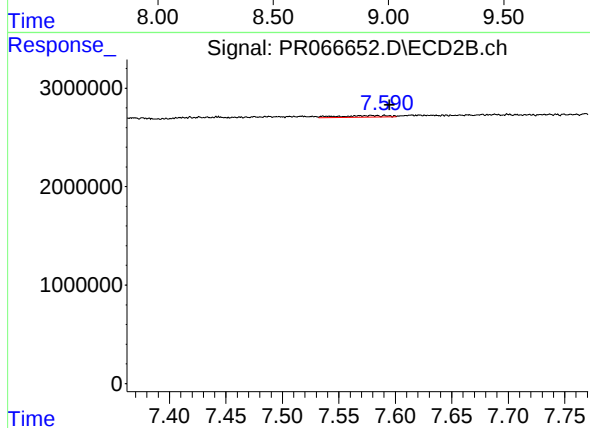

#40 AR-1262-5


R.T.: 7.591 min
Delta R.T.: -0.004 min
Response: 499574
Conc: 2.31 ng/ml

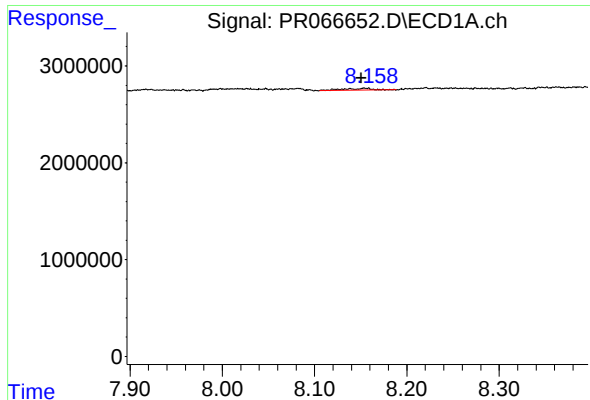

#41 AR-1268-1


R.T.: 8.155 min
Delta R.T.: 0.004 min
Response: 411824
Conc: 1.06 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

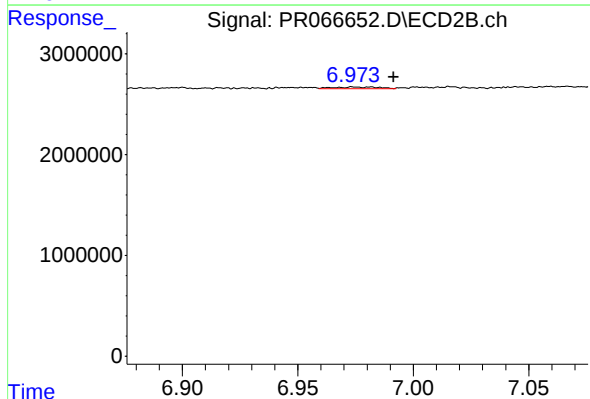


#41 AR-1268-1

R.T.: 6.980 min
Delta R.T.: -0.011 min
Response: 222028
Conc: 0.31 ng/ml

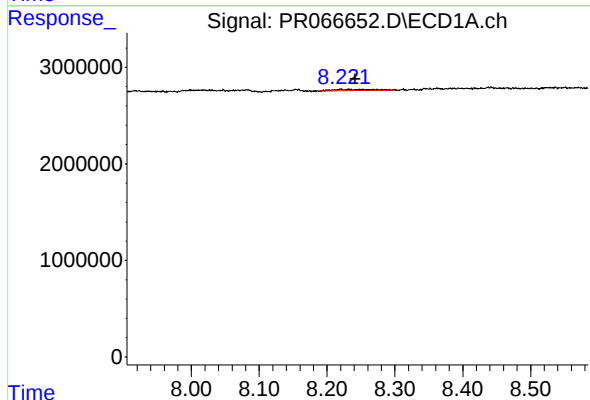


#42 AR-1268-2

R.T.: 8.220 min
Delta R.T.: -0.021 min
Response: 500692
Conc: 1.46 ng/ml

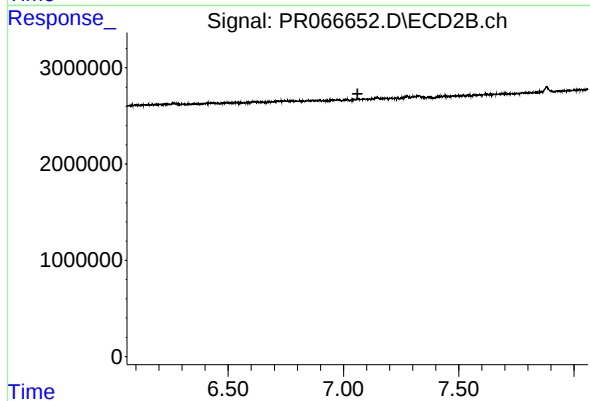

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 7.061 min
Response: 0
Conc: N.D.

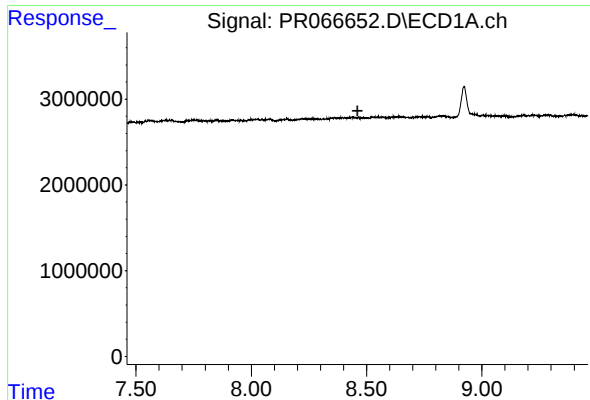

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

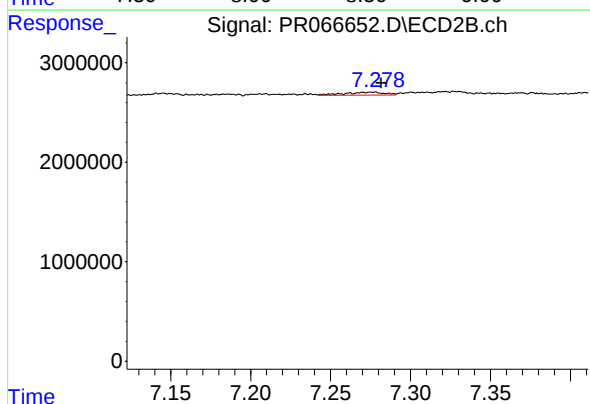


#43 AR-1268-3

R.T.: 7.275 min
Delta R.T.: -0.007 min
Response: 513302
Conc: 0.91 ng/ml

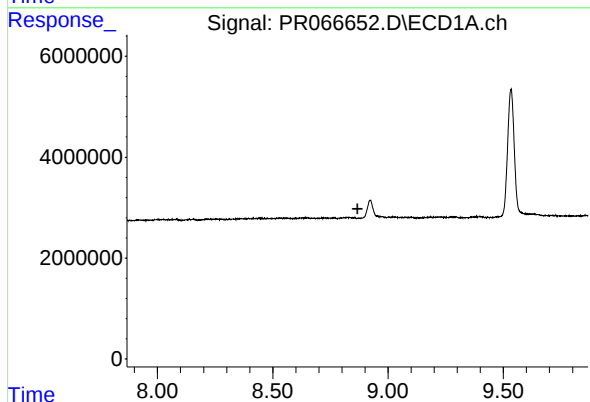


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 8.867 min
Response: 0
Conc: N.D.

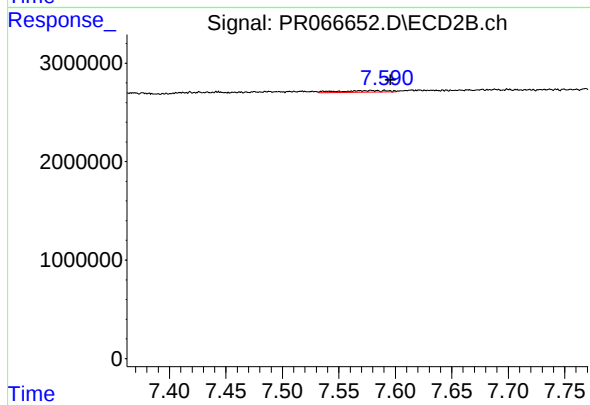

#44 AR-1268-4


R.T.: 7.591 min
Delta R.T.: -0.005 min
Response: 499574
Conc: 2.05 ng/ml

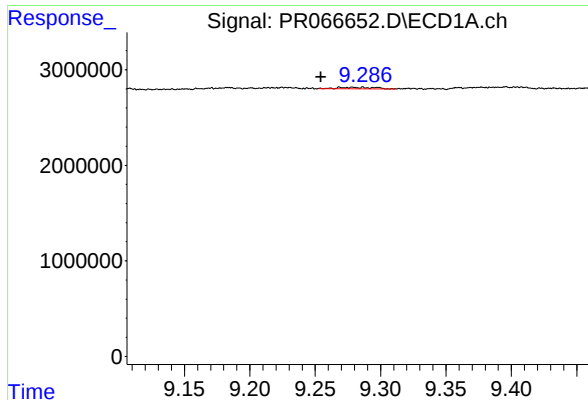

#45 AR-1268-5

R.T.: 9.279 min
Delta R.T.: 0.025 min
Response: 272472
Conc: 0.33 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

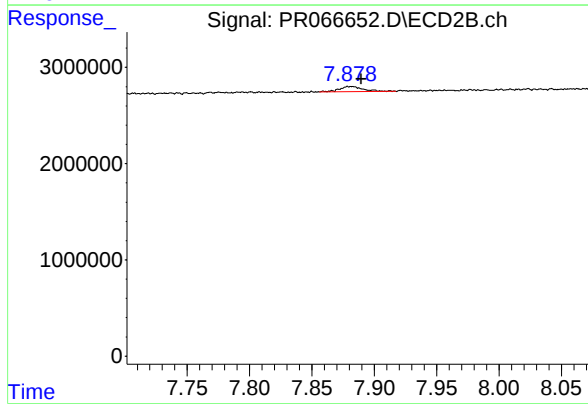

#45 AR-1268-5

R.T.: 7.881 min
Delta R.T.: -0.008 min
Response: 688833
Conc: 0.43 ng/ml