

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR050924\
 Data File : PR066655.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2024 06:16
 Operator : AJ\MA
 Sample : P2403-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT2-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 06:57:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 26 07:26:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.653	2.895	91787054	74888904	17.512	16.755
2) SA Decachlor...	9.534	8.121	39895921	75636035	17.036	16.115
Target Compounds						
3) L1 AR-1016-1	4.871	4.004	2470929	2213648	17.287	14.654
4) L1 AR-1016-2	4.894	4.021	2971844	2248652	13.589	10.480
5) L1 AR-1016-3	4.957	4.200	1845966	1443900	12.711	12.314
6) L1 AR-1016-4	5.057	4.249	1608585	3307446	13.999	34.284 #
7) L1 AR-1016-5	5.374	4.465	4145390	3814822	36.402	30.855
8) L2 AR-1221-1	3.859f	3.120	1121360	179650	18.571	3.316 #
9) L2 AR-1221-2	3.963	3.196	1443514	1148766	32.667	27.669
10) L2 AR-1221-3	4.039	3.280	258043	335301	1.987	2.775 #
11) L3 AR-1232-1	4.039	3.280	258043	335301	2.423	3.341 #
12) L3 AR-1232-2	4.585	4.021	1893328	2248652	30.853	22.594 #
13) L3 AR-1232-3	4.894	4.200	2971844	1443900	29.078	26.954
14) L3 AR-1232-4	5.057	4.290	1608585	3256083	29.872	67.134 #
15) L3 AR-1232-5	5.163	4.465	3754570	3814822	93.317	71.506
16) L4 AR-1242-1	4.871	4.004	2470929	2213648	20.760	17.684
17) L4 AR-1242-2	4.894	4.021	2971844	2248652	16.535	12.687
18) L4 AR-1242-3	4.957	4.200	1845966	1443900	15.496	15.027
19) L4 AR-1242-4	5.057	4.290	1608585	3256083	16.993	34.107 #
20) L4 AR-1242-5	5.846	4.833	3452481	5285856	38.394	43.036
21) L5 AR-1248-1	4.871	4.004	2470929	2213648	28.550	23.810
22) L5 AR-1248-2	5.163	4.249	3754570	3307446	28.208	24.442
23) L5 AR-1248-3	5.374	4.290	4145390	3256083	27.617	23.649
24) L5 AR-1248-4	5.806	4.465	3727256	3814822	26.159	23.078
25) L5 AR-1248-5	5.846	4.875	3452481	3642784	24.108	22.574
26) L6 AR-1254-1	5.776	4.833	3511873	5285856	21.133	21.509
27) L6 AR-1254-2	6.013	4.991	4123720	2039126	16.834	9.311 #
28) L6 AR-1254-3	6.402	5.411	3179685	3428841	12.863	9.975
29) L6 AR-1254-4	6.715	5.657	2143602	1776366	13.502	8.320 #
30) L6 AR-1254-5	7.186	6.100	168453	811362	0.945	2.521 #
31) L7 AR-1260-1	6.583	5.559	459095	1588801	2.209	6.269 #
32) L7 AR-1260-2	6.900f	5.753	1212116	318936	5.464	1.047 #
33) L7 AR-1260-3	7.253	5.918	576598	746419	3.438	2.564 #
34) L7 AR-1260-4	7.520	6.424	434034	119701	2.436	0.479 #
35) L7 AR-1260-5	7.831	6.682	187196	130031	0.641	0.232 #
36) L8 AR-1262-1	7.253	6.199	576598	191850	2.528	1.328 #
37) L8 AR-1262-2	7.831f	6.424	187196	119701	0.589	0.389 #
38) L8 AR-1262-3	0.000	7.012f	0	198632	N.D.	0.819 #
39) L8 AR-1262-4	8.258f	7.063	714061	144404	6.537	0.329 #
40) L8 AR-1262-5	0.000	7.605	0	105221	N.D.	0.487 #
41) L9 AR-1268-1	0.000	7.012f	0	198632	N.D.	0.274 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR050924\
Data File : PR066655.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2024 06:16
Operator : AJ\MA
Sample : P2403-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 70 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 06:57:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 26 07:26:35 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm


	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.258f	7.063	714061	144404	2.078	0.225 #
43) L9	AR-1268-3	0.000	7.275	0	699621	N.D.	1.234 #
44) L9	AR-1268-4	0.000	7.605	0	105221	N.D.	0.431 #
45) L9	AR-1268-5	0.000	7.881	0	555274	N.D.	0.343 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

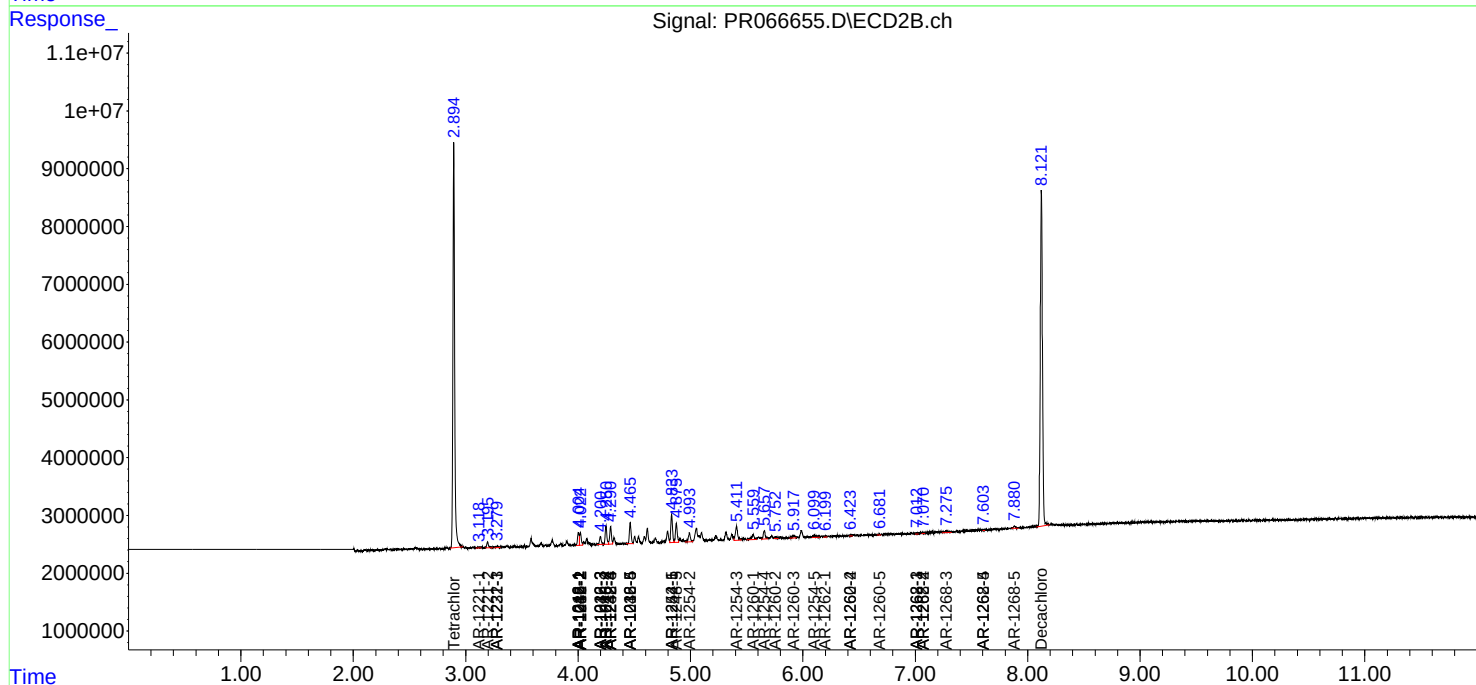


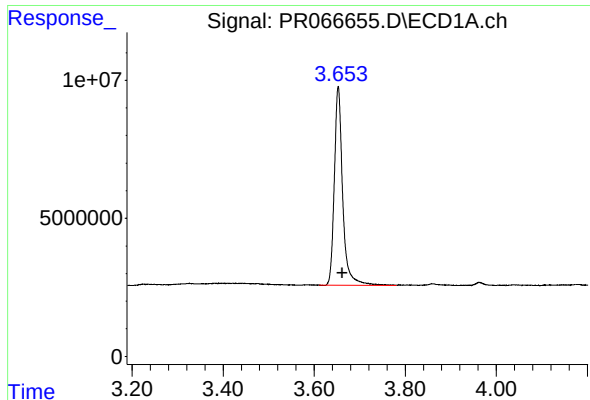

#1 Tetrachloro-m-xylene


R.T.: 3.653 min
Delta R.T.: -0.009 min
Response: 91787054
Conc: 17.51 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

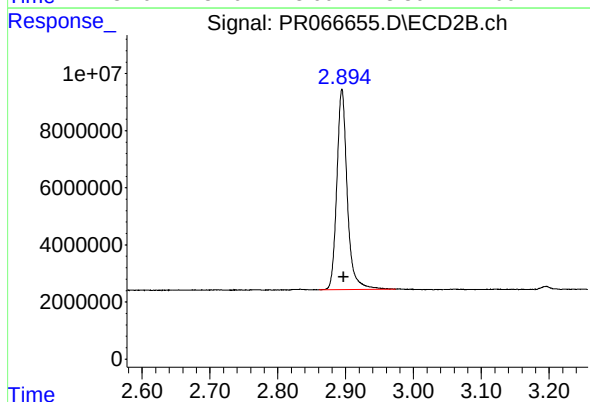


#1 Tetrachloro-m-xylene

R.T.: 2.895 min
Delta R.T.: -0.003 min
Response: 74888904
Conc: 16.75 ng/ml

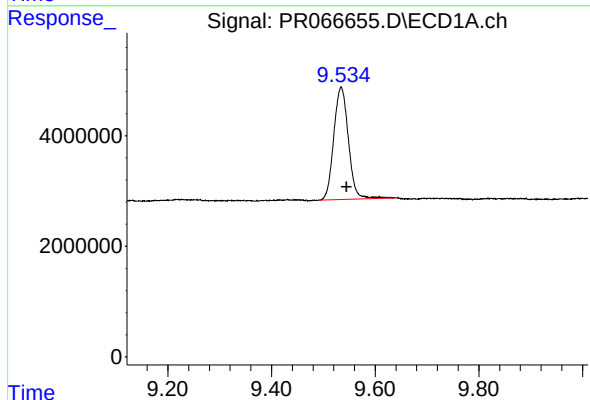


#2 Decachlorobiphenyl

R.T.: 9.534 min
Delta R.T.: -0.011 min
Response: 39895921
Conc: 17.04 ng/ml

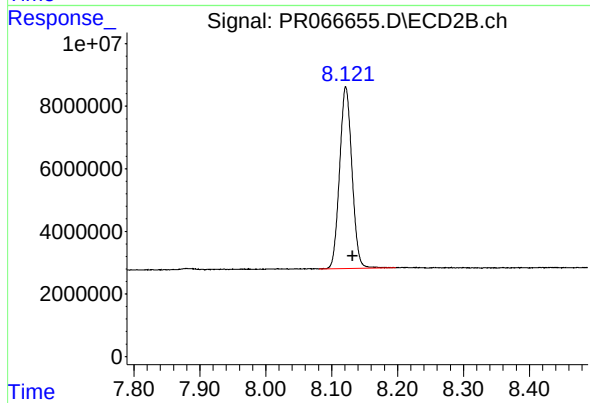

#2 Decachlorobiphenyl


R.T.: 8.121 min
Delta R.T.: -0.010 min
Response: 75636035
Conc: 16.11 ng/ml

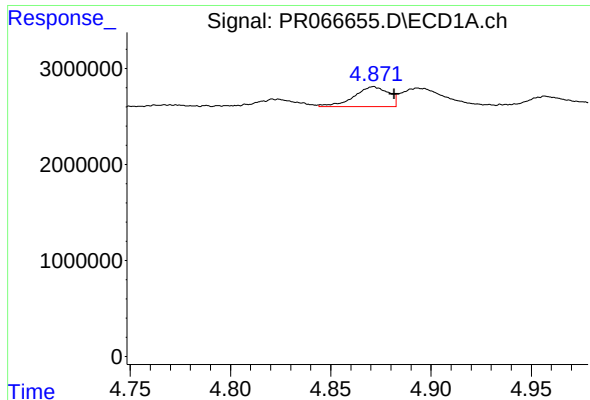

#3 AR-1016-1


R.T.: 4.871 min
Delta R.T.: -0.010 min
Response: 2470929
Conc: 17.29 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

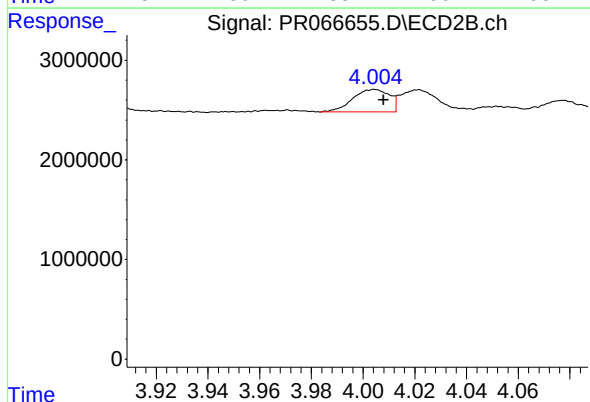


#3 AR-1016-1

R.T.: 4.004 min
Delta R.T.: -0.004 min
Response: 2213648
Conc: 14.65 ng/ml

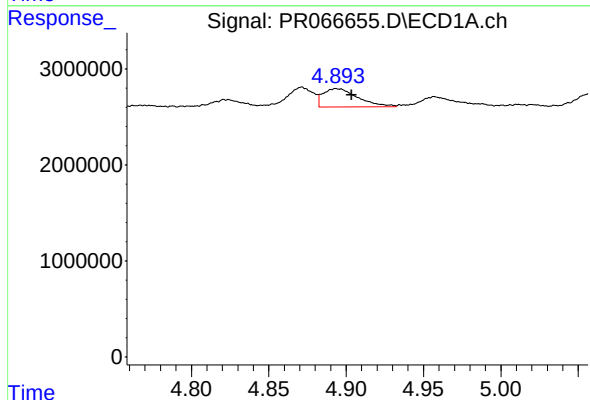


#4 AR-1016-2

R.T.: 4.894 min
Delta R.T.: -0.010 min
Response: 2971844
Conc: 13.59 ng/ml

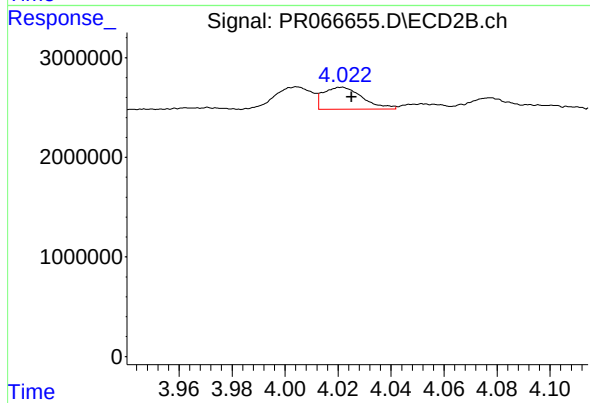

#4 AR-1016-2


R.T.: 4.021 min
Delta R.T.: -0.004 min
Response: 2248652
Conc: 10.48 ng/ml

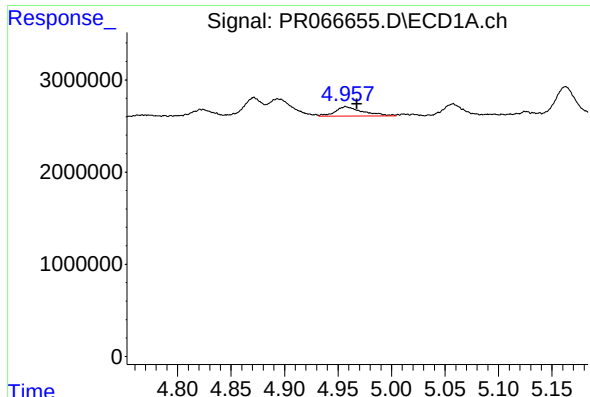

#5 AR-1016-3


R.T.: 4.957 min
Delta R.T.: -0.010 min
Response: 1845966
Conc: 12.71 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

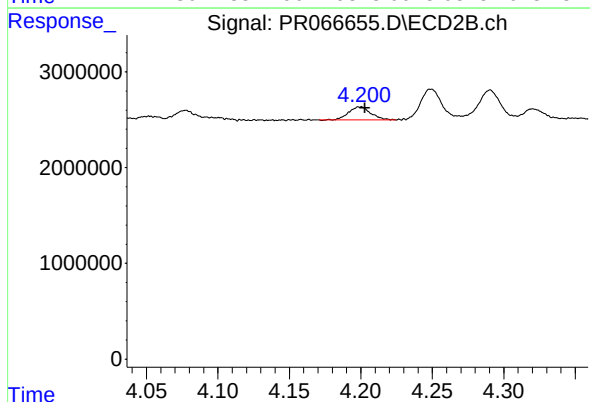


#5 AR-1016-3

R.T.: 4.200 min
Delta R.T.: -0.003 min
Response: 1443900
Conc: 12.31 ng/ml

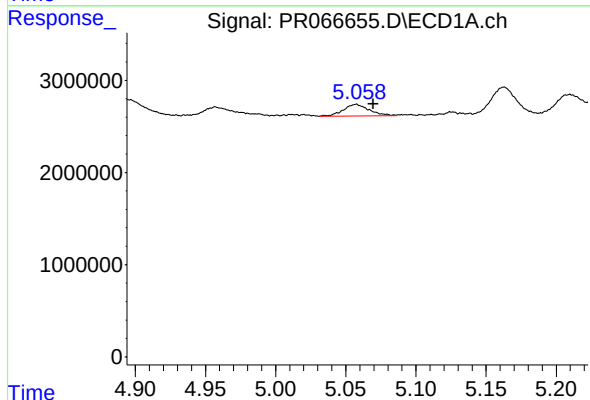


#6 AR-1016-4

R.T.: 5.057 min
Delta R.T.: -0.012 min
Response: 1608585
Conc: 14.00 ng/ml

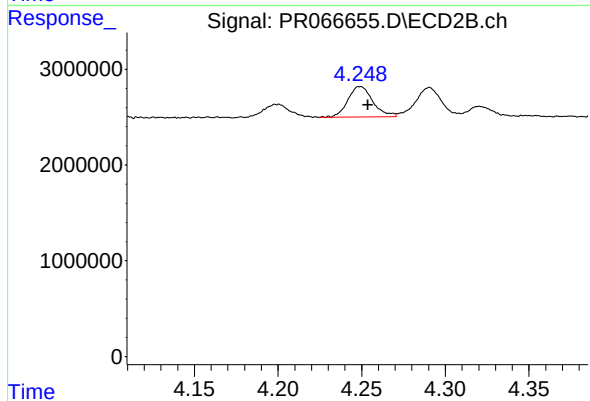

#6 AR-1016-4


R.T.: 4.249 min
Delta R.T.: -0.005 min
Response: 3307446
Conc: 34.28 ng/ml

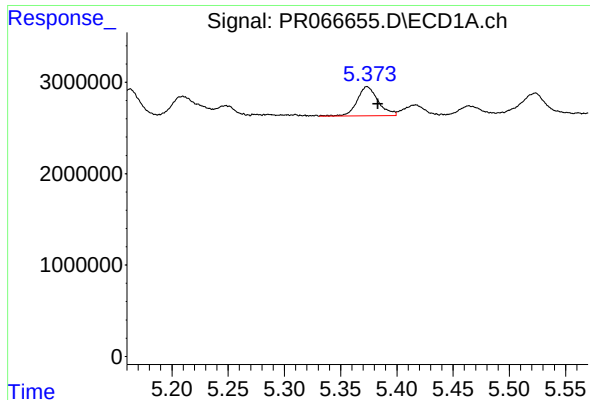

#7 AR-1016-5


R.T.: 5.374 min
Delta R.T.: -0.010 min
Response: 4145390
Conc: 36.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

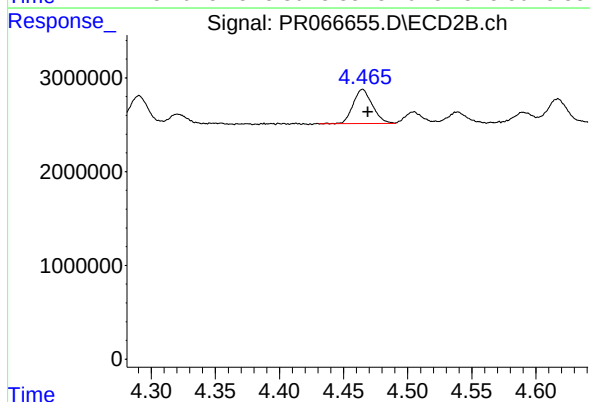


#7 AR-1016-5

R.T.: 4.465 min
Delta R.T.: -0.004 min
Response: 3814822
Conc: 30.86 ng/ml

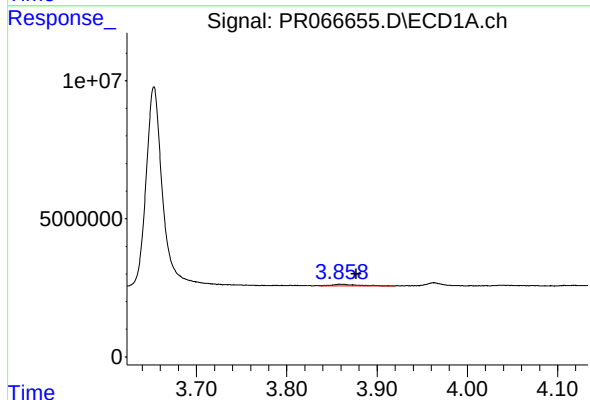


#8 AR-1221-1

R.T.: 3.859 min
Delta R.T.: -0.017 min
Response: 1121360
Conc: 18.57 ng/ml

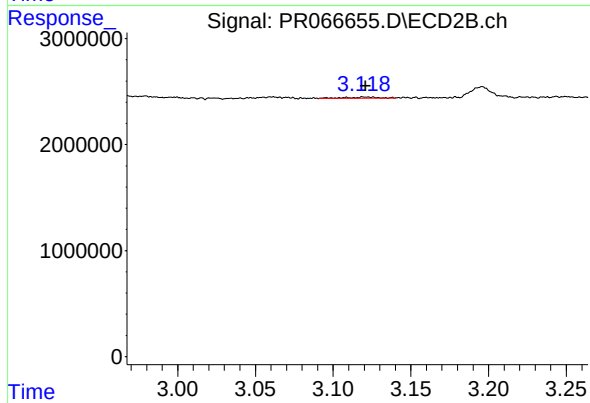

#8 AR-1221-1


R.T.: 3.120 min
Delta R.T.: -0.001 min
Response: 179650
Conc: 3.32 ng/ml

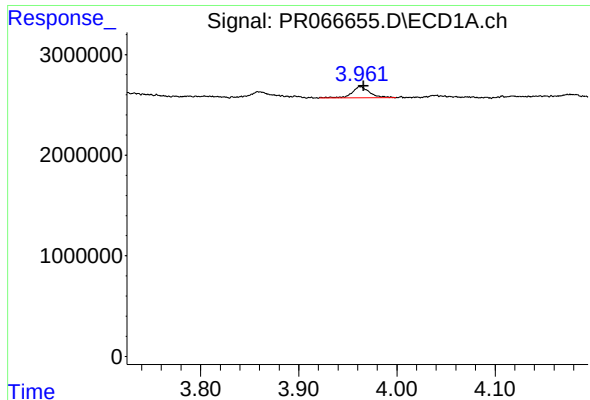

#9 AR-1221-2


R.T.: 3.963 min
Delta R.T.: -0.003 min
Response: 1443514
Conc: 32.67 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

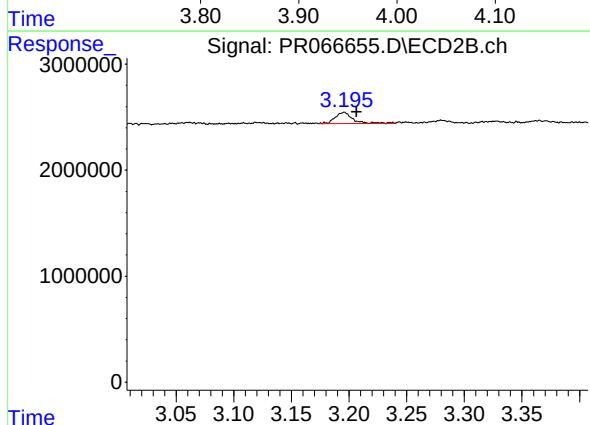


#9 AR-1221-2

R.T.: 3.196 min
Delta R.T.: -0.011 min
Response: 1148766
Conc: 27.67 ng/ml

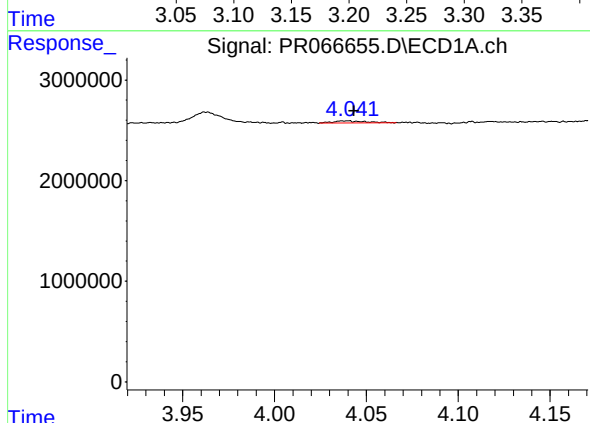


#10 AR-1221-3

R.T.: 4.039 min
Delta R.T.: -0.005 min
Response: 258043
Conc: 1.99 ng/ml

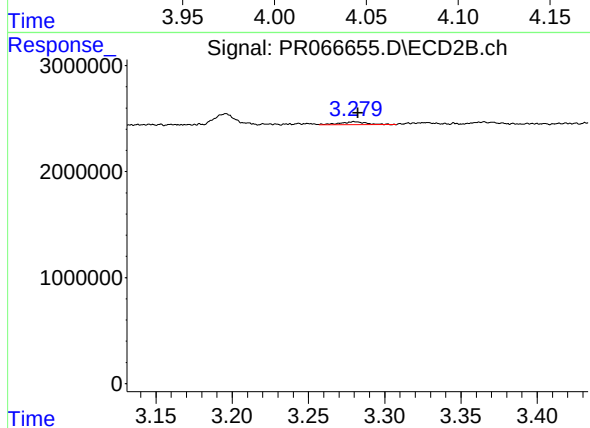

#10 AR-1221-3


R.T.: 3.280 min
Delta R.T.: -0.002 min
Response: 335301
Conc: 2.78 ng/ml

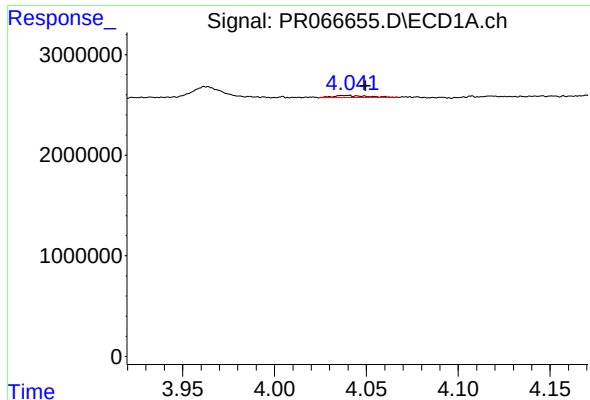

#11 AR-1232-1


R.T.: 4.039 min
Delta R.T.: -0.011 min
Response: 258043
Conc: 2.42 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

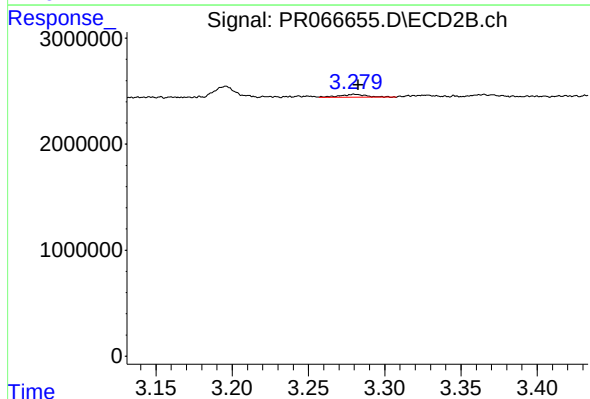


#11 AR-1232-1

R.T.: 3.280 min
Delta R.T.: -0.002 min
Response: 335301
Conc: 3.34 ng/ml

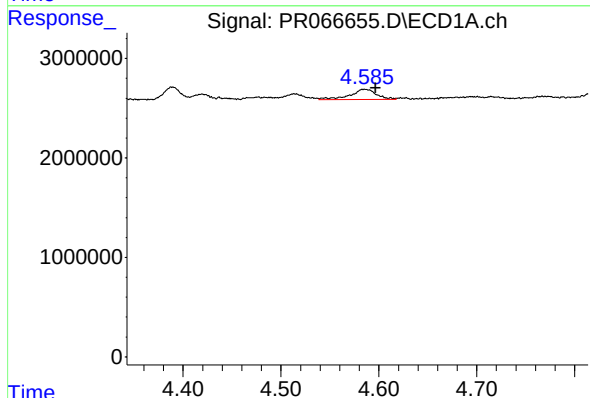


#12 AR-1232-2

R.T.: 4.585 min
Delta R.T.: -0.011 min
Response: 1893328
Conc: 30.85 ng/ml

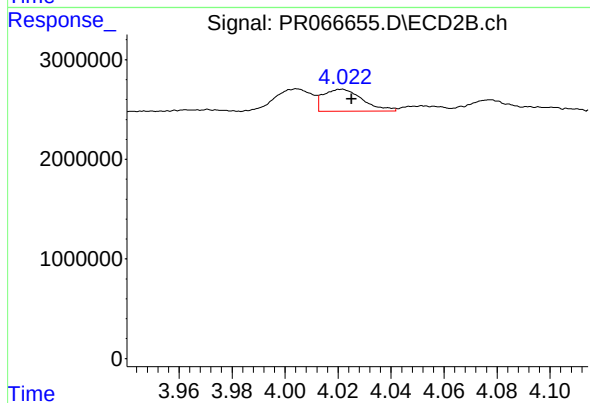

#12 AR-1232-2


R.T.: 4.021 min
Delta R.T.: -0.004 min
Response: 2248652
Conc: 22.59 ng/ml

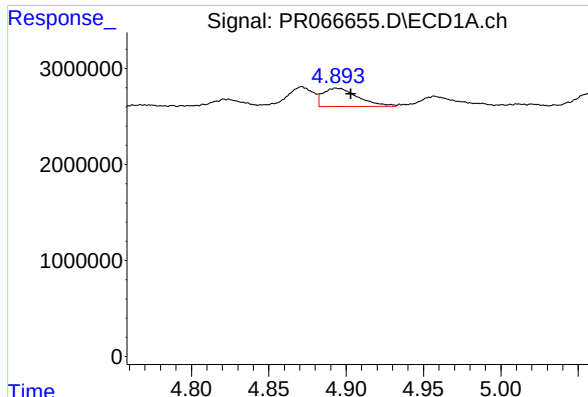

#13 AR-1232-3


R.T.: 4.894 min
Delta R.T.: -0.009 min
Response: 2971844
Conc: 29.08 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

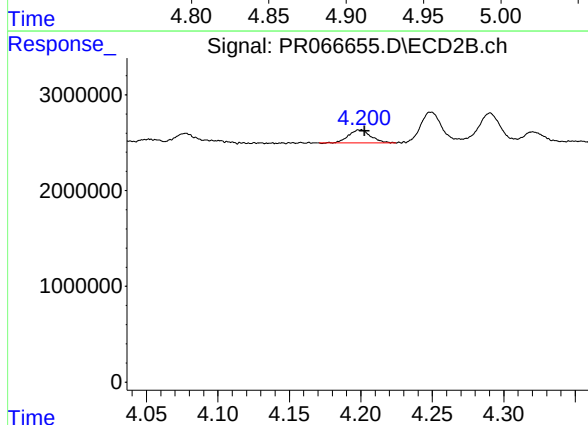


#13 AR-1232-3

R.T.: 4.200 min
Delta R.T.: -0.003 min
Response: 1443900
Conc: 26.95 ng/ml

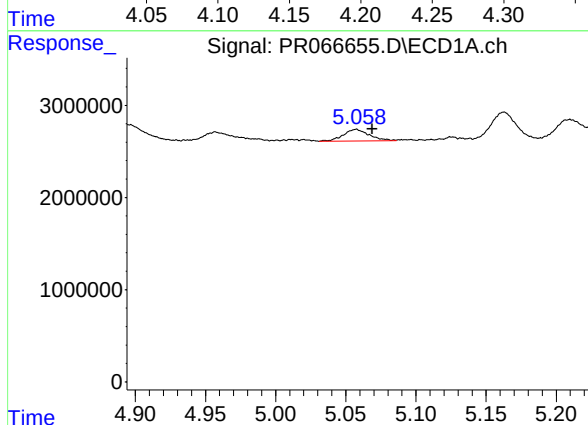


#14 AR-1232-4

R.T.: 5.057 min
Delta R.T.: -0.012 min
Response: 1608585
Conc: 29.87 ng/ml

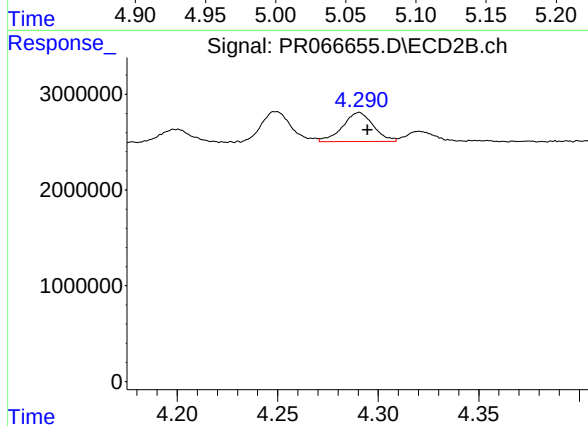

#14 AR-1232-4


R.T.: 4.290 min
Delta R.T.: -0.004 min
Response: 3256083
Conc: 67.13 ng/ml

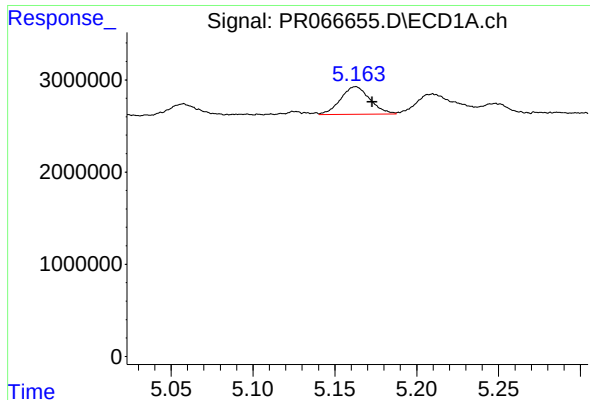

#15 AR-1232-5


R.T.: 5.163 min
Delta R.T.: -0.010 min
Response: 3754570
Conc: 93.32 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

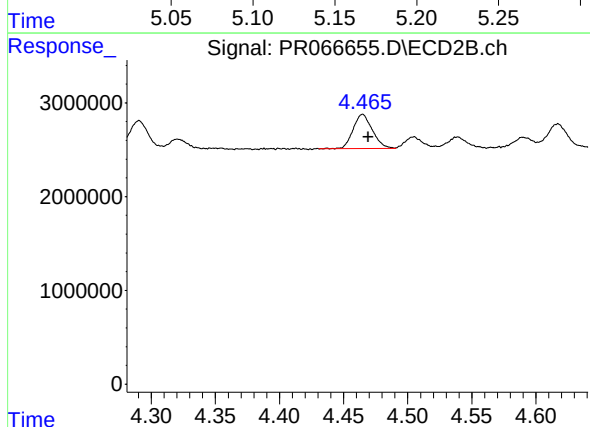


#15 AR-1232-5

R.T.: 4.465 min
Delta R.T.: -0.005 min
Response: 3814822
Conc: 71.51 ng/ml

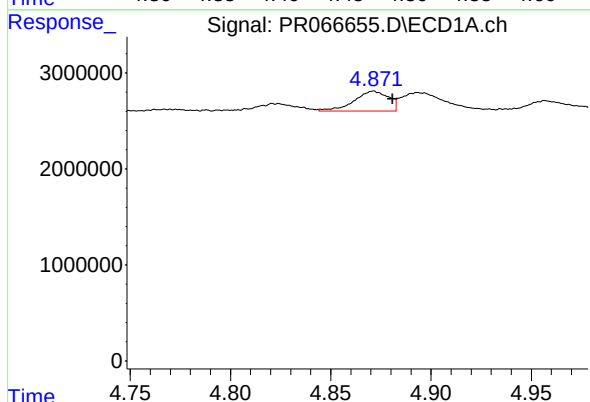


#16 AR-1242-1

R.T.: 4.871 min
Delta R.T.: -0.010 min
Response: 2470929
Conc: 20.76 ng/ml

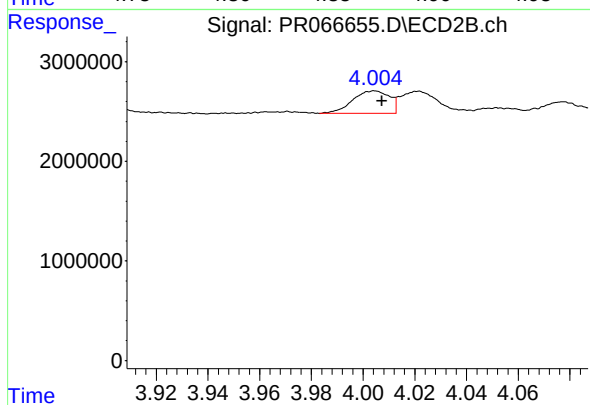

#16 AR-1242-1


R.T.: 4.004 min
Delta R.T.: -0.003 min
Response: 2213648
Conc: 17.68 ng/ml

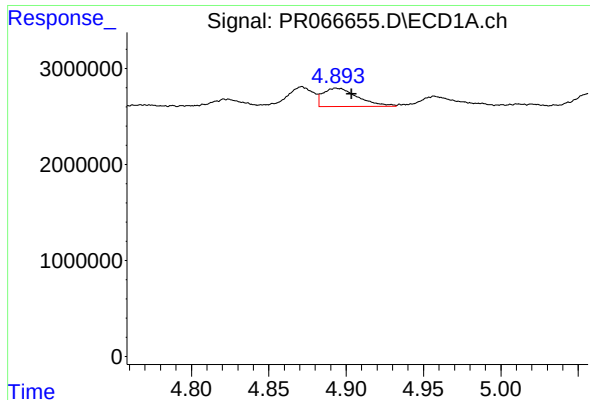

#17 AR-1242-2


R.T.: 4.894 min
Delta R.T.: -0.010 min
Response: 2971844
Conc: 16.53 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

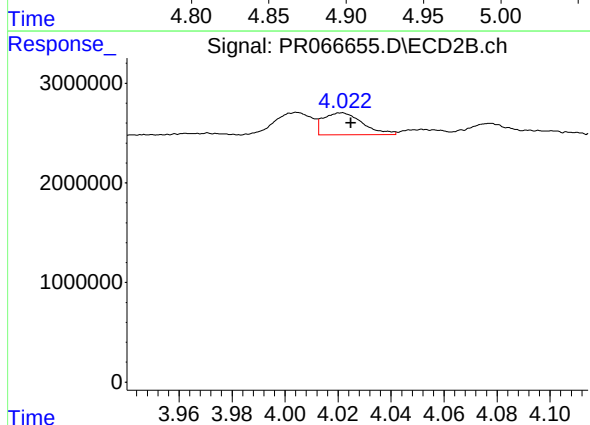


#17 AR-1242-2

R.T.: 4.021 min
Delta R.T.: -0.004 min
Response: 2248652
Conc: 12.69 ng/ml

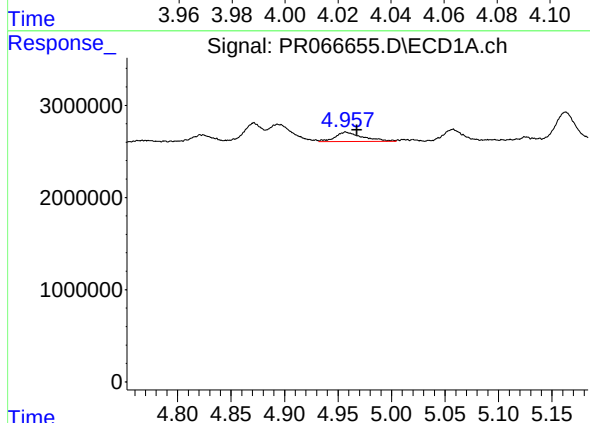


#18 AR-1242-3

R.T.: 4.957 min
Delta R.T.: -0.010 min
Response: 1845966
Conc: 15.50 ng/ml

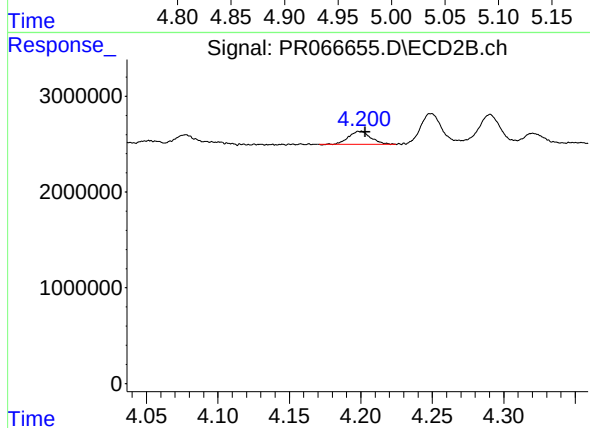

#18 AR-1242-3


R.T.: 4.200 min
Delta R.T.: -0.003 min
Response: 1443900
Conc: 15.03 ng/ml

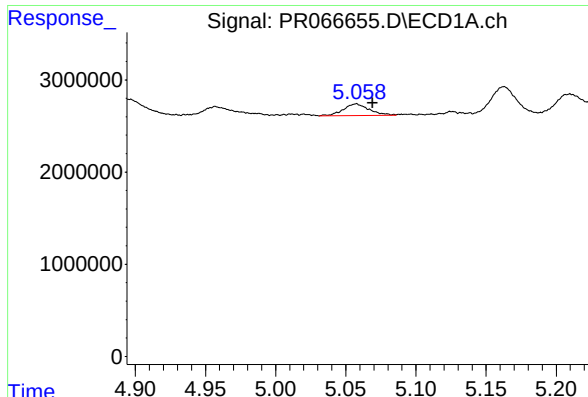

#19 AR-1242-4


R.T.: 5.057 min
Delta R.T.: -0.012 min
Response: 1608585
Conc: 16.99 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

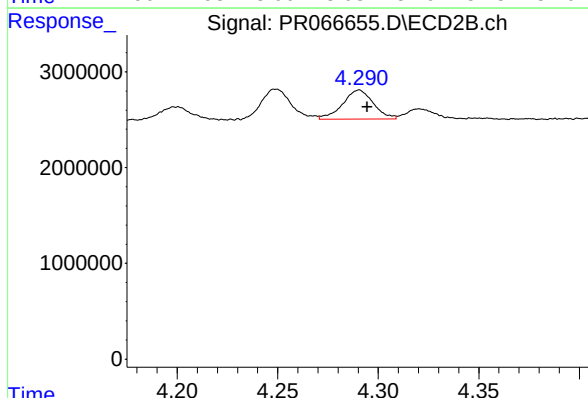


#19 AR-1242-4

R.T.: 4.290 min
Delta R.T.: -0.004 min
Response: 3256083
Conc: 34.11 ng/ml

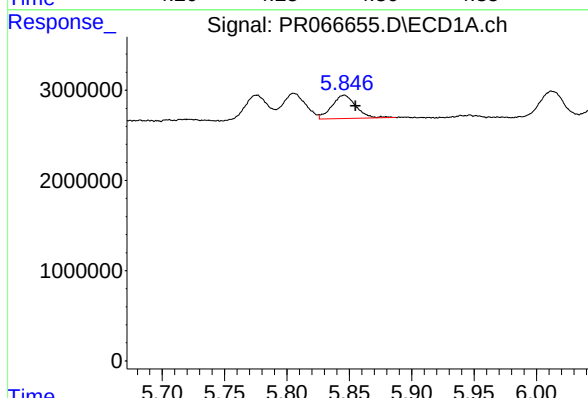


#20 AR-1242-5

R.T.: 5.846 min
Delta R.T.: -0.009 min
Response: 3452481
Conc: 38.39 ng/ml

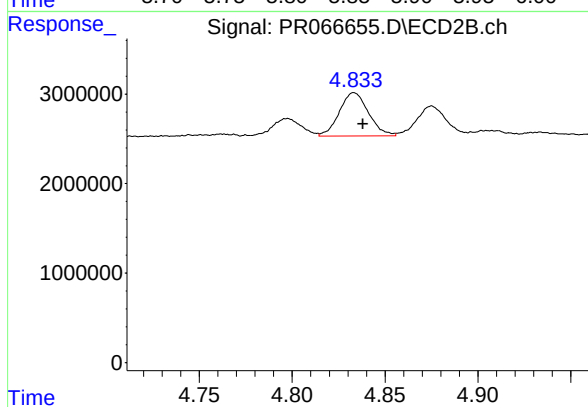

#20 AR-1242-5


R.T.: 4.833 min
Delta R.T.: -0.005 min
Response: 5285856
Conc: 43.04 ng/ml

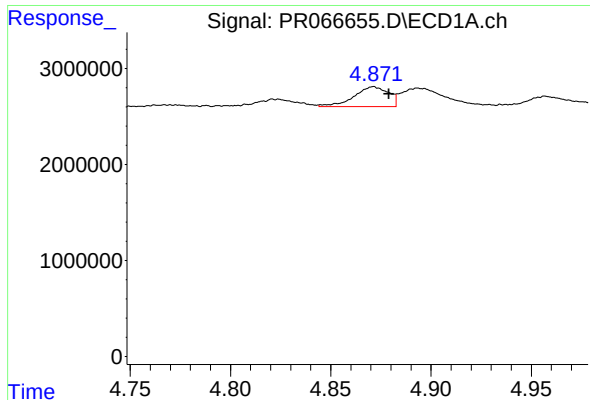

#21 AR-1248-1


R.T.: 4.871 min
Delta R.T.: -0.008 min
Response: 2470929
Conc: 28.55 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

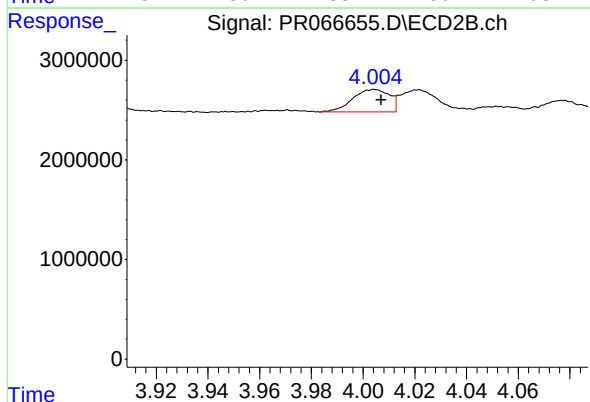


#21 AR-1248-1

R.T.: 4.004 min
Delta R.T.: -0.003 min
Response: 2213648
Conc: 23.81 ng/ml

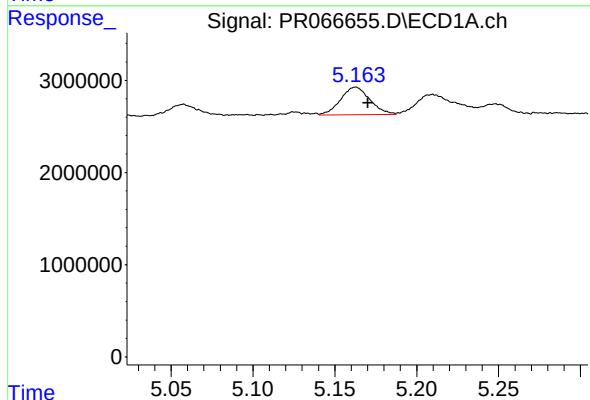


#22 AR-1248-2

R.T.: 5.163 min
Delta R.T.: -0.008 min
Response: 3754570
Conc: 28.21 ng/ml

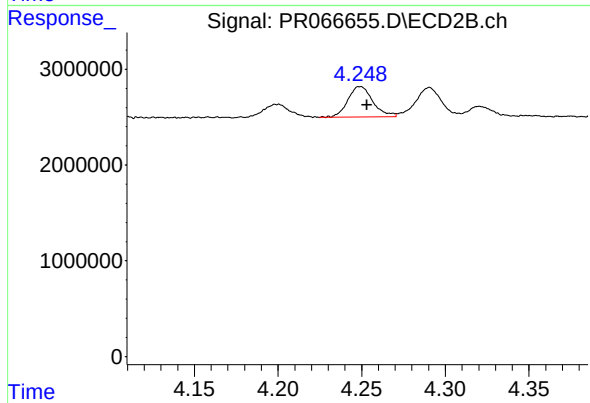

#22 AR-1248-2


R.T.: 4.249 min
Delta R.T.: -0.004 min
Response: 3307446
Conc: 24.44 ng/ml

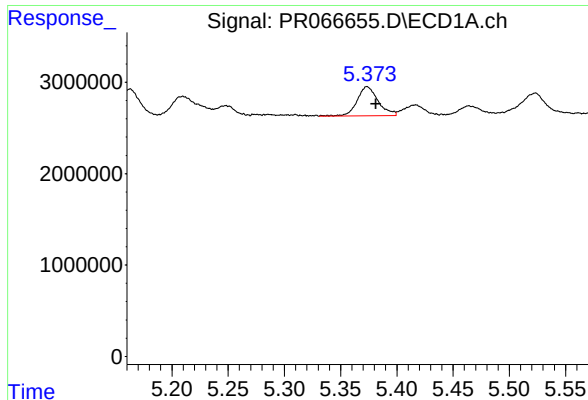

#23 AR-1248-3


R.T.: 5.374 min
Delta R.T.: -0.008 min
Response: 4145390
Conc: 27.62 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

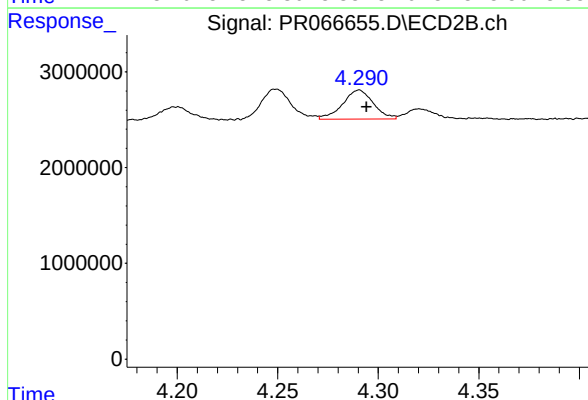


#23 AR-1248-3

R.T.: 4.290 min
Delta R.T.: -0.004 min
Response: 3256083
Conc: 23.65 ng/ml

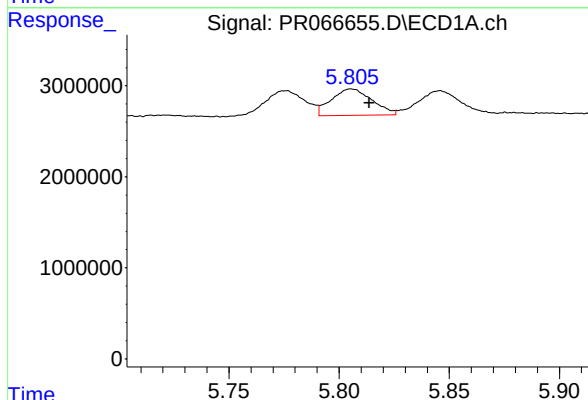


#24 AR-1248-4

R.T.: 5.806 min
Delta R.T.: -0.008 min
Response: 3727256
Conc: 26.16 ng/ml

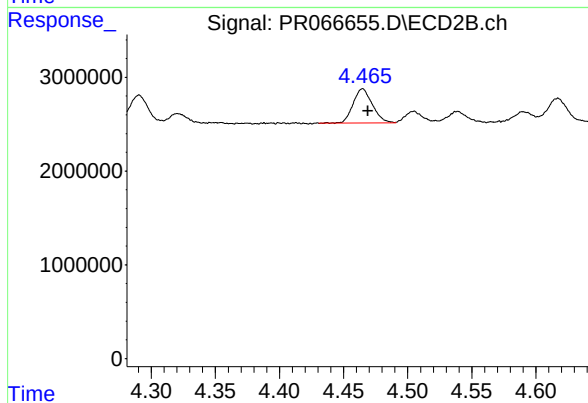

#24 AR-1248-4


R.T.: 4.465 min
Delta R.T.: -0.004 min
Response: 3814822
Conc: 23.08 ng/ml

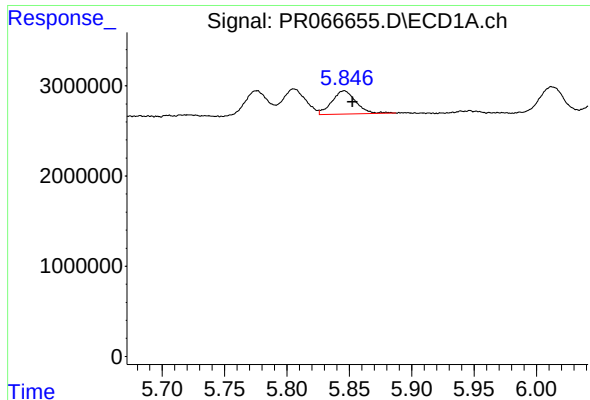

#25 AR-1248-5


R.T.: 5.846 min
Delta R.T.: -0.007 min
Response: 3452481
Conc: 24.11 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

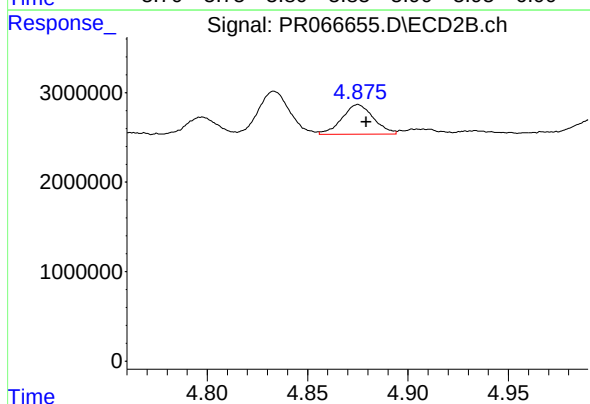


#25 AR-1248-5

R.T.: 4.875 min
Delta R.T.: -0.004 min
Response: 3642784
Conc: 22.57 ng/ml

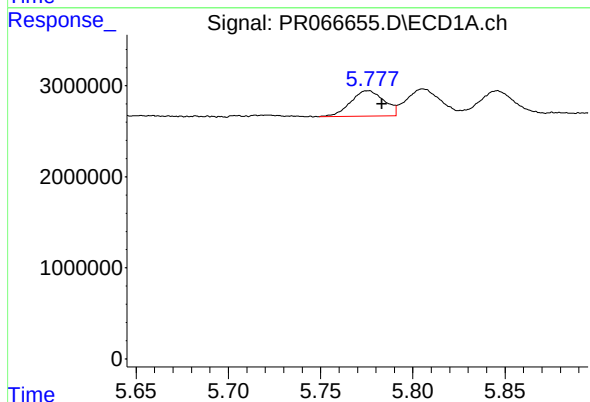


#26 AR-1254-1

R.T.: 5.776 min
Delta R.T.: -0.008 min
Response: 3511873
Conc: 21.13 ng/ml

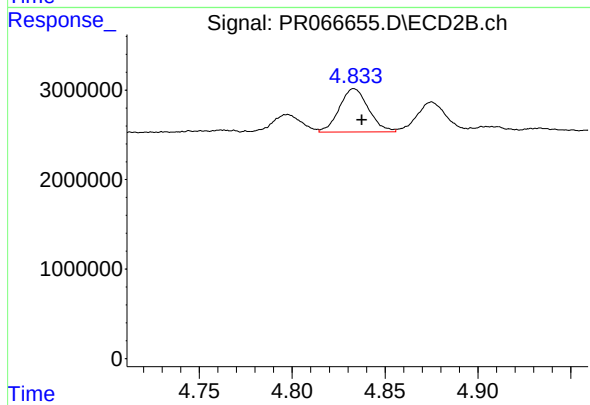

#26 AR-1254-1


R.T.: 4.833 min
Delta R.T.: -0.004 min
Response: 5285856
Conc: 21.51 ng/ml

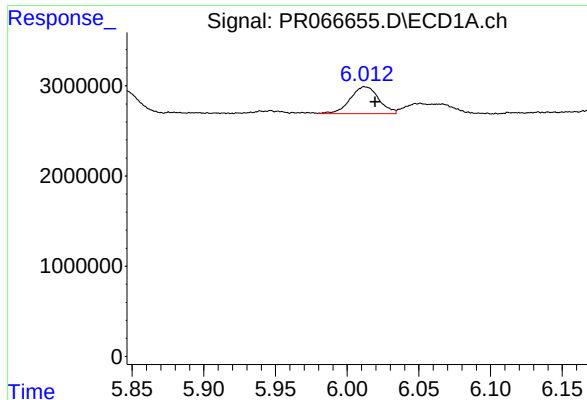

#27 AR-1254-2


R.T.: 6.013 min
Delta R.T.: -0.007 min
Response: 4123720
Conc: 16.83 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

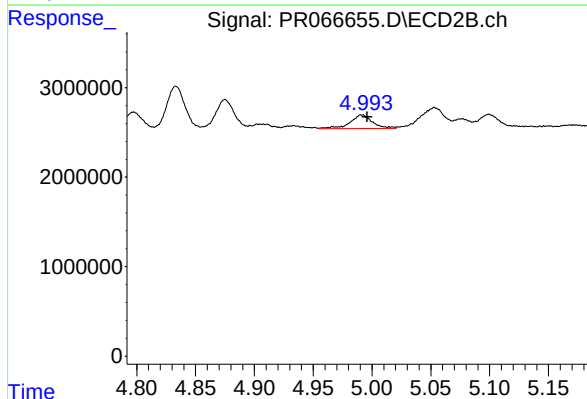


#27 AR-1254-2

R.T.: 4.991 min
Delta R.T.: -0.005 min
Response: 2039126
Conc: 9.31 ng/ml

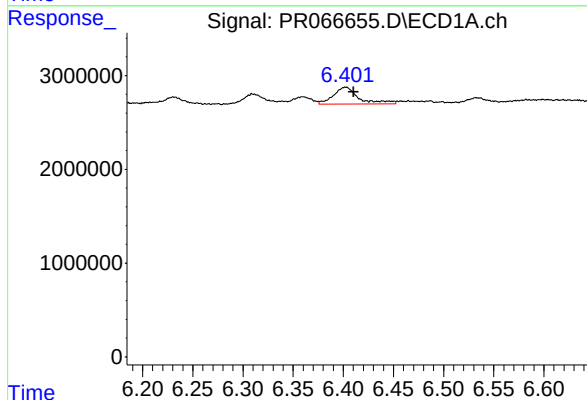


#28 AR-1254-3

R.T.: 6.402 min
Delta R.T.: -0.008 min
Response: 3179685
Conc: 12.86 ng/ml

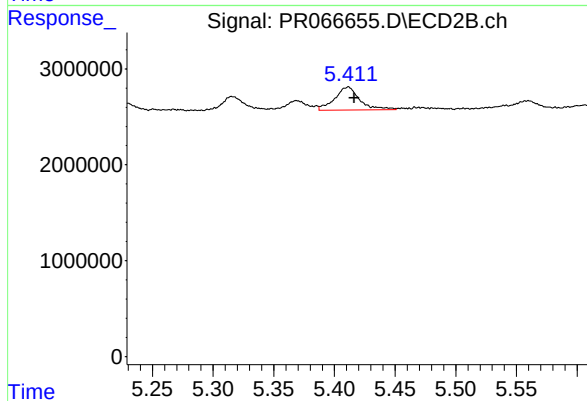

#28 AR-1254-3


R.T.: 5.411 min
Delta R.T.: -0.005 min
Response: 3428841
Conc: 9.98 ng/ml

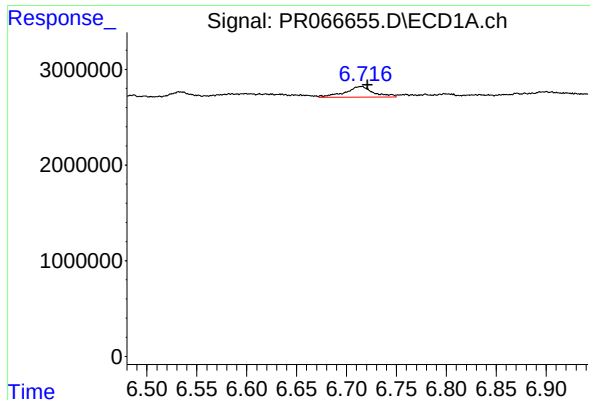

#29 AR-1254-4


R.T.: 6.715 min
Delta R.T.: -0.006 min
Response: 2143602
Conc: 13.50 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

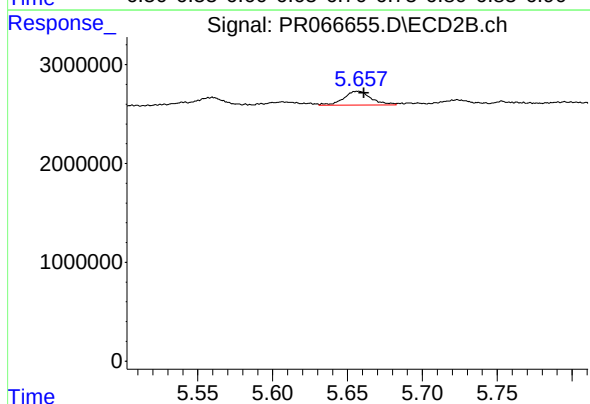


#29 AR-1254-4

R.T.: 5.657 min
Delta R.T.: -0.004 min
Response: 1776366
Conc: 8.32 ng/ml

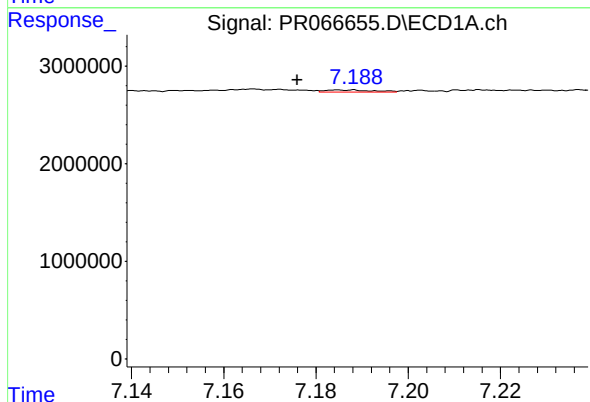


#30 AR-1254-5

R.T.: 7.186 min
Delta R.T.: 0.010 min
Response: 168453
Conc: 0.95 ng/ml

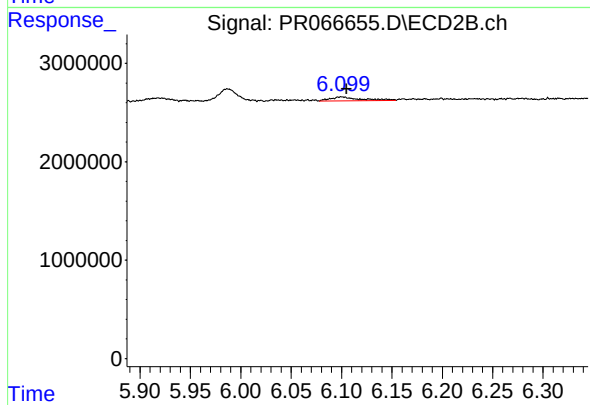

#30 AR-1254-5


R.T.: 6.100 min
Delta R.T.: -0.005 min
Response: 811362
Conc: 2.52 ng/ml

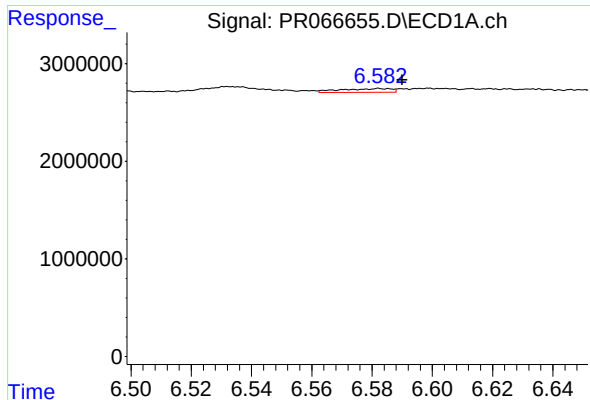

#31 AR-1260-1


R.T.: 6.583 min
Delta R.T.: -0.007 min
Response: 459095
Conc: 2.21 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

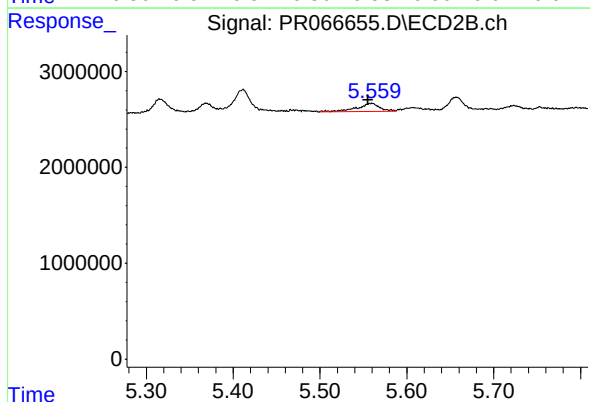


#31 AR-1260-1

R.T.: 5.559 min
Delta R.T.: 0.004 min
Response: 1588801
Conc: 6.27 ng/ml

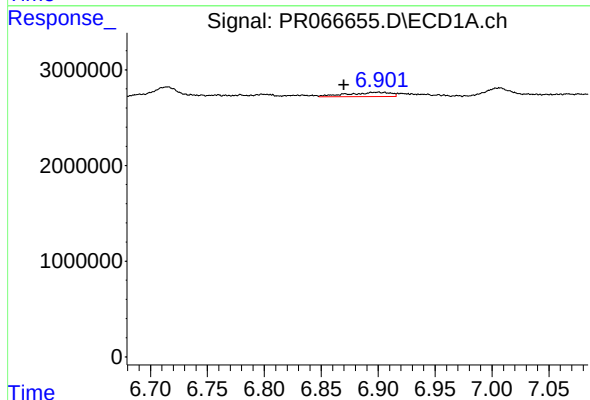


#32 AR-1260-2

R.T.: 6.900 min
Delta R.T.: 0.030 min
Response: 1212116
Conc: 5.46 ng/ml

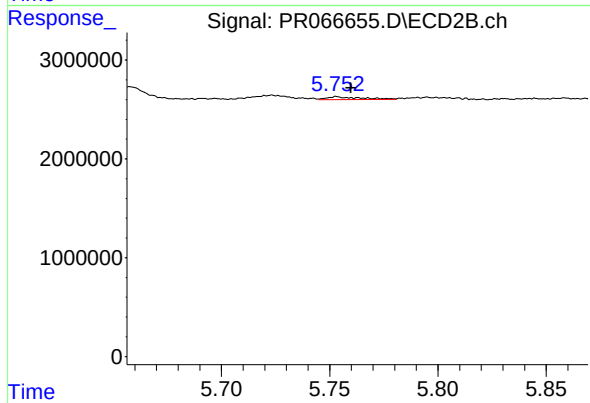

#32 AR-1260-2


R.T.: 5.753 min
Delta R.T.: -0.007 min
Response: 318936
Conc: 1.05 ng/ml

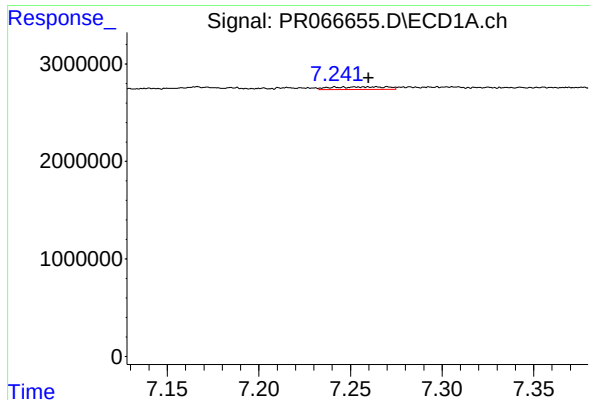

#33 AR-1260-3


R.T.: 7.253 min
Delta R.T.: -0.007 min
Response: 576598
Conc: 3.44 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

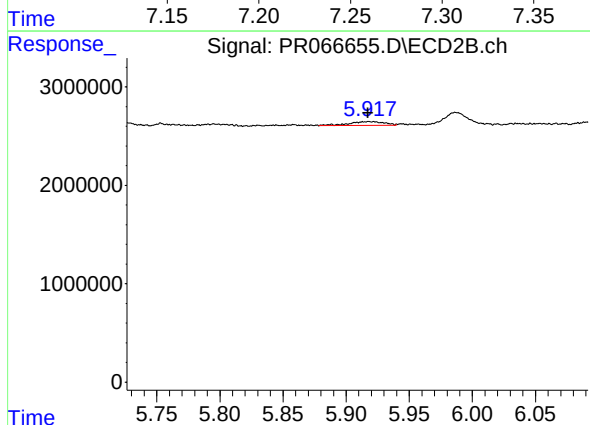


#33 AR-1260-3

R.T.: 5.918 min
Delta R.T.: 0.000 min
Response: 746419
Conc: 2.56 ng/ml

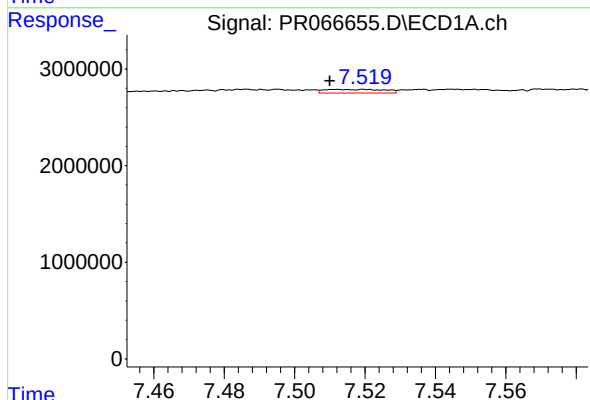


#34 AR-1260-4

R.T.: 7.520 min
Delta R.T.: 0.010 min
Response: 434034
Conc: 2.44 ng/ml

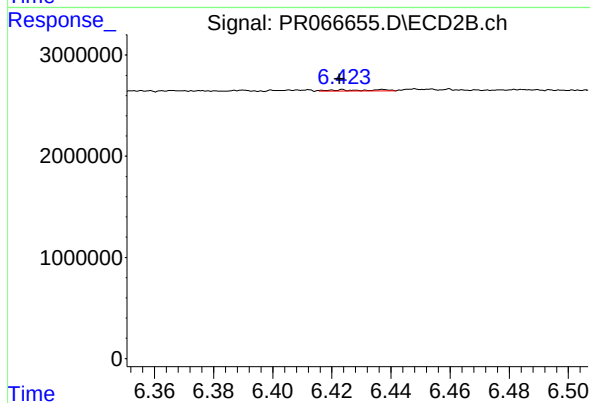

#34 AR-1260-4


R.T.: 6.424 min
Delta R.T.: 0.000 min
Response: 119701
Conc: 0.48 ng/ml

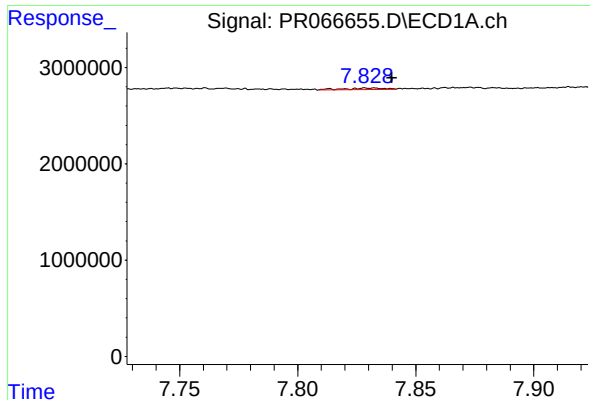

#35 AR-1260-5


R.T.: 7.831 min
Delta R.T.: -0.009 min
Response: 187196
Conc: 0.64 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

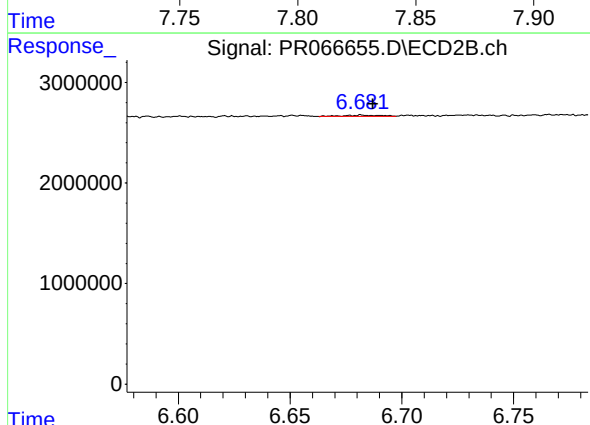


#35 AR-1260-5

R.T.: 6.682 min
Delta R.T.: -0.005 min
Response: 130031
Conc: 0.23 ng/ml

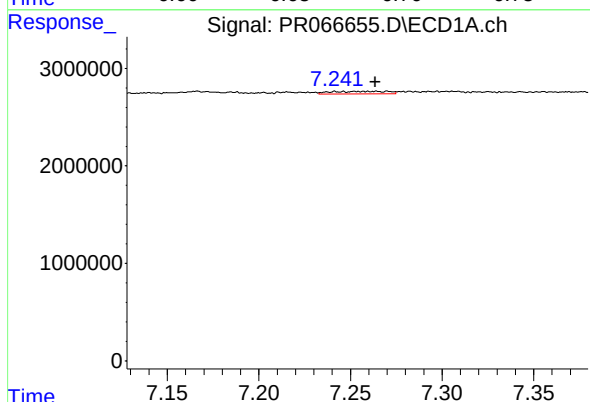


#36 AR-1262-1

R.T.: 7.253 min
Delta R.T.: -0.011 min
Response: 576598
Conc: 2.53 ng/ml

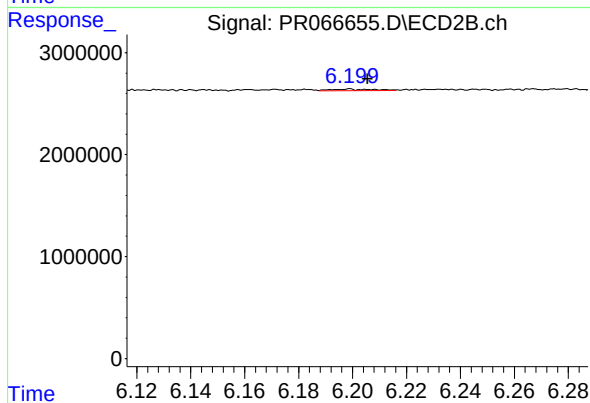

#36 AR-1262-1


R.T.: 6.199 min
Delta R.T.: -0.007 min
Response: 191850
Conc: 1.33 ng/ml

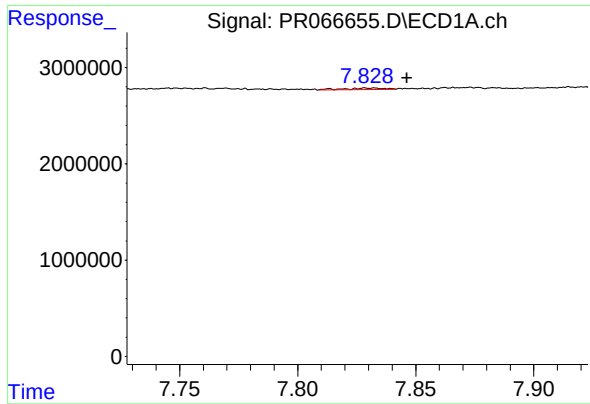

#37 AR-1262-2


R.T.: 7.831 min
Delta R.T.: -0.015 min
Response: 187196
Conc: 0.59 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

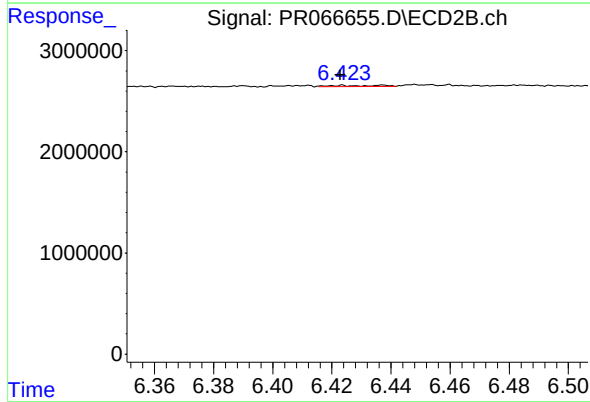


#37 AR-1262-2

R.T.: 6.424 min
Delta R.T.: 0.000 min
Response: 119701
Conc: 0.39 ng/ml

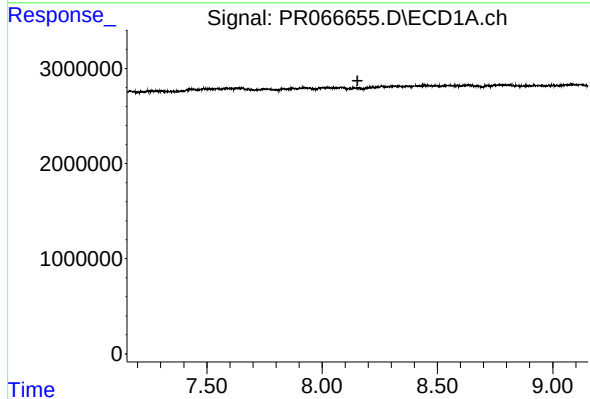


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.154 min
Response: 0
Conc: N.D.

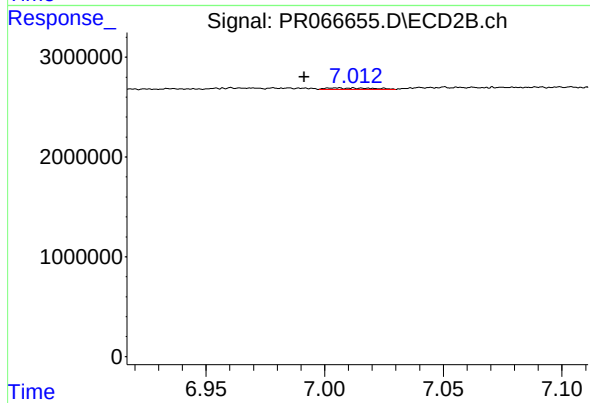

#38 AR-1262-3


R.T.: 7.012 min
Delta R.T.: 0.021 min
Response: 198632
Conc: 0.82 ng/ml

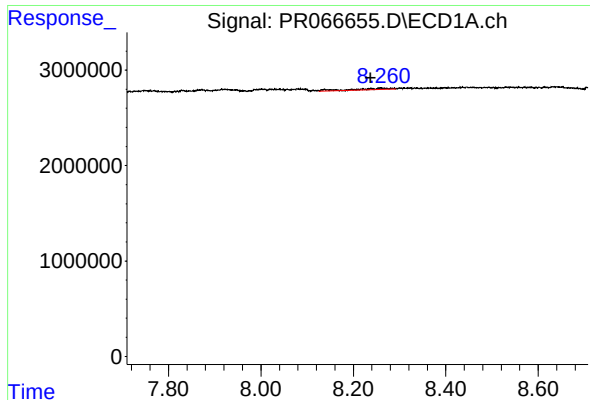

#39 AR-1262-4


R.T.: 8.258 min
Delta R.T.: 0.021 min
Response: 714061
Conc: 6.54 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

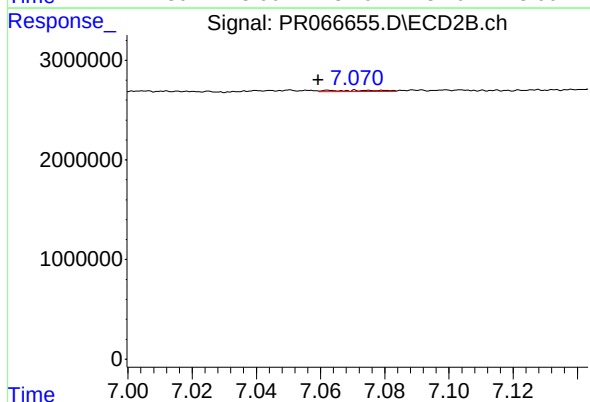


#39 AR-1262-4

R.T.: 7.063 min
Delta R.T.: 0.003 min
Response: 144404
Conc: 0.33 ng/ml

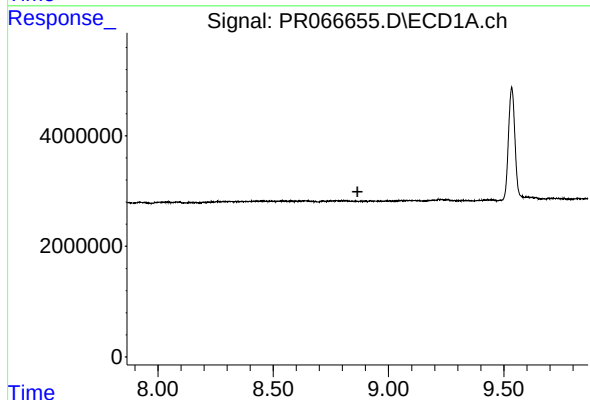


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 8.865 min
Response: 0
Conc: N.D.

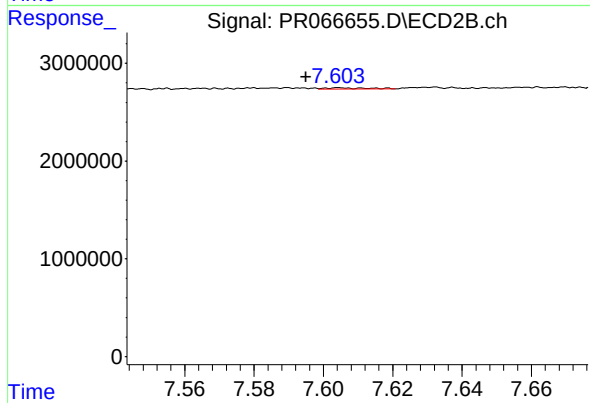

#40 AR-1262-5


R.T.: 7.605 min
Delta R.T.: 0.010 min
Response: 105221
Conc: 0.49 ng/ml

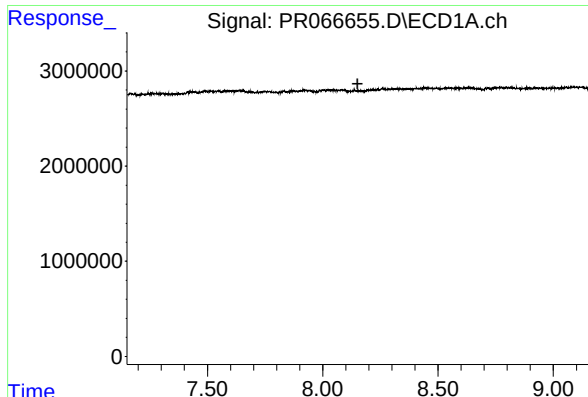

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

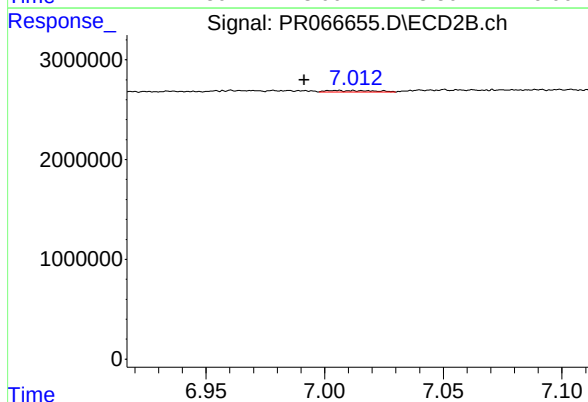


#41 AR-1268-1

R.T.: 7.012 min
Delta R.T.: 0.021 min
Response: 198632
Conc: 0.27 ng/ml

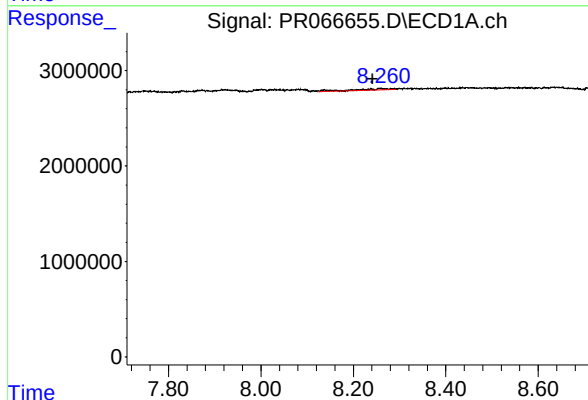


#42 AR-1268-2

R.T.: 8.258 min
Delta R.T.: 0.016 min
Response: 714061
Conc: 2.08 ng/ml

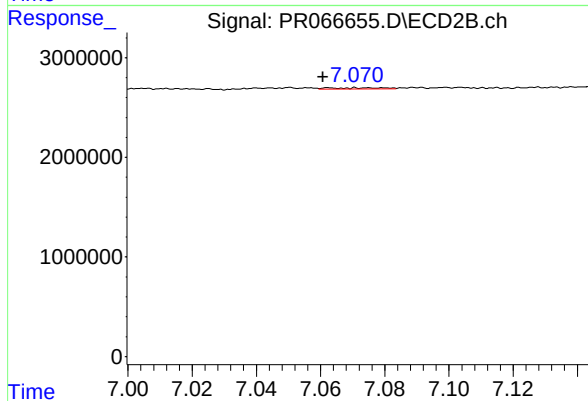

#42 AR-1268-2


R.T.: 7.063 min
Delta R.T.: 0.002 min
Response: 144404
Conc: 0.22 ng/ml

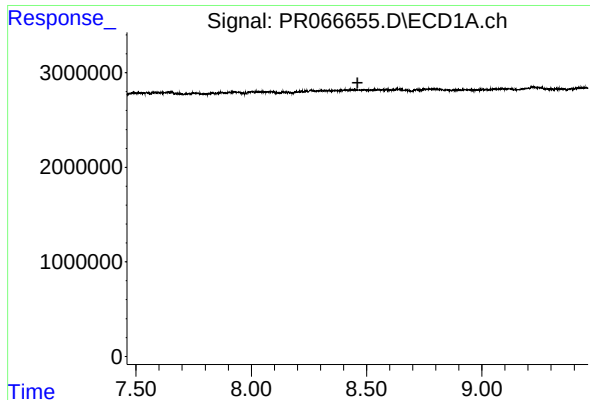

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

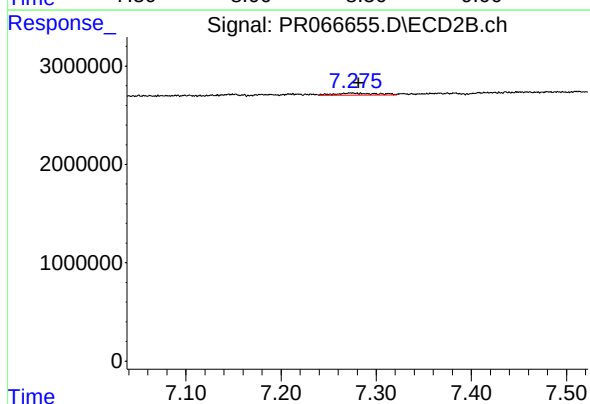


#43 AR-1268-3

R.T.: 7.275 min
Delta R.T.: -0.007 min
Response: 699621
Conc: 1.23 ng/ml

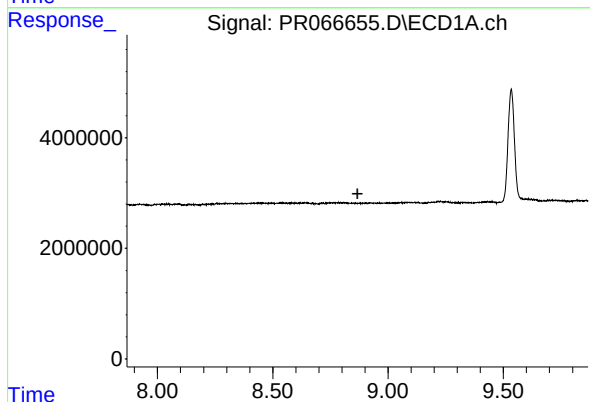


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 8.867 min
Response: 0
Conc: N.D.

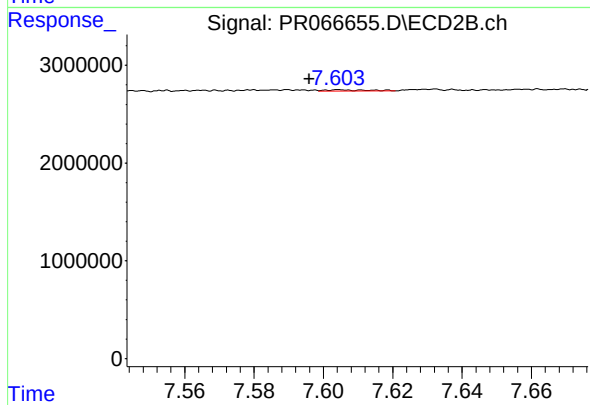

#44 AR-1268-4


R.T.: 7.603 min
Delta R.T.: 0.009 min
Response: 105221
Conc: 0.43 ng/ml

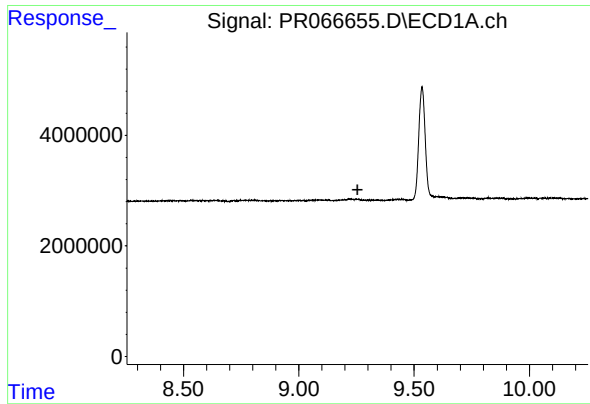

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.254 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

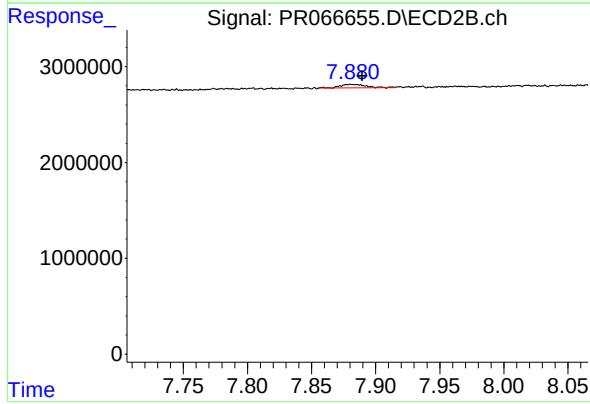

#45 AR-1268-5

R.T.: 7.881 min
Delta R.T.: -0.009 min
Response: 555274
Conc: 0.34 ng/ml