

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR050924\
 Data File : PR066656.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2024 06:31
 Operator : AJ\MA
 Sample : P2403-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT2-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 06:58:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 26 07:26:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.652	2.893	91228586	72717561	17.405	16.269
2) SA Decachlor...	9.533	8.121	39049933	73537308	16.675	15.667
Target Compounds						
3) L1 AR-1016-1	4.890	4.004	220353	131282	1.542	0.869 #
4) L1 AR-1016-2	4.902	4.023	202008	164688	0.924	0.768
6) L1 AR-1016-4	5.098f	4.249	154164	2275518	1.342	23.587 #
7) L1 AR-1016-5	5.374	4.464	1408133	1468772	12.365	11.880
8) L2 AR-1221-1	3.860f	0.000	1232447	0	20.411	N.D. #
9) L2 AR-1221-2	3.962	3.194	1337481	1116152	30.267	26.883
10) L2 AR-1221-3	4.059f	3.285	32647	182355	0.251	1.509 #
11) L3 AR-1232-1	4.059	3.285	32647	182355	0.307	1.817 #
12) L3 AR-1232-2	4.575f	4.023	439827	164688	7.167	1.655 #
13) L3 AR-1232-3	4.902	0.000	202008	0	1.977	N.D. #
14) L3 AR-1232-4	5.098f	4.289	154164	622653	2.863	12.838 #
15) L3 AR-1232-5	5.163	4.464	2830594	1468772	70.353	27.531 #
16) L4 AR-1242-1	4.890	4.004	220353	131282	1.851	1.049 #
17) L4 AR-1242-2	4.902	4.023	202008	164688	1.124	0.929
19) L4 AR-1242-4	5.098f	4.289	154164	622653	1.629	6.522 #
20) L4 AR-1242-5	5.849	4.832	1162604	5594426	12.929	45.548 #
21) L5 AR-1248-1	4.890	4.004	220353	131282	2.546	1.412 #
22) L5 AR-1248-2	5.163	4.249	2830594	2275518	21.266	16.816
23) L5 AR-1248-3	5.374	4.289	1408133	622653	9.381	4.522 #
24) L5 AR-1248-4	5.805	4.464	1916913	1468772	13.454	8.885 #
25) L5 AR-1248-5	5.849	4.874	1162604	831773	8.118	5.154 #
26) L6 AR-1254-1	5.777	4.832	5131763	5594426	30.881	22.765 #
27) L6 AR-1254-2	6.012	4.991	7018921	5297680	28.653	24.191
28) L6 AR-1254-3	6.403	5.411	6331745	8863957	25.615	25.787
29) L6 AR-1254-4	6.713	5.656	4435881	4486802	27.941	21.014
30) L6 AR-1254-5	7.167	6.098	4238414	6676050	23.782	20.747
31) L7 AR-1260-1	6.582	5.552	3081335	3989356	14.828	15.741
32) L7 AR-1260-2	6.863	5.755	2830480	3439551	12.759	11.294
33) L7 AR-1260-3	7.236f	5.909	785528	3595184	4.684	12.349 #
34) L7 AR-1260-4	0.000	6.418	0	454223	N.D.	1.819 #
35) L7 AR-1260-5	7.832	6.680	694818	821556	2.379	1.463 #
36) L8 AR-1262-1	7.236f	6.194	785528	305141	3.443	2.112 #
37) L8 AR-1262-2	7.832	6.418	694818	454223	2.188	1.476 #
38) L8 AR-1262-3	8.142	6.981	410299	96192	1.938	0.397 #
39) L8 AR-1262-4	8.246	7.049	74440	704477	0.681	1.603 #
40) L8 AR-1262-5	0.000	7.601	0	97603	N.D.	0.452 #
41) L9 AR-1268-1	8.142	6.981	410299	96192	1.052	0.133 #
42) L9 AR-1268-2	8.246	7.049	74440	704477	0.217	1.098 #
43) L9 AR-1268-3	8.433f	7.277	73317	354760	0.239	0.625 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR050924\
Data File : PR066656.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2024 06:31
Operator : AJ\MA
Sample : P2403-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 71 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 06:58:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 26 07:26:35 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	0.000	7.601	0	97603	N.D.	0.400 #
45) L9	AR-1268-5	0.000	7.880	0	454962	N.D.	0.281 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR050924\
Data File : PR066656.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2024 06:31
Operator : AJ\MA
Sample : P2403-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 71 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 06:58:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 26 07:26:35 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

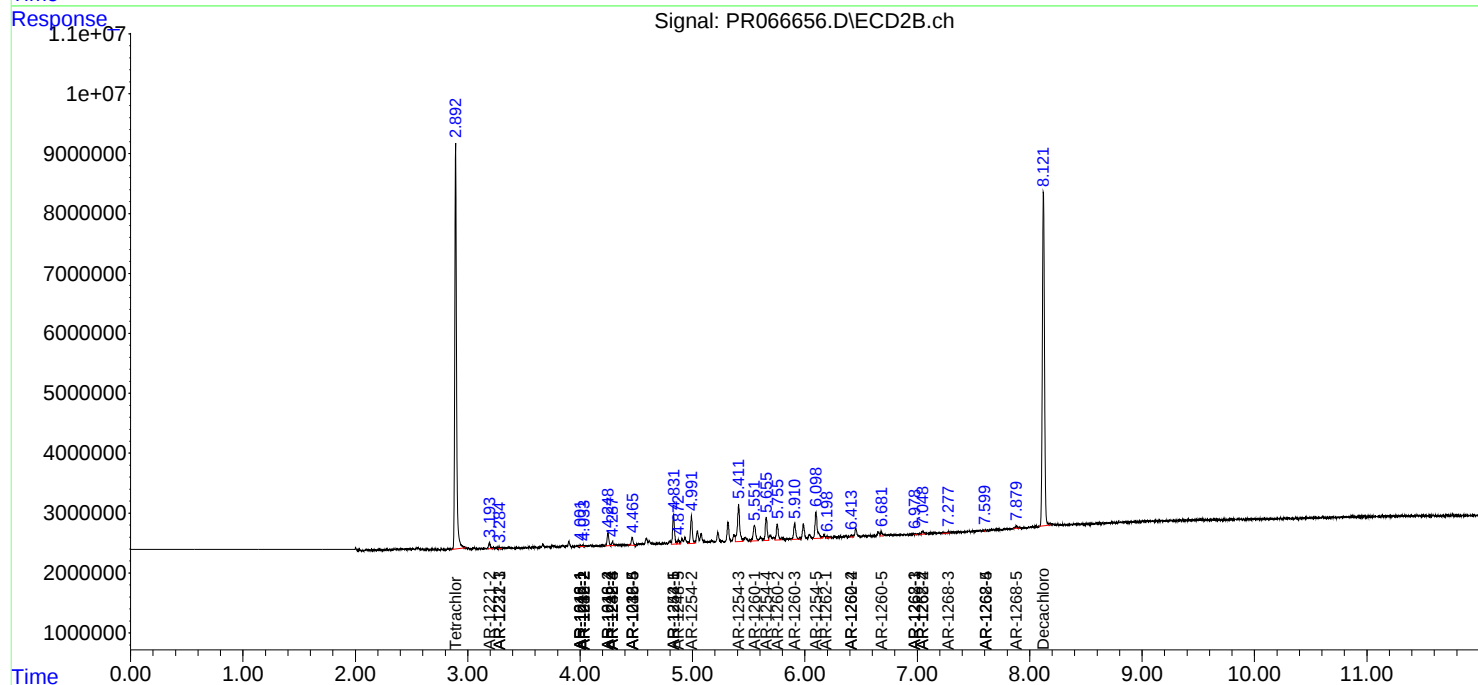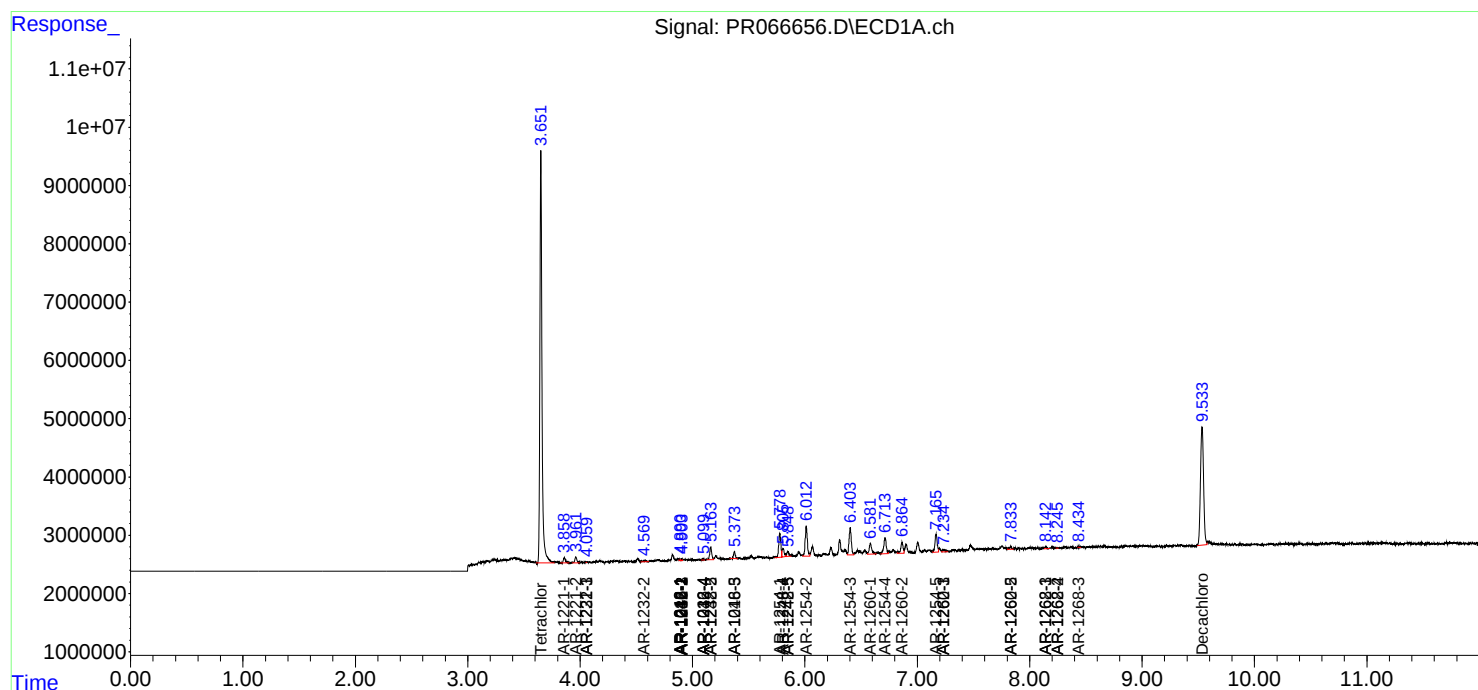


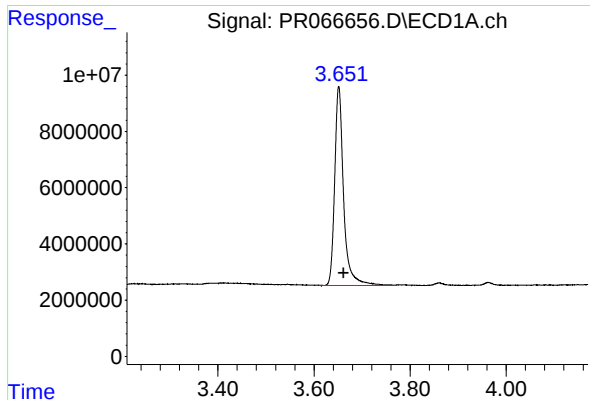

#1 Tetrachloro-m-xylene


R.T.: 3.652 min
Delta R.T.: -0.010 min
Response: 91228586
Conc: 17.41 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

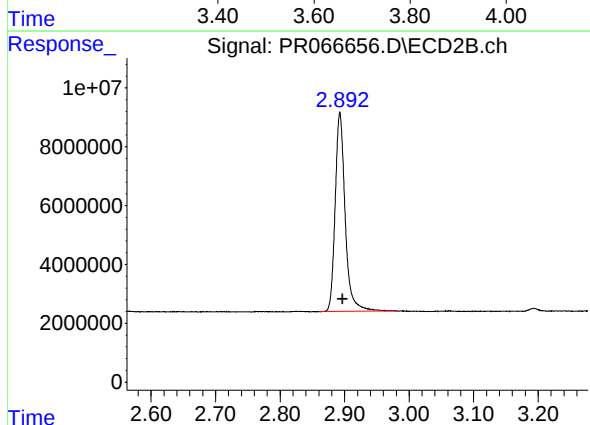


#1 Tetrachloro-m-xylene

R.T.: 2.893 min
Delta R.T.: -0.004 min
Response: 72717561
Conc: 16.27 ng/ml

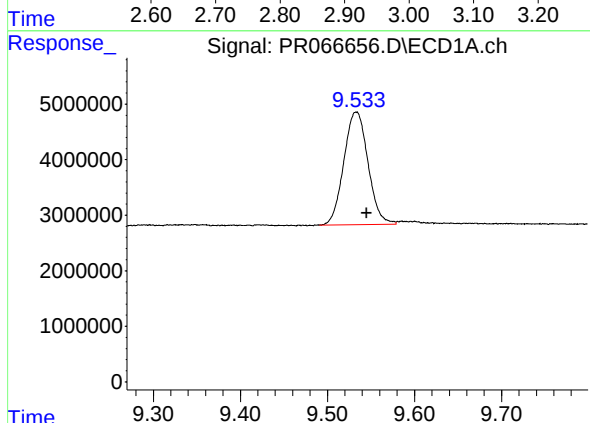


#2 Decachlorobiphenyl

R.T.: 9.533 min
Delta R.T.: -0.012 min
Response: 39049933
Conc: 16.68 ng/ml

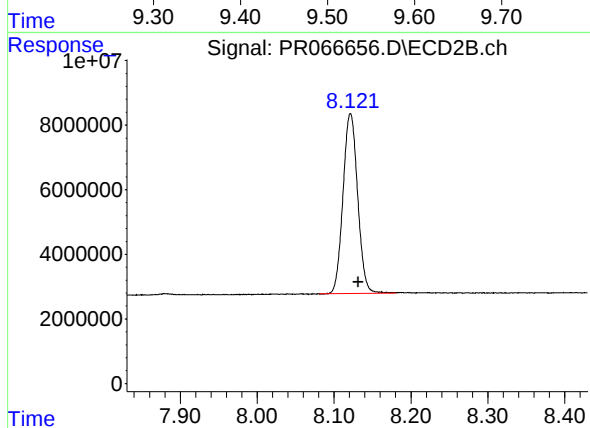

#2 Decachlorobiphenyl


R.T.: 8.121 min
Delta R.T.: -0.010 min
Response: 73537308
Conc: 15.67 ng/ml

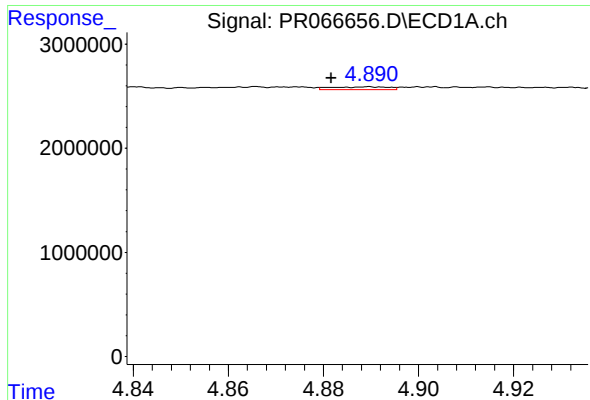

#3 AR-1016-1


R.T.: 4.890 min
Delta R.T.: 0.009 min
Response: 220353
Conc: 1.54 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

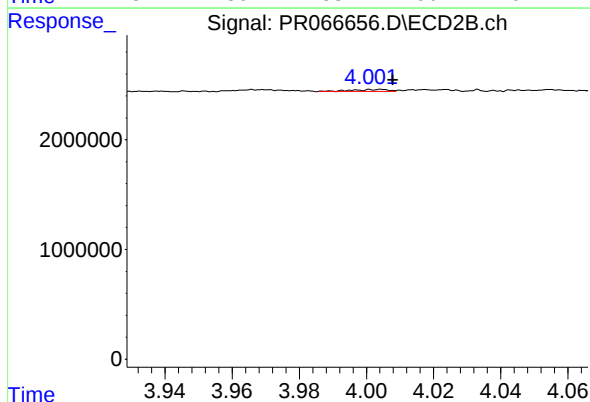


#3 AR-1016-1

R.T.: 4.004 min
Delta R.T.: -0.004 min
Response: 131282
Conc: 0.87 ng/ml

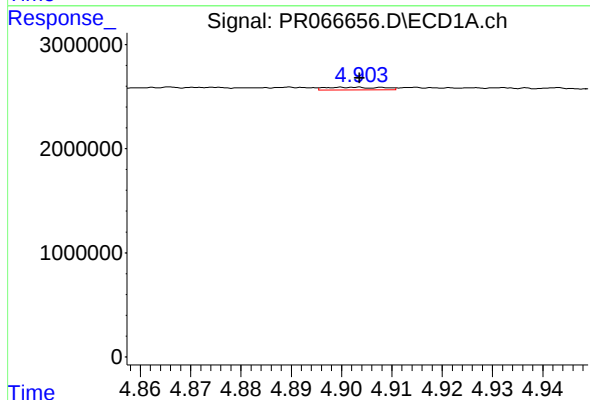


#4 AR-1016-2

R.T.: 4.902 min
Delta R.T.: -0.002 min
Response: 202008
Conc: 0.92 ng/ml

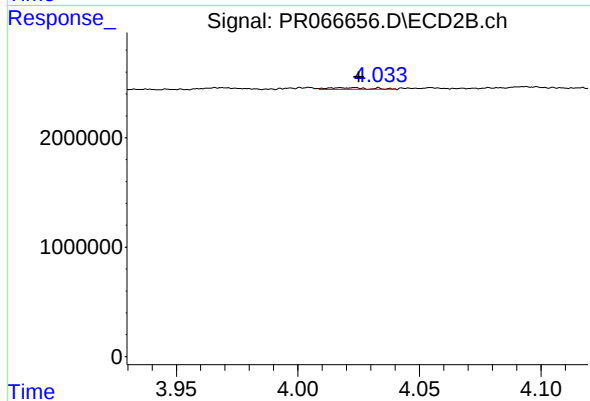

#4 AR-1016-2


R.T.: 4.023 min
Delta R.T.: -0.002 min
Response: 164688
Conc: 0.77 ng/ml

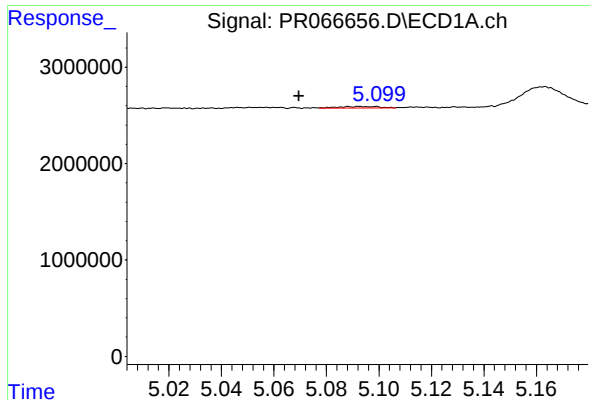

#6 AR-1016-4


R.T.: 5.098 min
Delta R.T.: 0.029 min
Response: 154164
Conc: 1.34 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

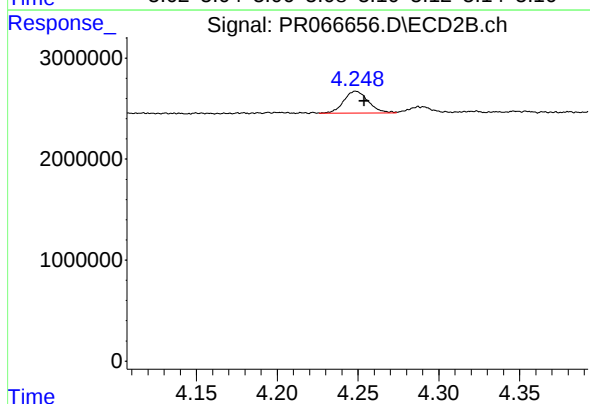


#6 AR-1016-4

R.T.: 4.249 min
Delta R.T.: -0.005 min
Response: 2275518
Conc: 23.59 ng/ml

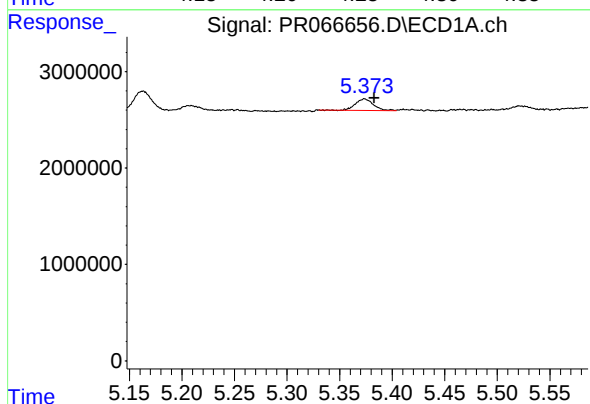


#7 AR-1016-5

R.T.: 5.374 min
Delta R.T.: -0.010 min
Response: 1408133
Conc: 12.37 ng/ml

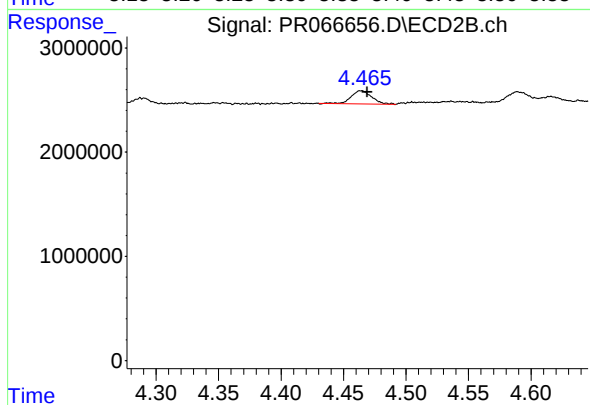

#7 AR-1016-5


R.T.: 4.464 min
Delta R.T.: -0.005 min
Response: 1468772
Conc: 11.88 ng/ml

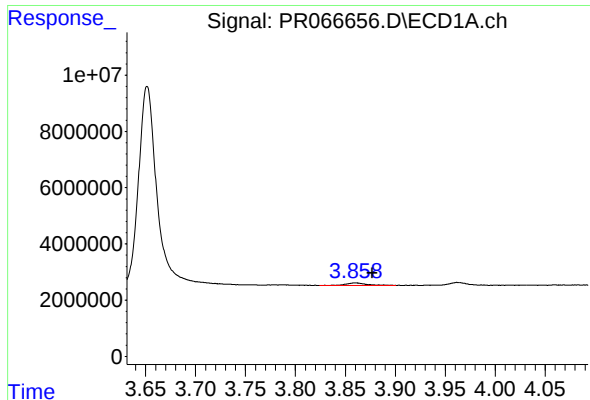

#8 AR-1221-1


R.T.: 3.860 min
Delta R.T.: -0.017 min
Response: 1232447
Conc: 20.41 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

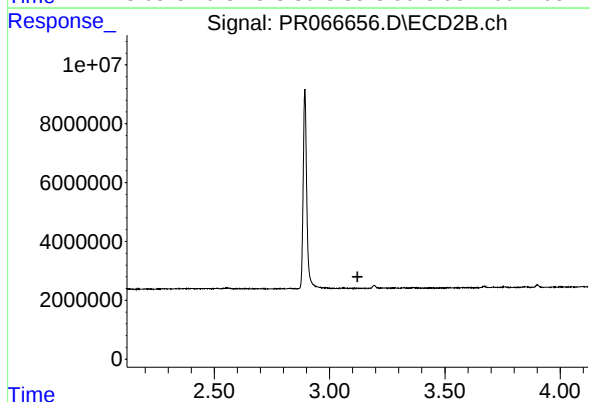


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T.: 3.121 min
Response: 0
Conc: N.D.

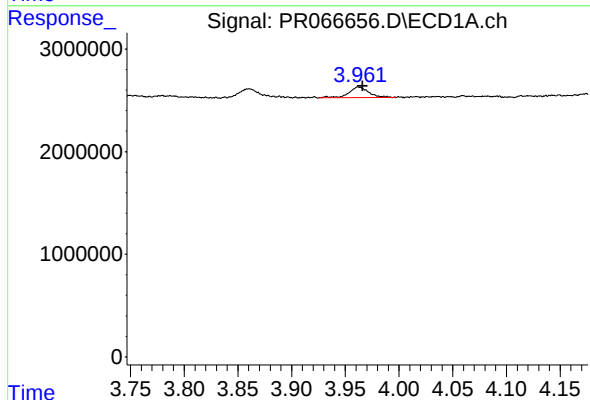


#9 AR-1221-2

R.T.: 3.962 min
Delta R.T.: -0.004 min
Response: 1337481
Conc: 30.27 ng/ml

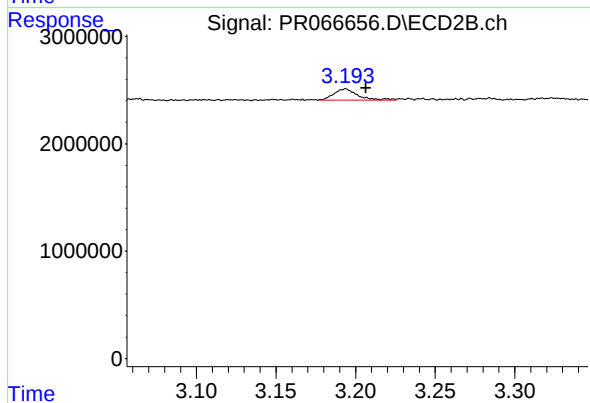

#9 AR-1221-2


R.T.: 3.194 min
Delta R.T.: -0.013 min
Response: 1116152
Conc: 26.88 ng/ml

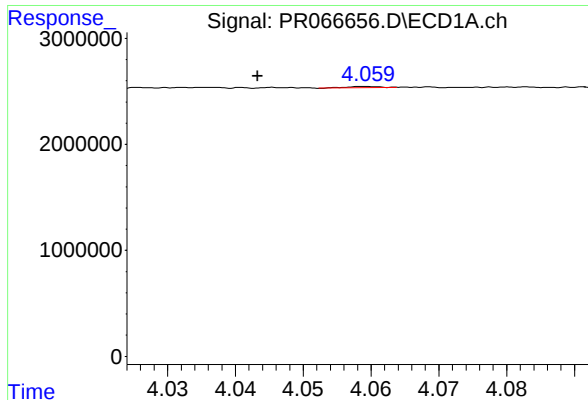

#10 AR-1221-3


R.T.: 4.059 min
Delta R.T.: 0.016 min
Response: 32647
Conc: 0.25 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

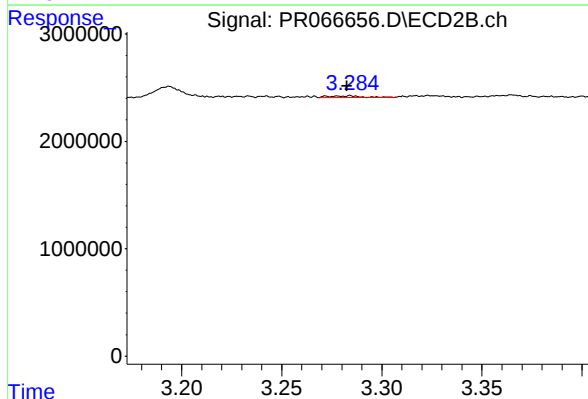


#10 AR-1221-3

R.T.: 3.285 min
Delta R.T.: 0.002 min
Response: 182355
Conc: 1.51 ng/ml

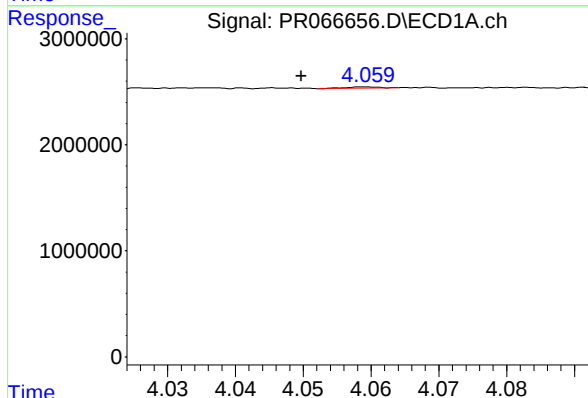


#11 AR-1232-1

R.T.: 4.059 min
Delta R.T.: 0.010 min
Response: 32647
Conc: 0.31 ng/ml

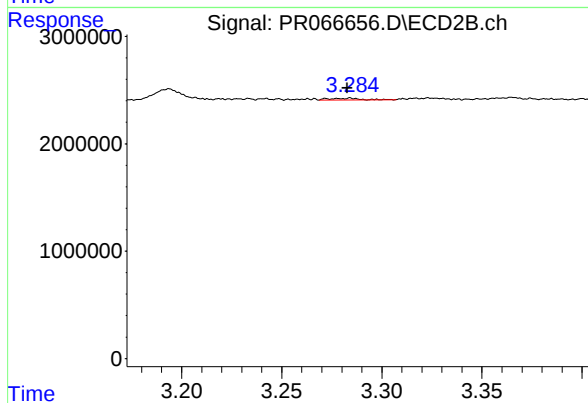

#11 AR-1232-1


R.T.: 3.285 min
Delta R.T.: 0.002 min
Response: 182355
Conc: 1.82 ng/ml

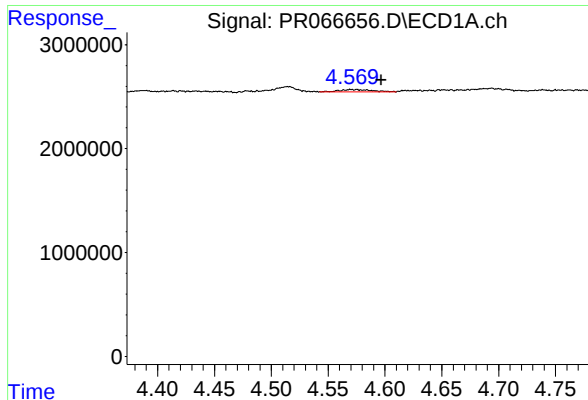

#12 AR-1232-2


R.T.: 4.575 min
Delta R.T.: -0.021 min
Response: 439827
Conc: 7.17 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

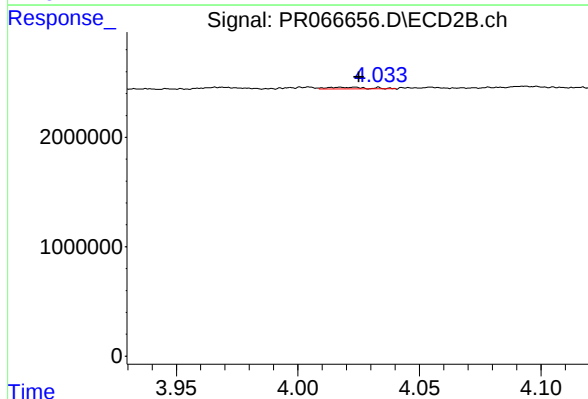


#12 AR-1232-2

R.T.: 4.023 min
Delta R.T.: -0.002 min
Response: 164688
Conc: 1.65 ng/ml

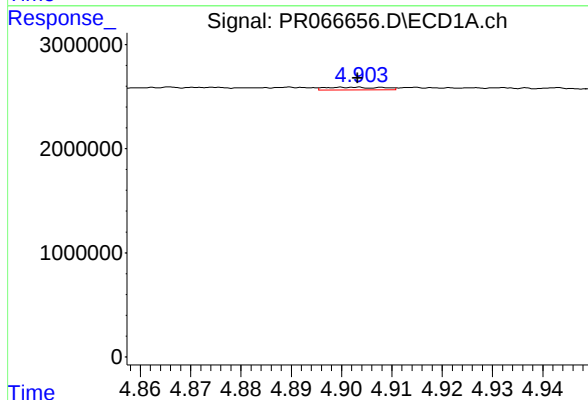


#13 AR-1232-3

R.T.: 4.902 min
Delta R.T.: -0.001 min
Response: 202008
Conc: 1.98 ng/ml

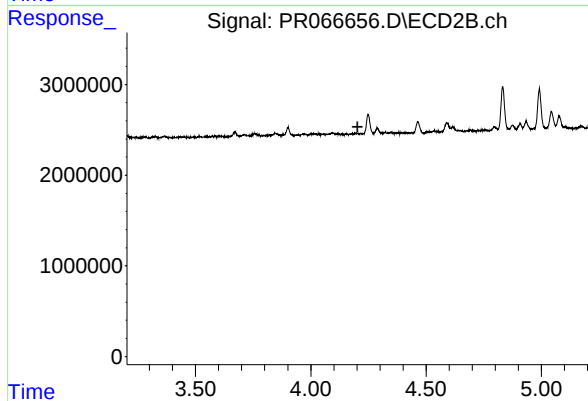

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T. : 4.203 min
Response: 0
Conc: N.D.

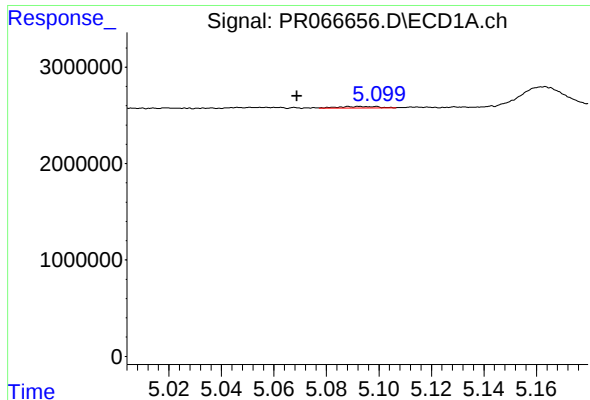

#14 AR-1232-4


R.T.: 5.098 min
Delta R.T.: 0.029 min
Response: 154164
Conc: 2.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

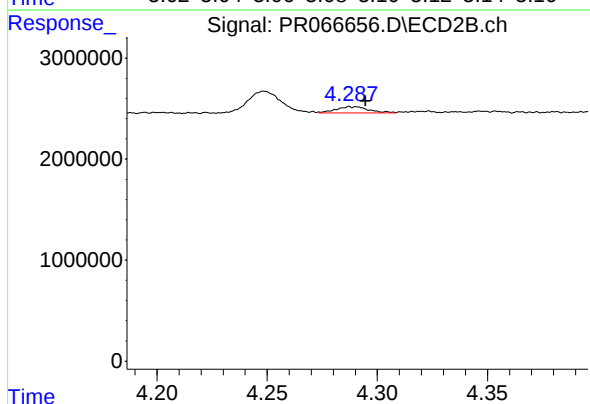


#14 AR-1232-4

R.T.: 4.289 min
Delta R.T.: -0.006 min
Response: 622653
Conc: 12.84 ng/ml

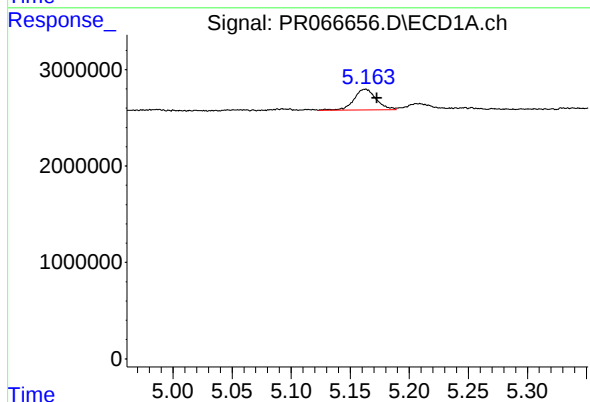


#15 AR-1232-5

R.T.: 5.163 min
Delta R.T.: -0.010 min
Response: 2830594
Conc: 70.35 ng/ml

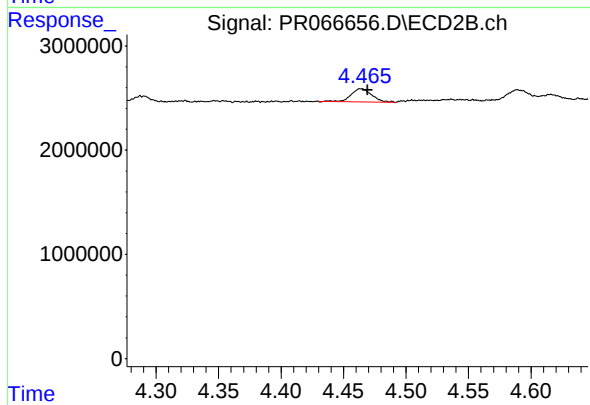

#15 AR-1232-5


R.T.: 4.464 min
Delta R.T.: -0.005 min
Response: 1468772
Conc: 27.53 ng/ml

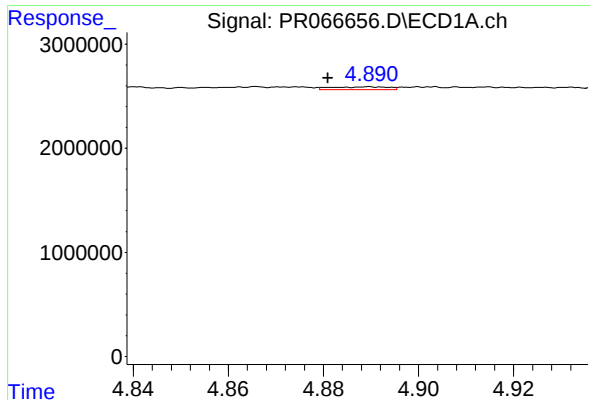

#16 AR-1242-1


R.T.: 4.890 min
Delta R.T.: 0.009 min
Response: 220353
Conc: 1.85 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

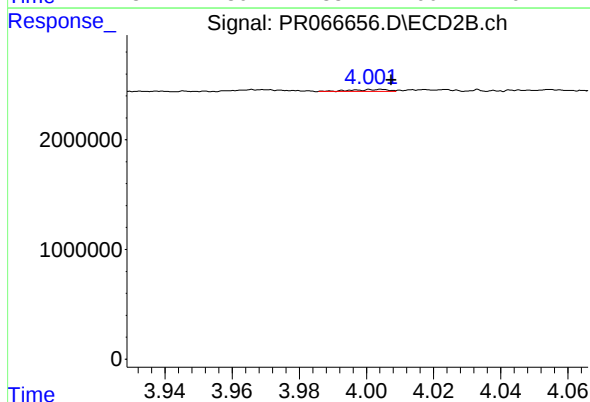


#16 AR-1242-1

R.T.: 4.004 min
Delta R.T.: -0.003 min
Response: 131282
Conc: 1.05 ng/ml

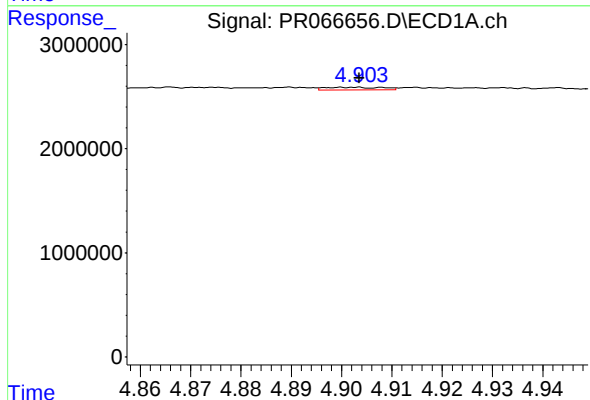


#17 AR-1242-2

R.T.: 4.902 min
Delta R.T.: -0.002 min
Response: 202008
Conc: 1.12 ng/ml

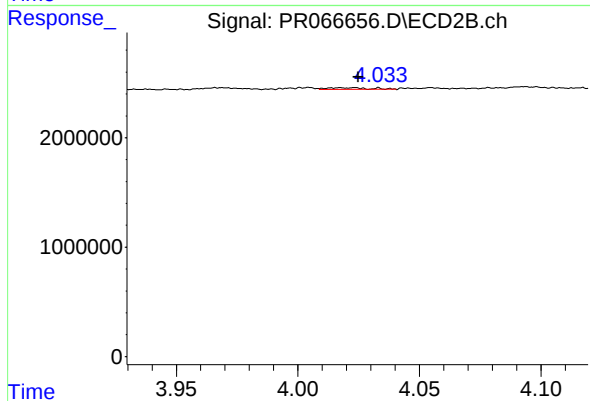

#17 AR-1242-2


R.T.: 4.023 min
Delta R.T.: -0.002 min
Response: 164688
Conc: 0.93 ng/ml

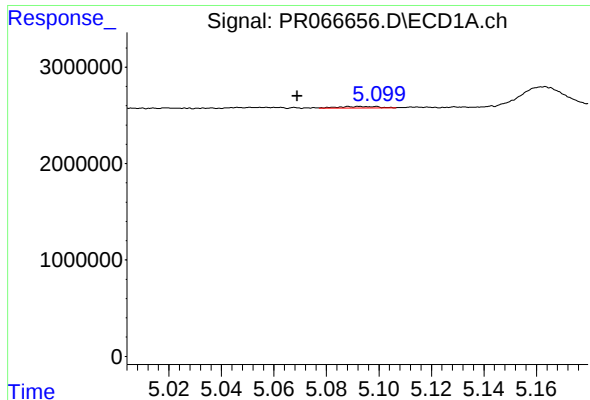

#19 AR-1242-4


R.T.: 5.098 min
Delta R.T.: 0.029 min
Response: 154164
Conc: 1.63 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

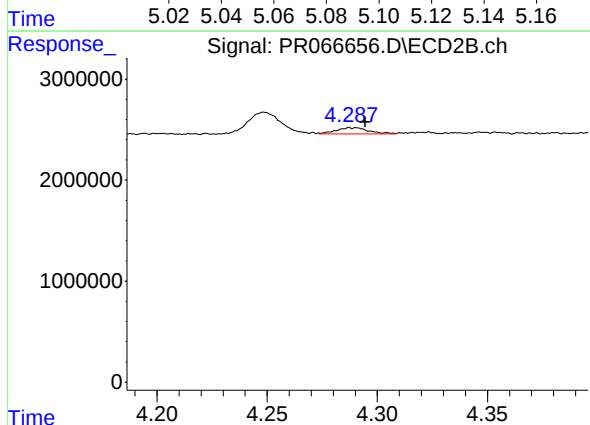


#19 AR-1242-4

R.T.: 4.289 min
Delta R.T.: -0.006 min
Response: 622653
Conc: 6.52 ng/ml

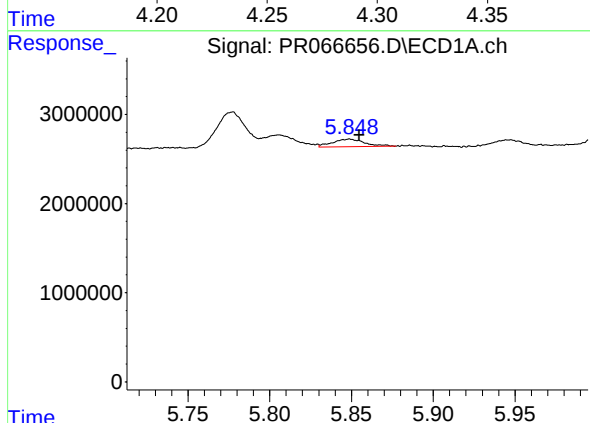


#20 AR-1242-5

R.T.: 5.849 min
Delta R.T.: -0.006 min
Response: 1162604
Conc: 12.93 ng/ml

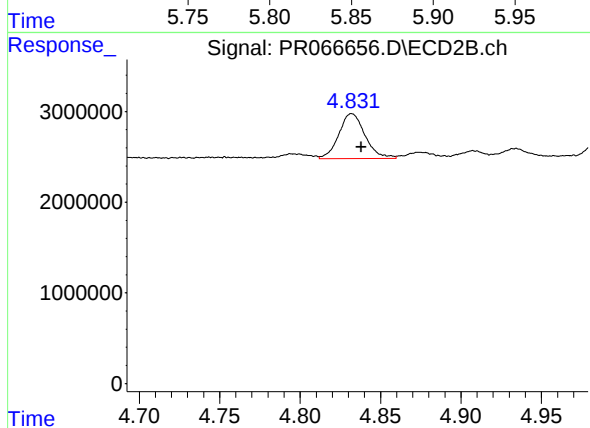

#20 AR-1242-5


R.T.: 4.832 min
Delta R.T.: -0.006 min
Response: 5594426
Conc: 45.55 ng/ml

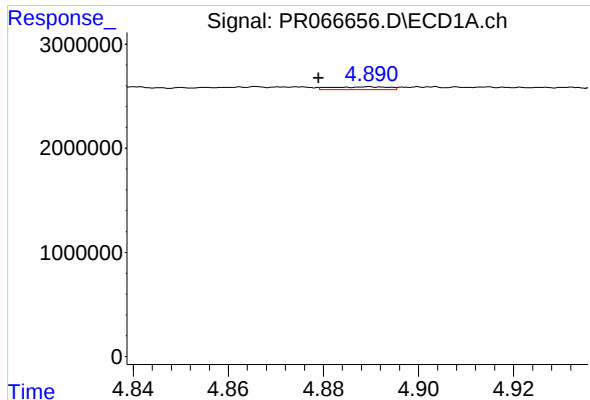

#21 AR-1248-1


R.T.: 4.890 min
Delta R.T.: 0.011 min
Response: 220353
Conc: 2.55 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

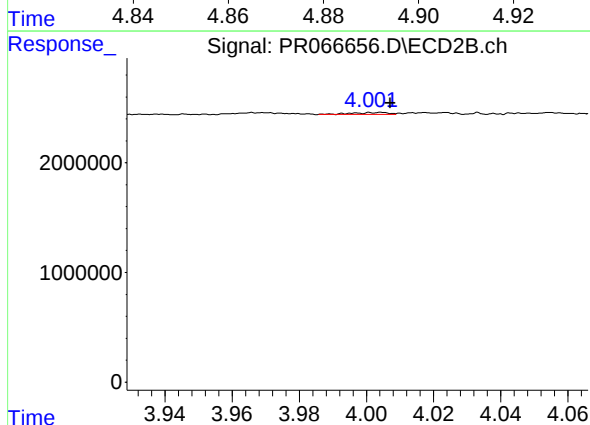


#21 AR-1248-1

R.T.: 4.004 min
Delta R.T.: -0.003 min
Response: 131282
Conc: 1.41 ng/ml

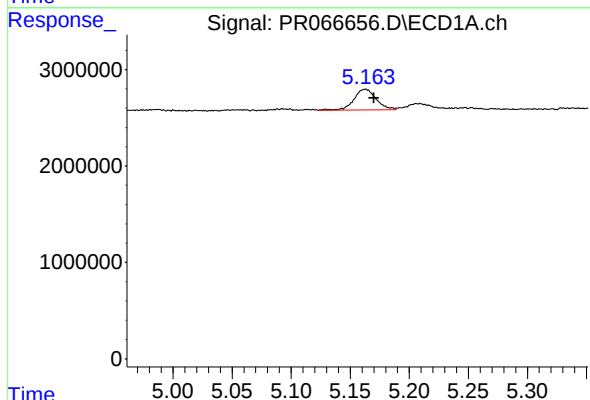


#22 AR-1248-2

R.T.: 5.163 min
Delta R.T.: -0.007 min
Response: 2830594
Conc: 21.27 ng/ml

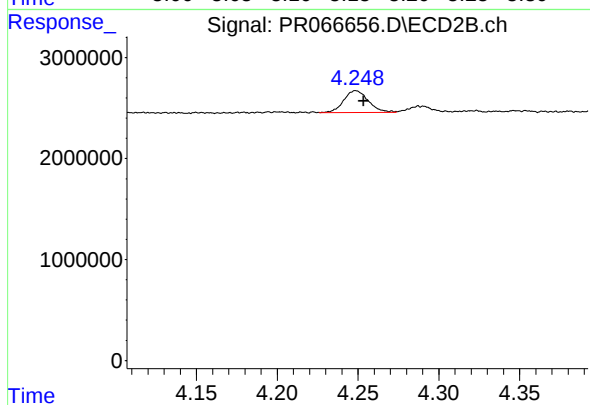

#22 AR-1248-2


R.T.: 4.249 min
Delta R.T.: -0.005 min
Response: 2275518
Conc: 16.82 ng/ml

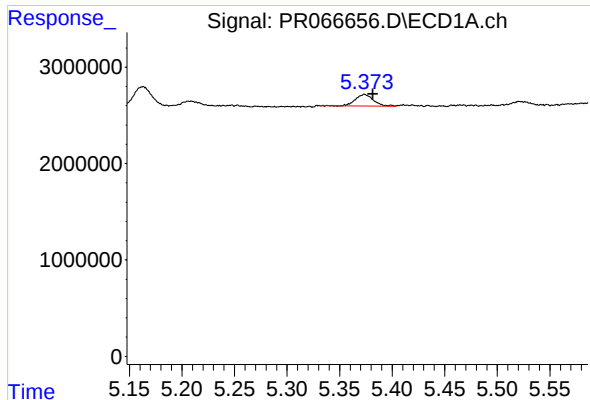

#23 AR-1248-3


R.T.: 5.374 min
Delta R.T.: -0.008 min
Response: 1408133
Conc: 9.38 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

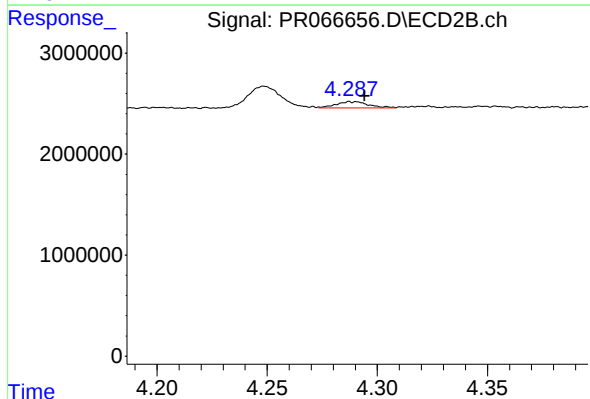


#23 AR-1248-3

R.T.: 4.289 min
Delta R.T.: -0.005 min
Response: 622653
Conc: 4.52 ng/ml

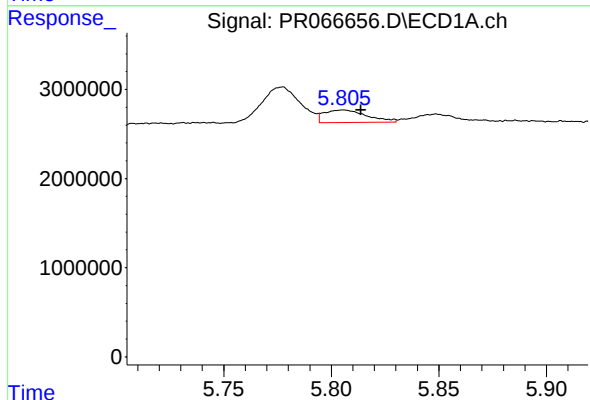


#24 AR-1248-4

R.T.: 5.805 min
Delta R.T.: -0.008 min
Response: 1916913
Conc: 13.45 ng/ml

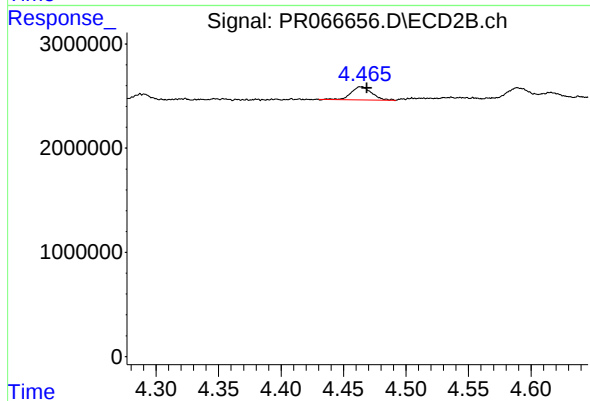

#24 AR-1248-4


R.T.: 4.464 min
Delta R.T.: -0.005 min
Response: 1468772
Conc: 8.89 ng/ml

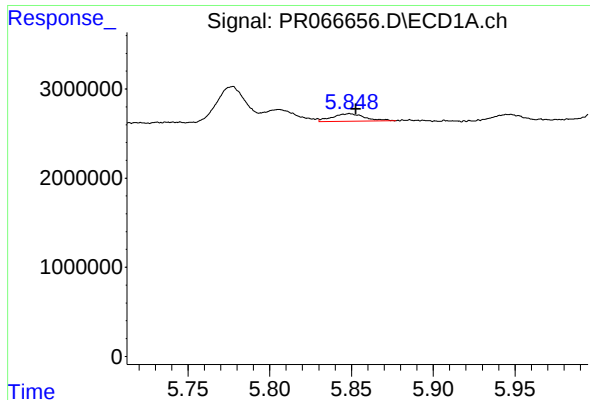

#25 AR-1248-5


R.T.: 5.849 min
Delta R.T.: -0.004 min
Response: 1162604
Conc: 8.12 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

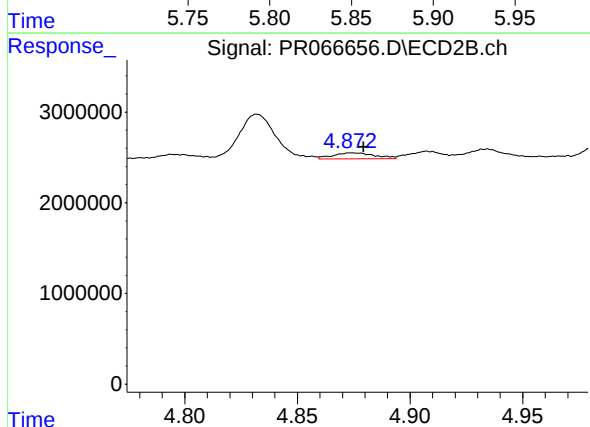


#25 AR-1248-5

R.T.: 4.874 min
Delta R.T.: -0.005 min
Response: 831773
Conc: 5.15 ng/ml

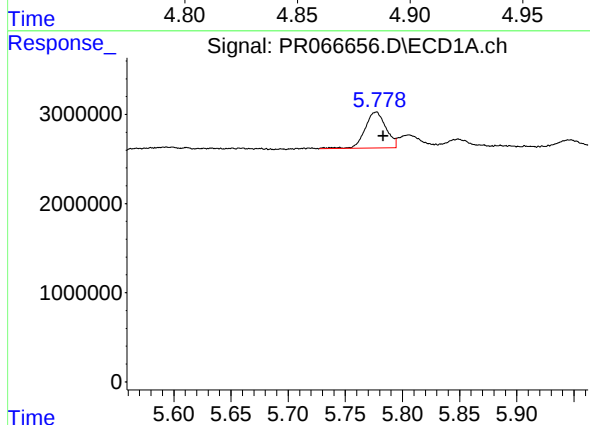


#26 AR-1254-1

R.T.: 5.777 min
Delta R.T.: -0.006 min
Response: 5131763
Conc: 30.88 ng/ml

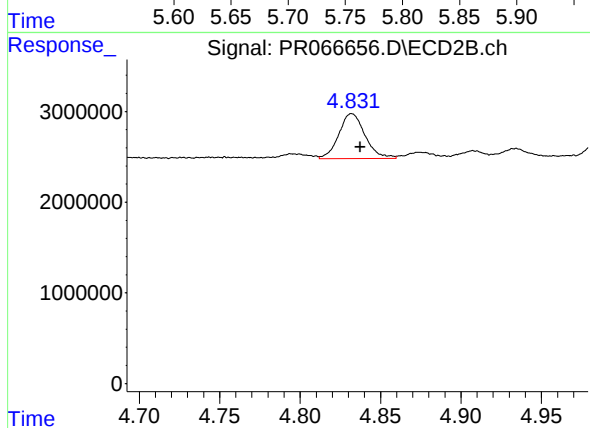

#26 AR-1254-1


R.T.: 4.832 min
Delta R.T.: -0.005 min
Response: 5594426
Conc: 22.77 ng/ml

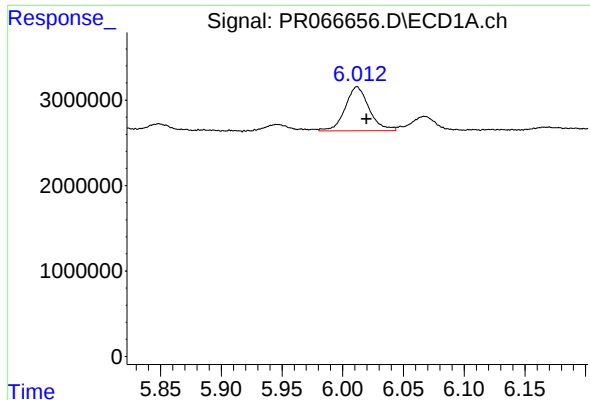

#27 AR-1254-2


R.T.: 6.012 min
Delta R.T.: -0.008 min
Response: 7018921
Conc: 28.65 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

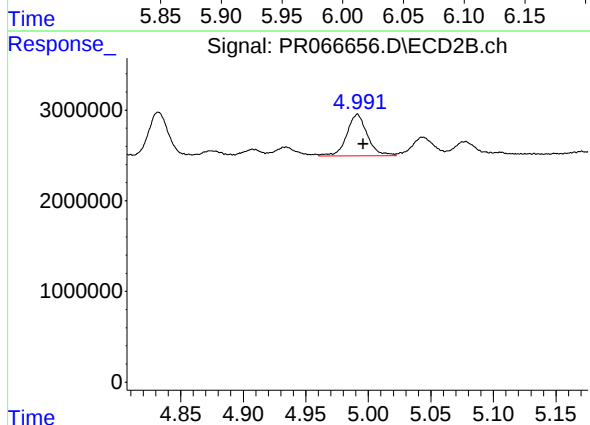


#27 AR-1254-2

R.T.: 4.991 min
Delta R.T.: -0.005 min
Response: 5297680
Conc: 24.19 ng/ml

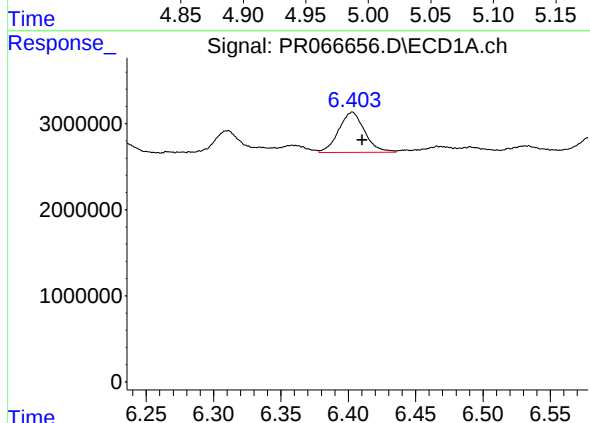


#28 AR-1254-3

R.T.: 6.403 min
Delta R.T.: -0.008 min
Response: 6331745
Conc: 25.62 ng/ml

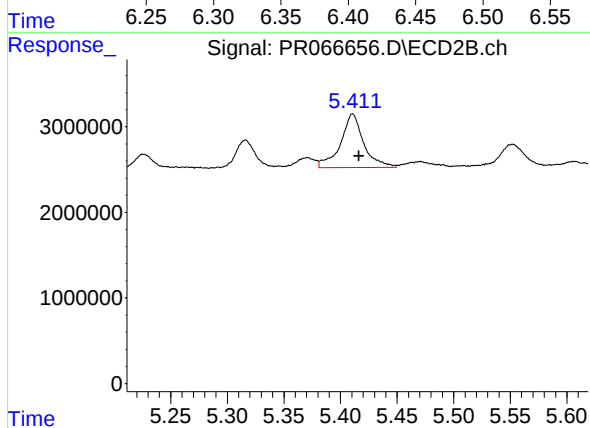

#28 AR-1254-3


R.T.: 5.411 min
Delta R.T.: -0.006 min
Response: 8863957
Conc: 25.79 ng/ml

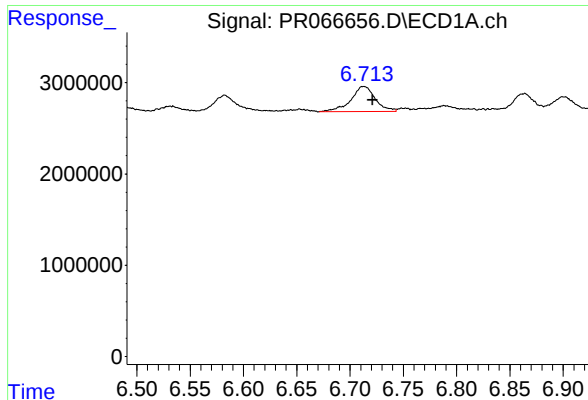

#29 AR-1254-4


R.T.: 6.713 min
Delta R.T.: -0.008 min
Response: 4435881
Conc: 27.94 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

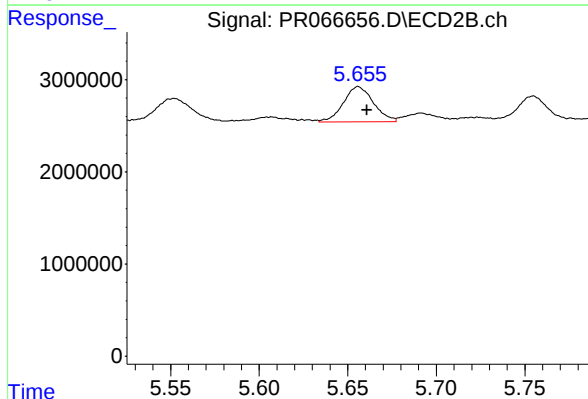


#29 AR-1254-4

R.T.: 5.656 min
Delta R.T.: -0.005 min
Response: 4486802
Conc: 21.01 ng/ml

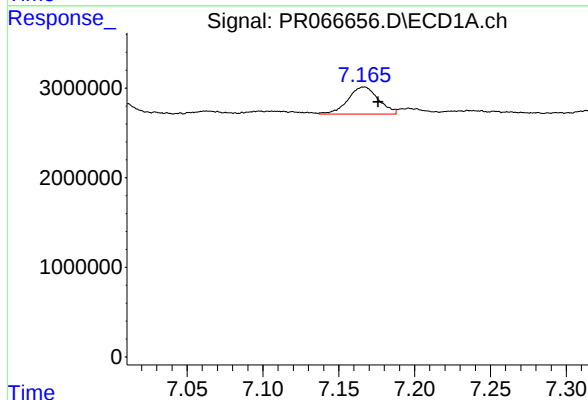


#30 AR-1254-5

R.T.: 7.167 min
Delta R.T.: -0.009 min
Response: 4238414
Conc: 23.78 ng/ml

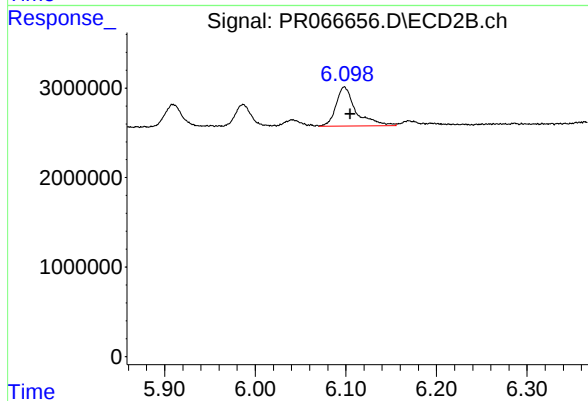

#30 AR-1254-5


R.T.: 6.098 min
Delta R.T.: -0.007 min
Response: 6676050
Conc: 20.75 ng/ml

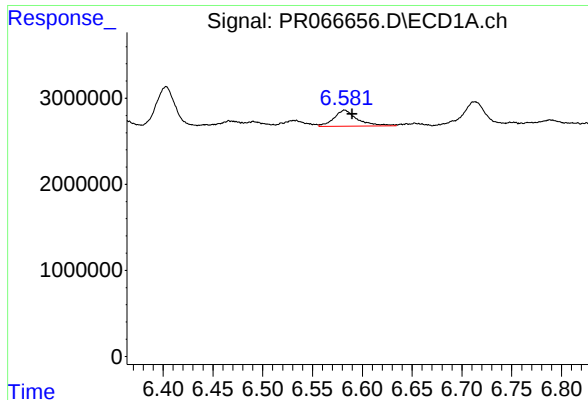

#31 AR-1260-1


R.T.: 6.582 min
Delta R.T.: -0.008 min
Response: 3081335
Conc: 14.83 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

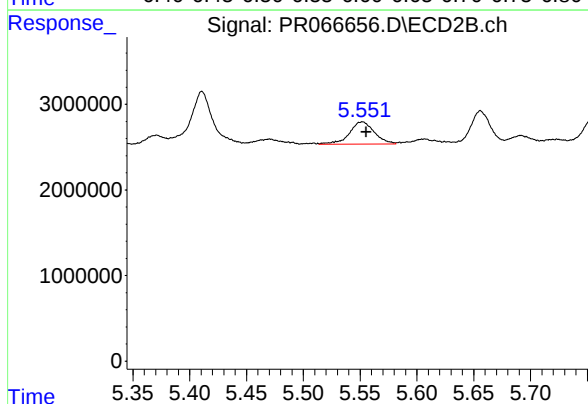


#31 AR-1260-1

R.T.: 5.552 min
Delta R.T.: -0.004 min
Response: 3989356
Conc: 15.74 ng/ml

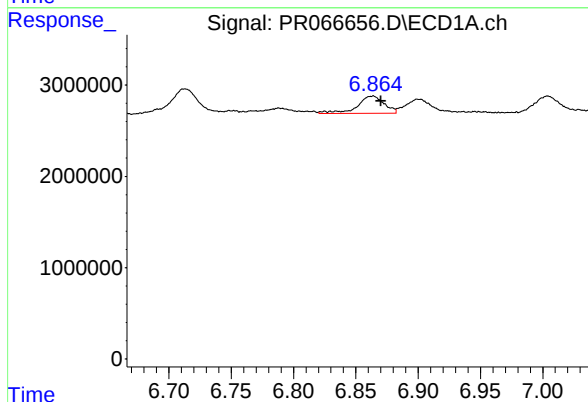


#32 AR-1260-2

R.T.: 6.863 min
Delta R.T.: -0.007 min
Response: 2830480
Conc: 12.76 ng/ml

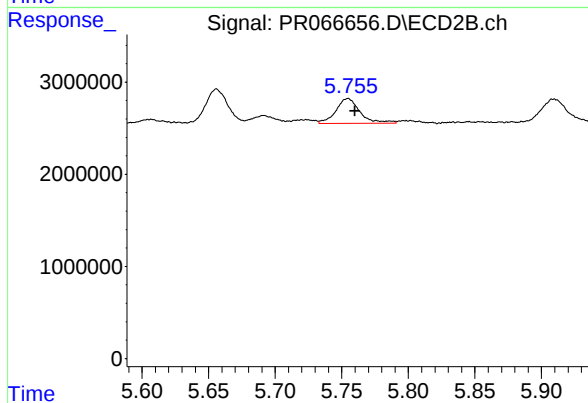

#32 AR-1260-2


R.T.: 5.755 min
Delta R.T.: -0.005 min
Response: 3439551
Conc: 11.29 ng/ml

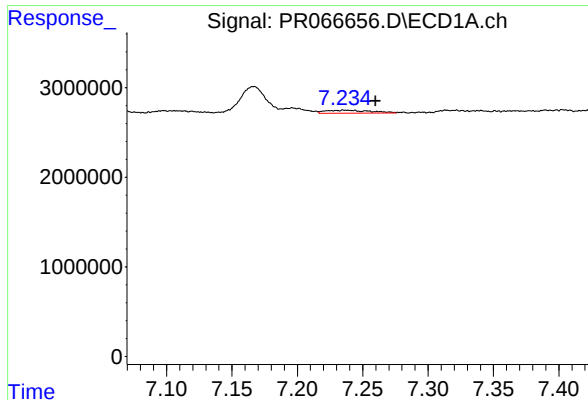

#33 AR-1260-3


R.T.: 7.236 min
Delta R.T.: -0.024 min
Response: 785528
Conc: 4.68 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

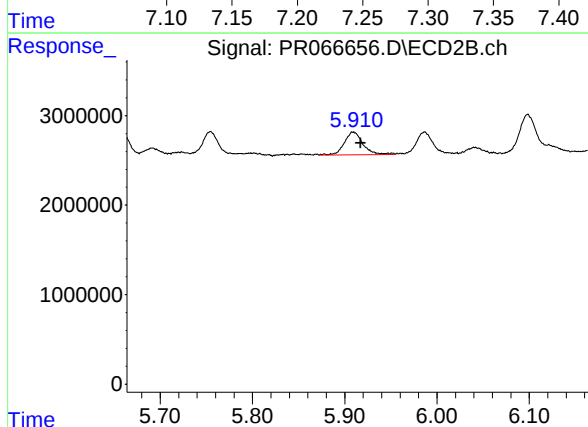


#33 AR-1260-3

R.T.: 5.909 min
Delta R.T.: -0.008 min
Response: 3595184
Conc: 12.35 ng/ml

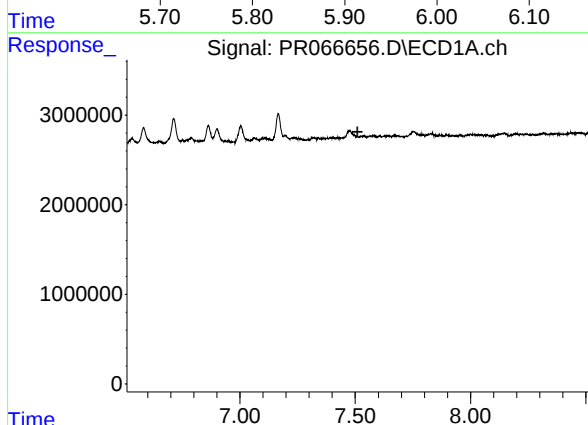


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.510 min
Response: 0
Conc: N.D.

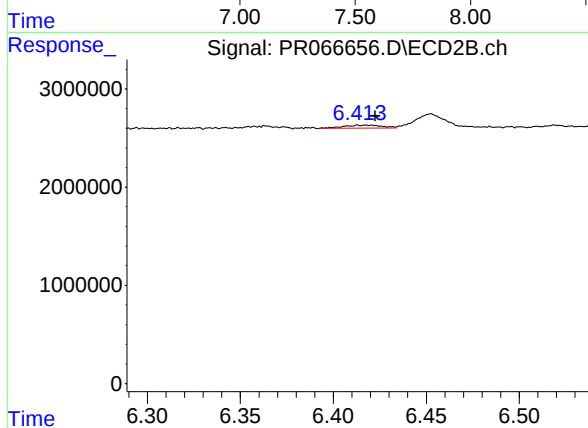

#34 AR-1260-4


R.T.: 6.418 min
Delta R.T.: -0.004 min
Response: 454223
Conc: 1.82 ng/ml

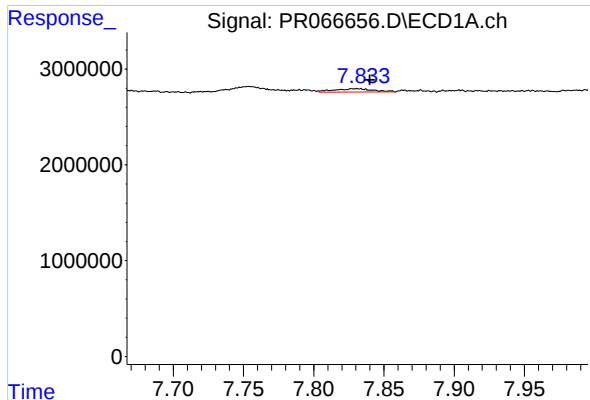

#35 AR-1260-5


R.T.: 7.832 min
Delta R.T.: -0.008 min
Response: 694818
Conc: 2.38 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

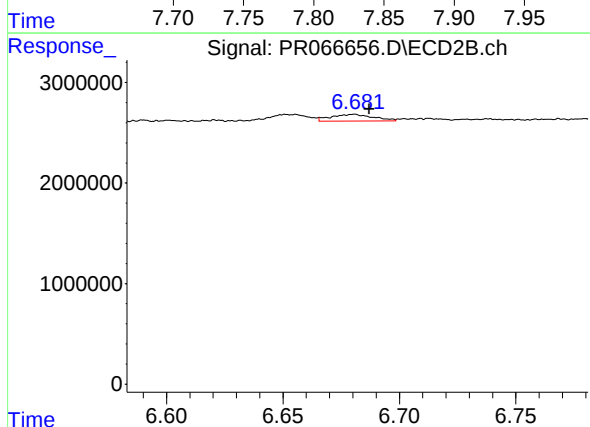


#35 AR-1260-5

R.T.: 6.680 min
Delta R.T.: -0.007 min
Response: 821556
Conc: 1.46 ng/ml

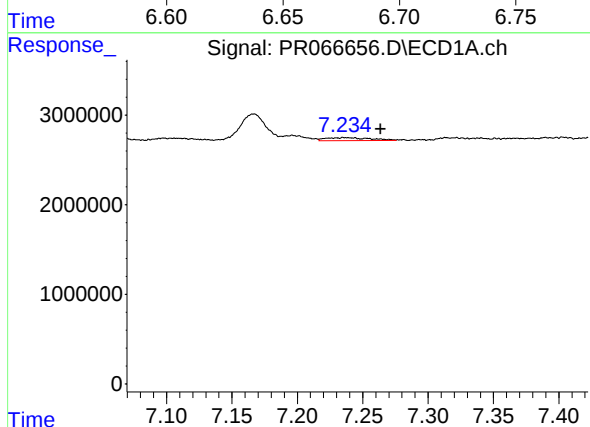


#36 AR-1262-1

R.T.: 7.236 min
Delta R.T.: -0.028 min
Response: 785528
Conc: 3.44 ng/ml

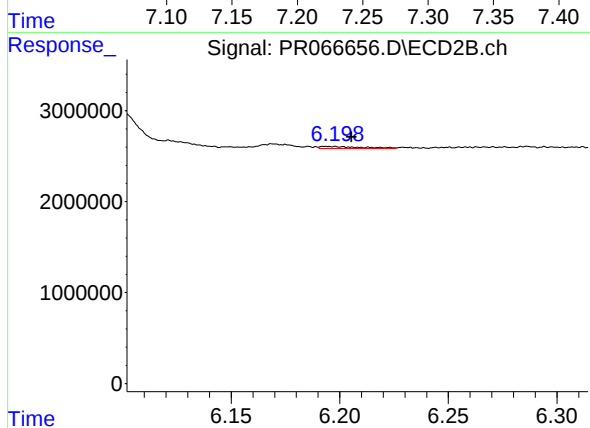

#36 AR-1262-1


R.T.: 6.194 min
Delta R.T.: -0.012 min
Response: 305141
Conc: 2.11 ng/ml

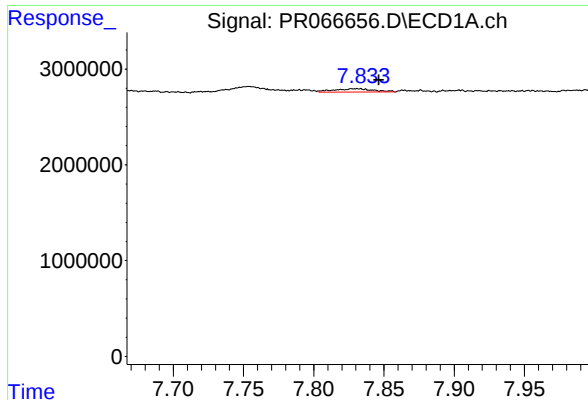

#37 AR-1262-2


R.T.: 7.832 min
Delta R.T.: -0.015 min
Response: 694818
Conc: 2.19 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

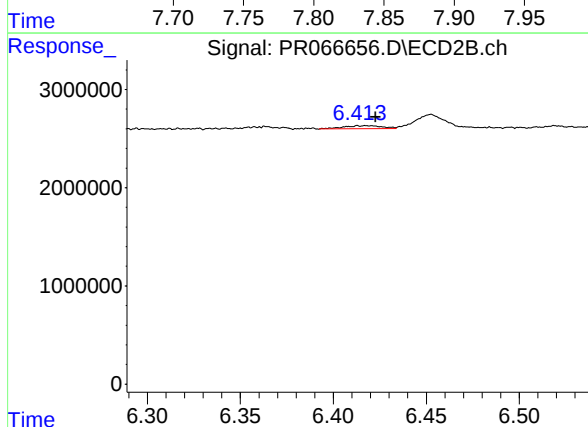


#37 AR-1262-2

R.T.: 6.418 min
Delta R.T.: -0.004 min
Response: 454223
Conc: 1.48 ng/ml

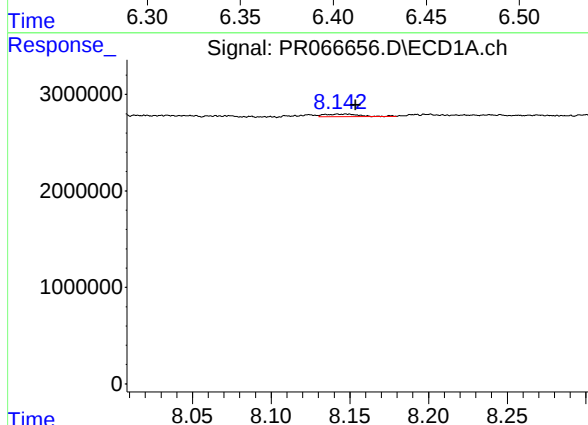


#38 AR-1262-3

R.T.: 8.142 min
Delta R.T.: -0.011 min
Response: 410299
Conc: 1.94 ng/ml

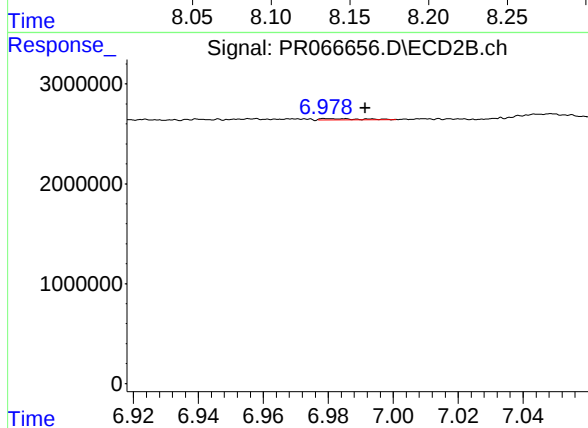

#38 AR-1262-3


R.T.: 6.981 min
Delta R.T.: -0.011 min
Response: 96192
Conc: 0.40 ng/ml

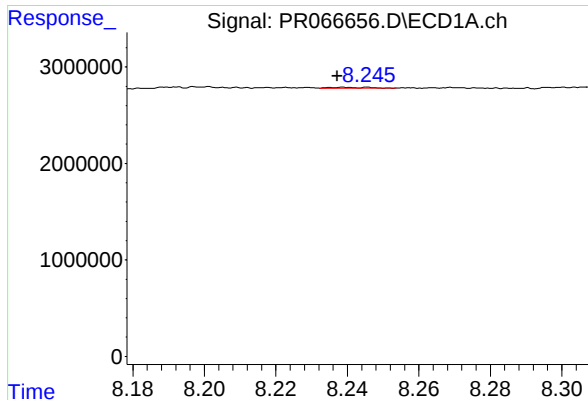

#39 AR-1262-4


R.T.: 8.246 min
Delta R.T.: 0.009 min
Response: 74440
Conc: 0.68 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

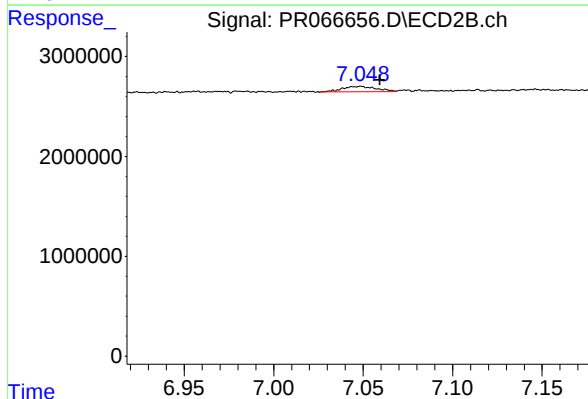


#39 AR-1262-4

R.T.: 7.049 min
Delta R.T.: -0.011 min
Response: 704477
Conc: 1.60 ng/ml

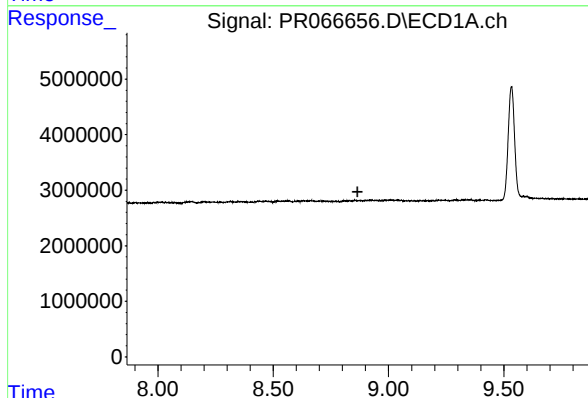


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 8.865 min
Response: 0
Conc: N.D.

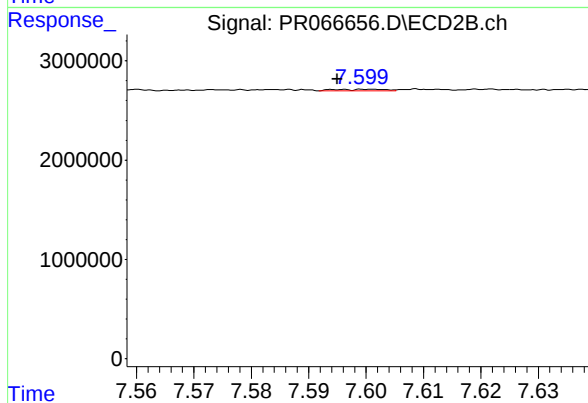

#40 AR-1262-5


R.T.: 7.601 min
Delta R.T.: 0.006 min
Response: 97603
Conc: 0.45 ng/ml

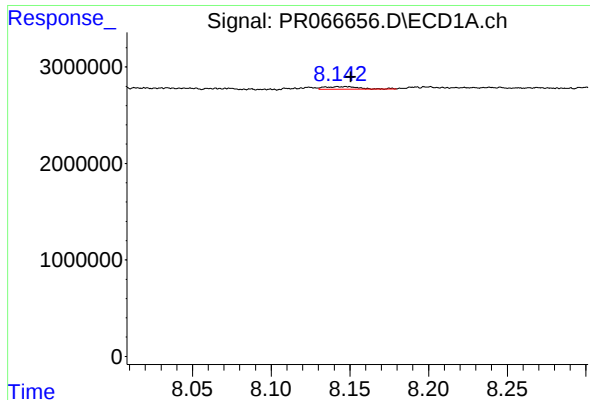

#41 AR-1268-1


R.T.: 8.142 min
Delta R.T.: -0.008 min
Response: 410299
Conc: 1.05 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

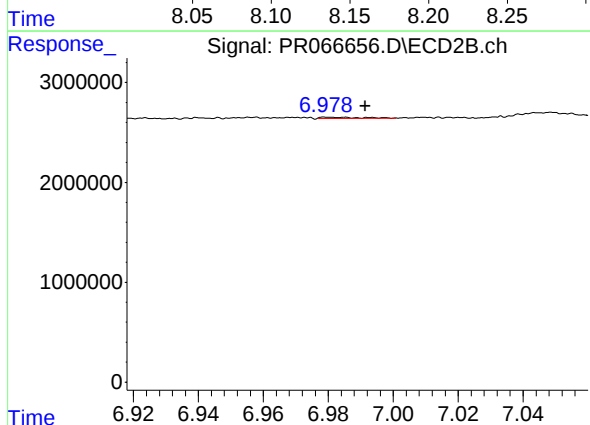


#41 AR-1268-1

R.T.: 6.981 min
Delta R.T.: -0.011 min
Response: 96192
Conc: 0.13 ng/ml

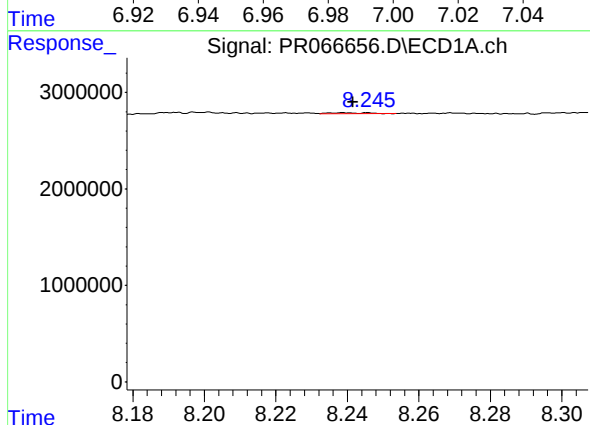


#42 AR-1268-2

R.T.: 8.246 min
Delta R.T.: 0.004 min
Response: 74440
Conc: 0.22 ng/ml

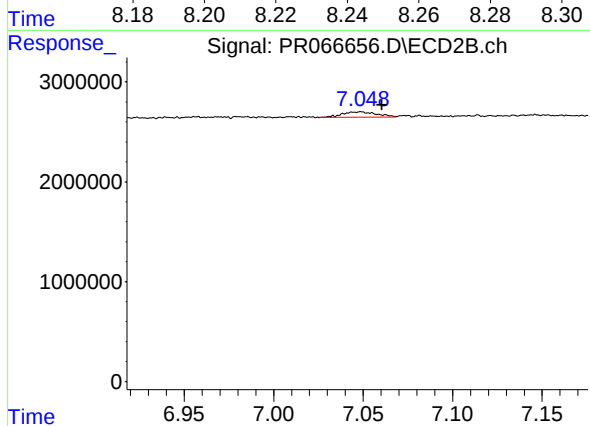

#42 AR-1268-2


R.T.: 7.049 min
Delta R.T.: -0.012 min
Response: 704477
Conc: 1.10 ng/ml

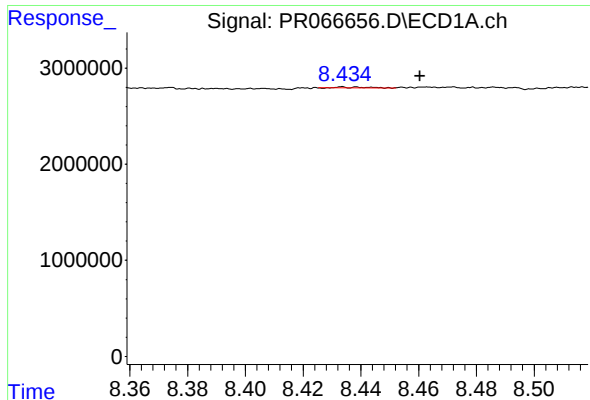

#43 AR-1268-3


R.T.: 8.433 min
Delta R.T.: -0.027 min
Response: 73317
Conc: 0.24 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

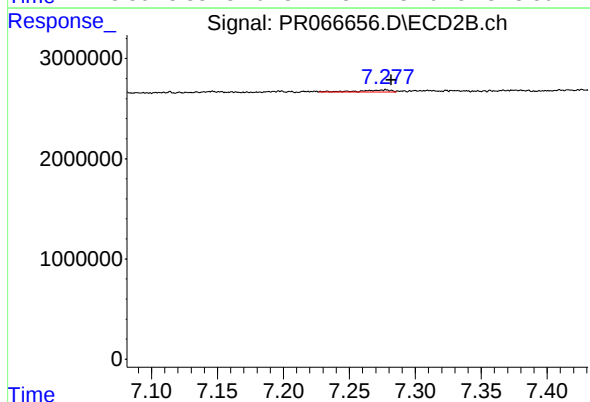


#43 AR-1268-3

R.T.: 7.277 min
Delta R.T.: -0.005 min
Response: 354760
Conc: 0.63 ng/ml

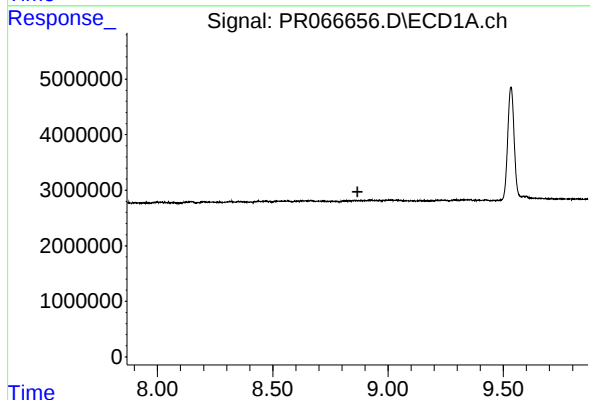


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 8.867 min
Response: 0
Conc: N.D.

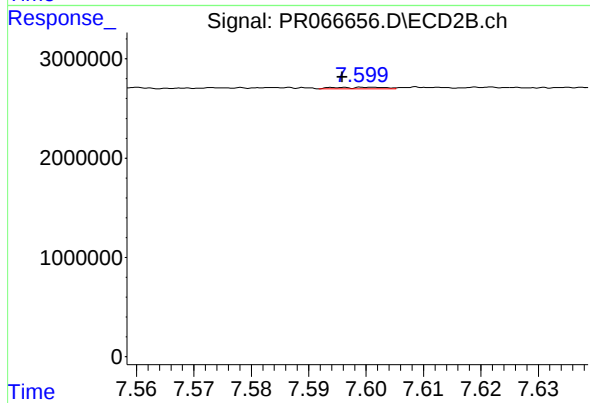

#44 AR-1268-4


R.T.: 7.601 min
Delta R.T.: 0.005 min
Response: 97603
Conc: 0.40 ng/ml

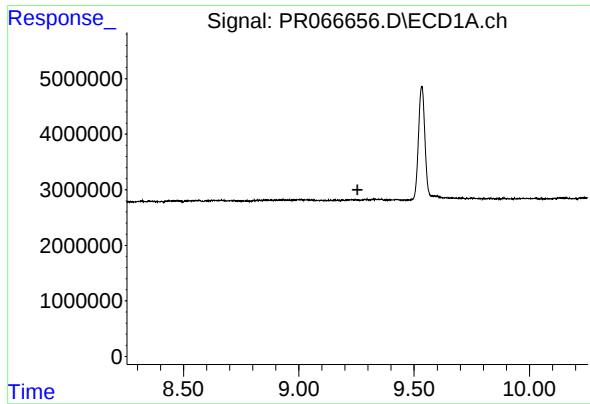

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.254 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

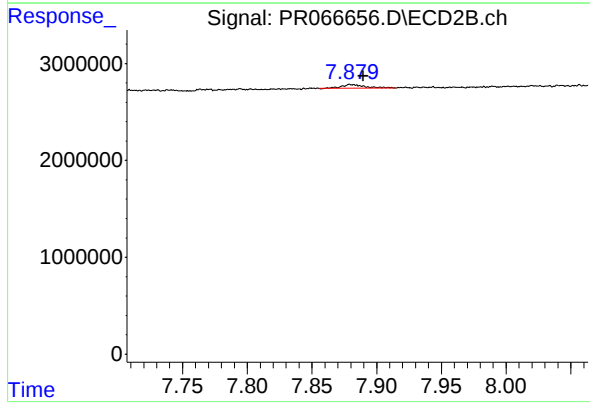

#45 AR-1268-5

R.T.: 7.880 min
Delta R.T.: -0.010 min
Response: 454962
Conc: 0.28 ng/ml