

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR050924\
 Data File : PR066657.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2024 06:45
 Operator : AJ\MA
 Sample : P2403-09
 Misc : AR1262 MDL 25 PPB
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT2-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 07:39:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 26 07:26:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.652	2.894	90407735	73994169	17.249	16.555
2) SA Decachlor...	9.534	8.121	40158875	74268799	17.149	15.823
Target Compounds						
3) L1 AR-1016-1	4.896	4.022	463397	512707	3.242	3.394
4) L1 AR-1016-2	4.908	4.022	337568	512707	1.544	2.389 #
5) L1 AR-1016-3	4.956	0.000	251735	0	1.733	N.D. #
6) L1 AR-1016-4	5.056	4.248	432503	190486	3.764	1.975 #
7) L1 AR-1016-5	5.378	4.465	129336	254646	1.136	2.060 #
8) L2 AR-1221-1	3.859f	0.000	1046990	0	17.340	N.D. #
9) L2 AR-1221-2	3.964	3.194	1460000	1603645	33.040	38.625
10) L2 AR-1221-3	4.039	3.283	167433	438515	1.289	3.630 #
11) L3 AR-1232-1	4.039	3.283	167433	438515	1.572	4.369 #
12) L3 AR-1232-2	4.578f	4.022	725315	512707	11.819	5.152 #
13) L3 AR-1232-3	4.908	0.000	337568	0	3.303	N.D. #
14) L3 AR-1232-4	5.056	4.288	432503	79977	8.032	1.649 #
15) L3 AR-1232-5	5.170	4.465	274282	254646	6.817	4.773 #
16) L4 AR-1242-1	4.896f	4.022	463397	512707	3.893	4.096
17) L4 AR-1242-2	4.908	4.022	337568	512707	1.878	2.893 #
18) L4 AR-1242-3	4.956	0.000	251735	0	2.113	N.D. #
19) L4 AR-1242-4	5.056	4.288	432503	79977	4.569	0.838 #
20) L4 AR-1242-5	5.845	4.832	342382	1122744	3.808	9.141 #
21) L5 AR-1248-1	4.896f	4.022	463397	512707	5.354	5.515
22) L5 AR-1248-2	5.170	4.248	274282	190486	2.061	1.408 #
23) L5 AR-1248-3	5.378	4.288	129336	79977	0.862	0.581 #
24) L5 AR-1248-4	0.000	4.465	0	254646	N.D.	1.540 #
25) L5 AR-1248-5	5.845	4.874	342382	271070	2.391	1.680 #
26) L6 AR-1254-1	5.777	4.832	3088680	1122744	18.586	4.569 #
27) L6 AR-1254-2	6.012	4.992	1004444	1843716	4.100	8.419 #
28) L6 AR-1254-3	6.397	5.430	1106699	3413316	4.477	9.930 #
29) L6 AR-1254-4	6.694f	5.658	1664377	358571	10.484	1.679 #
30) L6 AR-1254-5	7.162	6.097	4375503	3919509	24.551	12.180 #
31) L7 AR-1260-1	6.581	5.550	4758043	5040009	22.896	19.886
32) L7 AR-1260-2	6.863	5.754	4331256	6010462	19.525	19.736
33) L7 AR-1260-3	7.253	5.914	6299522	6190351	37.564	21.263 #
34) L7 AR-1260-4	7.494f	6.416	6078223	6691216	34.113	26.796
35) L7 AR-1260-5	7.832	6.680	7913752	12448193	27.098	22.171
36) L8 AR-1262-1	7.253	6.199	6299522	3229371	27.614	22.351
37) L8 AR-1262-2	7.832	6.416	7913752	6691216	24.917	21.745
38) L8 AR-1262-3	8.137f	6.984	5086117	5643107	24.024	23.281
39) L8 AR-1262-4	8.221f	7.051	4675786	9504222	42.805	21.626 #
40) L8 AR-1262-5	8.841f	7.587	1502551	4542709	14.783	21.041 #
41) L9 AR-1268-1	8.137	6.984	5086117	5643107	13.046	7.794 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR050924\
 Data File : PR066657.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2024 06:45
 Operator : AJ\MA
 Sample : P2403-09
 Misc : AR1262 MDL 25 PPB
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT2-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 07:39:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 26 07:26:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm


	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.221f	7.051	4675786	9504222	13.609	14.809
43) L9	AR-1268-3	0.000	7.272	0	663656	N.D.	1.170 #
44) L9	AR-1268-4	8.841f	7.587	1502551	4542709	12.931	18.613 #
45) L9	AR-1268-5	0.000	7.881	0	1925341	N.D.	1.188 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

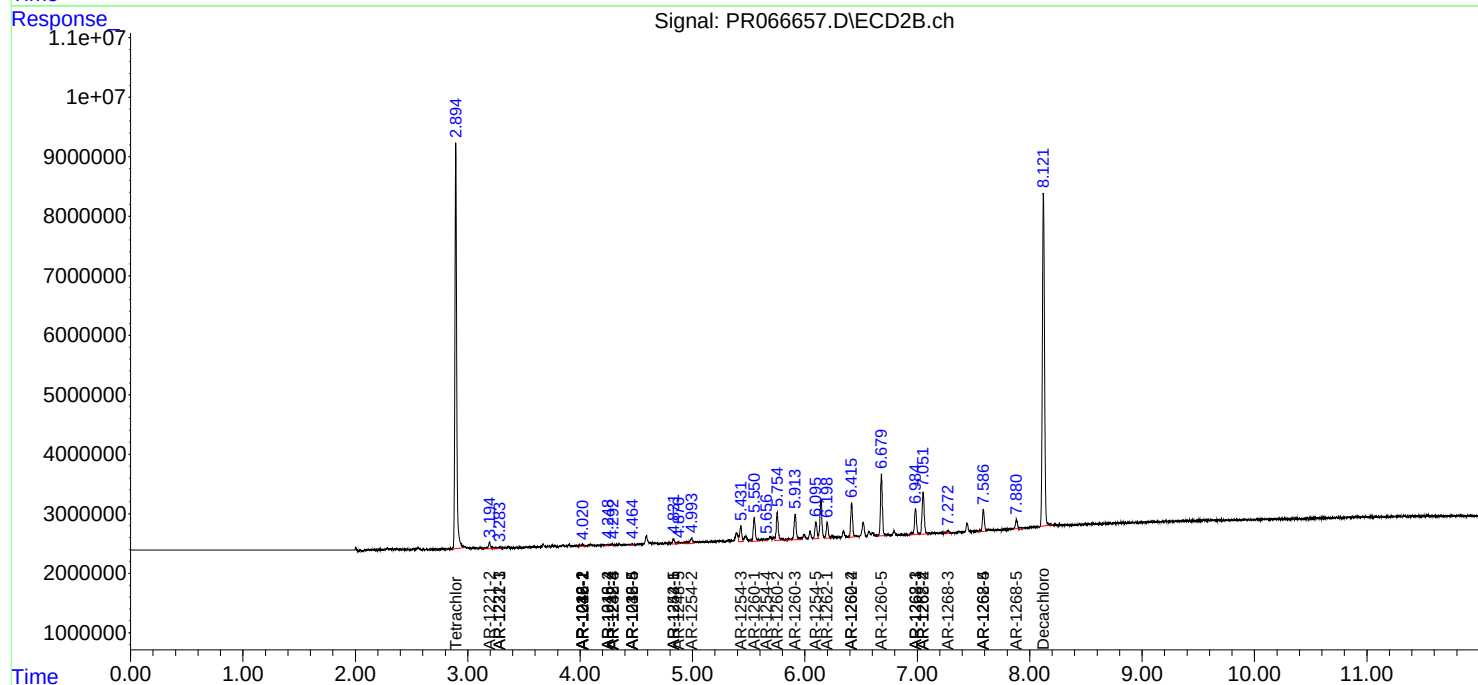


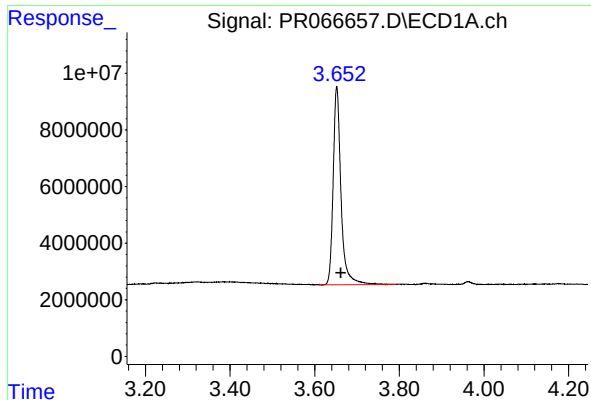

#1 Tetrachloro-m-xylene


R.T.: 3.652 min
Delta R.T.: -0.010 min
Response: 90407735
Conc: 17.25 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

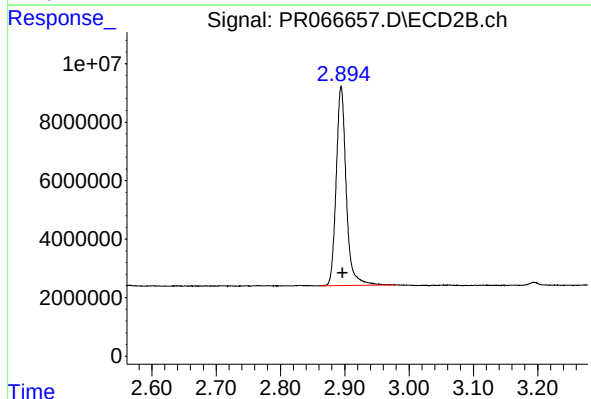


#1 Tetrachloro-m-xylene

R.T.: 2.894 min
Delta R.T.: -0.003 min
Response: 73994169
Conc: 16.55 ng/ml

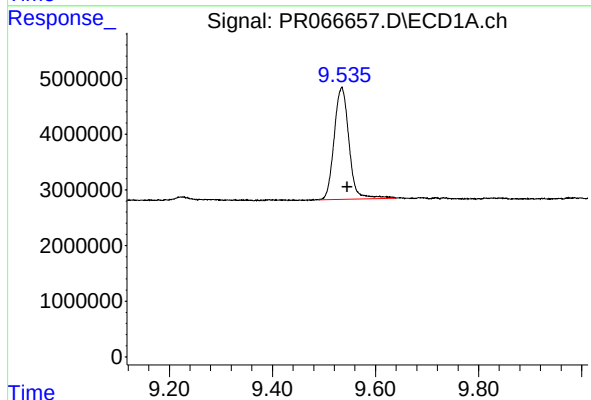


#2 Decachlorobiphenyl

R.T.: 9.534 min
Delta R.T.: -0.011 min
Response: 40158875
Conc: 17.15 ng/ml

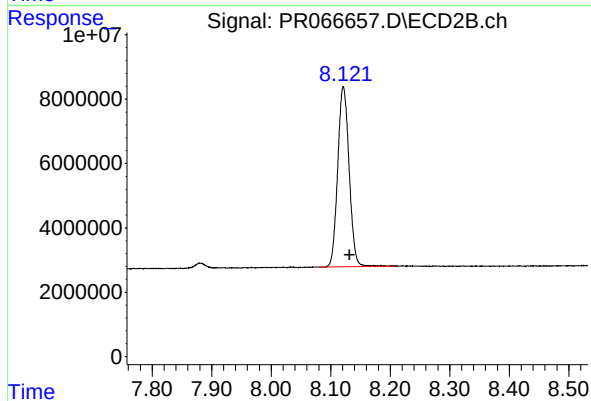

#2 Decachlorobiphenyl


R.T.: 8.121 min
Delta R.T.: -0.010 min
Response: 74268799
Conc: 15.82 ng/ml

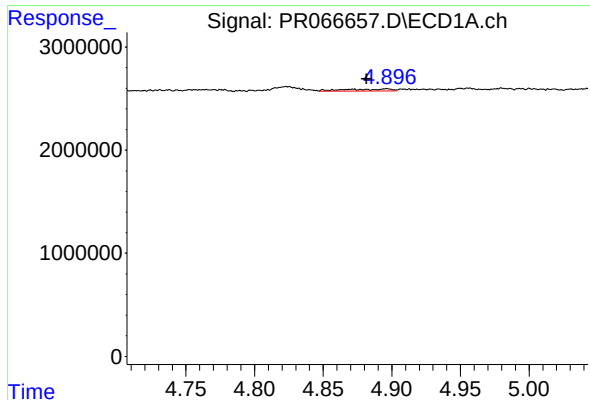

#3 AR-1016-1


R.T.: 4.896 min
Delta R.T.: 0.015 min
Response: 463397
Conc: 3.24 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

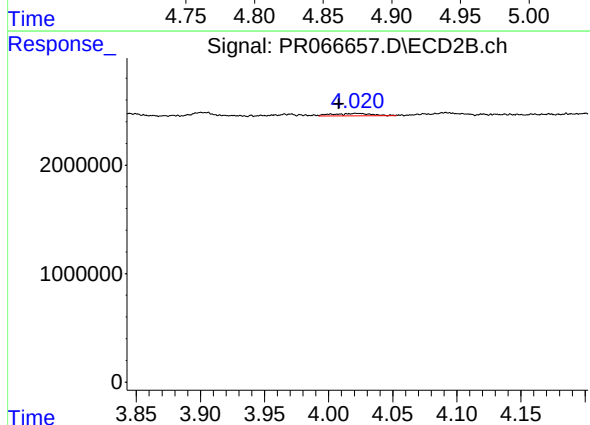


#3 AR-1016-1

R.T.: 4.022 min
Delta R.T.: 0.014 min
Response: 512707
Conc: 3.39 ng/ml

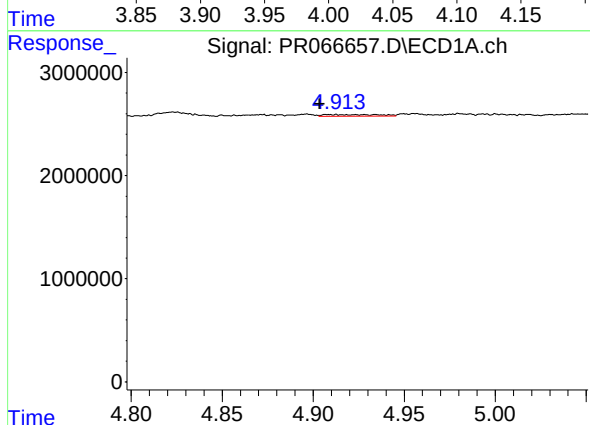


#4 AR-1016-2

R.T.: 4.908 min
Delta R.T.: 0.005 min
Response: 337568
Conc: 1.54 ng/ml

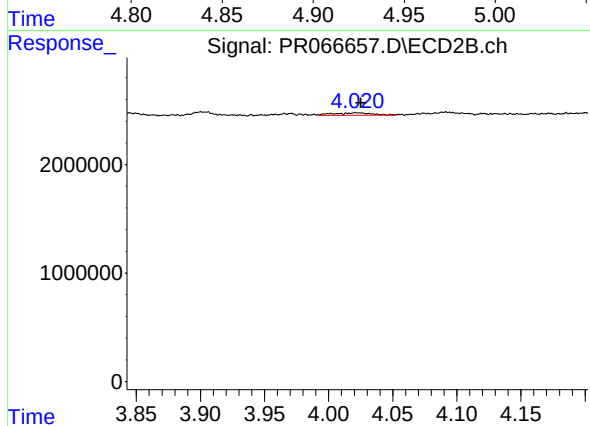

#4 AR-1016-2


R.T.: 4.022 min
Delta R.T.: -0.004 min
Response: 512707
Conc: 2.39 ng/ml

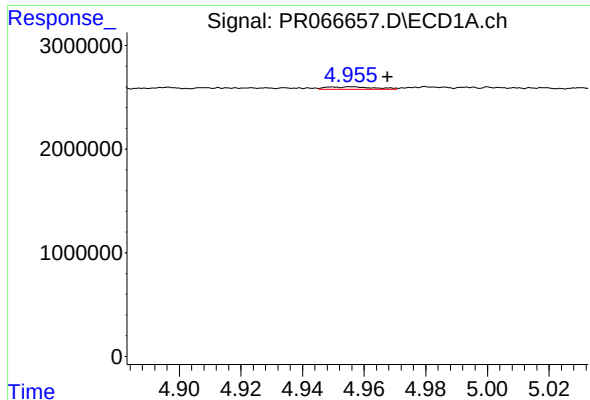

#5 AR-1016-3


R.T.: 4.956 min
Delta R.T.: -0.011 min
Response: 251735
Conc: 1.73 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

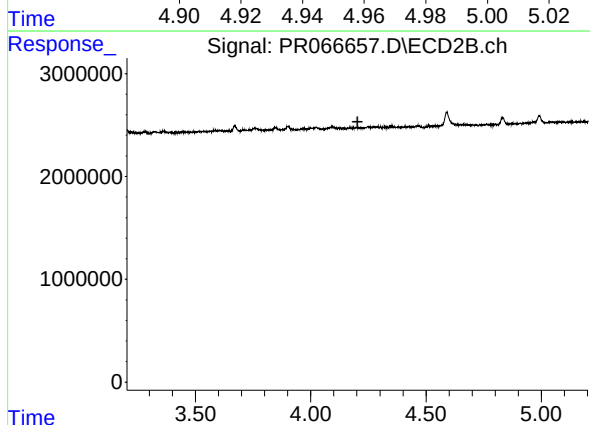


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T.: 4.203 min
Response: 0
Conc: N.D.

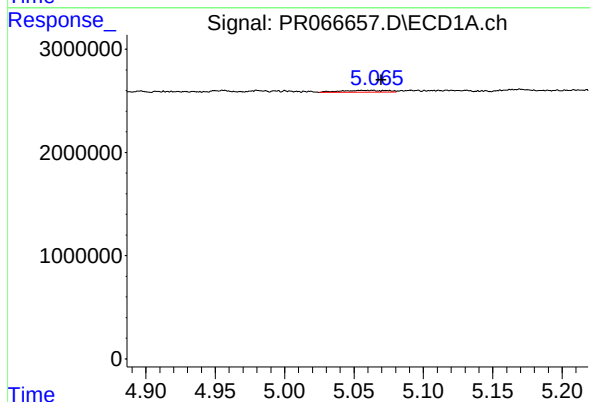


#6 AR-1016-4

R.T.: 5.056 min
Delta R.T.: -0.014 min
Response: 432503
Conc: 3.76 ng/ml

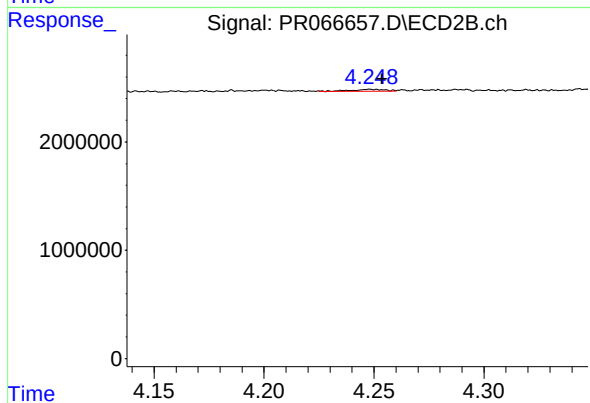

#6 AR-1016-4


R.T.: 4.248 min
Delta R.T.: -0.006 min
Response: 190486
Conc: 1.97 ng/ml

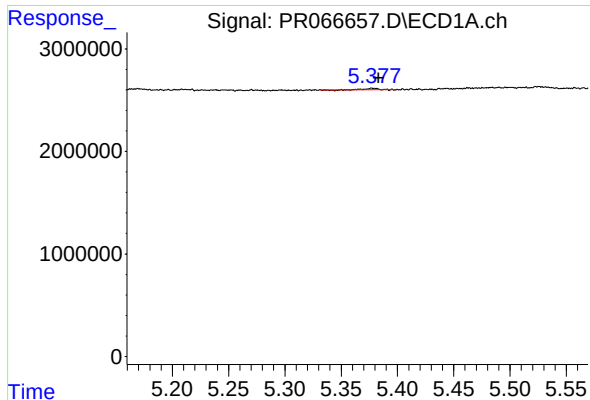

#7 AR-1016-5


R.T.: 5.378 min
Delta R.T.: -0.005 min
Response: 129336
Conc: 1.14 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

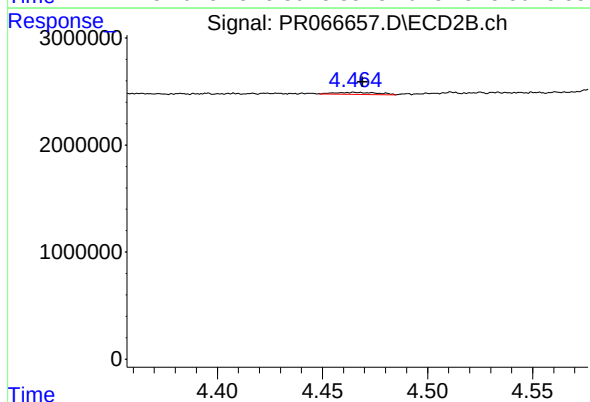


#7 AR-1016-5

R.T.: 4.465 min
Delta R.T.: -0.004 min
Response: 254646
Conc: 2.06 ng/ml

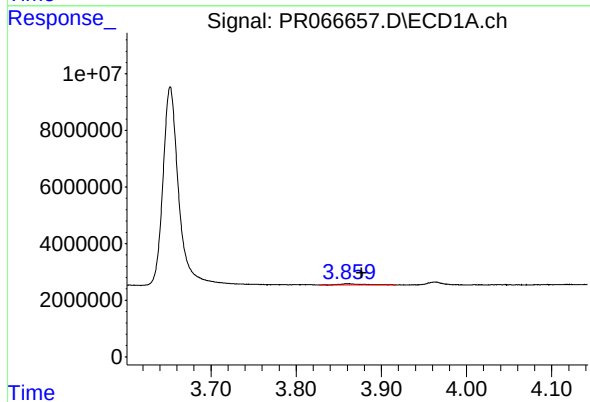


#8 AR-1221-1

R.T.: 3.859 min
Delta R.T.: -0.018 min
Response: 1046990
Conc: 17.34 ng/ml

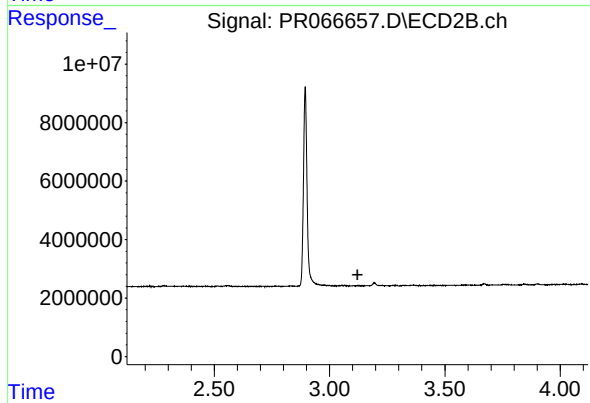

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.121 min
Response: 0
Conc: N.D.

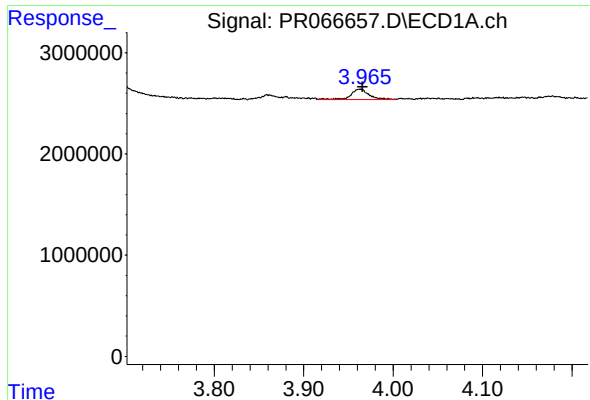

#9 AR-1221-2


R.T.: 3.964 min
Delta R.T.: -0.002 min
Response: 1460000
Conc: 33.04 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

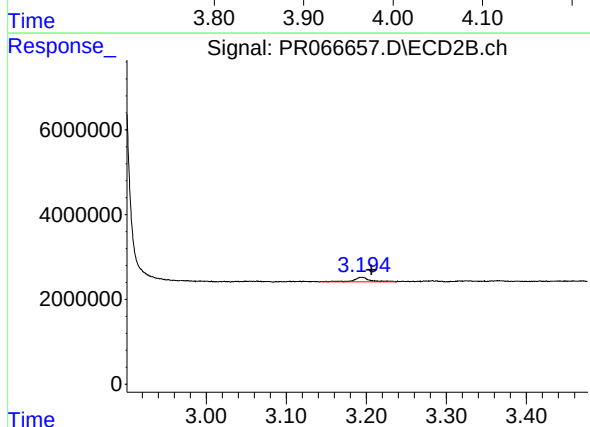


#9 AR-1221-2

R.T.: 3.194 min
Delta R.T.: -0.012 min
Response: 1603645
Conc: 38.62 ng/ml

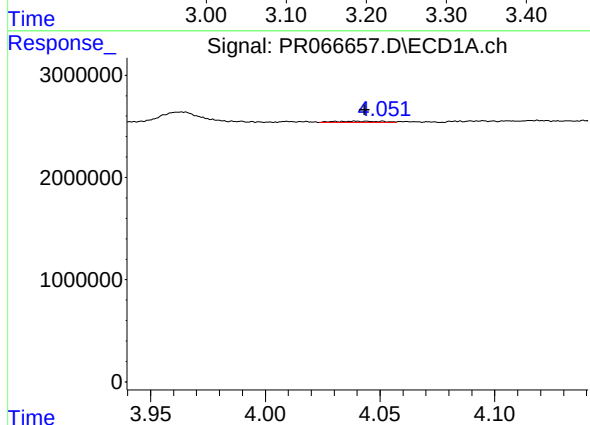


#10 AR-1221-3

R.T.: 4.039 min
Delta R.T.: -0.004 min
Response: 167433
Conc: 1.29 ng/ml

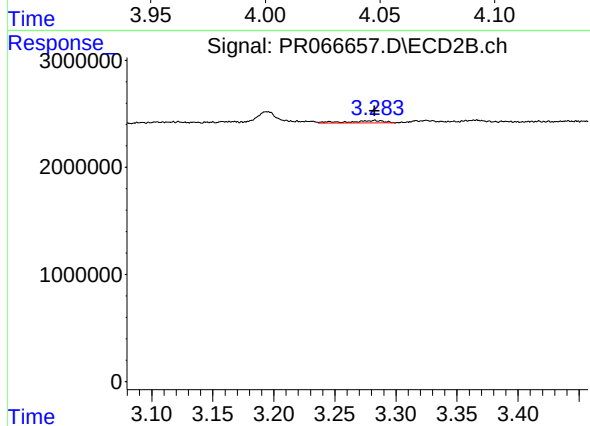

#10 AR-1221-3


R.T.: 3.283 min
Delta R.T.: 0.000 min
Response: 438515
Conc: 3.63 ng/ml

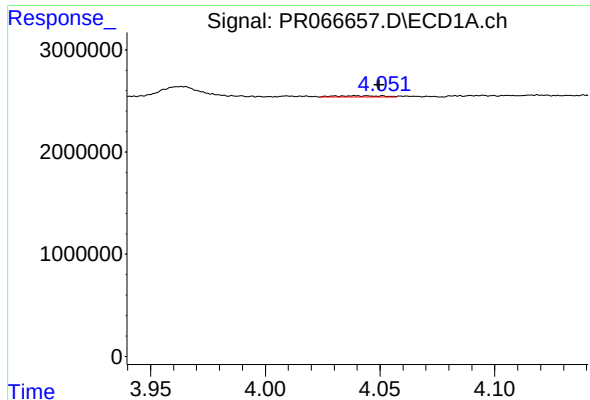

#11 AR-1232-1


R.T.: 4.039 min
Delta R.T.: -0.011 min
Response: 167433
Conc: 1.57 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

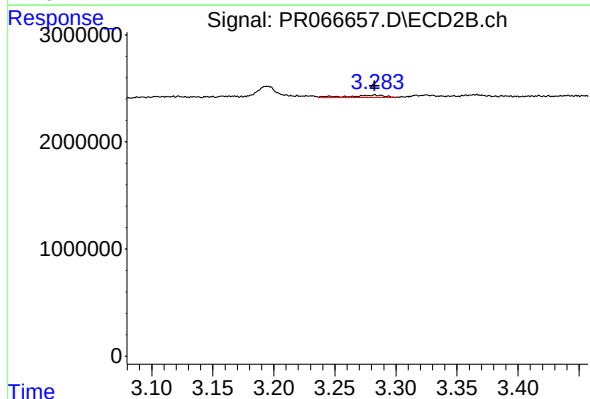


#11 AR-1232-1

R.T.: 3.283 min
Delta R.T.: 0.000 min
Response: 438515
Conc: 4.37 ng/ml

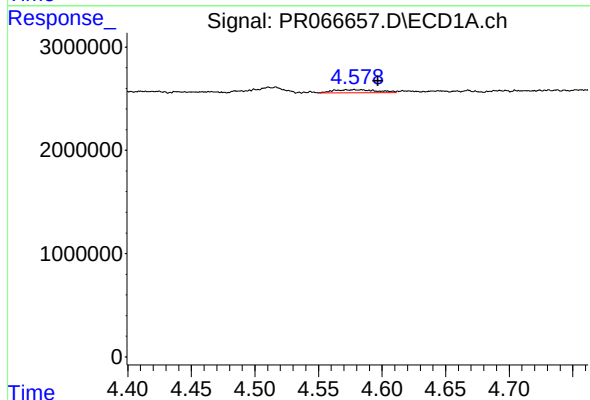


#12 AR-1232-2

R.T.: 4.578 min
Delta R.T.: -0.018 min
Response: 725315
Conc: 11.82 ng/ml

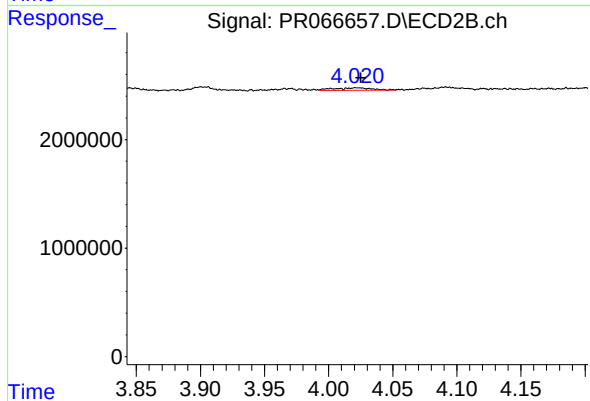

#12 AR-1232-2


R.T.: 4.022 min
Delta R.T.: -0.003 min
Response: 512707
Conc: 5.15 ng/ml

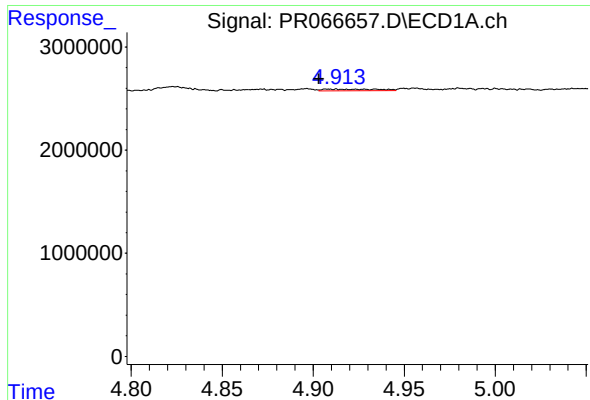

#13 AR-1232-3


R.T.: 4.908 min
Delta R.T.: 0.005 min
Response: 337568
Conc: 3.30 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

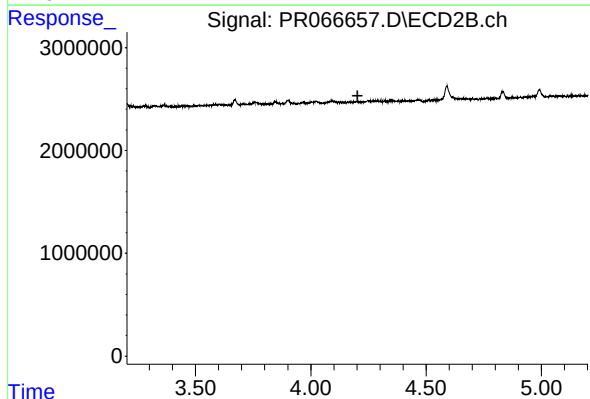


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 4.203 min
Response: 0
Conc: N.D.

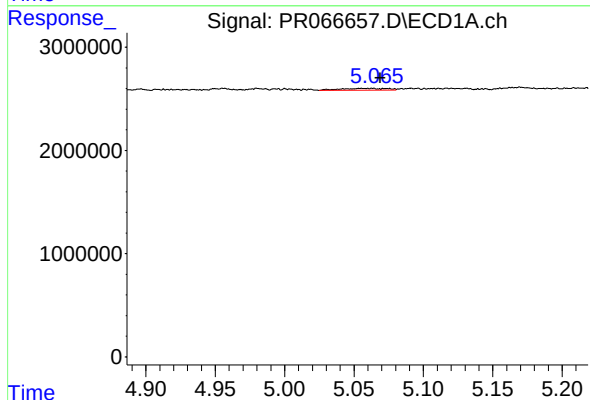


#14 AR-1232-4

R.T.: 5.056 min
Delta R.T.: -0.013 min
Response: 432503
Conc: 8.03 ng/ml

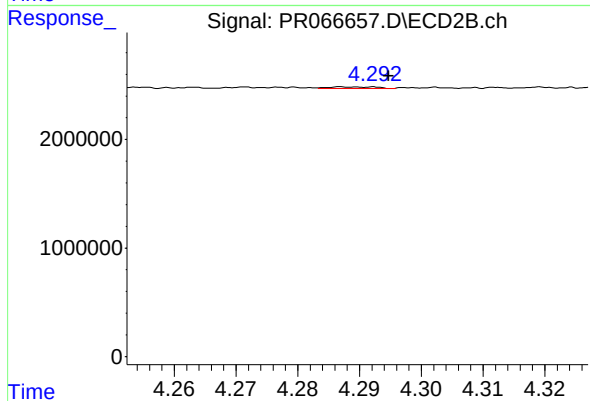

#14 AR-1232-4


R.T.: 4.288 min
Delta R.T.: -0.007 min
Response: 79977
Conc: 1.65 ng/ml

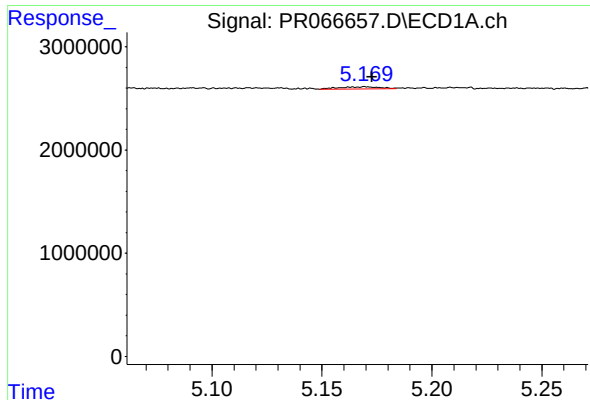

#15 AR-1232-5


R.T.: 5.170 min
Delta R.T.: -0.003 min
Response: 274282
Conc: 6.82 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

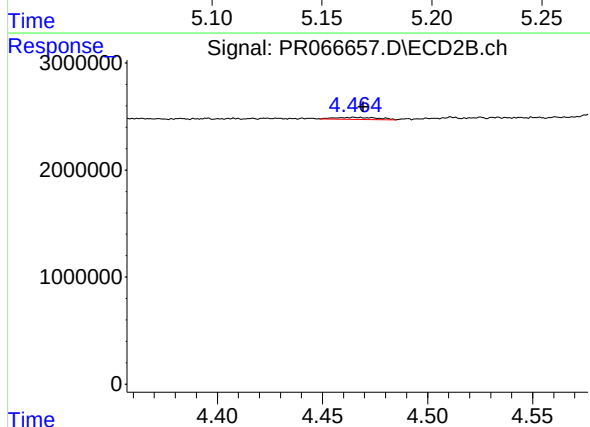


#15 AR-1232-5

R.T.: 4.465 min
Delta R.T.: -0.004 min
Response: 254646
Conc: 4.77 ng/ml

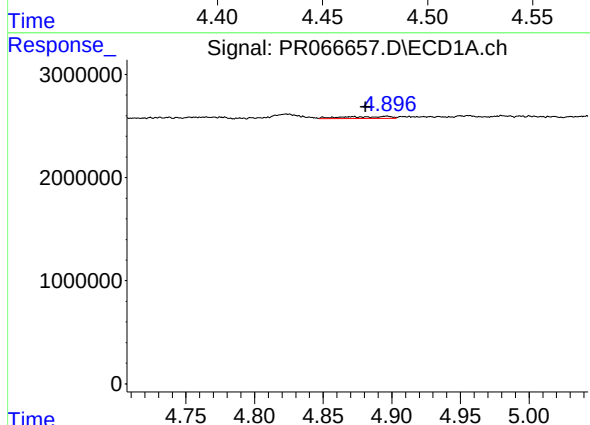


#16 AR-1242-1

R.T.: 4.896 min
Delta R.T.: 0.015 min
Response: 463397
Conc: 3.89 ng/ml

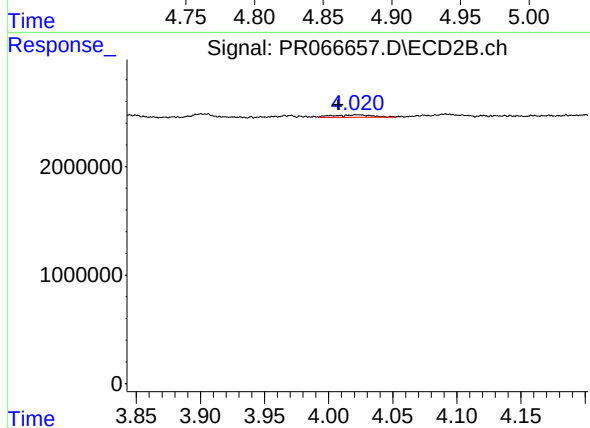

#16 AR-1242-1


R.T.: 4.022 min
Delta R.T.: 0.014 min
Response: 512707
Conc: 4.10 ng/ml

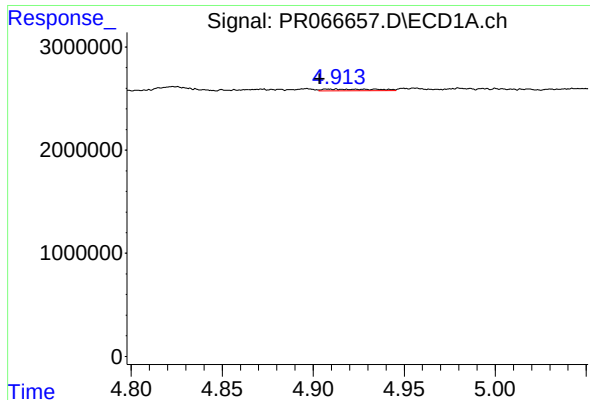

#17 AR-1242-2


R.T.: 4.908 min
Delta R.T.: 0.005 min
Response: 337568
Conc: 1.88 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

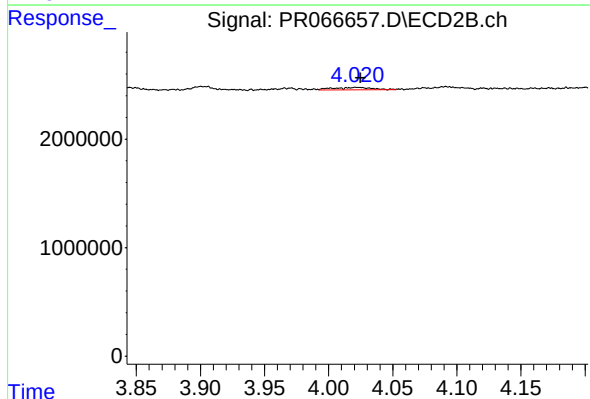


#17 AR-1242-2

R.T.: 4.022 min
Delta R.T.: -0.003 min
Response: 512707
Conc: 2.89 ng/ml

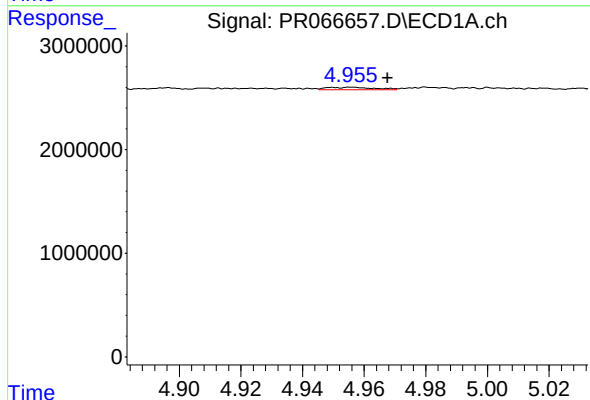


#18 AR-1242-3

R.T.: 4.956 min
Delta R.T.: -0.011 min
Response: 251735
Conc: 2.11 ng/ml

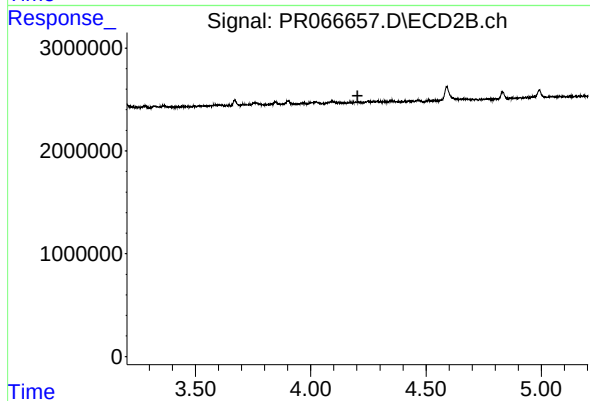

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 4.203 min
Response: 0
Conc: N.D.

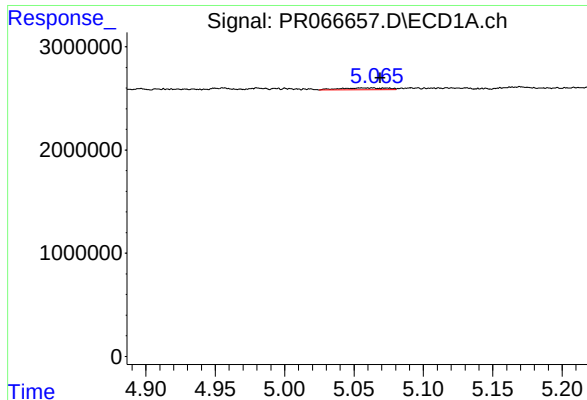

#19 AR-1242-4


R.T.: 5.056 min
Delta R.T.: -0.013 min
Response: 432503
Conc: 4.57 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

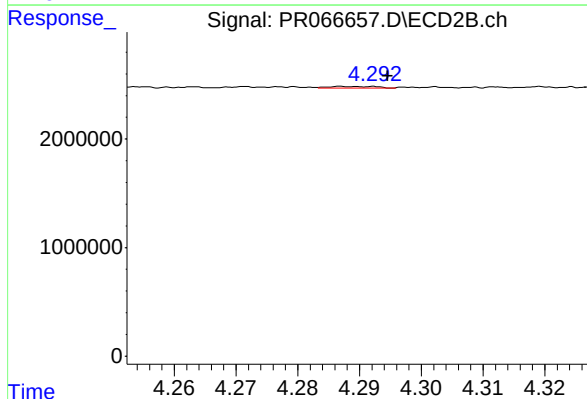


#19 AR-1242-4

R.T.: 4.288 min
Delta R.T.: -0.007 min
Response: 79977
Conc: 0.84 ng/ml

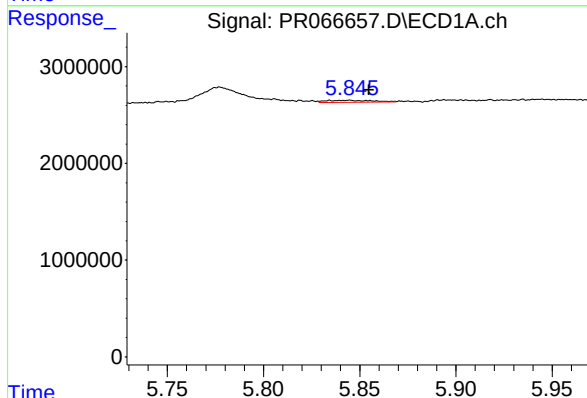


#20 AR-1242-5

R.T.: 5.845 min
Delta R.T.: -0.010 min
Response: 342382
Conc: 3.81 ng/ml

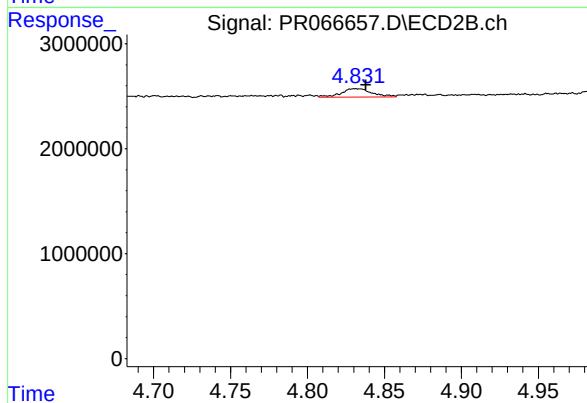

#20 AR-1242-5


R.T.: 4.832 min
Delta R.T.: -0.007 min
Response: 1122744
Conc: 9.14 ng/ml

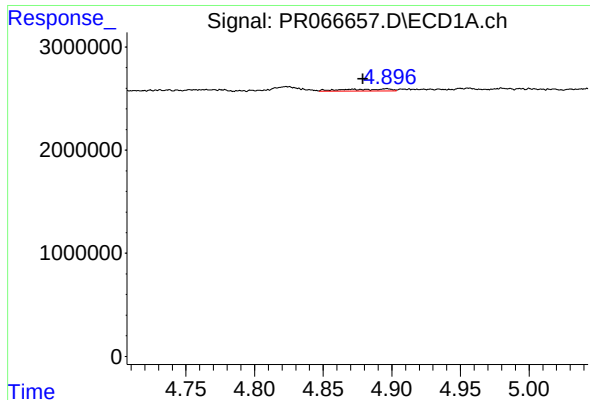

#21 AR-1248-1


R.T.: 4.896 min
Delta R.T.: 0.017 min
Response: 463397
Conc: 5.35 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

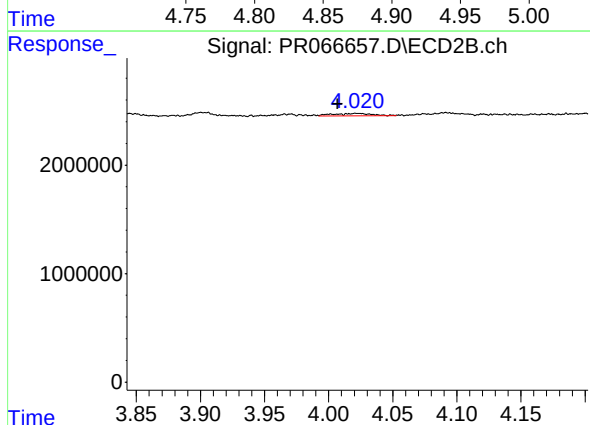


#21 AR-1248-1

R.T.: 4.022 min
Delta R.T.: 0.015 min
Response: 512707
Conc: 5.51 ng/ml

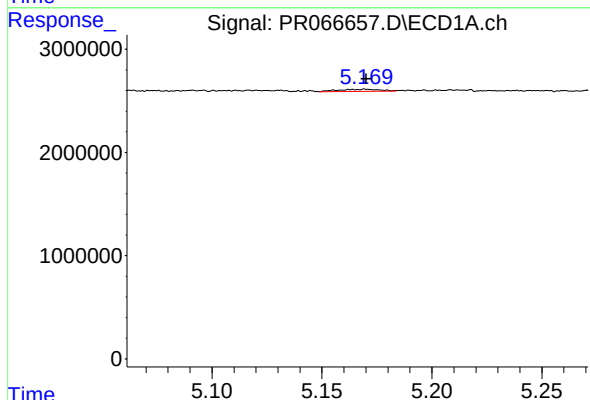


#22 AR-1248-2

R.T.: 5.170 min
Delta R.T.: 0.000 min
Response: 274282
Conc: 2.06 ng/ml

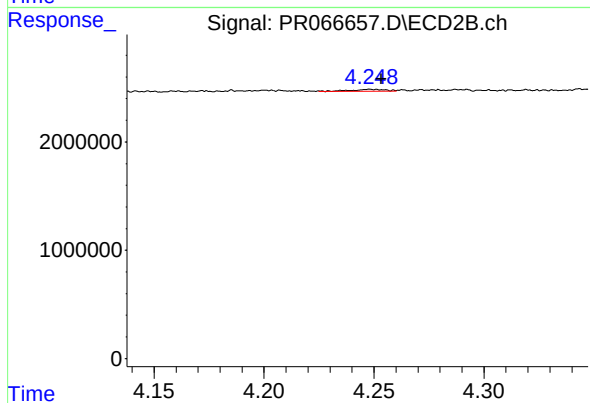

#22 AR-1248-2


R.T.: 4.248 min
Delta R.T.: -0.005 min
Response: 190486
Conc: 1.41 ng/ml

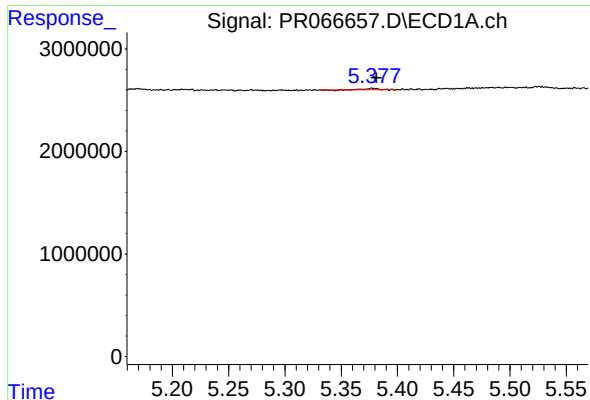

#23 AR-1248-3


R.T.: 5.378 min
Delta R.T.: -0.004 min
Response: 129336
Conc: 0.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

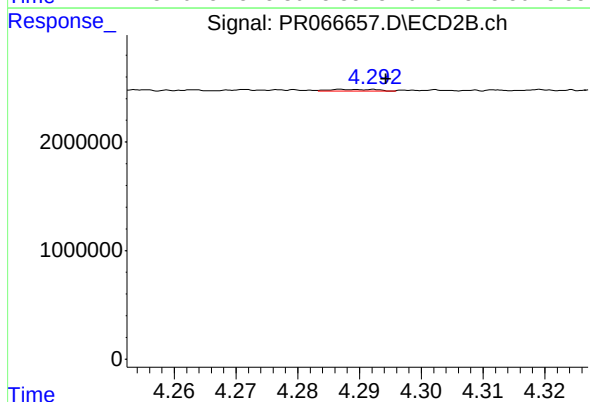


#23 AR-1248-3

R.T.: 4.288 min
Delta R.T.: -0.006 min
Response: 79977
Conc: 0.58 ng/ml

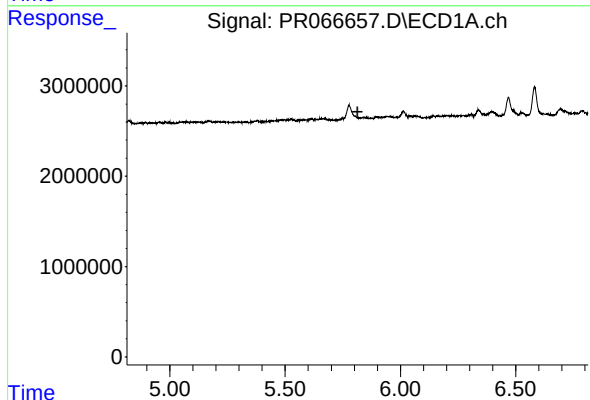


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 5.814 min
Response: 0
Conc: N.D.

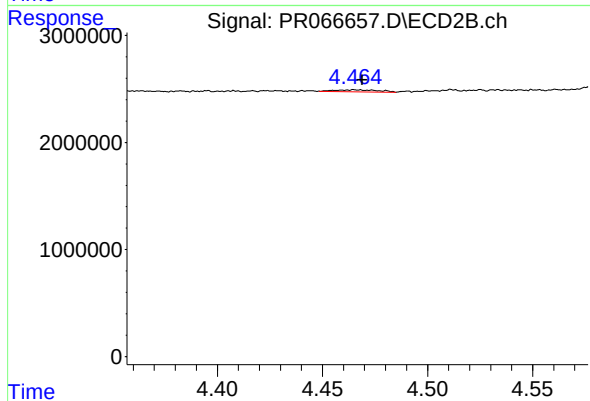

#24 AR-1248-4


R.T.: 4.465 min
Delta R.T.: -0.004 min
Response: 254646
Conc: 1.54 ng/ml

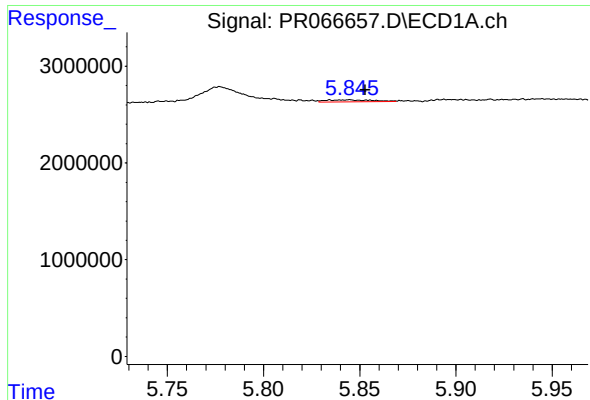

#25 AR-1248-5


R.T.: 5.845 min
Delta R.T.: -0.008 min
Response: 342382
Conc: 2.39 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

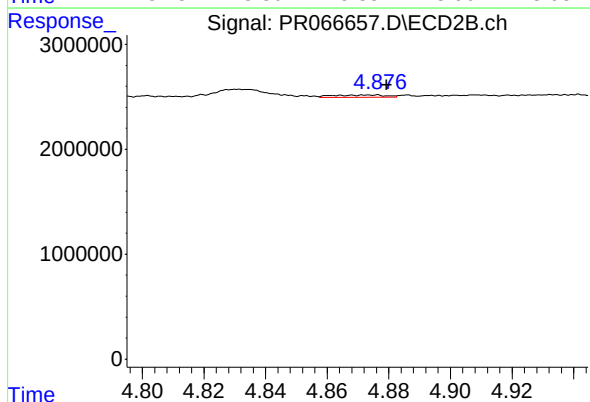


#25 AR-1248-5

R.T.: 4.874 min
Delta R.T.: -0.005 min
Response: 271070
Conc: 1.68 ng/ml

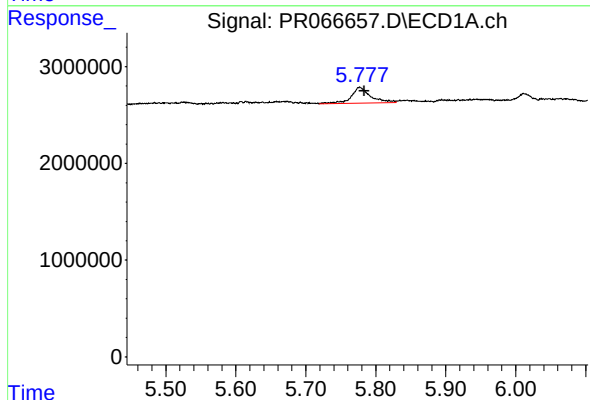


#26 AR-1254-1

R.T.: 5.777 min
Delta R.T.: -0.006 min
Response: 3088680
Conc: 18.59 ng/ml

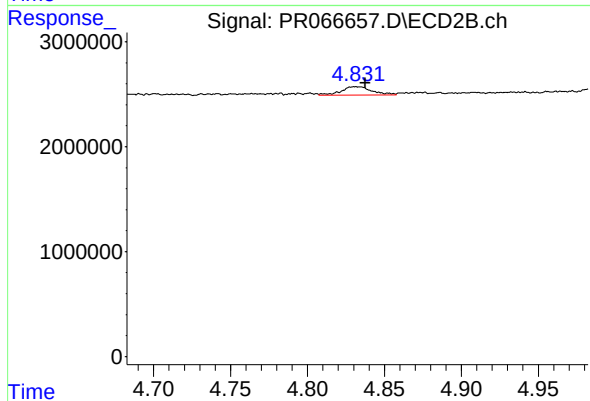

#26 AR-1254-1


R.T.: 4.832 min
Delta R.T.: -0.006 min
Response: 1122744
Conc: 4.57 ng/ml

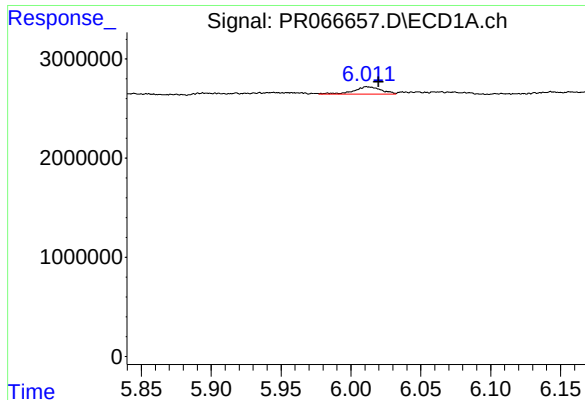

#27 AR-1254-2


R.T.: 6.012 min
Delta R.T.: -0.008 min
Response: 1004444
Conc: 4.10 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

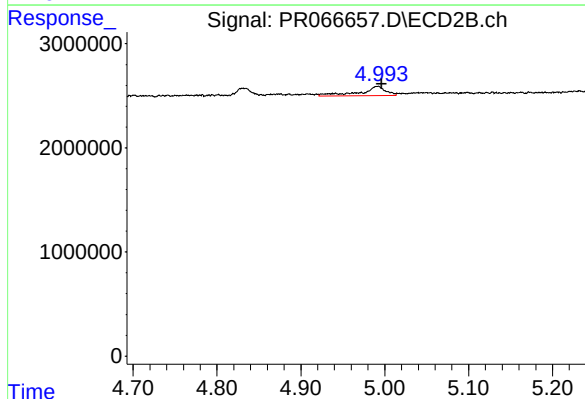


#27 AR-1254-2

R.T.: 4.992 min
Delta R.T.: -0.004 min
Response: 1843716
Conc: 8.42 ng/ml

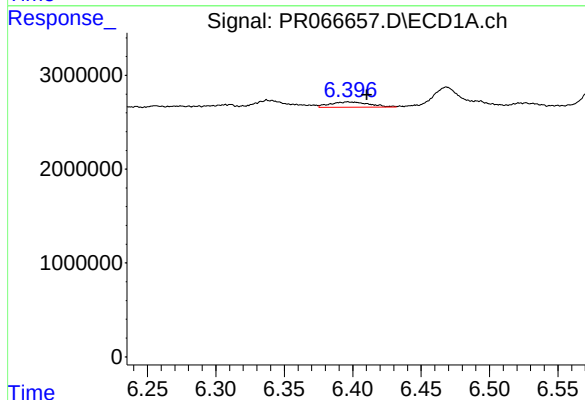


#28 AR-1254-3

R.T.: 6.397 min
Delta R.T.: -0.013 min
Response: 1106699
Conc: 4.48 ng/ml

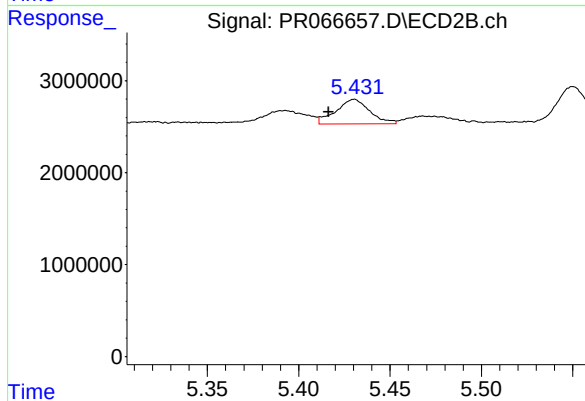

#28 AR-1254-3


R.T.: 5.430 min
Delta R.T.: 0.014 min
Response: 3413316
Conc: 9.93 ng/ml

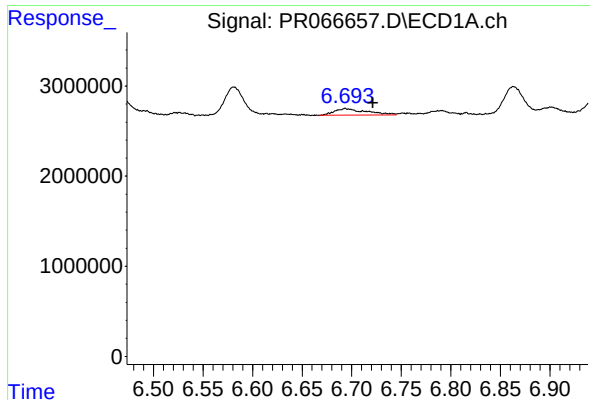

#29 AR-1254-4


R.T.: 6.694 min
Delta R.T.: -0.027 min
Response: 1664377
Conc: 10.48 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

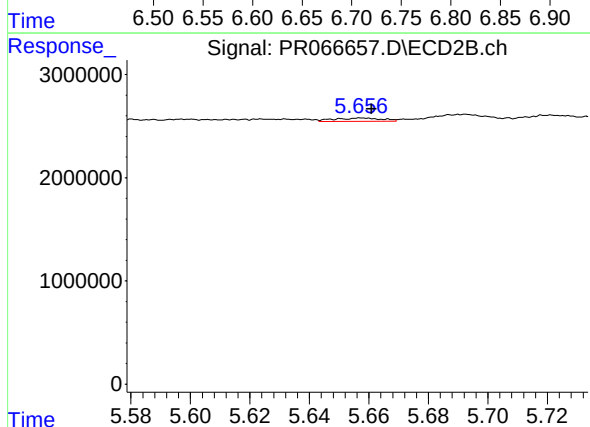


#29 AR-1254-4

R.T.: 5.658 min
Delta R.T.: -0.003 min
Response: 358571
Conc: 1.68 ng/ml

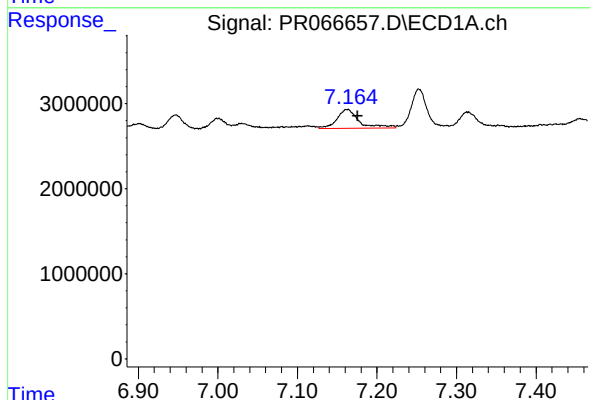


#30 AR-1254-5

R.T.: 7.162 min
Delta R.T.: -0.014 min
Response: 4375503
Conc: 24.55 ng/ml

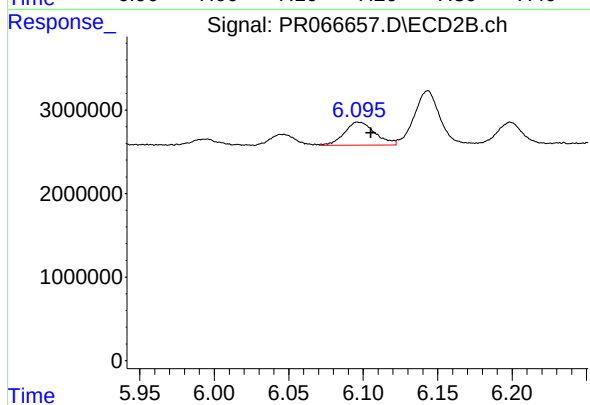

#30 AR-1254-5


R.T.: 6.097 min
Delta R.T.: -0.008 min
Response: 3919509
Conc: 12.18 ng/ml

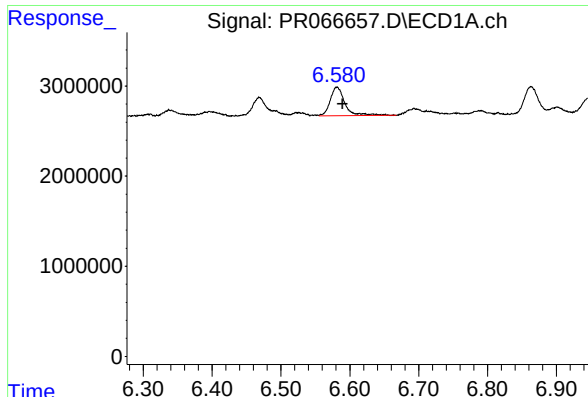

#31 AR-1260-1


R.T.: 6.581 min
Delta R.T.: -0.009 min
Response: 4758043
Conc: 22.90 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

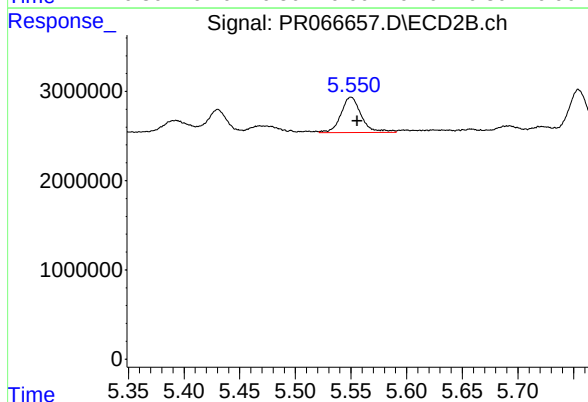


#31 AR-1260-1

R.T.: 5.550 min
Delta R.T.: -0.005 min
Response: 5040009
Conc: 19.89 ng/ml

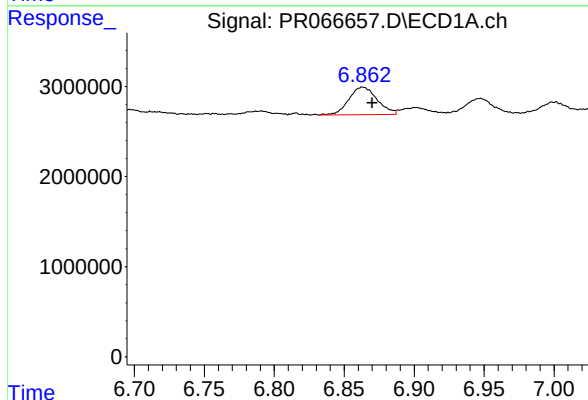


#32 AR-1260-2

R.T.: 6.863 min
Delta R.T.: -0.007 min
Response: 4331256
Conc: 19.52 ng/ml

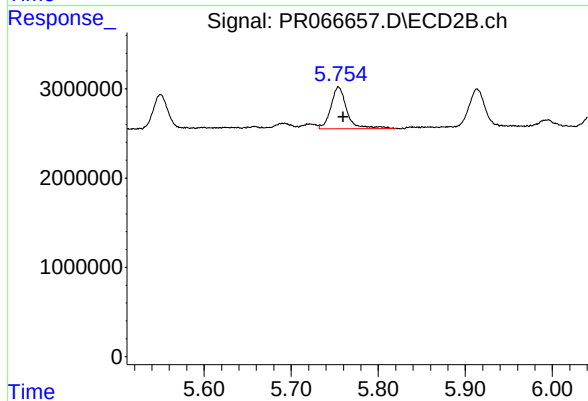

#32 AR-1260-2


R.T.: 5.754 min
Delta R.T.: -0.005 min
Response: 6010462
Conc: 19.74 ng/ml

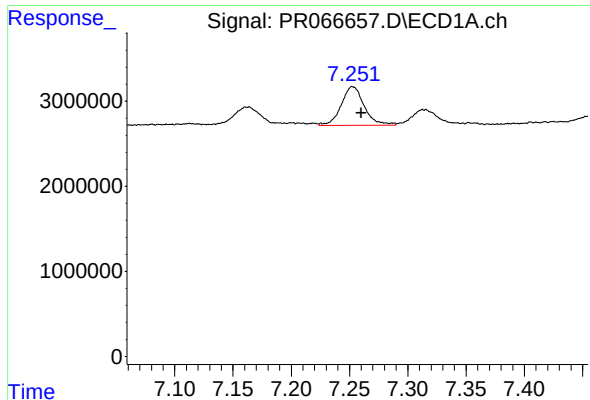

#33 AR-1260-3


R.T.: 7.253 min
Delta R.T.: -0.007 min
Response: 6299522
Conc: 37.56 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

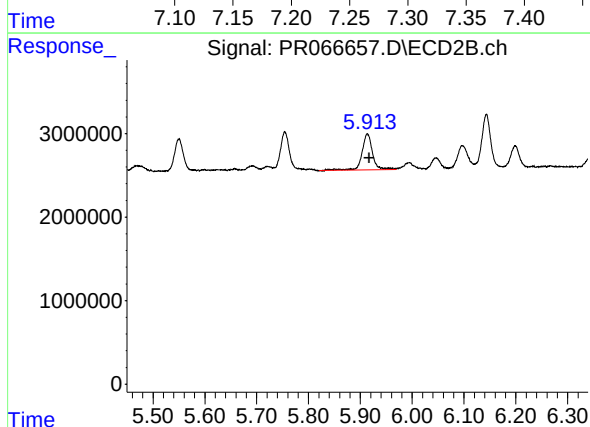


#33 AR-1260-3

R.T.: 5.914 min
Delta R.T.: -0.004 min
Response: 6190351
Conc: 21.26 ng/ml

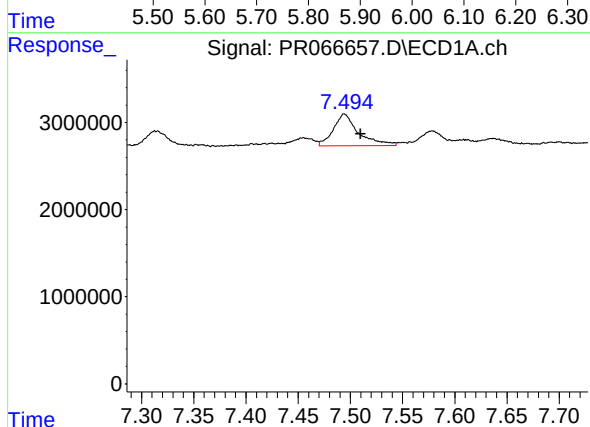


#34 AR-1260-4

R.T.: 7.494 min
Delta R.T.: -0.016 min
Response: 6078223
Conc: 34.11 ng/ml

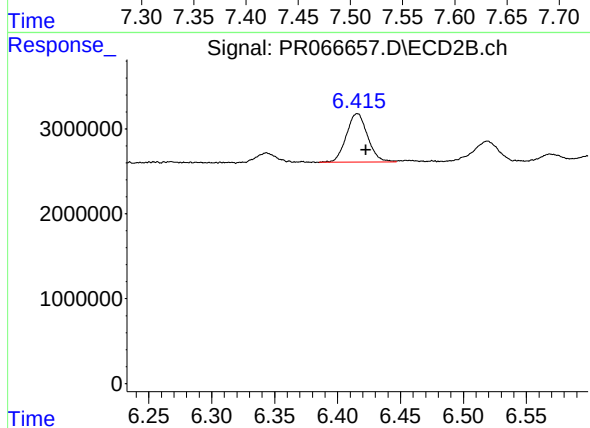

#34 AR-1260-4


R.T.: 6.416 min
Delta R.T.: -0.007 min
Response: 6691216
Conc: 26.80 ng/ml

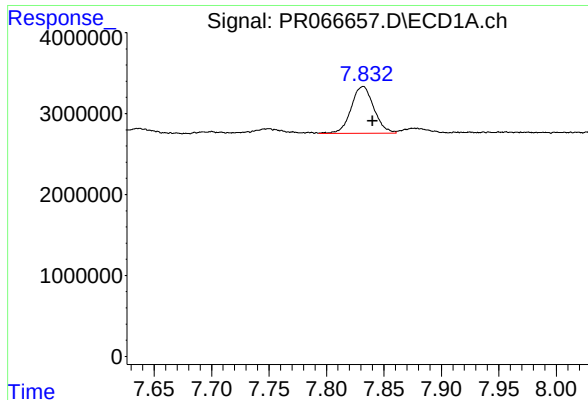

#35 AR-1260-5


R.T.: 7.832 min
Delta R.T.: -0.008 min
Response: 7913752
Conc: 27.10 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

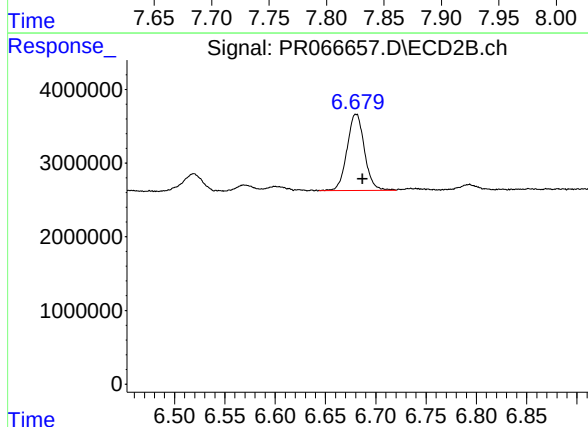


#35 AR-1260-5

R.T.: 6.680 min
Delta R.T.: -0.007 min
Response: 12448193
Conc: 22.17 ng/ml

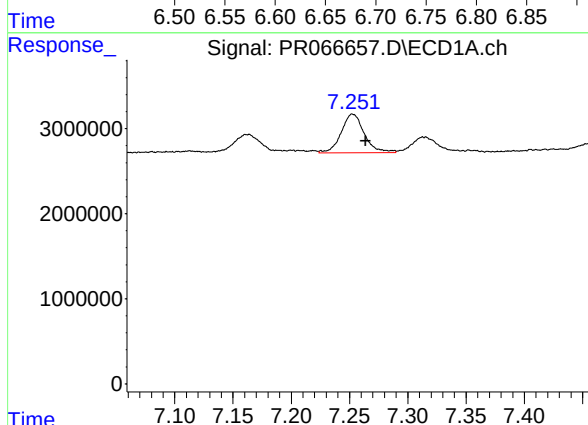


#36 AR-1262-1

R.T.: 7.253 min
Delta R.T.: -0.011 min
Response: 6299522
Conc: 27.61 ng/ml

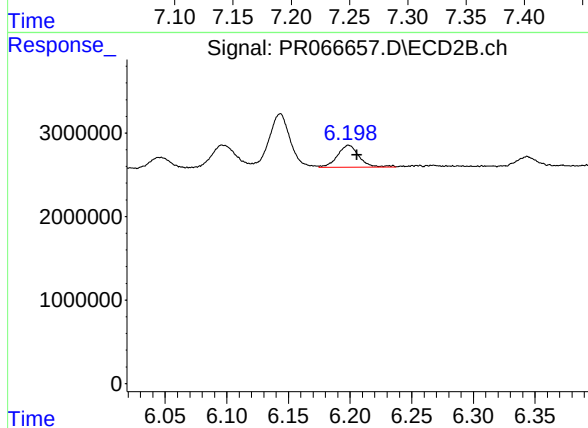

#36 AR-1262-1


R.T.: 6.199 min
Delta R.T.: -0.007 min
Response: 3229371
Conc: 22.35 ng/ml

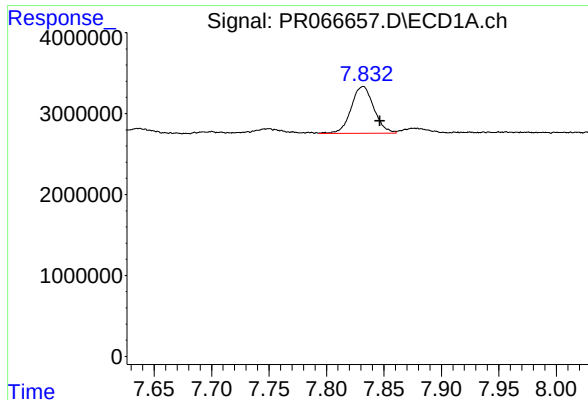

#37 AR-1262-2


R.T.: 7.832 min
Delta R.T.: -0.015 min
Response: 7913752
Conc: 24.92 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

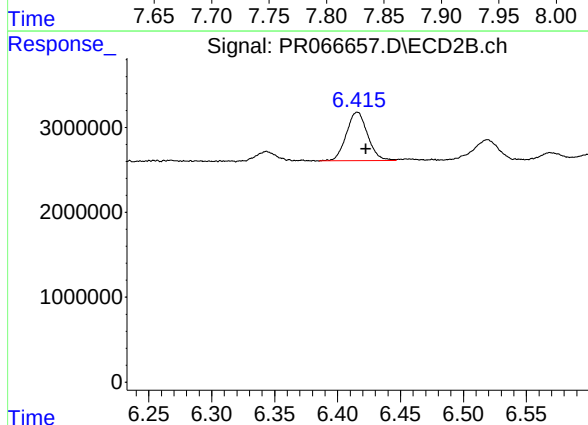


#37 AR-1262-2

R.T.: 6.416 min
Delta R.T.: -0.007 min
Response: 6691216
Conc: 21.75 ng/ml

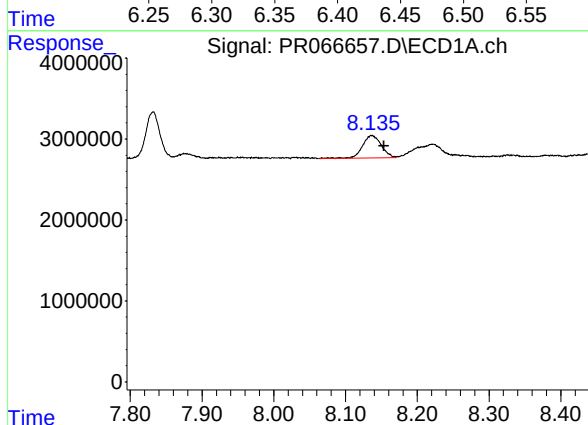


#38 AR-1262-3

R.T.: 8.137 min
Delta R.T.: -0.017 min
Response: 5086117
Conc: 24.02 ng/ml

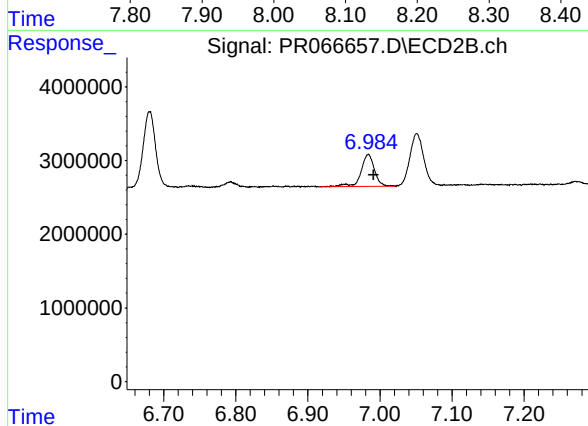

#38 AR-1262-3


R.T.: 6.984 min
Delta R.T.: -0.008 min
Response: 5643107
Conc: 23.28 ng/ml

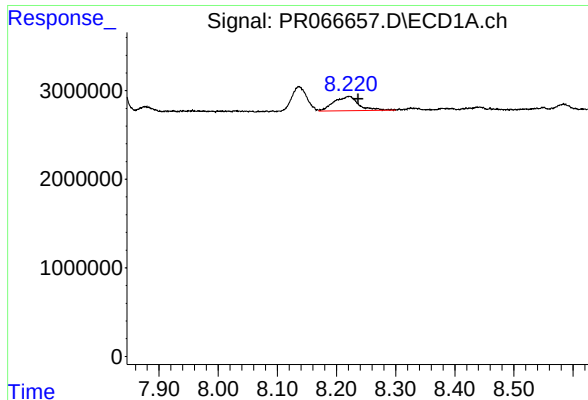

#39 AR-1262-4


R.T.: 8.221 min
Delta R.T.: -0.016 min
Response: 4675786
Conc: 42.81 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

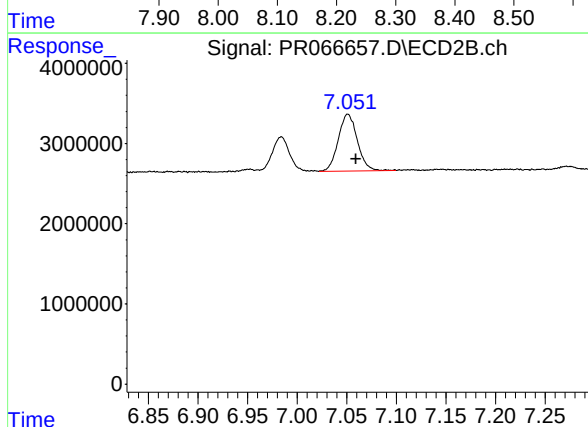


#39 AR-1262-4

R.T.: 7.051 min
Delta R.T.: -0.008 min
Response: 9504222
Conc: 21.63 ng/ml

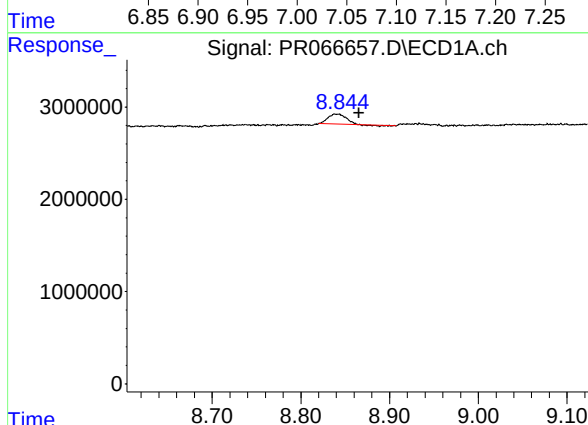


#40 AR-1262-5

R.T.: 8.841 min
Delta R.T.: -0.025 min
Response: 1502551
Conc: 14.78 ng/ml

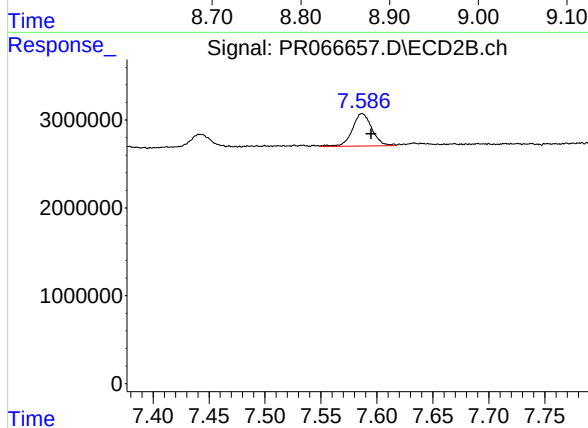

#40 AR-1262-5


R.T.: 7.587 min
Delta R.T.: -0.008 min
Response: 4542709
Conc: 21.04 ng/ml

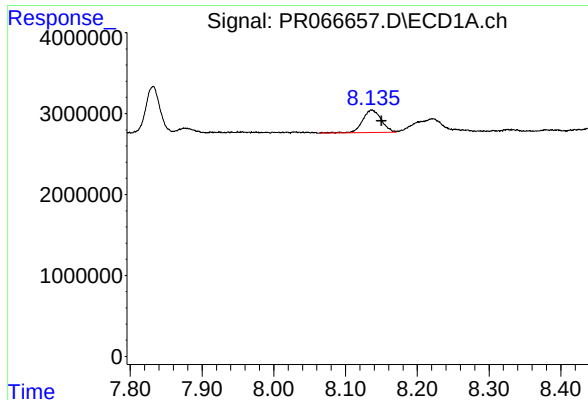

#41 AR-1268-1


R.T.: 8.137 min
Delta R.T.: -0.014 min
Response: 5086117
Conc: 13.05 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

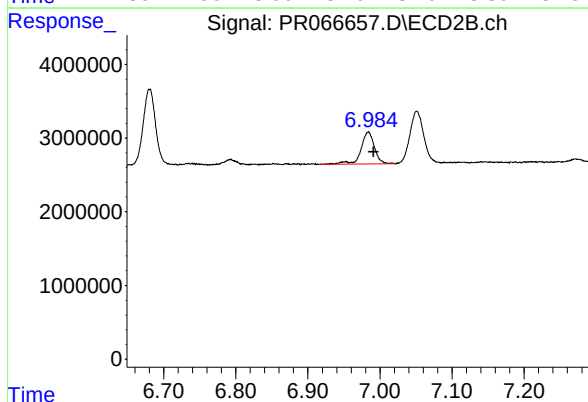


#41 AR-1268-1

R.T.: 6.984 min
Delta R.T.: -0.008 min
Response: 5643107
Conc: 7.79 ng/ml

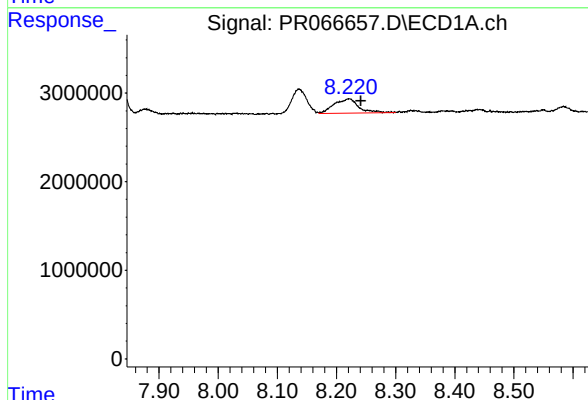


#42 AR-1268-2

R.T.: 8.221 min
Delta R.T.: -0.021 min
Response: 4675786
Conc: 13.61 ng/ml

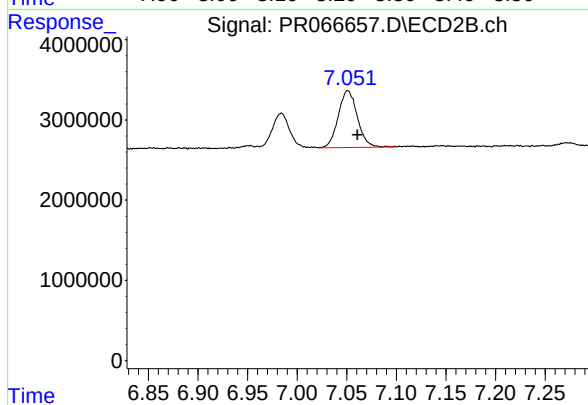

#42 AR-1268-2


R.T.: 7.051 min
Delta R.T.: -0.009 min
Response: 9504222
Conc: 14.81 ng/ml

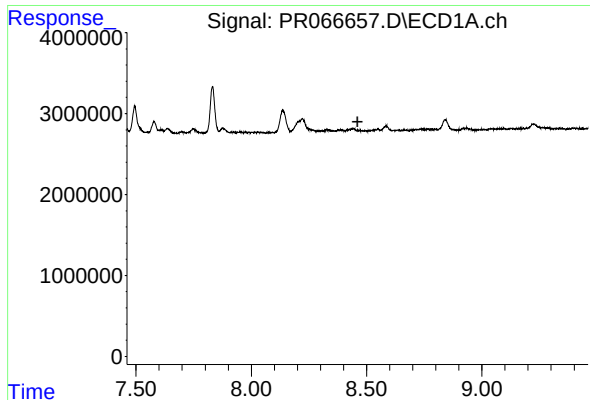

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

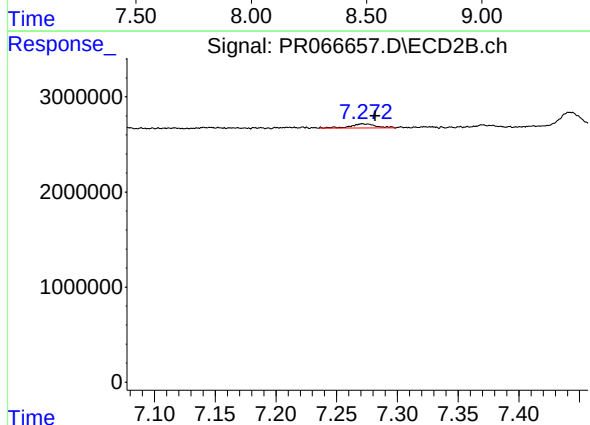


#43 AR-1268-3

R.T.: 7.272 min
Delta R.T.: -0.009 min
Response: 663656
Conc: 1.17 ng/ml

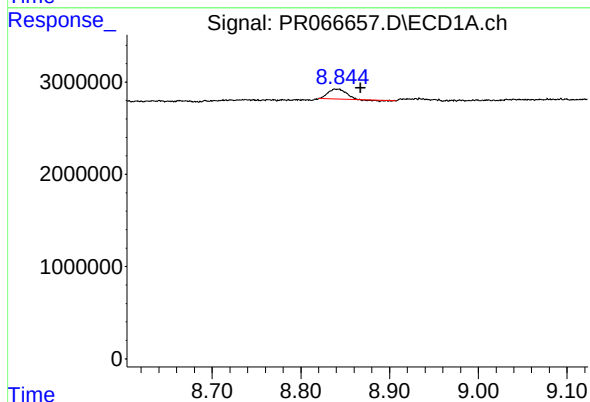


#44 AR-1268-4

R.T.: 8.841 min
Delta R.T.: -0.027 min
Response: 1502551
Conc: 12.93 ng/ml

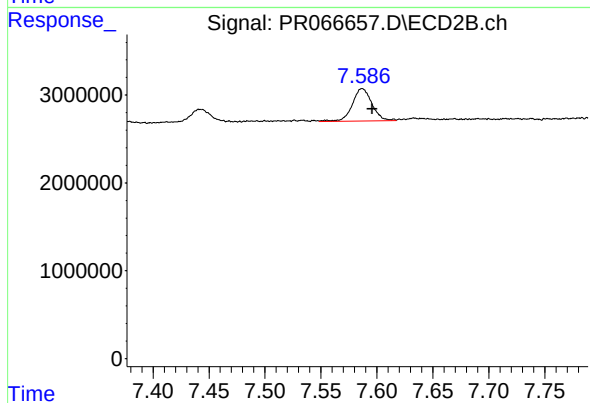

#44 AR-1268-4


R.T.: 7.587 min
Delta R.T.: -0.009 min
Response: 4542709
Conc: 18.61 ng/ml

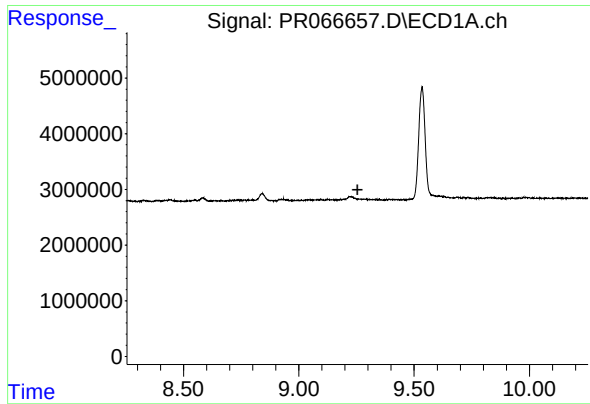

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.254 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

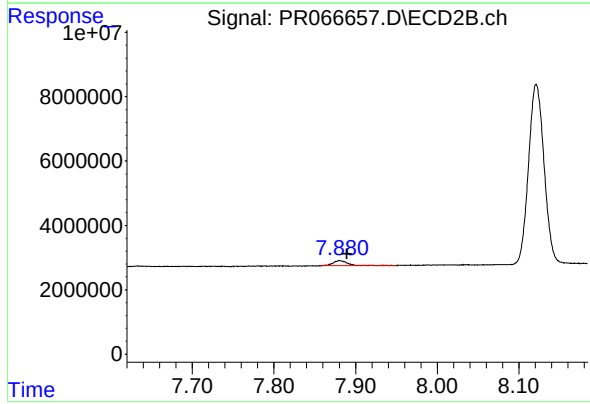

#45 AR-1268-5

R.T.: 7.881 min
Delta R.T.: -0.009 min
Response: 1925341
Conc: 1.19 ng/ml