

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR050924\
 Data File : PR066658.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2024 07:00
 Operator : AJ\MA
 Sample : P2403-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT2-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 07:39:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 26 07:26:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.652	2.892	91566450	70975437	17.470	15.879
2) SA Decachlor...	9.534	8.123	42967398	79967609	18.348	17.037
Target Compounds						
3) L1 AR-1016-1	4.893	4.007	719948	324780	5.037	2.150 #
4) L1 AR-1016-2	4.893	4.007f	719948	324780	3.292	1.514 #
5) L1 AR-1016-3	4.982	0.000	1253069	0	8.628	N.D. #
6) L1 AR-1016-4	0.000	4.240	0	132801	N.D.	1.377 #
7) L1 AR-1016-5	5.379	0.000	290765	0	2.553	N.D. #
8) L2 AR-1221-1	3.858f	3.149f	660344	121017	10.936	2.234 #
9) L2 AR-1221-2	3.963	3.193	1406443	1145595	31.828	27.592
10) L2 AR-1221-3	4.039	3.281	169848	199556	1.308	1.652 #
11) L3 AR-1232-1	4.039	3.281	169848	199556	1.595	1.988
12) L3 AR-1232-2	4.616f	4.007f	115159	324780	1.877	3.263 #
13) L3 AR-1232-3	4.893	0.000	719948	0	7.044	N.D. #
14) L3 AR-1232-4	0.000	4.287	0	247897	N.D.	5.111 #
15) L3 AR-1232-5	5.170	0.000	441452	0	10.972	N.D. #
16) L4 AR-1242-1	4.893	4.007	719948	324780	6.049	2.595 #
17) L4 AR-1242-2	4.893	4.007f	719948	324780	4.006	1.832 #
18) L4 AR-1242-3	4.982	0.000	1253069	0	10.519	N.D. #
19) L4 AR-1242-4	0.000	4.287	0	247897	N.D.	2.597 #
20) L4 AR-1242-5	5.844	4.866f	162709	410992	1.809	3.346 #
21) L5 AR-1248-1	4.893	4.007	719948	324780	8.318	3.493 #
22) L5 AR-1248-2	5.170	4.240	441452	132801	3.317	0.981 #
23) L5 AR-1248-3	5.379	4.287	290765	247897	1.937	1.800
24) L5 AR-1248-4	5.844f	0.000	162709	0	1.142	N.D. #
25) L5 AR-1248-5	5.844	4.866	162709	410992	1.136	2.547 #
26) L6 AR-1254-1	5.779	4.866f	1061431	410992	6.387	1.672 #
27) L6 AR-1254-2	6.015	4.985	502742	198229	2.052	0.905 #
28) L6 AR-1254-3	6.394f	5.434f	1608252	142088	6.506	0.413 #
29) L6 AR-1254-4	6.695f	5.673	1828335	82481	11.516	0.386 #
30) L6 AR-1254-5	7.155f	6.109	978437	92562	5.490	0.288 #
31) L7 AR-1260-1	6.569f	5.546	686206	164036	3.302	0.647 #
32) L7 AR-1260-2	6.899f	0.000	646048	0	2.912	N.D. #
33) L7 AR-1260-3	7.253	5.921	3050663	947674	18.191	3.255 #
34) L7 AR-1260-4	7.518	6.414	3681154	3748729	20.660	15.013 #
35) L7 AR-1260-5	7.831	6.681	1037248	1624408	3.552	2.893
36) L8 AR-1262-1	7.253	6.199	3050663	641048	13.373	4.437 #
37) L8 AR-1262-2	7.831	6.414	1037248	3748729	3.266	12.183 #
38) L8 AR-1262-3	8.134f	6.984	9399272	15068234	44.396	62.164 #
39) L8 AR-1262-4	8.225	7.053	8540680	13294391	78.187	30.251 #
40) L8 AR-1262-5	8.842f	7.588	1995387	5140683	19.631	23.811
41) L9 AR-1268-1	8.134f	6.984	9399272	15068234	24.109	20.811

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR050924\
 Data File : PR066658.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2024 07:00
 Operator : AJ\MA
 Sample : P2403-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT2-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 07:39:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 26 07:26:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.225f	7.053	8540680	13294391	24.858	20.714
43) L9	AR-1268-3	8.440f	7.273	3484318	12018048	11.350	21.190 #
44) L9	AR-1268-4	8.842f	7.588	1995387	5140683	17.172	21.064
45) L9	AR-1268-5	9.225f	7.882	12109150	34268967	14.850	21.148 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR050924\
Data File : PR066658.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2024 07:00
Operator : AJ\MA
Sample : P2403-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 73 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 07:39:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR042424.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 26 07:26:35 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

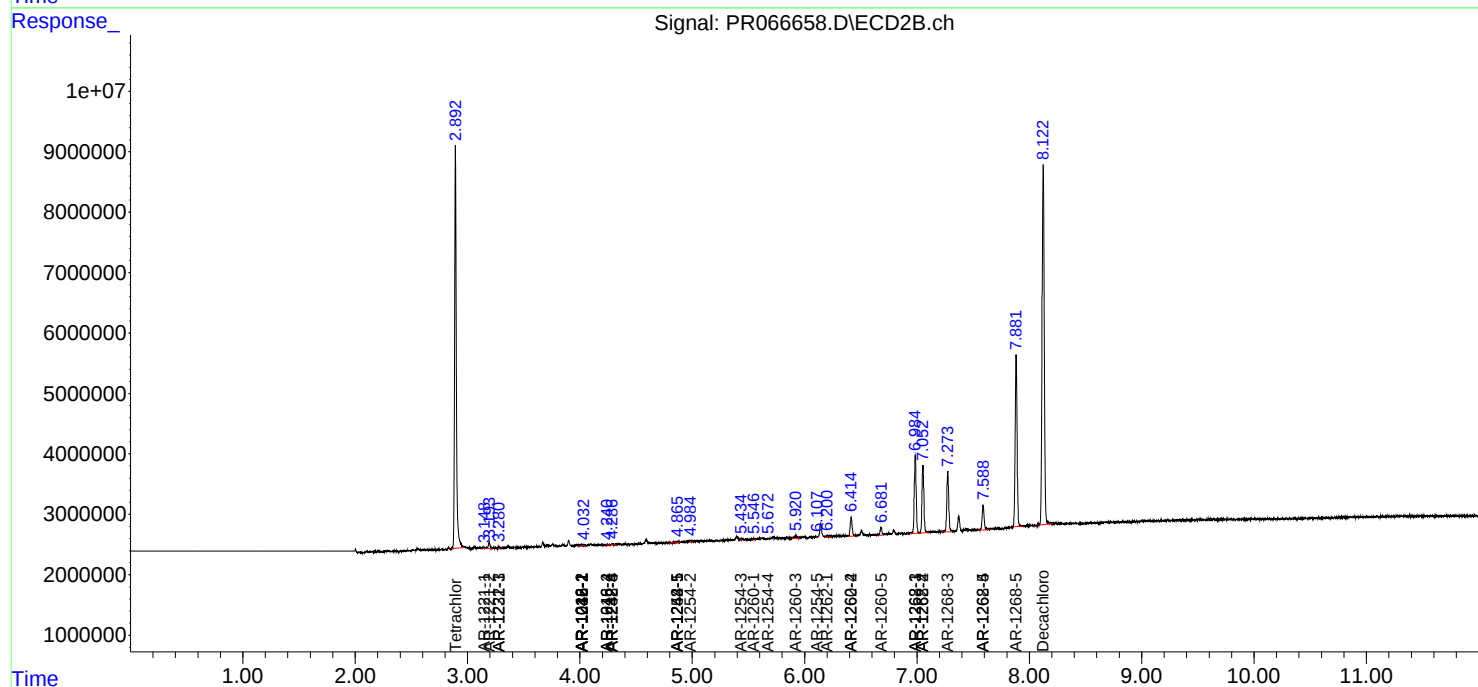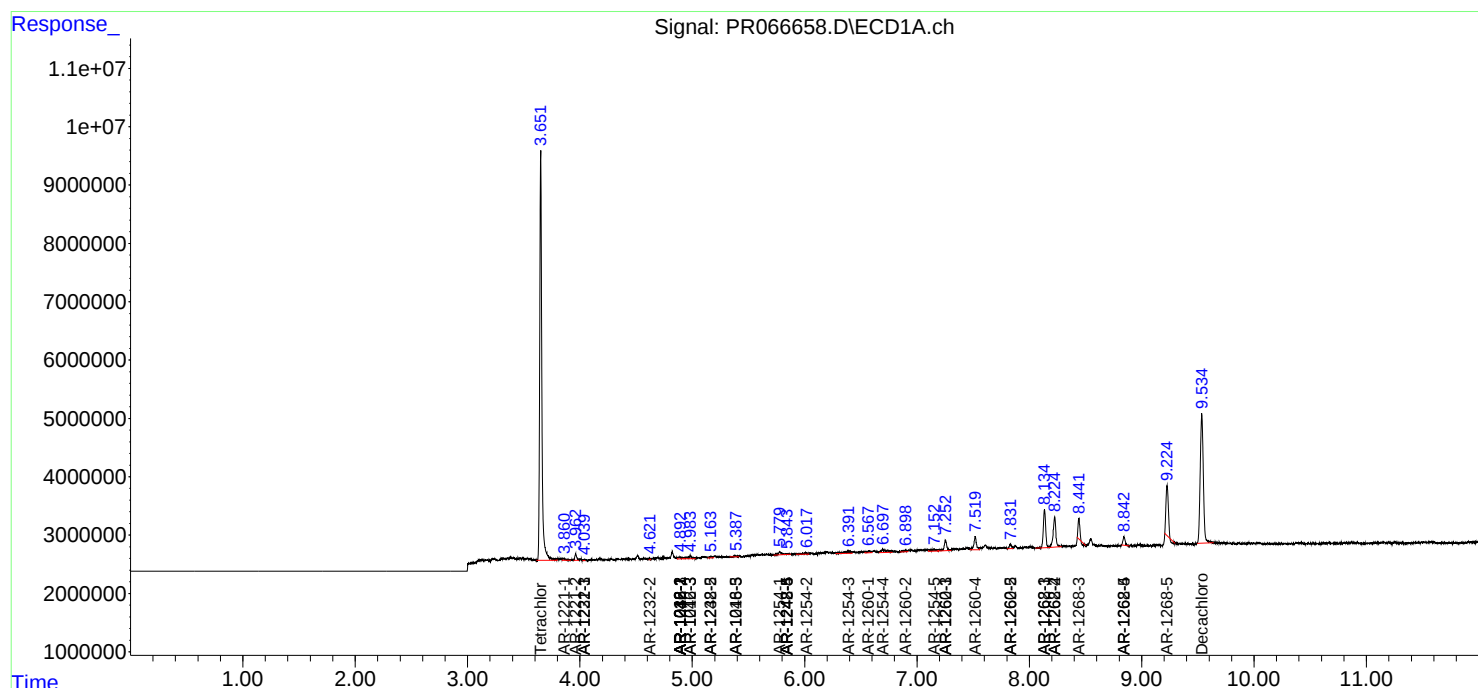


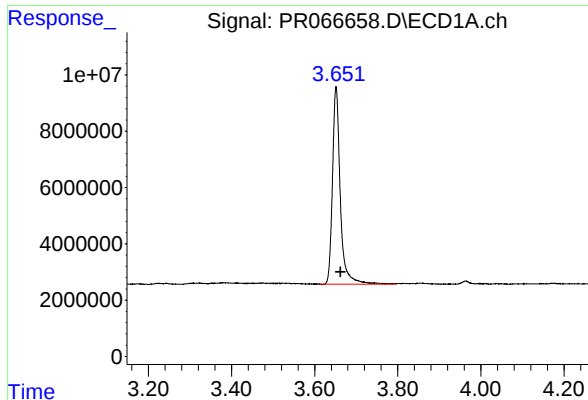

#1 Tetrachloro-m-xylene


R.T.: 3.652 min
Delta R.T.: -0.010 min
Response: 91566450
Conc: 17.47 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

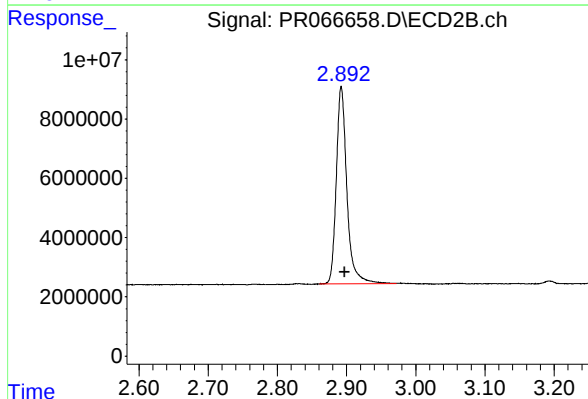


#1 Tetrachloro-m-xylene

R.T.: 2.892 min
Delta R.T.: -0.005 min
Response: 70975437
Conc: 15.88 ng/ml

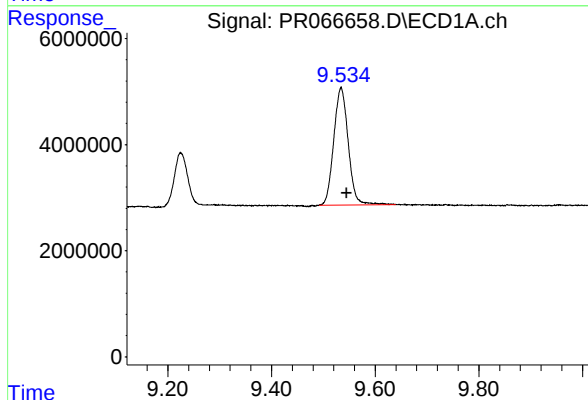


#2 Decachlorobiphenyl

R.T.: 9.534 min
Delta R.T.: -0.011 min
Response: 42967398
Conc: 18.35 ng/ml

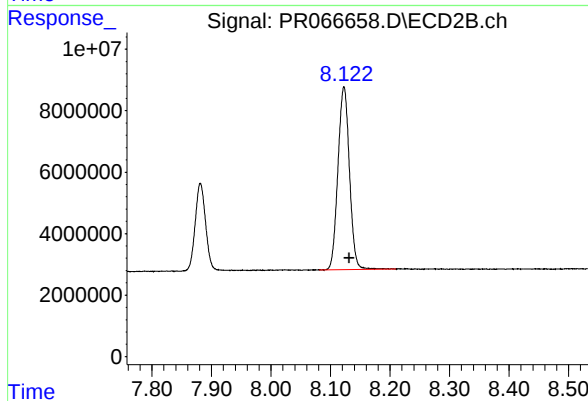

#2 Decachlorobiphenyl


R.T.: 8.123 min
Delta R.T.: -0.009 min
Response: 79967609
Conc: 17.04 ng/ml

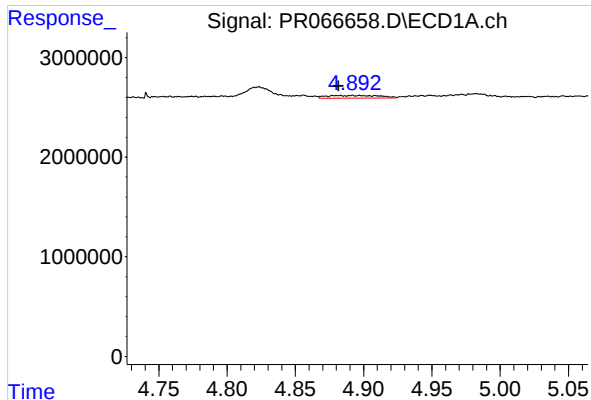

#3 AR-1016-1


R.T.: 4.893 min
Delta R.T.: 0.011 min
Response: 719948
Conc: 5.04 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

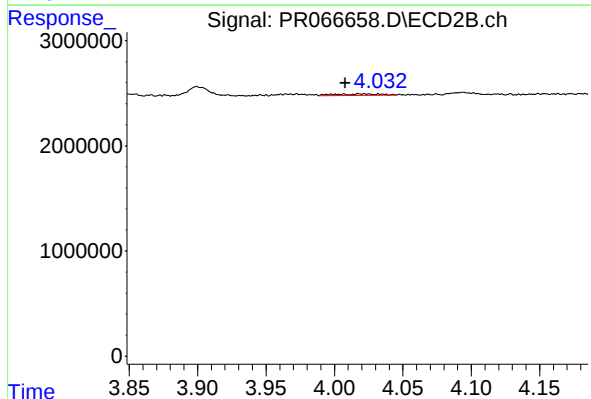


#3 AR-1016-1

R.T.: 4.007 min
Delta R.T.: -0.001 min
Response: 324780
Conc: 2.15 ng/ml

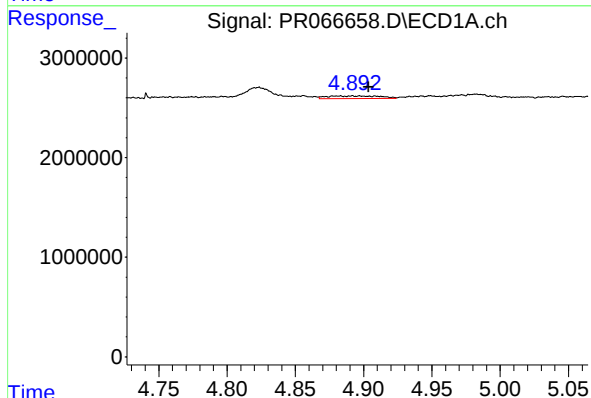


#4 AR-1016-2

R.T.: 4.893 min
Delta R.T.: -0.011 min
Response: 719948
Conc: 3.29 ng/ml

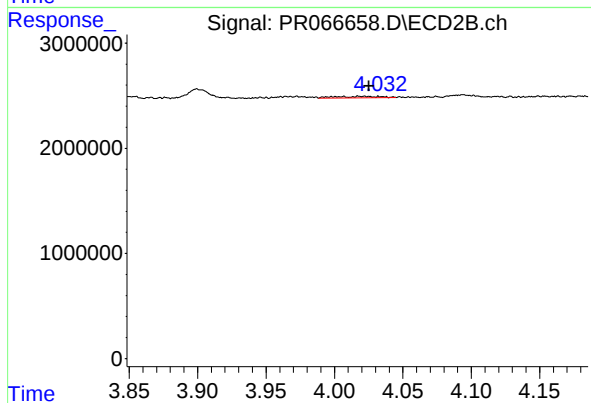

#4 AR-1016-2


R.T.: 4.007 min
Delta R.T.: -0.018 min
Response: 324780
Conc: 1.51 ng/ml

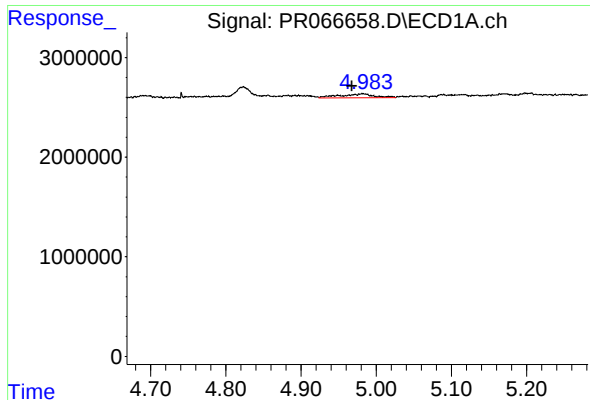

#5 AR-1016-3


R.T.: 4.982 min
Delta R.T.: 0.015 min
Response: 1253069
Conc: 8.63 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

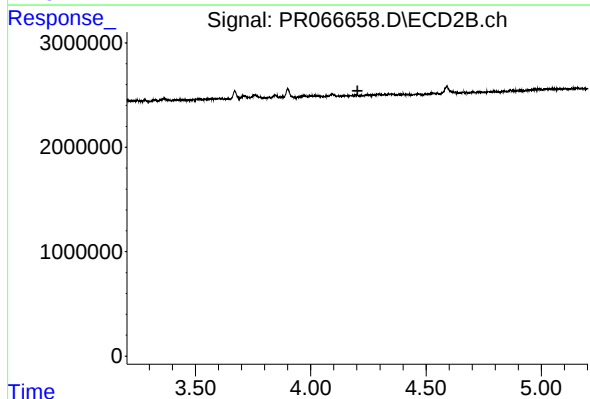


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.203 min
Response: 0
Conc: N.D.

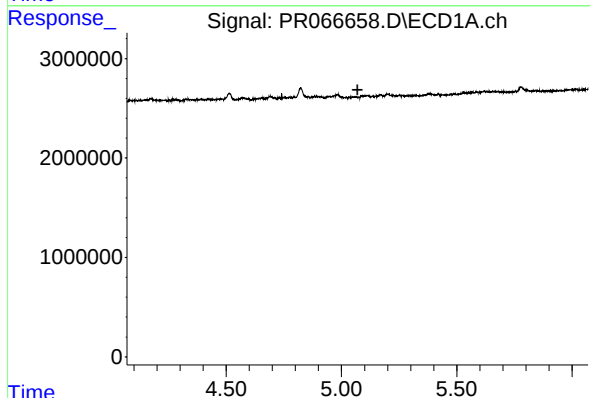


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 5.069 min
Response: 0
Conc: N.D.

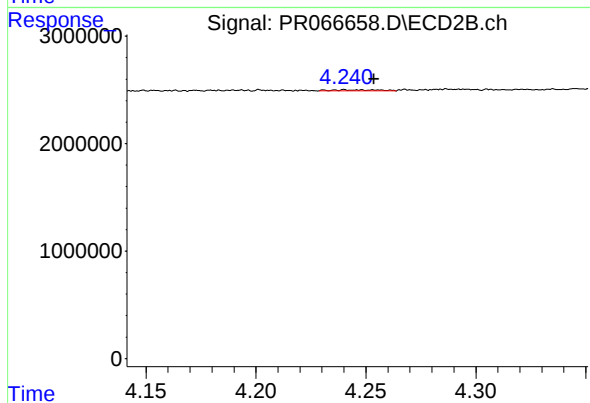

#6 AR-1016-4


R.T.: 4.240 min
Delta R.T.: -0.013 min
Response: 132801
Conc: 1.38 ng/ml

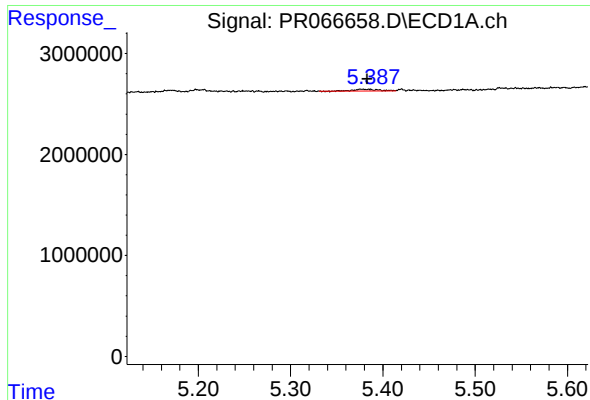

#7 AR-1016-5


R.T.: 5.379 min
Delta R.T.: -0.005 min
Response: 290765
Conc: 2.55 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

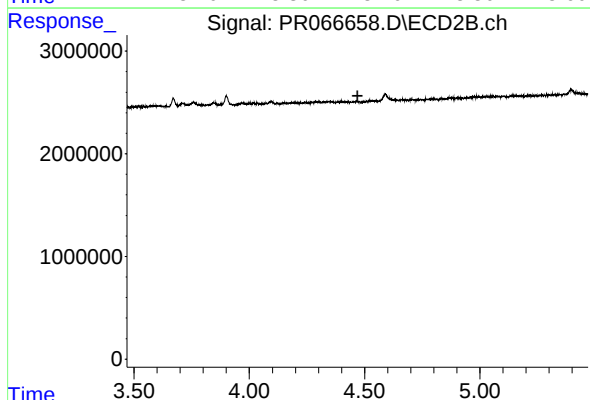


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T.: 4.469 min
Response: 0
Conc: N.D.

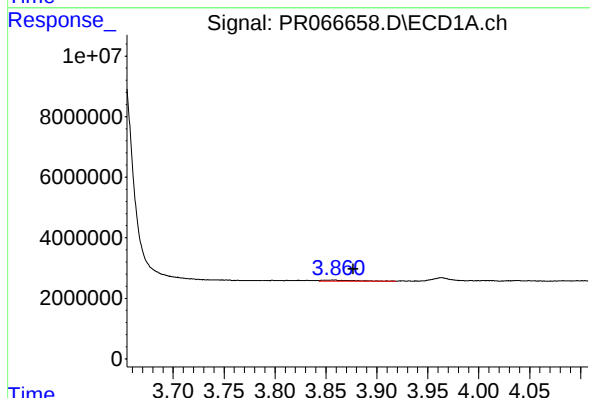


#8 AR-1221-1

R.T.: 3.858 min
Delta R.T.: -0.019 min
Response: 660344
Conc: 10.94 ng/ml

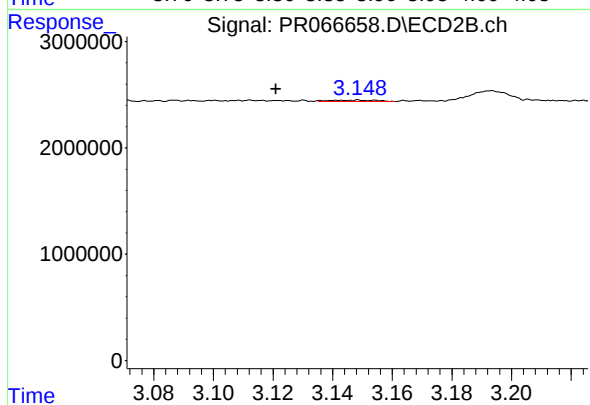

#8 AR-1221-1


R.T.: 3.149 min
Delta R.T.: 0.028 min
Response: 121017
Conc: 2.23 ng/ml

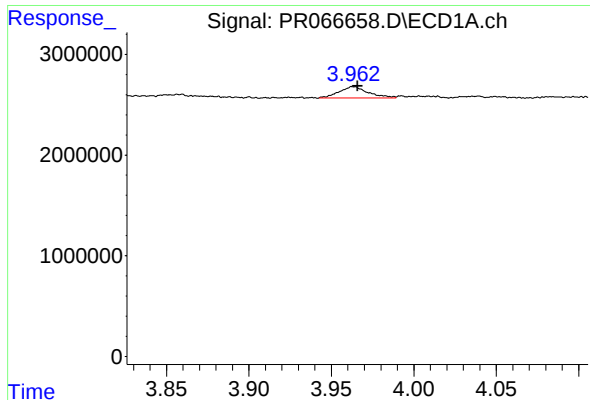

#9 AR-1221-2


R.T.: 3.963 min
Delta R.T.: -0.003 min
Response: 1406443
Conc: 31.83 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

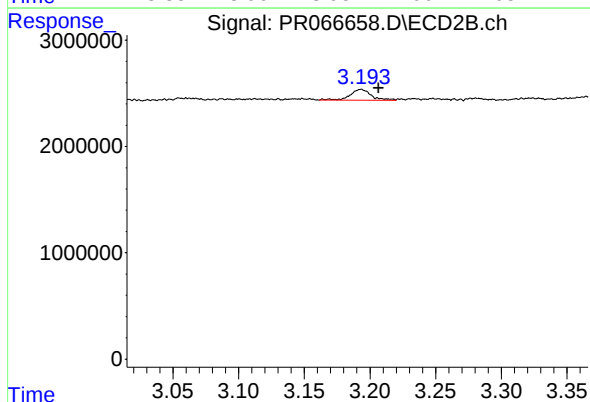


#9 AR-1221-2

R.T.: 3.193 min
Delta R.T.: -0.013 min
Response: 1145595
Conc: 27.59 ng/ml

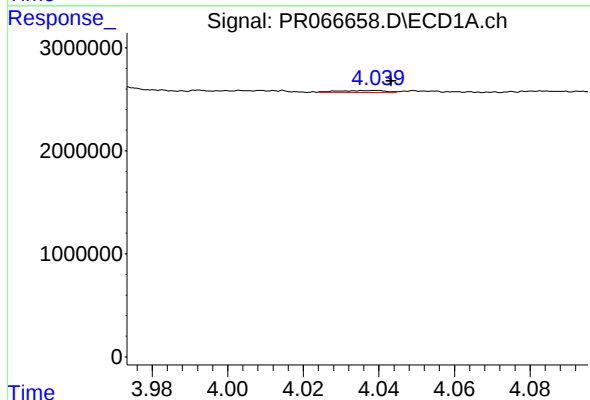


#10 AR-1221-3

R.T.: 4.039 min
Delta R.T.: -0.004 min
Response: 169848
Conc: 1.31 ng/ml

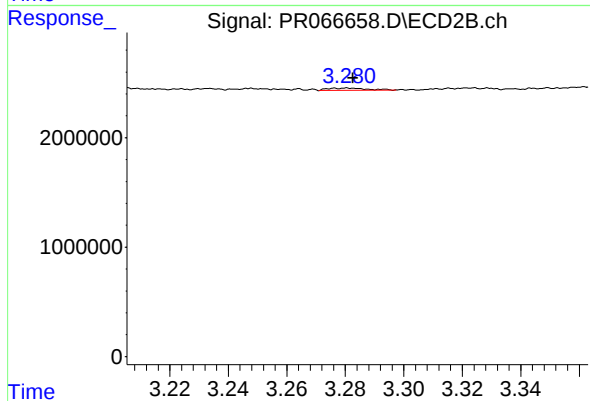

#10 AR-1221-3


R.T.: 3.281 min
Delta R.T.: -0.002 min
Response: 199556
Conc: 1.65 ng/ml

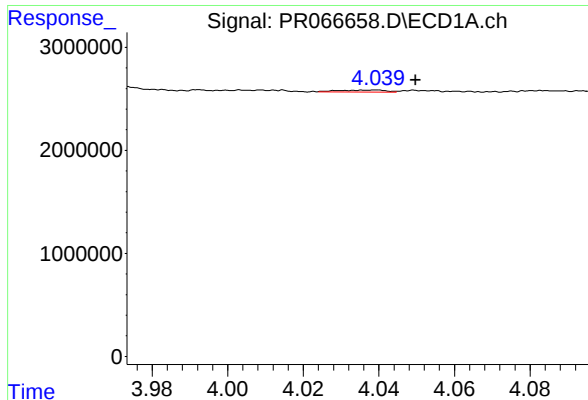

#11 AR-1232-1


R.T.: 4.039 min
Delta R.T.: -0.011 min
Response: 169848
Conc: 1.60 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

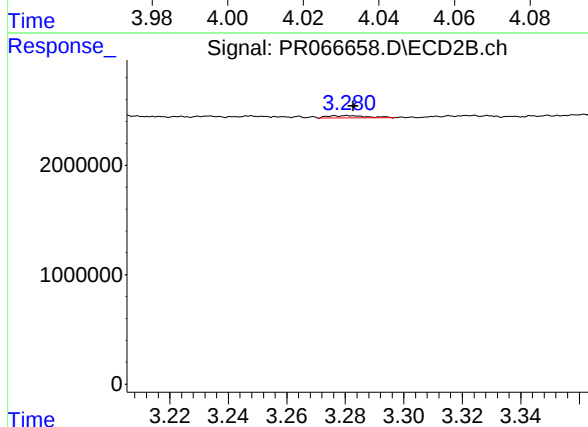


#11 AR-1232-1

R.T.: 3.281 min
Delta R.T.: -0.002 min
Response: 199556
Conc: 1.99 ng/ml

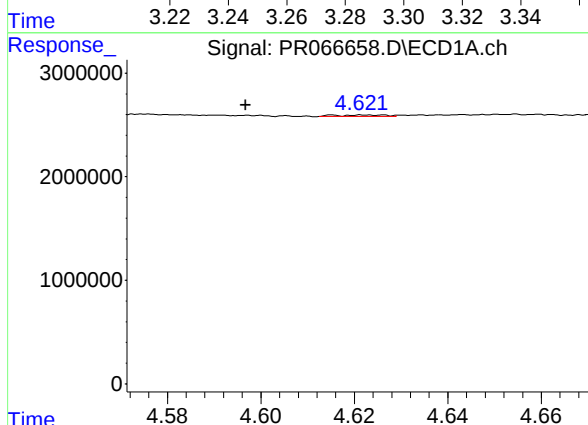


#12 AR-1232-2

R.T.: 4.616 min
Delta R.T.: 0.019 min
Response: 115159
Conc: 1.88 ng/ml

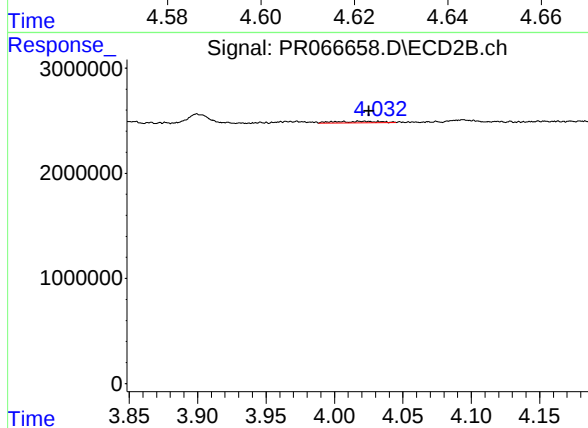

#12 AR-1232-2


R.T.: 4.007 min
Delta R.T.: -0.018 min
Response: 324780
Conc: 3.26 ng/ml

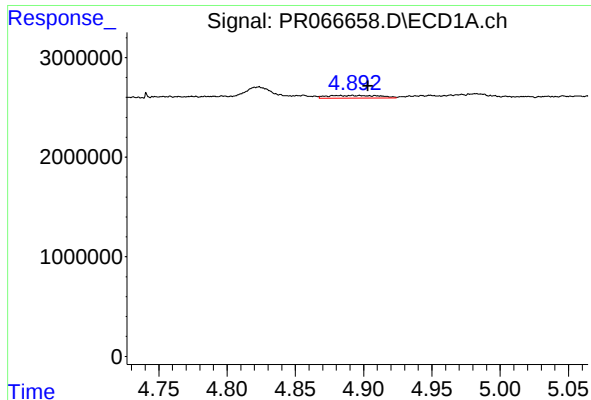

#13 AR-1232-3


R.T.: 4.893 min
Delta R.T.: -0.010 min
Response: 719948
Conc: 7.04 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

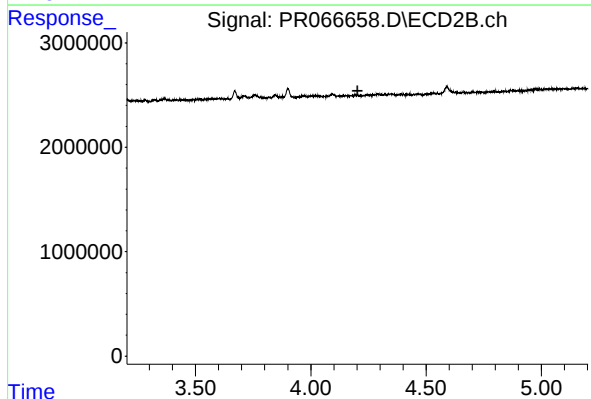


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 4.203 min
Response: 0
Conc: N.D.

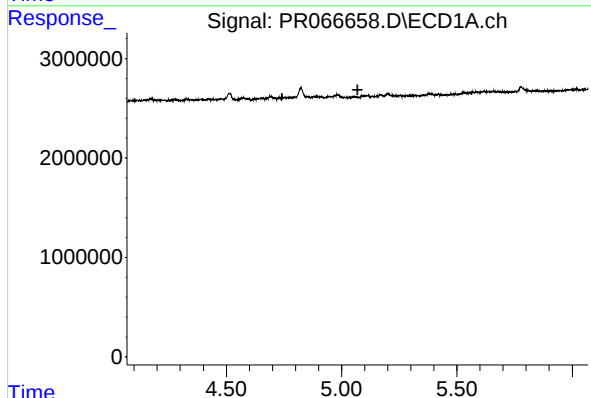


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.069 min
Response: 0
Conc: N.D.

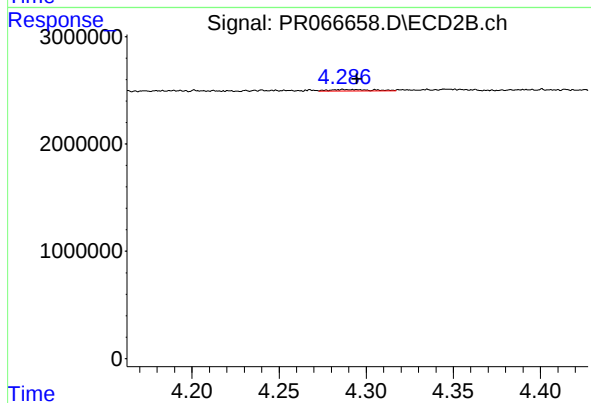

#14 AR-1232-4


R.T.: 4.287 min
Delta R.T.: -0.008 min
Response: 247897
Conc: 5.11 ng/ml

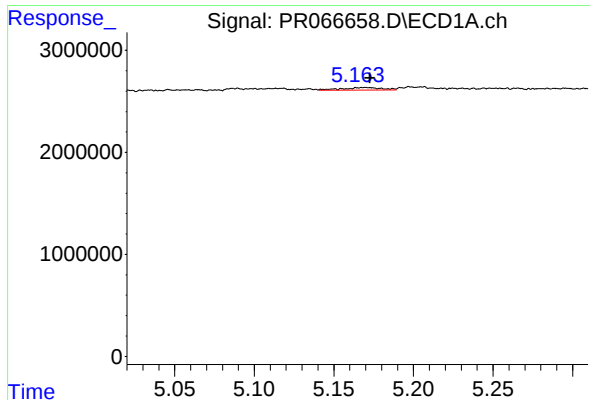

#15 AR-1232-5


R.T.: 5.170 min
Delta R.T.: -0.003 min
Response: 441452
Conc: 10.97 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

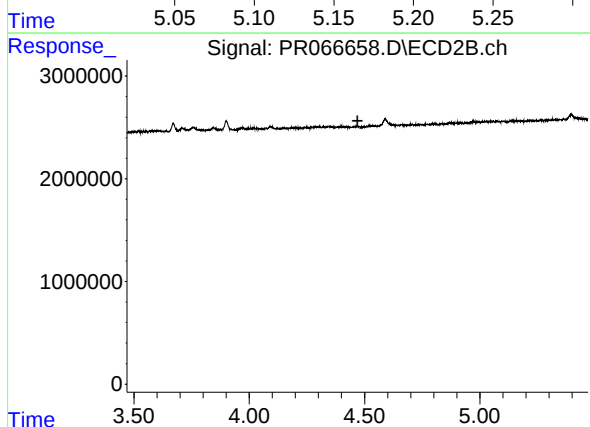


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 4.469 min
Response: 0
Conc: N.D.

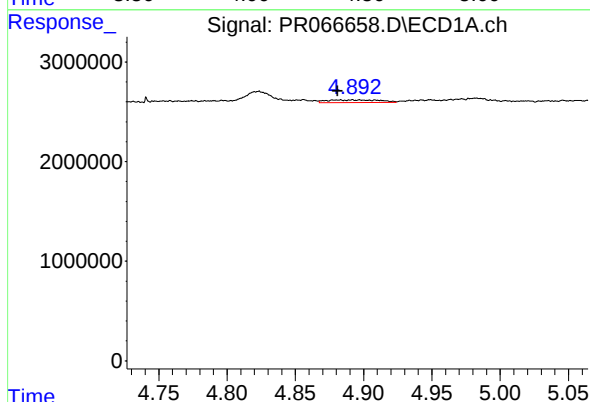


#16 AR-1242-1

R.T.: 4.893 min
Delta R.T.: 0.012 min
Response: 719948
Conc: 6.05 ng/ml

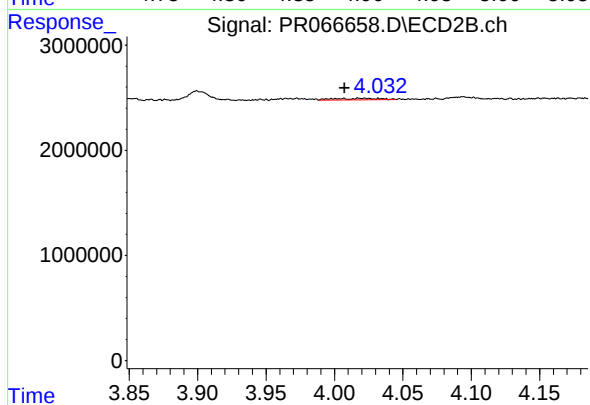

#16 AR-1242-1


R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 324780
Conc: 2.59 ng/ml

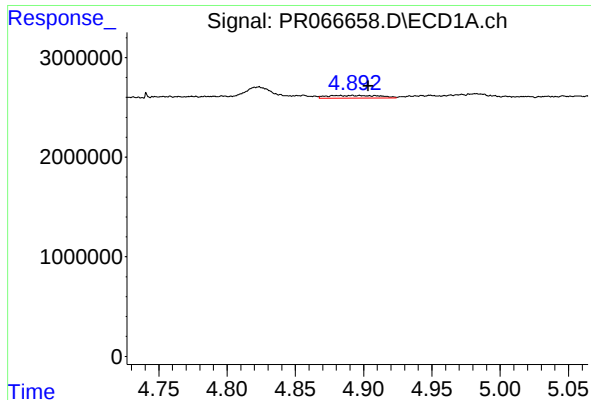

#17 AR-1242-2


R.T.: 4.893 min
Delta R.T.: -0.011 min
Response: 719948
Conc: 4.01 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

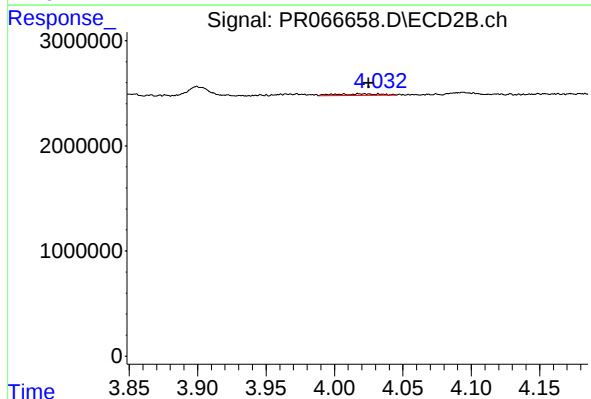


#17 AR-1242-2

R.T.: 4.007 min
Delta R.T.: -0.018 min
Response: 324780
Conc: 1.83 ng/ml

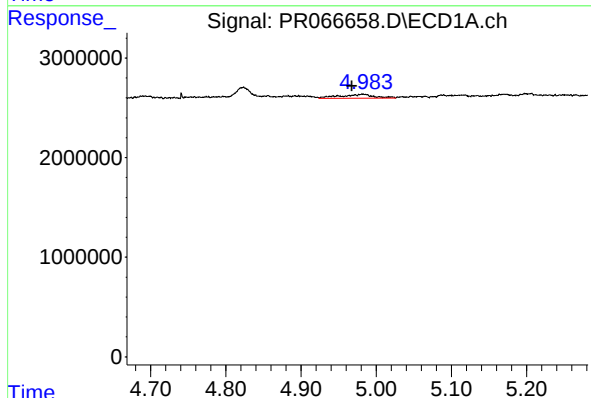


#18 AR-1242-3

R.T.: 4.982 min
Delta R.T.: 0.015 min
Response: 1253069
Conc: 10.52 ng/ml

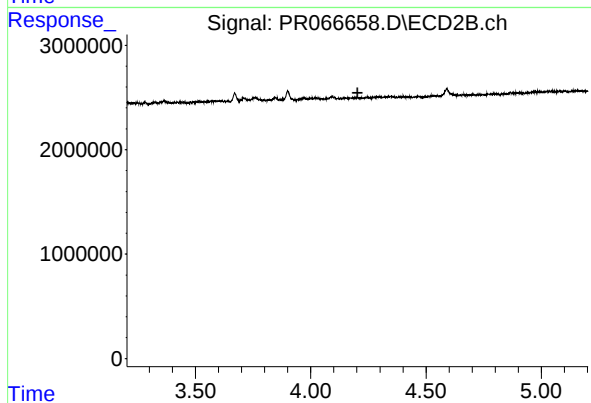

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 4.203 min
Response: 0
Conc: N.D.

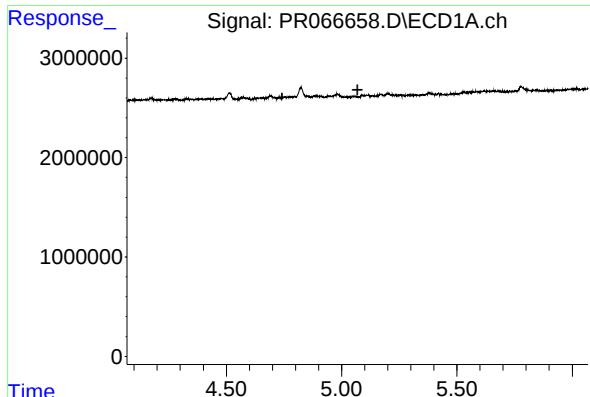

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

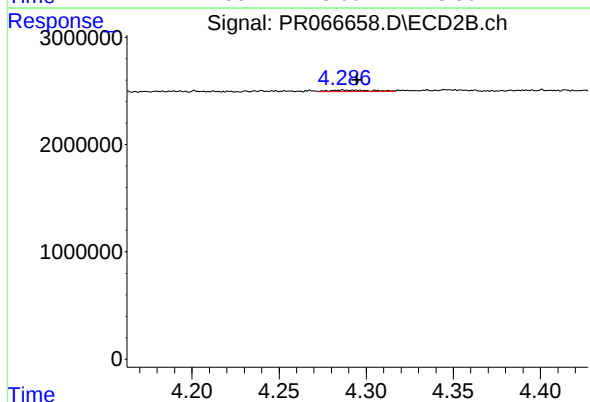


#19 AR-1242-4

R.T.: 4.287 min
Delta R.T.: -0.008 min
Response: 247897
Conc: 2.60 ng/ml

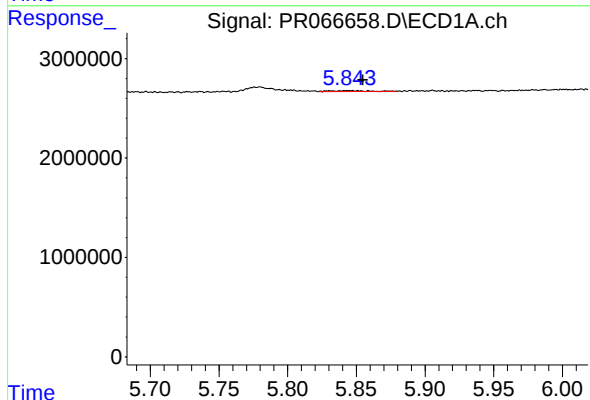


#20 AR-1242-5

R.T.: 5.844 min
Delta R.T.: -0.011 min
Response: 162709
Conc: 1.81 ng/ml

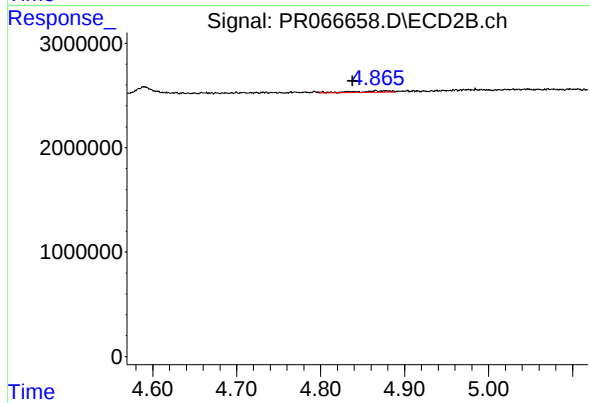

#20 AR-1242-5


R.T.: 4.866 min
Delta R.T.: 0.028 min
Response: 410992
Conc: 3.35 ng/ml

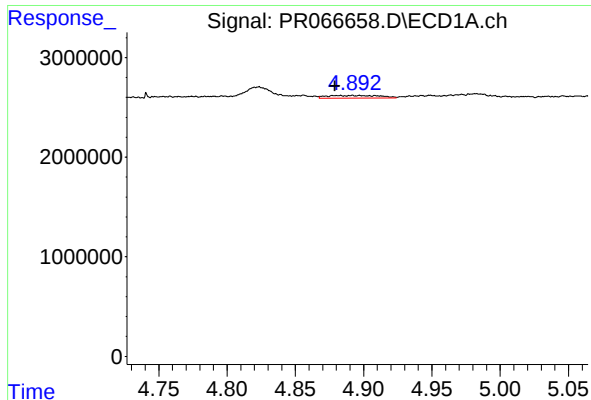

#21 AR-1248-1


R.T.: 4.893 min
Delta R.T.: 0.014 min
Response: 719948
Conc: 8.32 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

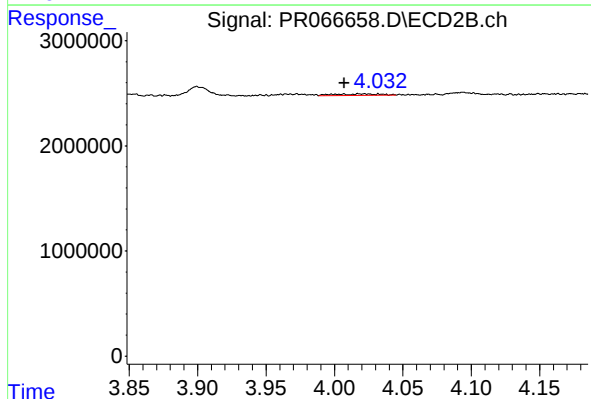


#21 AR-1248-1

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 324780
Conc: 3.49 ng/ml

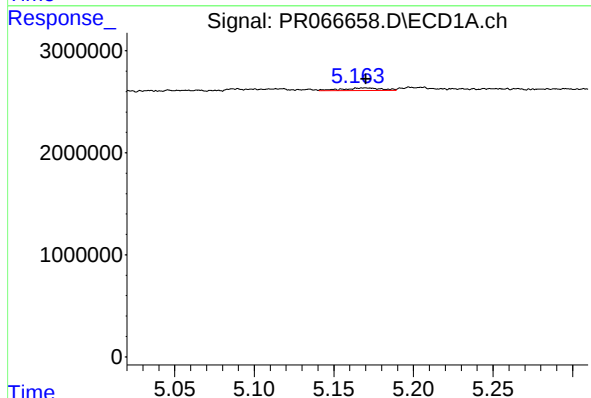


#22 AR-1248-2

R.T.: 5.170 min
Delta R.T.: 0.000 min
Response: 441452
Conc: 3.32 ng/ml

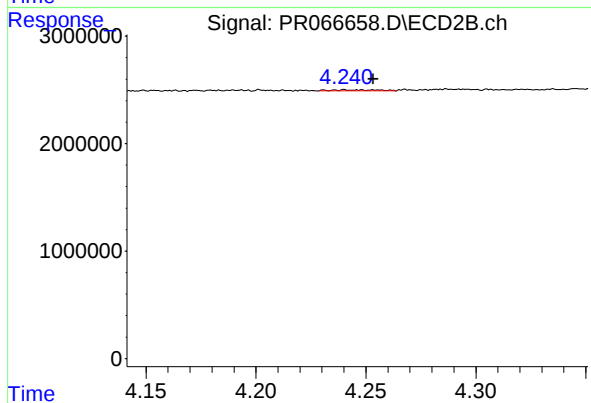

#22 AR-1248-2


R.T.: 4.240 min
Delta R.T.: -0.013 min
Response: 132801
Conc: 0.98 ng/ml

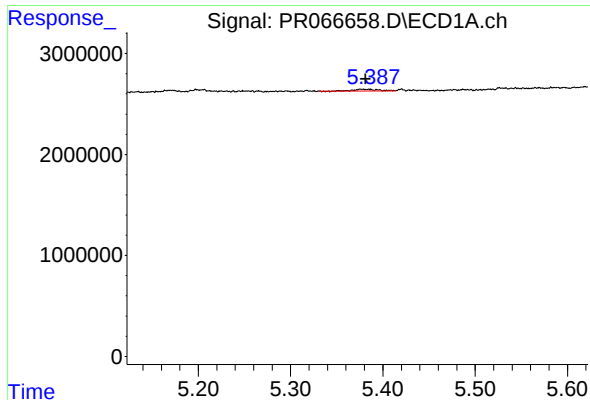

#23 AR-1248-3


R.T.: 5.379 min
Delta R.T.: -0.003 min
Response: 290765
Conc: 1.94 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

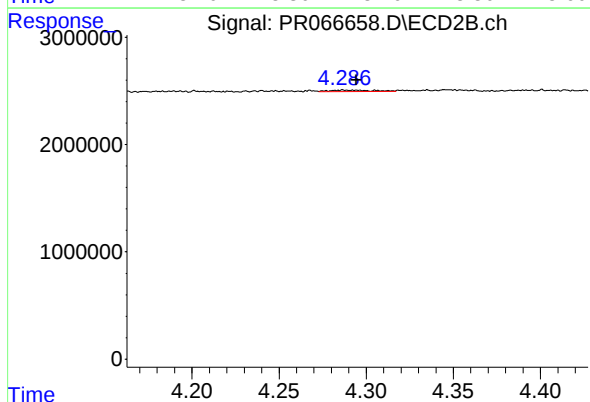


#23 AR-1248-3

R.T.: 4.287 min
Delta R.T.: -0.007 min
Response: 247897
Conc: 1.80 ng/ml

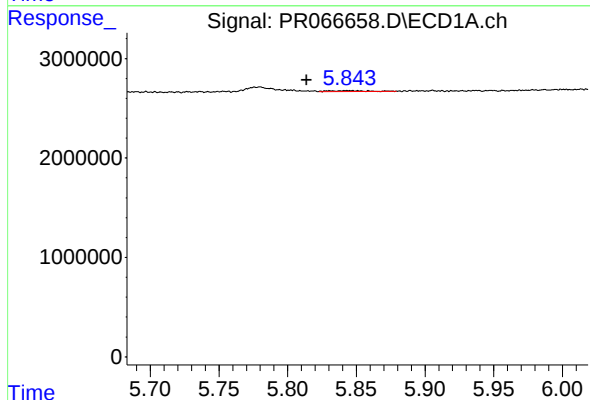


#24 AR-1248-4

R.T.: 5.844 min
Delta R.T.: 0.030 min
Response: 162709
Conc: 1.14 ng/ml

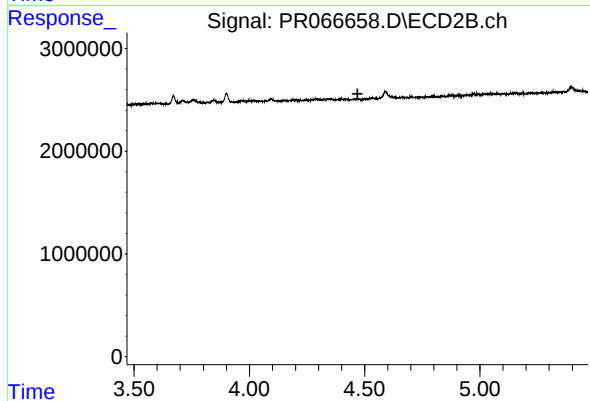

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 4.469 min
Response: 0
Conc: N.D.

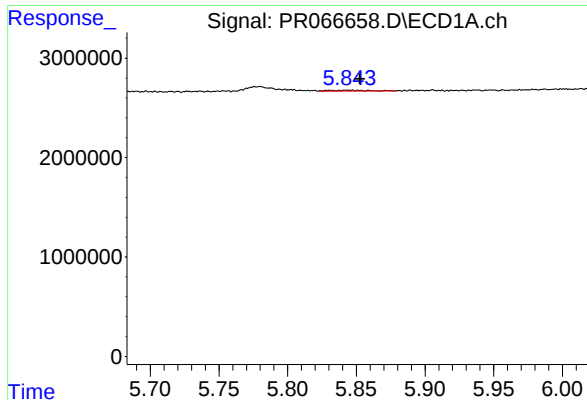

#25 AR-1248-5


R.T.: 5.844 min
Delta R.T.: -0.009 min
Response: 162709
Conc: 1.14 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

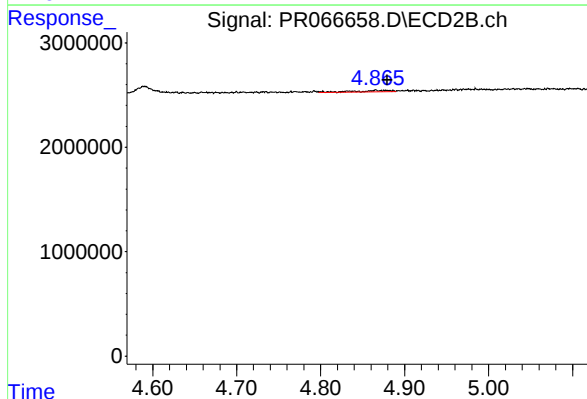


#25 AR-1248-5

R.T.: 4.866 min
Delta R.T.: -0.014 min
Response: 410992
Conc: 2.55 ng/ml

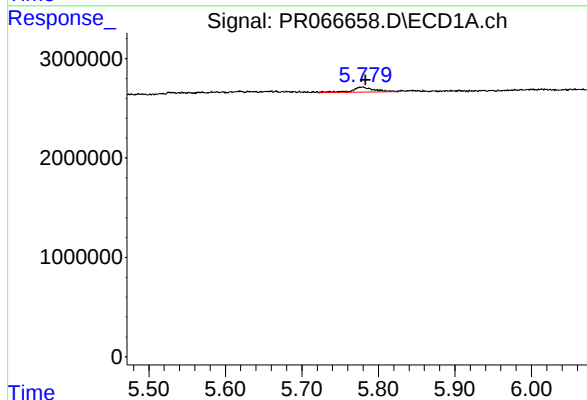


#26 AR-1254-1

R.T.: 5.779 min
Delta R.T.: -0.005 min
Response: 1061431
Conc: 6.39 ng/ml

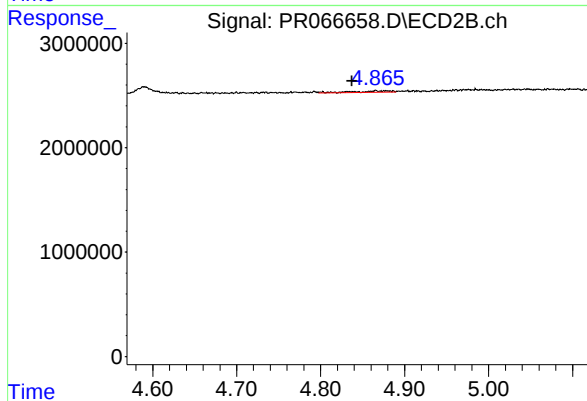

#26 AR-1254-1


R.T.: 4.866 min
Delta R.T.: 0.028 min
Response: 410992
Conc: 1.67 ng/ml

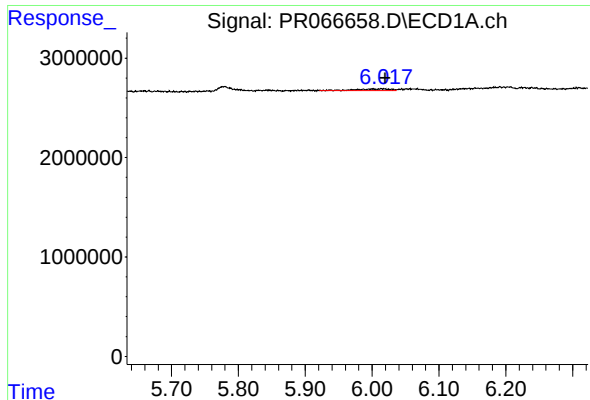

#27 AR-1254-2


R.T.: 6.015 min
Delta R.T.: -0.005 min
Response: 502742
Conc: 2.05 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

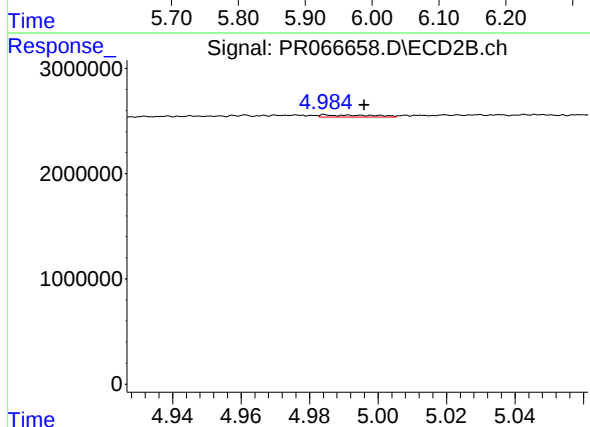


#27 AR-1254-2

R.T.: 4.985 min
Delta R.T.: -0.011 min
Response: 198229
Conc: 0.91 ng/ml

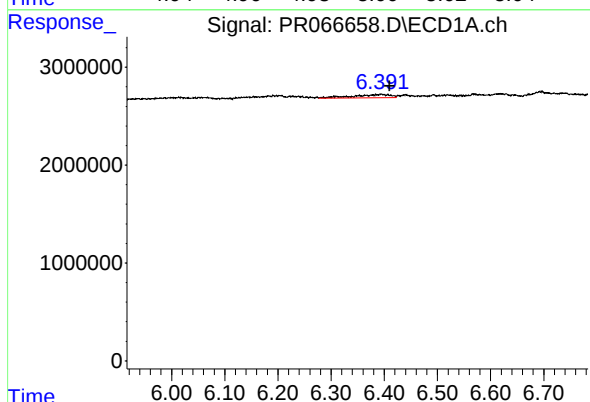


#28 AR-1254-3

R.T.: 6.394 min
Delta R.T.: -0.016 min
Response: 1608252
Conc: 6.51 ng/ml

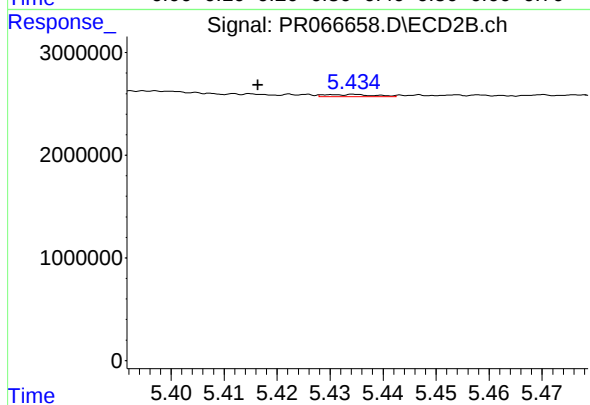

#28 AR-1254-3


R.T.: 5.434 min
Delta R.T.: 0.018 min
Response: 142088
Conc: 0.41 ng/ml

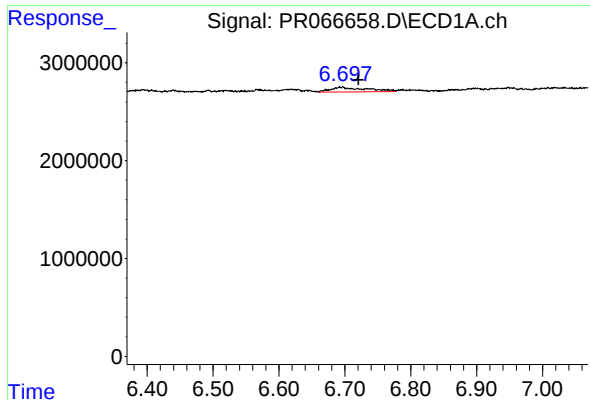

#29 AR-1254-4


R.T.: 6.695 min
Delta R.T.: -0.026 min
Response: 1828335
Conc: 11.52 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

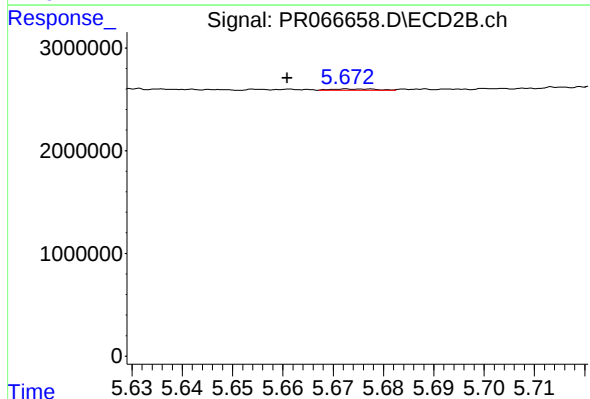


#29 AR-1254-4

R.T.: 5.673 min
Delta R.T.: 0.012 min
Response: 82481
Conc: 0.39 ng/ml

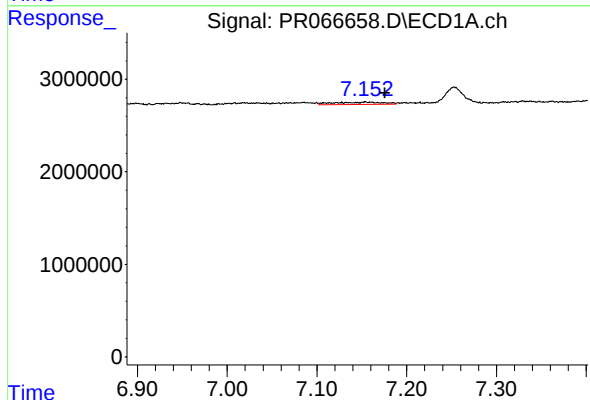


#30 AR-1254-5

R.T.: 7.155 min
Delta R.T.: -0.021 min
Response: 978437
Conc: 5.49 ng/ml

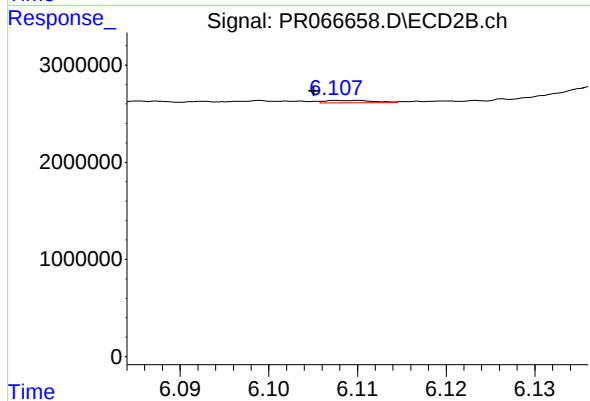

#30 AR-1254-5


R.T.: 6.109 min
Delta R.T.: 0.004 min
Response: 92562
Conc: 0.29 ng/ml

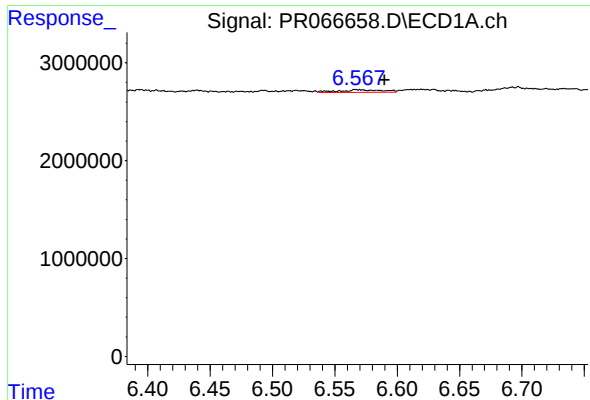

#31 AR-1260-1


R.T.: 6.569 min
Delta R.T.: -0.021 min
Response: 686206
Conc: 3.30 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

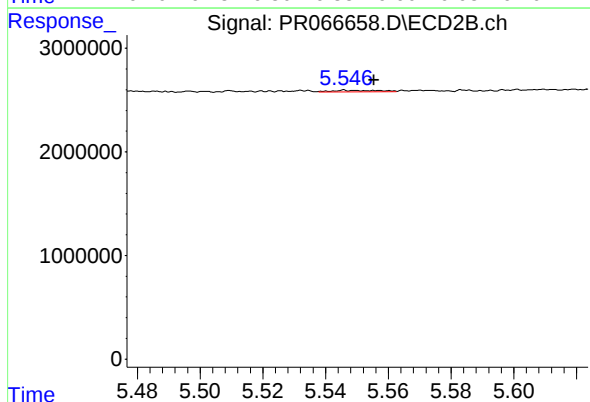


#31 AR-1260-1

R.T.: 5.546 min
Delta R.T.: -0.009 min
Response: 164036
Conc: 0.65 ng/ml

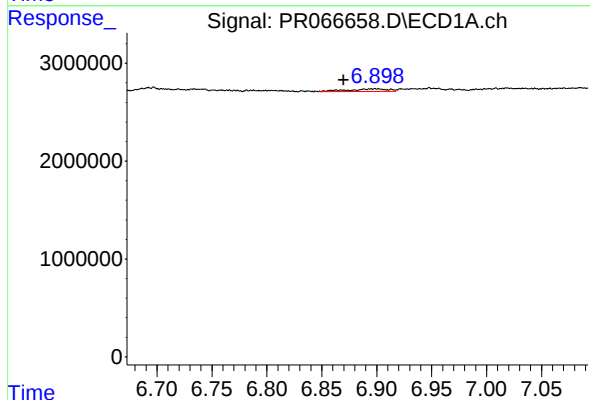


#32 AR-1260-2

R.T.: 6.899 min
Delta R.T.: 0.029 min
Response: 646048
Conc: 2.91 ng/ml

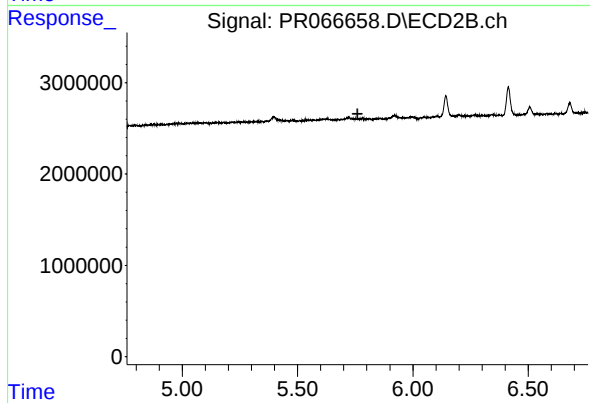

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 5.760 min
Response: 0
Conc: N.D.

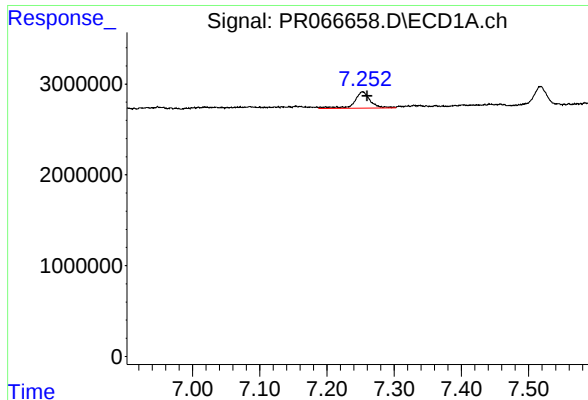

#33 AR-1260-3


R.T.: 7.253 min
Delta R.T.: -0.007 min
Response: 3050663
Conc: 18.19 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

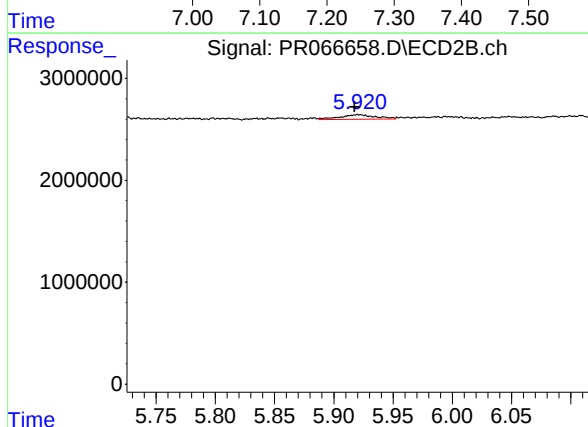


#33 AR-1260-3

R.T.: 5.921 min
Delta R.T.: 0.004 min
Response: 947674
Conc: 3.26 ng/ml

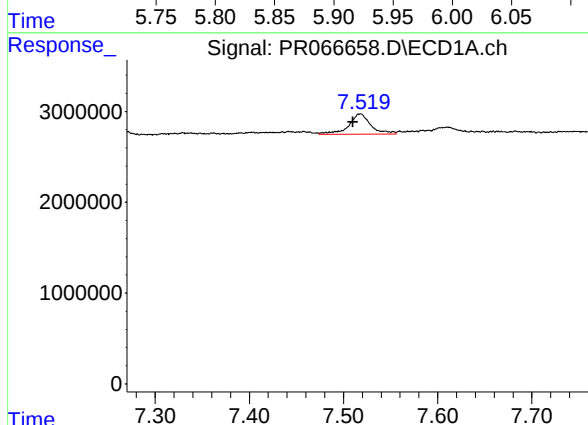


#34 AR-1260-4

R.T.: 7.518 min
Delta R.T.: 0.008 min
Response: 3681154
Conc: 20.66 ng/ml

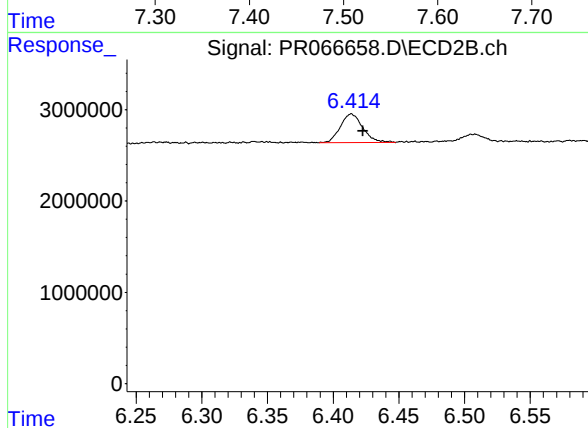

#34 AR-1260-4


R.T.: 6.414 min
Delta R.T.: -0.009 min
Response: 3748729
Conc: 15.01 ng/ml

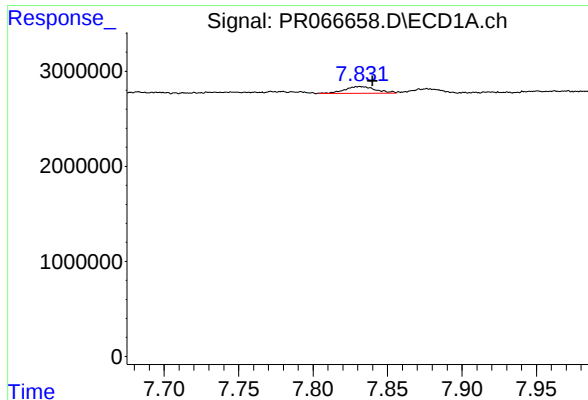

#35 AR-1260-5


R.T.: 7.831 min
Delta R.T.: -0.009 min
Response: 1037248
Conc: 3.55 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

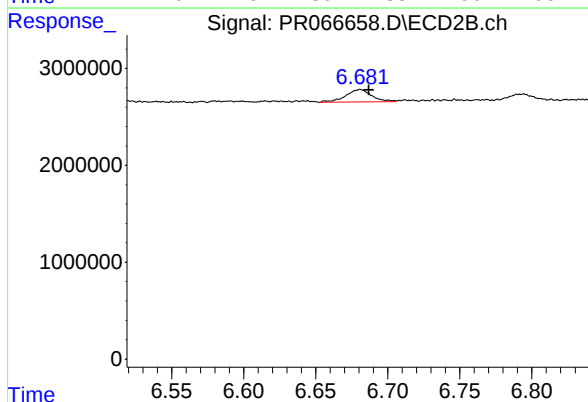


#35 AR-1260-5

R.T.: 6.681 min
Delta R.T.: -0.006 min
Response: 1624408
Conc: 2.89 ng/ml

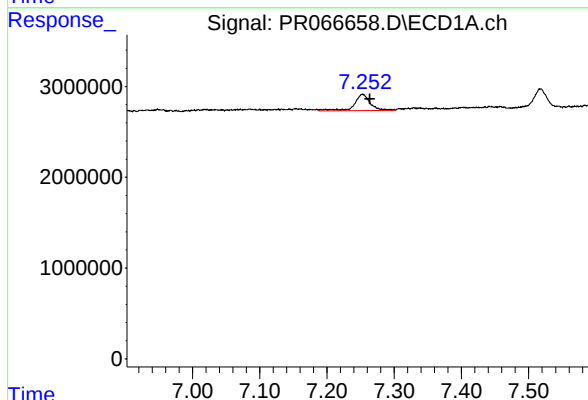


#36 AR-1262-1

R.T.: 7.253 min
Delta R.T.: -0.011 min
Response: 3050663
Conc: 13.37 ng/ml

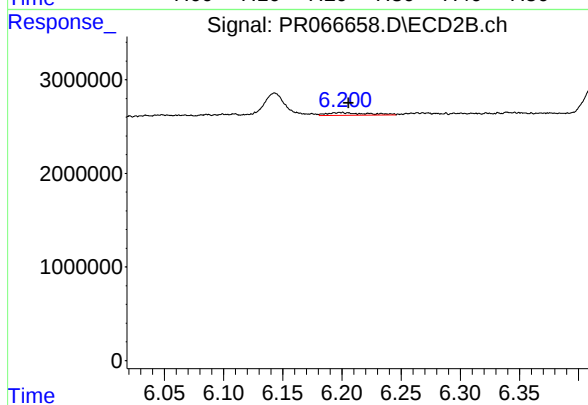

#36 AR-1262-1


R.T.: 6.199 min
Delta R.T.: -0.006 min
Response: 641048
Conc: 4.44 ng/ml

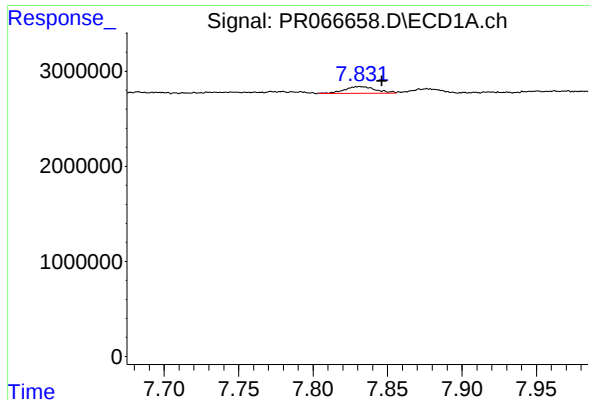

#37 AR-1262-2


R.T.: 7.831 min
Delta R.T.: -0.015 min
Response: 1037248
Conc: 3.27 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

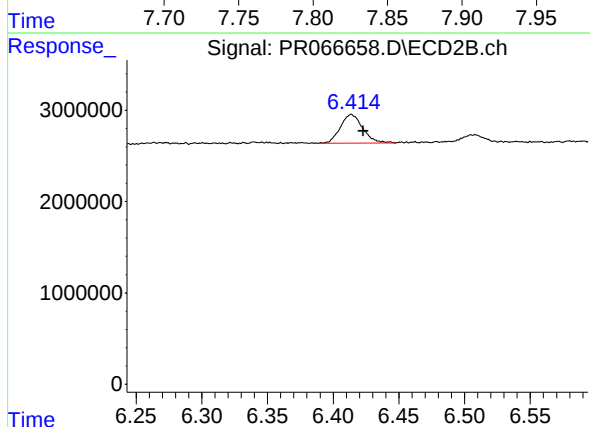


#37 AR-1262-2

R.T.: 6.414 min
Delta R.T.: -0.009 min
Response: 3748729
Conc: 12.18 ng/ml

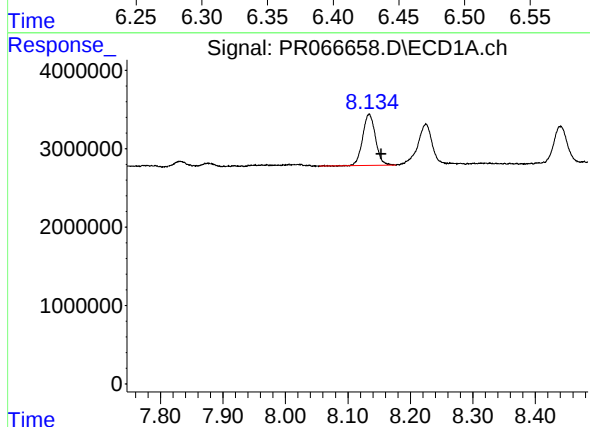


#38 AR-1262-3

R.T.: 8.134 min
Delta R.T.: -0.020 min
Response: 9399272
Conc: 44.40 ng/ml

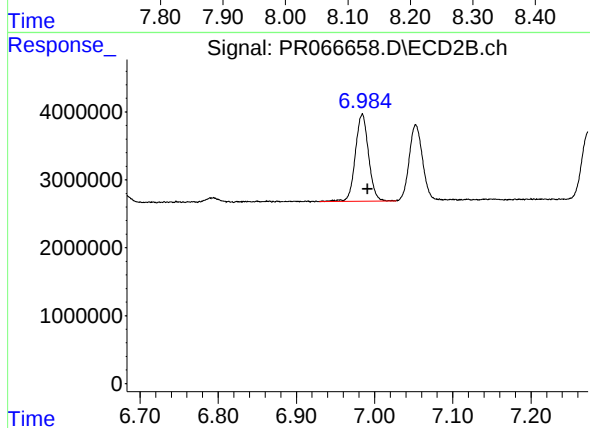

#38 AR-1262-3


R.T.: 6.984 min
Delta R.T.: -0.007 min
Response: 15068234
Conc: 62.16 ng/ml

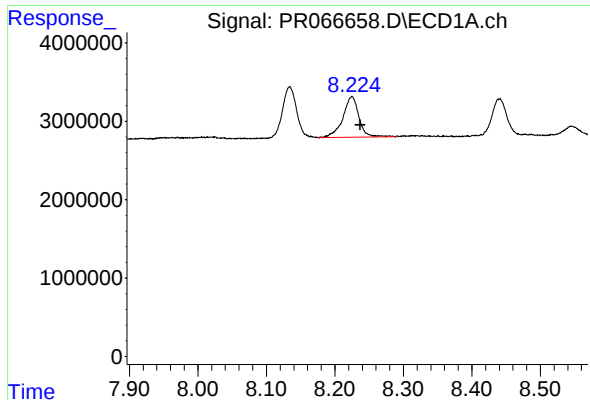

#39 AR-1262-4


R.T.: 8.225 min
Delta R.T.: -0.013 min
Response: 8540680
Conc: 78.19 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

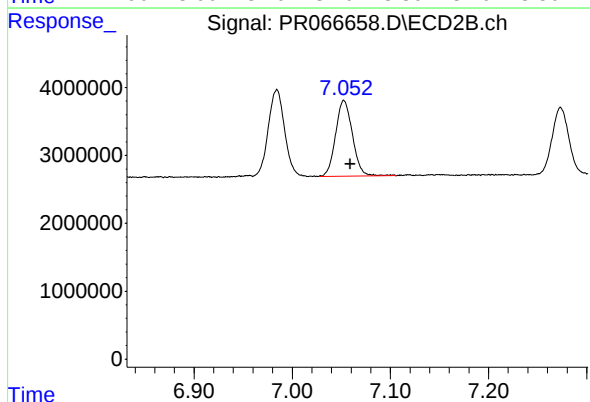


#39 AR-1262-4

R.T.: 7.053 min
Delta R.T.: -0.007 min
Response: 13294391
Conc: 30.25 ng/ml

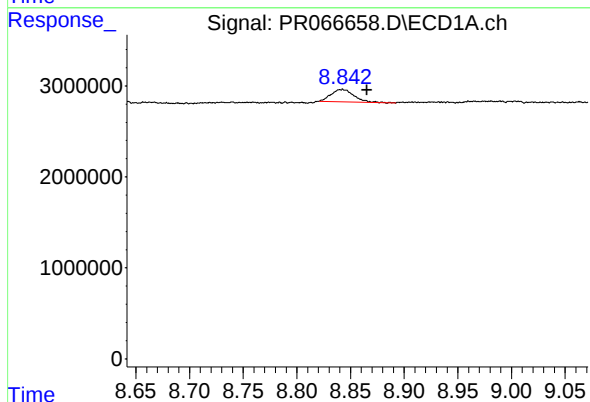


#40 AR-1262-5

R.T.: 8.842 min
Delta R.T.: -0.023 min
Response: 1995387
Conc: 19.63 ng/ml

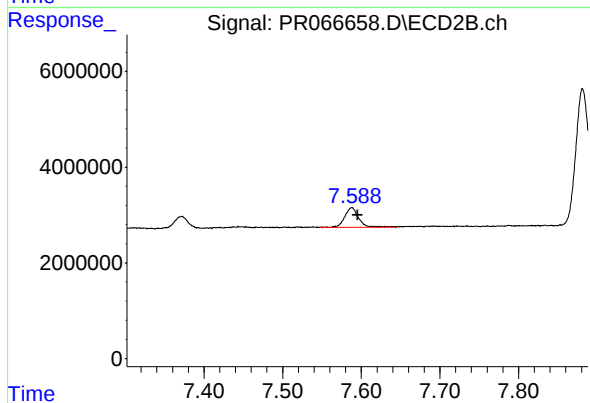

#40 AR-1262-5


R.T.: 7.588 min
Delta R.T.: -0.007 min
Response: 5140683
Conc: 23.81 ng/ml

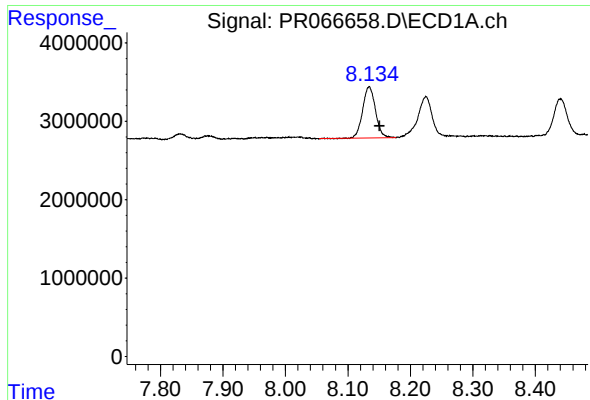

#41 AR-1268-1


R.T.: 8.134 min
Delta R.T.: -0.017 min
Response: 9399272
Conc: 24.11 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

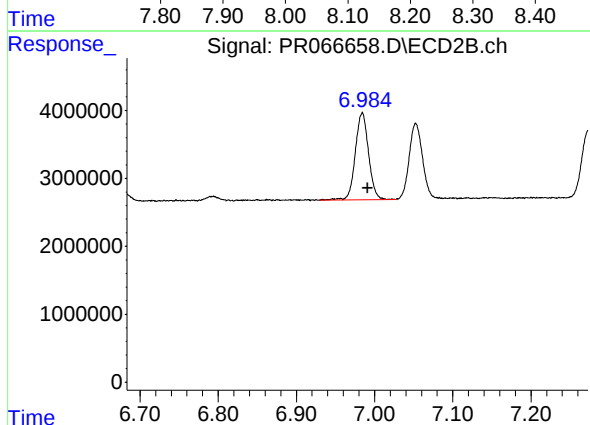


#41 AR-1268-1

R.T.: 6.984 min
Delta R.T.: -0.007 min
Response: 15068234
Conc: 20.81 ng/ml

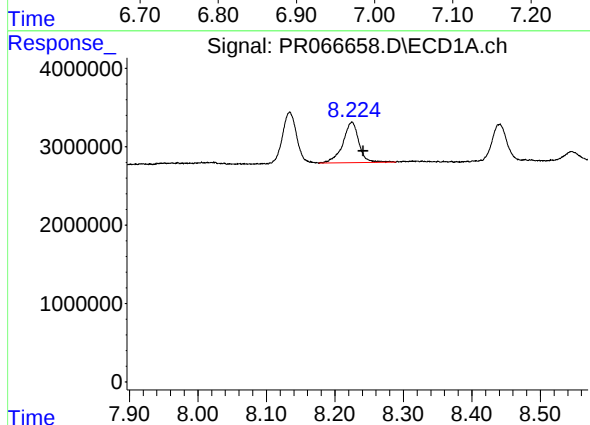


#42 AR-1268-2

R.T.: 8.225 min
Delta R.T.: -0.017 min
Response: 8540680
Conc: 24.86 ng/ml

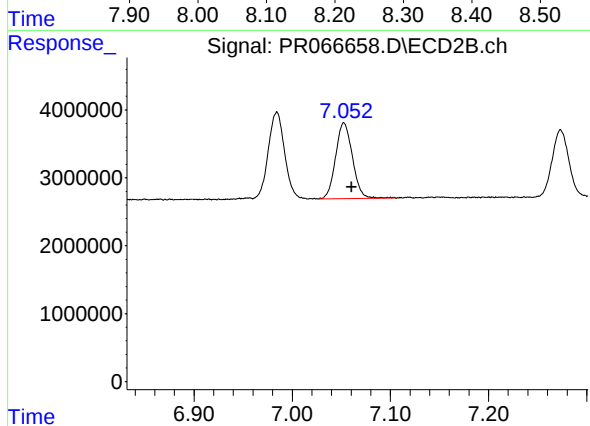

#42 AR-1268-2


R.T.: 7.053 min
Delta R.T.: -0.008 min
Response: 13294391
Conc: 20.71 ng/ml

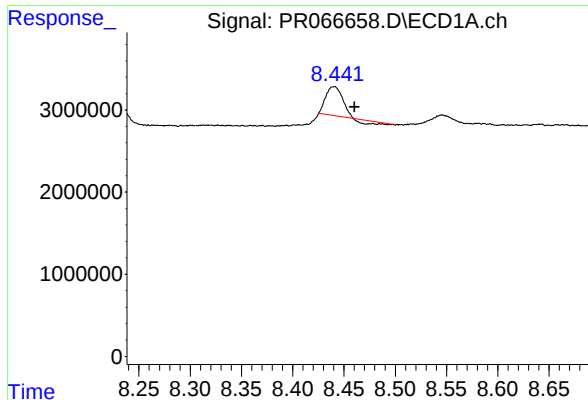

#43 AR-1268-3


R.T.: 8.440 min
Delta R.T.: -0.020 min
Response: 3484318
Conc: 11.35 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

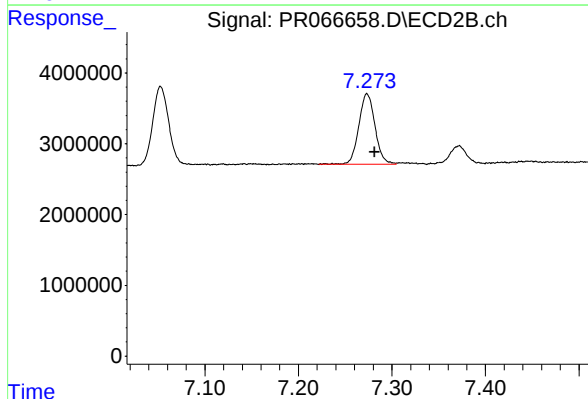


#43 AR-1268-3

R.T.: 7.273 min
Delta R.T.: -0.008 min
Response: 12018048
Conc: 21.19 ng/ml

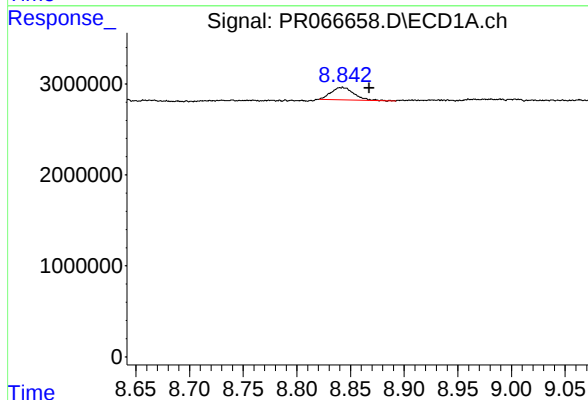


#44 AR-1268-4

R.T.: 8.842 min
Delta R.T.: -0.025 min
Response: 1995387
Conc: 17.17 ng/ml

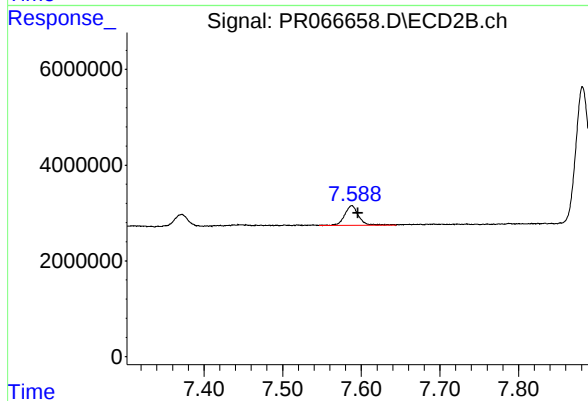

#44 AR-1268-4


R.T.: 7.588 min
Delta R.T.: -0.008 min
Response: 5140683
Conc: 21.06 ng/ml

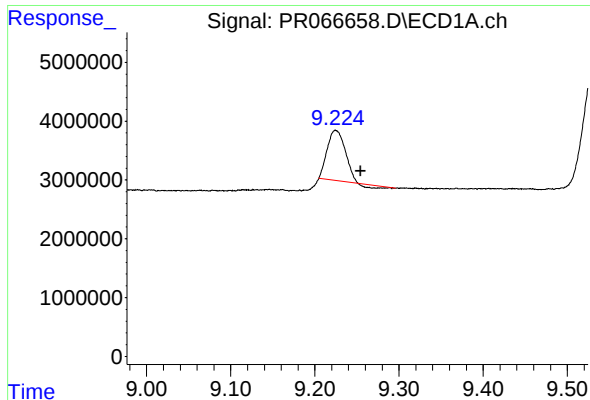

#45 AR-1268-5

R.T.: 9.225 min
Delta R.T.: -0.029 min
Response: 12109150
Conc: 14.85 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2024

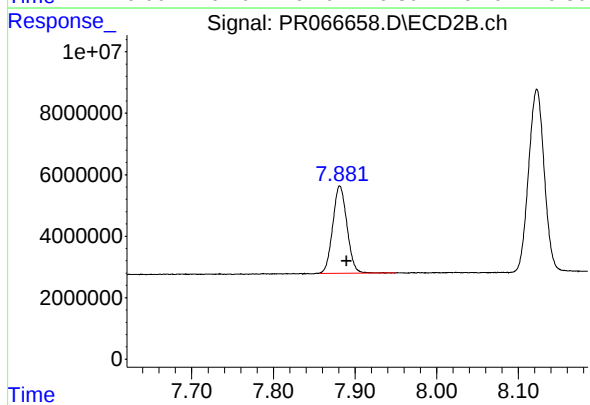

#45 AR-1268-5

R.T.: 7.882 min
Delta R.T.: -0.008 min
Response: 34268967
Conc: 21.15 ng/ml