

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051221\
 Data File : PD062859.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2021 09:09
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 03:54:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 08:49:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.971	21294669	253.9E6	23.948	21.928
28)	SA Decachlor...	8.199	9.027	25044079	266.4E6	23.655	23.084
Target Compounds							
7)	B delta-BHC	0.000	5.007f	0 19765708	N.D.	1.095	#
8)	B Heptachlo...	0.000	5.852	0 2787270	N.D.	0.174	#
14)	MA Endrin	0.000	6.684	0 10168762	N.D.	0.723	#
23)	Chlordane-1	4.337f	4.955	701294 146155	19.887	0.255	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051221\
Data File : PD062859.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2021 09:09
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 03:54:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 08:49:38 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

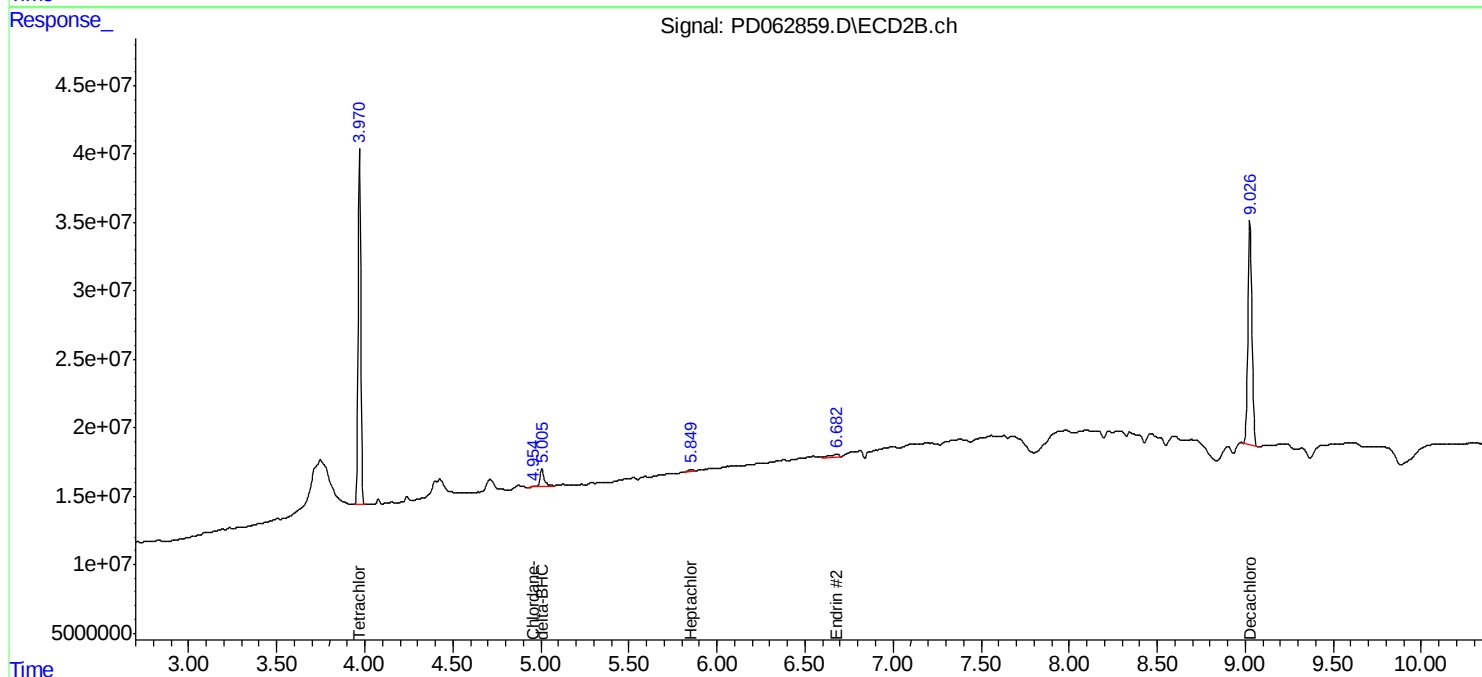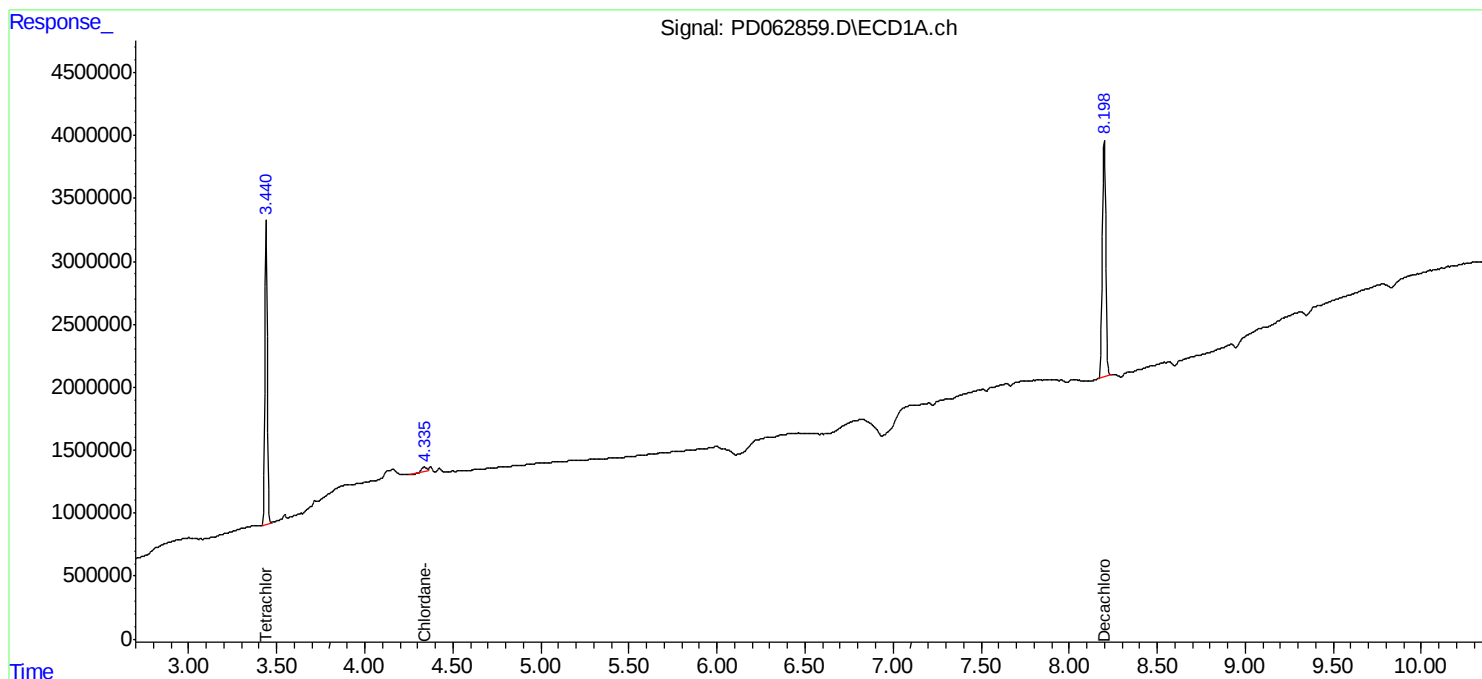


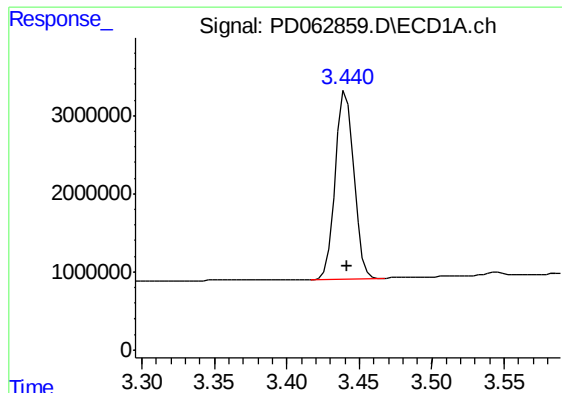

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: -0.001 min
Response: 21294669
Conc: 23.95 ng/ml

Instrument :
ECD_R
ClientSampleId :
I.BLK

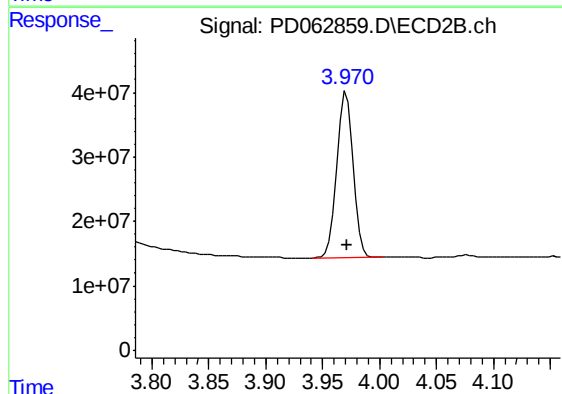


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 253861502
Conc: 21.93 ng/ml

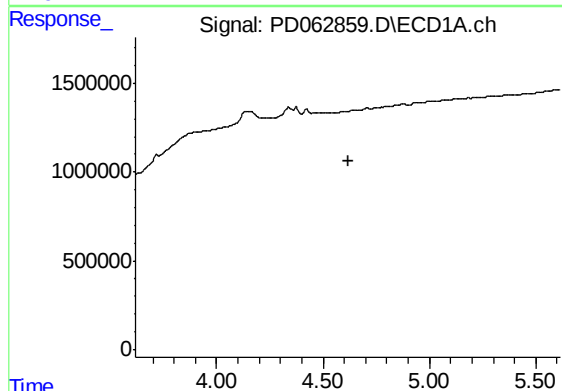


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.617 min
Response: 0
Conc: N.D.

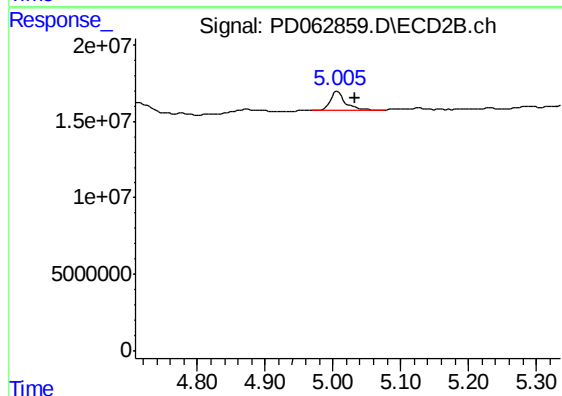

#7 delta-BHC


R.T.: 5.007 min
Delta R.T.: -0.025 min
Response: 19765708
Conc: 1.09 ng/ml

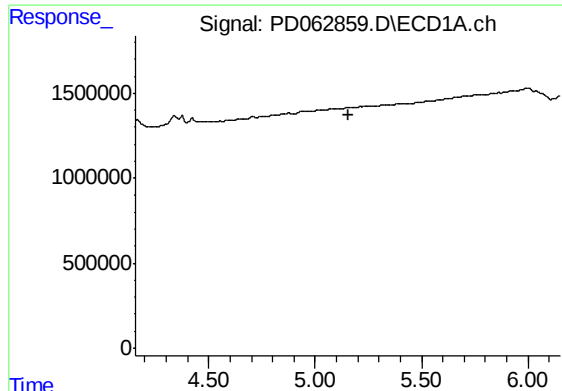

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
I.BLK

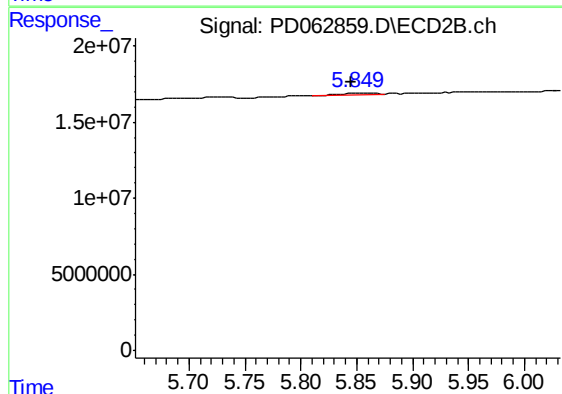


#8 Heptachlor epoxide

R.T.: 5.852 min
Delta R.T.: 0.007 min
Response: 2787270
Conc: 0.17 ng/ml

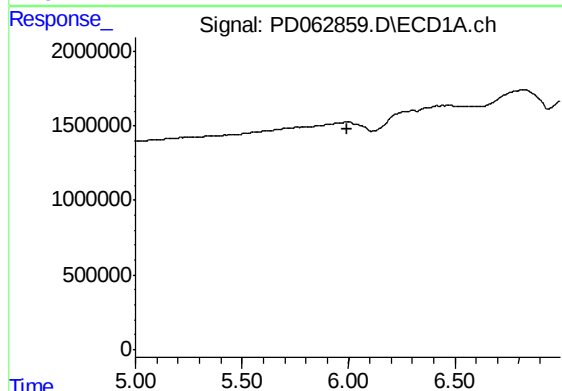


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

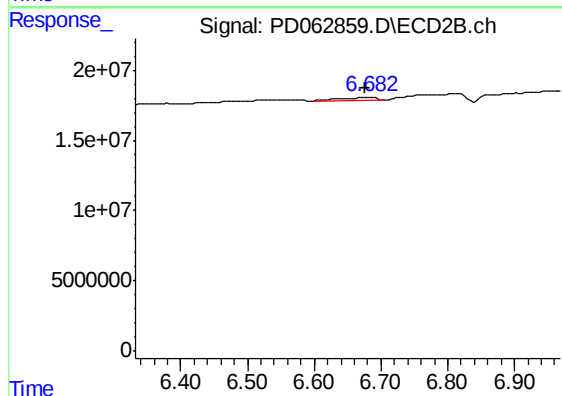

#14 Endrin


R.T.: 6.684 min
Delta R.T.: 0.009 min
Response: 10168762
Conc: 0.72 ng/ml

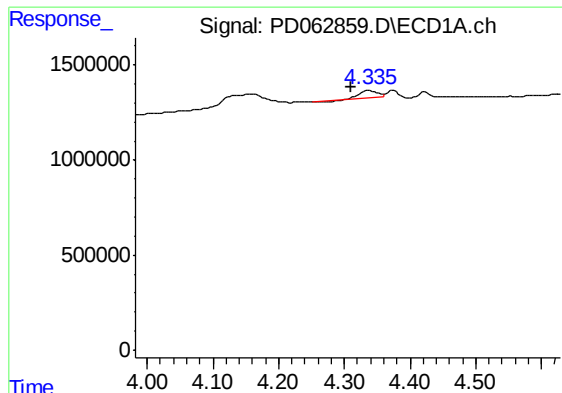

#23 Chlordane-1


R.T.: 4.337 min
Delta R.T.: 0.026 min
Response: 701294
Conc: 19.89 ng/ml

Instrument :
ECD_R
ClientSampleId :
I.BLK

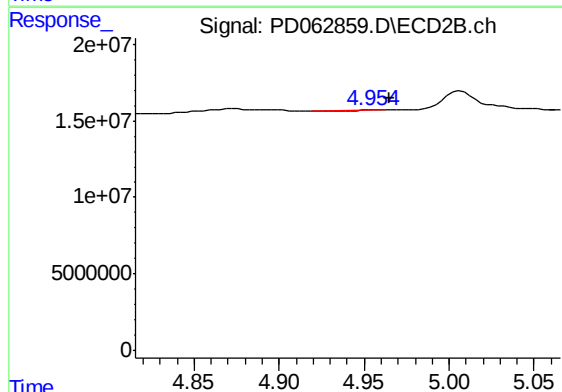


#23 Chlordane-1

R.T.: 4.955 min
Delta R.T.: -0.010 min
Response: 146155
Conc: 0.25 ng/ml

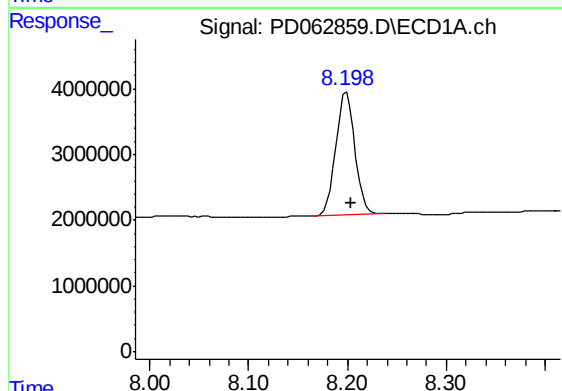

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: -0.004 min
Response: 25044079
Conc: 23.66 ng/ml

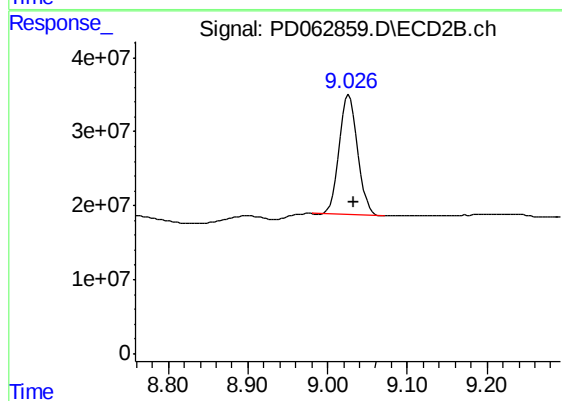

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: -0.005 min
Response: 266366750
Conc: 23.08 ng/ml