

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR051121\
 Data File : PR050241.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2021 11:12
 Operator : DD\AJ
 Sample : M2250-01
 Misc : AR1660 MDL 25 PPB
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-QT3-2021-05

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 22:53:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR050721CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 08 06:36:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.634	3.815	67934662	103.3E6	20.095	21.196
2)	SA Decachlor...	10.505	8.844	205.8E6	247.5E6	37.673	37.412
Target Compounds							
3)	L1 AR-1016-1	5.815	4.903	5066331	6081652	27.645	30.001
4)	L1 AR-1016-2	5.838	4.921	7992234	8010860	30.660	27.566
5)	L1 AR-1016-3	5.900	5.098	4940234	4460003	31.134	28.771
6)	L1 AR-1016-4	6.000	5.138	3894027	3699627	29.139	31.071
7)	L1 AR-1016-5	6.294	5.352	4282225	5272541	30.891	32.235
8)	L2 AR-1221-1	4.858	0.000	3248350	0	72.577	N.D. #
9)	L2 AR-1221-2	4.943	4.114	1519348	3560899	46.486	84.724 #
10)	L2 AR-1221-3	5.013	4.191	2287081	2958542	20.687	20.536
11)	L3 AR-1232-1	5.013	4.191	2287081	2958542	24.528	24.548
12)	L3 AR-1232-2	5.546	4.921	3663503	8010860	65.335	61.264
13)	L3 AR-1232-3	5.838	5.098	7992234	4460003	66.362	64.361
14)	L3 AR-1232-4	6.000	5.181	3894027	4594783	63.515	75.692
15)	L3 AR-1232-5	6.087	5.352	3919660	5272541	81.909	77.054
16)	L4 AR-1242-1	5.815	4.903	5066331	6081652	29.062	32.737
17)	L4 AR-1242-2	5.838	4.921	7992234	8010860	32.371	29.783
18)	L4 AR-1242-3	5.900	5.098	4940234	4460003	32.536	30.804
19)	L4 AR-1242-4	6.000	5.181	3894027	4594783	30.276	33.092
20)	L4 AR-1242-5	6.698f	5.703	510369	4006888	3.187	20.249 #
21)	L5 AR-1248-1	5.815	4.903	5066331	6081652	41.607	46.676
22)	L5 AR-1248-2	6.087	5.138	3919660	3699627	21.408	20.616
23)	L5 AR-1248-3	6.294	5.181	4282225	4594783	20.211	23.952
24)	L5 AR-1248-4	6.698	5.352	510369	5272541	1.931	22.206 #
25)	L5 AR-1248-5	6.698f	5.703f	510369	4006888	1.998	15.278 #
26)	L6 AR-1254-1	6.671	5.703	3465696	4006888	9.347	7.234
27)	L6 AR-1254-2	6.888	5.849	3938348	4012013	6.634	8.224
28)	L6 AR-1254-3	7.260	6.268	2539153	9278616	3.796	10.620 #
29)	L6 AR-1254-4	7.545	6.480	2024417	735396	3.993	1.317 #
30)	L6 AR-1254-5	7.965	6.895	13255809	15291085	24.261	18.863
31)	L7 AR-1260-1	7.420	6.382	9527649	10681629	36.121	32.107
32)	L7 AR-1260-2	7.677	6.568	11241369	13860588	34.866	33.486
33)	L7 AR-1260-3	8.036	6.722	7010460	12077833	28.475	30.547
34)	L7 AR-1260-4	8.270	7.193	8863510	8992098	30.267	26.024
35)	L7 AR-1260-5	8.607	7.432	16038829	21171699	26.556	24.426
36)	L8 AR-1262-1	8.036	6.895	7010460	15291085	14.188	46.504 #
37)	L8 AR-1262-2	8.607	7.432	16038829	21171699	17.528	17.327
38)	L8 AR-1262-3	8.954	7.716	10556943	3840704	17.476	8.550 #
39)	L8 AR-1262-4	9.007	7.779	5719991	15710645	12.864	17.596 #
40)	L8 AR-1262-5	9.721	8.279	4158407	4727124	12.873	11.545
41)	L9 AR-1268-1	8.954	7.716	10556943	3840704	9.373	2.666 #
42)	L9 AR-1268-2	9.007	7.779	5719991	15710645	5.604	11.737 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR051121\
 Data File : PR050241.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2021 11:12
 Operator : DD\AJ
 Sample : M2250-01
 Misc : AR1660 MDL 25 PPB
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-QT3-2021-05

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 22:53:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR050721CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 08 06:36:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	0.000	7.989	0	760118	N.D.	0.679 #
44) L9	AR-1268-4	9.721	8.279	4158407	4727124	10.947	9.859
45) L9	AR-1268-5	10.154	8.579	2396799	2911964	0.811	0.801



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR051121\
Data File : PR050241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2021 11:12
Operator : DD\AJ
Sample : M2250-01
Misc : AR1660 MDL 25 PPB
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 22:53:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR050721CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 08 06:36:02 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

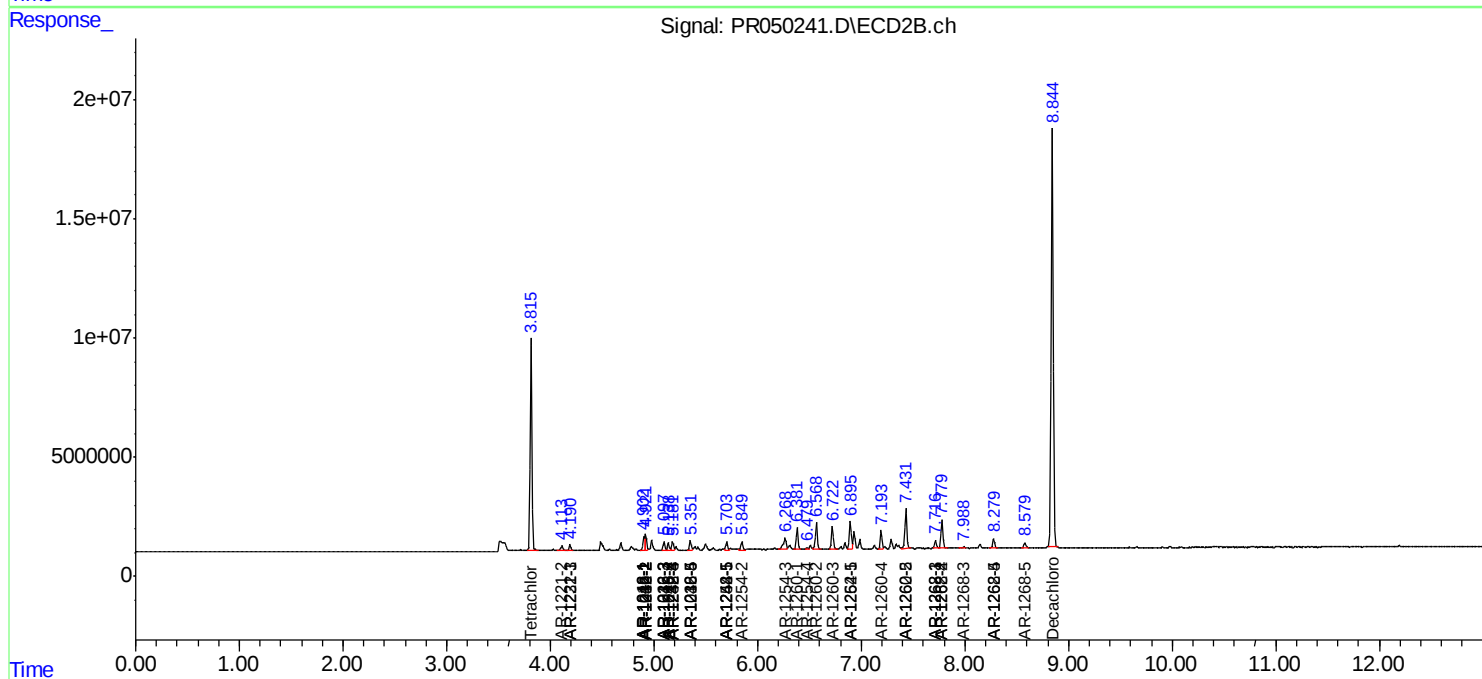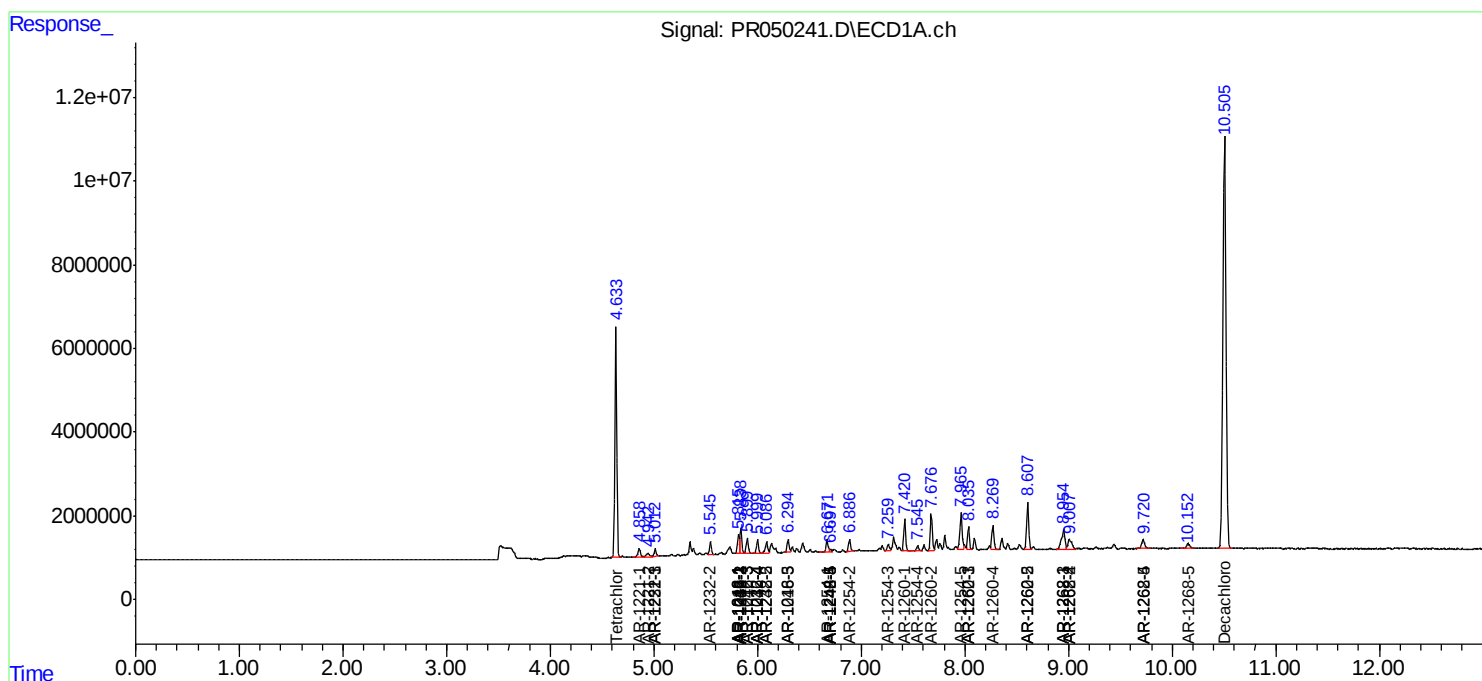


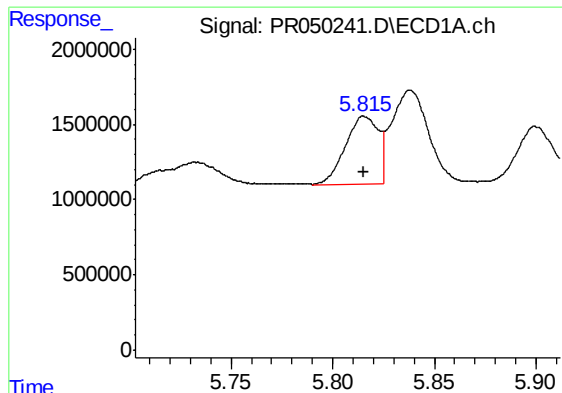

#3 AR-1016-1


R.T.: 5.815 min
Delta R.T.: 0.000 min
Response: 5066331
Conc: 27.64 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

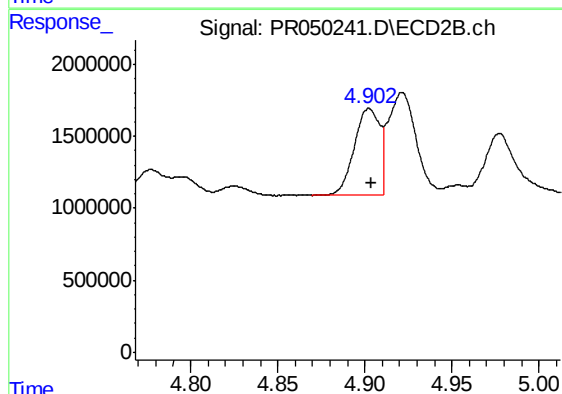


#3 AR-1016-1

R.T.: 4.903 min
Delta R.T.: -0.001 min
Response: 6081652
Conc: 30.00 ng/ml

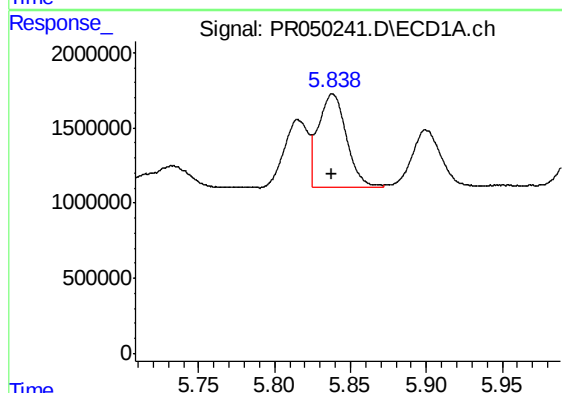


#4 AR-1016-2

R.T.: 5.838 min
Delta R.T.: 0.000 min
Response: 7992234
Conc: 30.66 ng/ml

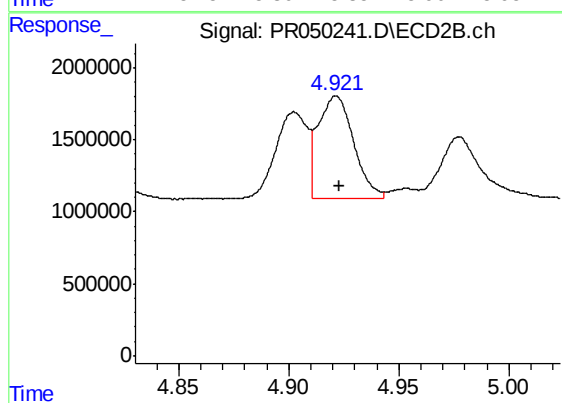

#4 AR-1016-2


R.T.: 4.921 min
Delta R.T.: -0.002 min
Response: 8010860
Conc: 27.57 ng/ml

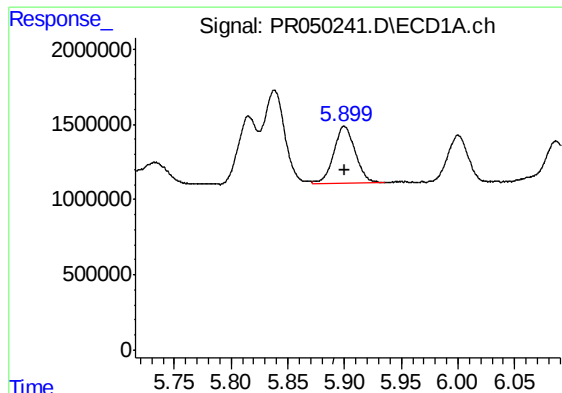

#5 AR-1016-3


R.T.: 5.900 min
Delta R.T.: 0.000 min
Response: 4940234
Conc: 31.13 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

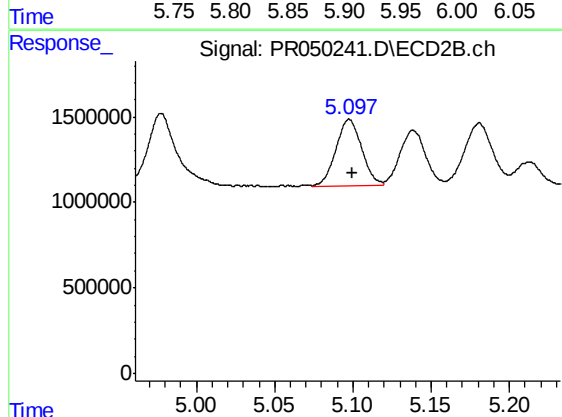


#5 AR-1016-3

R.T.: 5.098 min
Delta R.T.: -0.002 min
Response: 4460003
Conc: 28.77 ng/ml

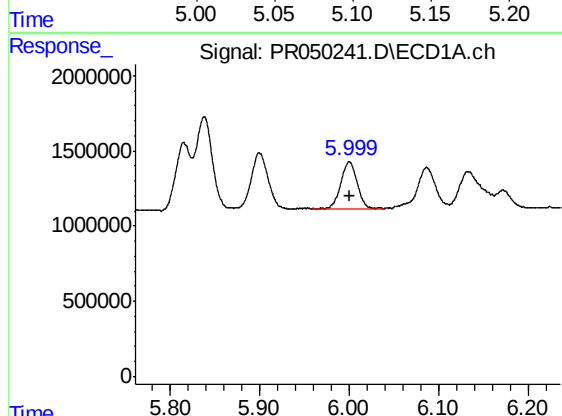


#6 AR-1016-4

R.T.: 6.000 min
Delta R.T.: 0.000 min
Response: 3894027
Conc: 29.14 ng/ml

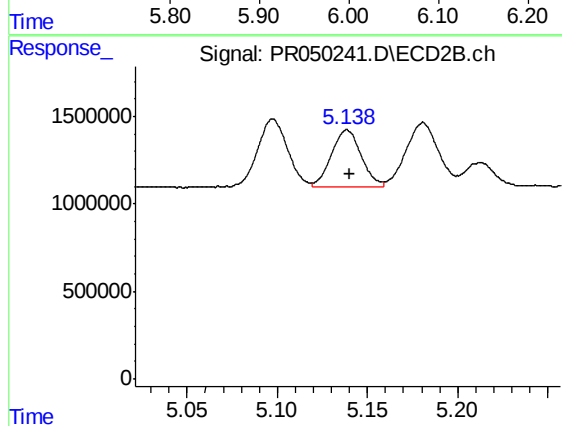

#6 AR-1016-4


R.T.: 5.138 min
Delta R.T.: -0.001 min
Response: 3699627
Conc: 31.07 ng/ml



#7 AR-1016-5


R.T.: 6.294 min
Delta R.T.: 0.000 min
Response: 4282225
Conc: 30.89 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

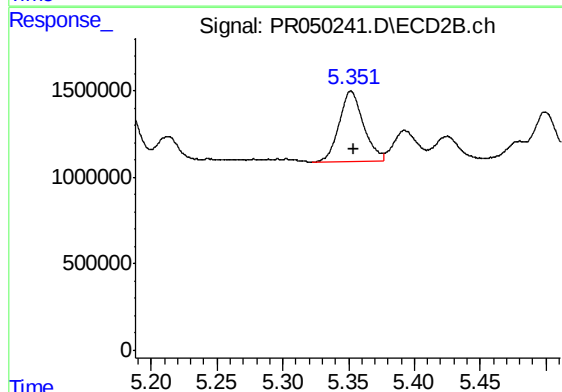


#7 AR-1016-5

R.T.: 5.352 min
Delta R.T.: -0.002 min
Response: 5272541
Conc: 32.24 ng/ml




#8 AR-1221-1

R.T.: 4.858 min
Delta R.T.: 0.012 min
Response: 3248350
Conc: 72.58 ng/ml

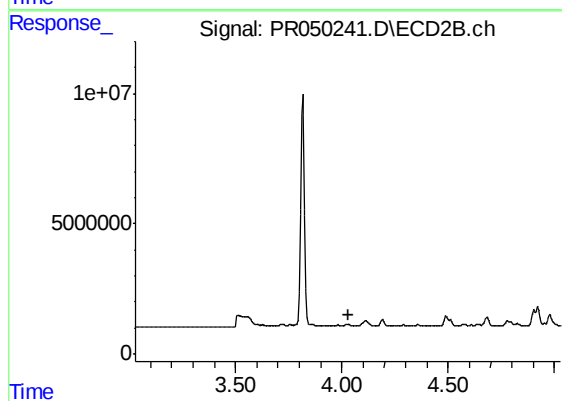

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 4.029 min
Response: 0
Conc: N.D.

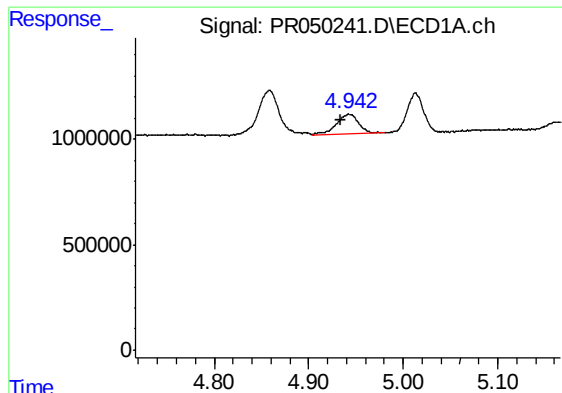

#9 AR-1221-2


R.T.: 4.943 min
Delta R.T.: 0.009 min
Response: 1519348
Conc: 46.49 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

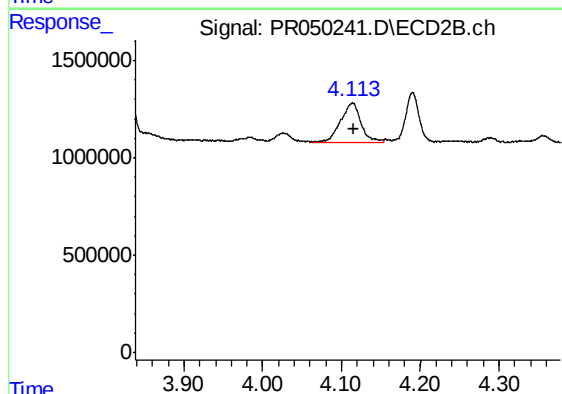


#9 AR-1221-2

R.T.: 4.114 min
Delta R.T.: -0.001 min
Response: 3560899
Conc: 84.72 ng/ml

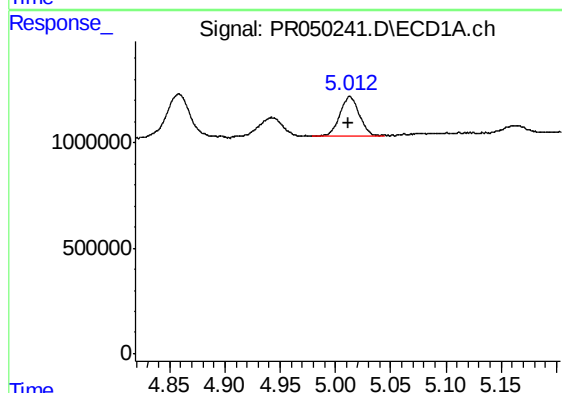


#10 AR-1221-3

R.T.: 5.013 min
Delta R.T.: 0.000 min
Response: 2287081
Conc: 20.69 ng/ml

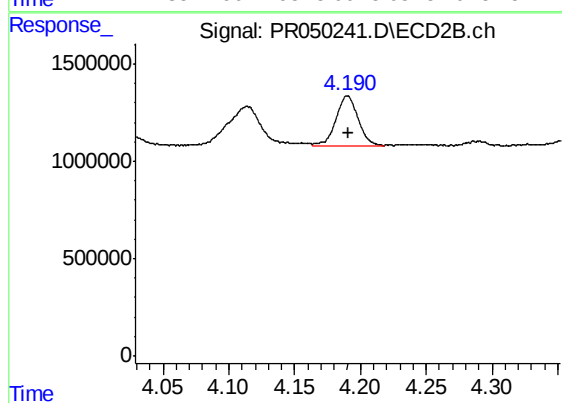

#10 AR-1221-3


R.T.: 4.191 min
Delta R.T.: 0.000 min
Response: 2958542
Conc: 20.54 ng/ml

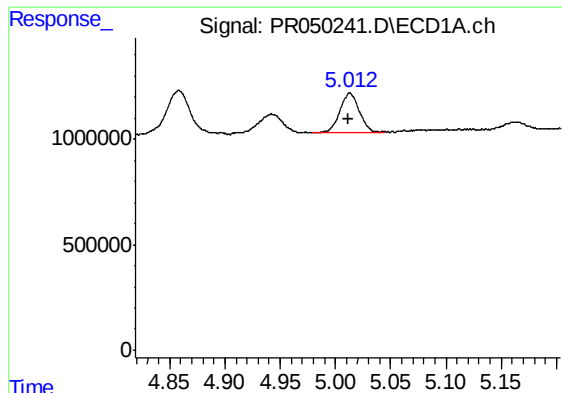

#11 AR-1232-1


R.T.: 5.013 min
Delta R.T.: 0.000 min
Response: 2287081
Conc: 24.53 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

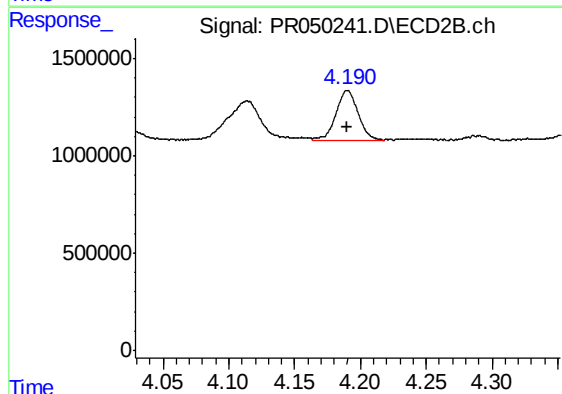


#11 AR-1232-1

R.T.: 4.191 min
Delta R.T.: 0.000 min
Response: 2958542
Conc: 24.55 ng/ml




#12 AR-1232-2

R.T.: 5.546 min
Delta R.T.: 0.000 min
Response: 3663503
Conc: 65.34 ng/ml

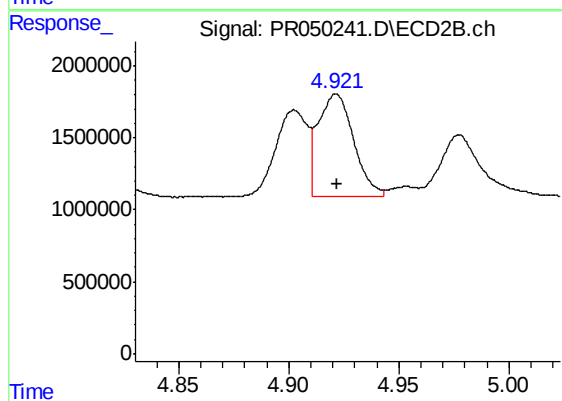

#12 AR-1232-2


R.T.: 4.921 min
Delta R.T.: 0.000 min
Response: 8010860
Conc: 61.26 ng/ml



#13 AR-1232-3


R.T.: 5.838 min
Delta R.T.: 0.000 min
Response: 7992234
Conc: 66.36 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

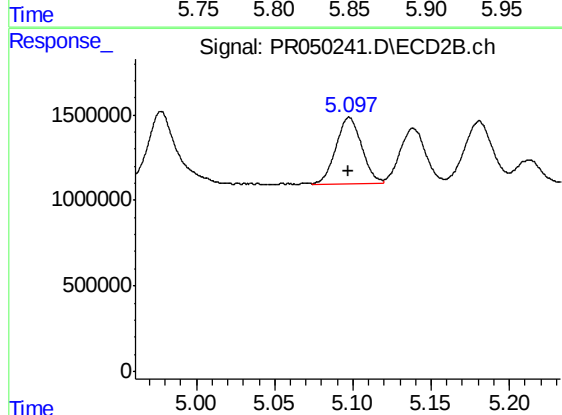


#13 AR-1232-3

R.T.: 5.098 min
Delta R.T.: 0.000 min
Response: 4460003
Conc: 64.36 ng/ml

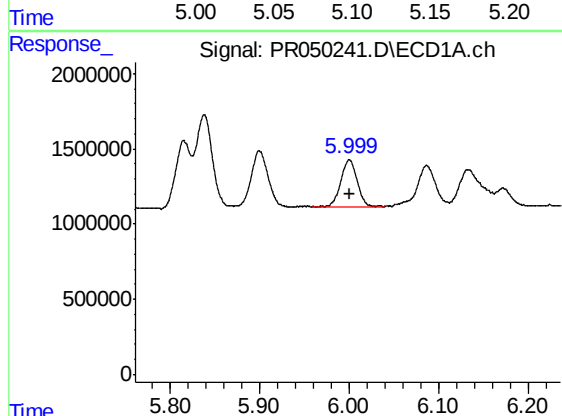


#14 AR-1232-4

R.T.: 6.000 min
Delta R.T.: 0.000 min
Response: 3894027
Conc: 63.51 ng/ml

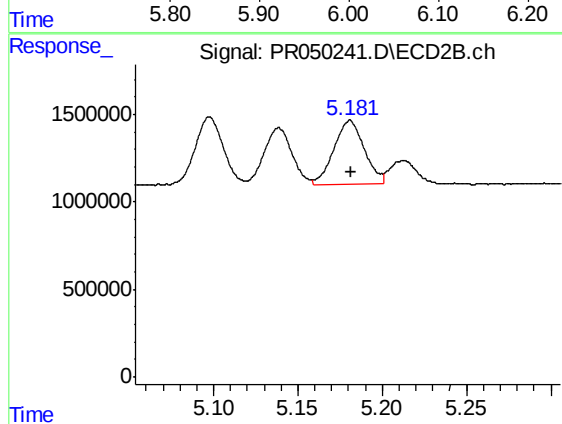

#14 AR-1232-4


R.T.: 5.181 min
Delta R.T.: 0.000 min
Response: 4594783
Conc: 75.69 ng/ml

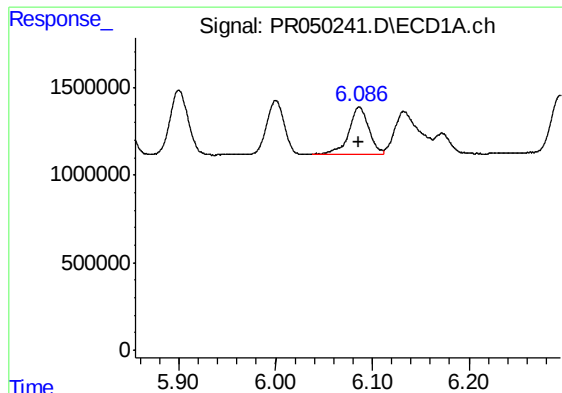

#15 AR-1232-5


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 3919660
Conc: 81.91 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

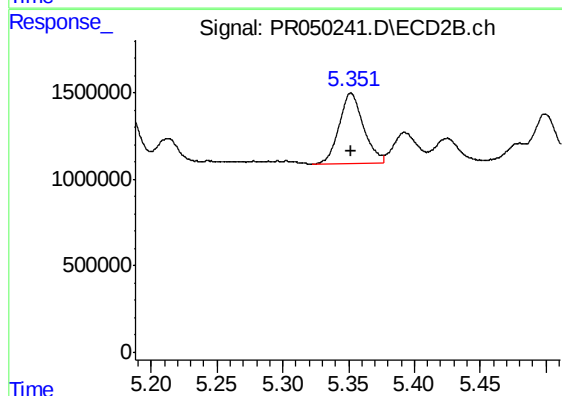


#15 AR-1232-5

R.T.: 5.352 min
Delta R.T.: 0.000 min
Response: 5272541
Conc: 77.05 ng/ml

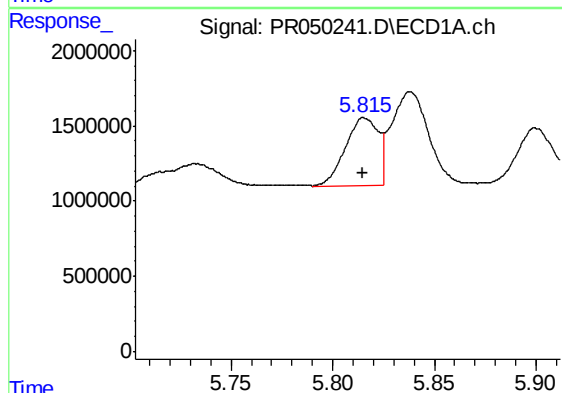


#16 AR-1242-1

R.T.: 5.815 min
Delta R.T.: 0.000 min
Response: 5066331
Conc: 29.06 ng/ml

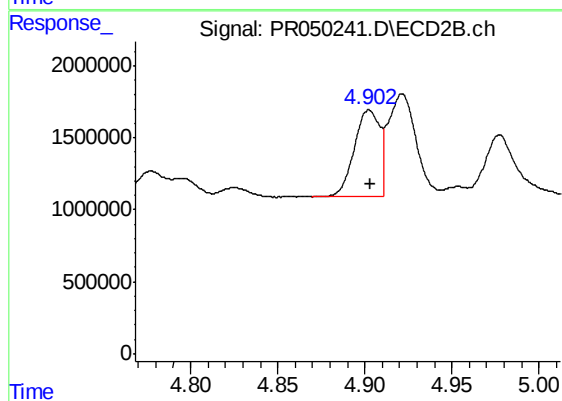

#16 AR-1242-1


R.T.: 4.903 min
Delta R.T.: 0.000 min
Response: 6081652
Conc: 32.74 ng/ml

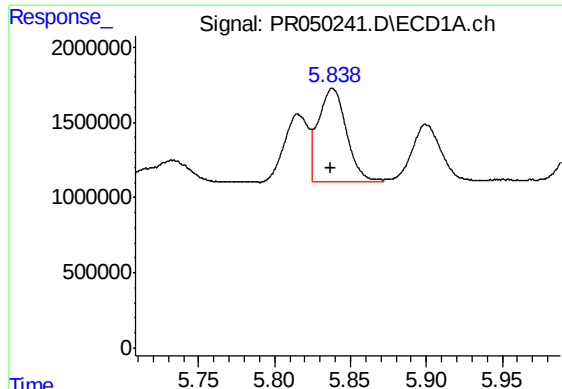

#17 AR-1242-2


R.T.: 5.838 min
Delta R.T.: 0.000 min
Response: 7992234
Conc: 32.37 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

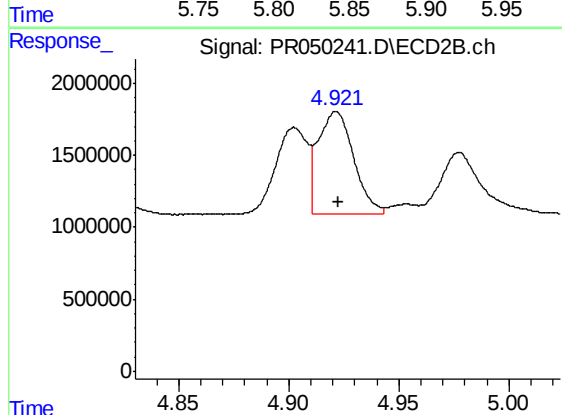


#17 AR-1242-2

R.T.: 4.921 min
Delta R.T.: -0.001 min
Response: 8010860
Conc: 29.78 ng/ml

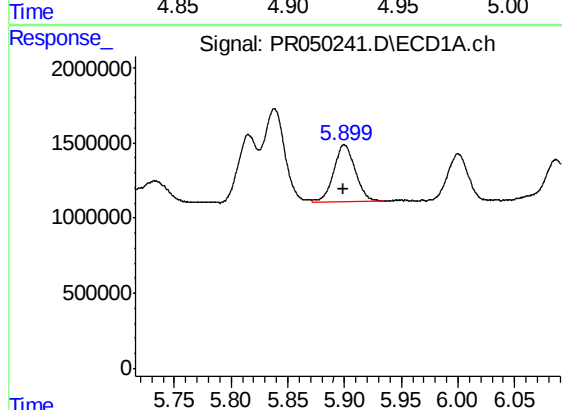


#18 AR-1242-3

R.T.: 5.900 min
Delta R.T.: 0.000 min
Response: 4940234
Conc: 32.54 ng/ml

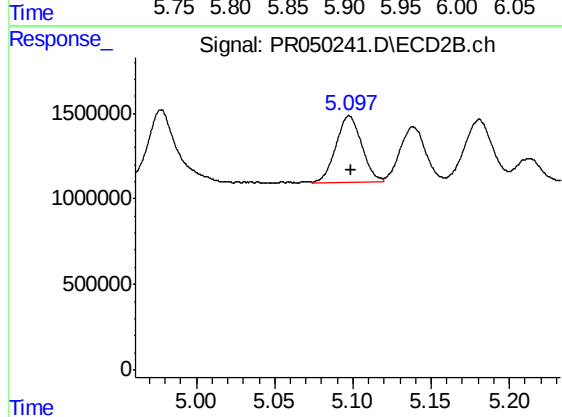

#18 AR-1242-3


R.T.: 5.098 min
Delta R.T.: 0.000 min
Response: 4460003
Conc: 30.80 ng/ml



#19 AR-1242-4


R.T.: 6.000 min
Delta R.T.: 0.000 min
Response: 3894027
Conc: 30.28 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

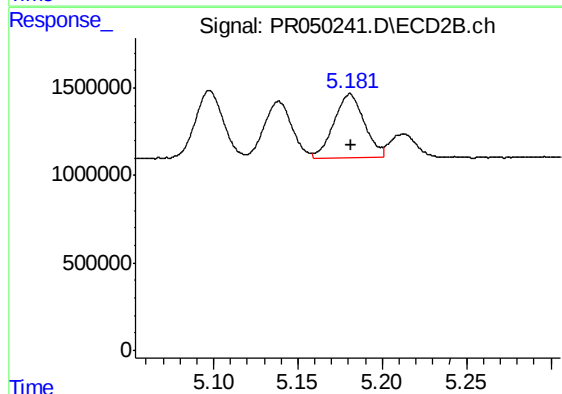


#19 AR-1242-4

R.T.: 5.181 min
Delta R.T.: 0.000 min
Response: 4594783
Conc: 33.09 ng/ml




#20 AR-1242-5

R.T.: 6.698 min
Delta R.T.: -0.039 min
Response: 510369
Conc: 3.19 ng/ml

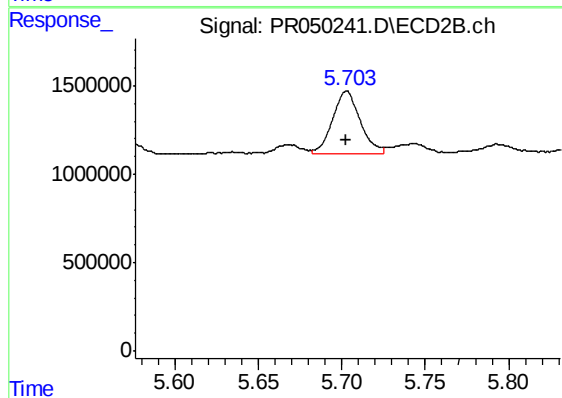

#20 AR-1242-5


R.T.: 5.703 min
Delta R.T.: 0.000 min
Response: 4006888
Conc: 20.25 ng/ml



#21 AR-1248-1


R.T.: 5.815 min
Delta R.T.: 0.000 min
Response: 5066331
Conc: 41.61 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

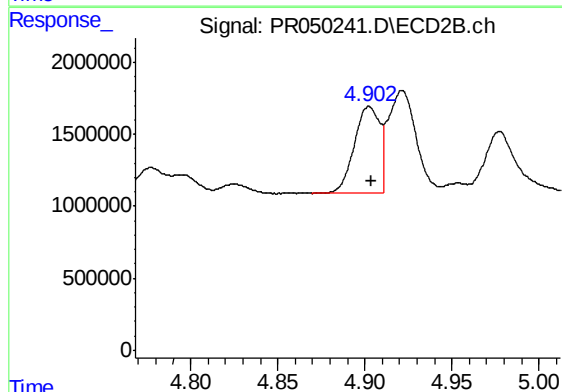


#21 AR-1248-1

R.T.: 4.903 min
Delta R.T.: -0.001 min
Response: 6081652
Conc: 46.68 ng/ml




#22 AR-1248-2

R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 3919660
Conc: 21.41 ng/ml

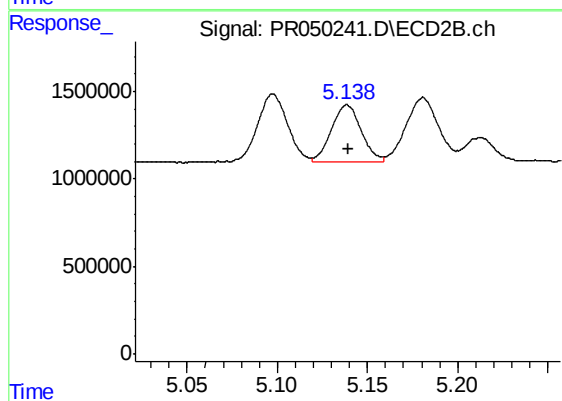

#22 AR-1248-2


R.T.: 5.138 min
Delta R.T.: -0.001 min
Response: 3699627
Conc: 20.62 ng/ml



#23 AR-1248-3


R.T.: 6.294 min
Delta R.T.: 0.000 min
Response: 4282225
Conc: 20.21 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

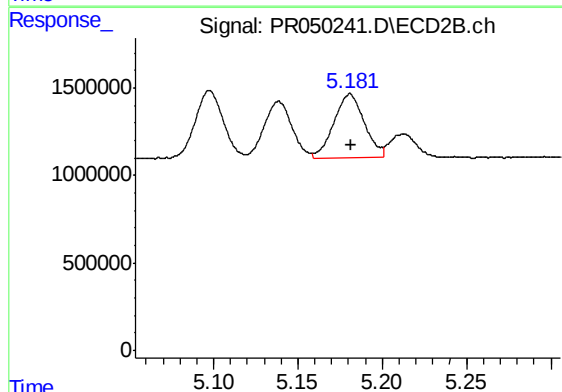


#23 AR-1248-3

R.T.: 5.181 min
Delta R.T.: 0.000 min
Response: 4594783
Conc: 23.95 ng/ml




#24 AR-1248-4

R.T.: 6.698 min
Delta R.T.: 0.000 min
Response: 510369
Conc: 1.93 ng/ml

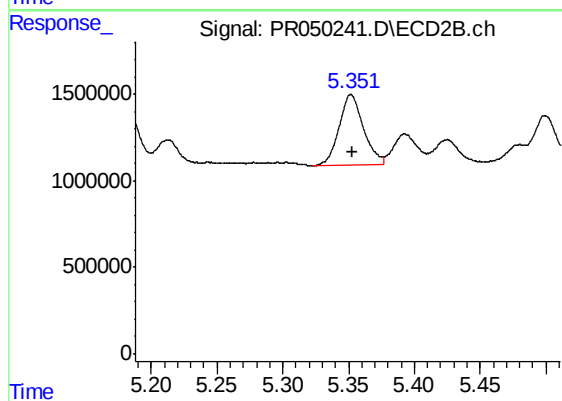

#24 AR-1248-4


R.T.: 5.352 min
Delta R.T.: 0.000 min
Response: 5272541
Conc: 22.21 ng/ml



#25 AR-1248-5


R.T.: 6.698 min
Delta R.T.: -0.039 min
Response: 510369
Conc: 2.00 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

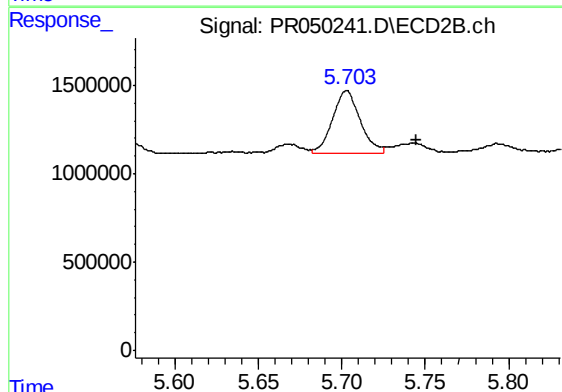


#25 AR-1248-5

R.T.: 5.703 min
Delta R.T.: -0.042 min
Response: 4006888
Conc: 15.28 ng/ml




#26 AR-1254-1

R.T.: 6.671 min
Delta R.T.: 0.000 min
Response: 3465696
Conc: 9.35 ng/ml

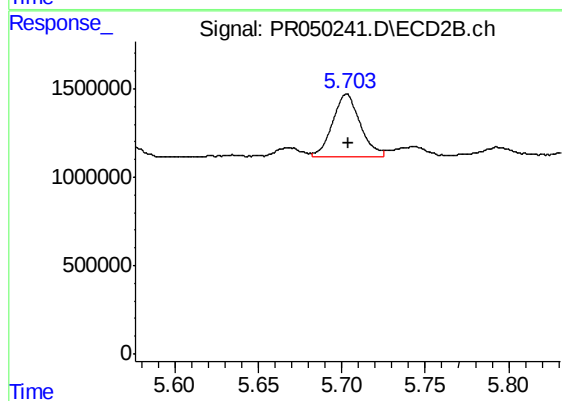

#26 AR-1254-1


R.T.: 5.703 min
Delta R.T.: -0.001 min
Response: 4006888
Conc: 7.23 ng/ml



#27 AR-1254-2


R.T.: 6.888 min
Delta R.T.: 0.000 min
Response: 3938348
Conc: 6.63 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

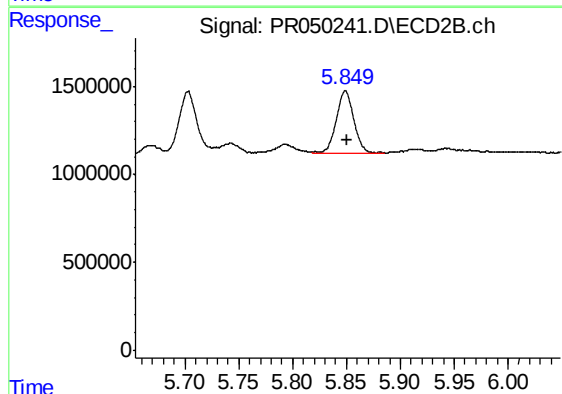


#27 AR-1254-2

R.T.: 5.849 min
Delta R.T.: -0.002 min
Response: 4012013
Conc: 8.22 ng/ml




#28 AR-1254-3

R.T.: 7.260 min
Delta R.T.: 0.002 min
Response: 2539153
Conc: 3.80 ng/ml

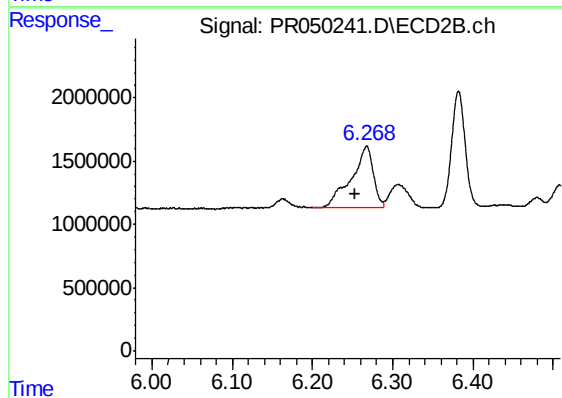

#28 AR-1254-3


R.T.: 6.268 min
Delta R.T.: 0.014 min
Response: 9278616
Conc: 10.62 ng/ml

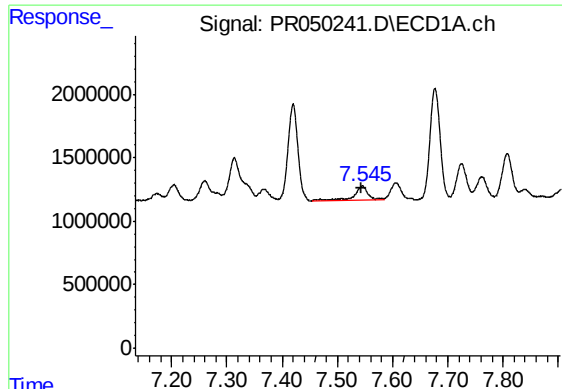

#29 AR-1254-4


R.T.: 7.545 min
Delta R.T.: 0.001 min
Response: 2024417
Conc: 3.99 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

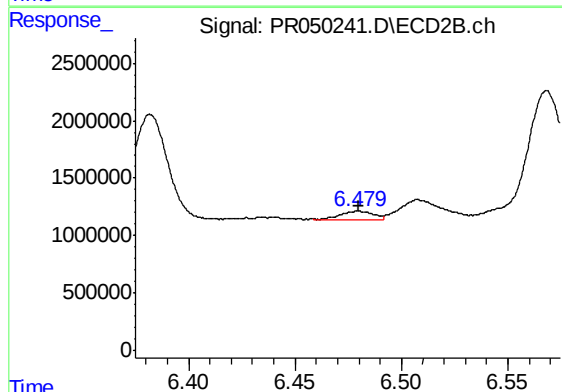


#29 AR-1254-4

R.T.: 6.480 min
Delta R.T.: 0.000 min
Response: 735396
Conc: 1.32 ng/ml




#30 AR-1254-5

R.T.: 7.965 min
Delta R.T.: 0.002 min
Response: 13255809
Conc: 24.26 ng/ml

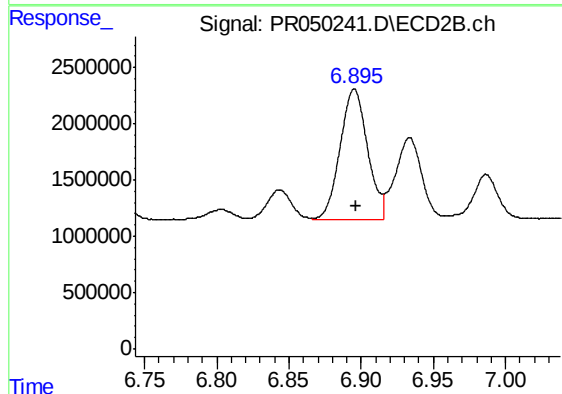

#30 AR-1254-5


R.T.: 6.895 min
Delta R.T.: -0.001 min
Response: 15291085
Conc: 18.86 ng/ml

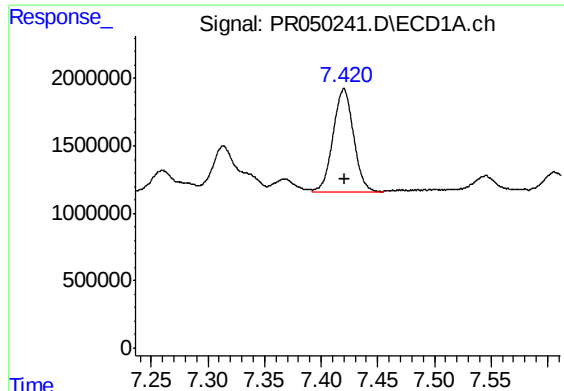

#31 AR-1260-1


R.T.: 7.420 min
Delta R.T.: 0.000 min
Response: 9527649
Conc: 36.12 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

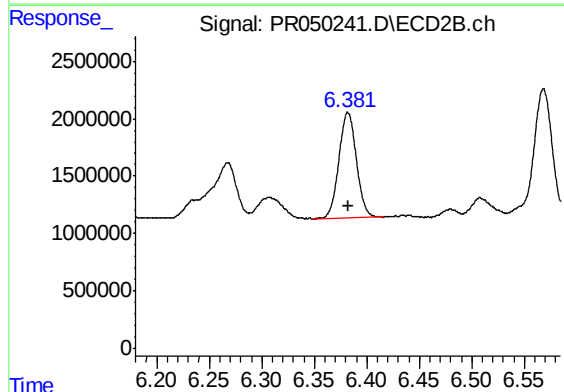


#31 AR-1260-1

R.T.: 6.382 min
Delta R.T.: 0.000 min
Response: 10681629
Conc: 32.11 ng/ml

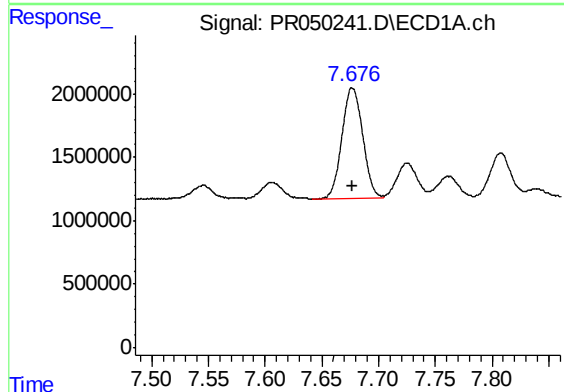


#32 AR-1260-2

R.T.: 7.677 min
Delta R.T.: 0.000 min
Response: 11241369
Conc: 34.87 ng/ml

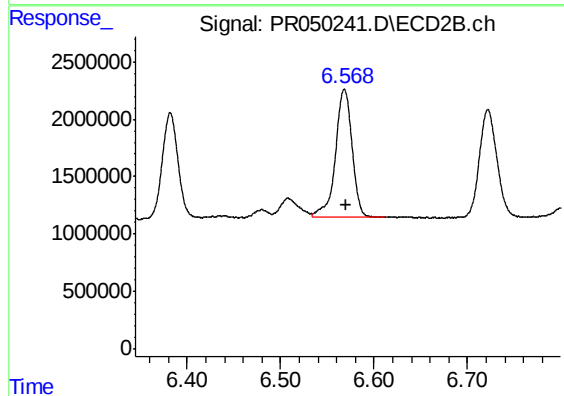

#32 AR-1260-2


R.T.: 6.568 min
Delta R.T.: -0.001 min
Response: 13860588
Conc: 33.49 ng/ml



#33 AR-1260-3


R.T.: 8.036 min
Delta R.T.: 0.000 min
Response: 7010460
Conc: 28.48 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

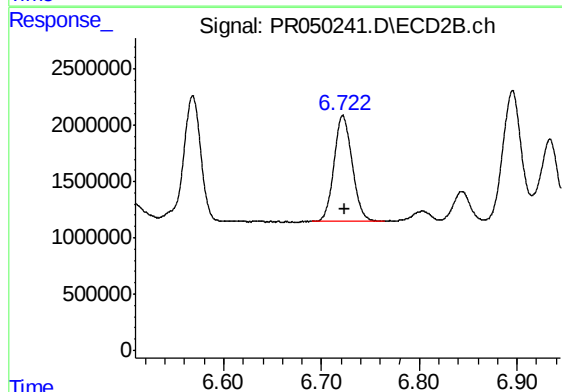


#33 AR-1260-3

R.T.: 6.722 min
Delta R.T.: -0.002 min
Response: 12077833
Conc: 30.55 ng/ml




#34 AR-1260-4

R.T.: 8.270 min
Delta R.T.: -0.001 min
Response: 8863510
Conc: 30.27 ng/ml

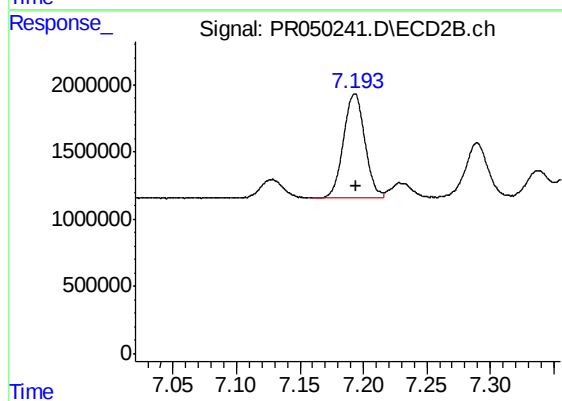

#34 AR-1260-4


R.T.: 7.193 min
Delta R.T.: -0.001 min
Response: 8992098
Conc: 26.02 ng/ml

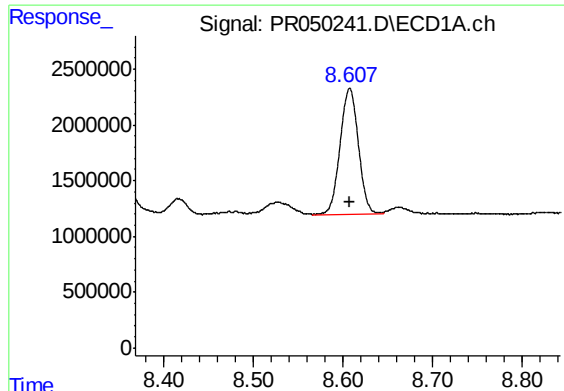

#35 AR-1260-5


R.T.: 8.607 min
Delta R.T.: 0.000 min
Response: 16038829
Conc: 26.56 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

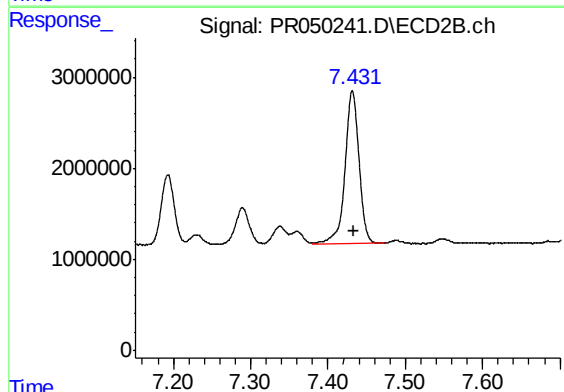


#35 AR-1260-5

R.T.: 7.432 min
Delta R.T.: -0.002 min
Response: 21171699
Conc: 24.43 ng/ml

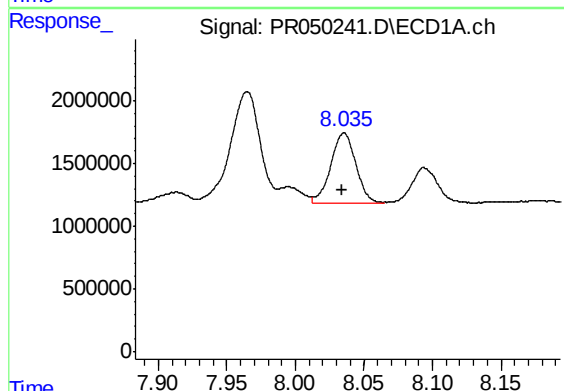


#36 AR-1262-1

R.T.: 8.036 min
Delta R.T.: 0.002 min
Response: 7010460
Conc: 14.19 ng/ml

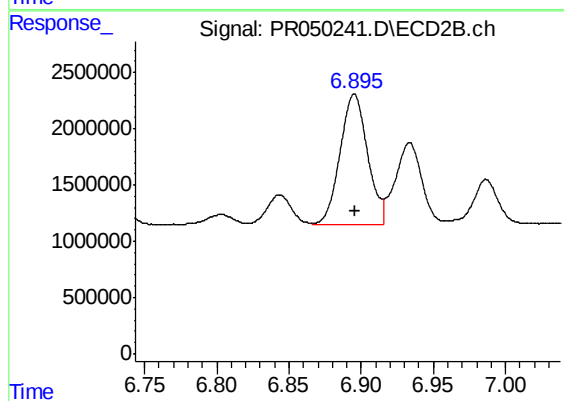

#36 AR-1262-1


R.T.: 6.895 min
Delta R.T.: 0.000 min
Response: 15291085
Conc: 46.50 ng/ml

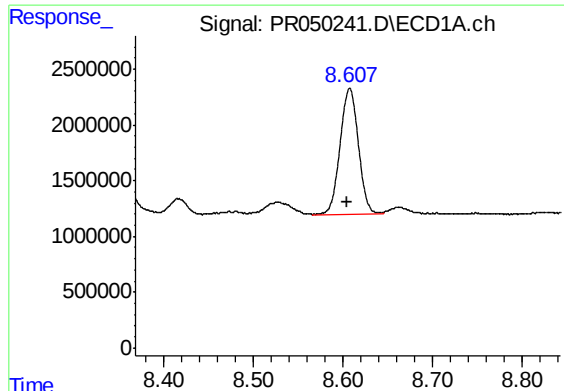

#37 AR-1262-2


R.T.: 8.607 min
Delta R.T.: 0.003 min
Response: 16038829
Conc: 17.53 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

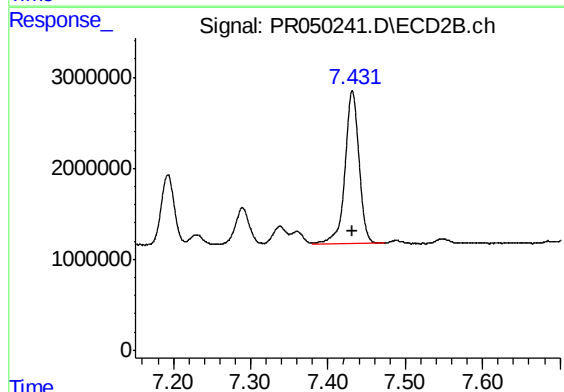


#37 AR-1262-2

R.T.: 7.432 min
Delta R.T.: 0.000 min
Response: 21171699
Conc: 17.33 ng/ml

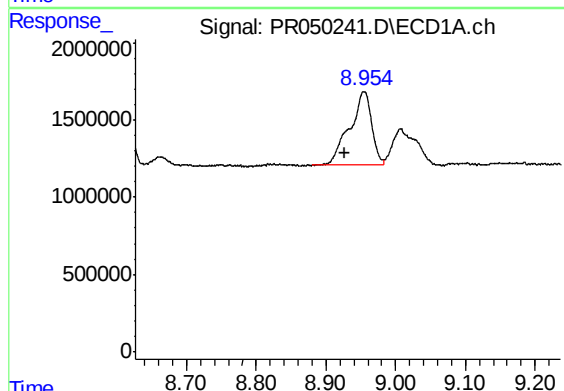


#38 AR-1262-3

R.T.: 8.954 min
Delta R.T.: 0.028 min
Response: 10556943
Conc: 17.48 ng/ml

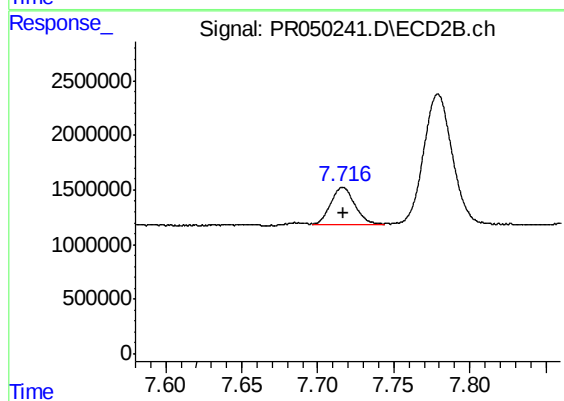

#38 AR-1262-3


R.T.: 7.716 min
Delta R.T.: 0.000 min
Response: 3840704
Conc: 8.55 ng/ml



#39 AR-1262-4


R.T.: 9.007 min
Delta R.T.: -0.017 min
Response: 5719991
Conc: 12.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

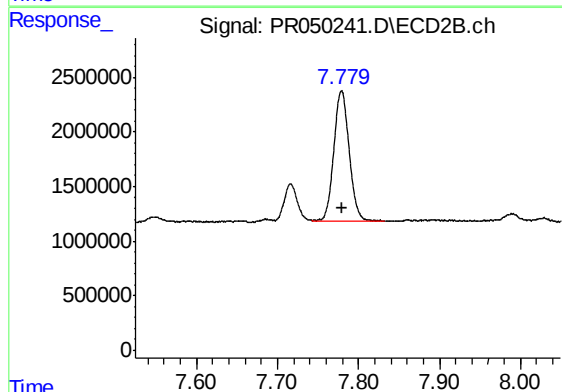


#39 AR-1262-4

R.T.: 7.779 min
Delta R.T.: 0.000 min
Response: 15710645
Conc: 17.60 ng/ml




#40 AR-1262-5

R.T.: 9.721 min
Delta R.T.: 0.003 min
Response: 4158407
Conc: 12.87 ng/ml

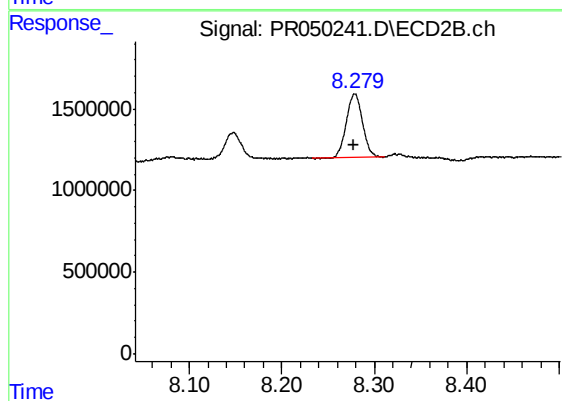

#40 AR-1262-5


R.T.: 8.279 min
Delta R.T.: 0.001 min
Response: 4727124
Conc: 11.55 ng/ml

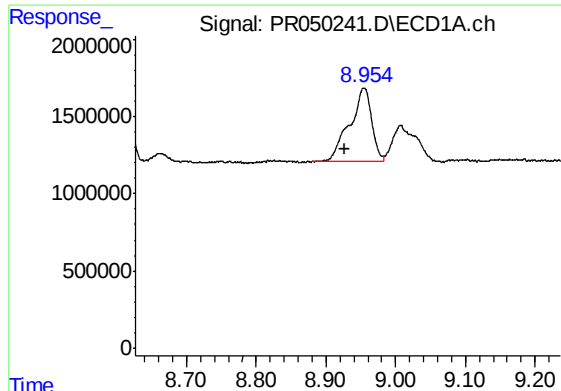

#41 AR-1268-1


R.T.: 8.954 min
Delta R.T.: 0.028 min
Response: 10556943
Conc: 9.37 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

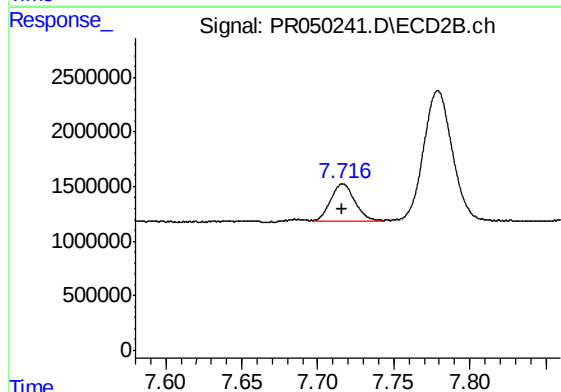


#41 AR-1268-1

R.T.: 7.716 min
Delta R.T.: 0.000 min
Response: 3840704
Conc: 2.67 ng/ml

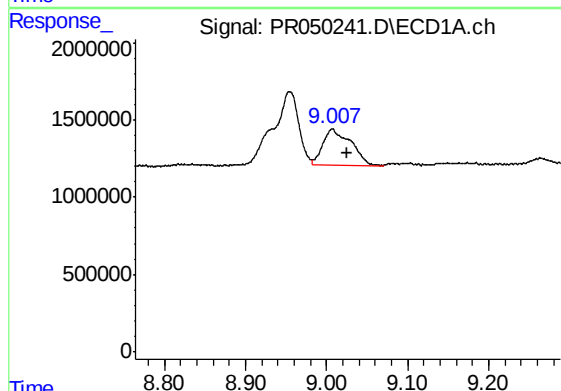


#42 AR-1268-2

R.T.: 9.007 min
Delta R.T.: -0.019 min
Response: 5719991
Conc: 5.60 ng/ml

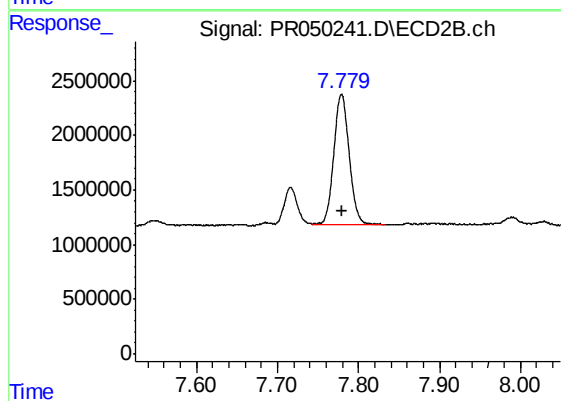

#42 AR-1268-2


R.T.: 7.779 min
Delta R.T.: -0.001 min
Response: 15710645
Conc: 11.74 ng/ml



#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.261 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

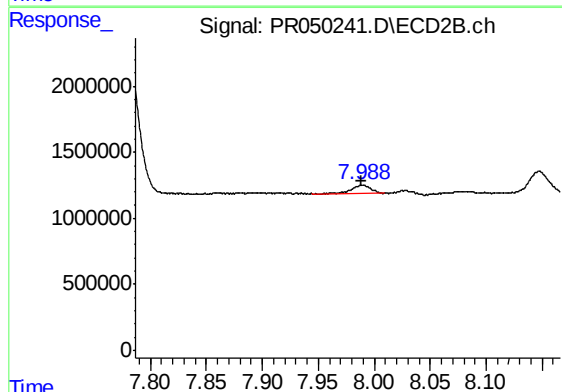


#43 AR-1268-3

R.T.: 7.989 min
Delta R.T.: 0.000 min
Response: 760118
Conc: 0.68 ng/ml




#44 AR-1268-4

R.T.: 9.721 min
Delta R.T.: 0.003 min
Response: 4158407
Conc: 10.95 ng/ml

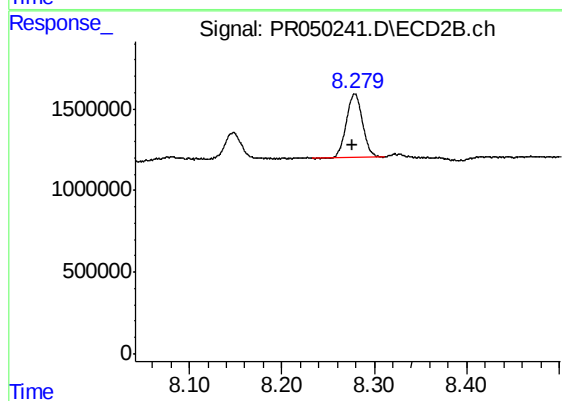

#44 AR-1268-4


R.T.: 8.279 min
Delta R.T.: 0.002 min
Response: 4727124
Conc: 9.86 ng/ml

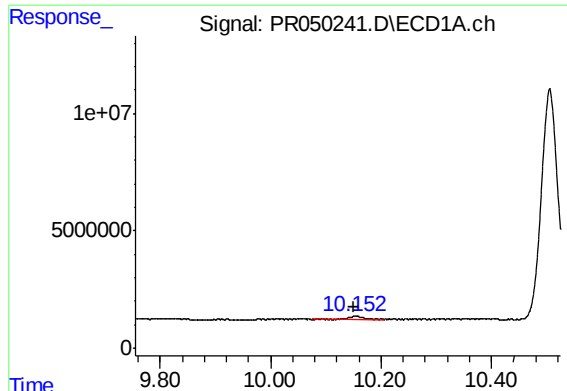

#45 AR-1268-5

R.T.: 10.154 min
Delta R.T.: 0.005 min
Response: 2396799
Conc: 0.81 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-QT3-2021-05

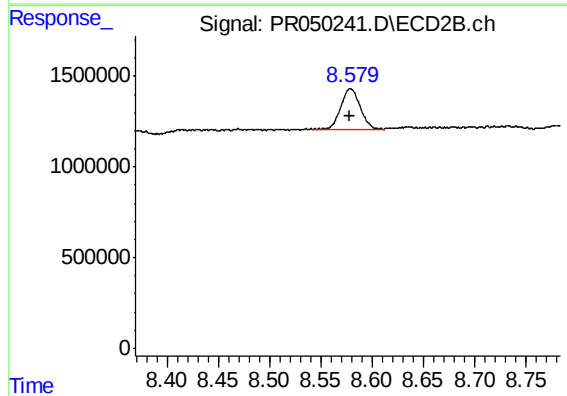

#45 AR-1268-5

R.T.: 8.579 min
Delta R.T.: 0.001 min
Response: 2911964
Conc: 0.80 ng/ml