

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR051519\
 Data File : PR037948.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2019 19:04
 Operator : SM\MA
 Sample : K2241-09
 Misc : AR1660 MDL 25PPB
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 04:23:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR051119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun May 12 00:51:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.792	4.640	31289013	94177695	17.363	18.676
2)	SA Decachlor...	8.778	10.400	50938557	111.0E6	26.699	24.395
Target Compounds							
3)	L1 AR-1016-1	4.865	5.794	2247257	5084184	28.822	27.031
4)	L1 AR-1016-2	4.884	5.816	2797236	7544398	25.951	27.852
5)	L1 AR-1016-3	5.058	5.877	1466036	4571208	25.847	28.077
6)	L1 AR-1016-4	5.098	5.977	1091276	3852604	23.877	27.982
7)	L1 AR-1016-5	5.310	6.266	2535815	3884448	40.886	28.596 #
9)	L2 AR-1221-2	4.089	0.000	947855	0	60.132	N.D. #
10)	L2 AR-1221-3	4.162	5.005	887060	2125539	17.589	16.482
11)	L3 AR-1232-1	4.162	5.005	887060	2125539	16.102	14.719
12)	L3 AR-1232-2	4.884	5.531	2797236	3010048	41.123	38.322
13)	L3 AR-1232-3	5.058	5.816	1466036	7544398	41.482	44.450
14)	L3 AR-1232-4	5.140	5.977	1176271	3852604	38.127	45.210
15)	L3 AR-1232-5	5.310	6.063	2535815	2800174	72.198	46.455 #
16)	L4 AR-1242-1	4.865	5.794	2247257	5084184	37.036	34.958
17)	L4 AR-1242-2	4.884	5.816	2797236	7544398	33.578	35.887
18)	L4 AR-1242-3	5.058	5.877	1466036	4571208	32.968	35.854
19)	L4 AR-1242-4	5.140	5.977	1176271	3852604	27.446	36.028 #
20)	L4 AR-1242-5	5.657	6.639	1093751	3375909	17.577	27.290 #
21)	L5 AR-1248-1	4.865	5.794	2247257	5084184	47.119	44.673
22)	L5 AR-1248-2	5.098	6.063	1091276	2800174	17.686	18.068
23)	L5 AR-1248-3	5.140	6.266	1176271	3884448	18.572	21.313
24)	L5 AR-1248-4	5.310	6.639	2535815	3375909	31.468	15.446 #
25)	L5 AR-1248-5	5.657	6.639	1093751	3375909	12.872	16.218 #
26)	L6 AR-1254-1	5.657	6.639	1093751	3375909	7.388	14.017 #
27)	L6 AR-1254-2	5.802	6.852	1464783	3160808	11.375	8.279 #
28)	L6 AR-1254-3	6.217	7.225	3228642	9452757	14.626	22.367 #
29)	L6 AR-1254-4	6.458	7.495	1163776	4081283	7.687	13.210 #
30)	L6 AR-1254-5	6.842	7.913	5355547	11774150	27.333	35.243 #
31)	L7 AR-1260-1	6.332	7.379	5186951	17342713	43.222	70.075 #
32)	L7 AR-1260-2	6.516	7.631	6240165	9590975	39.808	32.607
33)	L7 AR-1260-3	6.671	7.986	5614689	7328427	42.469	33.565
34)	L7 AR-1260-4	7.139	8.217	3436466	8500584	32.253	33.268
35)	L7 AR-1260-5	7.378	8.545	9170546	17129875	32.643	32.973
36)	L8 AR-1262-1	6.933	7.986	2178559	7328427	32.590	23.195 #
37)	L8 AR-1262-2	7.378	8.545	9170546	17129875	28.078	27.492
38)	L8 AR-1262-3	7.662	8.883	2530384	11245687	20.199	26.830 #
39)	L8 AR-1262-4	7.724	8.939	8657939	6669216	37.236	20.900 #
40)	L8 AR-1262-5	8.222	9.631	2219755	4676471	20.691	18.781
41)	L9 AR-1268-1	7.662	8.883	2530384	11245687	5.807	11.224 #
42)	L9 AR-1268-2	7.724	8.939	8657939	6669216	22.015	7.377 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR051519\
 Data File : PR037948.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2019 19:04
 Operator : SM\MA
 Sample : K2241-09
 Misc : AR1660 MDL 25PPB
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 04:23:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR051119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun May 12 00:51:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	8.222	9.631	2219755	4676471	17.302	13.754
45) L9	AR-1268-5	8.519	0.000	1373664	0	1.474	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR051519\
Data File : PR037948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2019 19:04
Operator : SM\MA
Sample : K2241-09
Misc : AR1660 MDL 25PPB
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 04:23:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR051119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun May 12 00:51:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

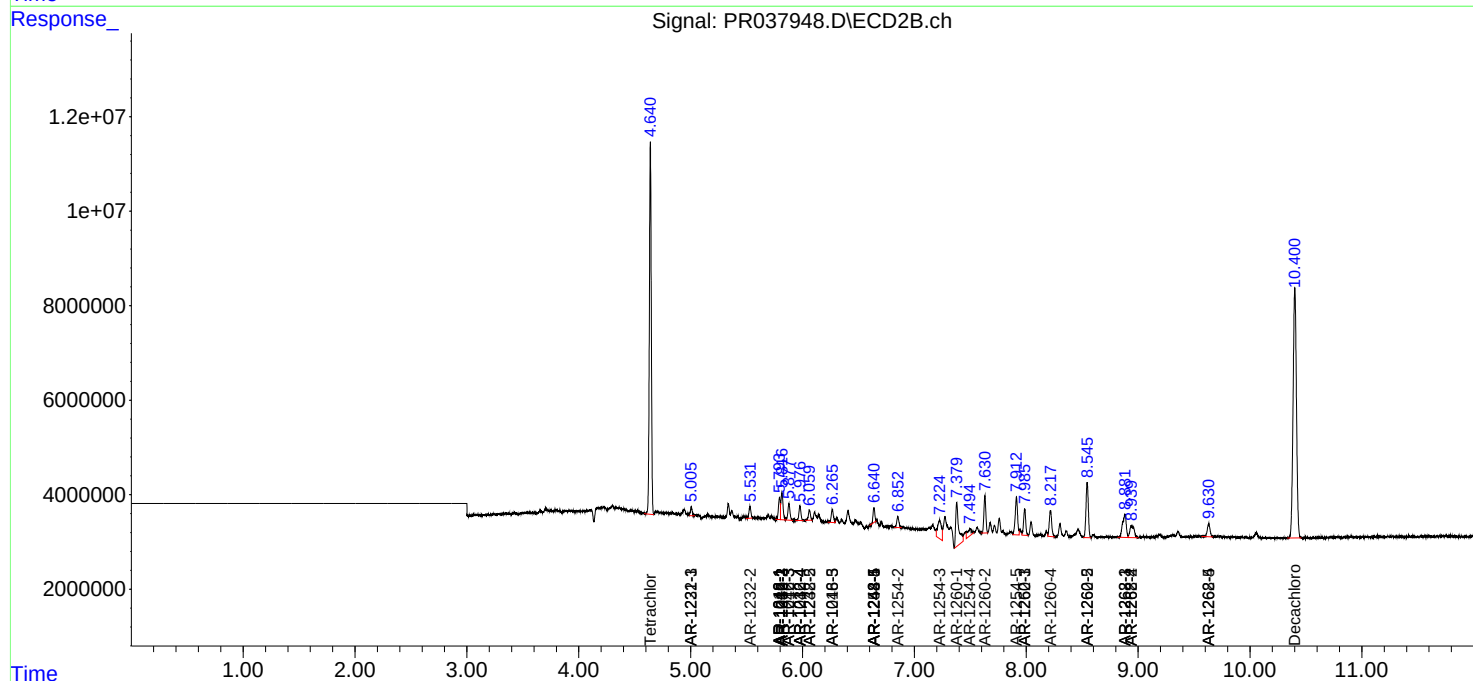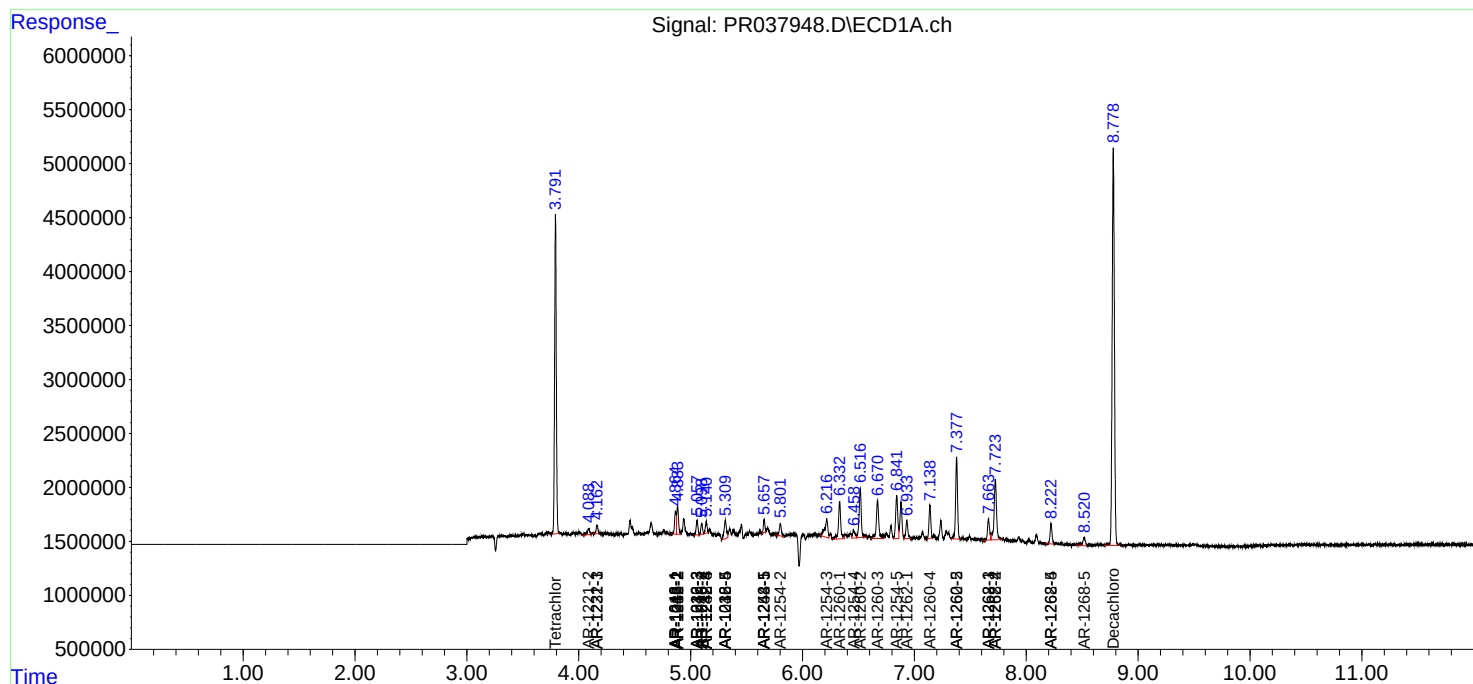


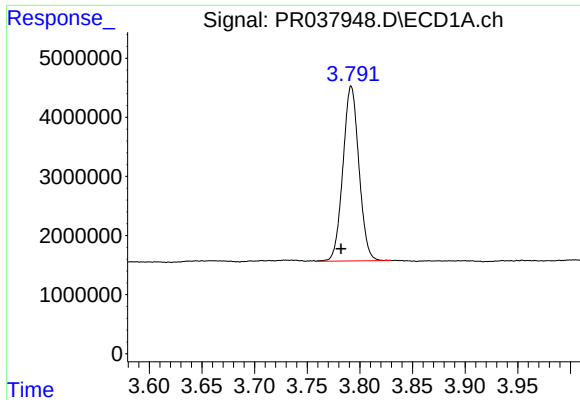

#1 Tetrachloro-m-xylene


R.T.: 3.792 min
Delta R.T.: 0.010 min
Response: 31289013
Conc: 17.36 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

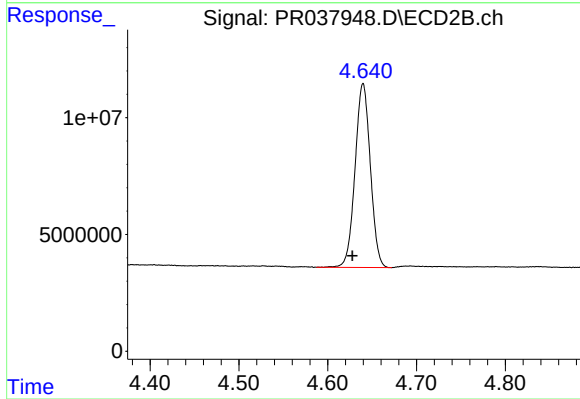


#1 Tetrachloro-m-xylene

R.T.: 4.640 min
Delta R.T.: 0.012 min
Response: 94177695
Conc: 18.68 ng/ml

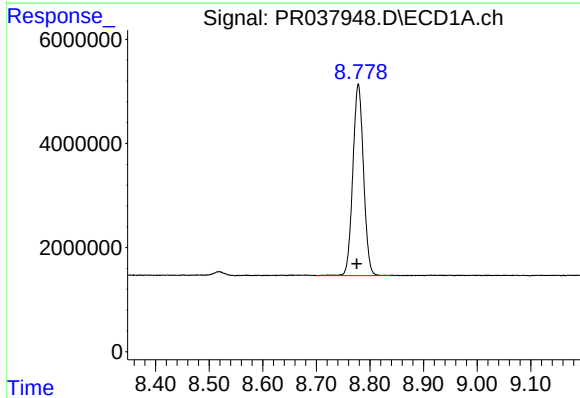


#2 Decachlorobiphenyl

R.T.: 8.778 min
Delta R.T.: 0.003 min
Response: 50938557
Conc: 26.70 ng/ml

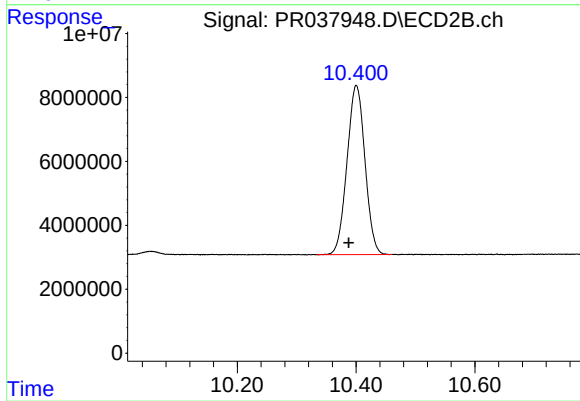

#2 Decachlorobiphenyl


R.T.: 10.400 min
Delta R.T.: 0.013 min
Response: 110953391
Conc: 24.40 ng/ml

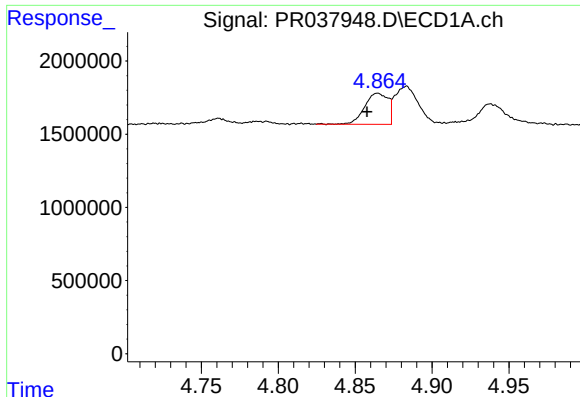

#3 AR-1016-1


R.T.: 4.865 min
Delta R.T.: 0.007 min
Response: 2247257
Conc: 28.82 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

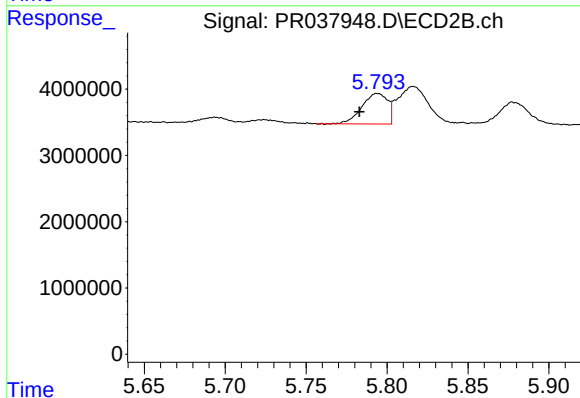


#3 AR-1016-1

R.T.: 5.794 min
Delta R.T.: 0.011 min
Response: 5084184
Conc: 27.03 ng/ml

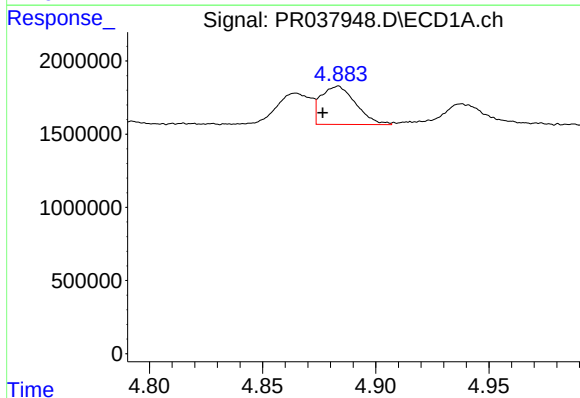


#4 AR-1016-2

R.T.: 4.884 min
Delta R.T.: 0.007 min
Response: 2797236
Conc: 25.95 ng/ml

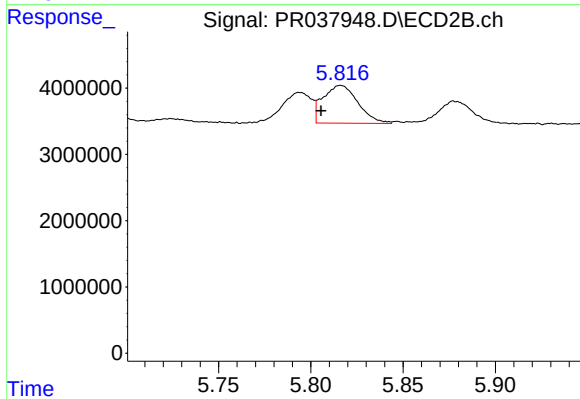

#4 AR-1016-2


R.T.: 5.816 min
Delta R.T.: 0.010 min
Response: 7544398
Conc: 27.85 ng/ml

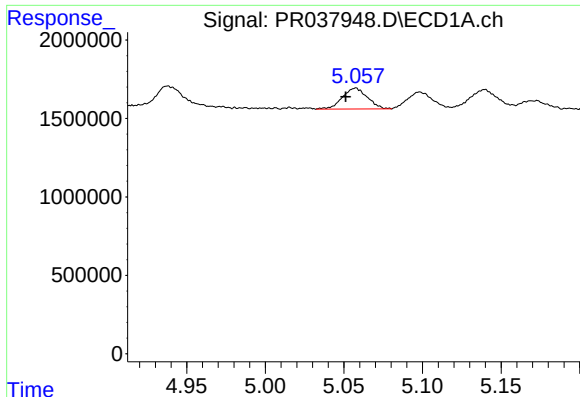

#5 AR-1016-3


R.T.: 5.058 min
Delta R.T.: 0.006 min
Response: 1466036
Conc: 25.85 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

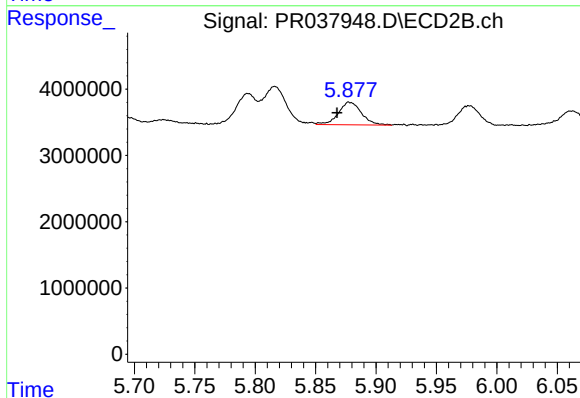


#5 AR-1016-3

R.T.: 5.877 min
Delta R.T.: 0.009 min
Response: 4571208
Conc: 28.08 ng/ml

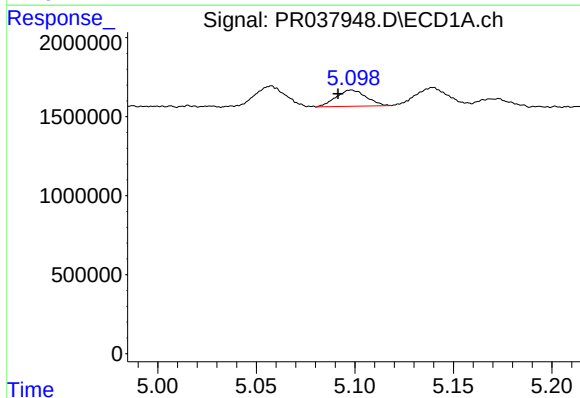


#6 AR-1016-4

R.T.: 5.098 min
Delta R.T.: 0.007 min
Response: 1091276
Conc: 23.88 ng/ml

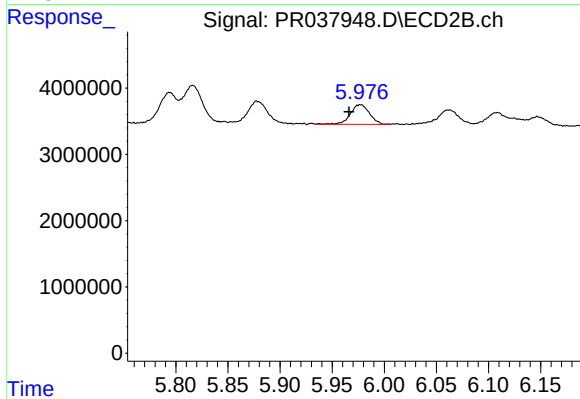

#6 AR-1016-4


R.T.: 5.977 min
Delta R.T.: 0.011 min
Response: 3852604
Conc: 27.98 ng/ml

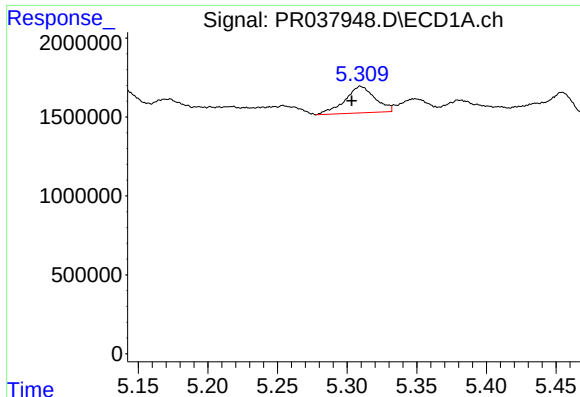

#7 AR-1016-5


R.T.: 5.310 min
Delta R.T.: 0.006 min
Response: 2535815
Conc: 40.89 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

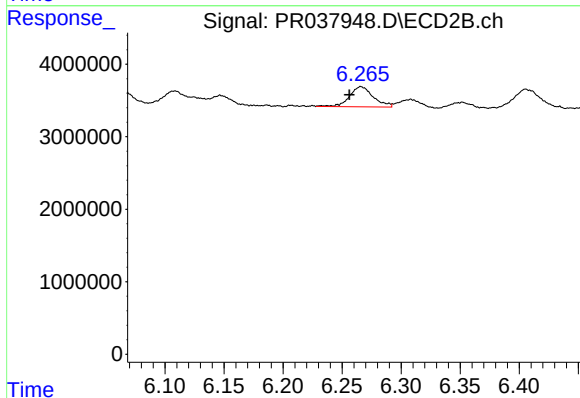


#7 AR-1016-5

R.T.: 6.266 min
Delta R.T.: 0.010 min
Response: 3884448
Conc: 28.60 ng/ml

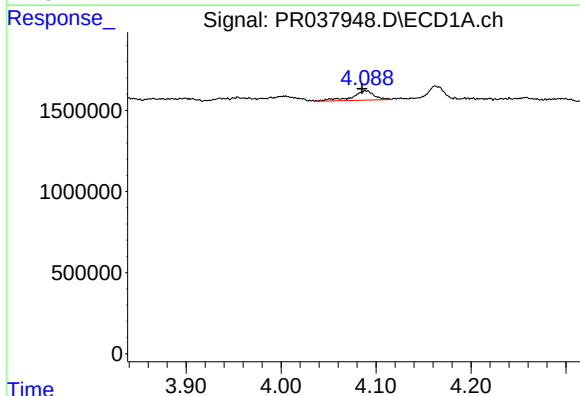


#9 AR-1221-2

R.T.: 4.089 min
Delta R.T.: 0.003 min
Response: 947855
Conc: 60.13 ng/ml

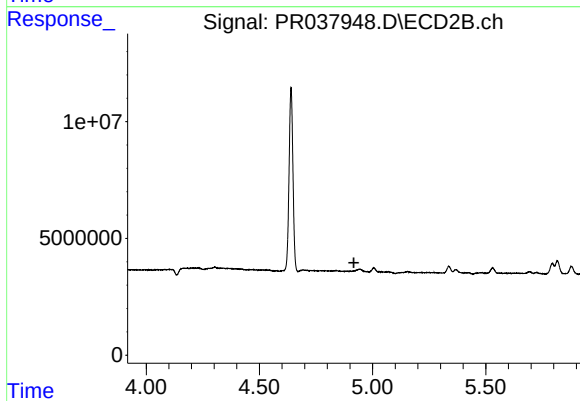

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.917 min
Response: 0
Conc: N.D.

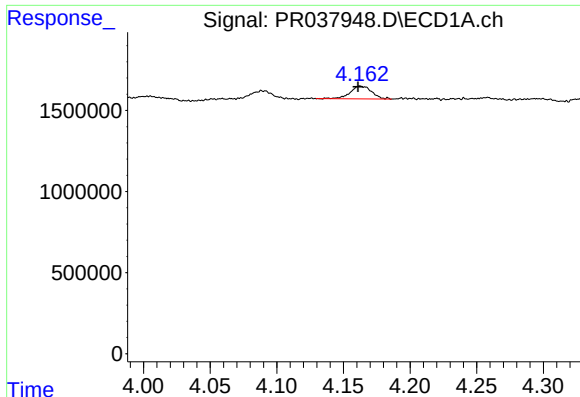

#10 AR-1221-3


R.T.: 4.162 min
Delta R.T.: 0.001 min
Response: 887060
Conc: 17.59 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

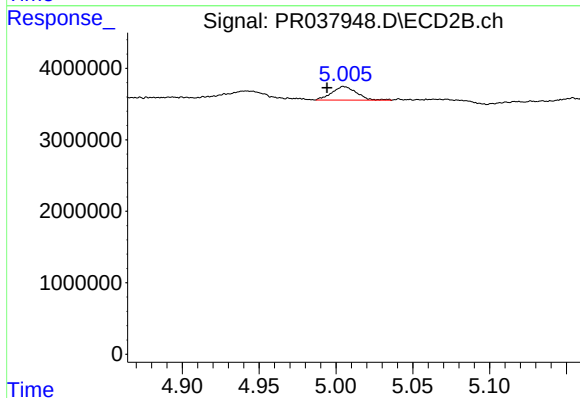


#10 AR-1221-3

R.T.: 5.005 min
Delta R.T.: 0.011 min
Response: 2125539
Conc: 16.48 ng/ml

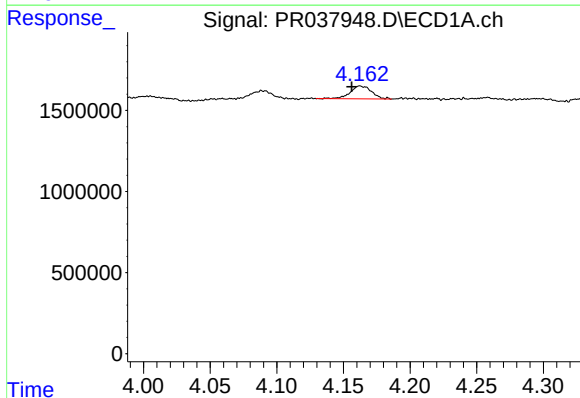


#11 AR-1232-1

R.T.: 4.162 min
Delta R.T.: 0.006 min
Response: 887060
Conc: 16.10 ng/ml

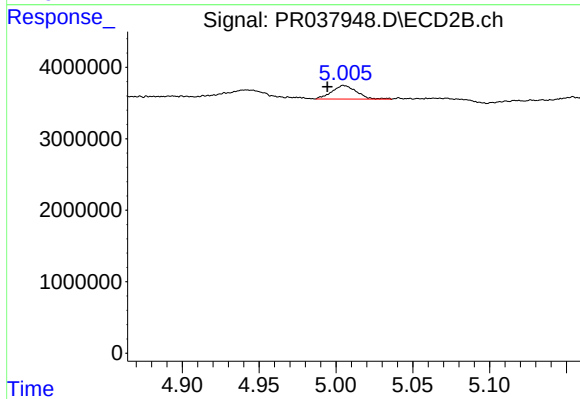

#11 AR-1232-1


R.T.: 5.005 min
Delta R.T.: 0.010 min
Response: 2125539
Conc: 14.72 ng/ml

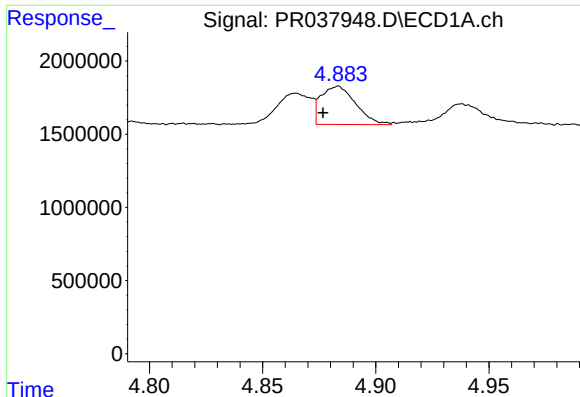

#12 AR-1232-2


R.T.: 4.884 min
Delta R.T.: 0.007 min
Response: 2797236
Conc: 41.12 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

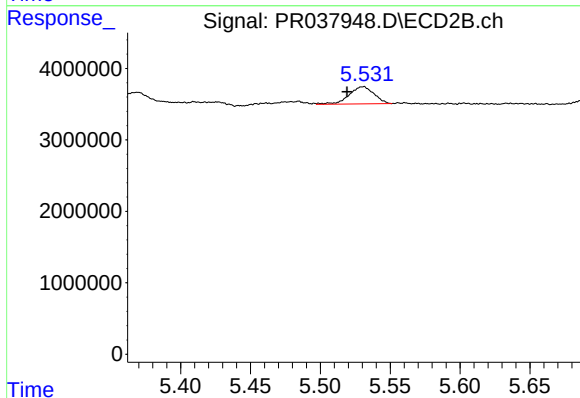


#12 AR-1232-2

R.T.: 5.531 min
Delta R.T.: 0.012 min
Response: 3010048
Conc: 38.32 ng/ml

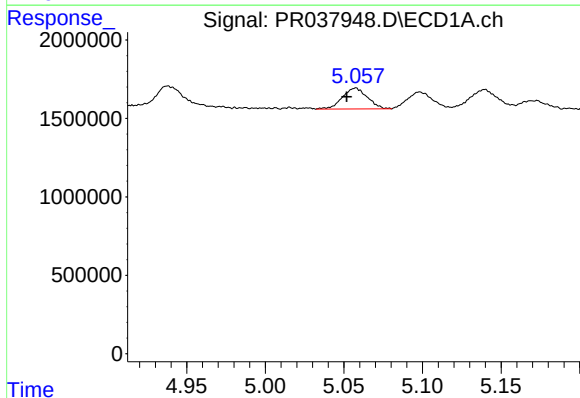


#13 AR-1232-3

R.T.: 5.058 min
Delta R.T.: 0.006 min
Response: 1466036
Conc: 41.48 ng/ml

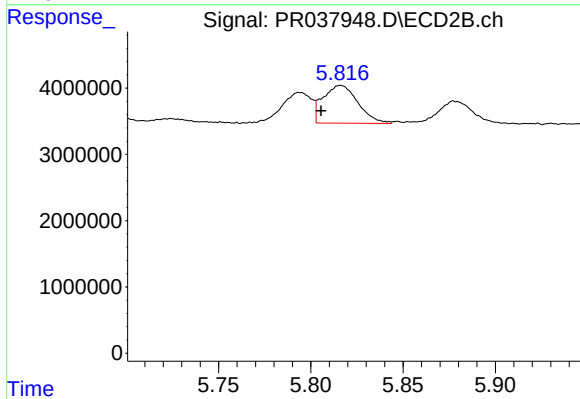

#13 AR-1232-3


R.T.: 5.816 min
Delta R.T.: 0.011 min
Response: 7544398
Conc: 44.45 ng/ml

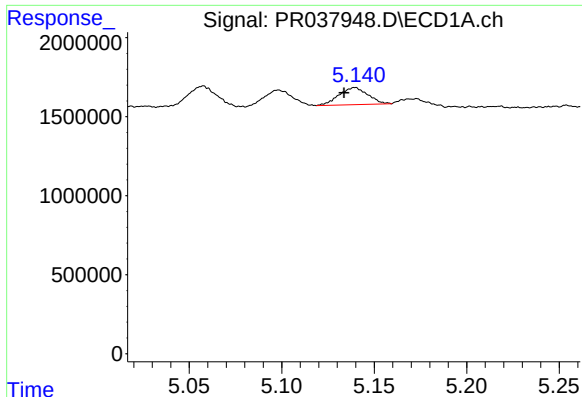

#14 AR-1232-4


R.T.: 5.140 min
Delta R.T.: 0.006 min
Response: 1176271
Conc: 38.13 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

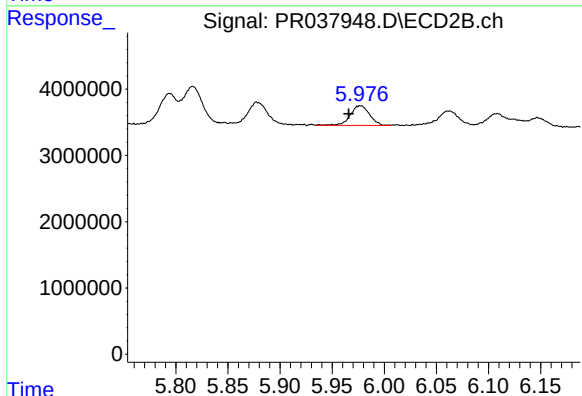


#14 AR-1232-4

R.T.: 5.977 min
Delta R.T.: 0.011 min
Response: 3852604
Conc: 45.21 ng/ml

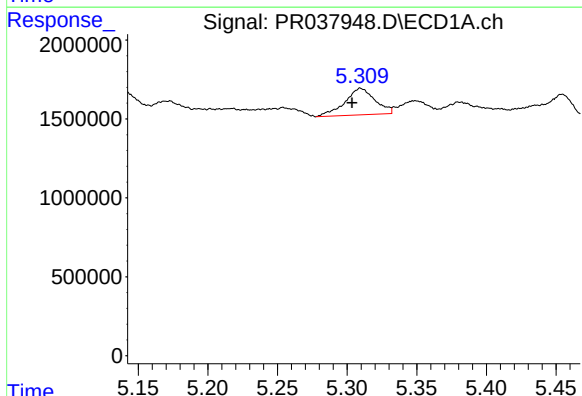


#15 AR-1232-5

R.T.: 5.310 min
Delta R.T.: 0.006 min
Response: 2535815
Conc: 72.20 ng/ml

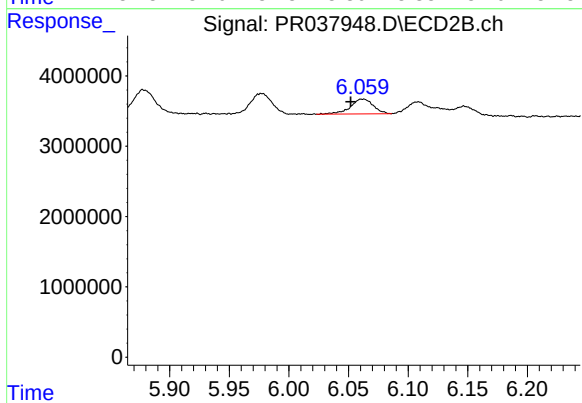

#15 AR-1232-5


R.T.: 6.063 min
Delta R.T.: 0.011 min
Response: 2800174
Conc: 46.45 ng/ml

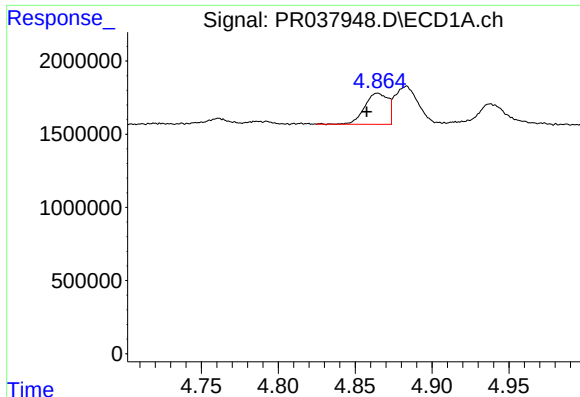

#16 AR-1242-1


R.T.: 4.865 min
Delta R.T.: 0.007 min
Response: 2247257
Conc: 37.04 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

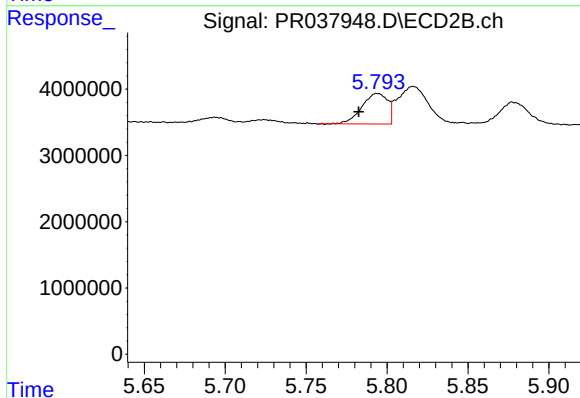


#16 AR-1242-1

R.T.: 5.794 min
Delta R.T.: 0.011 min
Response: 5084184
Conc: 34.96 ng/ml

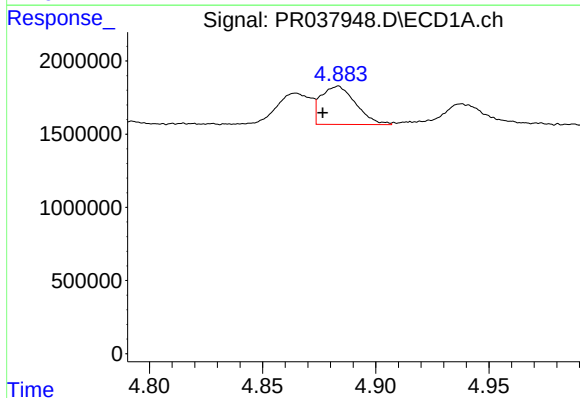


#17 AR-1242-2

R.T.: 4.884 min
Delta R.T.: 0.007 min
Response: 2797236
Conc: 33.58 ng/ml

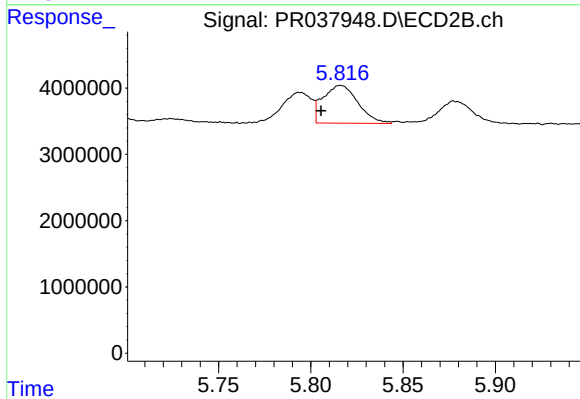

#17 AR-1242-2


R.T.: 5.816 min
Delta R.T.: 0.011 min
Response: 7544398
Conc: 35.89 ng/ml

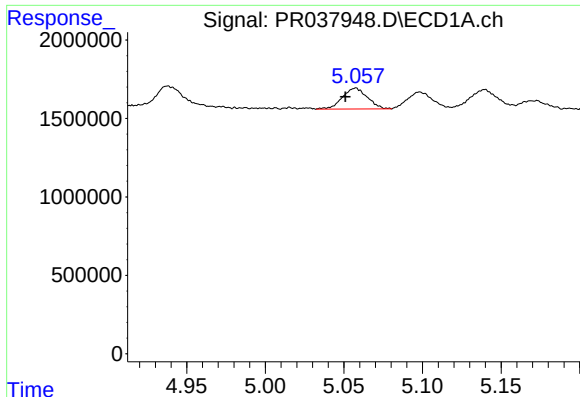

#18 AR-1242-3


R.T.: 5.058 min
Delta R.T.: 0.007 min
Response: 1466036
Conc: 32.97 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

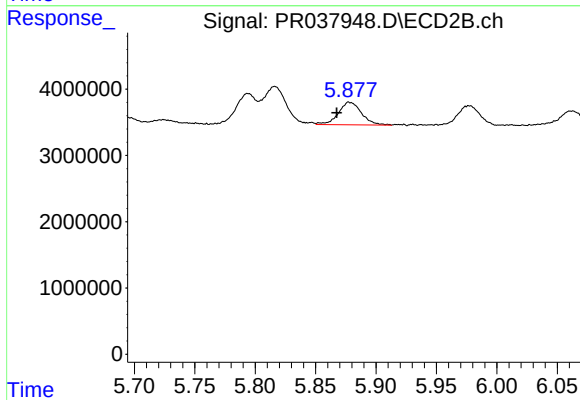


#18 AR-1242-3

R.T.: 5.877 min
Delta R.T.: 0.010 min
Response: 4571208
Conc: 35.85 ng/ml

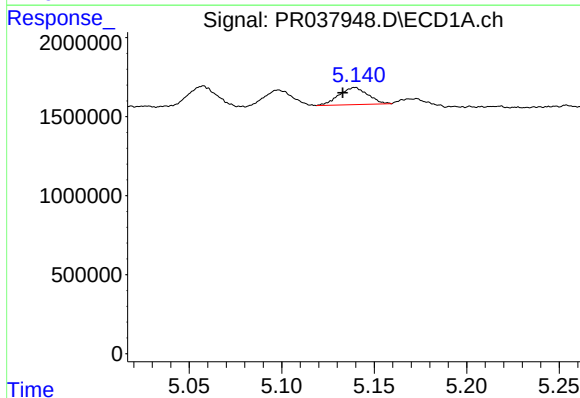


#19 AR-1242-4

R.T.: 5.140 min
Delta R.T.: 0.007 min
Response: 1176271
Conc: 27.45 ng/ml

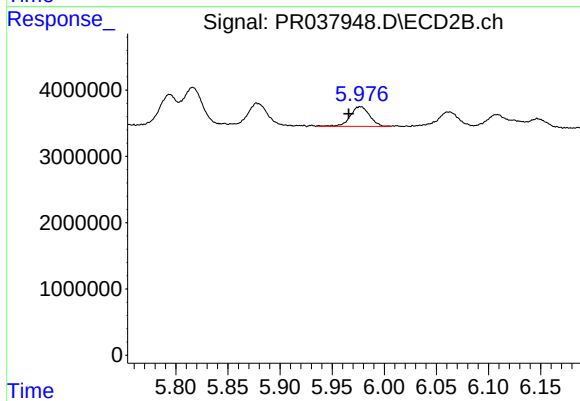

#19 AR-1242-4


R.T.: 5.977 min
Delta R.T.: 0.011 min
Response: 3852604
Conc: 36.03 ng/ml

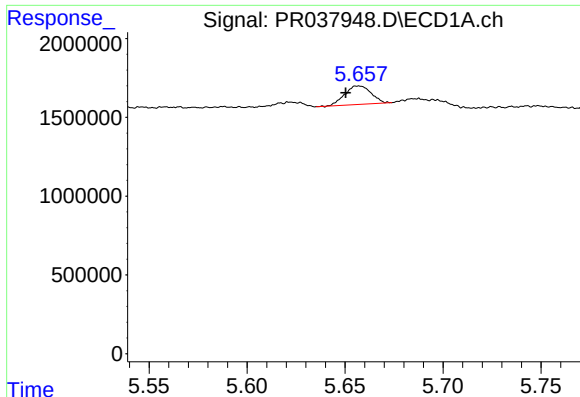

#20 AR-1242-5


R.T.: 5.657 min
Delta R.T.: 0.007 min
Response: 1093751
Conc: 17.58 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

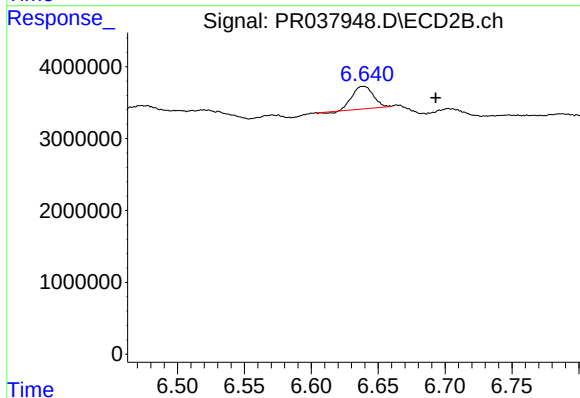


#20 AR-1242-5

R.T.: 6.639 min
Delta R.T.: -0.054 min
Response: 3375909
Conc: 27.29 ng/ml

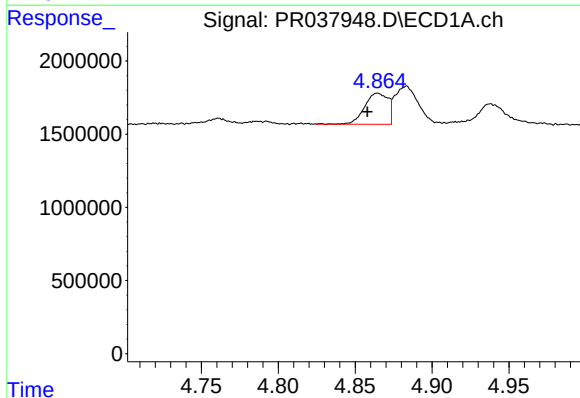


#21 AR-1248-1

R.T.: 4.865 min
Delta R.T.: 0.007 min
Response: 2247257
Conc: 47.12 ng/ml

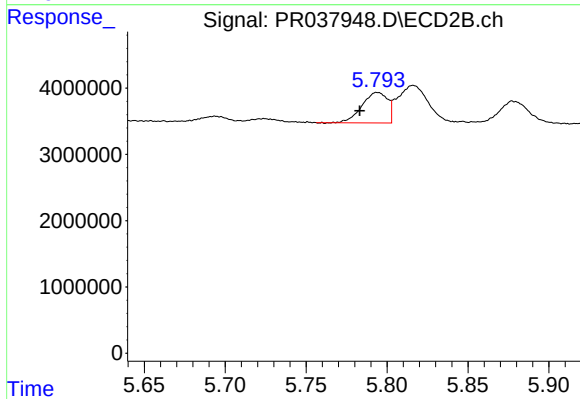

#21 AR-1248-1


R.T.: 5.794 min
Delta R.T.: 0.011 min
Response: 5084184
Conc: 44.67 ng/ml

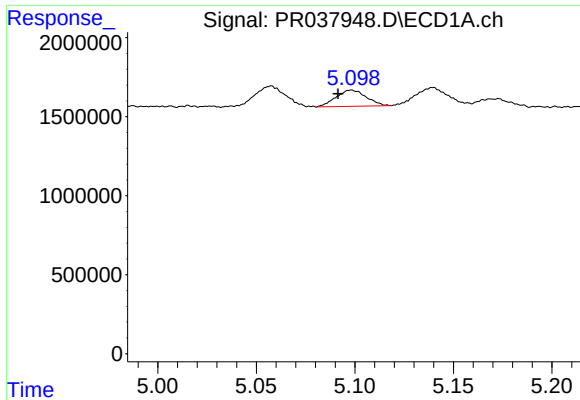

#22 AR-1248-2


R.T.: 5.098 min
Delta R.T.: 0.007 min
Response: 1091276
Conc: 17.69 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

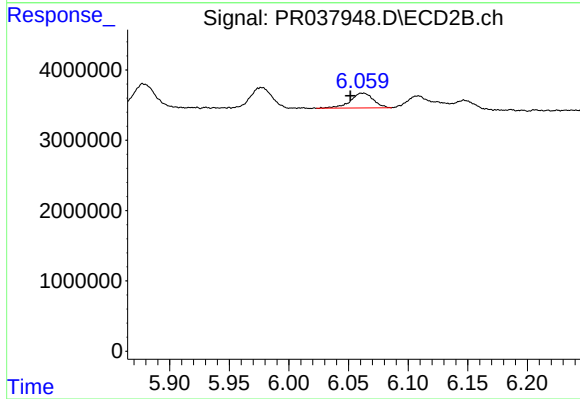


#22 AR-1248-2

R.T.: 6.063 min
Delta R.T.: 0.011 min
Response: 2800174
Conc: 18.07 ng/ml

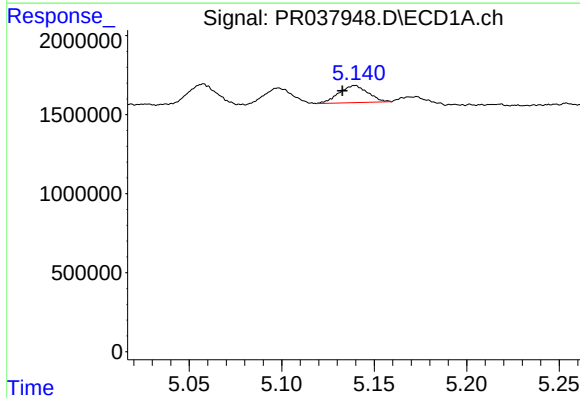


#23 AR-1248-3

R.T.: 5.140 min
Delta R.T.: 0.007 min
Response: 1176271
Conc: 18.57 ng/ml

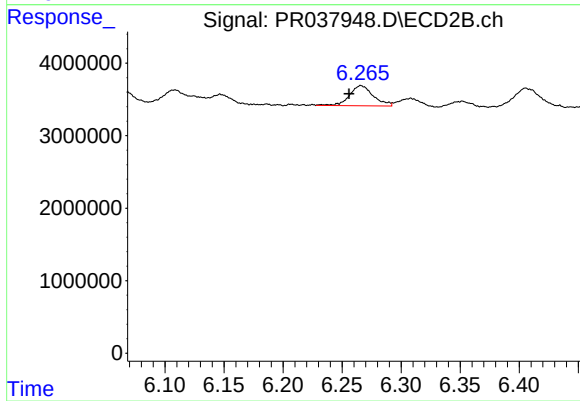

#23 AR-1248-3


R.T.: 6.266 min
Delta R.T.: 0.010 min
Response: 3884448
Conc: 21.31 ng/ml

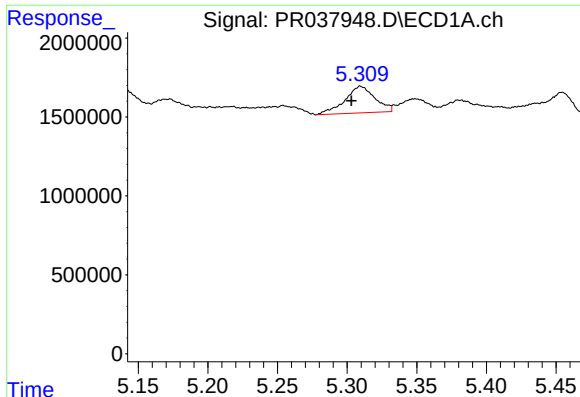

#24 AR-1248-4


R.T.: 5.310 min
Delta R.T.: 0.007 min
Response: 2535815
Conc: 31.47 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

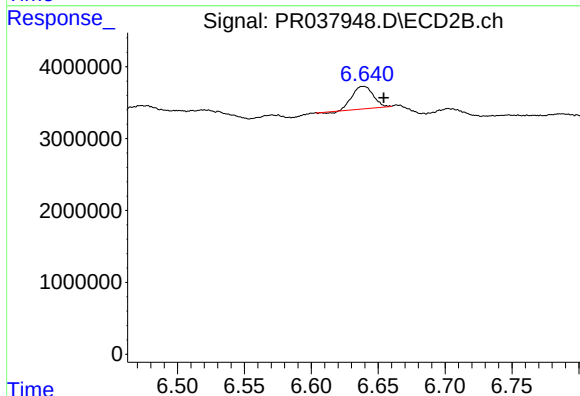


#24 AR-1248-4

R.T.: 6.639 min
Delta R.T.: -0.015 min
Response: 3375909
Conc: 15.45 ng/ml

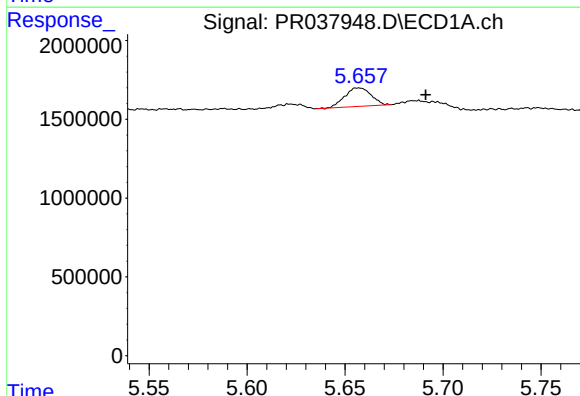


#25 AR-1248-5

R.T.: 5.657 min
Delta R.T.: -0.034 min
Response: 1093751
Conc: 12.87 ng/ml

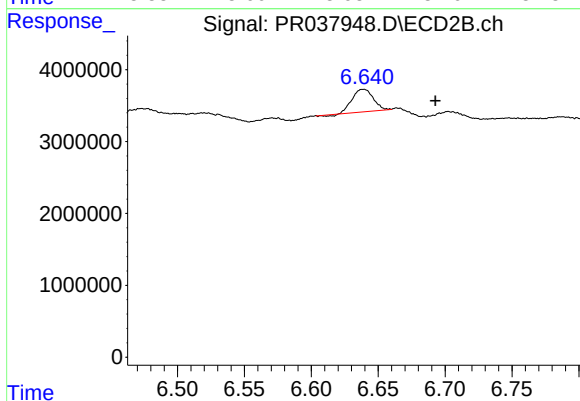

#25 AR-1248-5


R.T.: 6.639 min
Delta R.T.: -0.054 min
Response: 3375909
Conc: 16.22 ng/ml

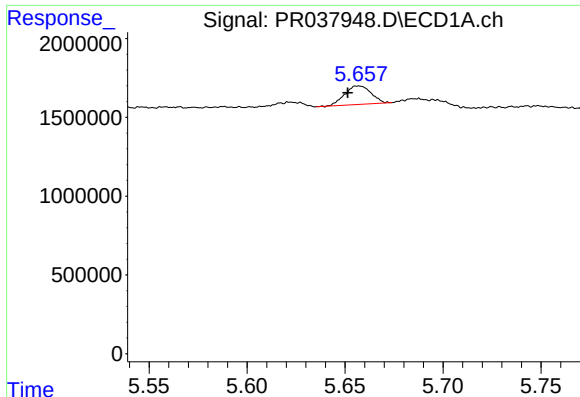

#26 AR-1254-1


R.T.: 5.657 min
Delta R.T.: 0.006 min
Response: 1093751
Conc: 7.39 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

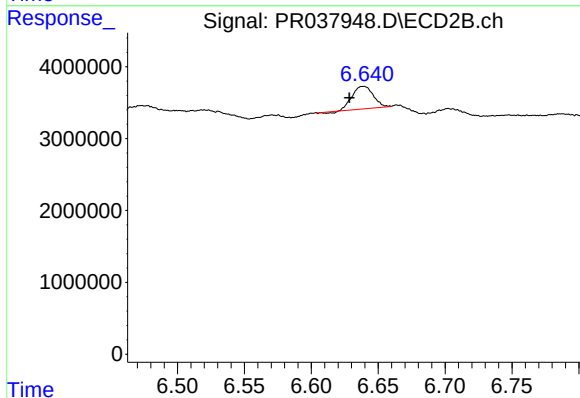


#26 AR-1254-1

R.T.: 6.639 min
Delta R.T.: 0.011 min
Response: 3375909
Conc: 14.02 ng/ml

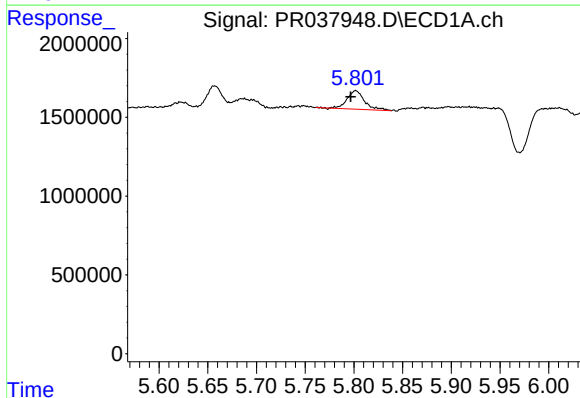


#27 AR-1254-2

R.T.: 5.802 min
Delta R.T.: 0.005 min
Response: 1464783
Conc: 11.38 ng/ml

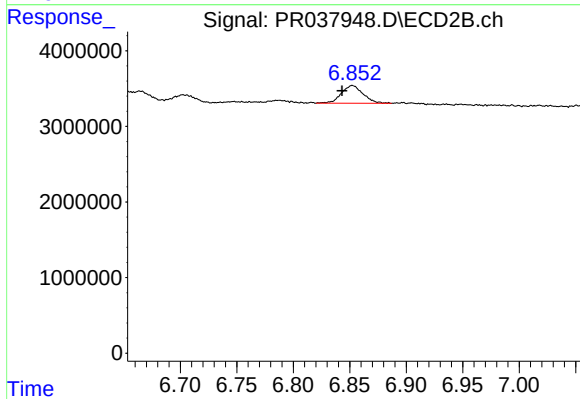

#27 AR-1254-2


R.T.: 6.852 min
Delta R.T.: 0.009 min
Response: 3160808
Conc: 8.28 ng/ml

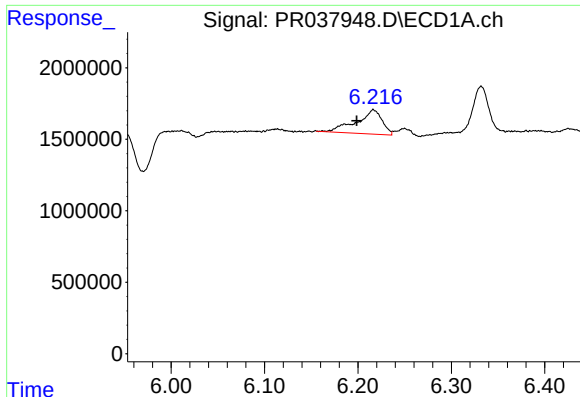

#28 AR-1254-3


R.T.: 6.217 min
Delta R.T.: 0.018 min
Response: 3228642
Conc: 14.63 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

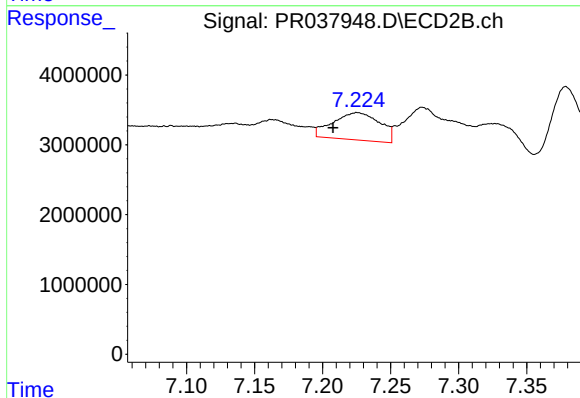


#28 AR-1254-3

R.T.: 7.225 min
Delta R.T.: 0.018 min
Response: 9452757
Conc: 22.37 ng/ml

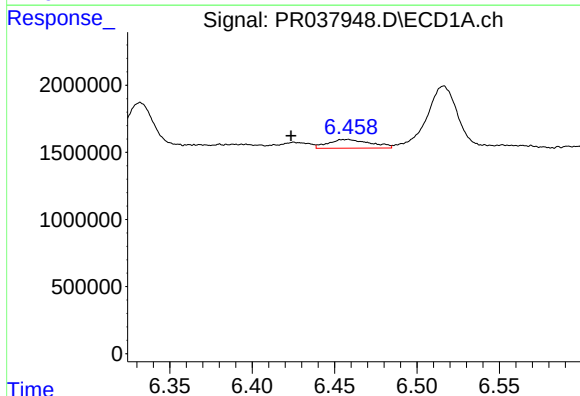


#29 AR-1254-4

R.T.: 6.458 min
Delta R.T.: 0.034 min
Response: 1163776
Conc: 7.69 ng/ml

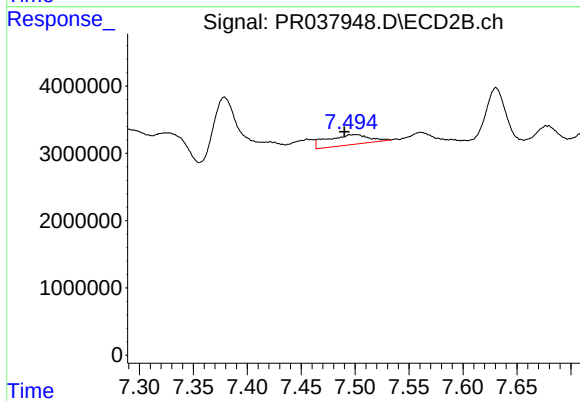

#29 AR-1254-4


R.T.: 7.495 min
Delta R.T.: 0.005 min
Response: 4081283
Conc: 13.21 ng/ml

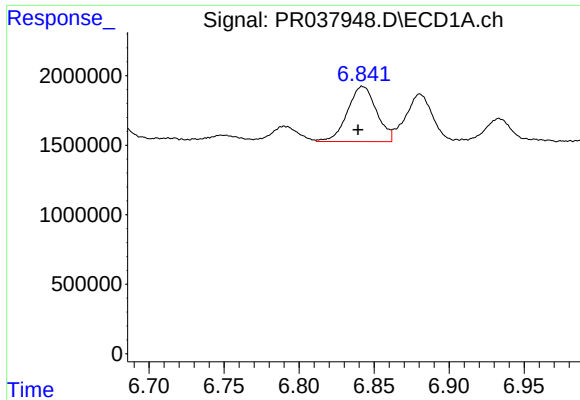

#30 AR-1254-5


R.T.: 6.842 min
Delta R.T.: 0.003 min
Response: 5355547
Conc: 27.33 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

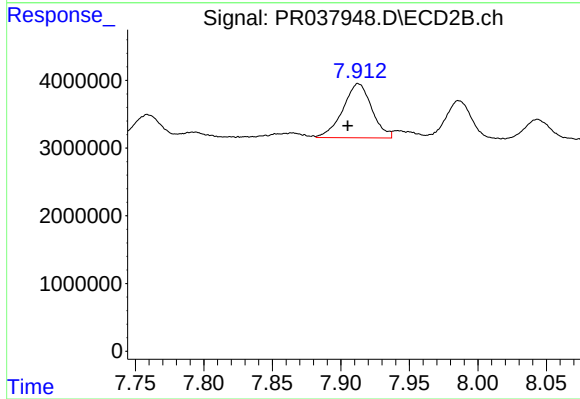


#30 AR-1254-5

R.T.: 7.913 min
Delta R.T.: 0.007 min
Response: 11774150
Conc: 35.24 ng/ml

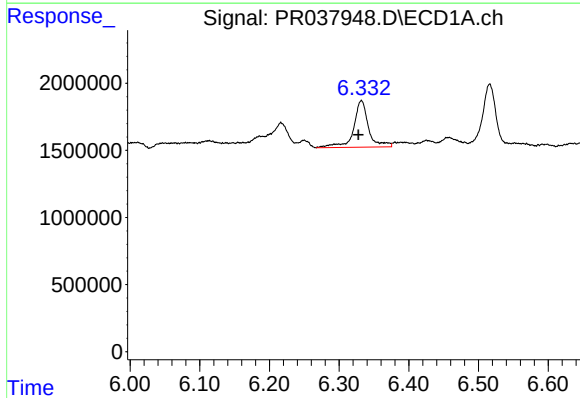


#31 AR-1260-1

R.T.: 6.332 min
Delta R.T.: 0.005 min
Response: 5186951
Conc: 43.22 ng/ml

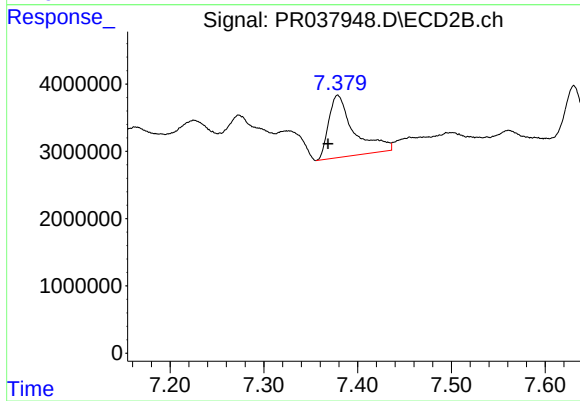

#31 AR-1260-1


R.T.: 7.379 min
Delta R.T.: 0.010 min
Response: 17342713
Conc: 70.08 ng/ml

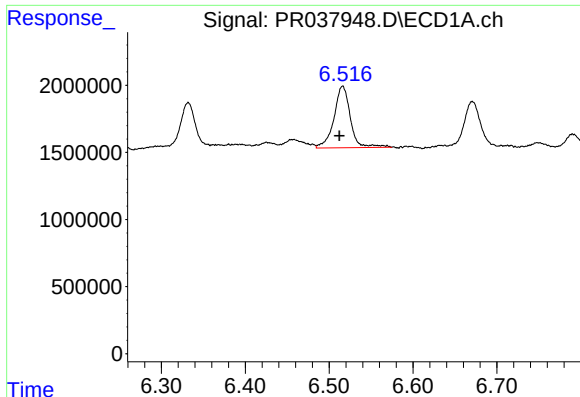

#32 AR-1260-2


R.T.: 6.516 min
Delta R.T.: 0.004 min
Response: 6240165
Conc: 39.81 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

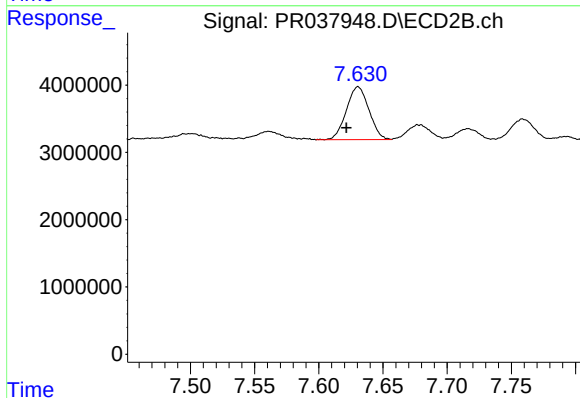


#32 AR-1260-2

R.T.: 7.631 min
Delta R.T.: 0.009 min
Response: 9590975
Conc: 32.61 ng/ml

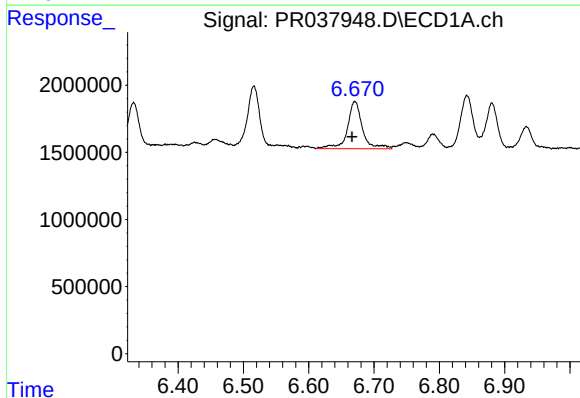


#33 AR-1260-3

R.T.: 6.671 min
Delta R.T.: 0.004 min
Response: 5614689
Conc: 42.47 ng/ml

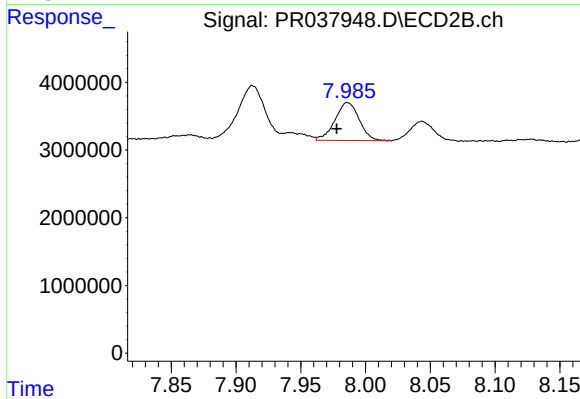

#33 AR-1260-3


R.T.: 7.986 min
Delta R.T.: 0.008 min
Response: 7328427
Conc: 33.57 ng/ml

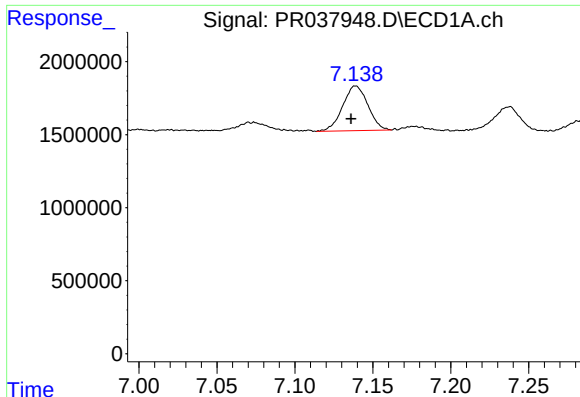

#34 AR-1260-4


R.T.: 7.139 min
Delta R.T.: 0.003 min
Response: 3436466
Conc: 32.25 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

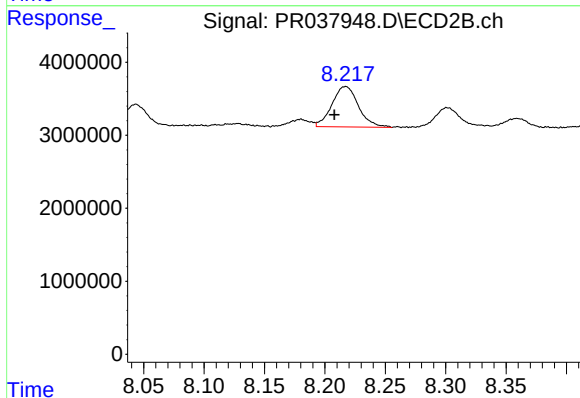


#34 AR-1260-4

R.T.: 8.217 min
Delta R.T.: 0.009 min
Response: 8500584
Conc: 33.27 ng/ml

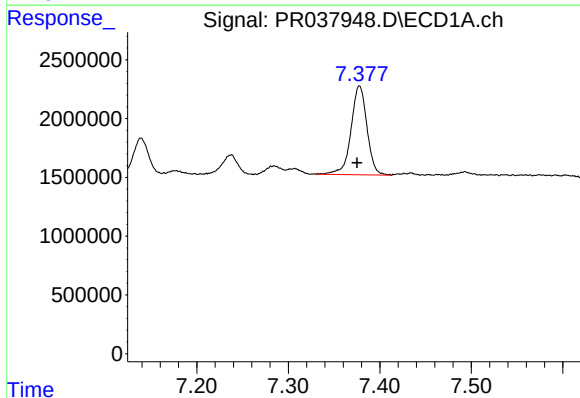


#35 AR-1260-5

R.T.: 7.378 min
Delta R.T.: 0.003 min
Response: 9170546
Conc: 32.64 ng/ml

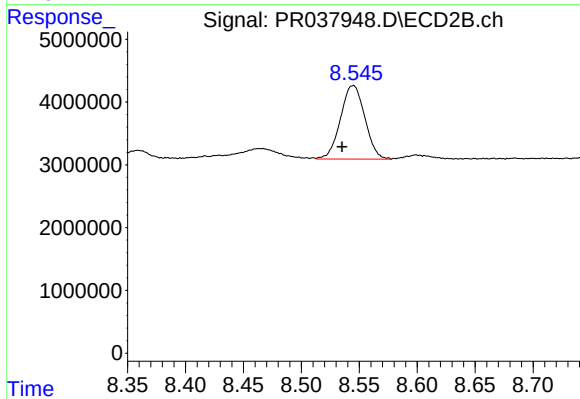

#35 AR-1260-5


R.T.: 8.545 min
Delta R.T.: 0.010 min
Response: 17129875
Conc: 32.97 ng/ml

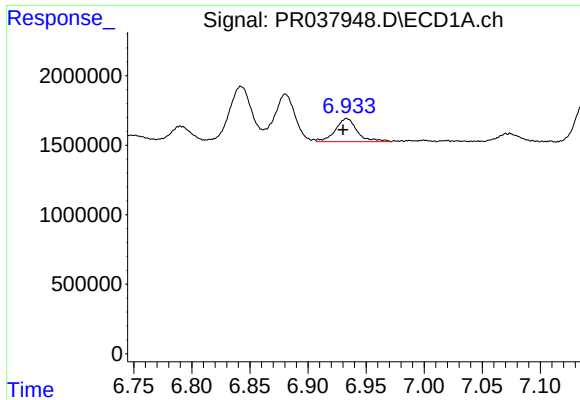

#36 AR-1262-1


R.T.: 6.933 min
Delta R.T.: 0.003 min
Response: 2178559
Conc: 32.59 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

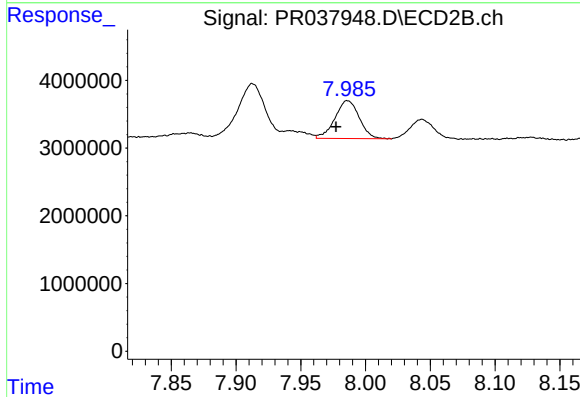


#36 AR-1262-1

R.T.: 7.986 min
Delta R.T.: 0.009 min
Response: 7328427
Conc: 23.19 ng/ml

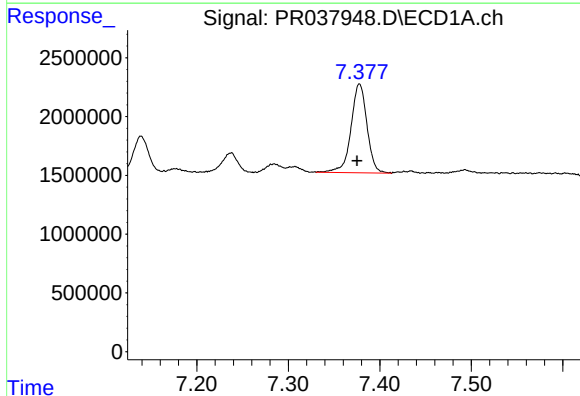


#37 AR-1262-2

R.T.: 7.378 min
Delta R.T.: 0.003 min
Response: 9170546
Conc: 28.08 ng/ml

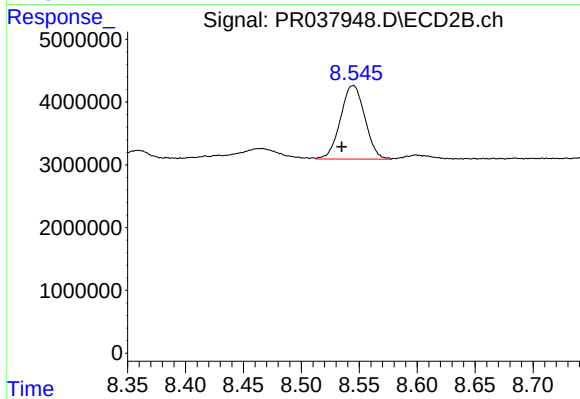

#37 AR-1262-2


R.T.: 8.545 min
Delta R.T.: 0.010 min
Response: 17129875
Conc: 27.49 ng/ml

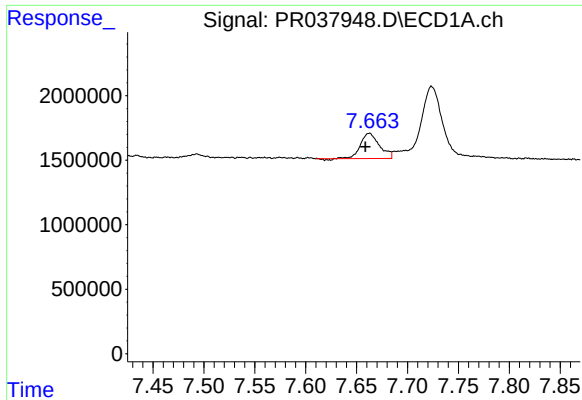

#38 AR-1262-3


R.T.: 7.662 min
Delta R.T.: 0.004 min
Response: 2530384
Conc: 20.20 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

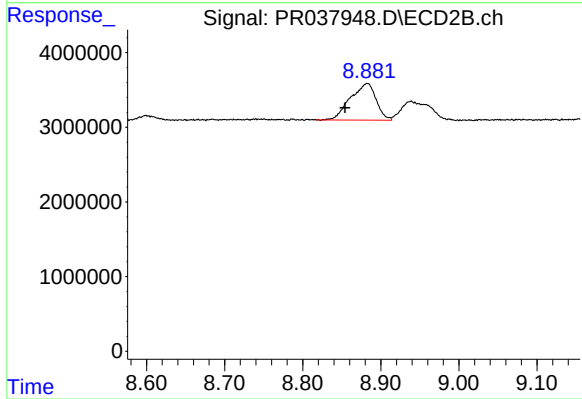


#38 AR-1262-3

R.T.: 8.883 min
Delta R.T.: 0.028 min
Response: 11245687
Conc: 26.83 ng/ml

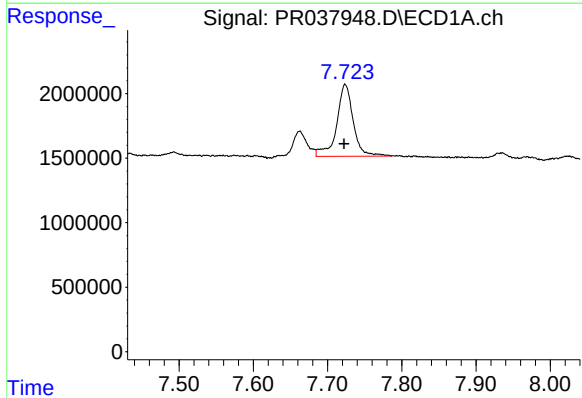


#39 AR-1262-4

R.T.: 7.724 min
Delta R.T.: 0.002 min
Response: 8657939
Conc: 37.24 ng/ml

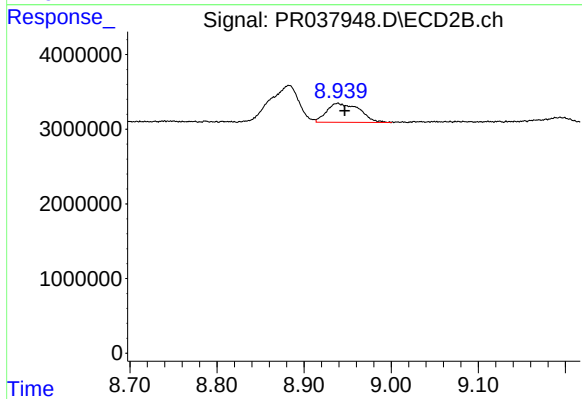

#39 AR-1262-4


R.T.: 8.939 min
Delta R.T.: -0.008 min
Response: 6669216
Conc: 20.90 ng/ml

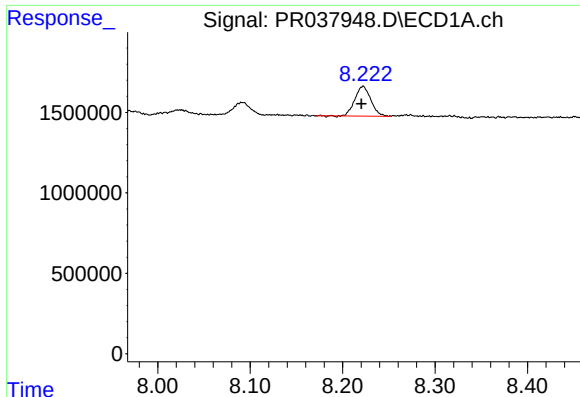

#40 AR-1262-5


R.T.: 8.222 min
Delta R.T.: 0.002 min
Response: 2219755
Conc: 20.69 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

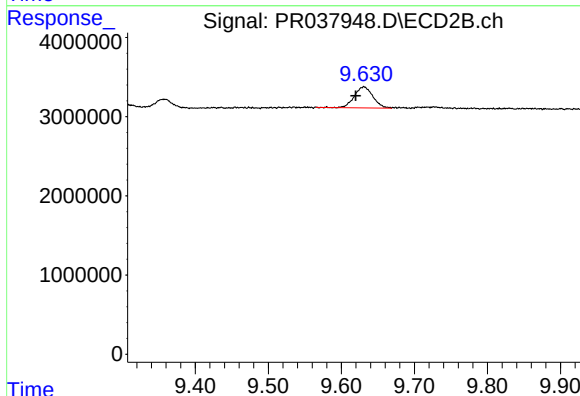


#40 AR-1262-5

R.T.: 9.631 min
Delta R.T.: 0.011 min
Response: 4676471
Conc: 18.78 ng/ml

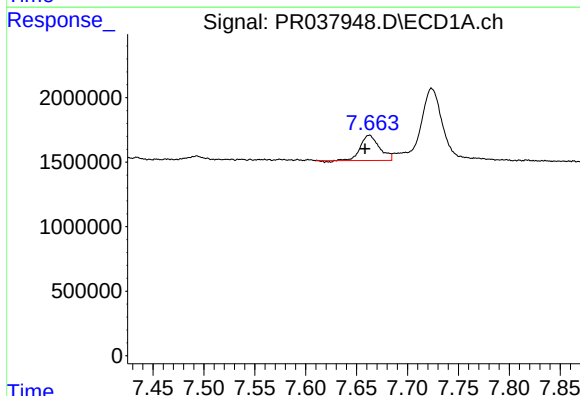


#41 AR-1268-1

R.T.: 7.662 min
Delta R.T.: 0.004 min
Response: 2530384
Conc: 5.81 ng/ml

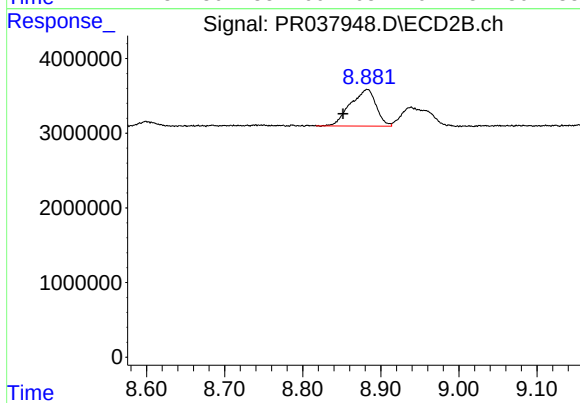

#41 AR-1268-1


R.T.: 8.883 min
Delta R.T.: 0.031 min
Response: 11245687
Conc: 11.22 ng/ml

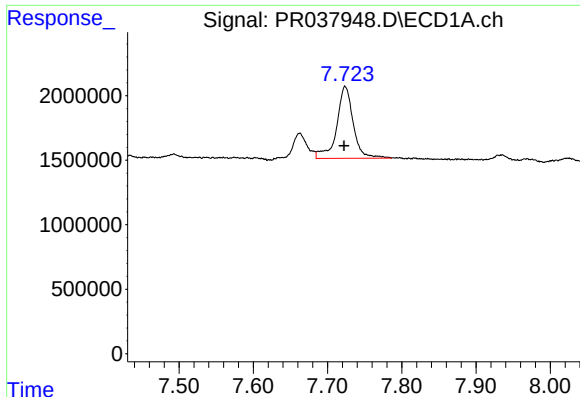

#42 AR-1268-2


R.T.: 7.724 min
Delta R.T.: 0.002 min
Response: 8657939
Conc: 22.02 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

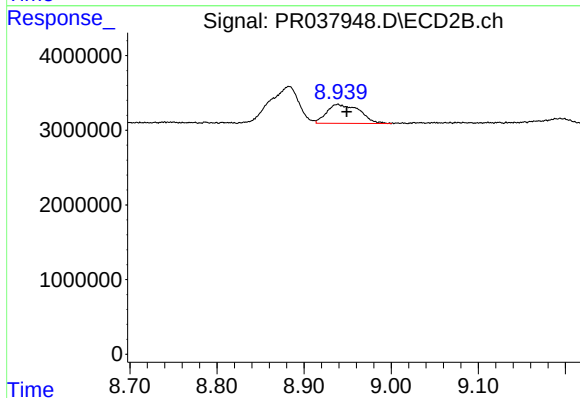


#42 AR-1268-2

R.T.: 8.939 min
Delta R.T.: -0.010 min
Response: 6669216
Conc: 7.38 ng/ml

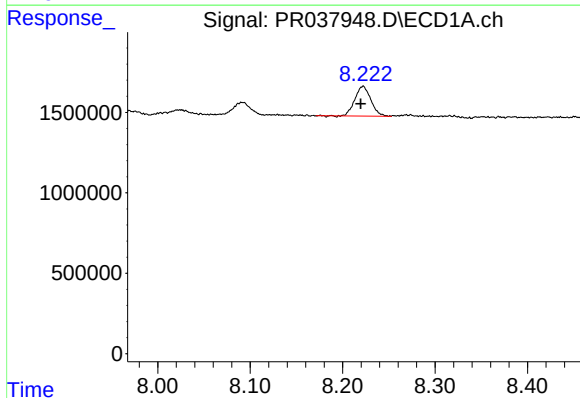


#44 AR-1268-4

R.T.: 8.222 min
Delta R.T.: 0.003 min
Response: 2219755
Conc: 17.30 ng/ml

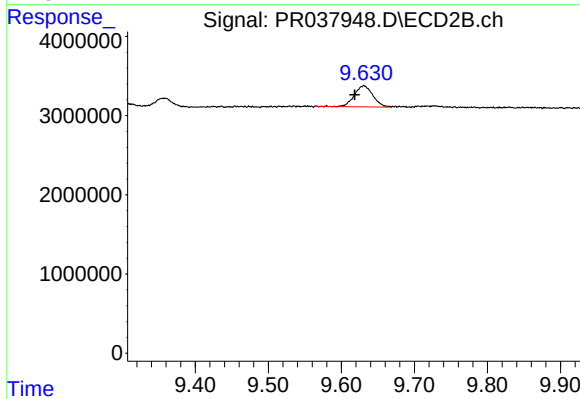

#44 AR-1268-4


R.T.: 9.631 min
Delta R.T.: 0.013 min
Response: 4676471
Conc: 13.75 ng/ml

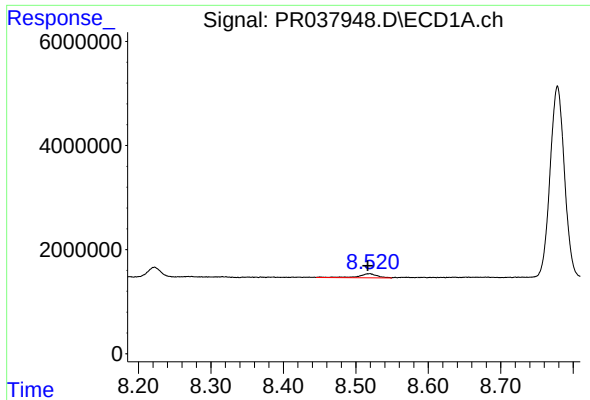

#45 AR-1268-5

R.T.: 8.519 min
Delta R.T.: 0.003 min
Response: 1373664
Conc: 1.47 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-MDL-WATER-03-QT2-2019

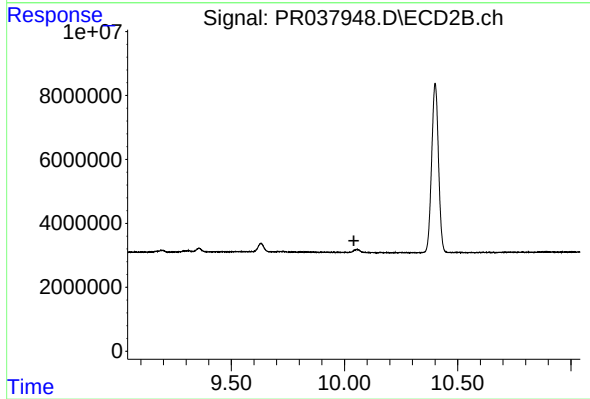

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.042 min
Response: 0
Conc: N.D.