

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR051619\
 Data File : PR037981.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2019 18:15
 Operator : SM\MA
 Sample : K2865-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 TP-22-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 02:31:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR051119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun May 12 00:51:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.778	4.627	42219292	121.3E6	23.428	24.051
2)	SA Decachlor...	8.768	10.387	29426477	76217682	15.424	16.758
Target Compounds							
9)	L2 AR-1221-2	0.000	4.933	0	1594591	N.D.	41.103 #
10)	L2 AR-1221-3	4.196	4.933	813638	1594591	16.134	12.365
11)	L3 AR-1232-1	4.196	4.933	813638	1594591	14.769	11.042 #
27)	L6 AR-1254-2	5.849	0.000	210038	0	1.631	N.D. #
29)	L6 AR-1254-4	6.358	0.000	90346	0	0.597	N.D. #
31)	L7 AR-1260-1	6.322	0.000	1407340	0	11.727	N.D. #
35)	L7 AR-1260-5	0.000	8.589	0	3813549	N.D.	7.341 #
37)	L8 AR-1262-2	0.000	8.589	0	3813549	N.D.	6.121 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR051619\
Data File : PR037981.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2019 18:15
Operator : SM\MA
Sample : K2865-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampled :
TP-22-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 02:31:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR051119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun May 12 00:51:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

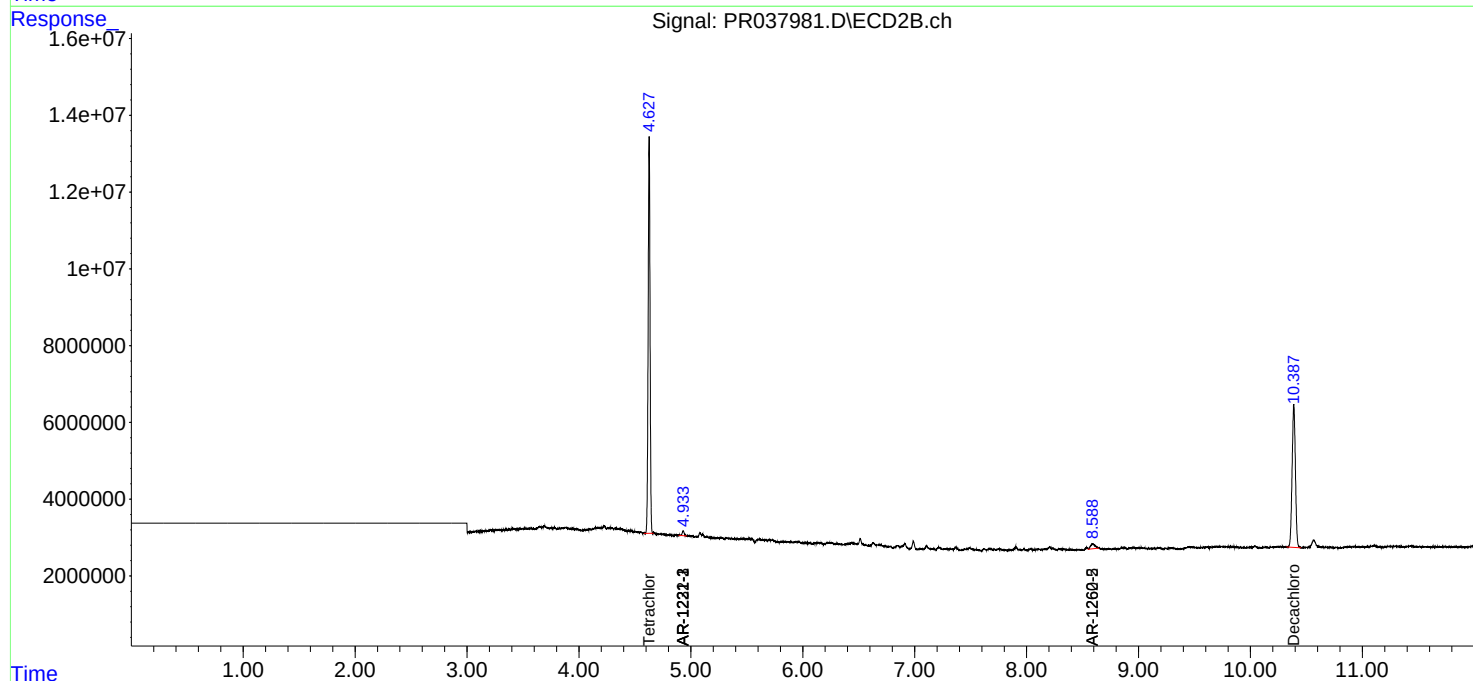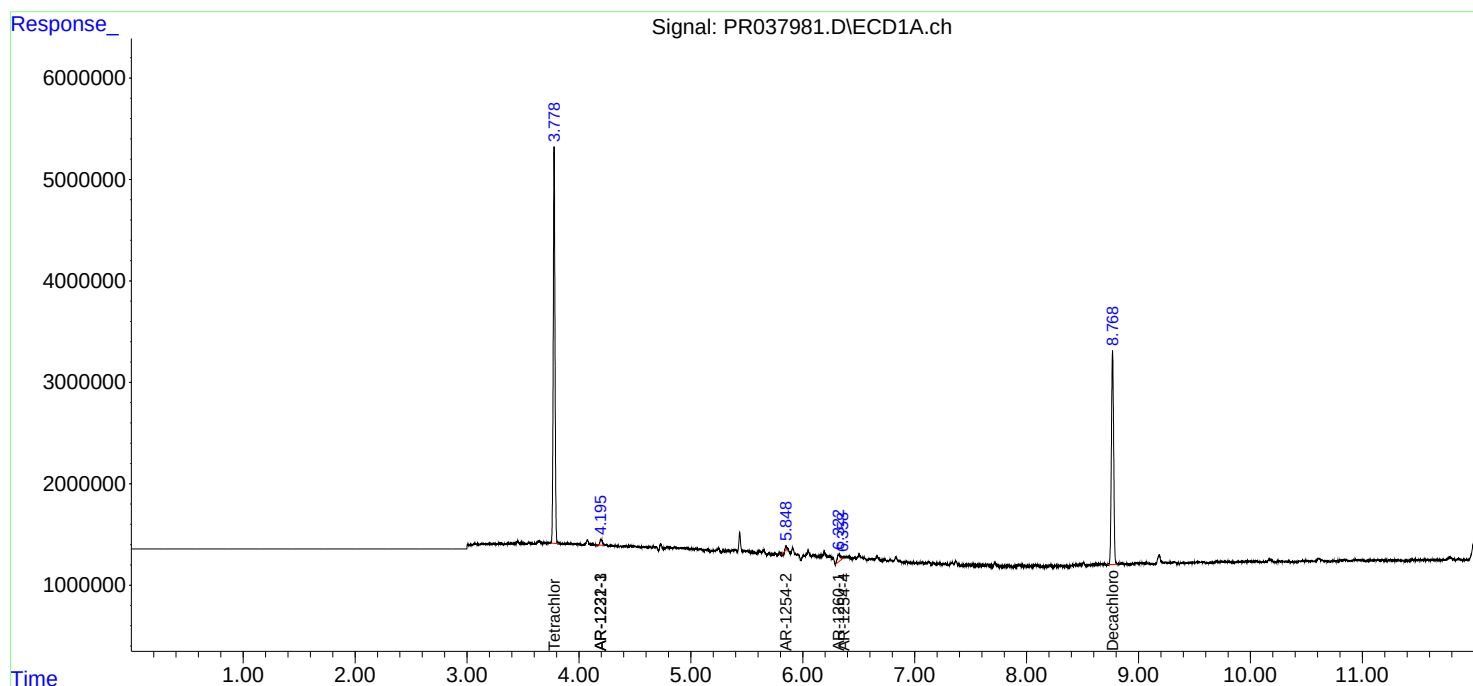


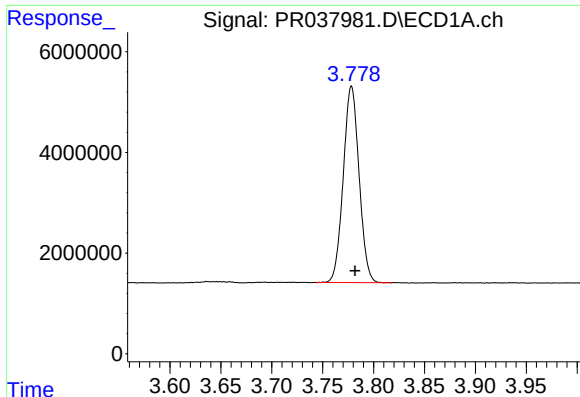

#1 Tetrachloro-m-xylene


R.T.: 3.778 min
Delta R.T.: -0.004 min
Response: 42219292
Conc: 23.43 ng/ml

Instrument :
ECD_R
ClientSampleId :
TP-22-S

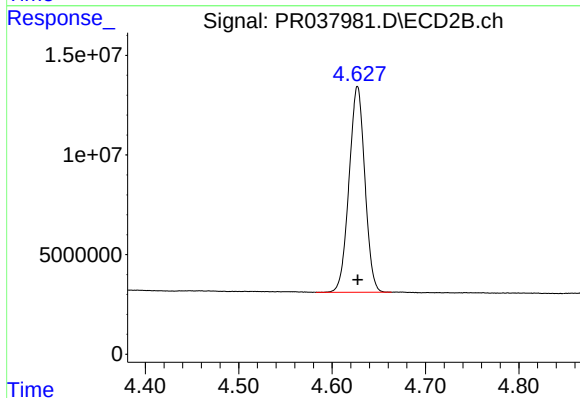


#1 Tetrachloro-m-xylene

R.T.: 4.627 min
Delta R.T.: 0.000 min
Response: 121283549
Conc: 24.05 ng/ml

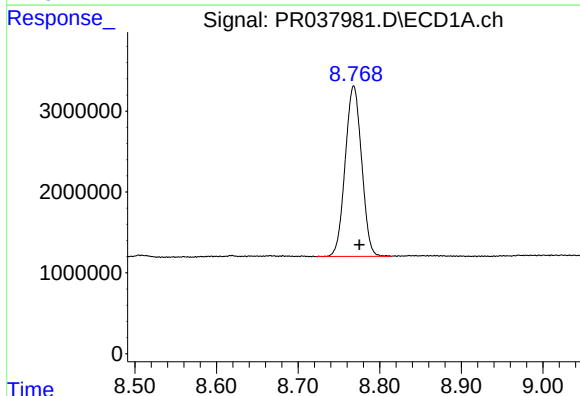


#2 Decachlorobiphenyl

R.T.: 8.768 min
Delta R.T.: -0.007 min
Response: 29426477
Conc: 15.42 ng/ml

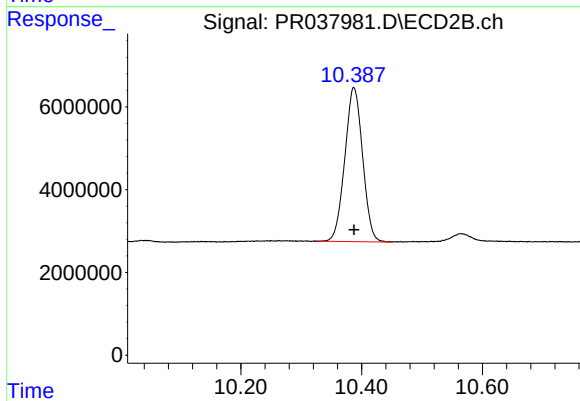

#2 Decachlorobiphenyl


R.T.: 10.387 min
Delta R.T.: 0.000 min
Response: 76217682
Conc: 16.76 ng/ml

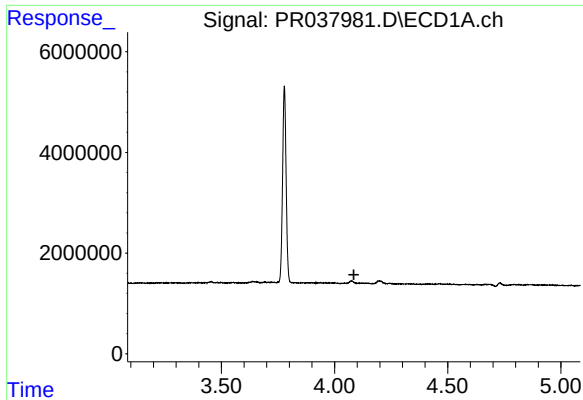

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.085 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
TP-22-S

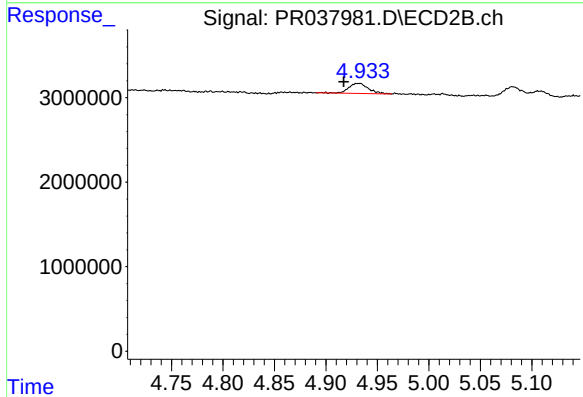


#9 AR-1221-2

R.T.: 4.933 min
Delta R.T.: 0.016 min
Response: 1594591
Conc: 41.10 ng/ml

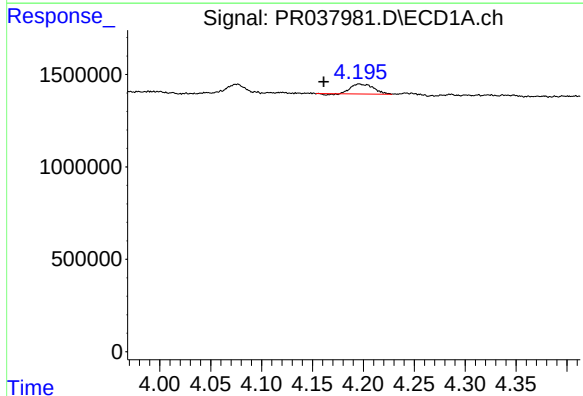


#10 AR-1221-3

R.T.: 4.196 min
Delta R.T.: 0.035 min
Response: 813638
Conc: 16.13 ng/ml

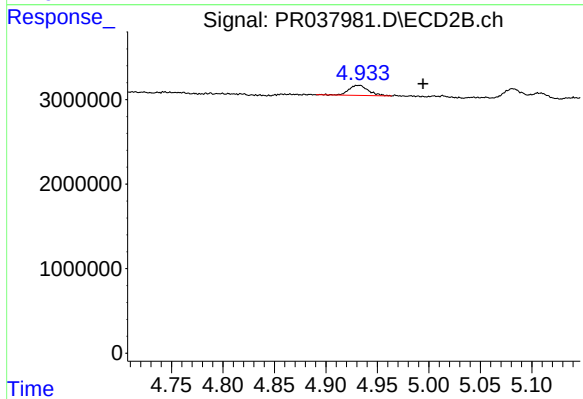

#10 AR-1221-3


R.T.: 4.933 min
Delta R.T.: -0.061 min
Response: 1594591
Conc: 12.36 ng/ml

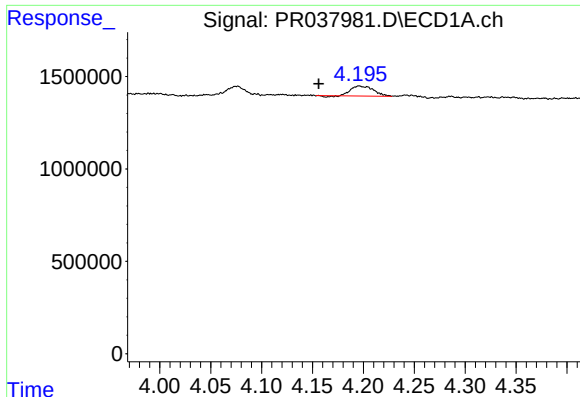

#11 AR-1232-1


R.T.: 4.196 min
Delta R.T.: 0.040 min
Response: 813638
Conc: 14.77 ng/ml

Instrument :
ECD_R
ClientSampleId :
TP-22-S

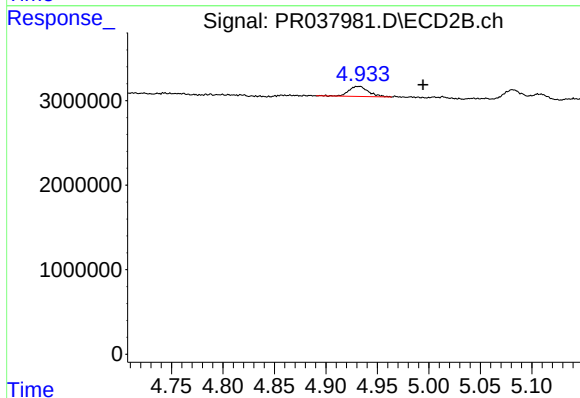


#11 AR-1232-1

R.T.: 4.933 min
Delta R.T.: -0.061 min
Response: 1594591
Conc: 11.04 ng/ml

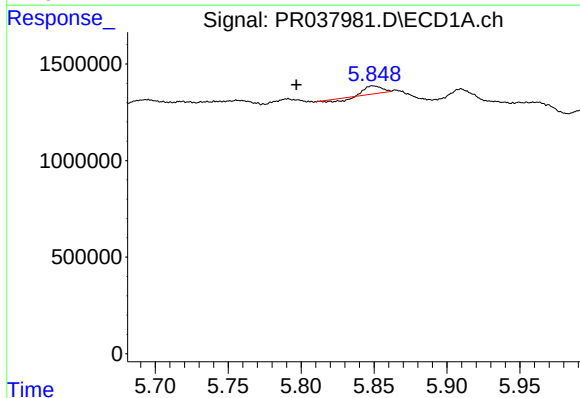


#27 AR-1254-2

R.T.: 5.849 min
Delta R.T.: 0.052 min
Response: 210038
Conc: 1.63 ng/ml

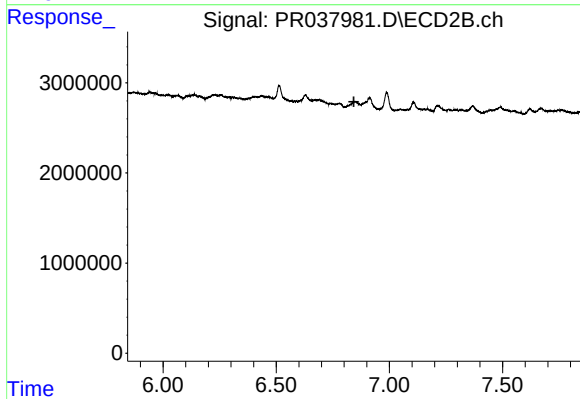

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.843 min
Response: 0
Conc: N.D.

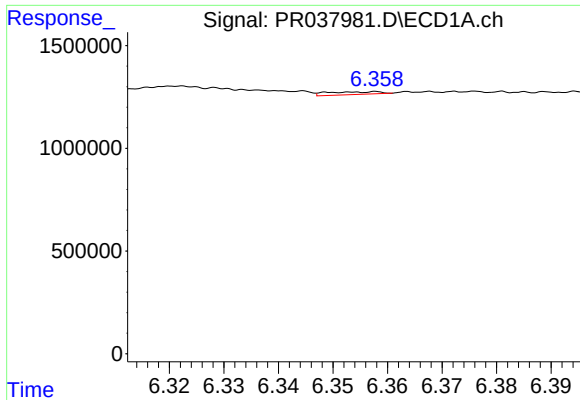

#29 AR-1254-4


R.T.: 6.358 min
Delta R.T.: -0.066 min
Response: 90346
Conc: 0.60 ng/ml

Instrument :
ECD_R
ClientSampleId :
TP-22-S

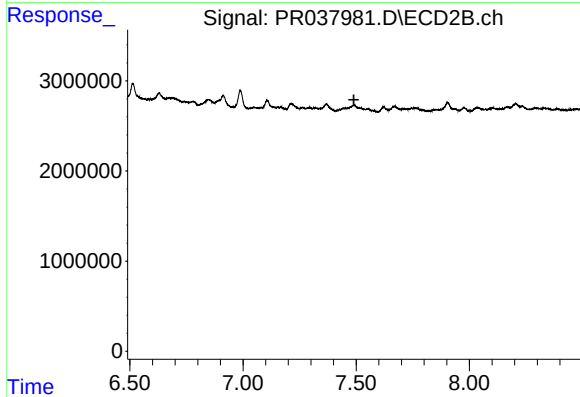


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.490 min
Response: 0
Conc: N.D.

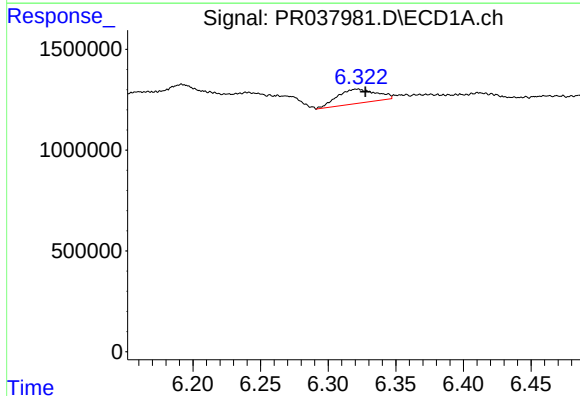


#31 AR-1260-1

R.T.: 6.322 min
Delta R.T.: -0.005 min
Response: 1407340
Conc: 11.73 ng/ml

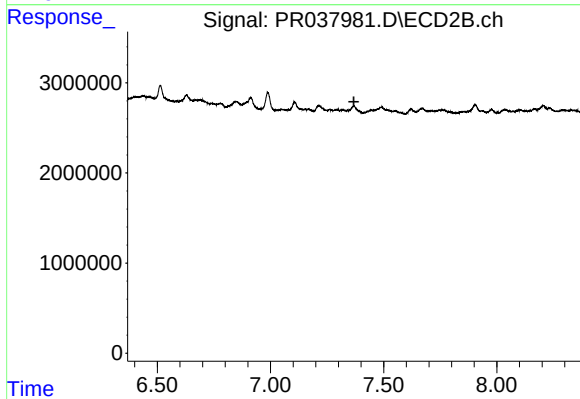

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 7.369 min
Response: 0
Conc: N.D.

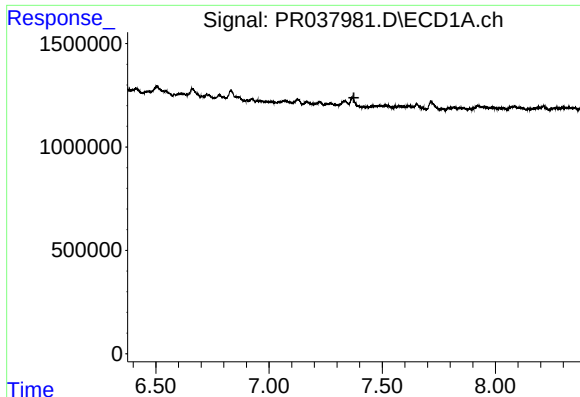

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 7.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
TP-22-S

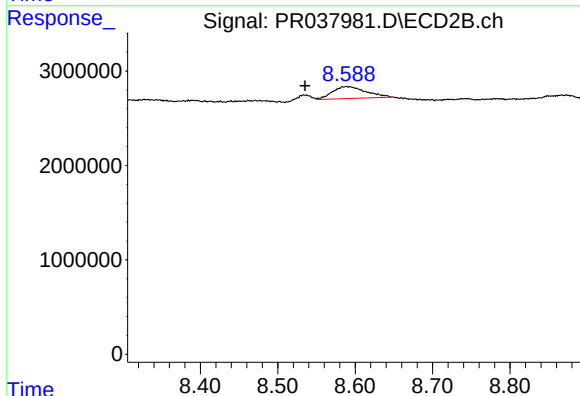


#35 AR-1260-5

R.T.: 8.589 min
Delta R.T.: 0.054 min
Response: 3813549
Conc: 7.34 ng/ml

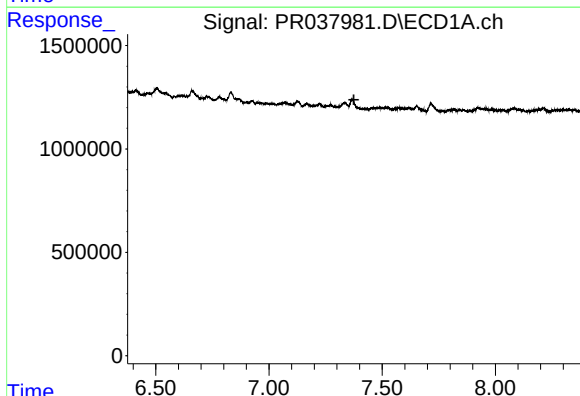

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 7.375 min
Response: 0
Conc: N.D.

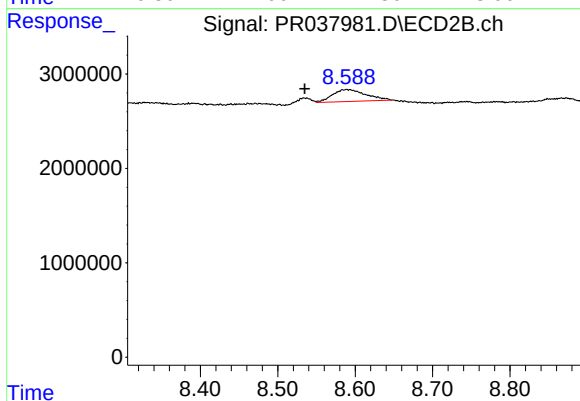

#37 AR-1262-2

R.T.: 8.589 min
Delta R.T.: 0.054 min
Response: 3813549
Conc: 6.12 ng/ml