

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR051619\
 Data File : PR037961.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2019 11:44
 Operator : SM\MA
 Sample : K2761-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 FK-SF-03-006-A

Manual Integrations
 APPROVED

Ankita
 5/17/2019 1:23:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 12:00:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR051119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun May 12 00:51:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.789	4.627	44507904	132.6E6	24.698	26.297m
2) SA Decachlor...	8.811	10.399	27810214	76133120	14.577	16.739

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR051619\
Data File : PR037961.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2019 11:44
Operator : SM\MA
Sample : K2761-01
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
FK-SF-03-006-A


Manual Integrations
APPROVED

Ankita
5/17/2019 1:23:31 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 12:00:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR051119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun May 12 00:51:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

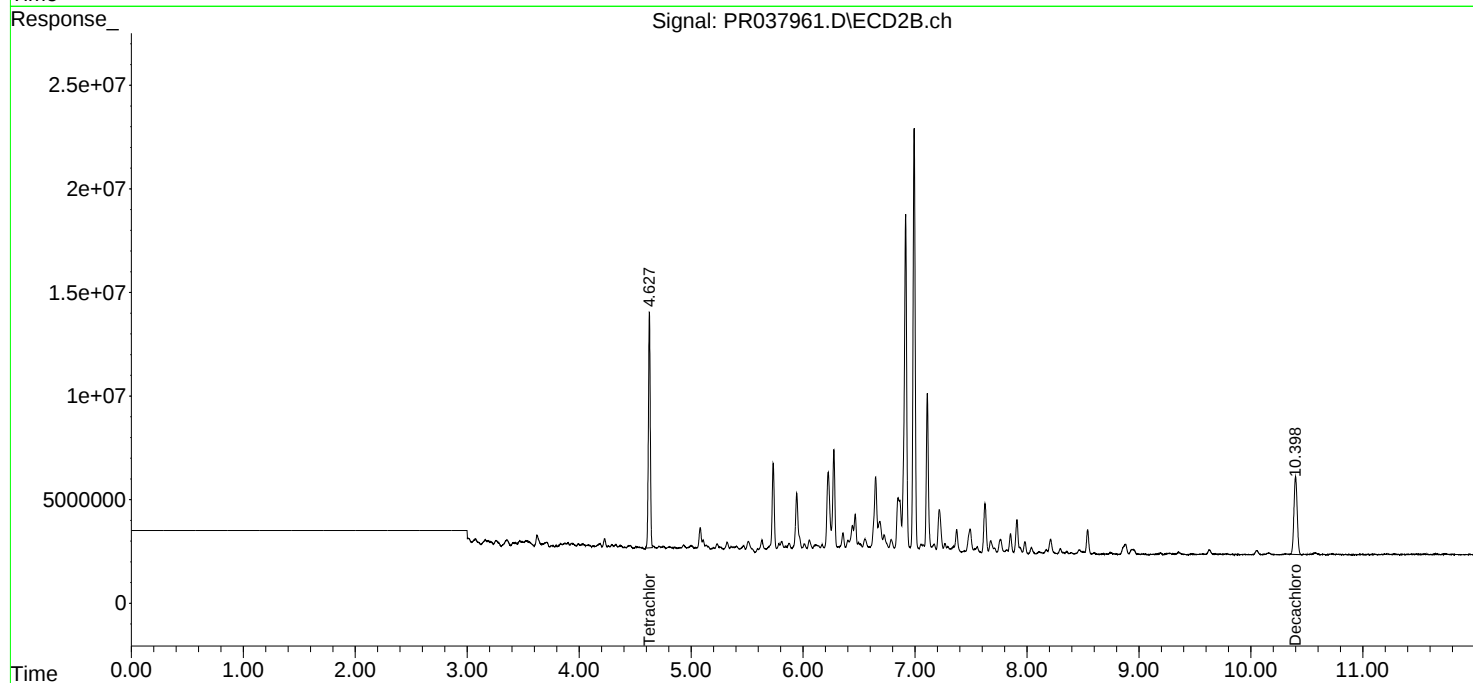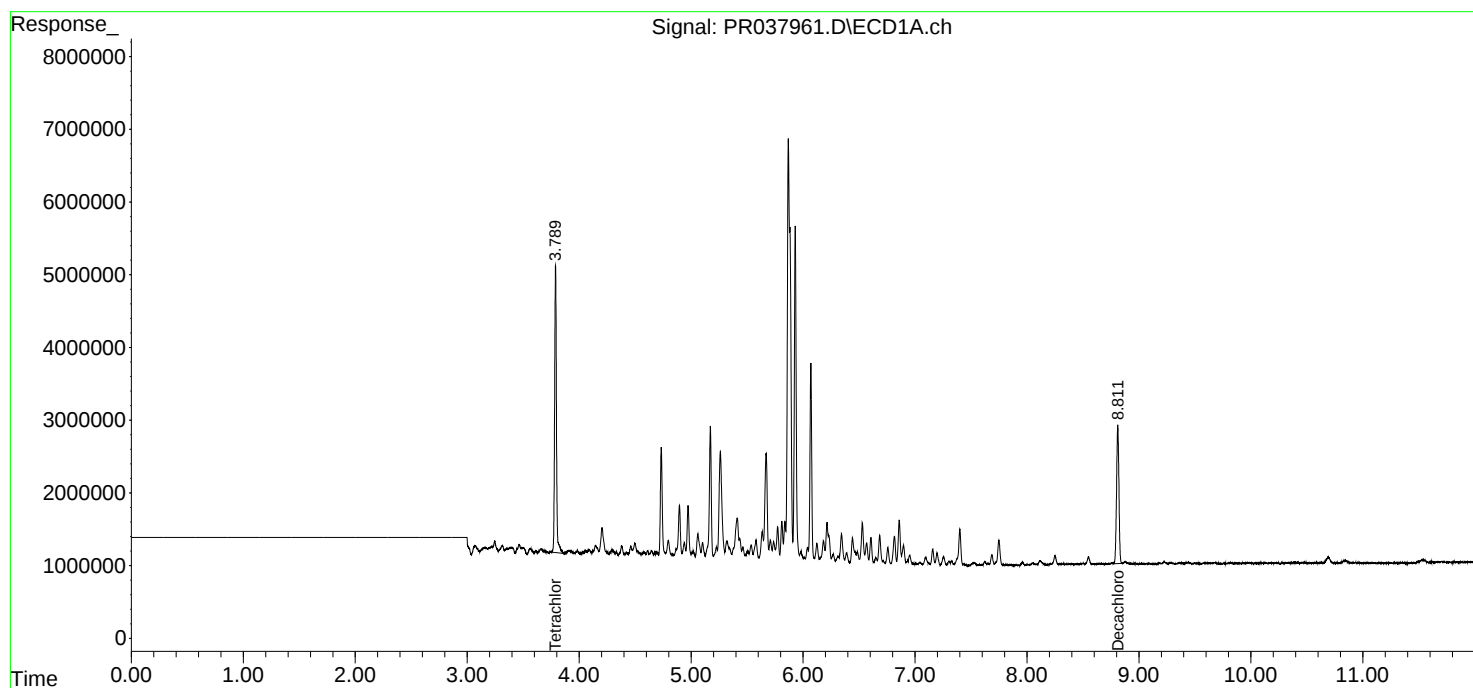

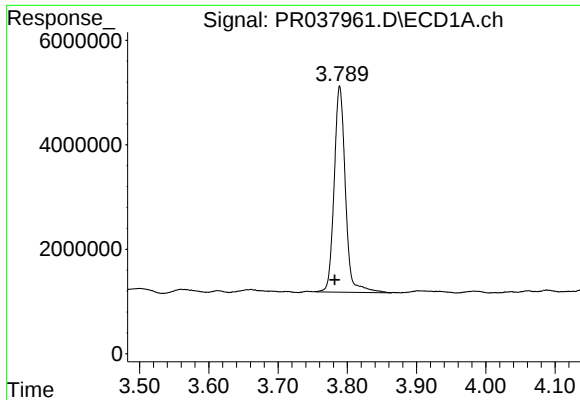


#1 Tetrachloro-m-xylene

R.T.: 3.789 min
Delta R.T.: 0.007 min
Response: 44507904
Conc: 24.70 ng/ml

Instrument :
ECD_R
ClientSampleId :
FK-SF-03-006-A


Manual Integrations
APPROVED

Ankita
5/17/2019 1:23:31 PM

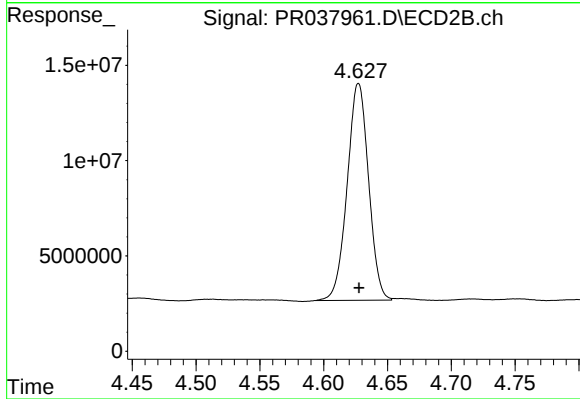


#1 Tetrachloro-m-xylene

R.T.: 4.627 min
Delta R.T.: 0.000 min
Response: 132612827
Conc: 26.30 ng/ml m

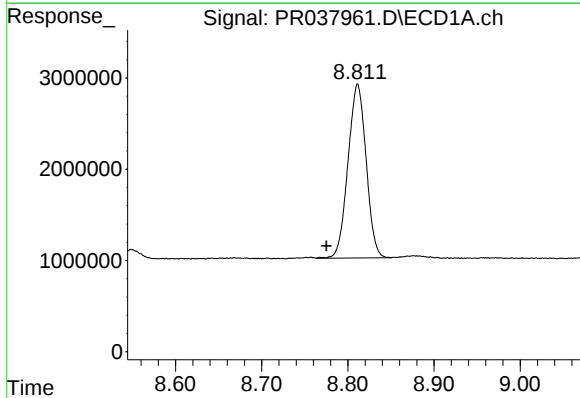

#2 Decachlorobiphenyl

R.T.: 8.811 min
Delta R.T.: 0.036 min
Response: 27810214
Conc: 14.58 ng/ml

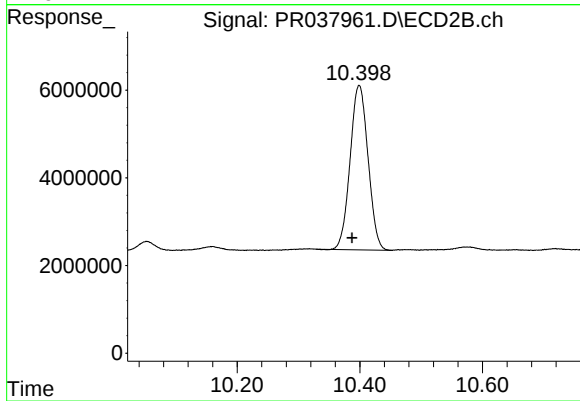

#2 Decachlorobiphenyl

R.T.: 10.399 min
Delta R.T.: 0.012 min
Response: 76133120
Conc: 16.74 ng/ml