

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052119\
 Data File : PR038147.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2019 21:10
 Operator : SM\MA
 Sample : K2951-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 TP-12-S

Manual Integrations
 APPROVED

Ankita
 5/22/2019 4:03:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 01:51:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 22 01:39:47 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.782	4.631	48658831	149.1E6	34.235m	33.637
2)	SA Decachlor...	8.764	10.387	41029105	107.3E6	14.600m	16.540
Target Compounds							
31)	L7 AR-1260-1	6.322	7.369	9912221	24419083	75.038m	81.746m
32)	L7 AR-1260-2	6.507	7.622	15448748	32301393	87.462m	88.641
33)	L7 AR-1260-3	6.660	7.979	9819651	18615761	62.695m	66.117
34)	L7 AR-1260-4	7.129	8.207	7370232	25448656	54.750m	75.760 #
35)	L7 AR-1260-5	7.367	8.535	20807404	47069458	54.505m	67.336

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052119\
Data File : PR038147.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2019 21:10
Operator : SM\MA
Sample : K2951-03
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampled :
TP-12-S


Manual Integrations
APPROVED

Ankita
5/22/2019 4:03:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 01:51:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052119.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 22 01:39:47 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

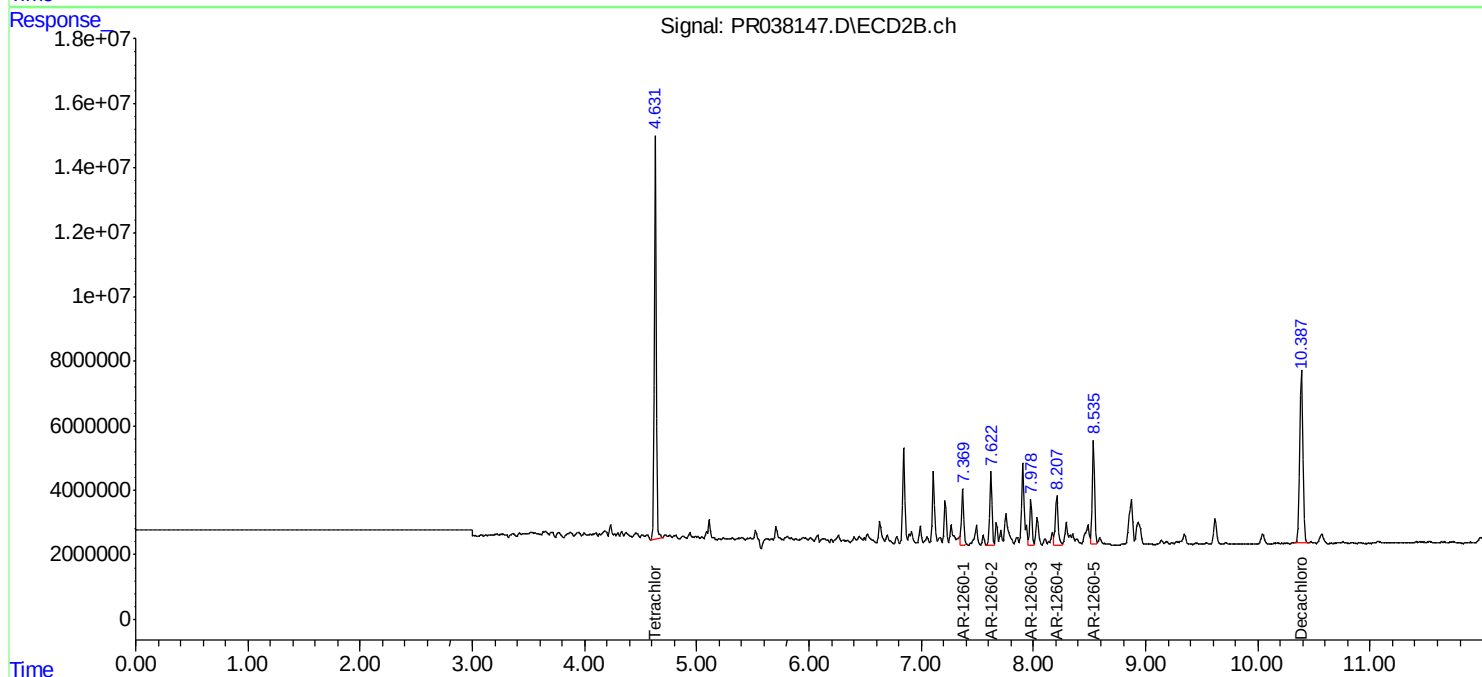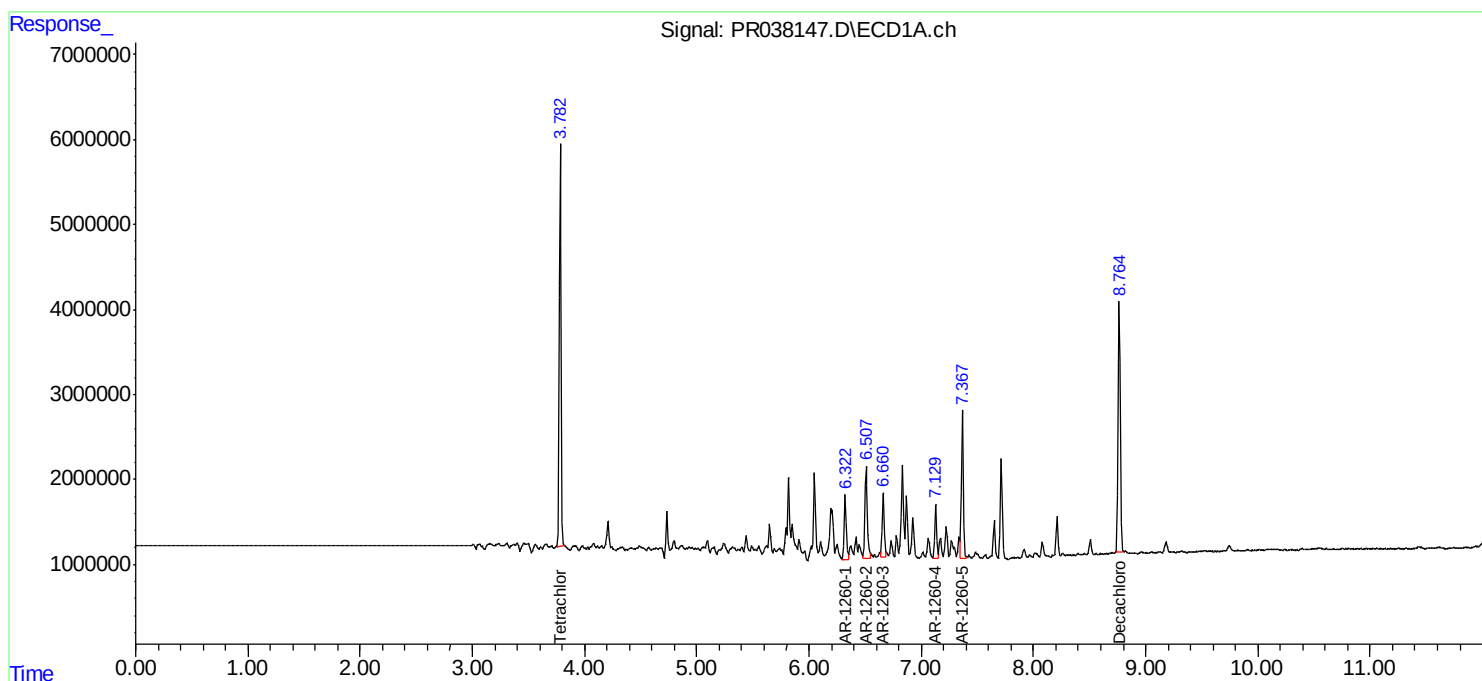

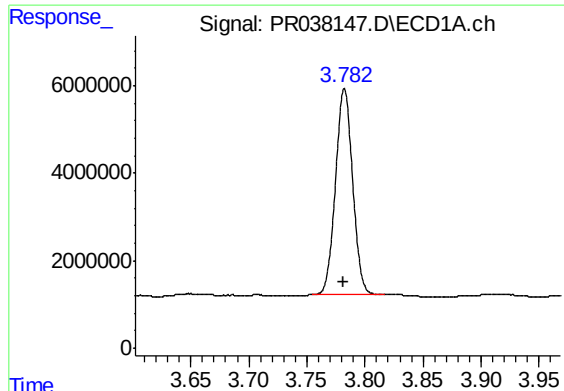


#1 Tetrachloro-m-xylene

R.T.: 3.782 min
Delta R.T.: 0.000 min
Response: 48658831
Conc: 34.23 ng/ml m

Instrument :
ECD_R
ClientSampleId :
TP-12-S


Manual Integrations
APPROVED

Ankita
5/22/2019 4:03:55 PM

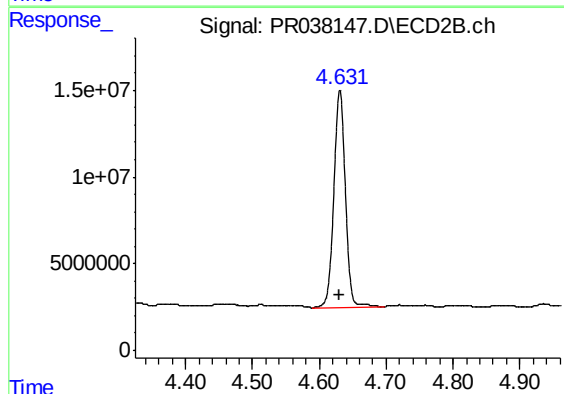


#1 Tetrachloro-m-xylene

R.T.: 4.631 min
Delta R.T.: 0.000 min
Response: 149077775
Conc: 33.64 ng/ml

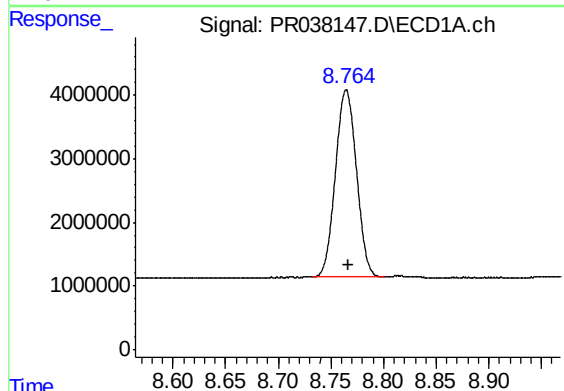


#2 Decachlorobiphenyl

R.T.: 8.764 min
Delta R.T.: -0.003 min
Response: 41029105
Conc: 14.60 ng/ml m

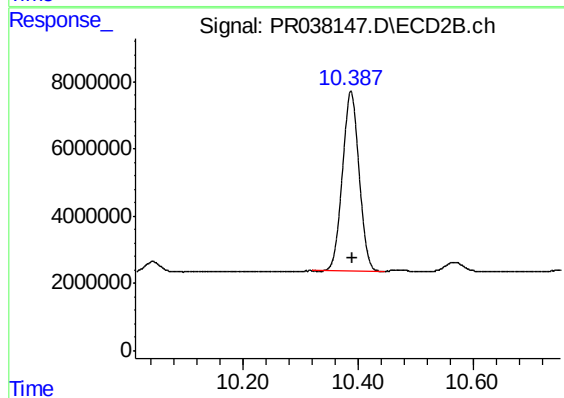

#2 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: -0.002 min
Response: 107341459
Conc: 16.54 ng/ml

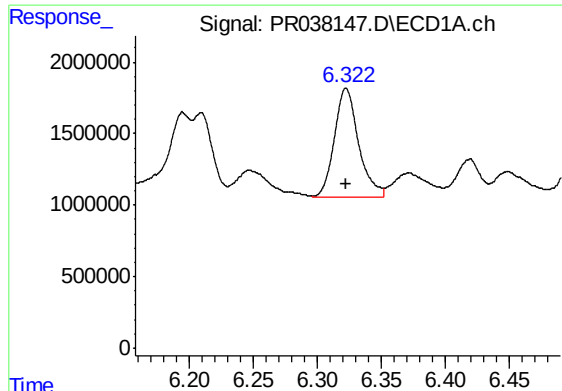


#31 AR-1260-1

R.T.: 6.322 min
Delta R.T.: 0.000 min
Response: 9912221
Conc: 75.04 ng/ml m

Instrument :
ECD_R
ClientSampleId :
TP-12-S


Manual Integrations
APPROVED

Ankita
5/22/2019 4:03:55 PM

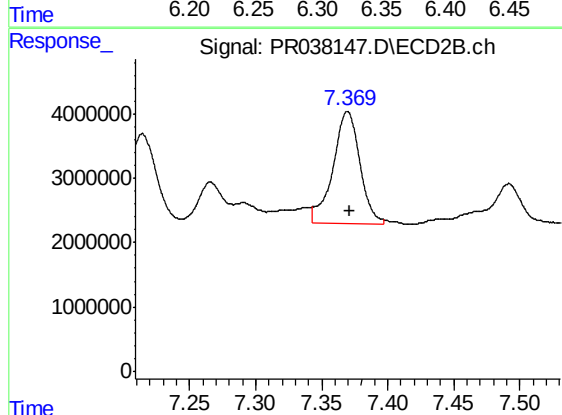


#31 AR-1260-1

R.T.: 7.369 min
Delta R.T.: -0.002 min
Response: 24419083
Conc: 81.75 ng/ml m

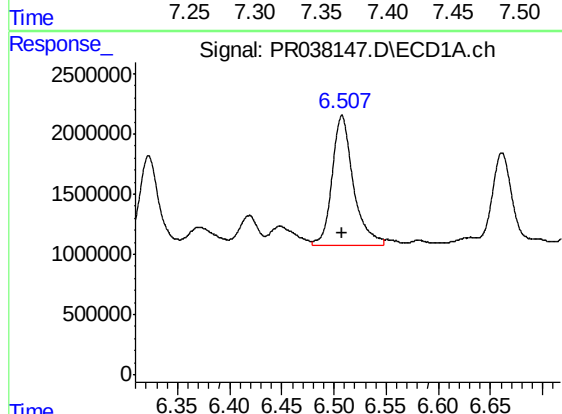


#32 AR-1260-2

R.T.: 6.507 min
Delta R.T.: 0.000 min
Response: 15448748
Conc: 87.46 ng/ml m

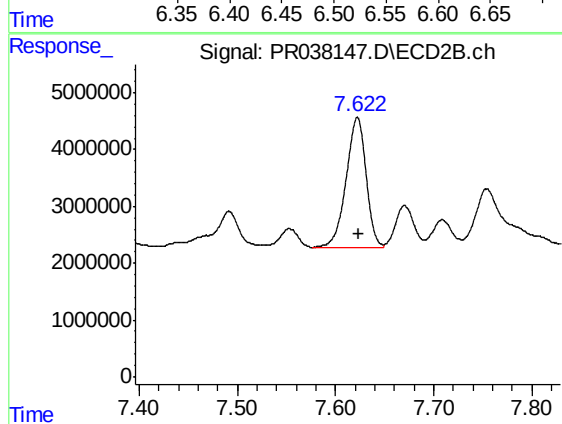

#32 AR-1260-2

R.T.: 7.622 min
Delta R.T.: -0.001 min
Response: 32301393
Conc: 88.64 ng/ml

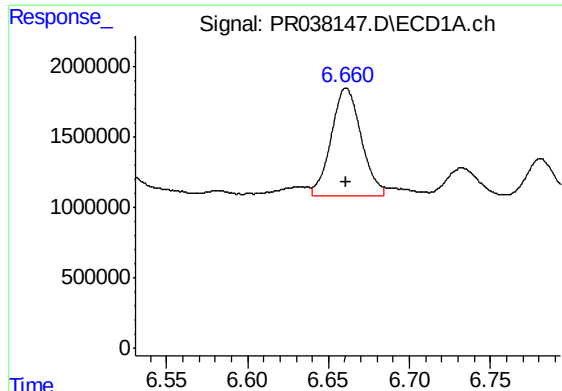


#33 AR-1260-3

R.T.: 6.660 min
Delta R.T.: -0.002 min
Response: 9819651
Conc: 62.70 ng/ml m

Instrument :
ECD_R
ClientSampleId :
TP-12-S


Manual Integrations
APPROVED

Ankita
5/22/2019 4:03:55 PM

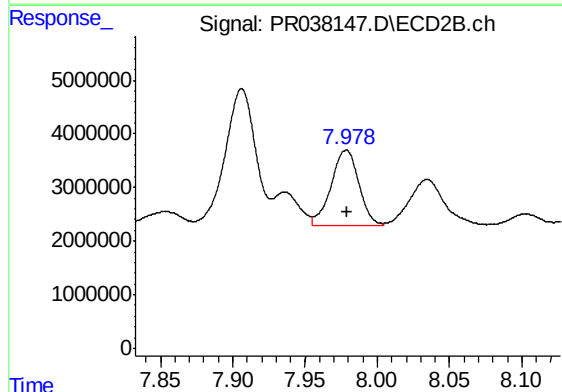


#33 AR-1260-3

R.T.: 7.979 min
Delta R.T.: 0.000 min
Response: 18615761
Conc: 66.12 ng/ml

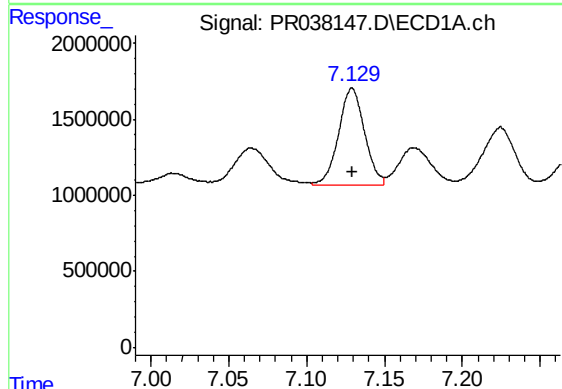


#34 AR-1260-4

R.T.: 7.129 min
Delta R.T.: -0.001 min
Response: 7370232
Conc: 54.75 ng/ml m

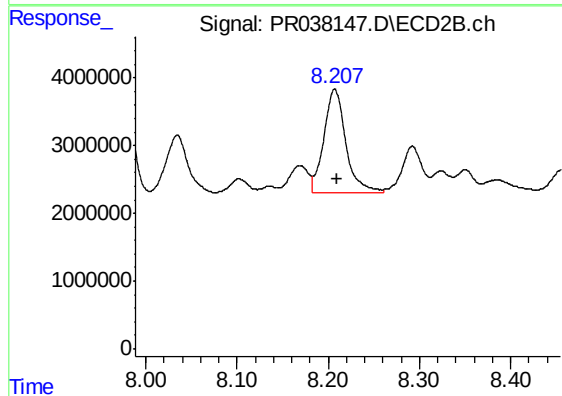

#34 AR-1260-4

R.T.: 8.207 min
Delta R.T.: -0.003 min
Response: 25448656
Conc: 75.76 ng/ml

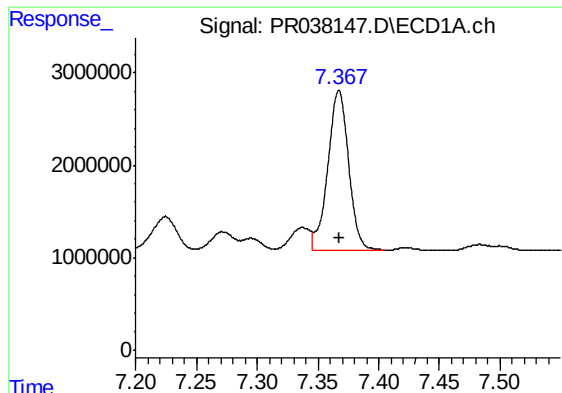


#35 AR-1260-5

R.T.: 7.367 min
Delta R.T.: -0.002 min
Response: 20807404
Conc: 54.51 ng/ml m

Instrument :
ECD_R
ClientSampleId :
TP-12-S

Manual Integrations
APPROVED

Ankita
5/22/2019 4:03:55 PM

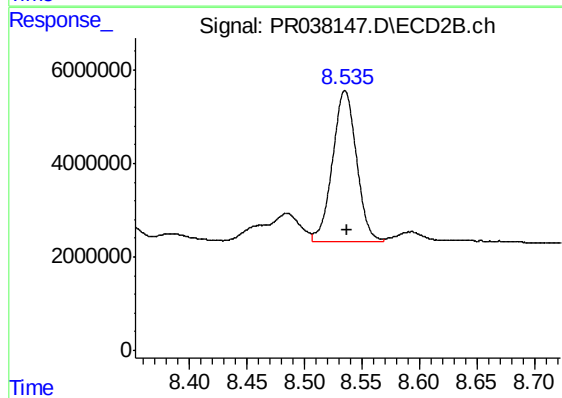

#35 AR-1260-5

R.T.: 8.535 min
Delta R.T.: -0.002 min
Response: 47069458
Conc: 67.34 ng/ml