

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052324\
 Data File : PR066784.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2024 18:16
 Operator : AJ\MA
 Sample : P2547-19MS
 Misc :
 ALS Vial : 31 Sample Multiplier: 1


Instrument :
 ECD_R
 ClientSampleId :
 BH5X5MS

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 05/23/2024
 Supervised By :Ankita Jodhani 05/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 22:47:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052124CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 22 04:28:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

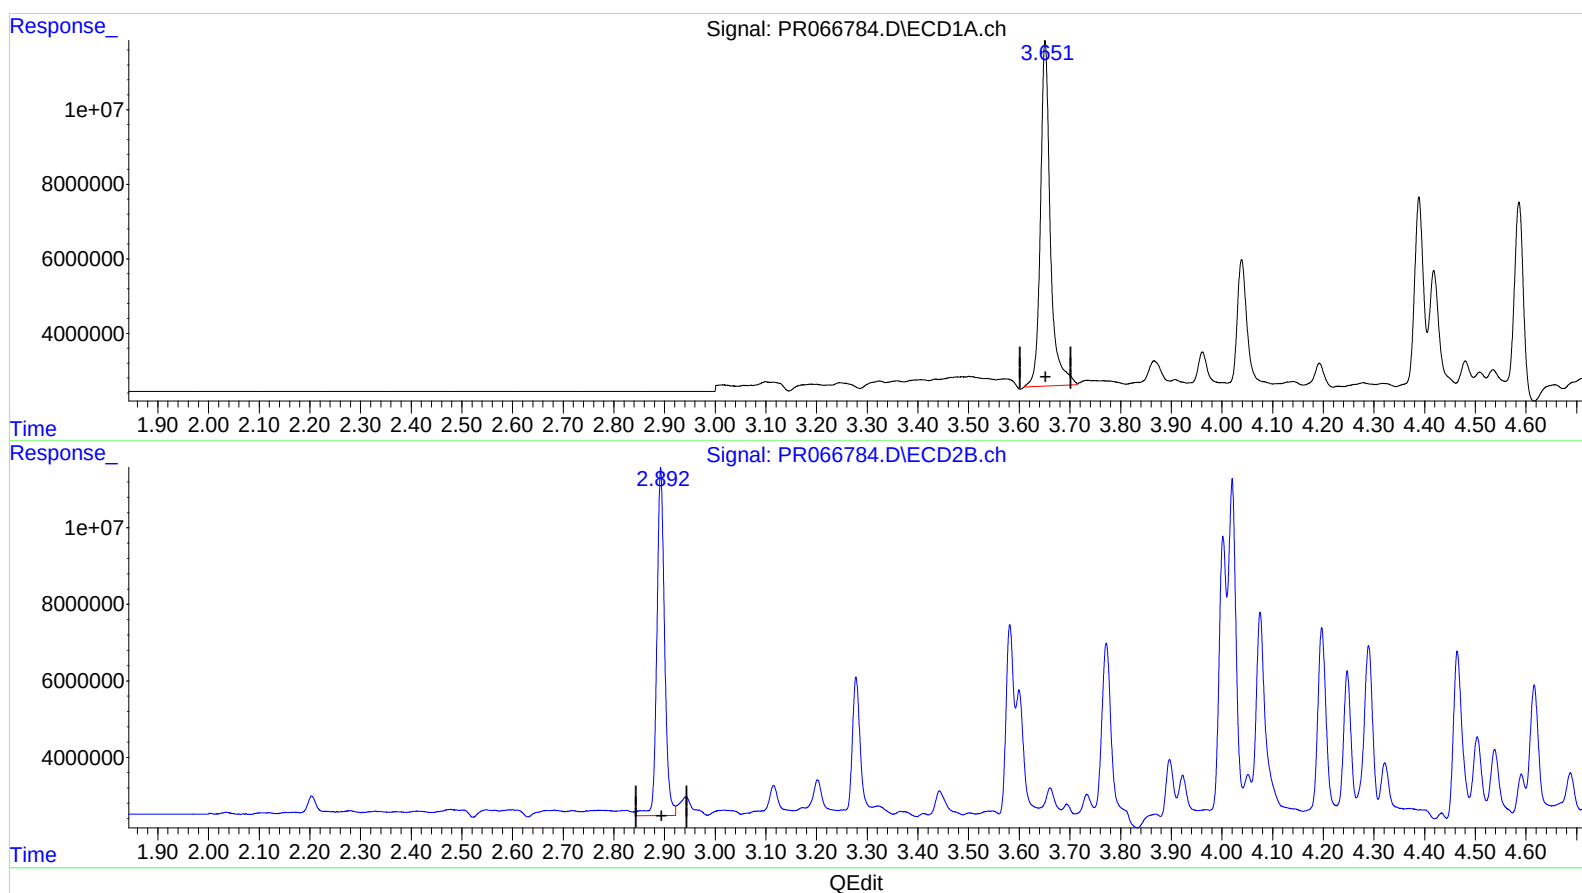

(1) Tetrachloro-m-xylene (SA)

3.651min 20.403 ng/ml

response 125164416

(1) Tetrachloro-m-xylene #2 (SA)

2.893min 20.747 ng/ml

response 96596278

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052324\
Data File : PR066784.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2024 18:16
Operator : AJ\MA
Sample : P2547-19MS
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
BH5X5MS

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 05/23/2024
Supervised By :Ankita Jodhani 05/23/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 22:47:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052124CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 22 04:28:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

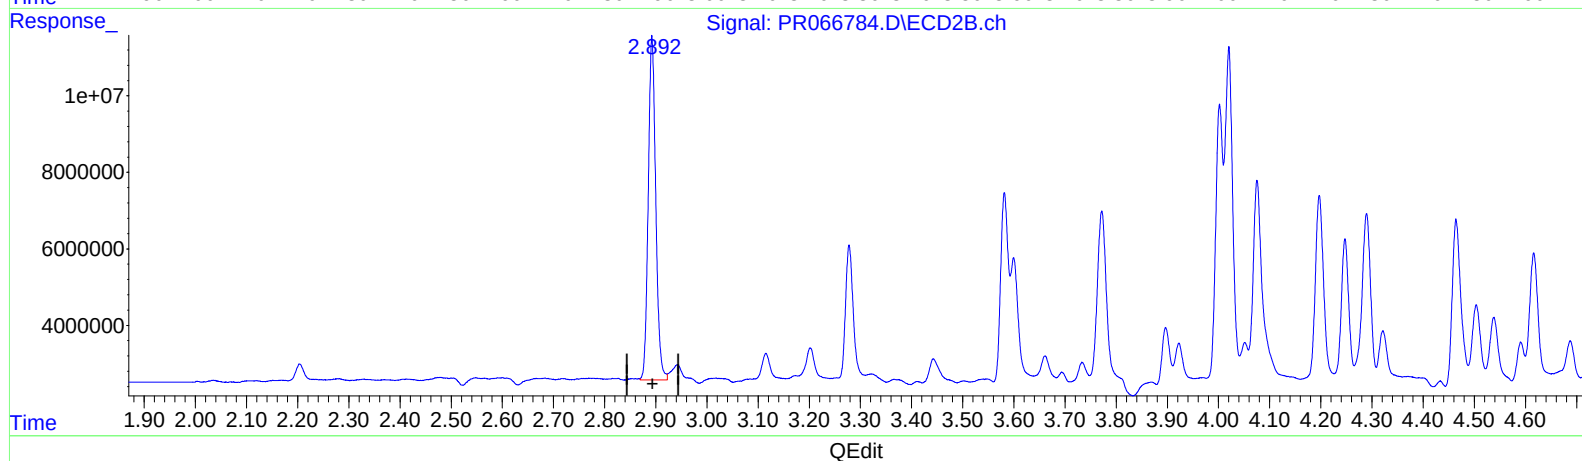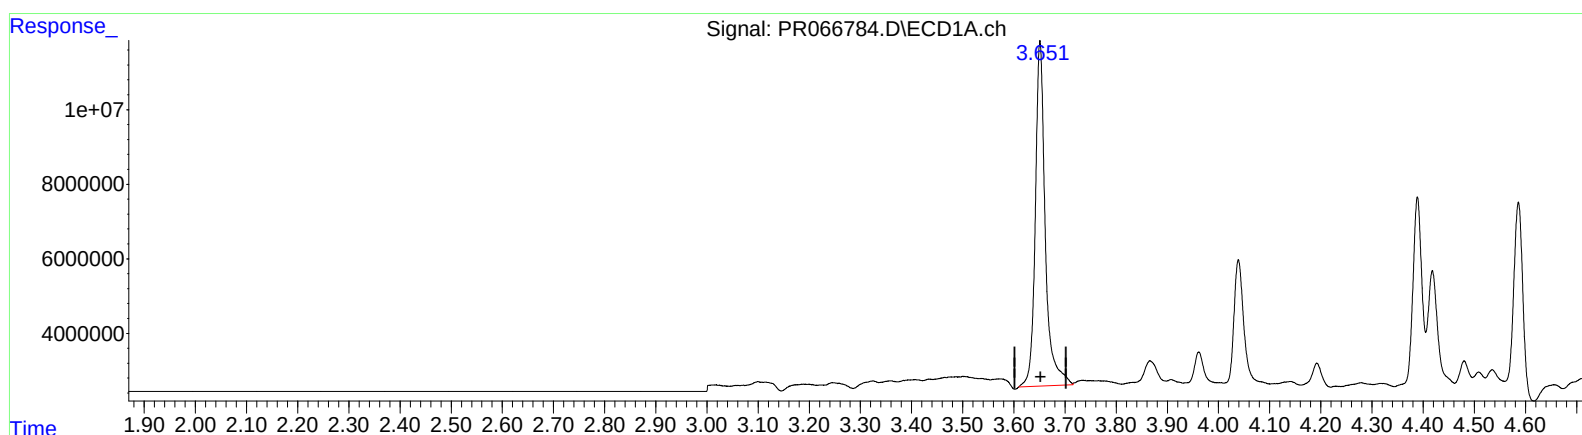

(1) Tetrachloro-m-xylene (SA)

3.651min 20.403 ng/ml

response 125164416

(1) Tetrachloro-m-xylene #2 (SA)

2.892min 19.653 ng/ml m

response 91505373