

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052421\
 Data File : PR050548.D
 Signal(s) : ECD2B.ch
 Acq On : 24 May 21 01:29 pm
 Operator : DD\AJ
 Sample : M2262-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT2-2021

Integration File: autoint1.e
 Quant Time: May 24 17:31:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 22 08:50:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.632	3.814	63219594	90378699	15.089	15.305
2) SA Decachlor...	10.499	8.838	108.2E6	117.7E6	16.007	15.632
Target Compounds						
8) L2 AR-1221-1	4.845	4.026	1417391	1641664	27.382m	25.754
9) L2 AR-1221-2	4.939	4.113	1758723	2348233	43.662	47.799
10) L2 AR-1221-3	5.010	4.189	3387124	4151993	27.228	26.717


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052421\
Data File : PR050548.D
Signal(s) : ECD2B.ch
Acq On : 24 May 21 01:29 pm
Operator : DD\AJ
Sample : M2262-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

Integration File: autoint1.e
Quant Time: May 24 17:31:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052221.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 22 08:50:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

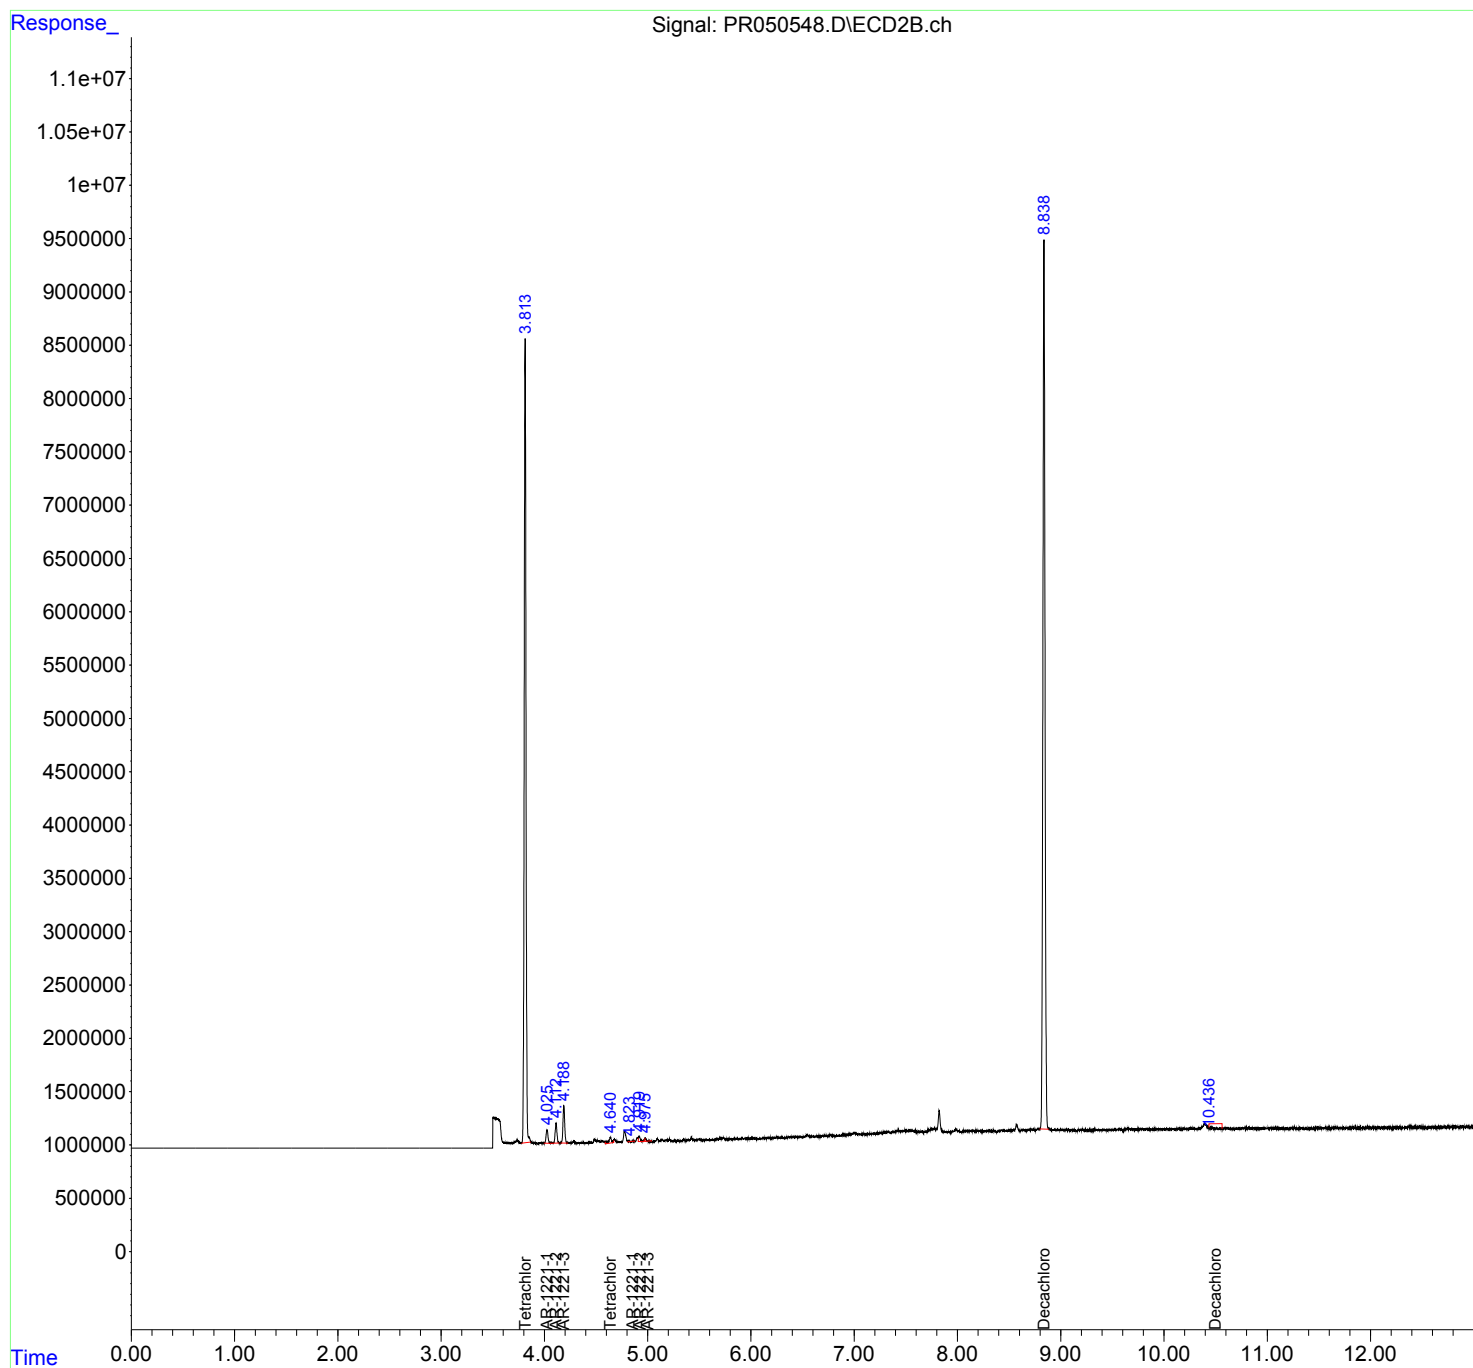


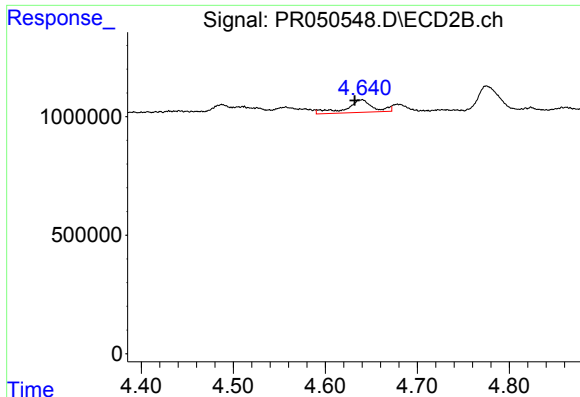

#1 Tetrachloro-m-xylene


R.T.: 4.632 min
Delta R.T.: 0.000 min
Response: 63219594
Conc: 15.09 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

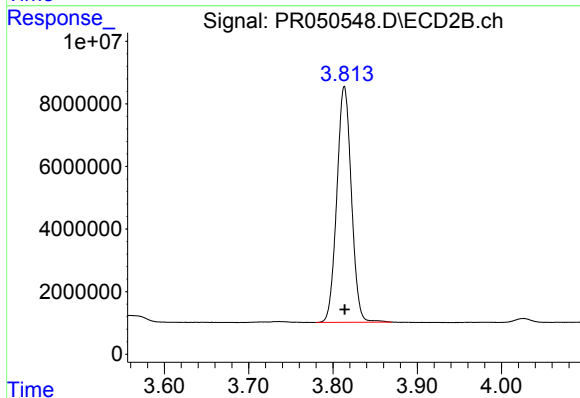


#1 Tetrachloro-m-xylene

R.T.: 3.814 min
Delta R.T.: 0.000 min
Response: 90378699
Conc: 15.31 ng/ml

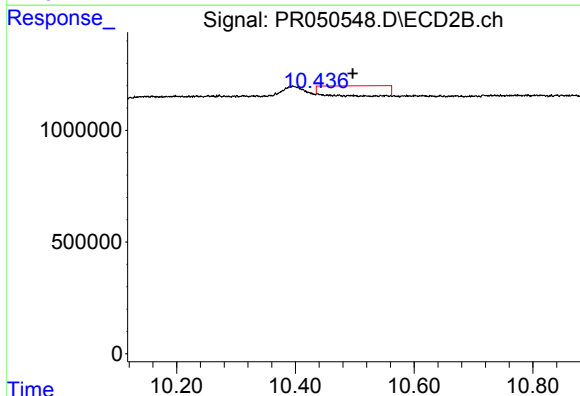


#2 Decachlorobiphenyl

R.T.: 10.499 min
Delta R.T.: 0.003 min
Response: 108223816
Conc: 16.01 ng/ml

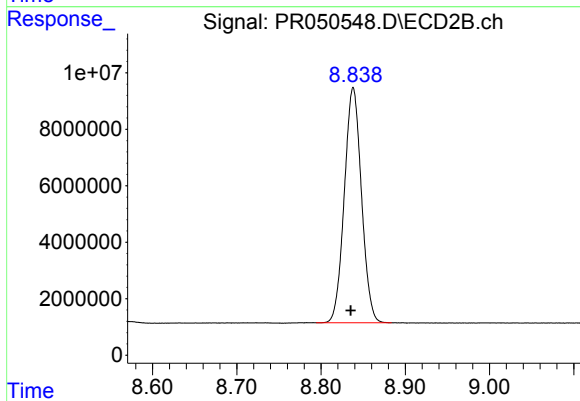

#2 Decachlorobiphenyl


R.T.: 8.838 min
Delta R.T.: 0.003 min
Response: 117743817
Conc: 15.63 ng/ml

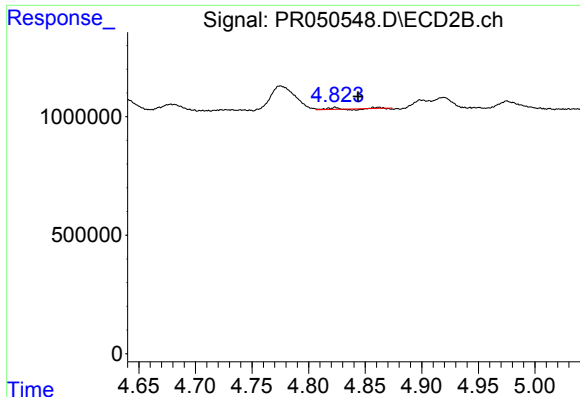

#8 AR-1221-1


R.T.: 4.845 min
Delta R.T.: 0.001 min
Response: 1417391
Conc: 27.38 ng/ml m

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

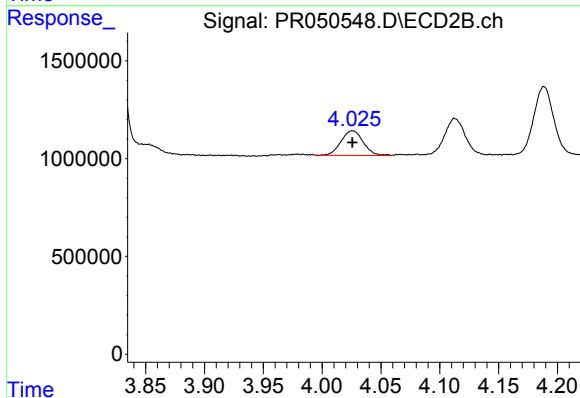


#8 AR-1221-1

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 1641664
Conc: 25.75 ng/ml

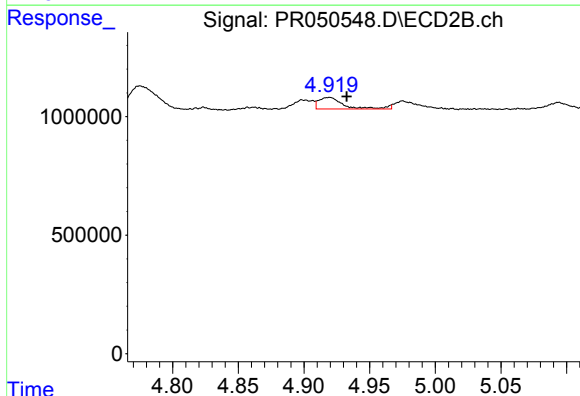


#9 AR-1221-2

R.T.: 4.939 min
Delta R.T.: 0.006 min
Response: 1758723
Conc: 43.66 ng/ml

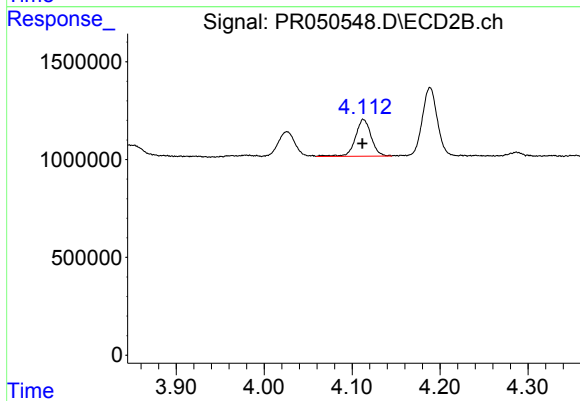

#9 AR-1221-2


R.T.: 4.113 min
Delta R.T.: 0.000 min
Response: 2348233
Conc: 47.80 ng/ml

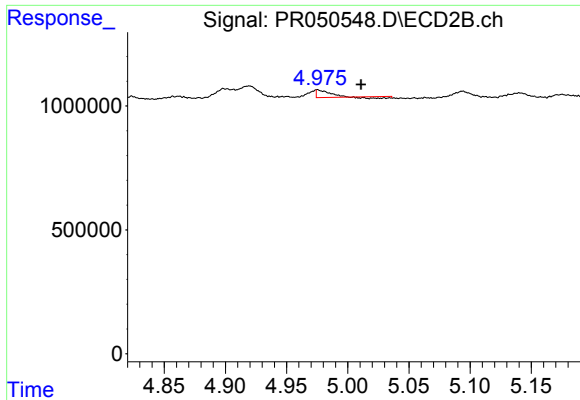

#10 AR-1221-3

R.T.: 5.010 min
Delta R.T.: 0.000 min
Response: 3387124
Conc: 27.23 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

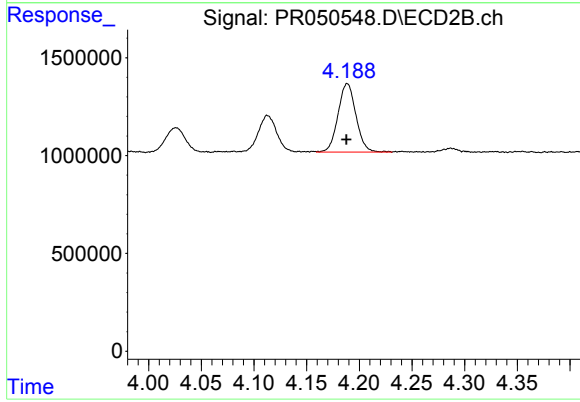

#10 AR-1221-3

R.T.: 4.189 min
Delta R.T.: 0.000 min
Response: 4151993
Conc: 26.72 ng/ml