

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052421\
 Data File : PR050549.D
 Signal(s) : ECD1A.ch
 Acq On : 24 May 21 01:45 pm
 Operator : DD\AJ
 Sample : M2262-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT2-2021

Integration File: autoint1.e
 Quant Time: May 24 17:32:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 22 08:50:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.631	3.814	62934810	89224868	15.021	15.110
2) SA Decachlor...	10.499	8.839	110.3E6	118.9E6	16.319	15.783
Target Compounds						
11) L3 AR-1232-1	5.010	4.189	2500355	3020097	25.921	25.509
12) L3 AR-1232-2	5.543	4.919	1469812	2693246	24.050	20.205
13) L3 AR-1232-3	5.836	5.095	2990793	1663601	22.605	23.721
14) L3 AR-1232-4	5.998	5.178	1566412	1624159	23.363	26.386
15) L3 AR-1232-5	6.082	5.349	1154850	1864545	21.873m	26.676


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052421\
Data File : PR050549.D
Signal(s) : ECD1A.ch
Acq On : 24 May 21 01:45 pm
Operator : DD\AJ
Sample : M2262-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

Integration File: autoint1.e
Quant Time: May 24 17:32:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052221.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 22 08:50:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

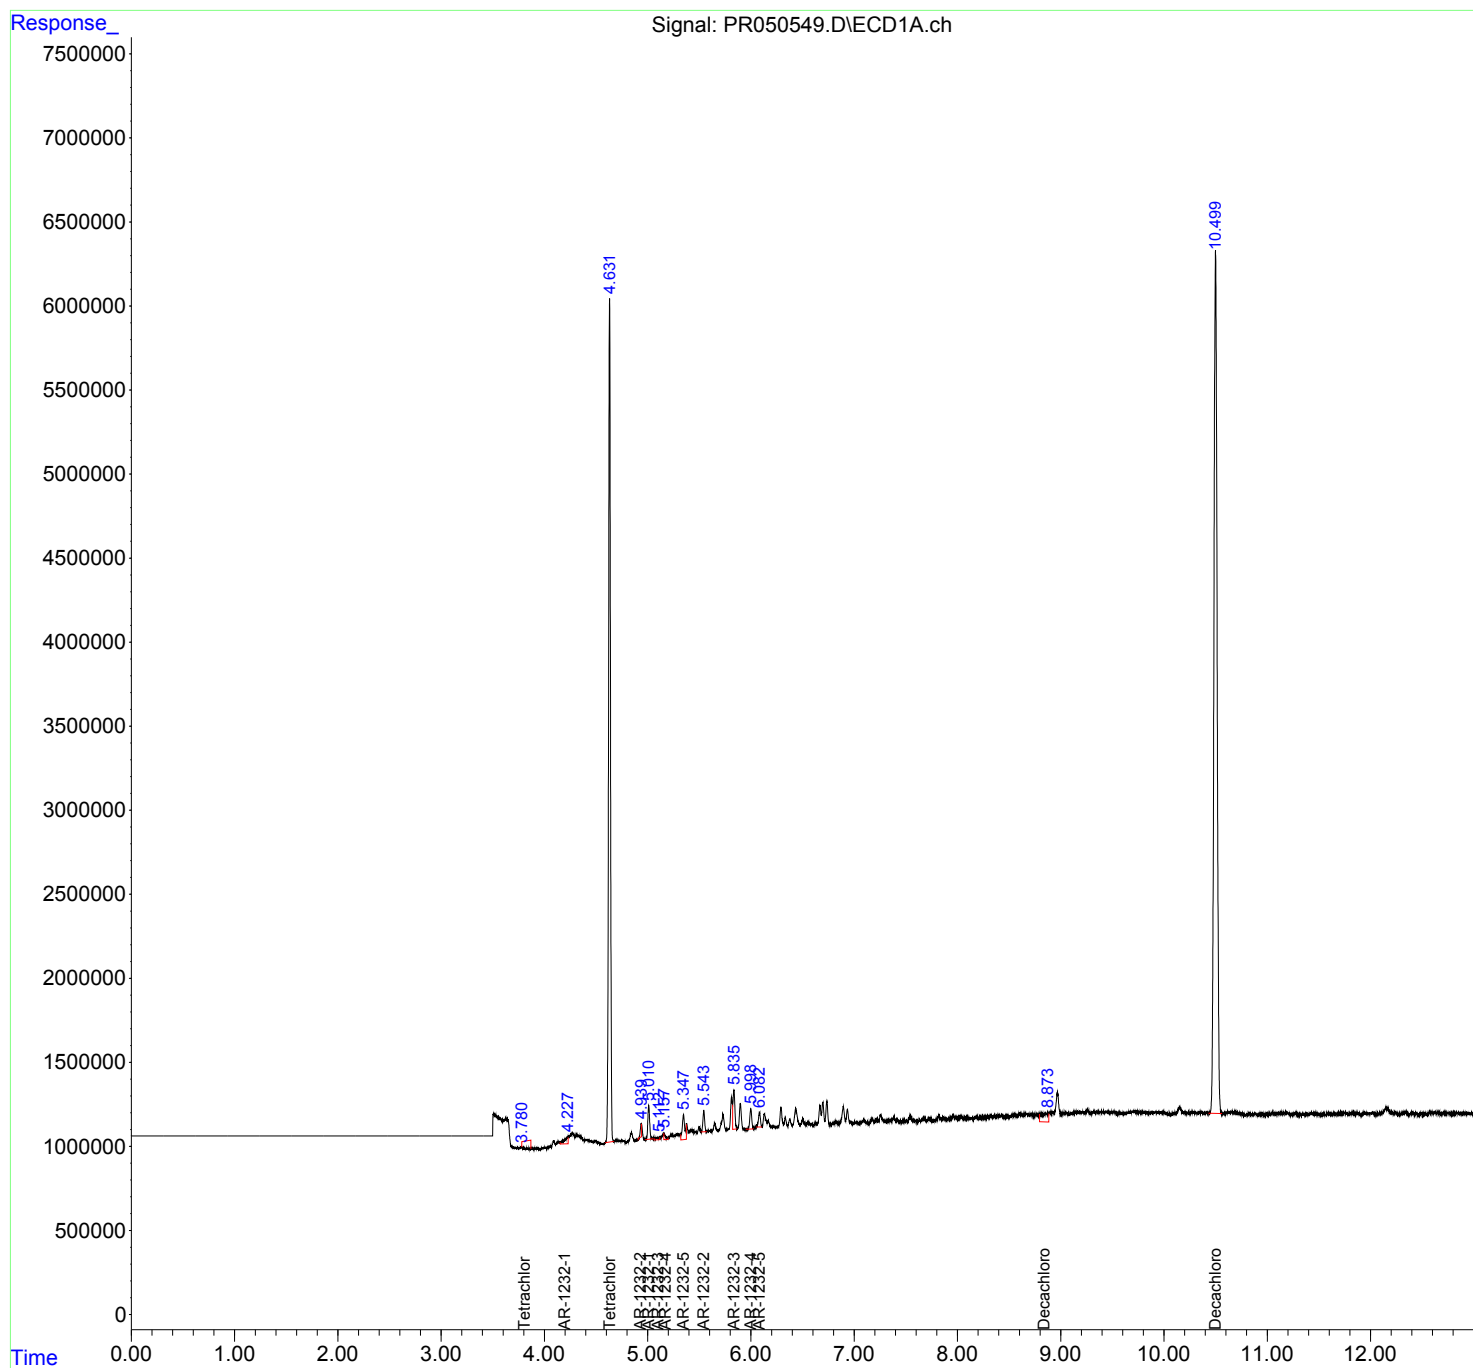


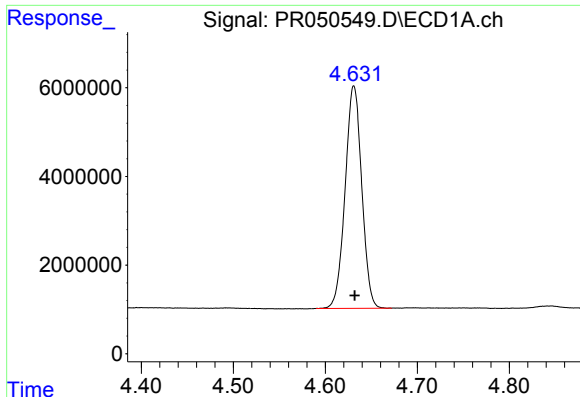

#1 Tetrachloro-m-xylene


R.T.: 4.631 min
Delta R.T.: -0.001 min
Response: 62934810
Conc: 15.02 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

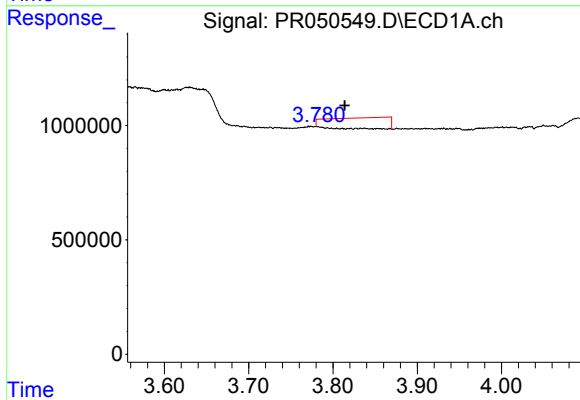


#1 Tetrachloro-m-xylene

R.T.: 3.814 min
Delta R.T.: 0.000 min
Response: 89224868
Conc: 15.11 ng/ml

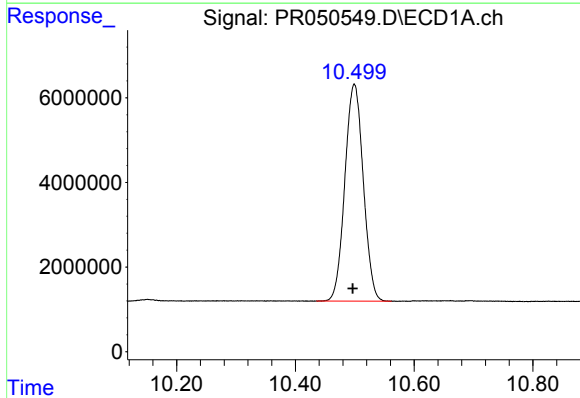


#2 Decachlorobiphenyl

R.T.: 10.499 min
Delta R.T.: 0.003 min
Response: 110333303
Conc: 16.32 ng/ml

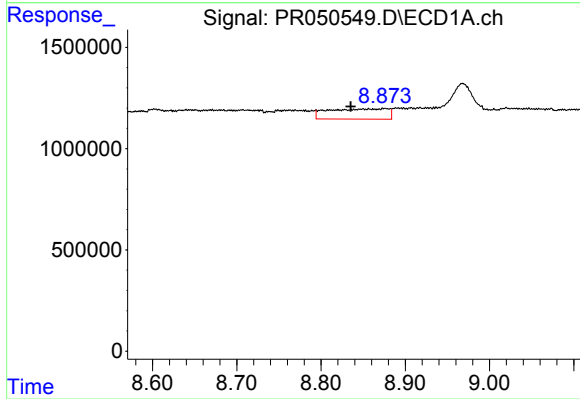

#2 Decachlorobiphenyl


R.T.: 8.839 min
Delta R.T.: 0.004 min
Response: 118877043
Conc: 15.78 ng/ml

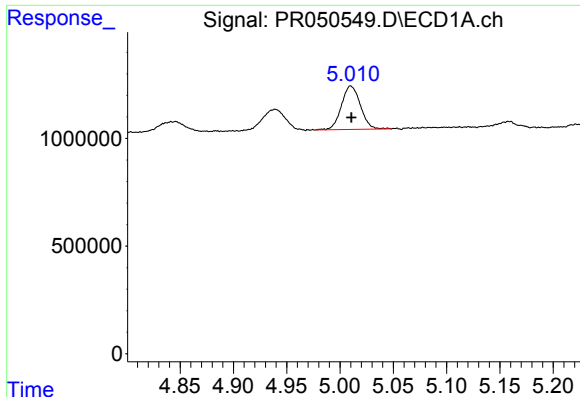

#11 AR-1232-1


R.T.: 5.010 min
Delta R.T.: 0.000 min
Response: 2500355
Conc: 25.92 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

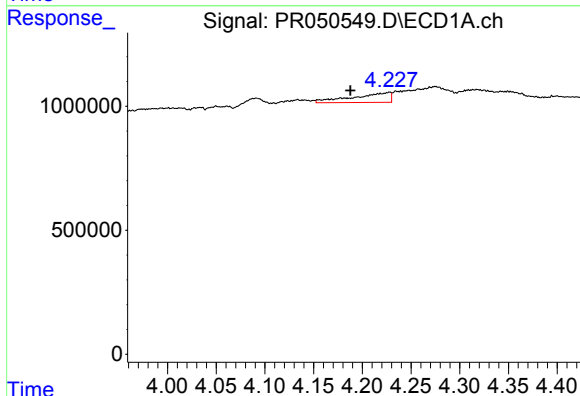


#11 AR-1232-1

R.T.: 4.189 min
Delta R.T.: 0.000 min
Response: 3020097
Conc: 25.51 ng/ml

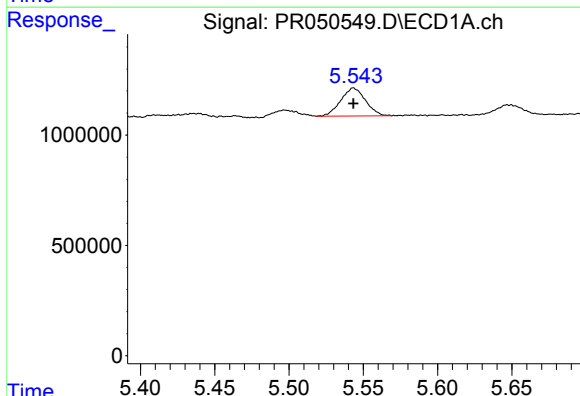


#12 AR-1232-2

R.T.: 5.543 min
Delta R.T.: 0.000 min
Response: 1469812
Conc: 24.05 ng/ml

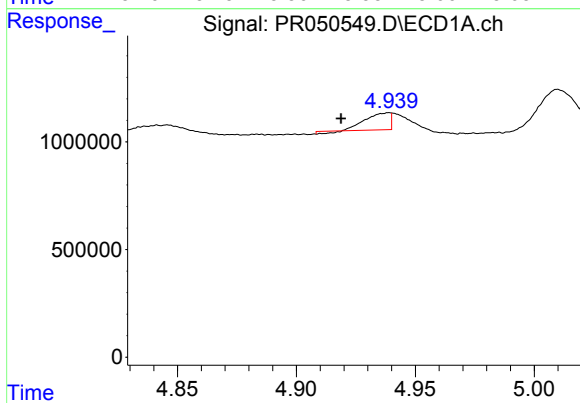

#12 AR-1232-2


R.T.: 4.919 min
Delta R.T.: 0.000 min
Response: 2693246
Conc: 20.20 ng/ml

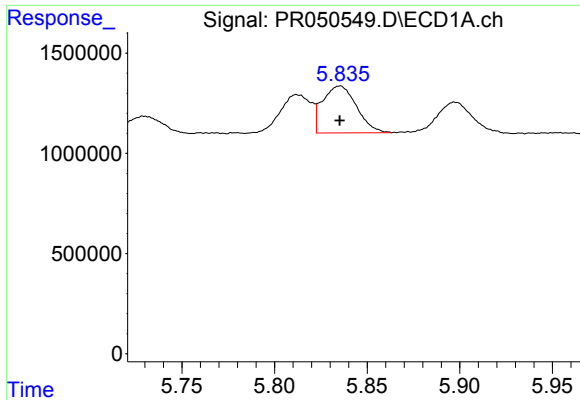

#13 AR-1232-3


R.T.: 5.836 min
Delta R.T.: 0.000 min
Response: 2990793
Conc: 22.60 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

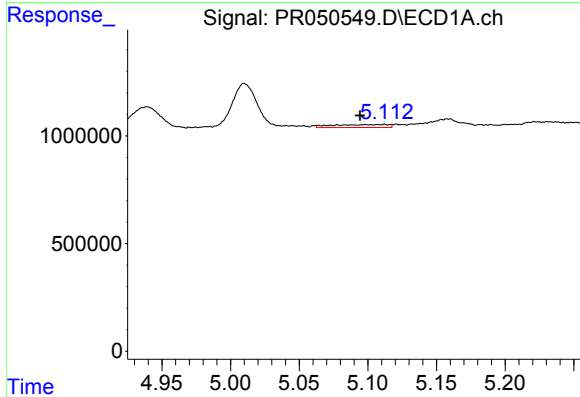


#13 AR-1232-3

R.T.: 5.095 min
Delta R.T.: 0.000 min
Response: 1663601
Conc: 23.72 ng/ml

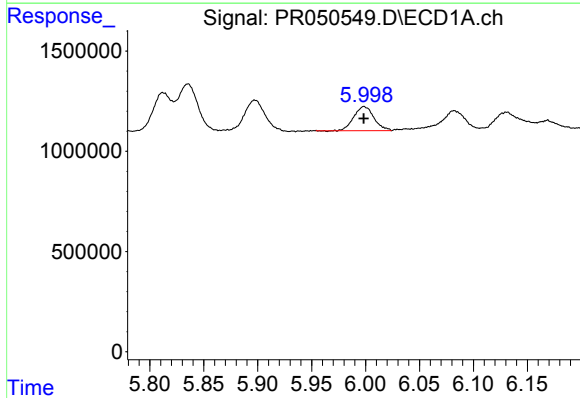


#14 AR-1232-4

R.T.: 5.998 min
Delta R.T.: 0.000 min
Response: 1566412
Conc: 23.36 ng/ml

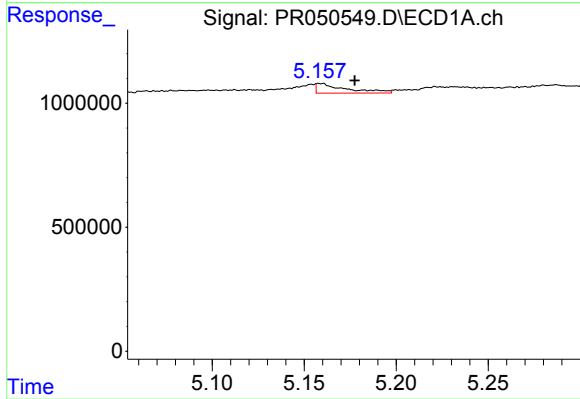

#14 AR-1232-4


R.T.: 5.178 min
Delta R.T.: 0.000 min
Response: 1624159
Conc: 26.39 ng/ml

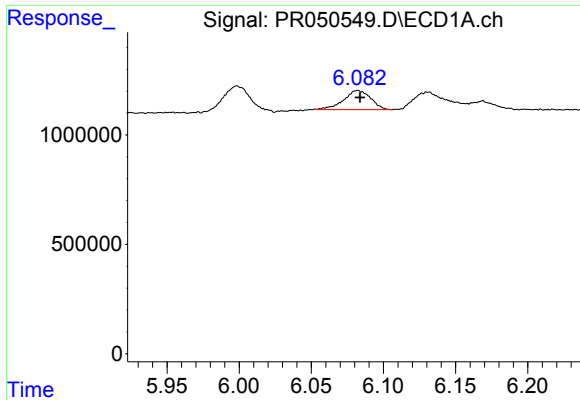

#15 AR-1232-5

R.T.: 6.082 min
Delta R.T.: -0.002 min
Response: 1154850
Conc: 21.87 ng/ml m

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

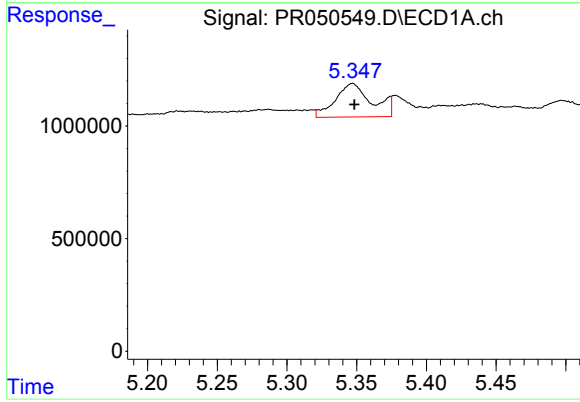

#15 AR-1232-5

R.T.: 5.349 min
Delta R.T.: 0.000 min
Response: 1864545
Conc: 26.68 ng/ml