

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052421\
 Data File : PR050551.D
 Signal(s) : ECD2B.ch
 Acq On : 24 May 21 02:16 pm
 Operator : DD\AJ
 Sample : M2262-09
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT2-2021


Integration File: autoint1.e
 Quant Time: May 24 17:32:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 22 08:50:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.632	3.813	63349597	88413773	15.120	14.972
2) SA Decachlor...	10.500	8.838	106.1E6	113.1E6	15.692	15.022
Target Compounds						
21) L5 AR-1248-1	5.813	4.899	2580796	3164976	19.776	24.203
22) L5 AR-1248-2	6.084	5.136	3179049	3680292	16.843	20.917
23) L5 AR-1248-3	6.292	5.178	4188178	3608948	19.271	19.445
24) L5 AR-1248-4	6.697	5.348	5269206	5501988	20.016	23.675
25) L5 AR-1248-5	6.736	5.740	4796026	5597042	19.119	22.431


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

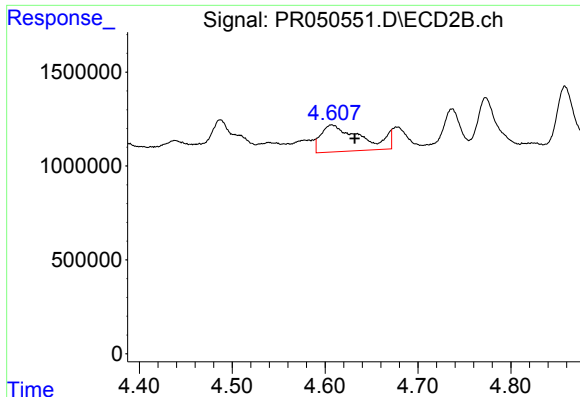

#1 Tetrachloro-m-xylene


R.T.: 4.632 min
Delta R.T.: 0.000 min
Response: 63349597
Conc: 15.12 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

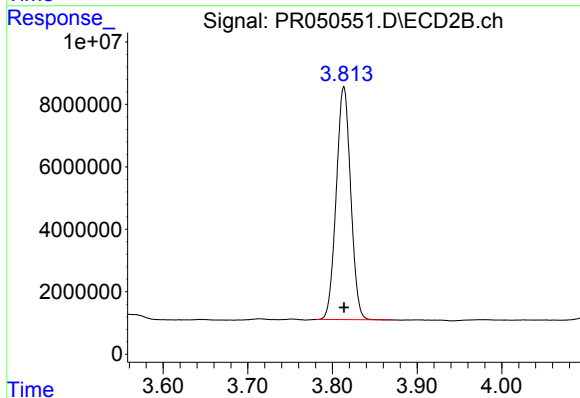


#1 Tetrachloro-m-xylene

R.T.: 3.813 min
Delta R.T.: 0.000 min
Response: 88413773
Conc: 14.97 ng/ml

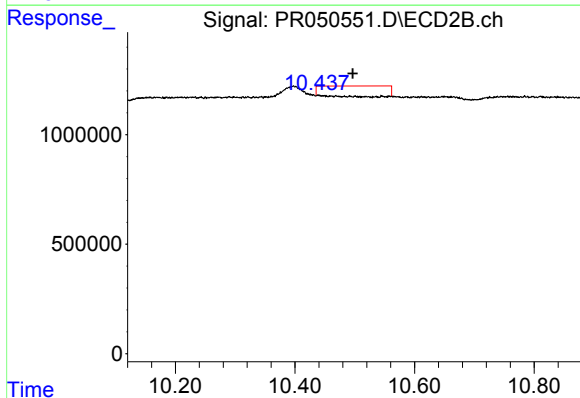


#2 Decachlorobiphenyl

R.T.: 10.500 min
Delta R.T.: 0.003 min
Response: 106088116
Conc: 15.69 ng/ml

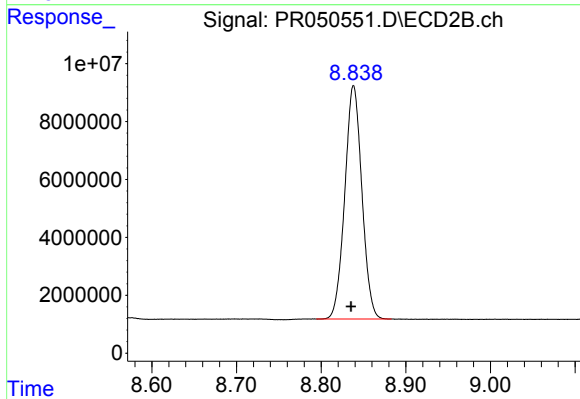

#2 Decachlorobiphenyl


R.T.: 8.838 min
Delta R.T.: 0.003 min
Response: 113142951
Conc: 15.02 ng/ml

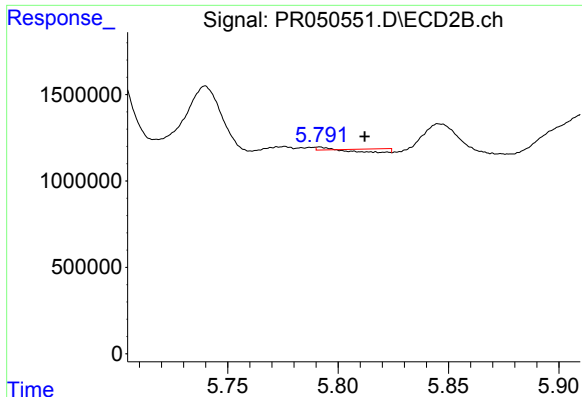

#21 AR-1248-1


R.T.: 5.813 min
Delta R.T.: 0.000 min
Response: 2580796
Conc: 19.78 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

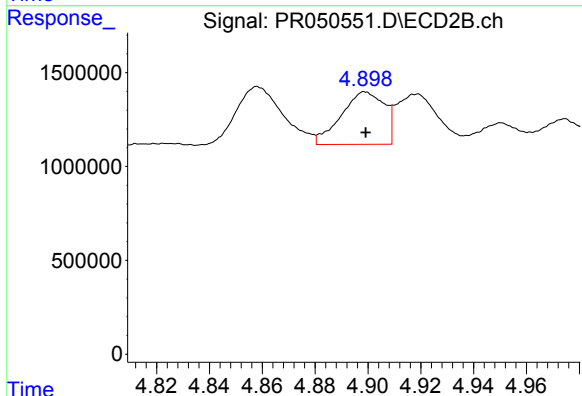


#21 AR-1248-1

R.T.: 4.899 min
Delta R.T.: 0.000 min
Response: 3164976
Conc: 24.20 ng/ml

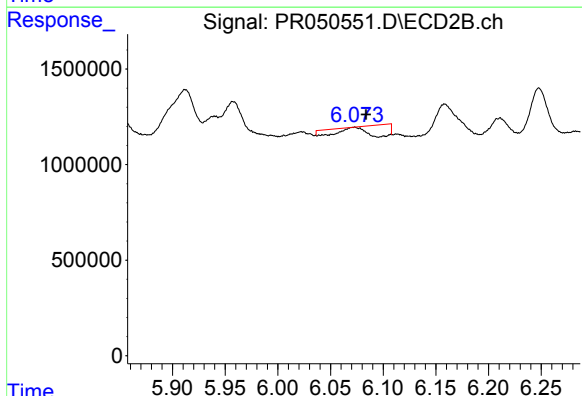


#22 AR-1248-2

R.T.: 6.084 min
Delta R.T.: 0.000 min
Response: 3179049
Conc: 16.84 ng/ml

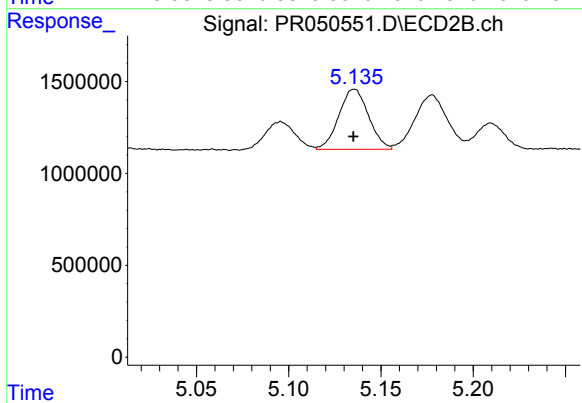

#22 AR-1248-2


R.T.: 5.136 min
Delta R.T.: 0.000 min
Response: 3680292
Conc: 20.92 ng/ml

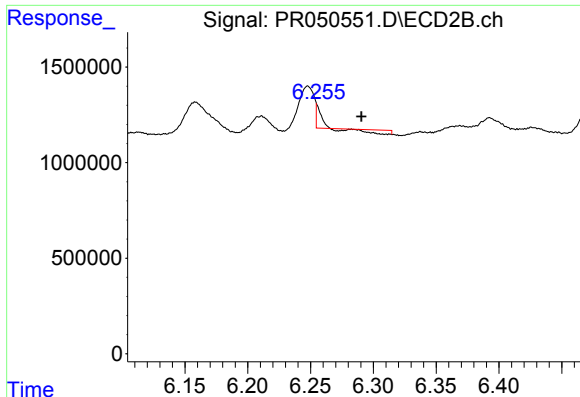

#23 AR-1248-3


R.T.: 6.292 min
Delta R.T.: 0.001 min
Response: 4188178
Conc: 19.27 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

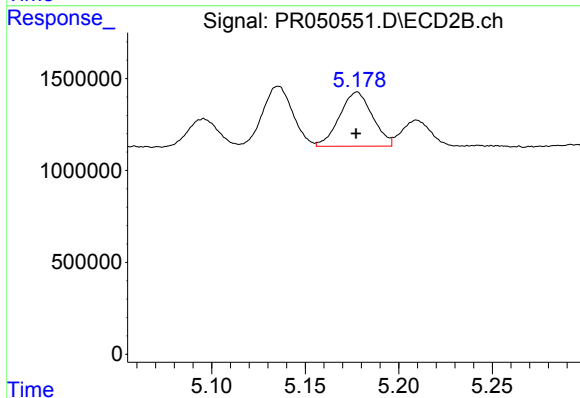


#23 AR-1248-3

R.T.: 5.178 min
Delta R.T.: 0.000 min
Response: 3608948
Conc: 19.45 ng/ml

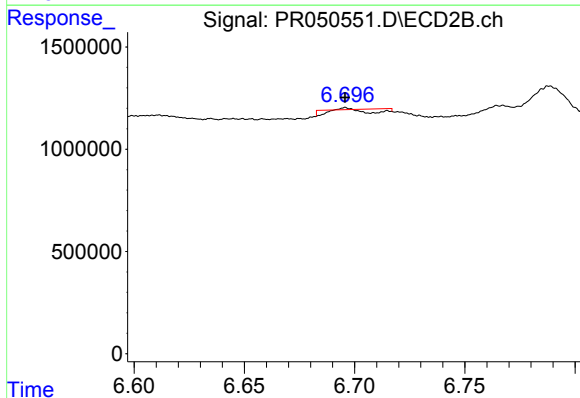


#24 AR-1248-4

R.T.: 6.697 min
Delta R.T.: 0.001 min
Response: 5269206
Conc: 20.02 ng/ml

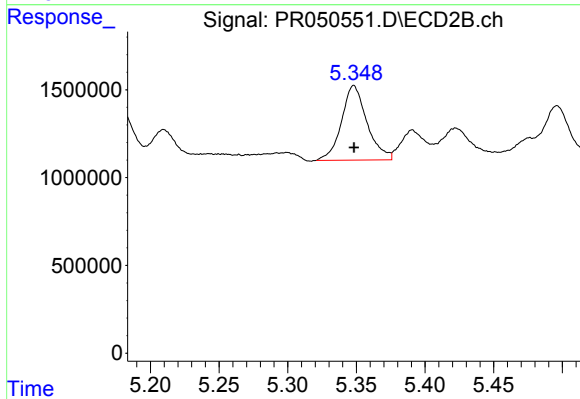

#24 AR-1248-4


R.T.: 5.348 min
Delta R.T.: 0.000 min
Response: 5501988
Conc: 23.68 ng/ml

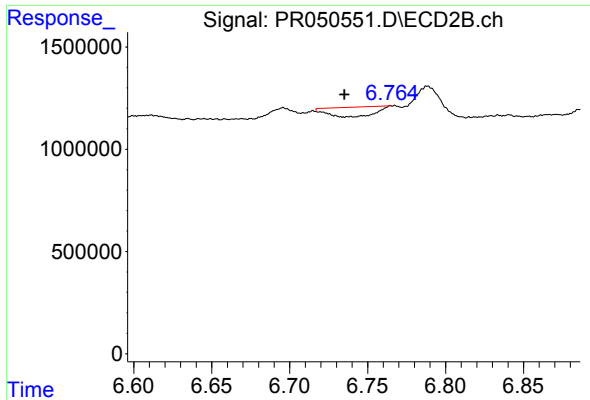

#25 AR-1248-5

R.T.: 6.736 min
Delta R.T.: 0.000 min
Response: 4796026
Conc: 19.12 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

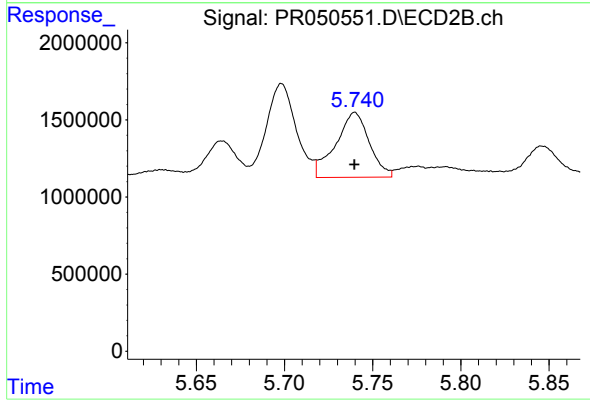

#25 AR-1248-5

R.T.: 5.740 min
Delta R.T.: 0.000 min
Response: 5597042
Conc: 22.43 ng/ml