

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052421\
 Data File : PR050552.D
 Signal(s) : ECD2B.ch
 Acq On : 24 May 21 02:31 pm
 Operator : DD\AJ
 Sample : M2262-09
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT2-2021

Integration File: autoint1.e
 Quant Time: May 24 17:33:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 22 08:50:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.631	3.813	79302111	112.4E6	18.927	19.030
2)	SA Decachlor...	10.498	8.839	131.5E6	142.1E6	19.448	18.870
Target Compounds							
26)	L6 AR-1254-1	6.668	5.699	6912641	9493853	26.391	25.272
27)	L6 AR-1254-2	6.885	5.846	10704586	9033995	25.719	26.893
28)	L6 AR-1254-3	7.256	6.249	10844697	13674387	23.802	23.353
29)	L6 AR-1254-4	7.542	6.475	8522834	8549523	24.402	22.819
30)	L6 AR-1254-5	7.962	6.891	8896946	12732305	22.895m	23.008


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052421\
Data File : PR050552.D
Signal(s) : ECD2B.ch
Acq On : 24 May 21 02:31 pm
Operator : DD\AJ
Sample : M2262-09
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

Integration File: autoint1.e
Quant Time: May 24 17:33:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052221.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 22 08:50:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

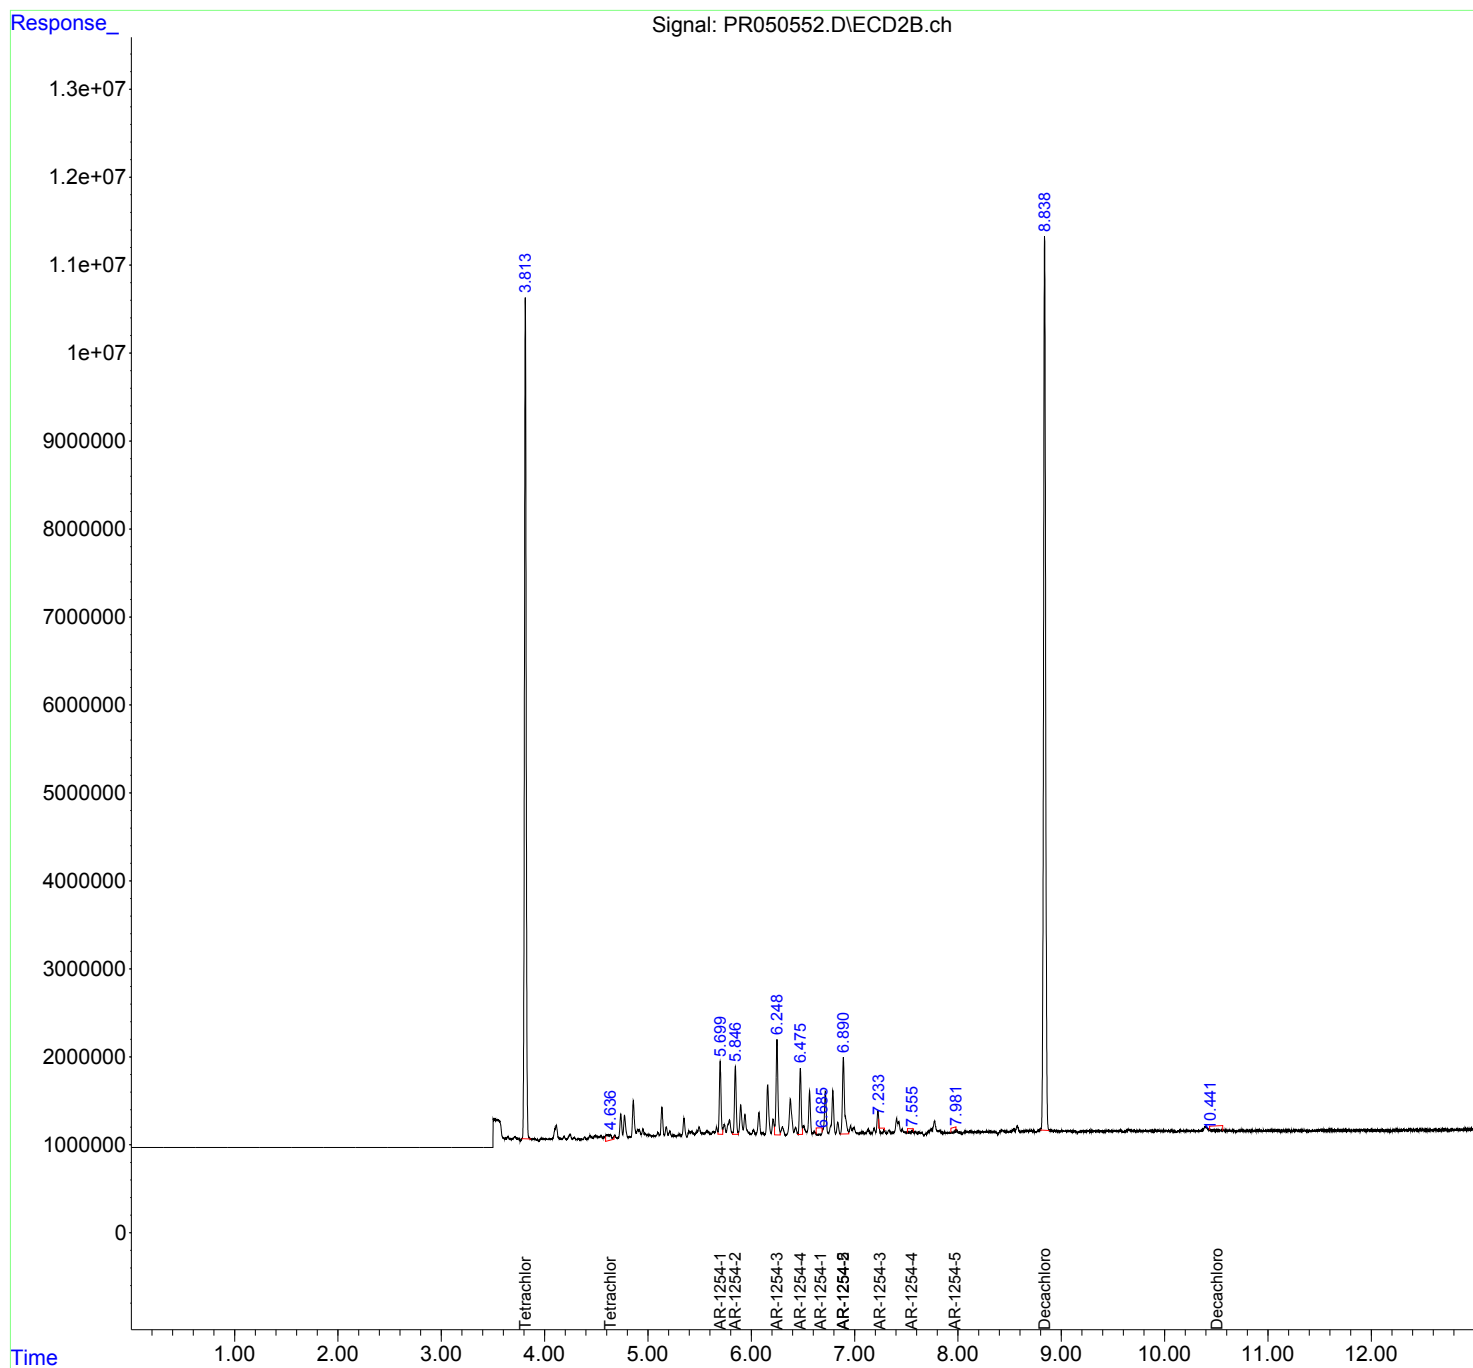


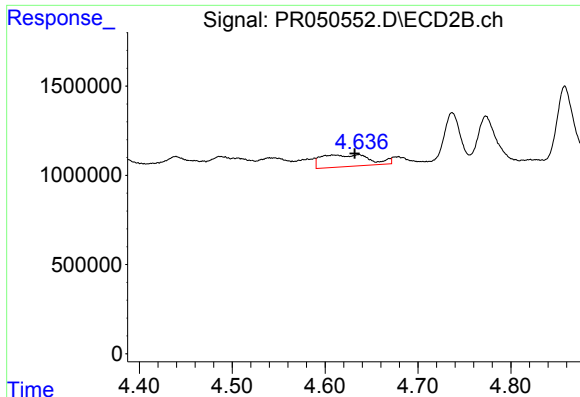

#1 Tetrachloro-m-xylene


R.T.: 4.631 min
Delta R.T.: 0.000 min
Response: 79302111
Conc: 18.93 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

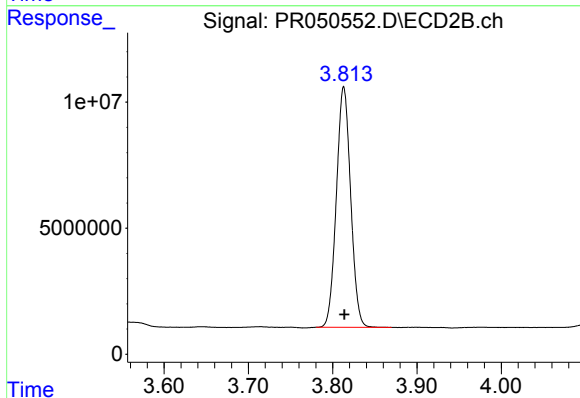


#1 Tetrachloro-m-xylene

R.T.: 3.813 min
Delta R.T.: 0.000 min
Response: 112374955
Conc: 19.03 ng/ml

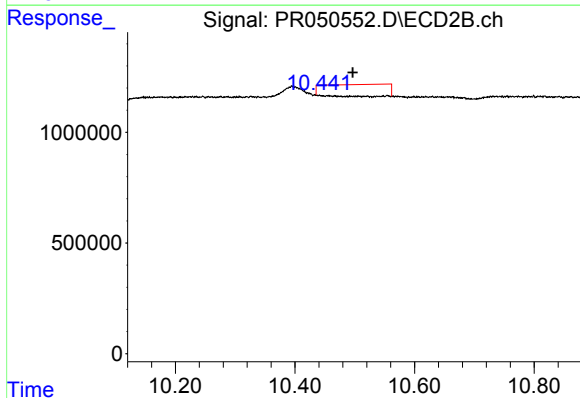


#2 Decachlorobiphenyl

R.T.: 10.498 min
Delta R.T.: 0.002 min
Response: 131484900
Conc: 19.45 ng/ml

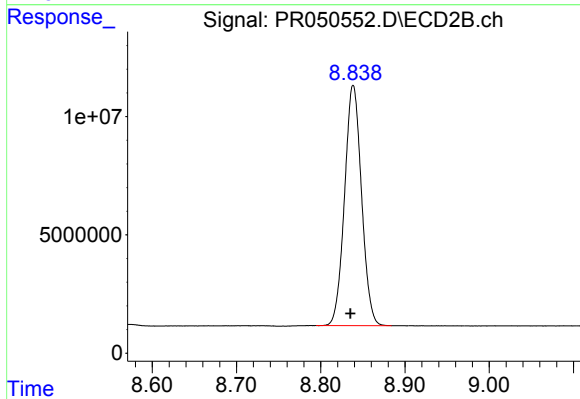

#2 Decachlorobiphenyl


R.T.: 8.839 min
Delta R.T.: 0.003 min
Response: 142126610
Conc: 18.87 ng/ml

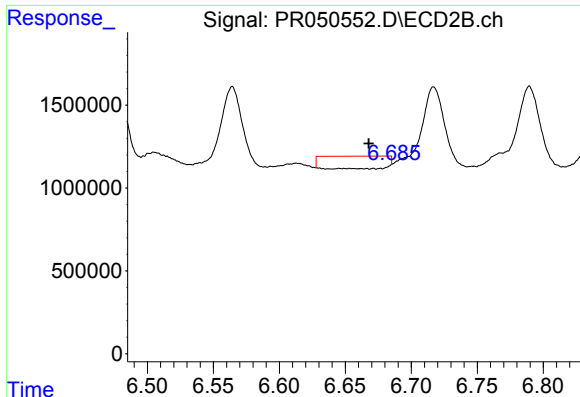

#26 AR-1254-1


R.T.: 6.668 min
Delta R.T.: 0.000 min
Response: 6912641
Conc: 26.39 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

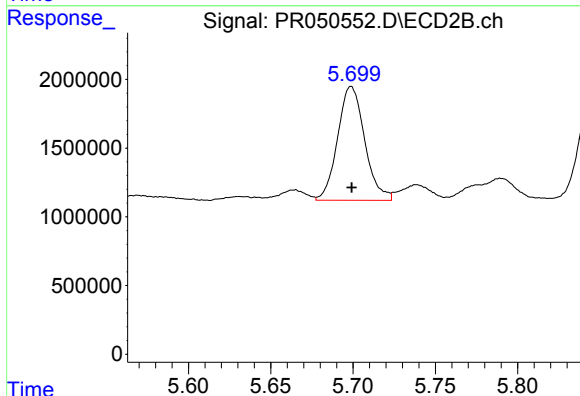


#26 AR-1254-1

R.T.: 5.699 min
Delta R.T.: 0.000 min
Response: 9493853
Conc: 25.27 ng/ml

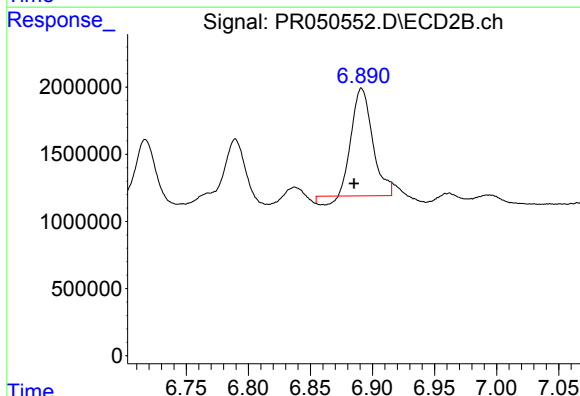


#27 AR-1254-2

R.T.: 6.885 min
Delta R.T.: 0.000 min
Response: 10704586
Conc: 25.72 ng/ml

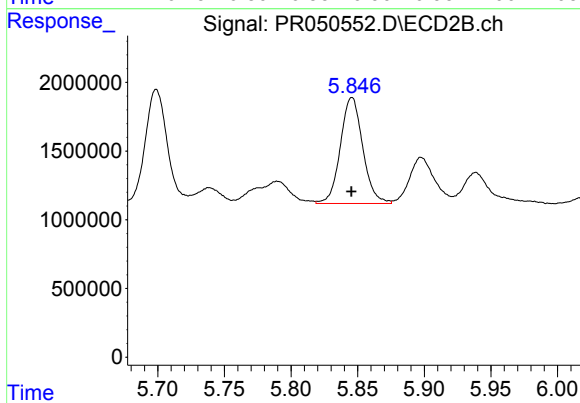

#27 AR-1254-2


R.T.: 5.846 min
Delta R.T.: 0.000 min
Response: 9033995
Conc: 26.89 ng/ml

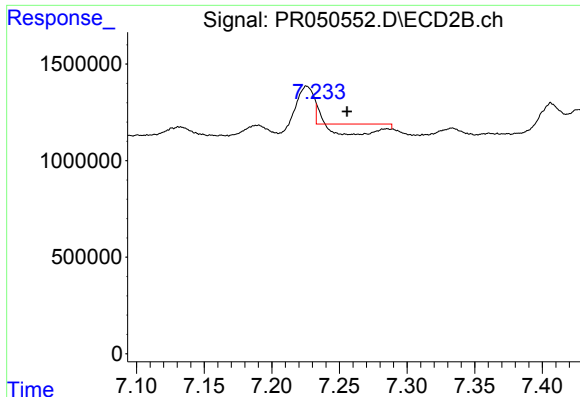

#28 AR-1254-3


R.T.: 7.256 min
Delta R.T.: 0.000 min
Response: 10844697
Conc: 23.80 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

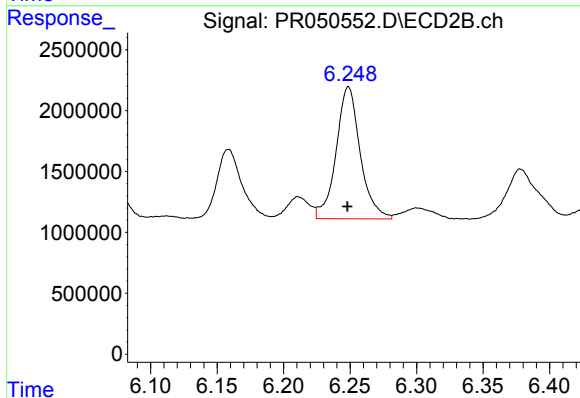


#28 AR-1254-3

R.T.: 6.249 min
Delta R.T.: 0.000 min
Response: 13674387
Conc: 23.35 ng/ml

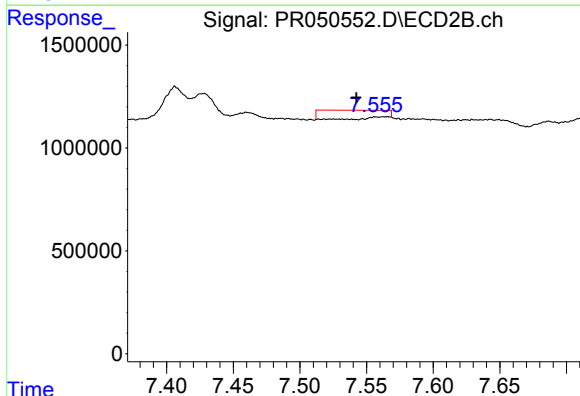


#29 AR-1254-4

R.T.: 7.542 min
Delta R.T.: 0.000 min
Response: 8522834
Conc: 24.40 ng/ml

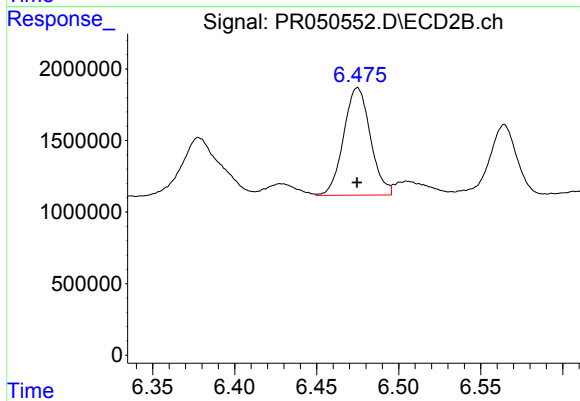

#29 AR-1254-4


R.T.: 6.475 min
Delta R.T.: 0.000 min
Response: 8549523
Conc: 22.82 ng/ml

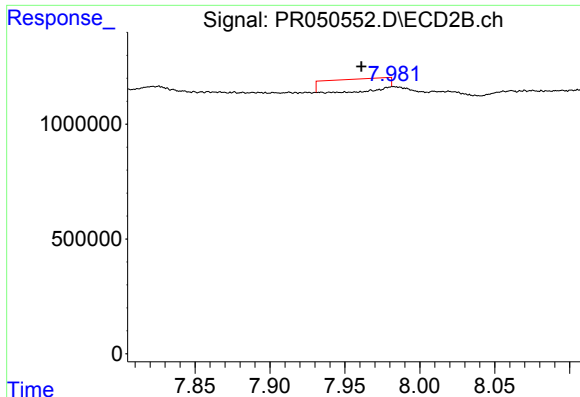

#30 AR-1254-5

R.T.: 7.962 min
Delta R.T.: 0.000 min
Response: 8896946
Conc: 22.89 ng/ml m

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

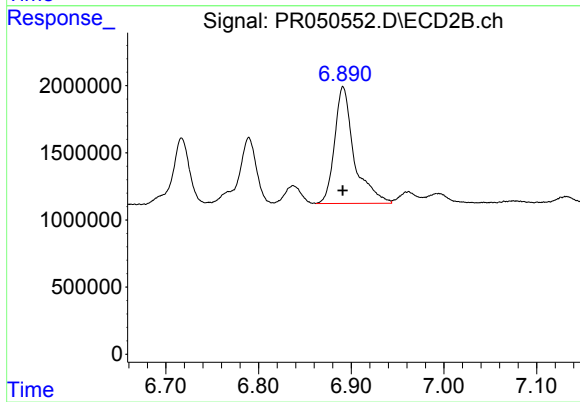

#30 AR-1254-5

R.T.: 6.891 min
Delta R.T.: 0.000 min
Response: 12732305
Conc: 23.01 ng/ml