

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052421\
 Data File : PR050554.D
 Signal(s) : ECD2B.ch
 Acq On : 24 May 21 03:02 pm
 Operator : DD\AJ
 Sample : M2262-09
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT2-2021

Integration File: autoint1.e
 Quant Time: May 24 17:34:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 22 08:50:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.632	3.814	77808024	110.4E6	18.571	18.691
2) SA Decachlor...	10.499	8.838	138.9E6	149.7E6	20.546	19.880
Target Compounds						
41) L9 AR-1268-1	8.924	7.712	23851025	25849084	24.961	22.654
42) L9 AR-1268-2	9.025	7.776	21178871	23614240	24.666	22.306
43) L9 AR-1268-3	9.261	7.984	17866198	20572339	24.693	23.484
44) L9 AR-1268-4	9.716	8.274	8167973	8900465	25.687	23.778
45) L9 AR-1268-5	10.148	8.575	57412992	62137394	22.565	21.487


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052421\
Data File : PR050554.D
Signal(s) : ECD2B.ch
Acq On : 24 May 21 03:02 pm
Operator : DD\AJ
Sample : M2262-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

Integration File: autoint1.e
Quant Time: May 24 17:34:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052221.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 22 08:50:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

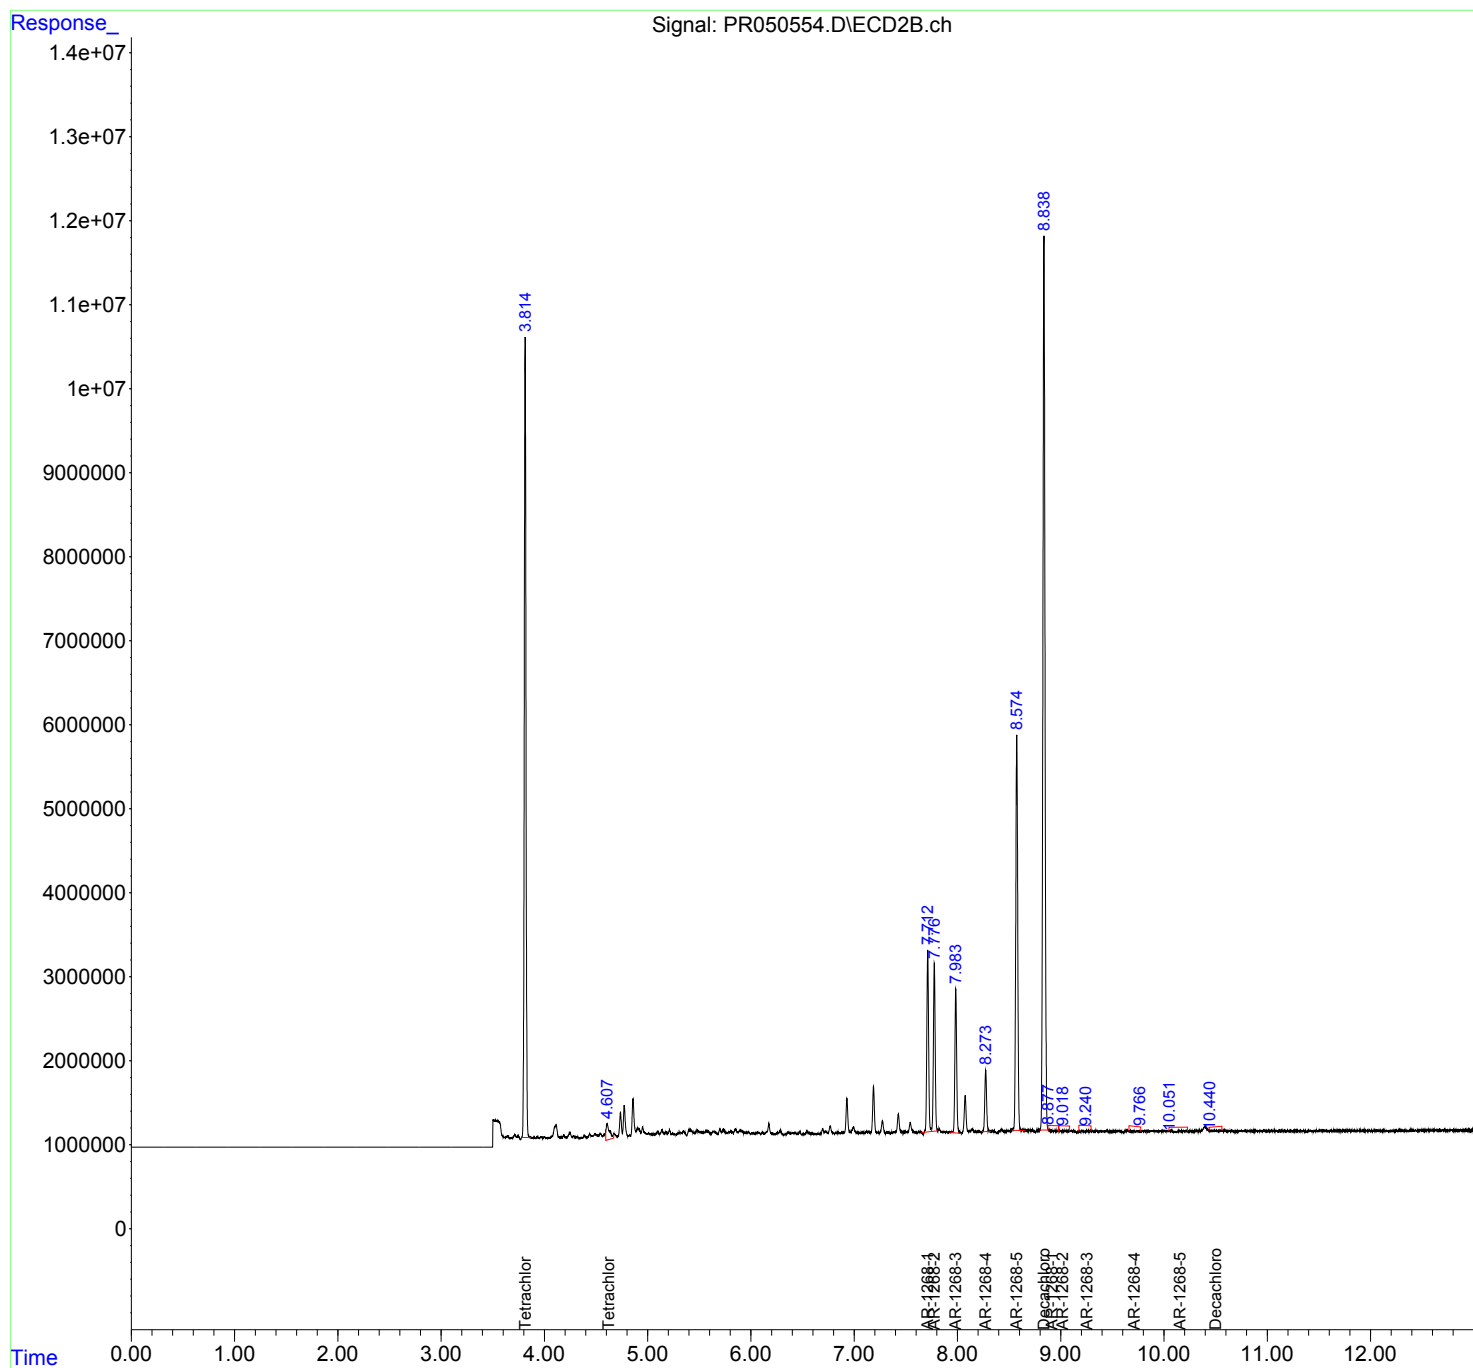


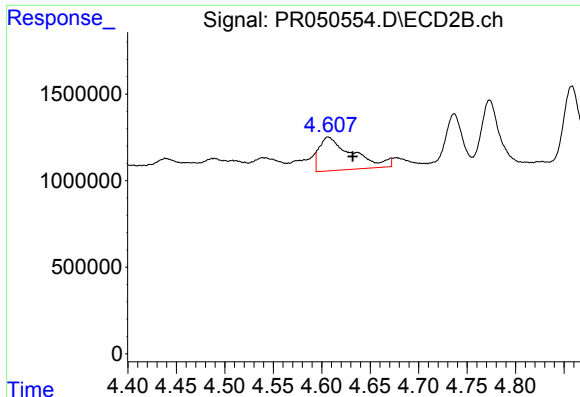

#1 Tetrachloro-m-xylene


R.T.: 4.632 min
Delta R.T.: 0.000 min
Response: 77808024
Conc: 18.57 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

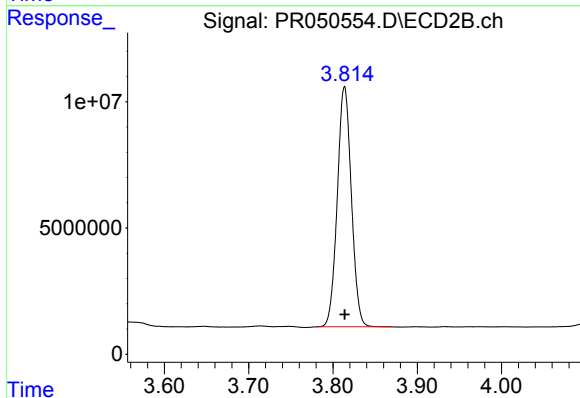


#1 Tetrachloro-m-xylene

R.T.: 3.814 min
Delta R.T.: 0.000 min
Response: 110372291
Conc: 18.69 ng/ml

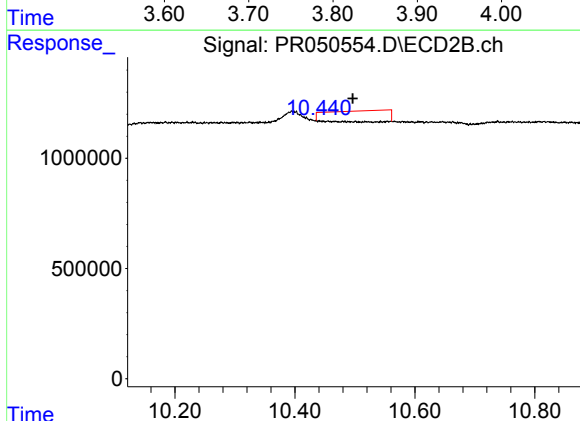


#2 Decachlorobiphenyl

R.T.: 10.499 min
Delta R.T.: 0.002 min
Response: 138910351
Conc: 20.55 ng/ml

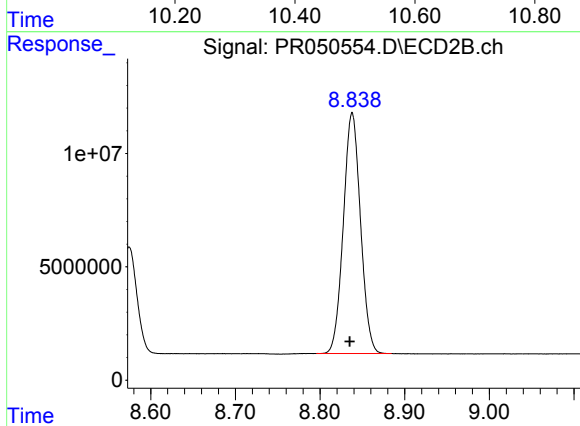

#2 Decachlorobiphenyl


R.T.: 8.838 min
Delta R.T.: 0.003 min
Response: 149739223
Conc: 19.88 ng/ml

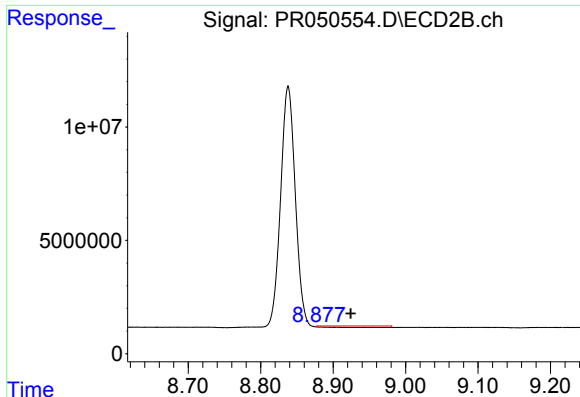

#41 AR-1268-1


R.T.: 8.924 min
Delta R.T.: 0.000 min
Response: 23851025
Conc: 24.96 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

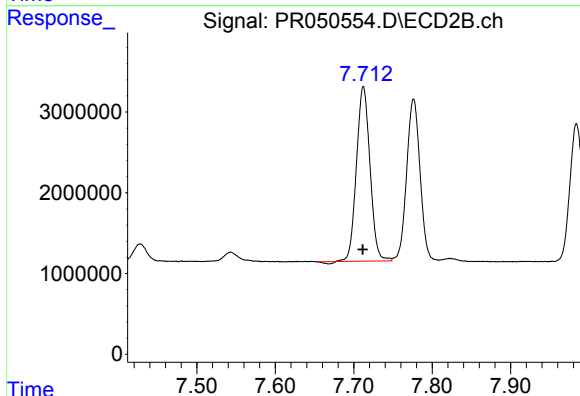


#41 AR-1268-1

R.T.: 7.712 min
Delta R.T.: 0.000 min
Response: 25849084
Conc: 22.65 ng/ml

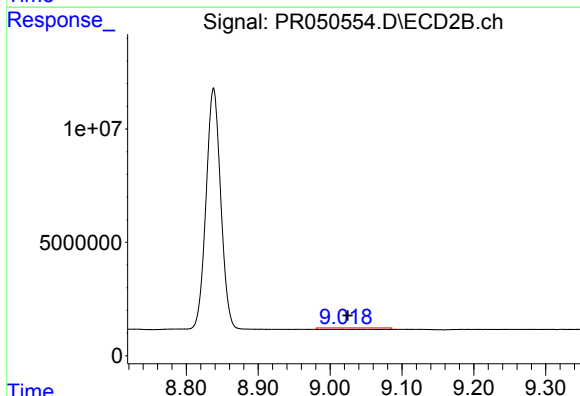


#42 AR-1268-2

R.T.: 9.025 min
Delta R.T.: 0.000 min
Response: 21178871
Conc: 24.67 ng/ml

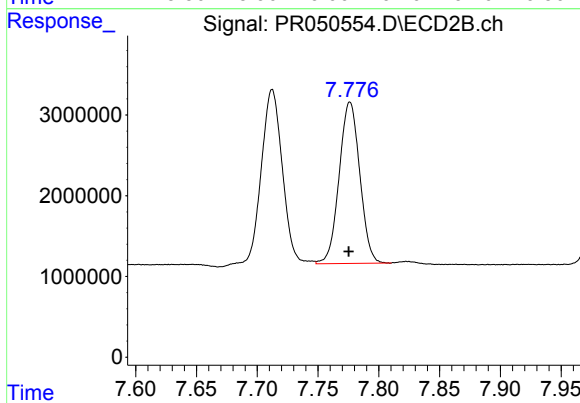

#42 AR-1268-2


R.T.: 7.776 min
Delta R.T.: 0.000 min
Response: 23614240
Conc: 22.31 ng/ml

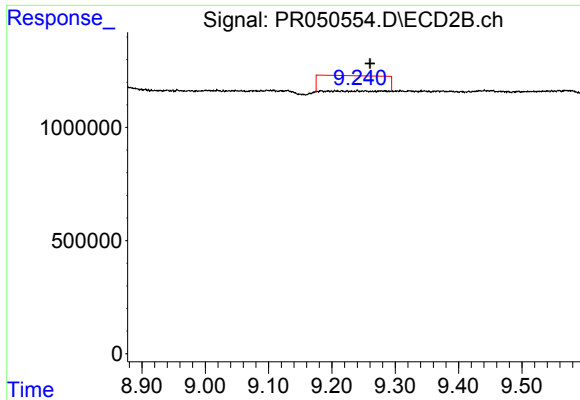

#43 AR-1268-3


R.T.: 9.261 min
Delta R.T.: 0.000 min
Response: 17866198
Conc: 24.69 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

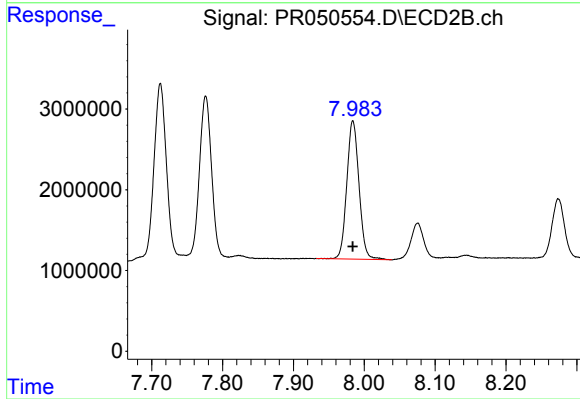


#43 AR-1268-3

R.T.: 7.984 min
Delta R.T.: 0.000 min
Response: 20572339
Conc: 23.48 ng/ml

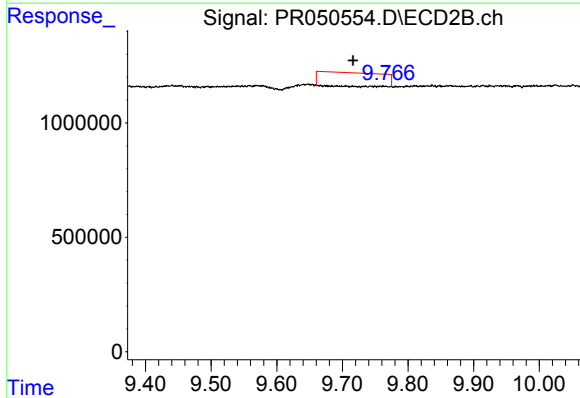


#44 AR-1268-4

R.T.: 9.716 min
Delta R.T.: 0.000 min
Response: 8167973
Conc: 25.69 ng/ml

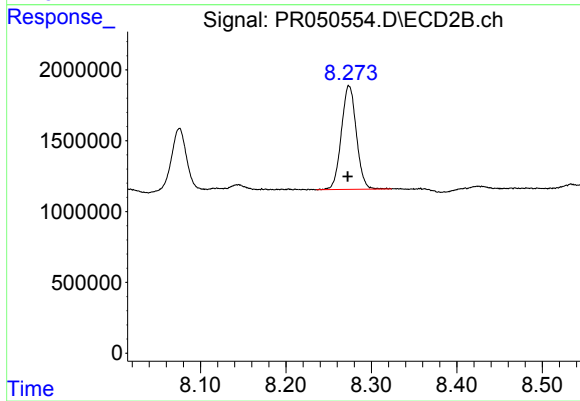

#44 AR-1268-4


R.T.: 8.274 min
Delta R.T.: 0.002 min
Response: 8900465
Conc: 23.78 ng/ml

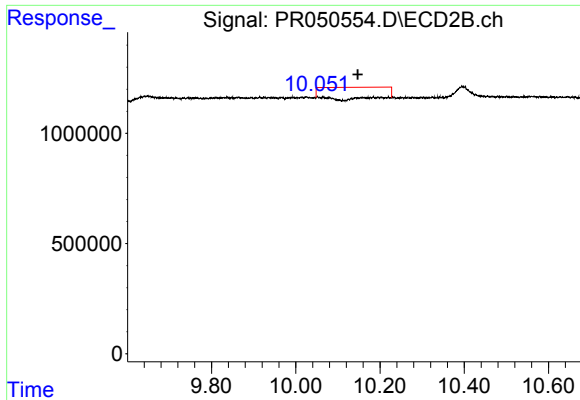

#45 AR-1268-5

R.T.: 10.148 min
Delta R.T.: 0.000 min
Response: 57412992
Conc: 22.57 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT2-2021

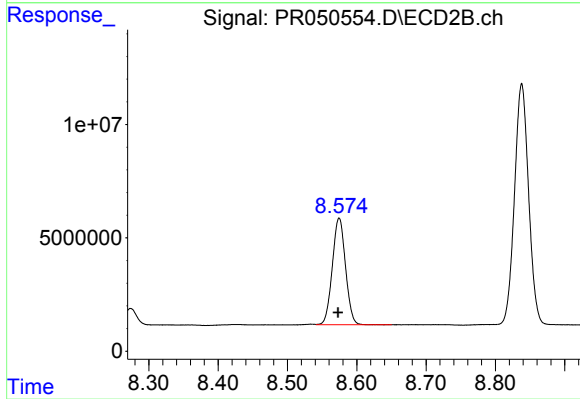

#45 AR-1268-5

R.T.: 8.575 min
Delta R.T.: 0.001 min
Response: 62137394
Conc: 21.49 ng/ml