

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052522\
 Data File : PR054329.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2022 15:40
 Operator : AJ\MA
 Sample : N2981-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 SB-13(0.5-1)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/27/2022
 Supervised By :Ankita Jodhani 05/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 02:22:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 25 15:27:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.650	2.922	76354076	37913557	20.701	20.071
2) SA Decachlor...	9.539	8.162	27271212	25392740	17.850	17.633

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052522\
Data File : PR054329.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2022 15:40
Operator : AJ\MA
Sample : N2981-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
SB-13(0.5-1)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/27/2022
Supervised By :Ankita Jodhani 05/27/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 02:22:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052522.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 25 15:27:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

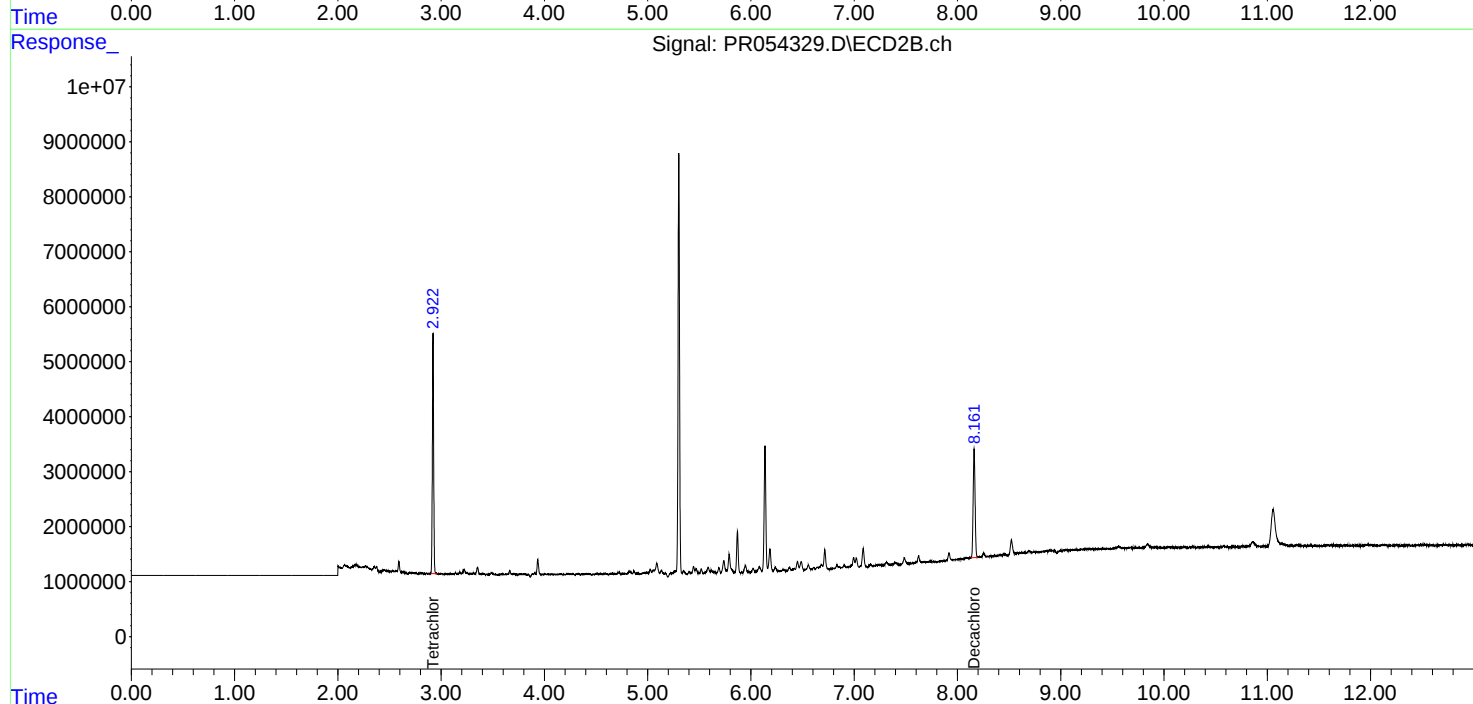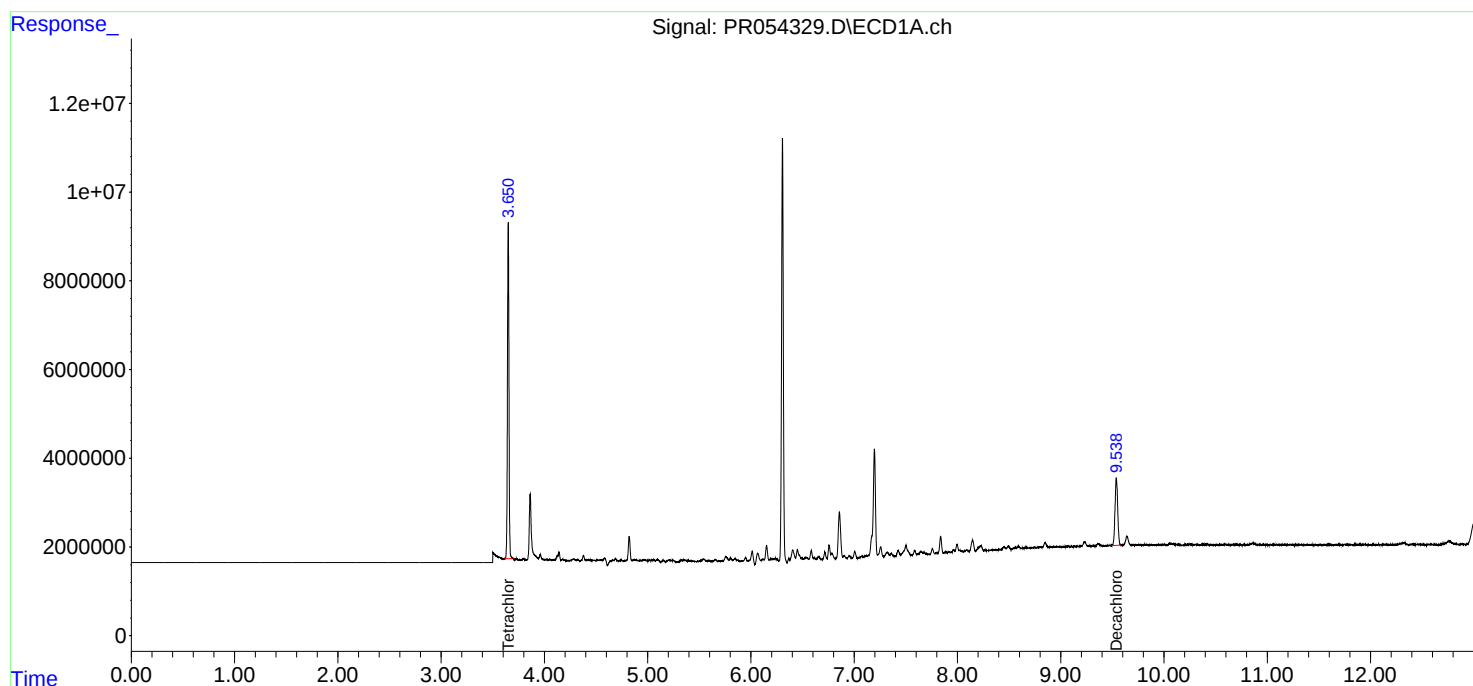

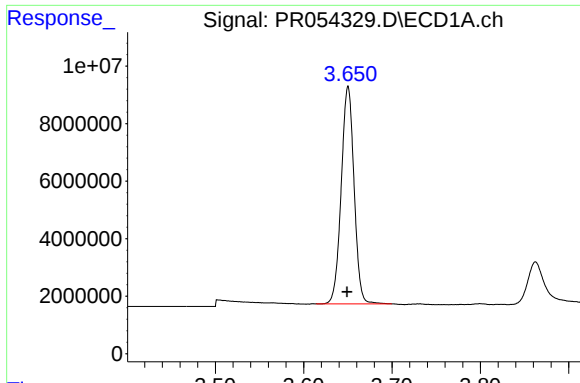


#1 Tetrachloro-m-xylene

R.T.: 3.650 min
Delta R.T.: 0.001 min
Response: 76354076
Conc: 20.70 ng/ml

Instrument :
ECD_R
ClientSampleId :
SB-13(0.5-1)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/27/2022
Supervised By :Ankita Jodhani 05/27/2022

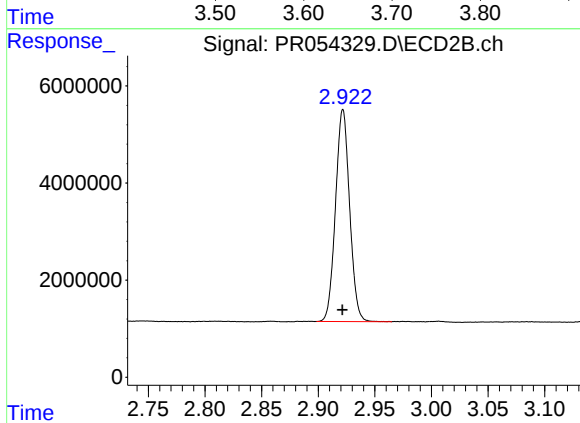


#1 Tetrachloro-m-xylene

R.T.: 2.922 min
Delta R.T.: 0.000 min
Response: 37913557
Conc: 20.07 ng/ml

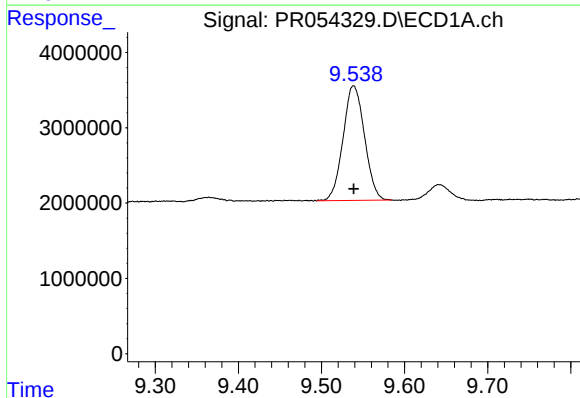

#2 Decachlorobiphenyl

R.T.: 9.539 min
Delta R.T.: 0.000 min
Response: 27271212
Conc: 17.85 ng/ml

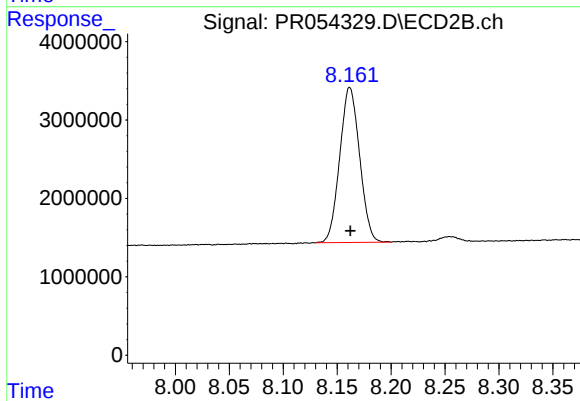

#2 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 25392740
Conc: 17.63 ng/ml