

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR052524\  
Data File : PR066908.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 24 May 2024 12:26  
Operator : AJ\MA  
Sample : P2570-11  
Misc :  
ALS Vial : 19 Sample Multiplier: 1



Instrument :  
ECD\_R  
ClientSampleId :  
BH6C0

## Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 05/28/2024  
Supervised By :Ankita Jodhani 05/28/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 25 00:08:06 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR052124CLP.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed May 22 04:28:16 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

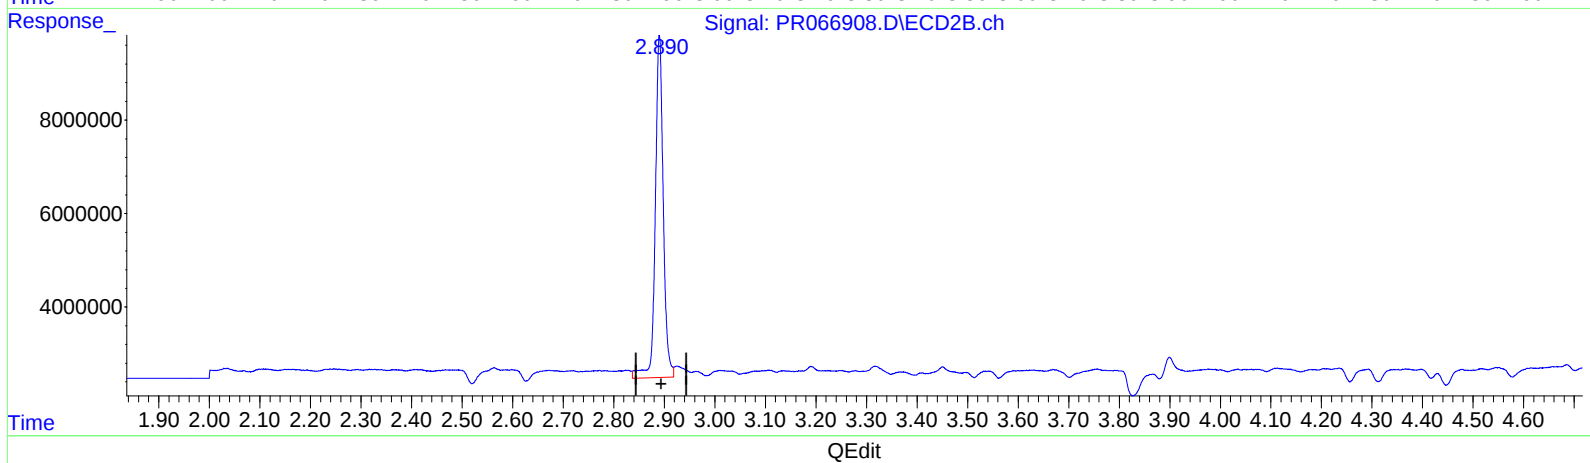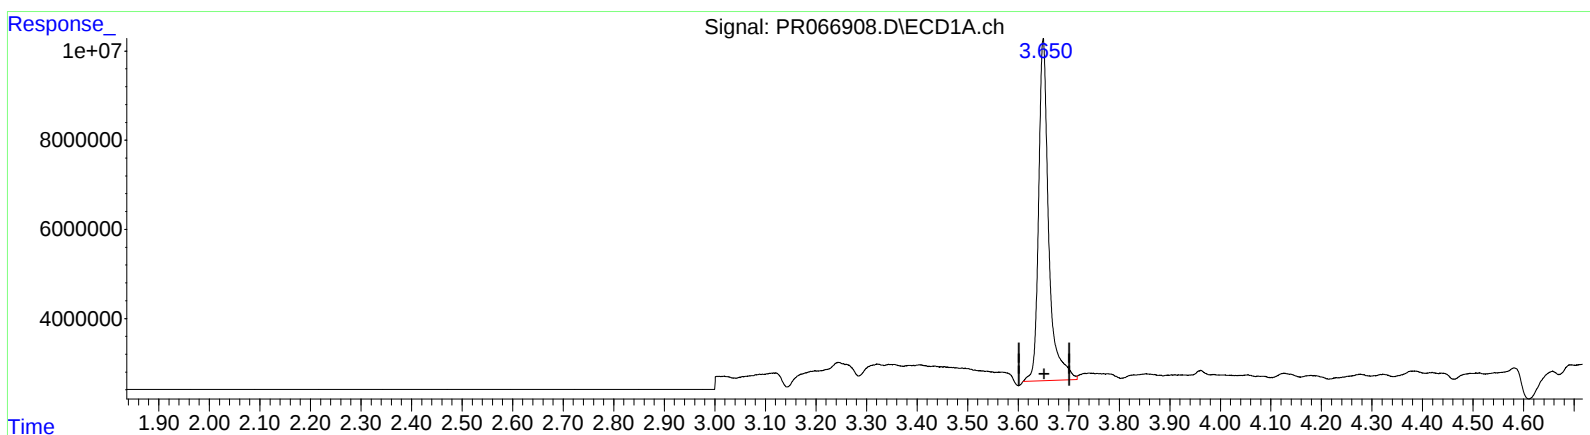

(1) Tetrachloro-m-xylene (SA)

3.650min 17.311 ng/ml

response 106195220

(1) Tetrachloro-m-xylene #2 (SA)

2.890min 17.280 ng/ml

response 80454967

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR052524\  
Data File : PR066908.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 24 May 2024 12:26  
Operator : AJ\MA  
Sample : P2570-11  
Misc :  
ALS Vial : 19 Sample Multiplier: 1



Instrument :  
ECD\_R  
ClientSampleId :  
BH6C0

## Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 05/28/2024  
Supervised By :Ankita Jodhani 05/28/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 25 00:08:06 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR052124CLP.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed May 22 04:28:16 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

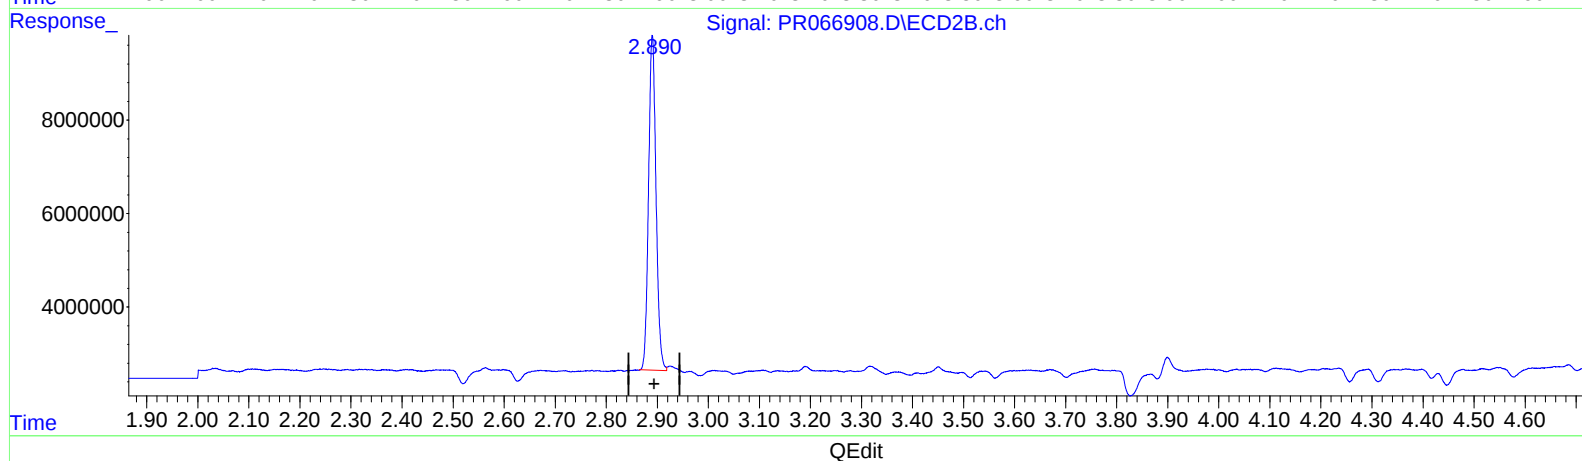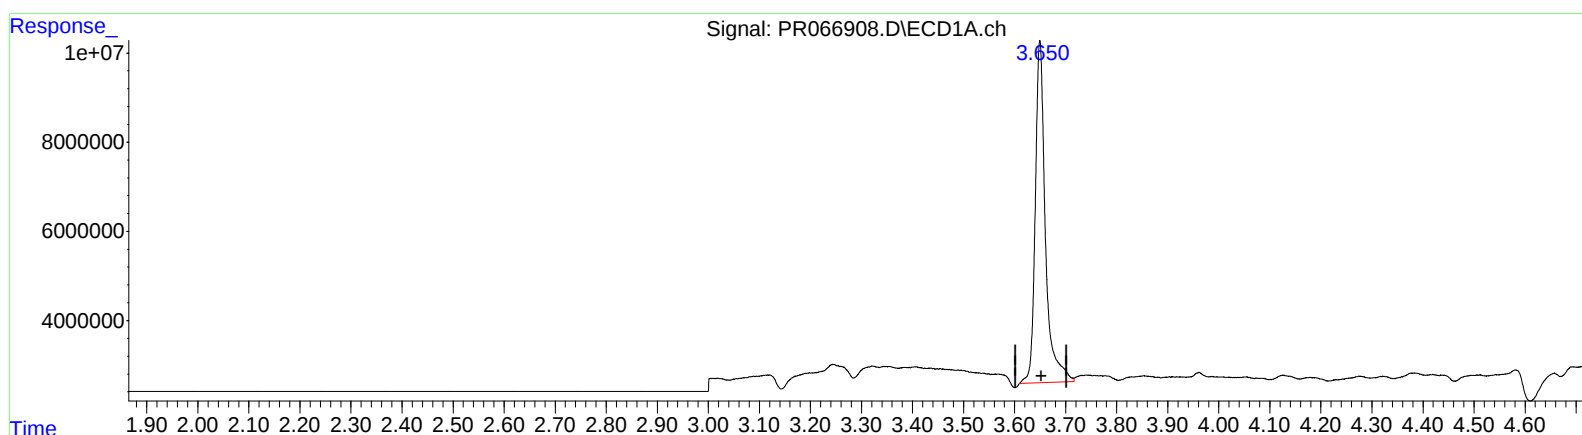

(1) Tetrachloro-m-xylene (SA)

3.650min 17.311 ng/ml

response 106195220

(1) Tetrachloro-m-xylene #2 (SA)

2.890min 15.629 ng/ml m

response 72768155