

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052722\
 Data File : PR054530.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2022 03:51
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/28/2022
 Supervised By :Ankita Jodhani 05/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 04:42:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 25 15:27:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.647	2.921	109.2E6	53876069	29.595	28.522
2) SA Decachlor...	9.534	8.155	45033562	48322030	29.476	33.555m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR052722\
Data File : PR054530.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2022 03:51
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/28/2022
Supervised By :Ankita Jodhani 05/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 04:42:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052522.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 25 15:27:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

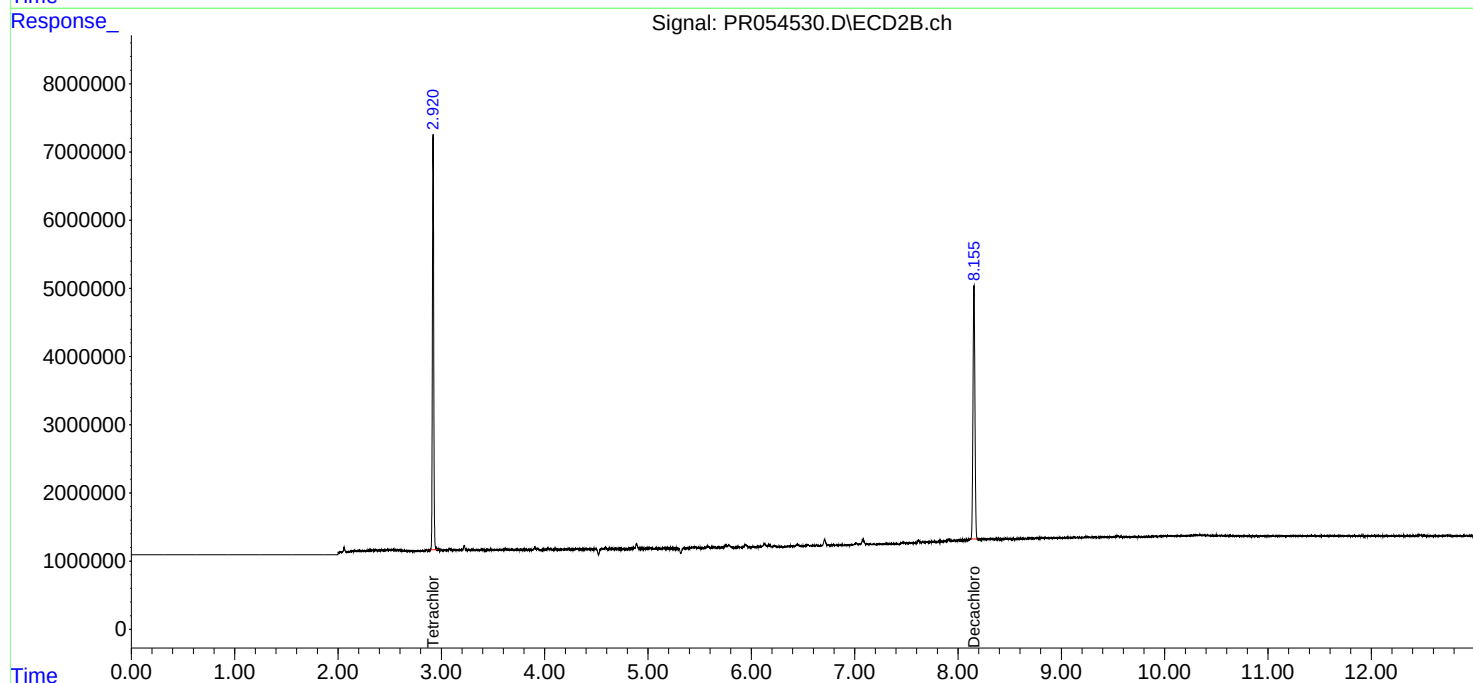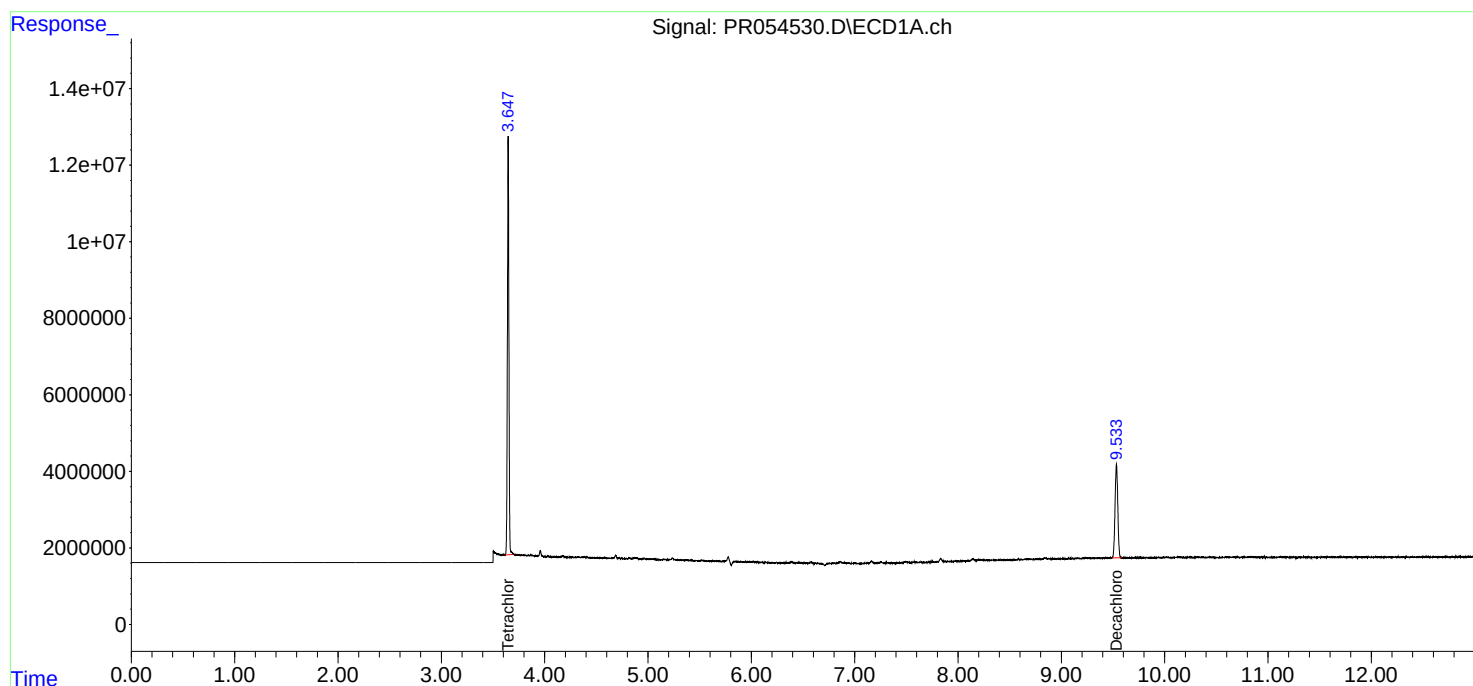

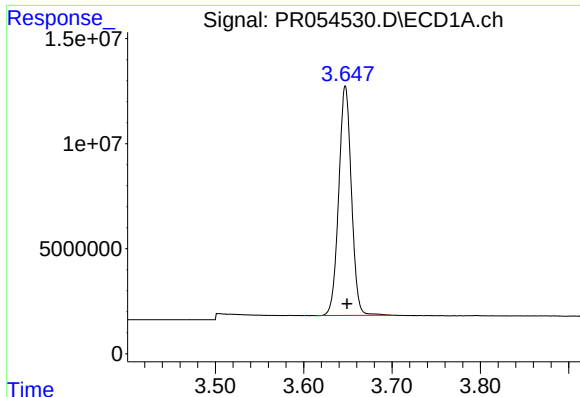

#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: -0.002 min
Response: 109160986
Conc: 29.60 ng/ml

Instrument :

ECD_R


ClientSampleId :

I.BLK

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 05/28/2022
Supervised By :Ankita Jodhani 05/28/2022

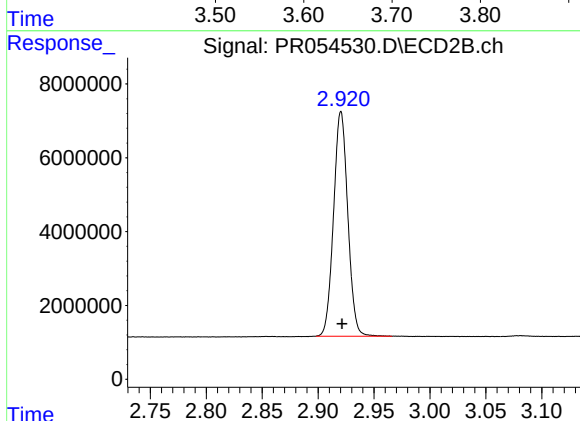


#1 Tetrachloro-m-xylene

R.T.: 2.921 min
Delta R.T.: 0.000 min
Response: 53876069
Conc: 28.52 ng/ml

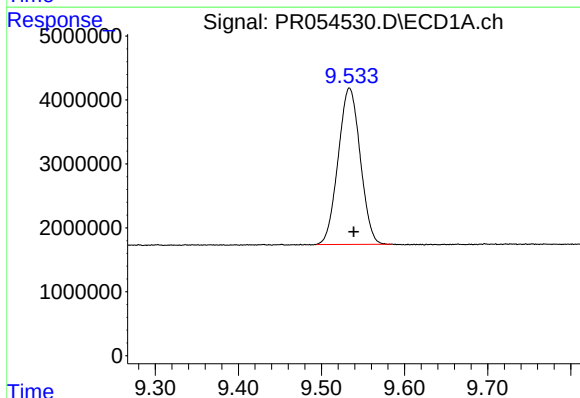

#2 Decachlorobiphenyl

R.T.: 9.534 min
Delta R.T.: -0.005 min
Response: 45033562
Conc: 29.48 ng/ml

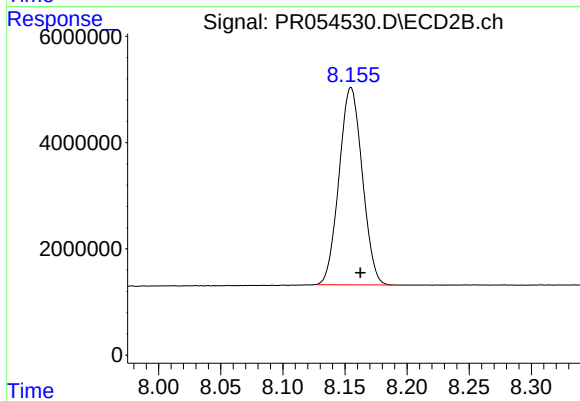

#2 Decachlorobiphenyl

R.T.: 8.155 min
Delta R.T.: -0.008 min
Response: 48322030
Conc: 33.55 ng/ml m