

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR053024\
Data File : PR067223.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2024 04:40
Operator : AJ\MA
Sample : P2647-15
Misc :
ALS Vial : 65 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
BHBS9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 05/31/2024
Supervised By :Ankita Jodhani 05/31/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 07:32:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052124CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 22 04:28:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

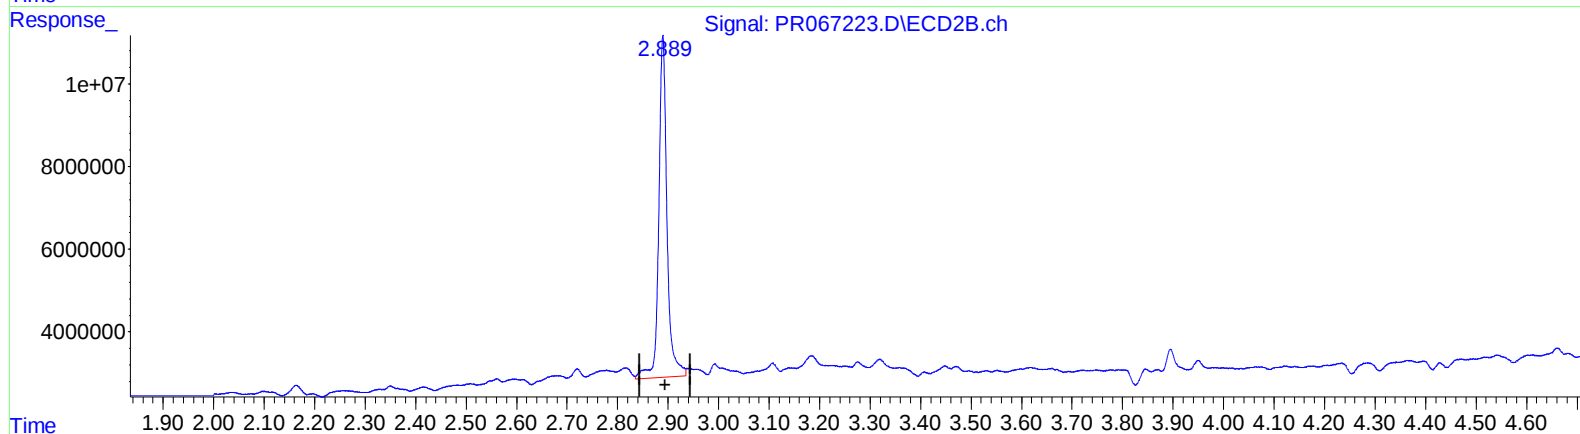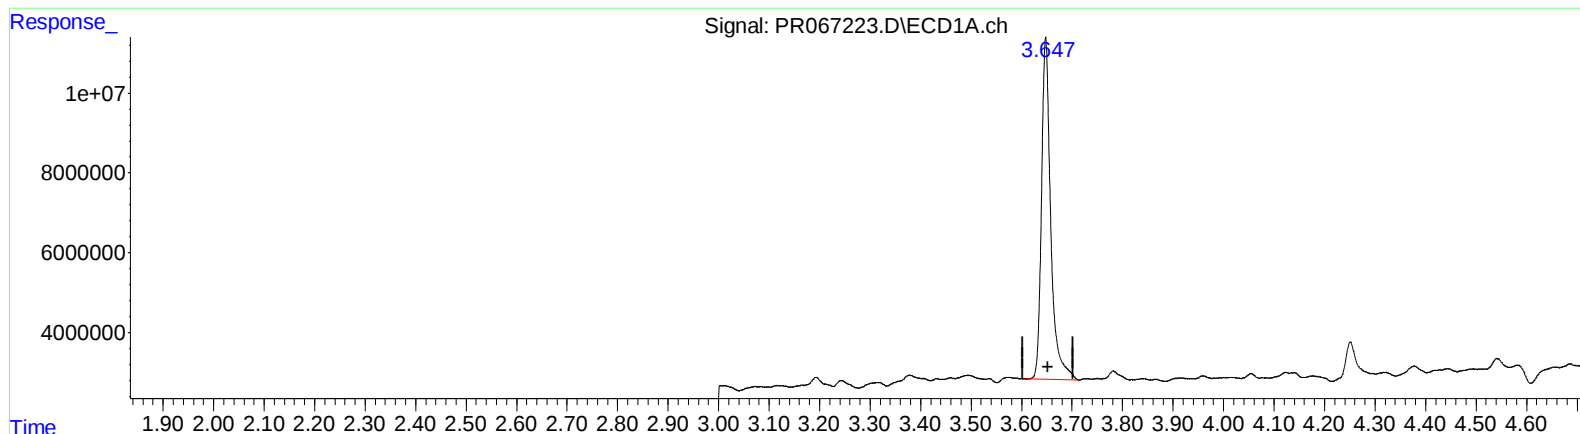

QEdit

(1) Tetrachloro-m-xylene (SA)

3.648min 17.812 ng/ml

response 109270136

(1) Tetrachloro-m-xylene #2 (SA)

2.890min 20.186 ng/ml

response 93985155

(+) = Expected Retention Time

PR052124CLP.M Fri May 31 09:22:31 2024

Page: 1

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR053024\
Data File : PR067223.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2024 04:40
Operator : AJ\MA
Sample : P2647-15
Misc :
ALS Vial : 65 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
BHBS9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 05/31/2024
Supervised By :Ankita Jodhani 05/31/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 07:32:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052124CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 22 04:28:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

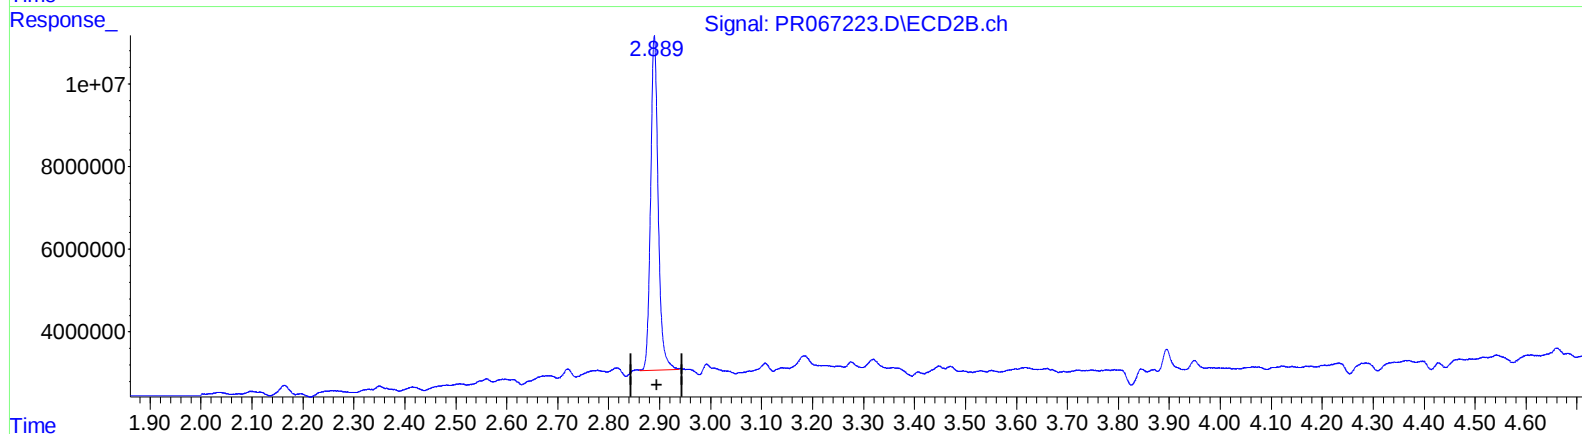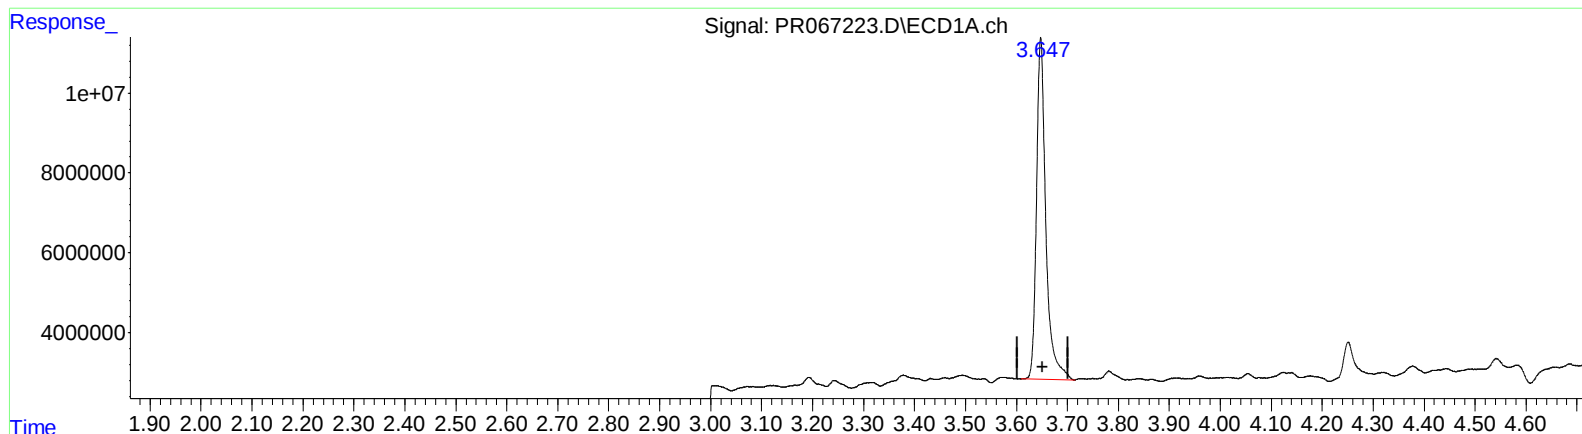

QEdit

(1) Tetrachloro-m-xylene (SA)

3.648min 17.812 ng/ml

response 109270136

(1) Tetrachloro-m-xylene #2 (SA)

2.889min 17.982 ng/ml m

response 83724342

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR053024\
 Data File : PR067223.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2024 04:40
 Operator : AJ\MA
 Sample : P2647-15
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 BHBS9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 05/31/2024
 Supervised By :Ankita Jodhani 05/31/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 07:32:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052124CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 22 04:28:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.648	2.889	109.3E6	83724342	17.812	17.982m
2) SA Decachlor...	9.525	8.109	47110253	79866183	36.281	35.871

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR053024\
Data File : PR067223.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2024 04:40
Operator : AJ\MA
Sample : P2647-15
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
BHBS9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 05/31/2024
Supervised By :Ankita Jodhani 05/31/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 07:32:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR052124CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 22 04:28:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

