

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR060722\
 Data File : PR054752.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jun 2022 00:53
 Operator : AJ\MA
 Sample : N3209-06
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 WC-14B-10

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/08/2022
 Supervised By :Ankita Jodhani 06/08/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 01:46:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR053122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 01 05:23:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.650	2.925	56456800	29407279	13.986	15.860
2) SA Decachlor...	9.536	8.149	28260370	27174533	17.292	16.247

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR060722\
Data File : PR054752.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jun 2022 00:53
Operator : AJ\MA
Sample : N3209-06
Misc :
ALS Vial : 51 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
WC-14B-10


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2022
Supervised By :Ankita Jodhani 06/08/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 01:46:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR053122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 01 05:23:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

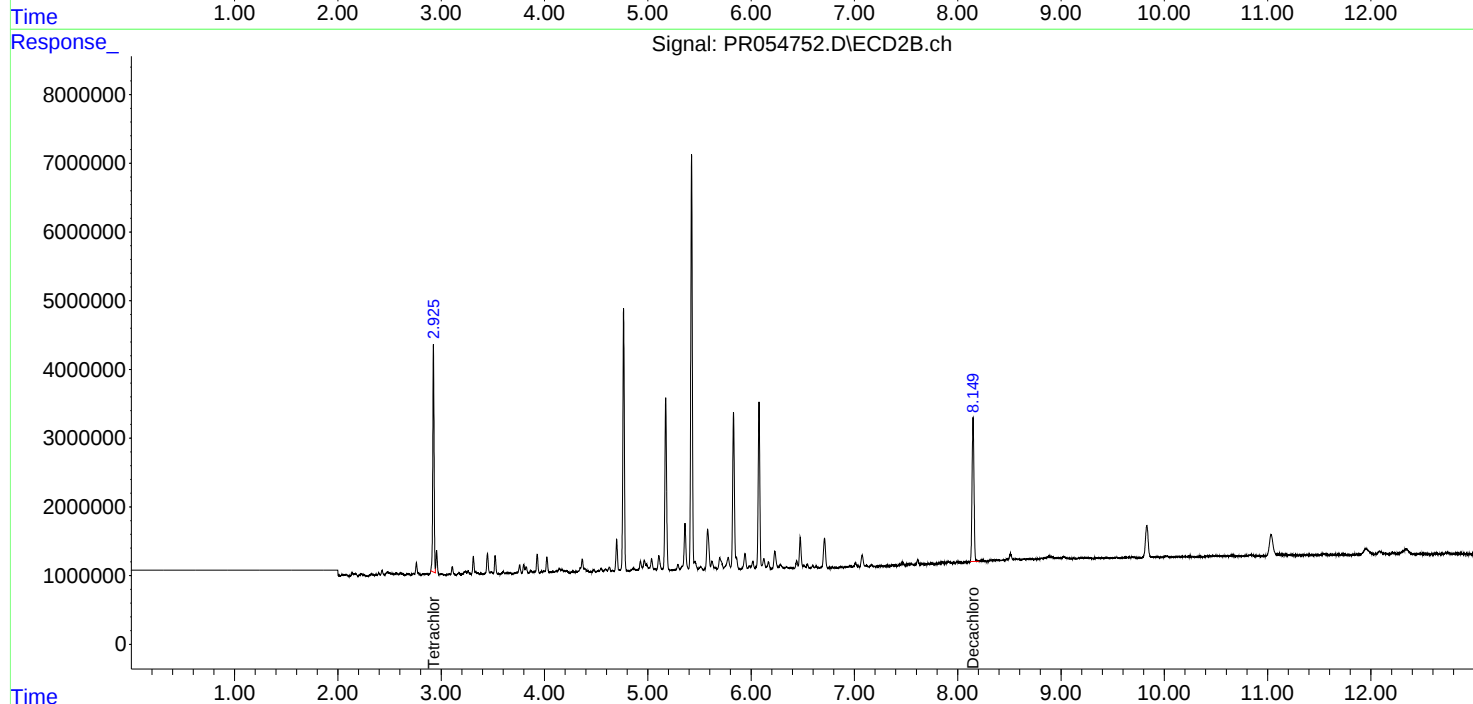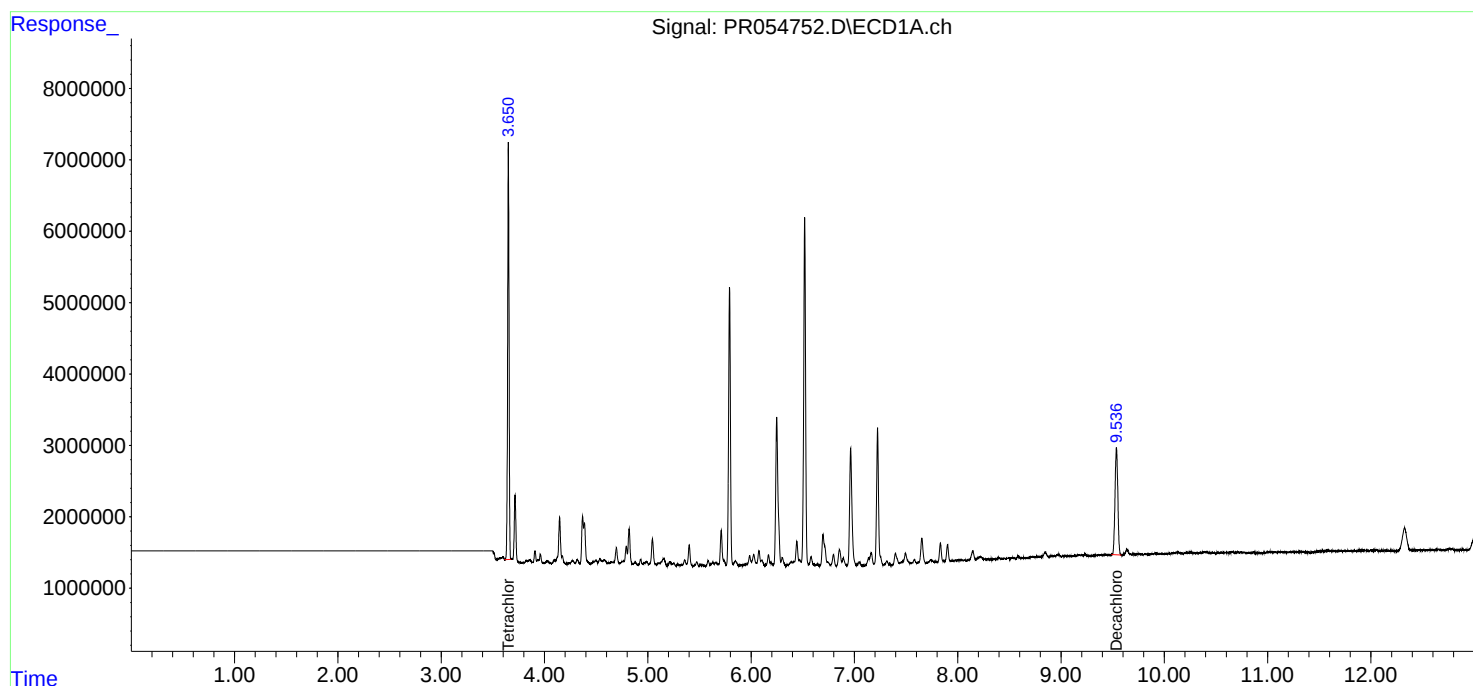

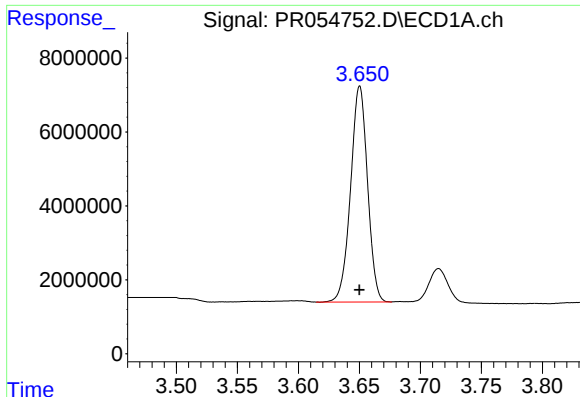

#1 Tetrachloro-m-xylene

R.T.: 3.650 min
Delta R.T.: 0.000 min
Response: 56456800
Conc: 13.99 ng/ml

Instrument :

ECD_R


ClientSampleId :

WC-14B-10

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 06/08/2022
Supervised By :Ankita Jodhani 06/08/2022

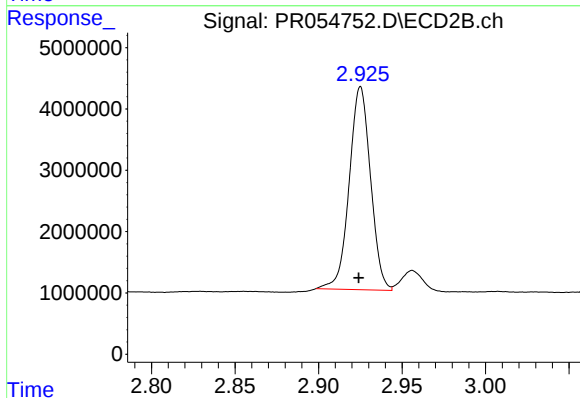


#1 Tetrachloro-m-xylene

R.T.: 2.925 min
Delta R.T.: 0.001 min
Response: 29407279
Conc: 15.86 ng/ml

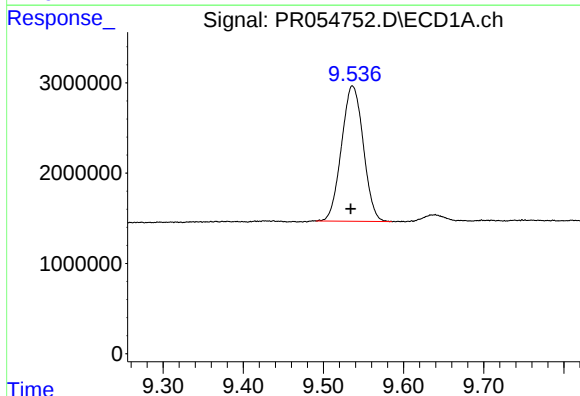

#2 Decachlorobiphenyl

R.T.: 9.536 min
Delta R.T.: 0.002 min
Response: 28260370
Conc: 17.29 ng/ml

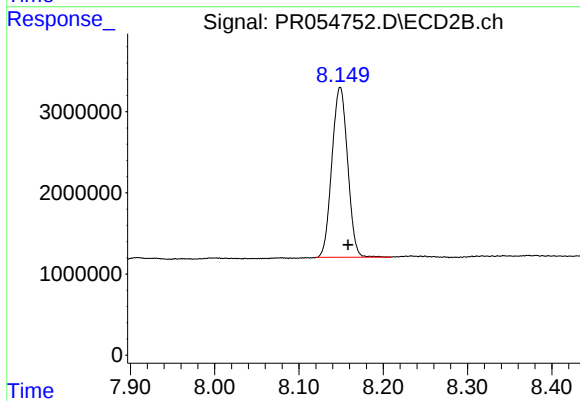

#2 Decachlorobiphenyl

R.T.: 8.149 min
Delta R.T.: -0.009 min
Response: 27174533
Conc: 16.25 ng/ml